

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
 Data File : BP017079.D
 Acq On : 10 Sep 2023 08:25
 Operator : MA/JU
 Sample : 04268-02
 Misc :
 ALS Vial : 92 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0GH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017079.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	36	40	50	rBV	98184	128984	1.38%	0.146%
2	3.764	112	115	127	rBV	406701	658525	7.06%	0.746%
3	3.958	143	148	153	rVB	73322	103951	1.11%	0.118%
4	4.069	164	167	172	rBV	18734	26210	0.28%	0.030%
5	5.011	321	327	332	rBV	12506	20961	0.22%	0.024%
6	5.599	422	427	431	rBV2	12114	19776	0.21%	0.022%
7	6.916	646	651	659	rVB9	12741	29181	0.31%	0.033%
8	7.116	679	685	701	rVB	398521	648931	6.95%	0.735%
9	7.310	709	718	729	rBV	1445160	2269367	24.31%	2.570%
10	7.487	740	748	762	rBV	1406675	2173498	23.29%	2.462%
11	7.969	822	830	841	rBV	1269278	2043248	21.89%	2.314%
12	8.675	943	950	968	rBV	1119019	1830421	19.61%	2.073%
13	9.163	1025	1033	1044	rBV	1716612	2804640	30.05%	3.177%
14	9.881	1146	1155	1165	rBV	1351327	2190829	23.47%	2.481%
15	10.404	1236	1244	1258	rBV	1997130	3224023	34.54%	3.652%
16	10.793	1300	1310	1320	rBV	1866586	3040585	32.58%	3.444%
17	10.951	1329	1337	1353	rBV	1634411	2781093	29.80%	3.150%
18	11.869	1483	1493	1499	rVB2	14817	33373	0.36%	0.038%
19	12.375	1573	1579	1587	rVB2	34821	56923	0.61%	0.064%
20	13.469	1759	1765	1775	rBV	51534	85003	0.91%	0.096%
21	13.587	1781	1785	1788	rVB6	7049	10269	0.11%	0.012%
22	13.863	1827	1832	1837	rVB2	8442	13012	0.14%	0.015%
23	14.040	1855	1862	1875	rBV	3939277	5378853	57.63%	6.092%
24	14.245	1890	1897	1898	rBV7	5435	9676	0.10%	0.011%
25	14.322	1903	1910	1929	rVV	4288163	6118851	65.56%	6.931%
26	14.622	1954	1961	1969	rBV	2652772	3848169	41.23%	4.359%
27	14.845	1993	1999	2011	rBV	229637	431288	4.62%	0.489%
28	15.016	2024	2028	2032	rVV7	7727	14877	0.16%	0.017%
29	15.057	2032	2035	2040	rVB5	10002	13699	0.15%	0.016%
30	15.622	2122	2131	2139	rBV	5555023	7850711	84.11%	8.892%
31	15.745	2146	2152	2165	rVV	1565096	2068028	22.16%	2.342%
32	15.857	2167	2171	2176	rVB2	27060	36123	0.39%	0.041%
33	17.392	2425	2432	2440	rBV	3142893	4398187	47.12%	4.982%
34	17.492	2442	2449	2462	rVV	6257896	8470889	90.75%	9.595%
35	18.022	2536	2539	2544	rVB7	15633	21475	0.23%	0.024%
36	18.233	2570	2575	2587	rBV	241956	395025	4.23%	0.447%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017079.D
Acq On : 10 Sep 2023 08:25
Operator : MA/JU
Sample : 04268-02
Misc :
ALS Vial : 92 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0GH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Title : SVOA CALIBRATION

37	18.751	2661	2663	2669	rBV7	12617	16296	0.17%	0.018%
38	19.298	2753	2756	2760	rBV3	58461	72505	0.78%	0.082%
39	19.369	2764	2768	2773	rVB	78229	106361	1.14%	0.120%
40	19.469	2781	2785	2791	rBV2	92927	134882	1.45%	0.153%
41	19.604	2805	2808	2812	rBV2	62178	65005	0.70%	0.074%
42	19.727	2823	2829	2837	rBV	7569202	9333819	100.00%	10.572%
43	21.163	3070	3073	3080	rVB2	158160	255151	2.73%	0.289%
44	21.486	3123	3128	3134	rBV2	2959652	3751927	40.20%	4.250%
45	23.851	3523	3530	3548	rVB	3873831	7776029	83.31%	8.808%
46	24.015	3552	3558	3568	rVB	1727902	3526160	37.78%	3.994%




Sum of corrected areas: 88286789

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017079.D
Acq On : 10 Sep 2023 08:25
Operator : MA/JU
Sample : 04268-02
Misc :
ALS Vial : 92 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0GH2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

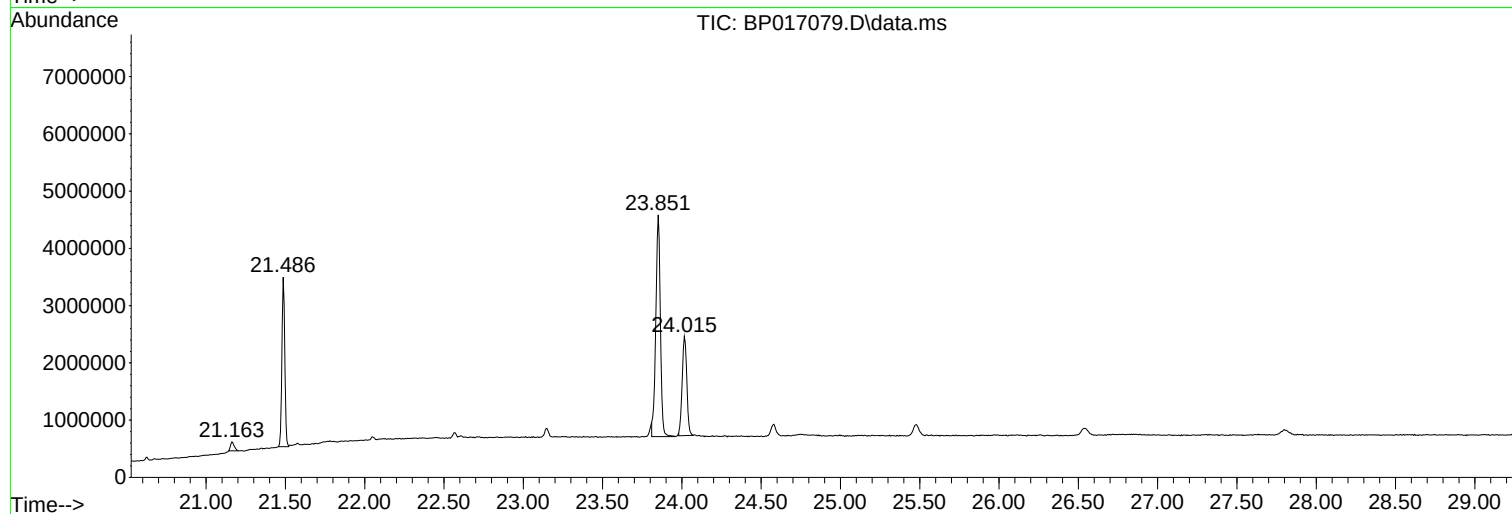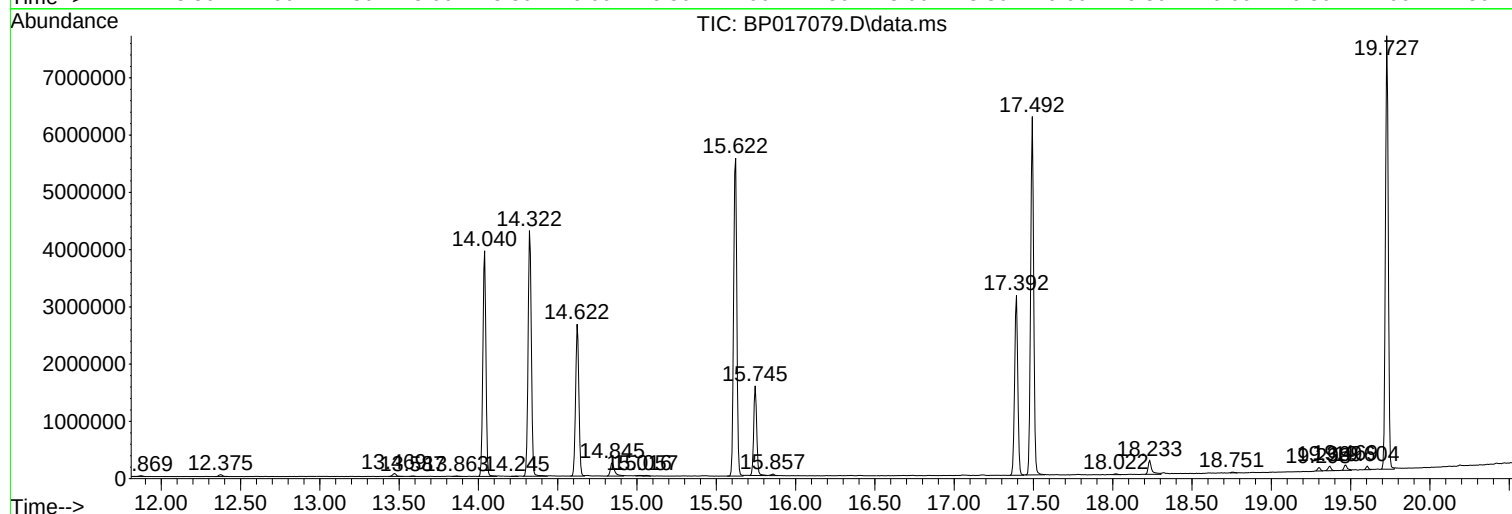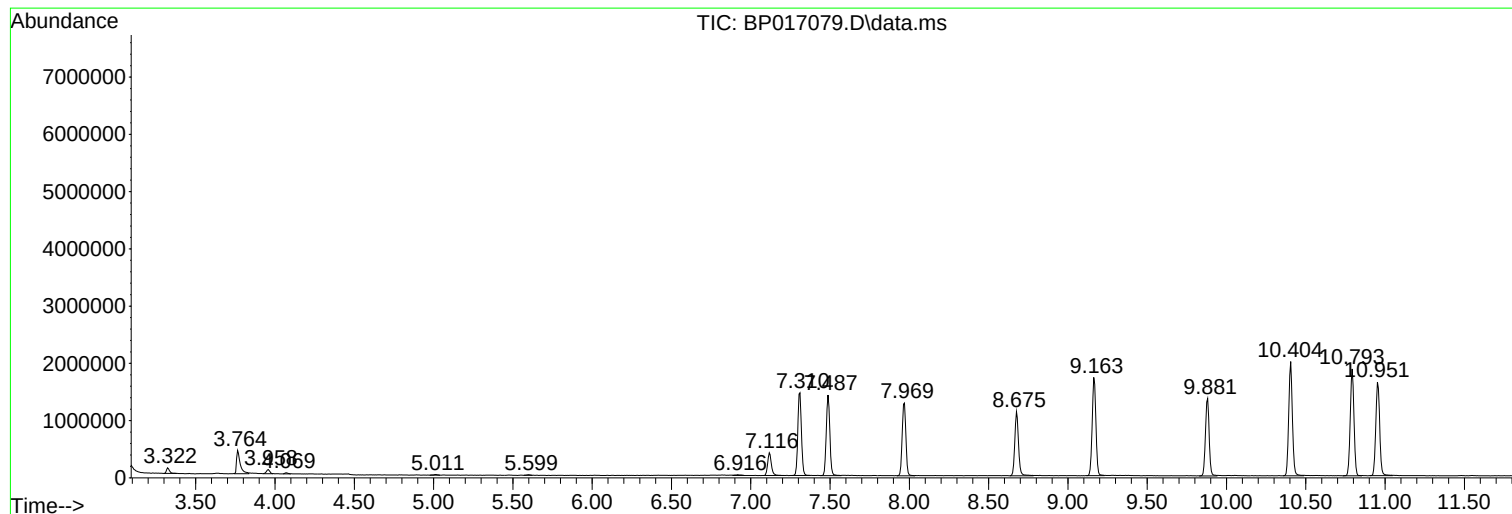

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017079.D
Acq On : 10 Sep 2023 08:25
Operator : MA/JU
Sample : 04268-02
Misc :
ALS Vial : 92 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0GH2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090823\
Data File : BP017079.D
Acq On : 10 Sep 2023 08:25
Operator : MA/JU
Sample : 04268-02
Misc :
ALS Vial : 92 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0GH2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc