

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP090919\
 Data File : BP000134.D
 Acq On : 09 Sep 2019 15:31
 Operator : HP/JU
 Sample : K4708-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Sep 10 03:36:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 02:43:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	439977	20.00	ng/ul	0.00
18) Naphthalene-d8	8.17	136	1728108	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.95	164	952496	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.45	188	1779470	20.00	ng/ul	0.00
78) Chrysene-d12	14.14	240	1537499	20.00	ng/ul	0.00
86) Perylene-d12	15.68	264	1599589	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.60	96	64481	5.20	ng/uL	0.00
5) Phenol-d5	6.51	99	1034166	27.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.57	67	538242	27.47	ng/ul	0.00
9) 2-Chlorophenol-d4	6.66	132	846110	27.92	ng/ul	0.00
13) 4-Methylphenol-d8	7.26	113	796112	28.28	ng/ul	0.00
19) Nitrobenzene-d5	7.45	128	387639	29.54	ng/ul	0.00
22) 2-Nitrophenol-d4	7.77	143	398648	31.21	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	8.02	165	723216	26.67	ng/ul	0.00
29) 4-Chloroaniline-d4	8.23	131	1023853	30.54	ng/ul	0.00
44) Dimethylphthalate-d6	9.63	166	1925152	27.37	ng/ul	0.00
47) Acenaphthylene-d8	9.79	160	2383599	27.42	ng/ul	0.00
52) 4-Nitrophenol-d4	10.03	143	322252	25.64	ng/ul	0.00
58) Fluorene-d10	10.47	176	1613442	27.01	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.52	200	187774	22.96	ng/ul	0.00
71) Anthracene-d10	11.50	188	2335554	27.10	ng/ul	0.00
79) Pyrene-d10	12.90	212	2495204	27.29	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.58	264	2341172	28.24	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.52	94	74936	1.919	ng/ul 99
45) Dimethylphthalate	9.65	163	516323	7.275	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP090919\
Data File : BP000134.D
Acq On : 09 Sep 2019 15:31
Operator : HP/JU
Sample : K4708-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Sep 10 03:36:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 02:43:18 2019
Response via : Initial Calibration

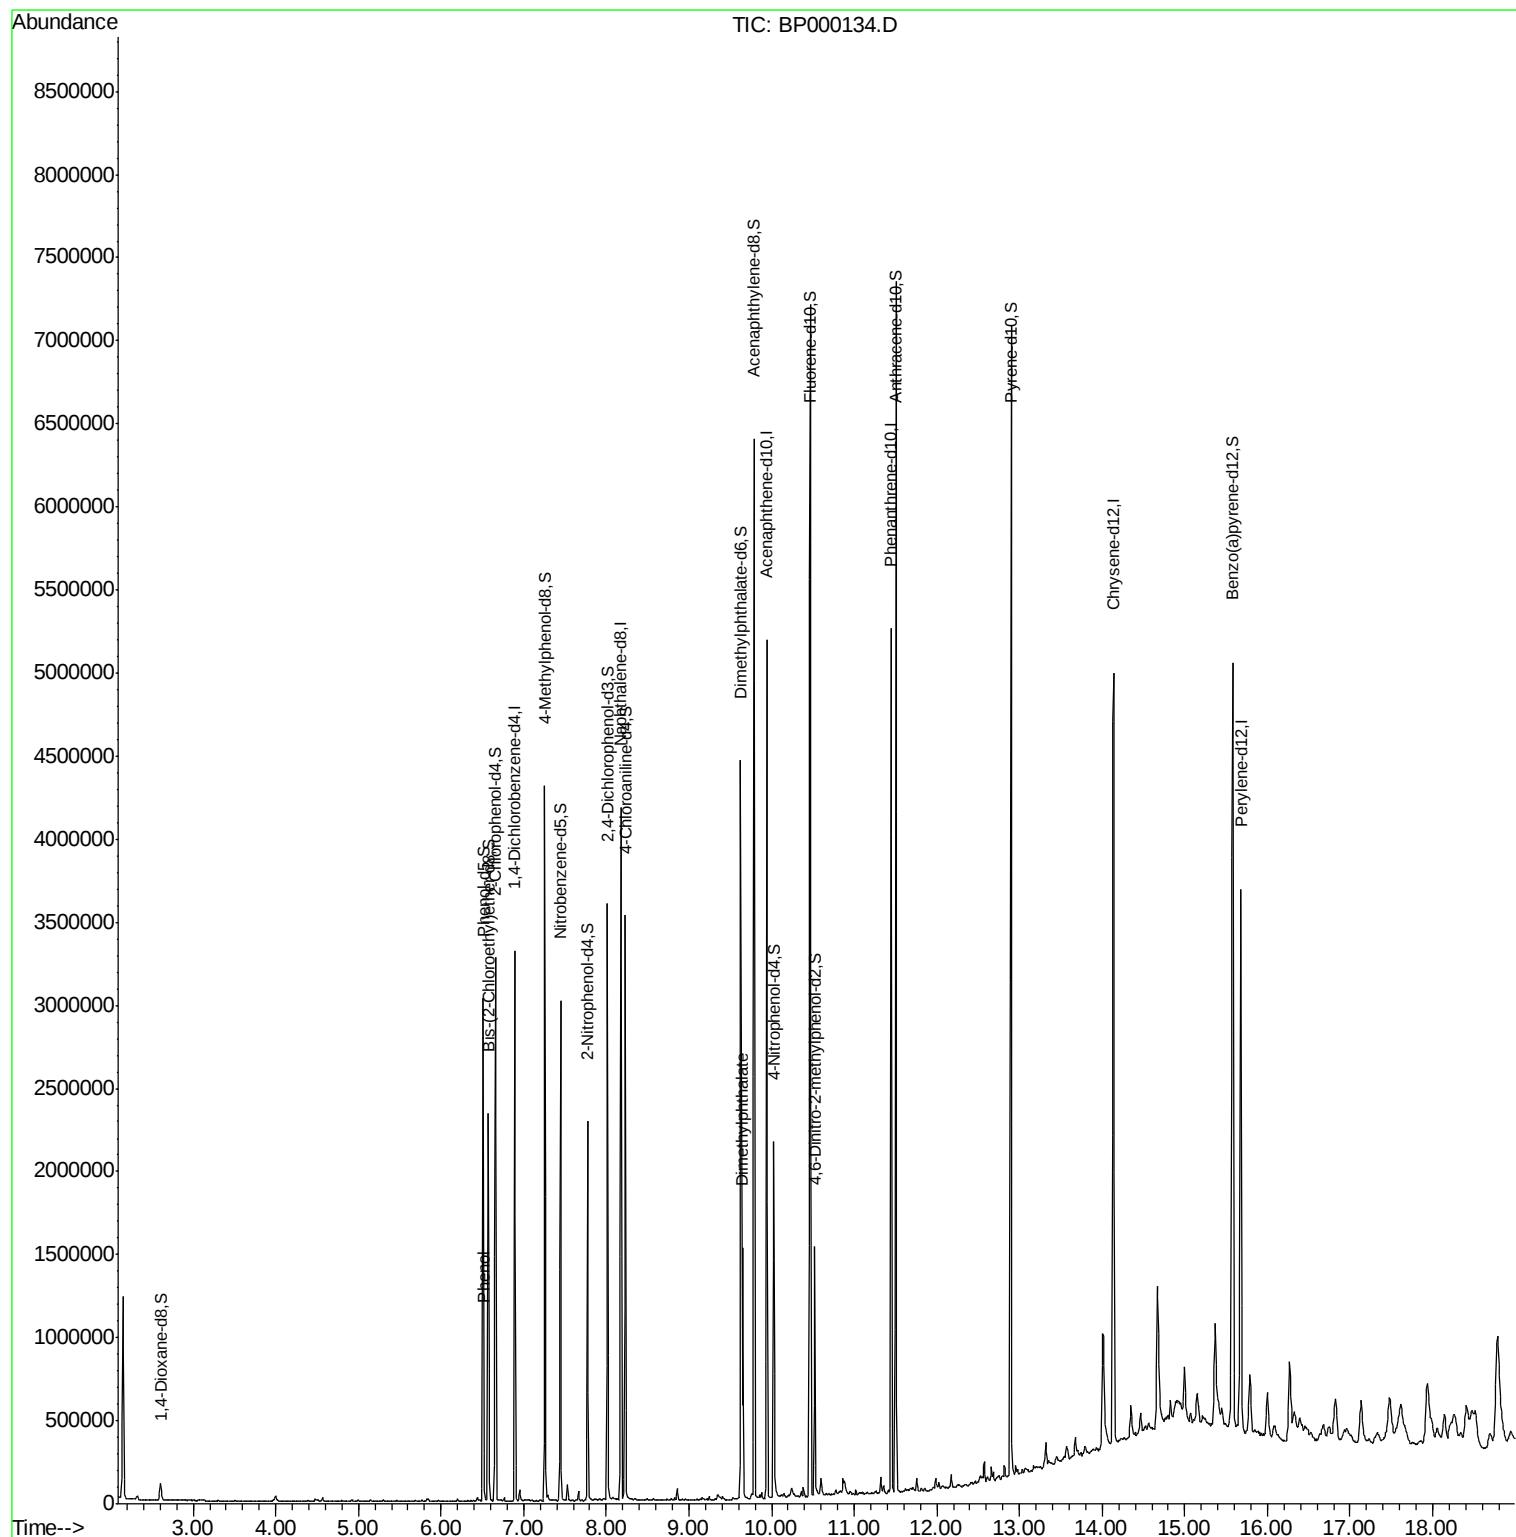

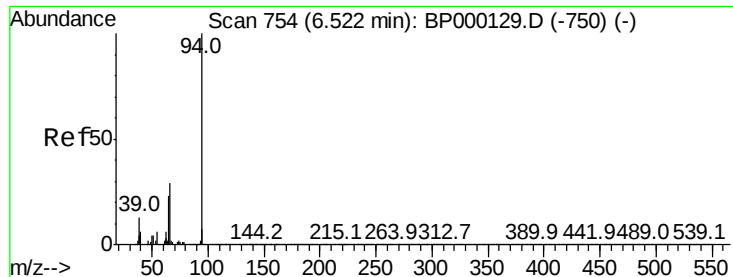





#6

Phenol

Concen: 1.919 ng/ul
 RT: 6.52 min Scan# 754
 Delta R.T. -0.00 min
 Lab File: BP000134.D
 Acq: 09 Sep 2019 15:31

Instrument :
 BNA_P
 ClientSampled :

Tot Ion: 94 Resp: 74936
 Ion Ratio Lower Upper
 94 100
 65 22.8 18.8 28.2
 66 29.8 24.2 36.2

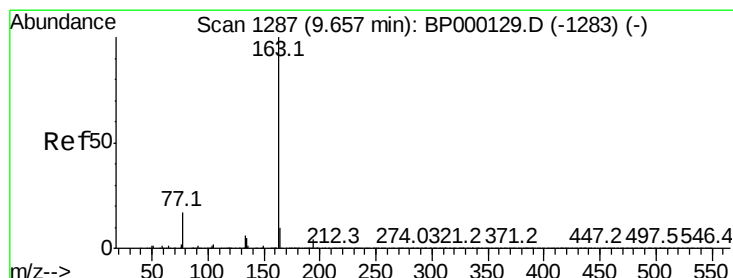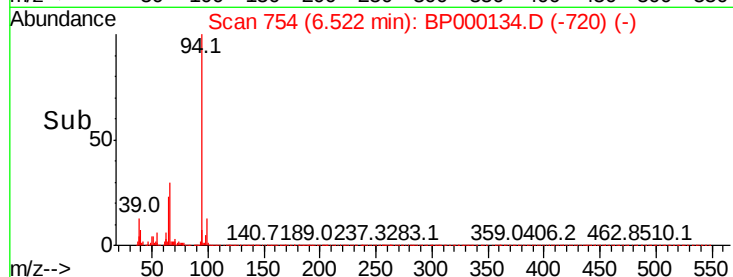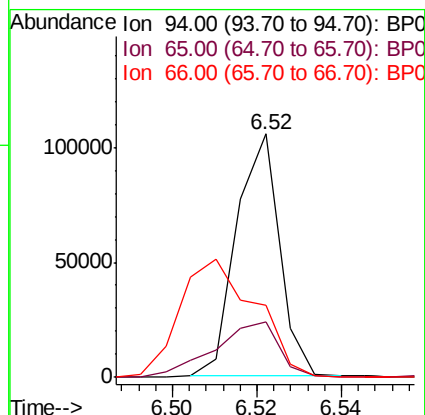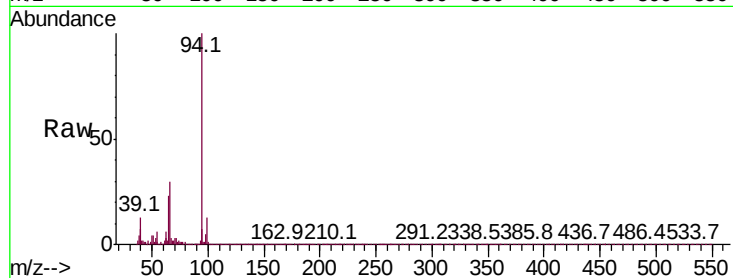

#45

Dimethylphthalate

Concen: 7.275 ng/ul
 RT: 9.65 min Scan# 1286
 Delta R.T. -0.01 min
 Lab File: BP000134.D
 Acq: 09 Sep 2019 15:31

Tgt Ion: 163 Resp: 516323
 Ion Ratio Lower Upper
 163 100
 194 4.0 3.2 4.8
 164 10.2 8.4 12.6

