

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP090919\
 Data File : BP000146.D
 Acq On : 09 Sep 2019 20:51
 Operator : HP/JU
 Sample : K4633-02MS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Sep 10 03:38:10 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 02:43:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	327250	20.00	ng/ul	0.00
18) Naphthalene-d8	8.18	136	1281538	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.95	164	710764	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.45	188	1305645	20.00	ng/ul	0.00
78) Chrysene-d12	14.13	240	1077439	20.00	ng/ul	-0.01
86) Perylene-d12	15.67	264	1113786	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.60	96	52885	5.73	ng/uL	0.00
5) Phenol-d5	6.51	99	920061	33.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.58	67	494389	33.92	ng/ul	0.00
9) 2-Chlorophenol-d4	6.66	132	752681	33.39	ng/ul	0.00
13) 4-Methylphenol-d8	7.26	113	491121	23.45	ng/ul	0.00
19) Nitrobenzene-d5	7.45	128	370344	38.06	ng/ul	0.00
22) 2-Nitrophenol-d4	7.78	143	387999	40.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	8.02	165	656292	32.64	ng/ul	0.00
29) 4-Chloroaniline-d4	8.23	131	692885	27.87	ng/ul	0.00
44) Dimethylphthalate-d6	9.63	166	1907819	36.35	ng/ul	0.00
47) Acenaphthylene-d8	9.79	160	2249278	34.68	ng/ul	0.00
52) 4-Nitrophenol-d4	10.03	143	307387	32.78	ng/ul	0.00
58) Fluorene-d10	10.47	176	1587918	35.63	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.52	200	197694	32.94	ng/ul	0.00
71) Anthracene-d10	11.50	188	1961257	31.02	ng/ul	0.00
79) Pyrene-d10	12.90	212	2350162	36.68	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.59	264	2142753	37.12	ng/ul	0.00

Target Compounds

					Ovalue
6) Phenol	6.52	94	1015185	34.946	ng/ul 99
10) 2-Chlorophenol	6.68	128	732460	30.781	ng/ul 96
15) N-Nitroso-di-n-propylamine	7.29	70	510710	34.609	ng/ul 99
33) 4-Chloro-3-methylphenol	8.72	107	619952	30.306	ng/ul 100
45) Dimethylphthalate	9.65	163	773065	14.597	ng/ul 100
50) Acenaphthene	9.98	153	1541219	32.825	ng/ul 99
53) 4-Nitrophenol	10.04	109	223944	32.085	ng/ul 98
55) 2,4-Dinitrotoluene	10.12	165	494323	35.837	ng/ul# 95
69) Pentachlorophenol	11.25	266	280039	30.981	ng/ul 98
70) Phenanthrene	11.47	178	852604	11.042	ng/ul 98
72) Anthracene	11.52	178	124362	1.637	ng/ul 99
75) Carbazole	11.67	167	122721	1.889	ng/ul 99
77) Fluoranthene	12.68	202	1831966	23.524	ng/ul 99
80) Pyrene	12.92	202	3942374	48.499	ng/ul 100
83) Benzo(a)anthracene	14.13	228	892002	11.437	ng/ul 99
85) Chrysene	14.16	228	1002877	14.013	ng/ul 98
88) Benzo(b)fluoranthene	15.22	252	1595073	21.608	ng/ul 100
89) Benzo(k)fluoranthene	15.22	252	1595073	22.923	ng/ul 99
91) Benzo(a)pyrene	15.61	252	916059	13.226	ng/ul 98
92) Indeno(1,2,3-cd)pyrene	17.23	276	766644	9.622	ng/ul 97
93) Dibenzo(a,h)anthracene	17.25	278	204143	3.093	ng/ul 98
94) Benzo(a,h,i)perylene	17.70	276	677657	10.200	ng/ul 99

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP090919\
Data File : BP000146.D
Acq On : 09 Sep 2019 20:51
Operator : HP/JU
Sample : K4633-02MS
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Sep 10 03:38:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 02:43:18 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP090919\
Data File : BP000146.D
Acq On : 09 Sep 2019 20:51
Operator : HP/JU
Sample : K4633-02MS
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampled :

Quant Time: Sep 10 03:38:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 02:43:18 2019
Response via : Initial Calibration

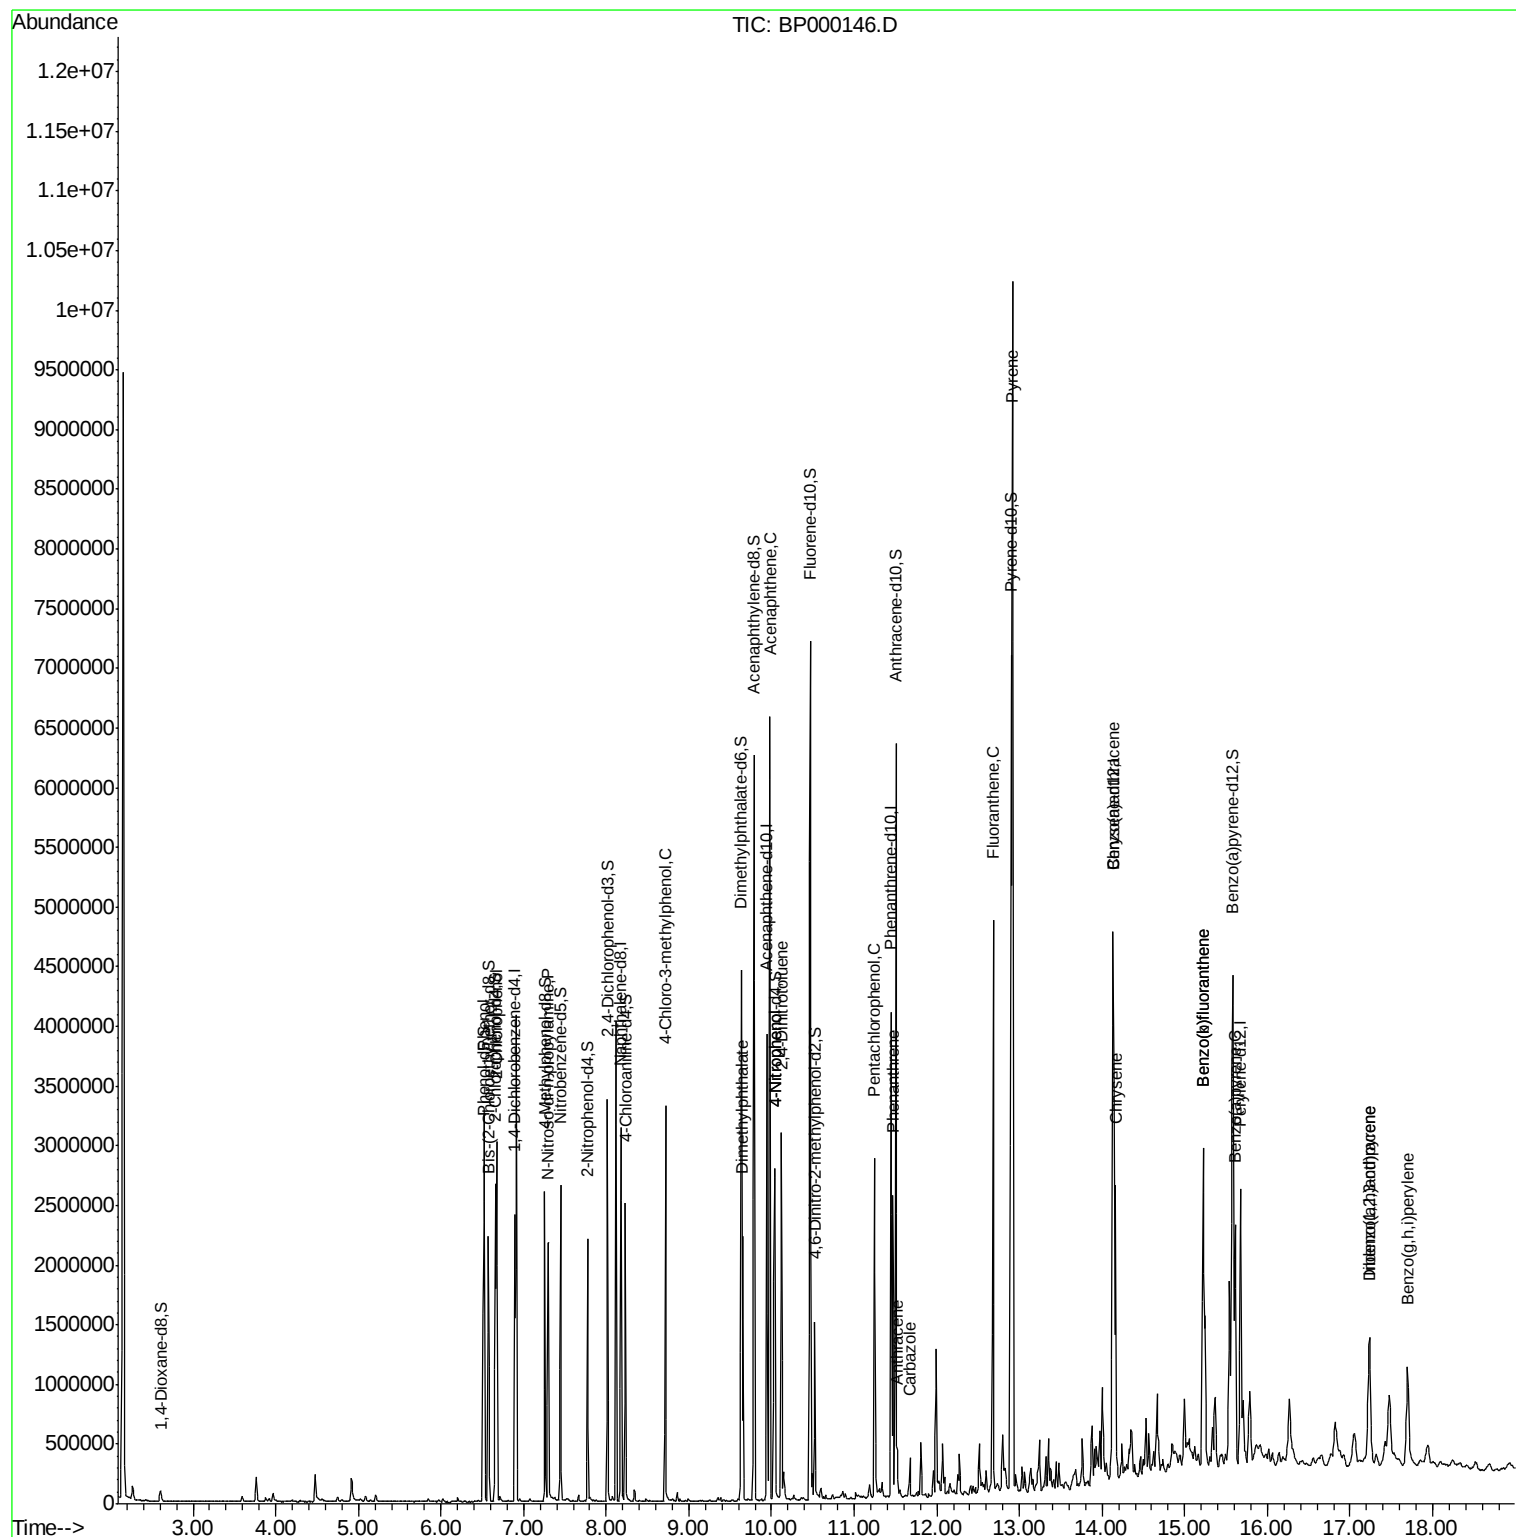

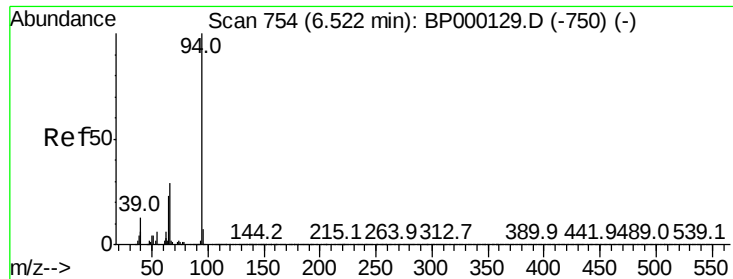

#6

Phenol

Concen: 34.946 ng/ul

RT: 6.52 min Scan# 754

Delta R.T. 0.00 min

Lab File: BP000146.D

Acq: 09 Sep 2019 20:51


Instrument :

BNA_P

ClientSampleId :

Tot Ion: 94 Resp: 1015185




Ion	Ratio	Lower	Upper
94	100		
65	23.5	18.8	28.2
66	31.4	24.2	36.2



Abundance Ion 94.00 (93.70 to 94.70): BP0

Ion 65.00 (64.70 to 65.70): BP0

Ion 66.00 (65.70 to 66.70): BP0

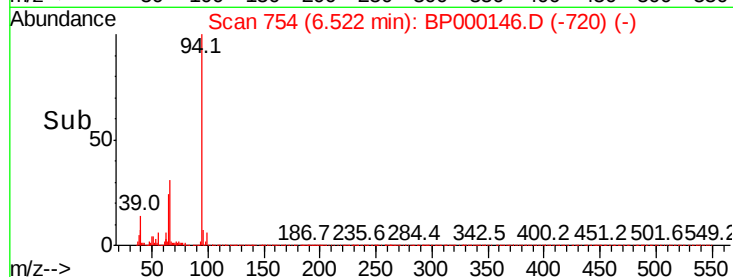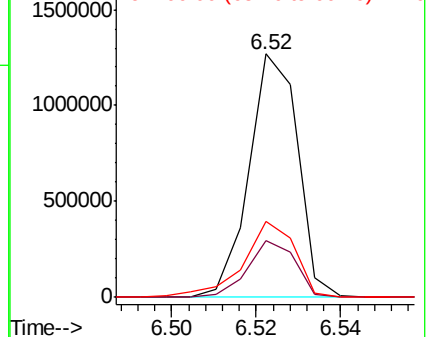

#10

2-Chlorophenol

Concen: 30.781 ng/ul

RT: 6.68 min Scan# 780


Delta R.T. 0.00 min

Lab File: BP000146.D

Acq: 09 Sep 2019 20:51

Tgt Ion: 128 Resp: 732460



Ion	Ratio	Lower	Upper
128	100		
64	40.3	29.6	44.4
130	32.0	26.2	39.4




Abundance Ion 128.00 (127.70 to 128.70): E

Ion 64.00 (63.70 to 64.70): BP0

Ion 130.00 (129.70 to 130.70): E



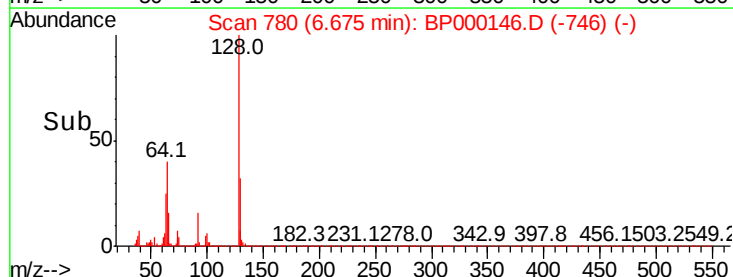
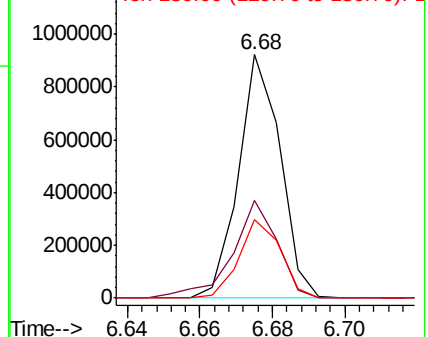


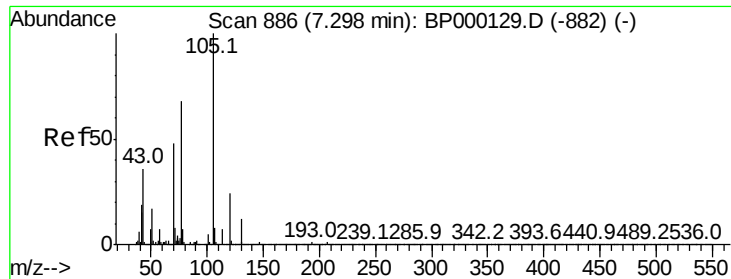

#15
N-Nitroso-di-n-propylamine
Concen: 34.609 ng/ul
RT: 7.29 min Scan# 885
Delta R.T. -0.01 min
Lab File: BP000146.D
Acq: 09 Sep 2019 20:51




Instrument :
BNA_P
ClientSampleId :


Tot Ion:	70	Resp:	510710
Ion	Ratio	Lower	Upper
70	100		
42	41.5	33.7	50.5
101	10.9	8.4	12.6
130	22.3	18.1	27.1

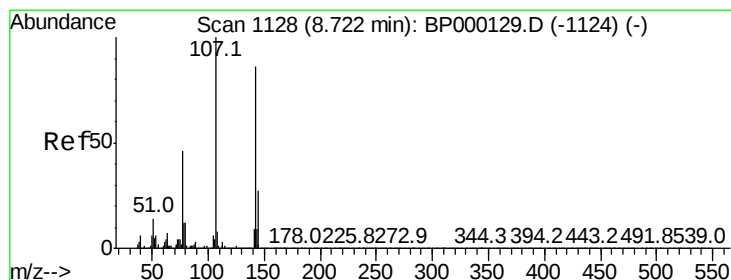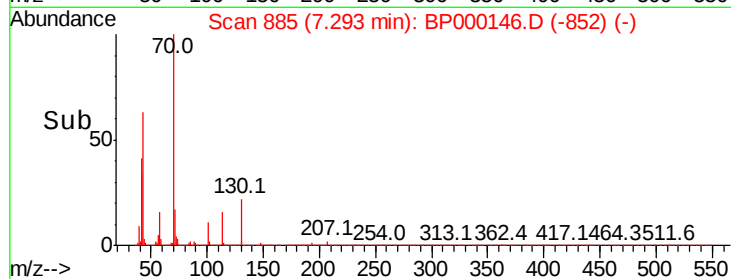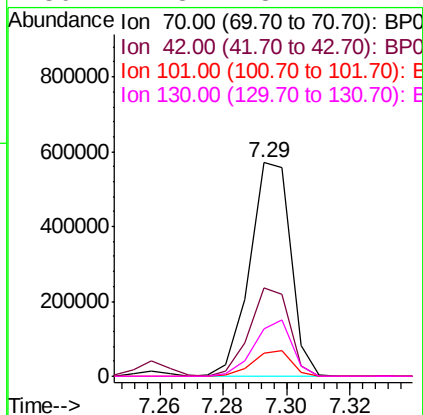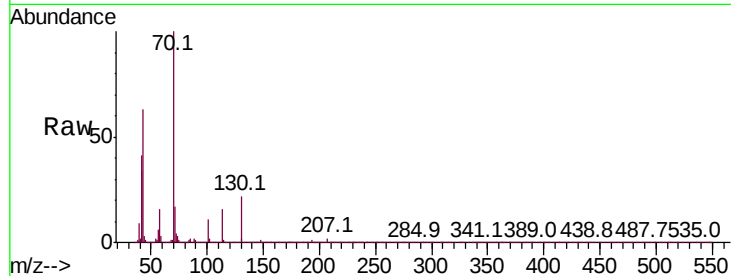

#33
4-Chloro-3-methylphenol
Concen: 30.306 ng/ul
RT: 8.72 min Scan# 1127
Delta R.T. -0.01 min
Lab File: BP000146.D
Acq: 09 Sep 2019 20:51

Tgt Ion:	107	Resp:	619952
Ion	Ratio	Lower	Upper
107	100		
144	26.8	21.5	32.3
142	81.9	65.8	98.8


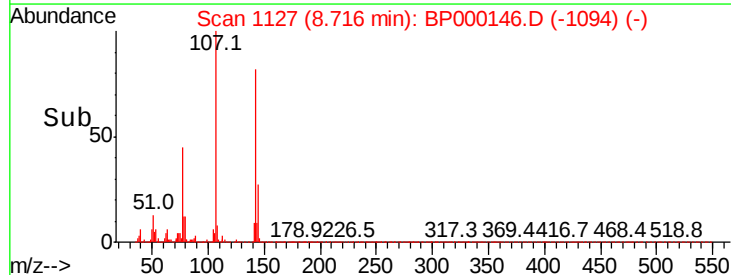
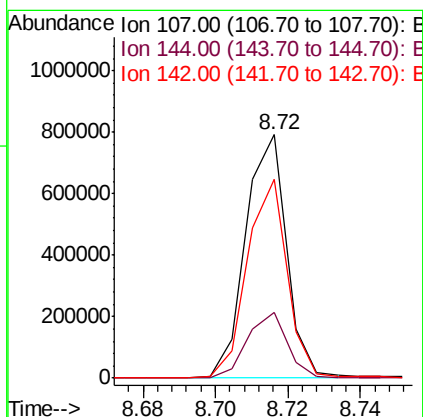
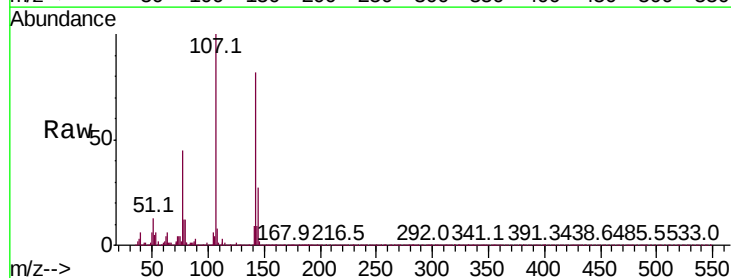


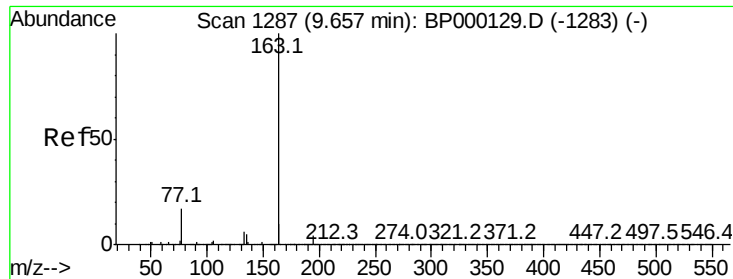

#45
Dimethylphthalate
Concen: 14.597 ng/ul
RT: 9.65 min Scan# 1286
Delta R.T. -0.01 min
Lab File: BP000146.D
Acq: 09 Sep 2019 20:51




Instrument :
BNA_P
ClientSampleId :


Tot Ion:163 Resp: 773065
Ion Ratio Lower Upper
163 100
194 4.0 3.2 4.8
164 10.4 8.4 12.6

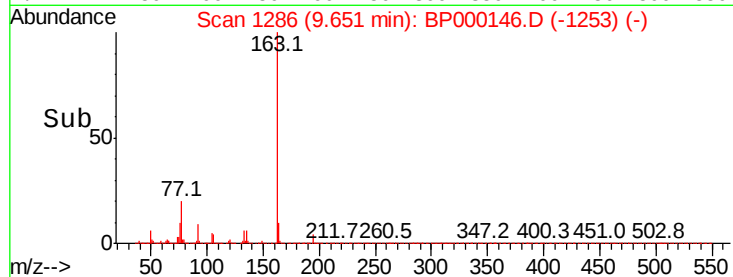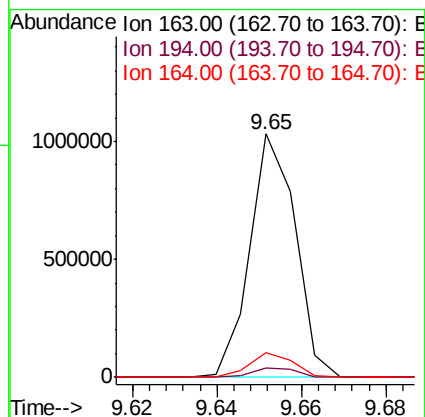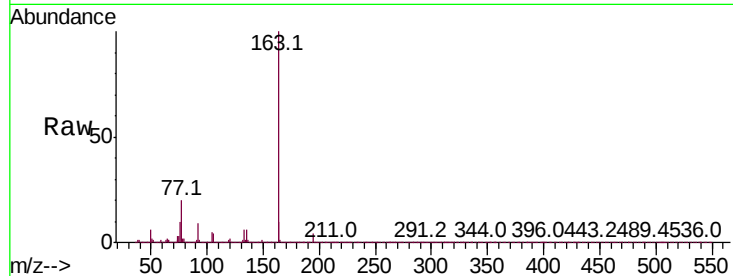

#50
Acenaphthene
Concen: 32.825 ng/ul
RT: 9.98 min Scan# 1342
Delta R.T. 0.00 min
Lab File: BP000146.D
Acq: 09 Sep 2019 20:51

Tgt Ion:153 Resp: 1541219
Ion Ratio Lower Upper
153 100
152 48.4 38.0 57.0
154 90.4 72.6 108.8

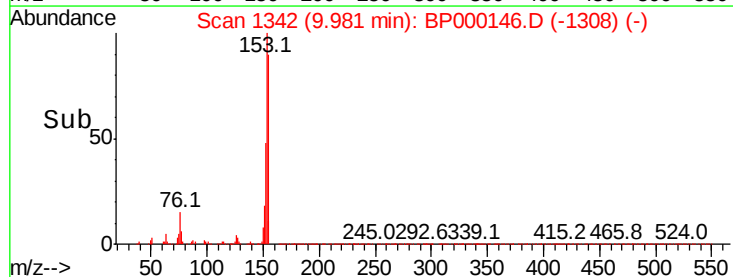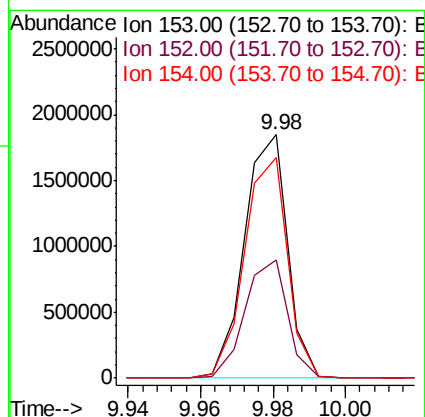

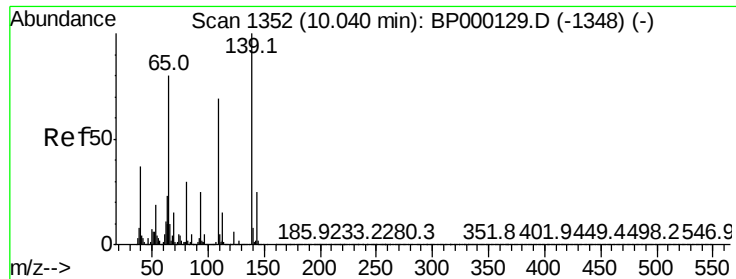

#53

4-Nitrophenol

Concen: 32.085 ng/ul

RT: 10.04 min Scan# 1352

Delta R.T. 0.00 min

Lab File: BP000146.D

Acq: 09 Sep 2019 20:51

Instrument :

BNA_P

ClientSampleId :





Tot Ion:109 Resp: 223944

Ion Ratio Lower Upper

109 100

139 145.2 118.6 177.8

65 116.7 95.4 143.2

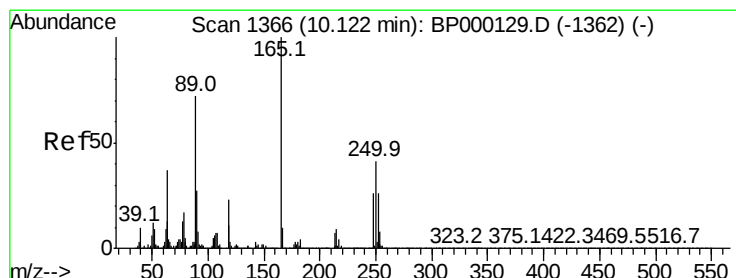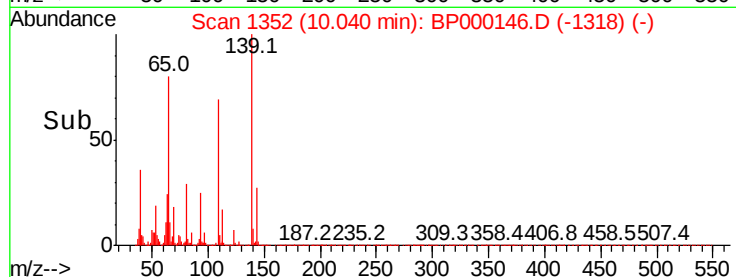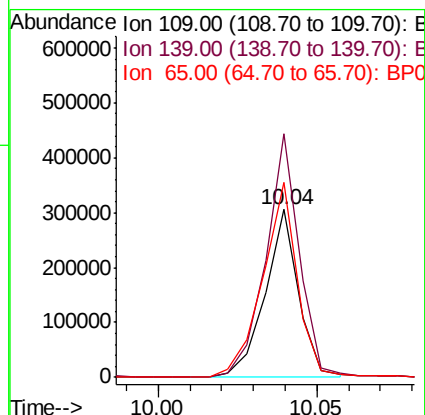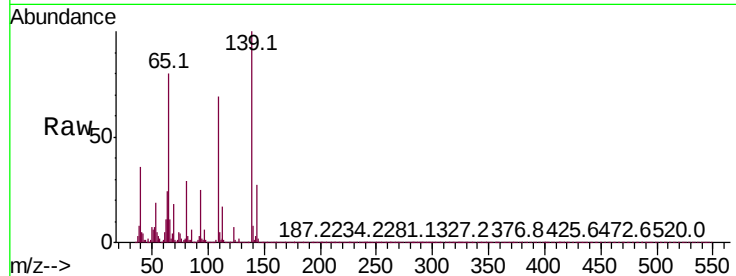

#55

2,4-Dinitrotoluene

Concen: 35.837 ng/ul

RT: 10.12 min Scan# 1366

Delta R.T. 0.00 min

Lab File: BP000146.D

Acq: 09 Sep 2019 20:51




Tgt Ion:165 Resp: 494323


Ion Ratio Lower Upper

165 100

63 34.8 25.4 38.0

182 2.8 3.1 4.7#

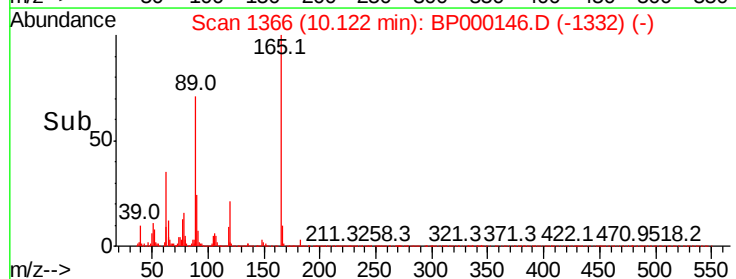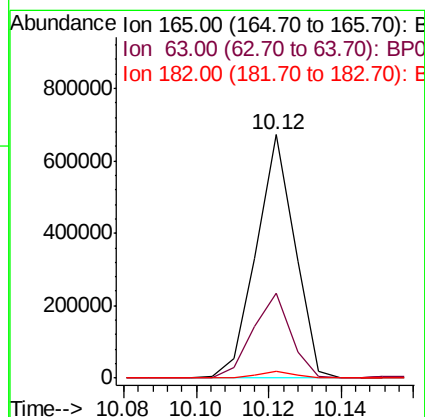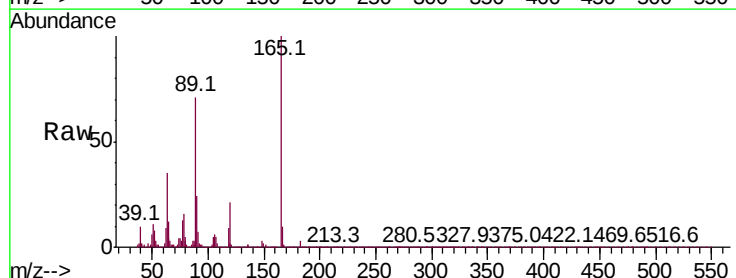

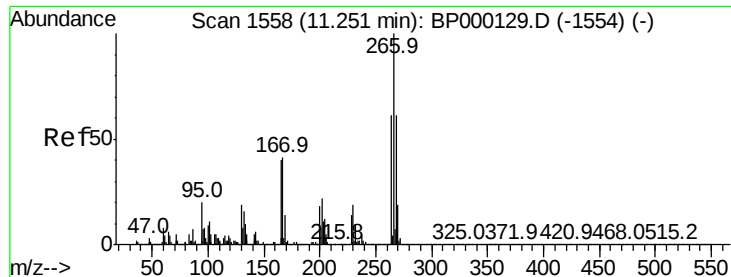

#69

Pentachlorophenol

Concen: 30.981 ng/ul

RT: 11.25 min Scan# 1557

Delta R.T. -0.01 min

Lab File: BP000146.D

Acq: 09 Sep 2019 20:51

Instrument :

BNA_P

ClientSampleId :


Tot Ion:266 Resp: 280039

Ion Ratio Lower Upper

266 100

264 65.6 50.6 75.8




268 63.7 51.2 76.8

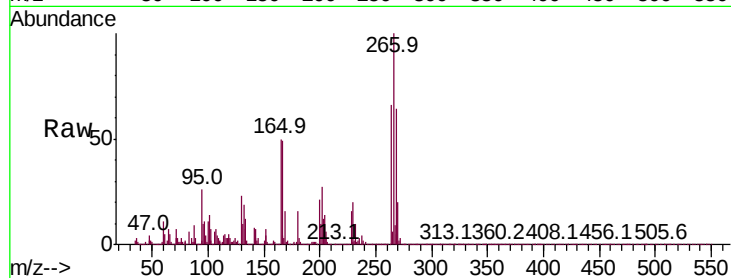

Abundance Ion 265.70 (265.40 to 266.40): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

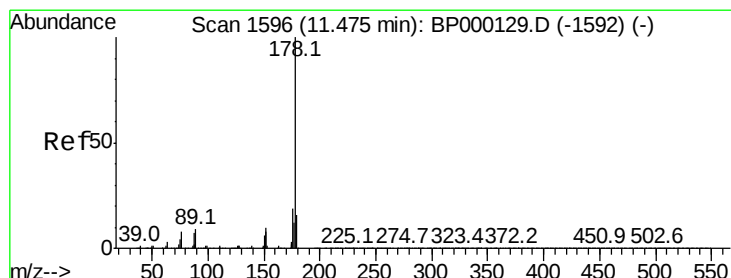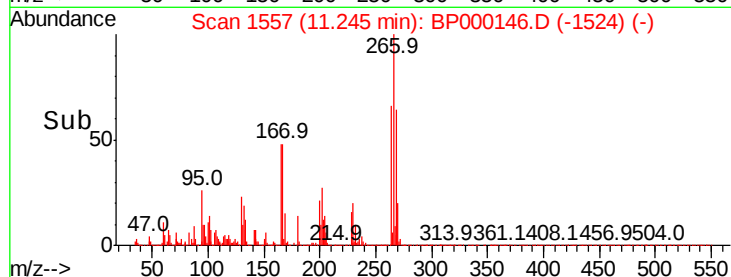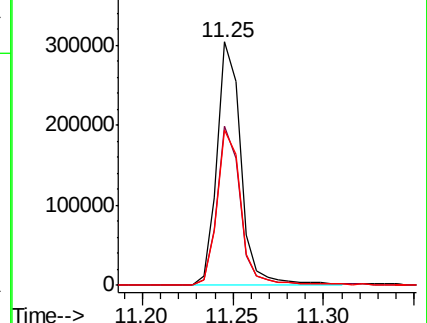

#70

Phenanthrene

Concen: 11.042 ng/ul

RT: 11.47 min Scan# 1595

Delta R.T. -0.01 min

Lab File: BP000146.D

Acq: 09 Sep 2019 20:51


Tgt Ion:178 Resp: 852604

Ion Ratio Lower Upper

178 100

179 15.4 12.5 18.7



176 18.5 15.7 23.5

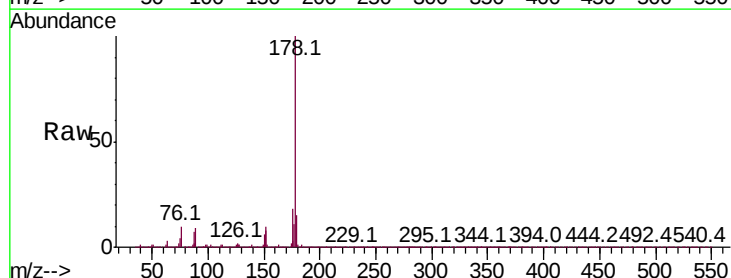


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

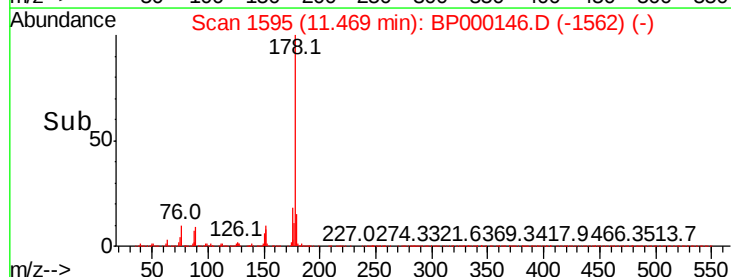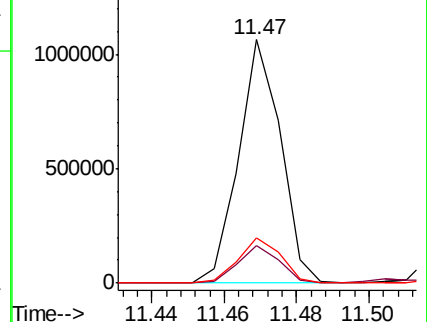

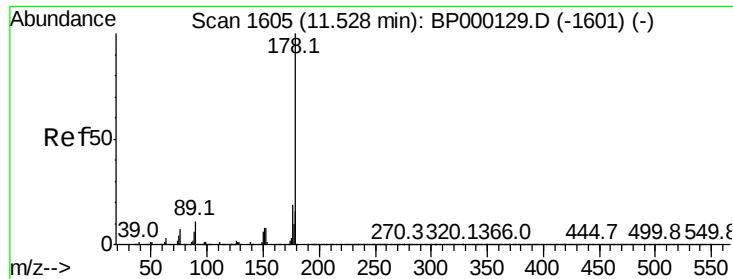

#72

Anthracene

Concen: 1.637 ng/ul

RT: 11.52 min Scan# 1604

Delta R.T. -0.01 min

Lab File: BP000146.D

Acq: 09 Sep 2019 20:51

Instrument :

BNA_P

ClientSampleId :


Tot Ion:178 Resp: 124362

Ion Ratio Lower Upper

178 100

179 15.6 12.3 18.5




176 18.6 15.1 22.7

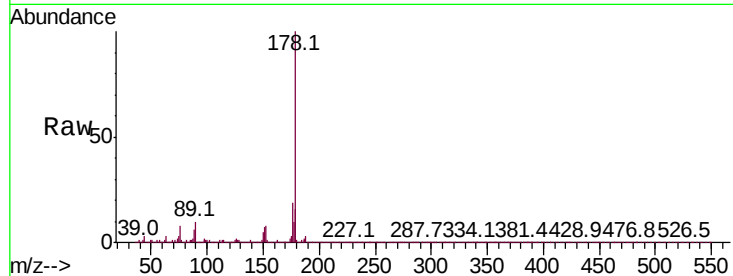

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

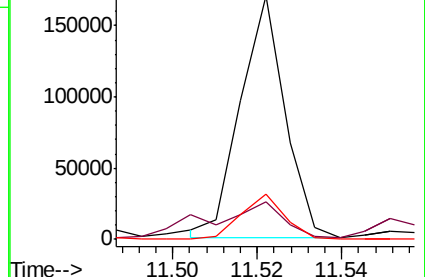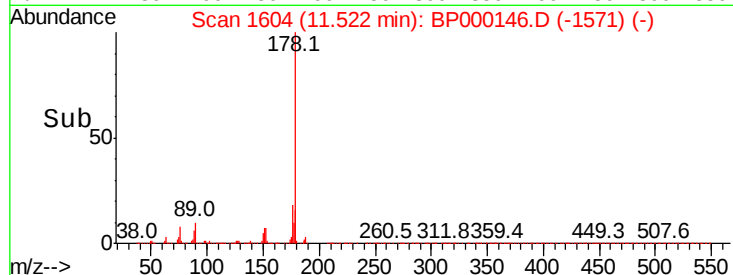

#75

Carbazole

Concen: 1.889 ng/ul

RT: 11.67 min Scan# 1630

Delta R.T. -0.01 min

Lab File: BP000146.D

Acq: 09 Sep 2019 20:51


Tgt Ion:167 Resp: 122721

Ion Ratio Lower Upper

167 100

166 21.5 17.3 25.9



139 12.7 10.6 15.8




Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

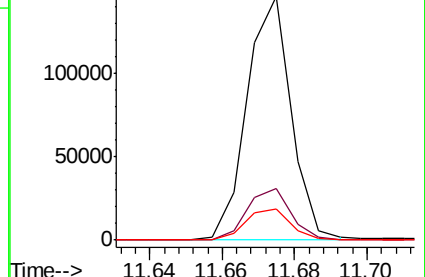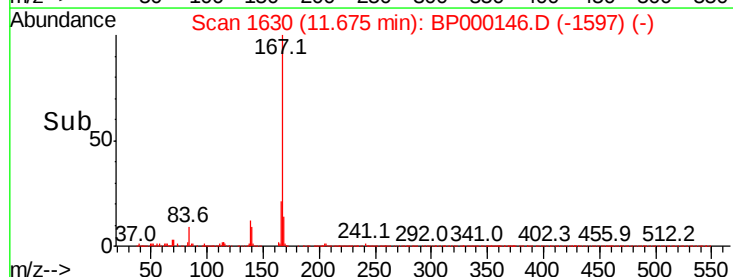

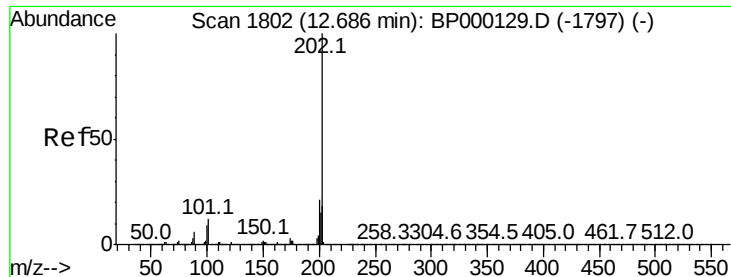

#77

Fluoranthene

Concen: 23.524 ng/ul

RT: 12.68 min Scan# 1801

Delta R.T. -0.01 min

Lab File: BP000146.D

Acq: 09 Sep 2019 20:51


Instrument :

BNA_P

ClientSampleId :

Tot Ion:202 Resp: 1831966

Ion	Ratio	Lower	Upper
202	100		
101	11.8	10.0	15.0
100	9.1	7.4	11.2



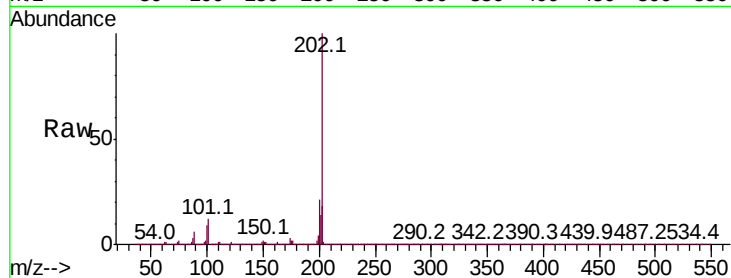


Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BF

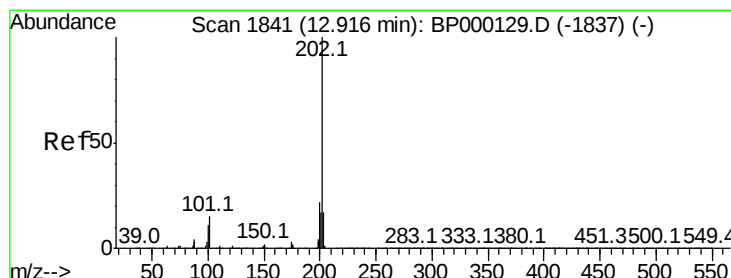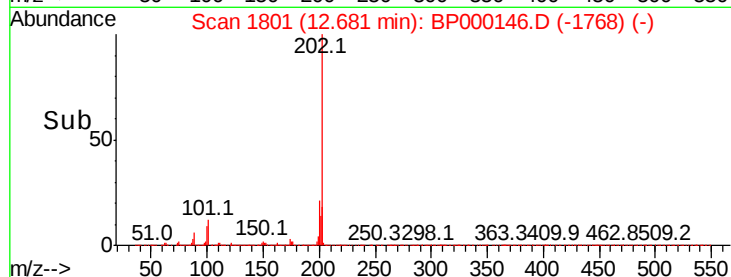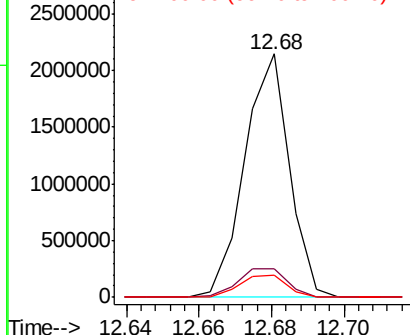

#80

Pyrene

Concen: 48.499 ng/ul

RT: 12.92 min Scan# 1841


Delta R.T. 0.00 min

Lab File: BP000146.D

Acq: 09 Sep 2019 20:51

Tgt Ion:202 Resp: 3942374

Ion	Ratio	Lower	Upper
202	100		
101	16.4	13.4	20.0
100	13.5	10.8	16.2


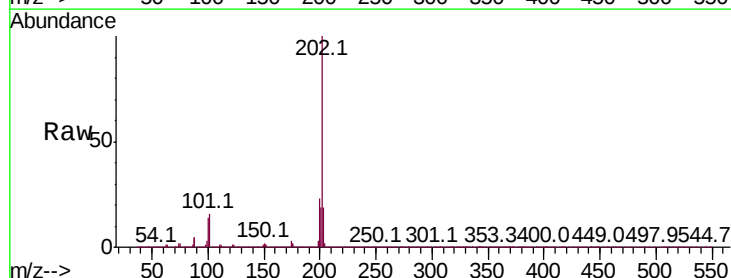



Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BF



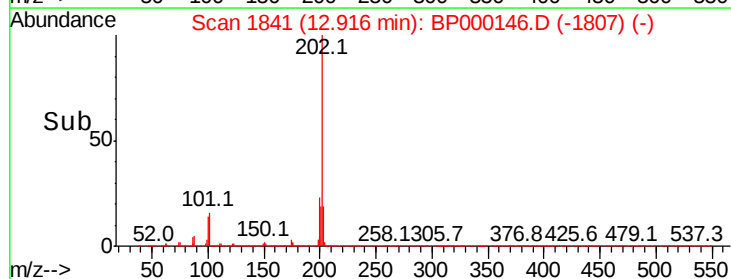
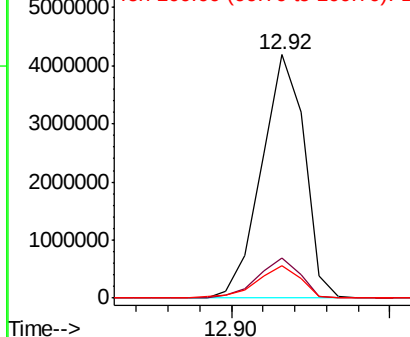


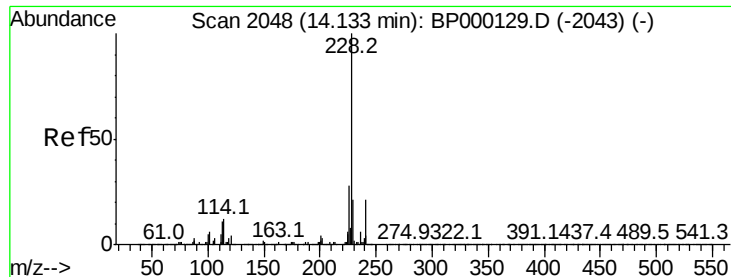

#83
Benzo(a)anthracene
Concen: 11.437 ng/ul
RT: 14.13 min Scan# 2047
Delta R.T. -0.01 min
Lab File: BP000146.D
Acq: 09 Sep 2019 20:51




Instrument :
BNA_P
ClientSampleId :


Tot Ion:228 Resp: 892002
Ion Ratio Lower Upper
228 100
229 20.5 15.9 23.9
226 28.0 22.1 33.1

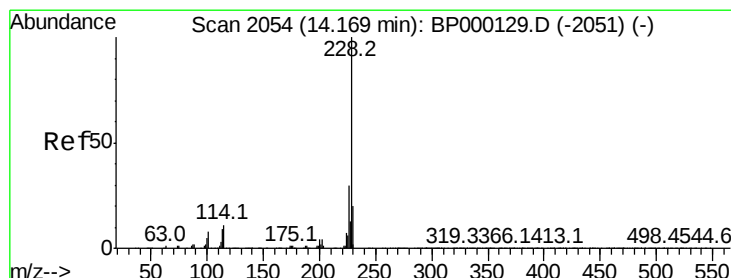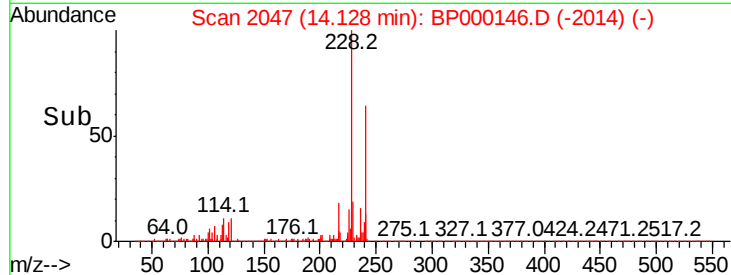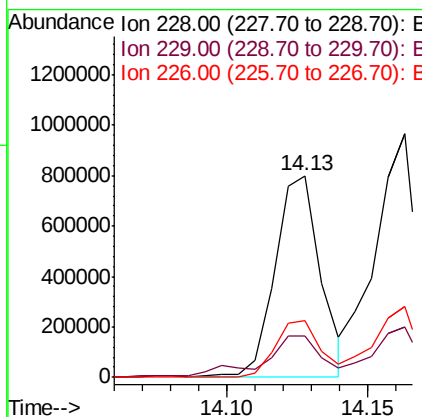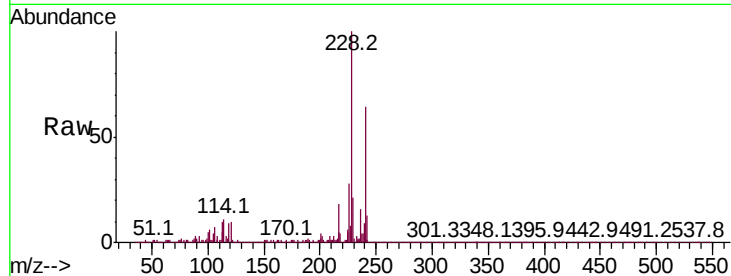

#85
Chrysene
Concen: 14.013 ng/ul
RT: 14.16 min Scan# 2053
Delta R.T. -0.01 min
Lab File: BP000146.D
Acq: 09 Sep 2019 20:51

Tgt Ion:228 Resp: 1002877
Ion Ratio Lower Upper
228 100
226 29.0 24.4 36.6
229 20.9 16.0 24.0


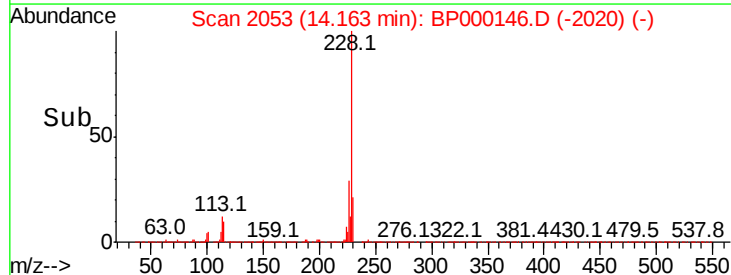
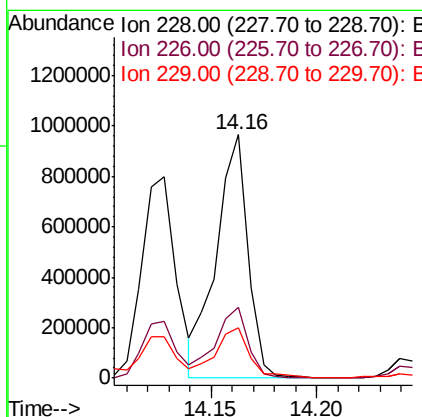
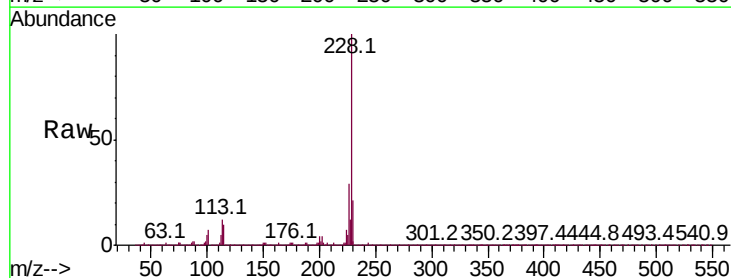


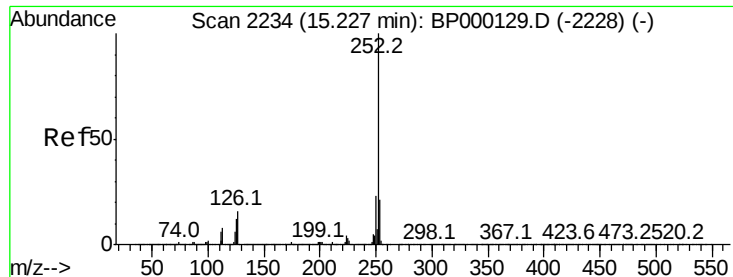

#88
Benzo(b)fluoranthene
Concen: 21.608 ng/ul
RT: 15.22 min Scan# 2233
Delta R.T. -0.01 min
Lab File: BP000146.D
Acq: 09 Sep 2019 20:51




Instrument :
BNA_P
ClientSampleId :


Tot Ion:252 Resp: 1595073
Ion Ratio Lower Upper
252 100
253 21.8 17.5 26.3
125 12.5 9.9 14.9

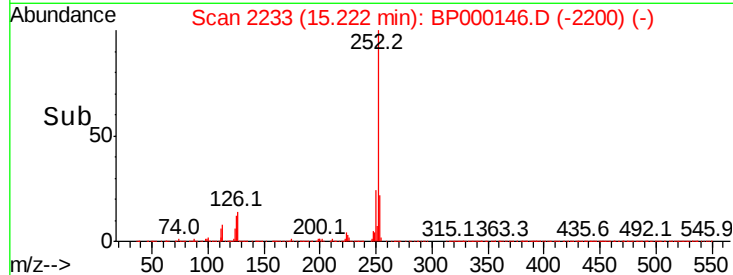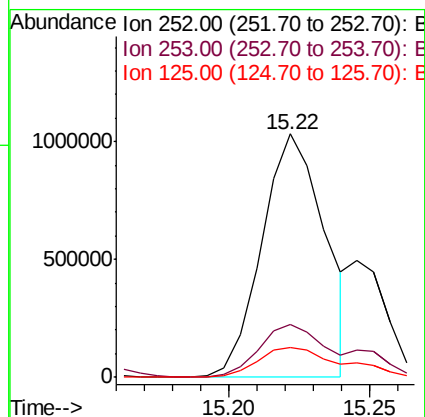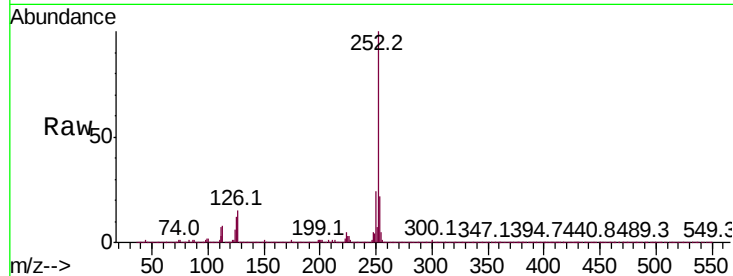

#89
Benzo(k)fluoranthene
Concen: 22.923 ng/ul
RT: 15.22 min Scan# 2233
Delta R.T. -0.04 min
Lab File: BP000146.D
Acq: 09 Sep 2019 20:51

Tgt Ion:252 Resp: 1595073
Ion Ratio Lower Upper
252 100
253 21.8 18.0 27.0
125 12.5 10.2 15.2

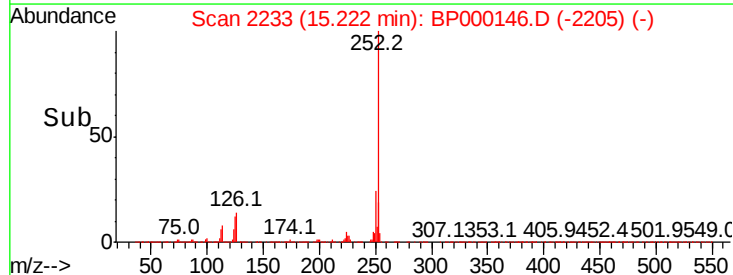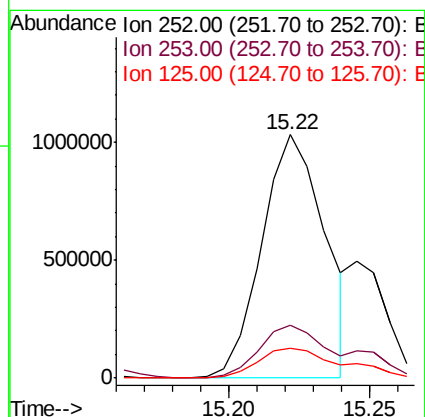

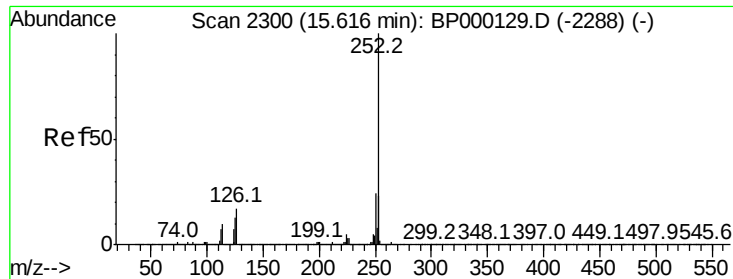

#91

Benzo(a)pyrene

Concen: 13.226 ng/u1

RT: 15.61 min Scan# 2299

Delta R.T. -0.01 min

Lab File: BP000146.D

Acq: 09 Sep 2019 20:51

Instrument :

BNA_P

ClientSampled :


Tot Ion:252 Resp: 916059

Ion Ratio Lower Upper

252 100

253 23.4 17.5 26.3




125 12.8 10.2 15.2

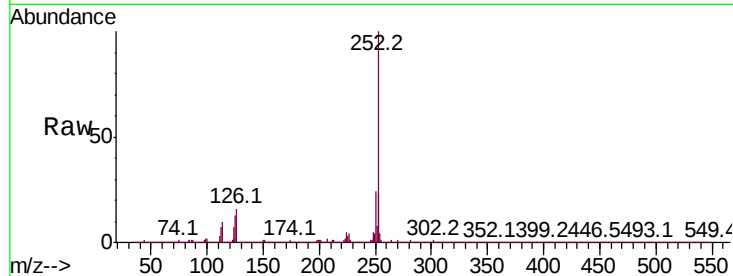

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

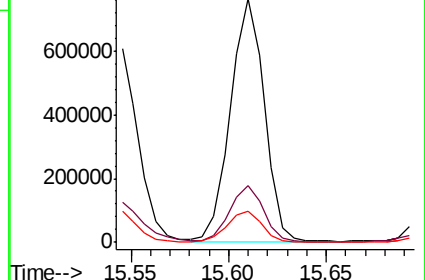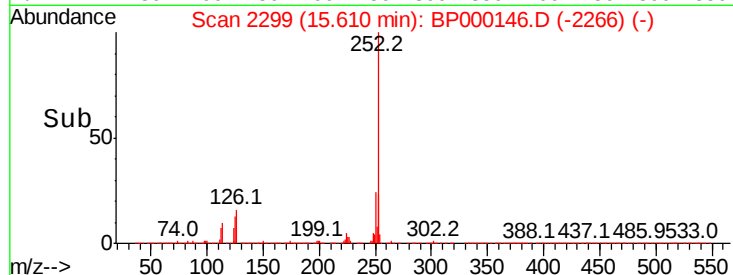

#92

Indeno(1,2,3-cd)pyrene

Concen: 9.622 ng/u1

RT: 17.23 min Scan# 2575

Delta R.T. -0.02 min

Lab File: BP000146.D

Acq: 09 Sep 2019 20:51


Tgt Ion:276 Resp: 766644

Ion Ratio Lower Upper

276 100

138 26.0 20.0 30.0



277 26.0 19.4 29.0




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

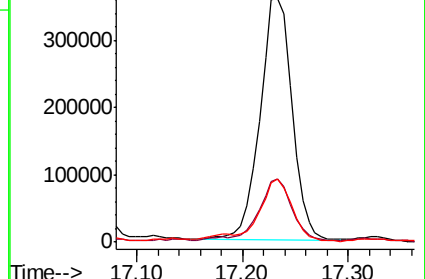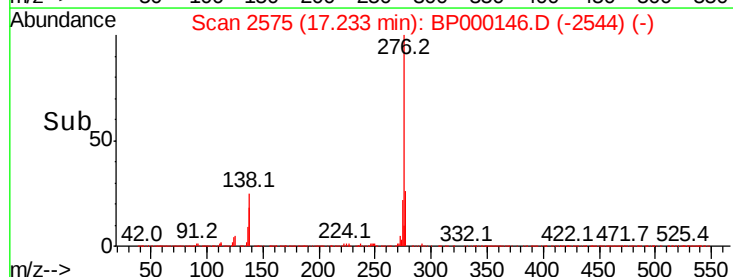

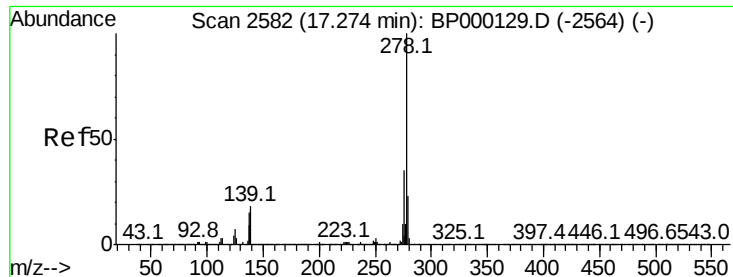

#93

Dibenzo(a,h)anthracene

Concen: 3.093 ng/u1

RT: 17.25 min Scan# 2577

Delta R.T. -0.03 min

Lab File: BP000146.D

Acq: 09 Sep 2019 20:51

Instrument :

BNA_P

ClientSampled :


Tot Ion:278 Resp: 204143

Ion Ratio Lower Upper

278 100

139 20.6 15.1 22.7




279 24.2 19.2 28.8



Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

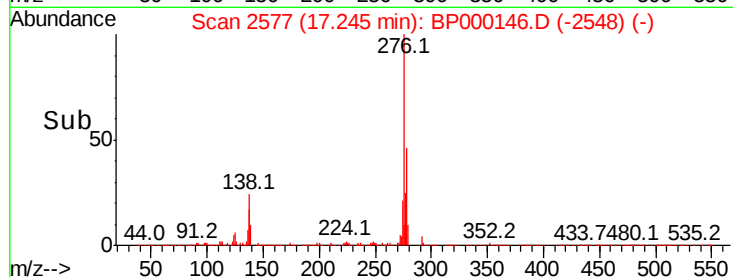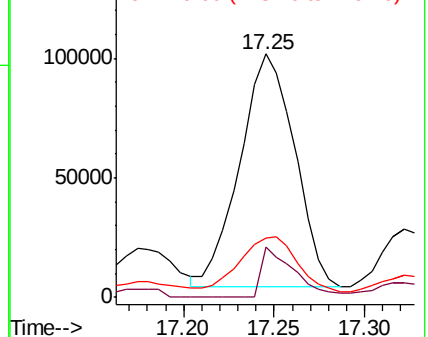

#94

Benzo(g,h,i)perylene

Concen: 10.200 ng/u1

RT: 17.70 min Scan# 2654

Delta R.T. -0.02 min

Lab File: BP000146.D

Acq: 09 Sep 2019 20:51


Tgt Ion:276 Resp: 677657

Ion Ratio Lower Upper

276 100

138 25.2 20.0 30.0

277 22.9 19.1 28.7



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

