

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP090919\
 Data File : BP000132.D
 Acq On : 09 Sep 2019 14:42
 Operator : HP/JU
 Sample : K4708-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB5Q0

Quant Time: Sep 10 03:35:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 02:43:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	428964	20.00	ng/ul	0.00
18) Naphthalene-d8	8.17	136	1673106	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.95	164	932269	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.45	188	1736956	20.00	ng/ul	0.00
78) Chrysene-d12	14.13	240	1507167	20.00	ng/ul	-0.01
86) Perylene-d12	15.67	264	1591261	20.00	ng/ul	-0.01

System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.60	96	48292	3.99	ng/uL	0.00
5) Phenol-d5	6.51	99	820900	22.47	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.57	67	426879	22.34	ng/ul	0.00
9) 2-Chlorophenol-d4	6.66	132	654860	22.16	ng/ul	0.00
13) 4-Methylphenol-d8	7.26	113	623642	22.72	ng/ul	0.00
19) Nitrobenzene-d5	7.45	128	301860	23.76	ng/ul	0.00
22) 2-Nitrophenol-d4	7.77	143	306296	24.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	8.02	165	573839	21.86	ng/ul	0.00
29) 4-Chloroaniline-d4	8.23	131	783168	24.13	ng/ul	0.00
44) Dimethylphthalate-d6	9.63	166	1635846	23.76	ng/ul	0.00
47) Acenaphthylene-d8	9.79	160	1928966	22.67	ng/ul	0.00
52) 4-Nitrophenol-d4	10.03	143	284144	23.10	ng/ul	0.00
58) Fluorene-d10	10.47	176	1366848	23.38	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.52	200	158461	19.85	ng/ul	0.00
71) Anthracene-d10	11.50	188	2102735	25.00	ng/ul	0.00
79) Pyrene-d10	12.89	212	2349063	26.21	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.58	264	2287534	27.73	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	6.52	94	49547	1.301	ng/ul	98
45) Dimethylphthalate	9.65	163	451846	6.505	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP090919\
Data File : BP000132.D
Acq On : 09 Sep 2019 14:42
Operator : HP/JU
Sample : K4708-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB5Q0

Quant Time: Sep 10 03:35:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 02:43:18 2019
Response via : Initial Calibration

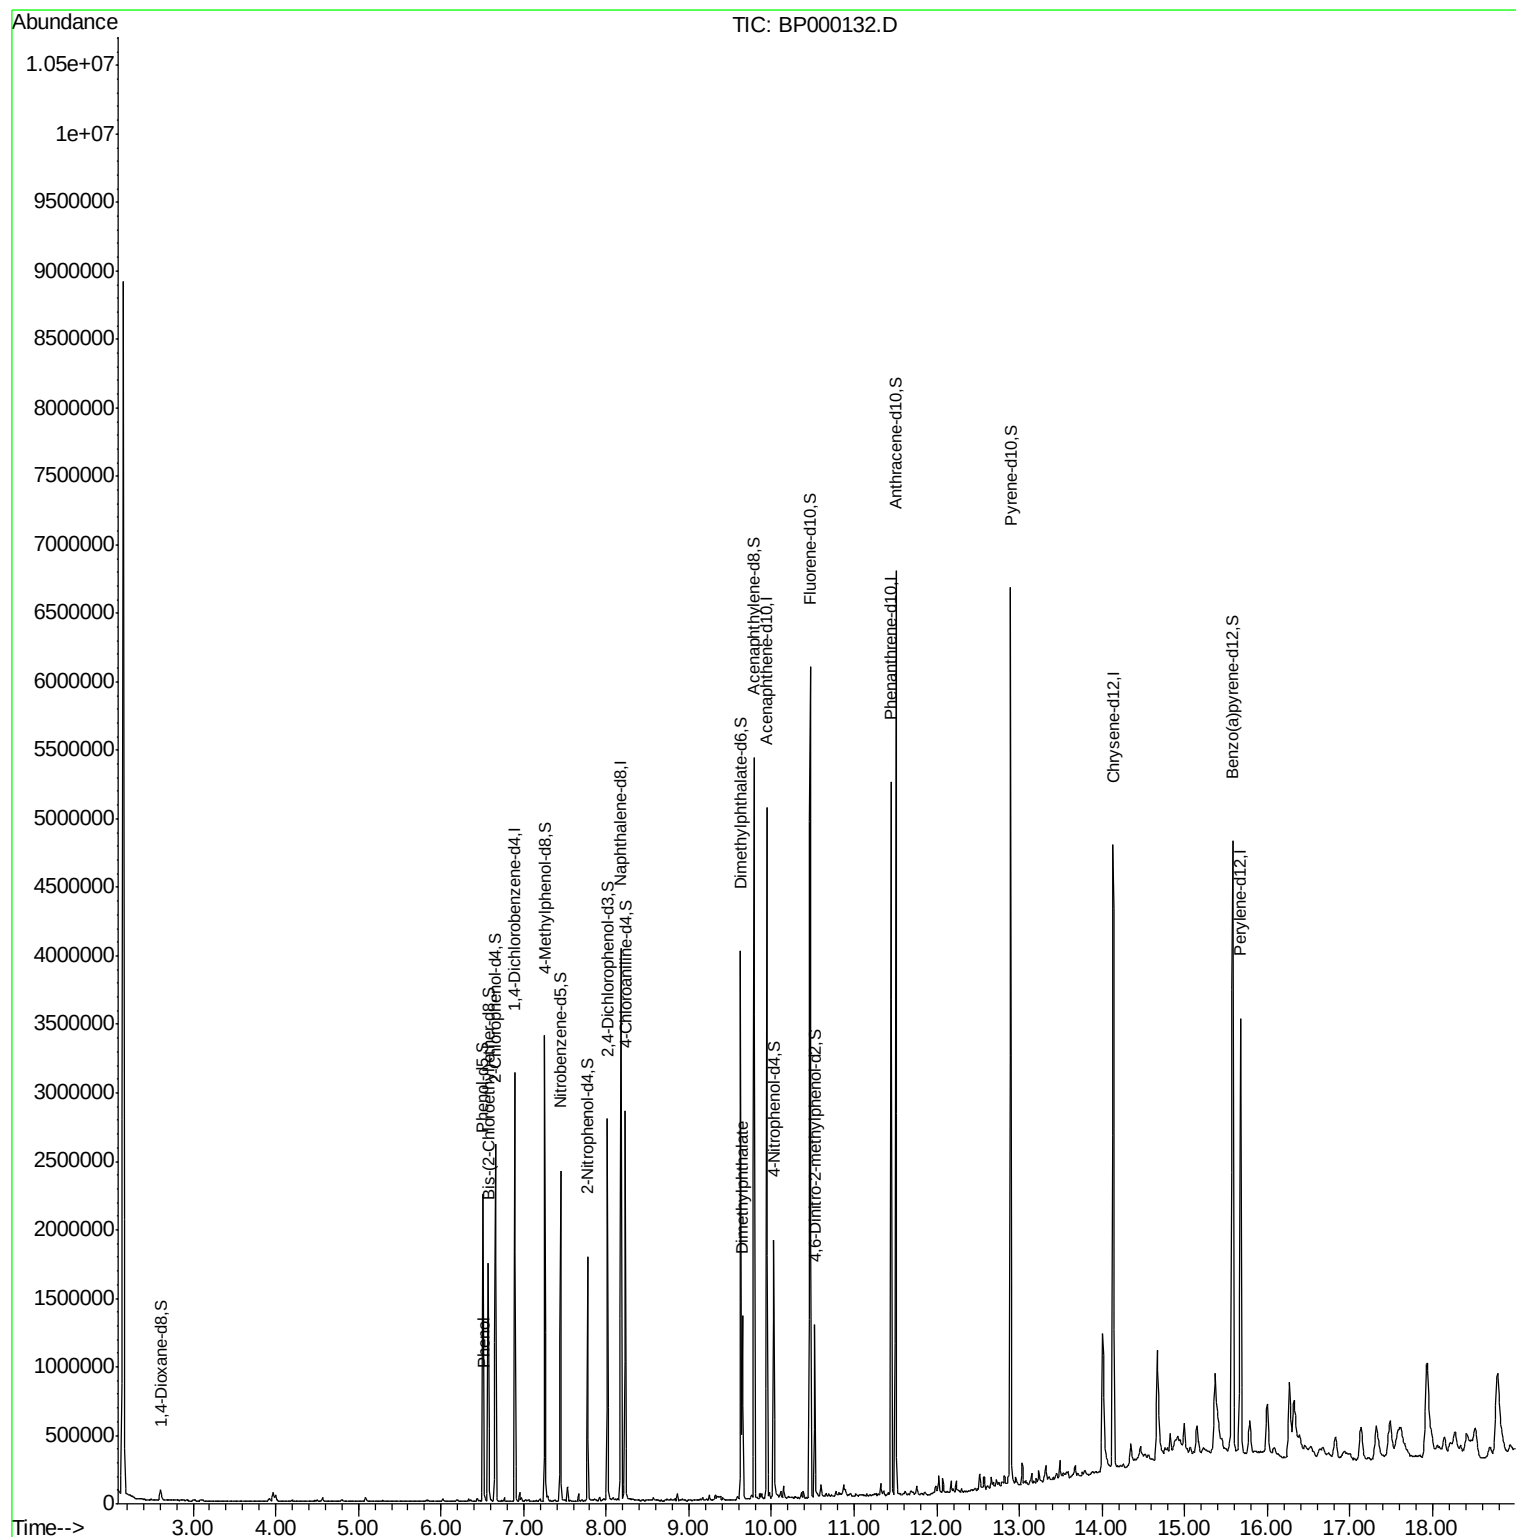

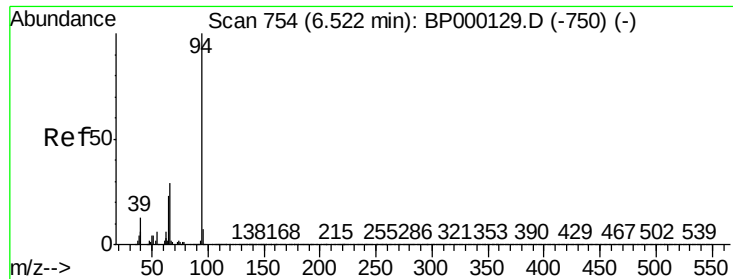

#6

Phenol

Concen: 1.301 ng/ul

RT: 6.52 min Scan# 754

Delta R.T. -0.00 min

Lab File: BP000132.D

Acq: 09 Sep 2019 14:42

Instrument :





BNA_P

ClientSampleId :

CB5Q0

Tot Ion: 94 Resp: 49547

Ion	Ratio	Lower	Upper
94	100		
65	22.6	18.8	28.2
66	28.8	24.2	36.2

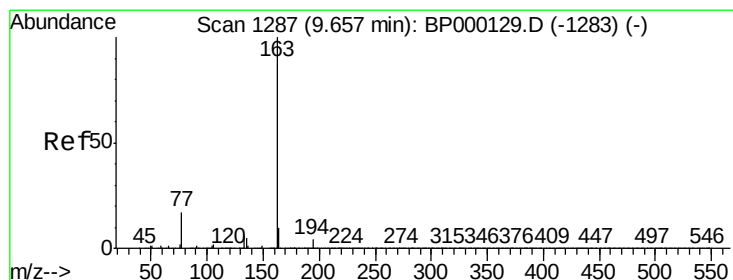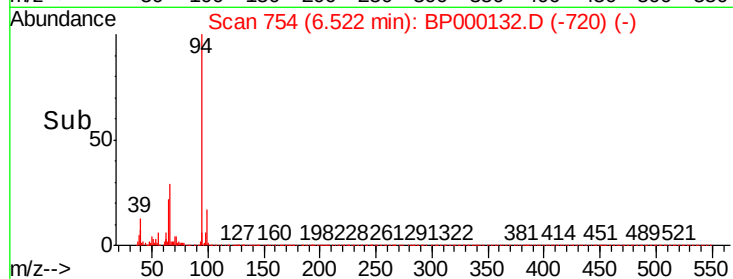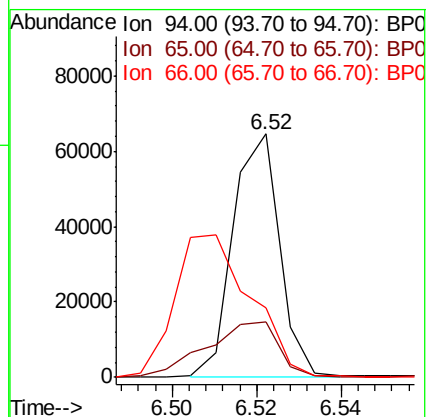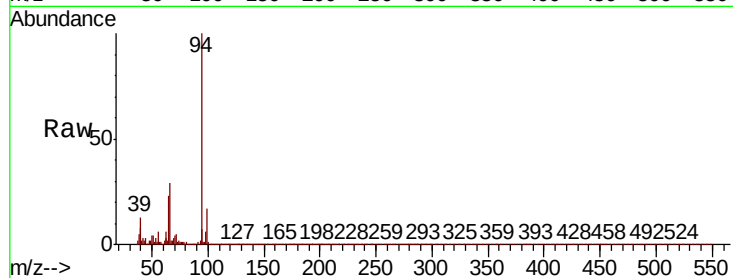

#45

Dimethylphthalate

Concen: 6.505 ng/ul

RT: 9.65 min Scan# 1286

Delta R.T. -0.01 min

Lab File: BP000132.D

Acq: 09 Sep 2019 14:42

Tgt Ion: 163 Resp: 451846

Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.2	4.8
164	10.1	8.4	12.6

