

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP090919\
 Data File : BP000137.D
 Acq On : 09 Sep 2019 16:44
 Operator : HP/JU
 Sample : K4708-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB5Q5

Quant Time: Sep 10 03:36:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 02:43:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	443132	20.00	ng/ul	0.00
18) Naphthalene-d8	8.18	136	1736861	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.95	164	963799	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.45	188	1733533	20.00	ng/ul	0.00
78) Chrysene-d12	14.13	240	1518646	20.00	ng/ul	-0.01
86) Perylene-d12	15.67	264	1602018	20.00	ng/ul	-0.01

System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.60	96	57375	4.59	ng/uL	0.00
5) Phenol-d5	6.50	99	917363	24.30	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.57	67	475140	24.07	ng/ul	0.00
9) 2-Chlorophenol-d4	6.66	132	753545	24.69	ng/ul	0.00
13) 4-Methylphenol-d8	7.26	113	703971	24.83	ng/ul	0.00
19) Nitrobenzene-d5	7.45	128	347706	26.37	ng/ul	0.00
22) 2-Nitrophenol-d4	7.78	143	355655	27.70	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	8.02	165	635733	23.33	ng/ul	0.00
29) 4-Chloroaniline-d4	8.23	131	926784	27.50	ng/ul	0.00
44) Dimethylphthalate-d6	9.63	166	1695408	23.82	ng/ul	0.00
47) Acenaphthylene-d8	9.79	160	2092071	23.79	ng/ul	0.00
52) 4-Nitrophenol-d4	10.03	143	293553	23.08	ng/ul	0.00
58) Fluorene-d10	10.47	176	1450040	23.99	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.52	200	159536	20.02	ng/ul	0.00
71) Anthracene-d10	11.50	188	2081978	24.80	ng/ul	0.00
79) Pyrene-d10	12.89	212	2149506	23.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.58	264	2033053	24.48	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	9.65	163	227129	3.163	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP090919\
Data File : BP000137.D
Acq On : 09 Sep 2019 16:44
Operator : HP/JU
Sample : K4708-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB5Q5

Quant Time: Sep 10 03:36:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 02:43:18 2019
Response via : Initial Calibration

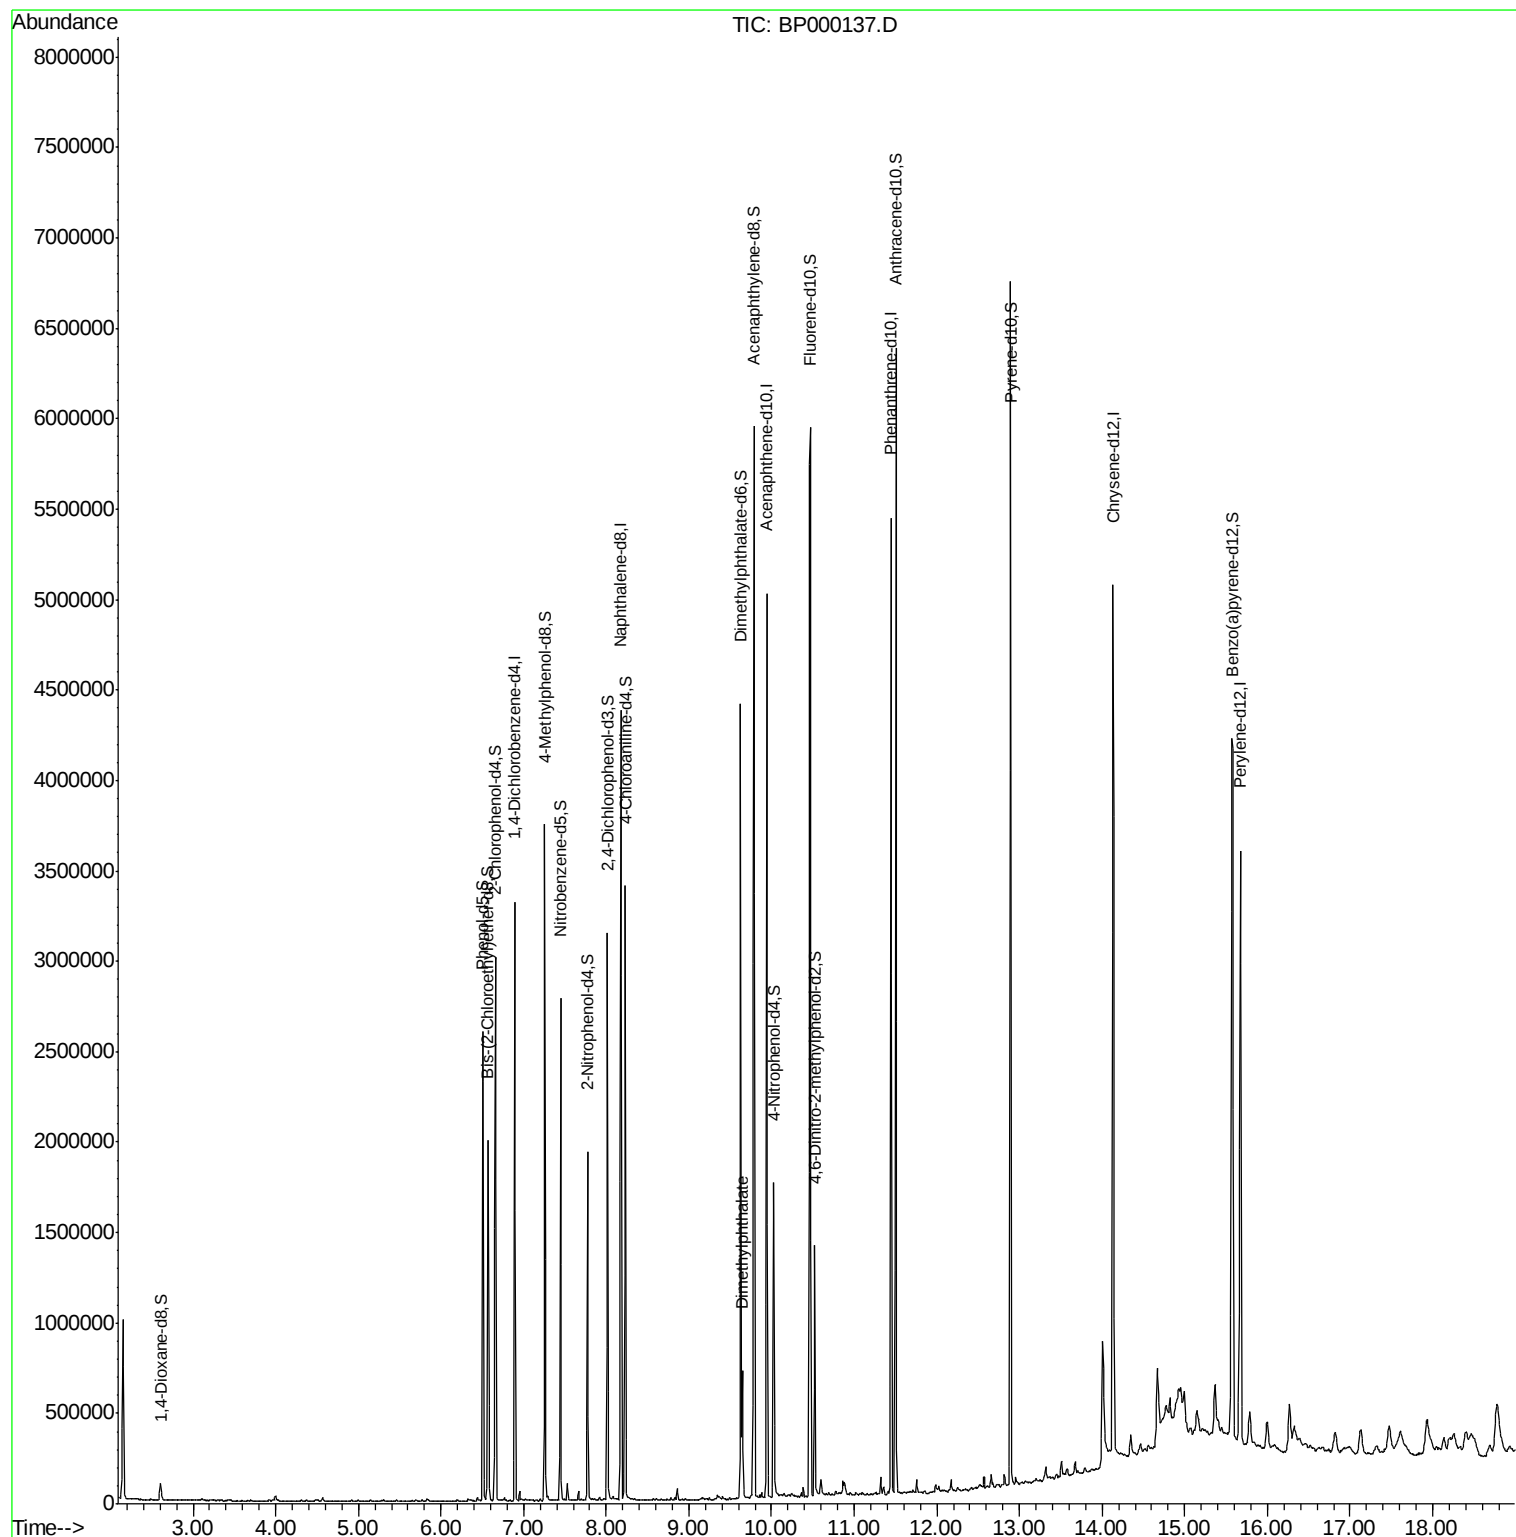

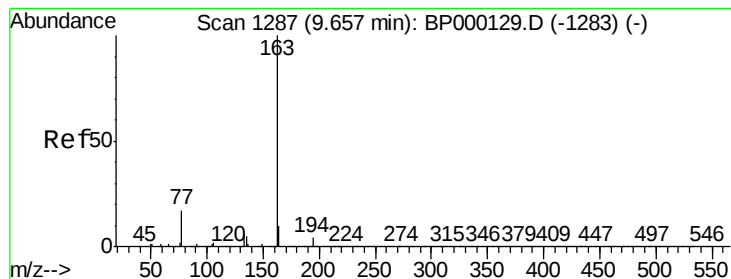

#45

Dimethylphthalate

Concen: 3.163 ng/ul

RT: 9.65 min Scan# 1286

Delta R.T. -0.01 min

Lab File: BP000137.D

Acq: 09 Sep 2019 16:44

Instrument :

BNA_P

ClientSampleId :

CB5Q5


Tot Ion:163 Resp: 227129

Ion Ratio Lower Upper

163 100

194 4.1 3.2 4.8

164 10.1 8.4 12.6

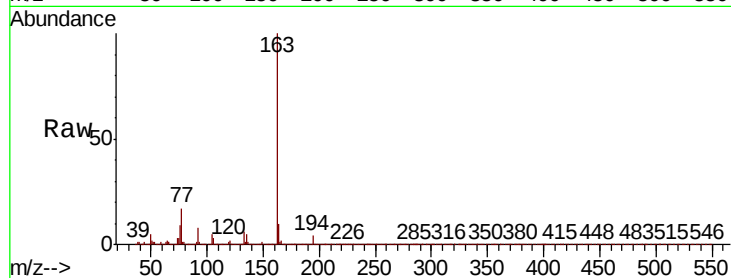

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

