


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006895.D
Acq On : 09 Sep 2021 12:07
Operator : CG/JU
Sample : PB138843BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK843

Manual Integrations
APPROVED

mohammad
9/10/2021 3:25:53 PM

Quant Time: Sep 09 12:43:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION
Qlast Update : Thu Sep 09 11:07:24 2021
Response via : Initial Calibration

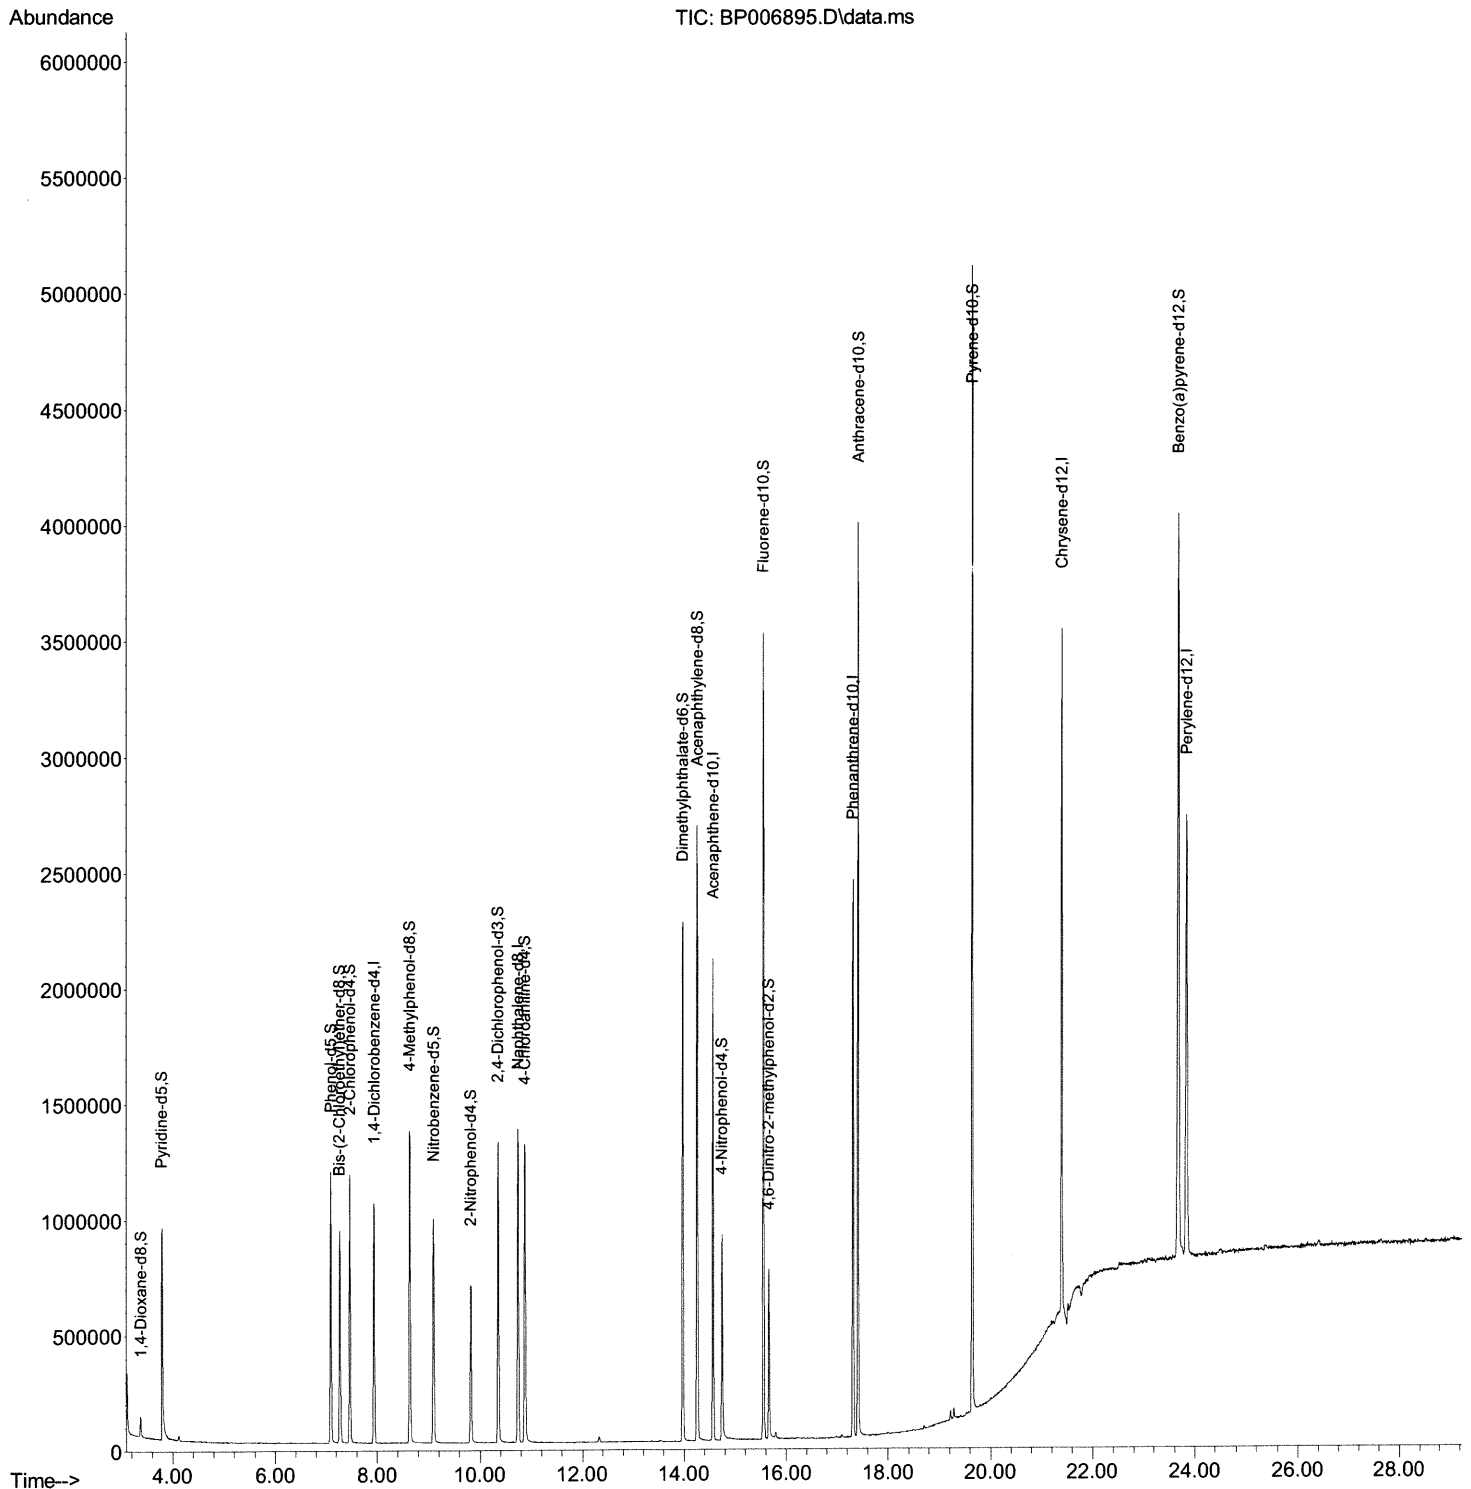

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006895.D
 Acq On : 09 Sep 2021 12:07
 Operator : CG/JU
 Sample : PB138843BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK843

Manual Integrations
 APPROVED

mohammad
 9/10/2021 3:25:53 PM

Quant Time: Sep 09 12:43:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 09 11:07:24 2021
 Response via : Initial Calibration

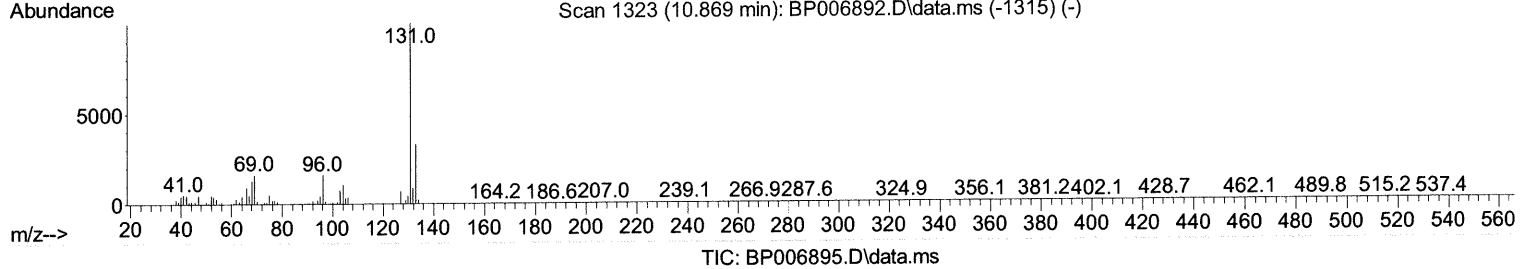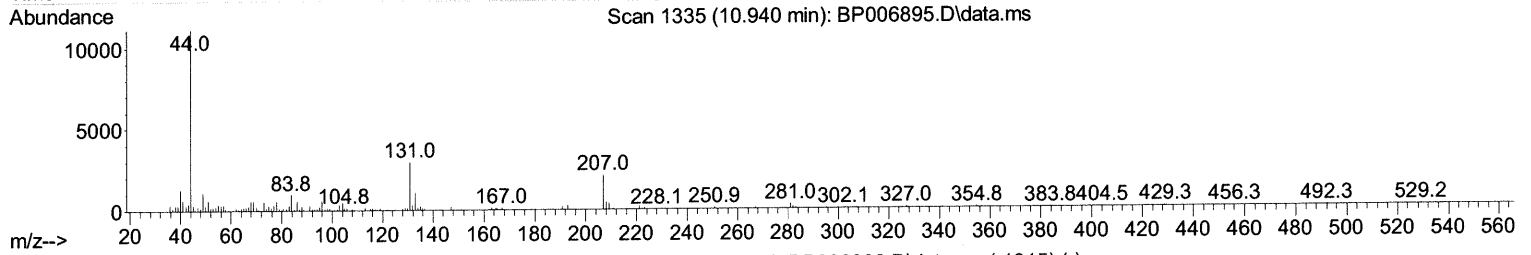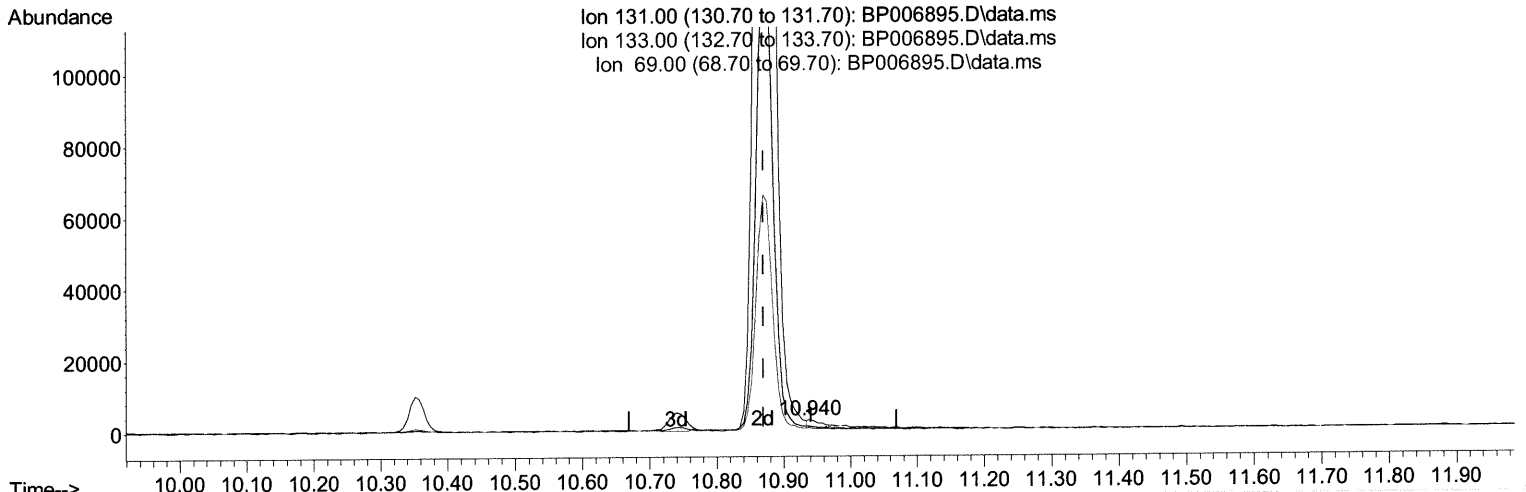

(31) 4-Chloroaniline-d4 (S)

10.940min (+ 0.071) 0.11 ng/ul

response 2465

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.90	37.55
69.00	20.40	19.16
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006895.D
Acq On : 09 Sep 2021 12:07
Operator : CG/JU
Sample : PB138843BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK843

Manual Integrations
APPROVED

mohammad
9/10/2021 3:25:53 PM

Quant Time: Sep 09 12:43:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 09 11:07:24 2021
Response via : Initial Calibration

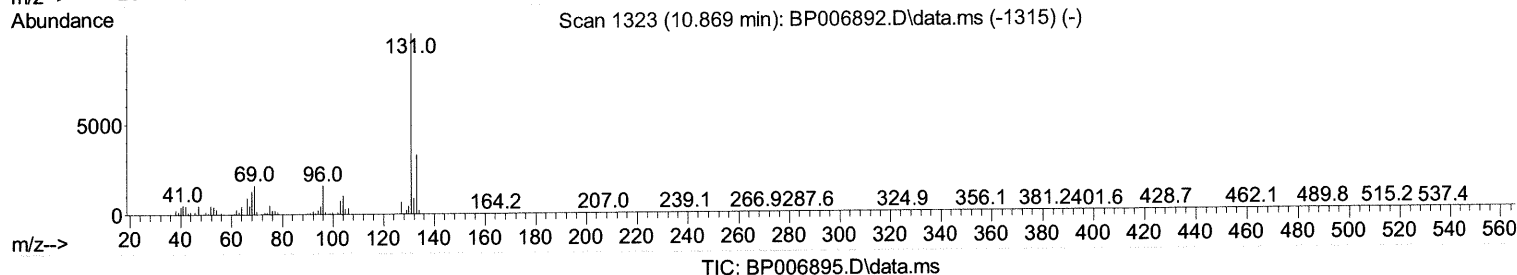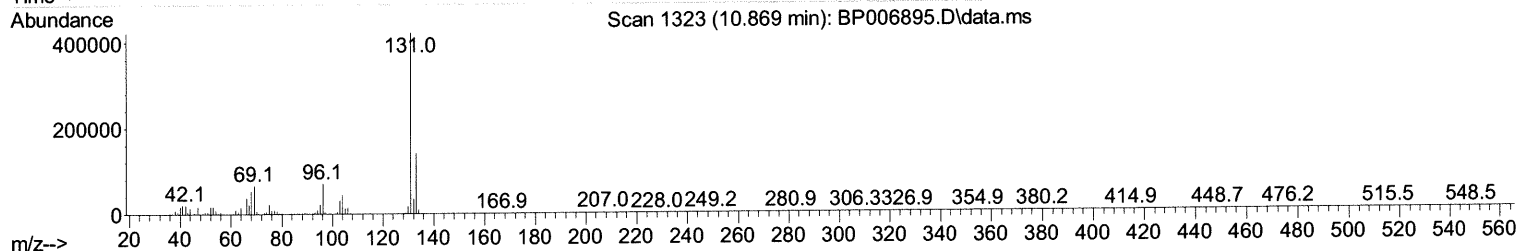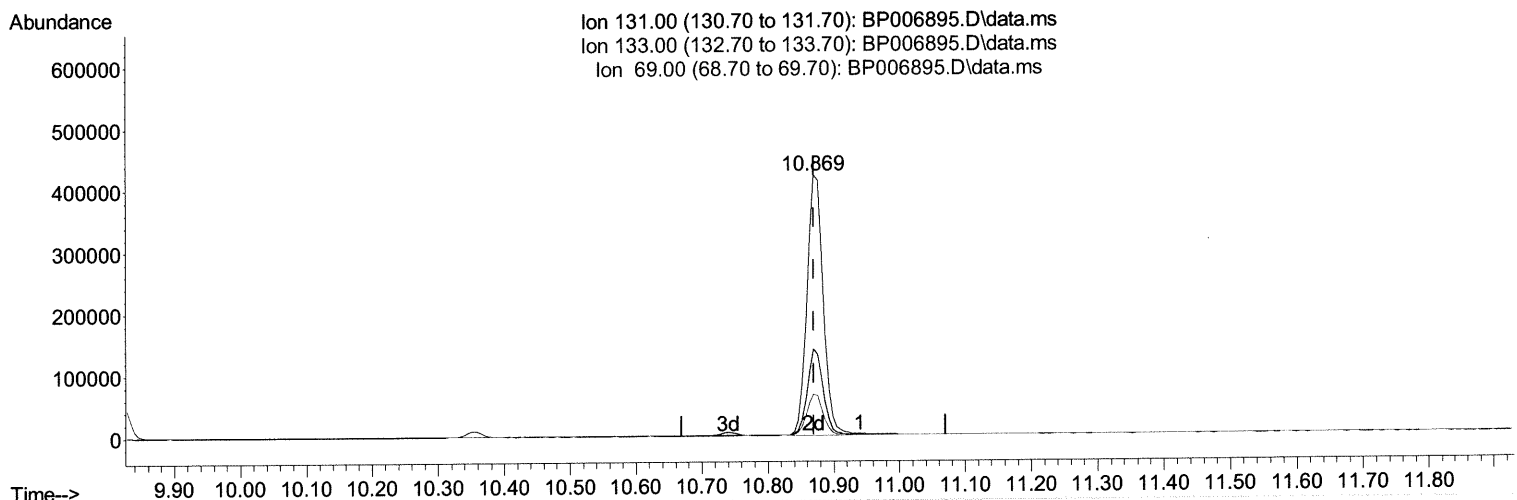

TIC: BP006895.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.869min (-0.000) 32.62 ng/ul m 09/13/21 JU

response 727998

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.90	33.13
69.00	20.40	15.64#
0.00	0.00	0.00

Instrument :
BNA_P
ClientSampleId :
SBLK843

Manual Integrations

mohammad
9/10/2021 3:25:53 PM

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	295218	20.000	ng/ul	0.00
20) Naphthalene-d8	10.740	136	1147674	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.563	164	707417	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.310	188	1442669	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.392	240	1394617	20.000	ng/ul	0.00
88) Perylene-d12	23.833	264	1423812	20.000	ng/ul	0.00

3)	1,4-Dioxane-d8	3.370	96	47514	6.405	ng/ul	0.00
4)	Pyridine-d5	3.781	84	596636	30.863	ng/ul	0.00
7)	Phenol-d5	7.093	99	689789	31.791	ng/ul	0.00
9)	Bis-(2-Chloroethyl)eth...	7.263	67	411838	33.049	ng/ul	0.00
11)	2-Chlorophenol-d4	7.463	132	563362	32.162	ng/ul	0.00
15)	4-Methylphenol-d8	8.634	113	531486	31.192	ng/ul	0.00
21)	Nitrobenzene-d5	9.099	128	249783	35.932	ng/ul	0.00
24)	2-Nitrophenol-d4	9.816	143	240237	35.102	ng/ul	0.00
28)	2,4-Dichlorophenol-d3	10.352	165	499130	30.930	ng/ul	0.00
31)	4-Chloroaniline-d4	10.869	131	727998m	32.621	ng/ul	0.00
46)	Dimethylphthalate-d6	13.975	166	1590494	34.713	ng/ul	0.00
49)	Acenaphthylene-d8	14.257	160	1923721	33.151	ng/ul	0.00
54)	4-Nitrophenol-d4	14.740	143	213524	26.825	ng/ul	0.00
60)	Fluorene-d10	15.551	176	1358229	33.588	ng/ul	0.00
65)	4,6-Dinitro-2-methylph...	15.663	200	163365	25.598	ng/ul	0.00
73)	Anthracene-d10	17.410	188	2202885	36.883	ng/ul	0.00
81)	Pyrene-d10	19.639	212	2531731	38.763	ng/ul	0.00
92)	Benzo(a)pyrene-d12	23.674	264	2428624	35.357	ng/ul	0.00

(#) = qualifier out of range (m) = manual integration (+) = signals summed