


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006958.D
Acq On : 11 Sep 2021 00:52
Operator : CG/JU
Sample : M3651-15
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKM9

Manual Integrations
APPROVED

mohammad
9/13/2021 10:22:36 AM

Quant Time: Sep 11 01:59:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 09 11:07:24 2021
Response via : Initial Calibration

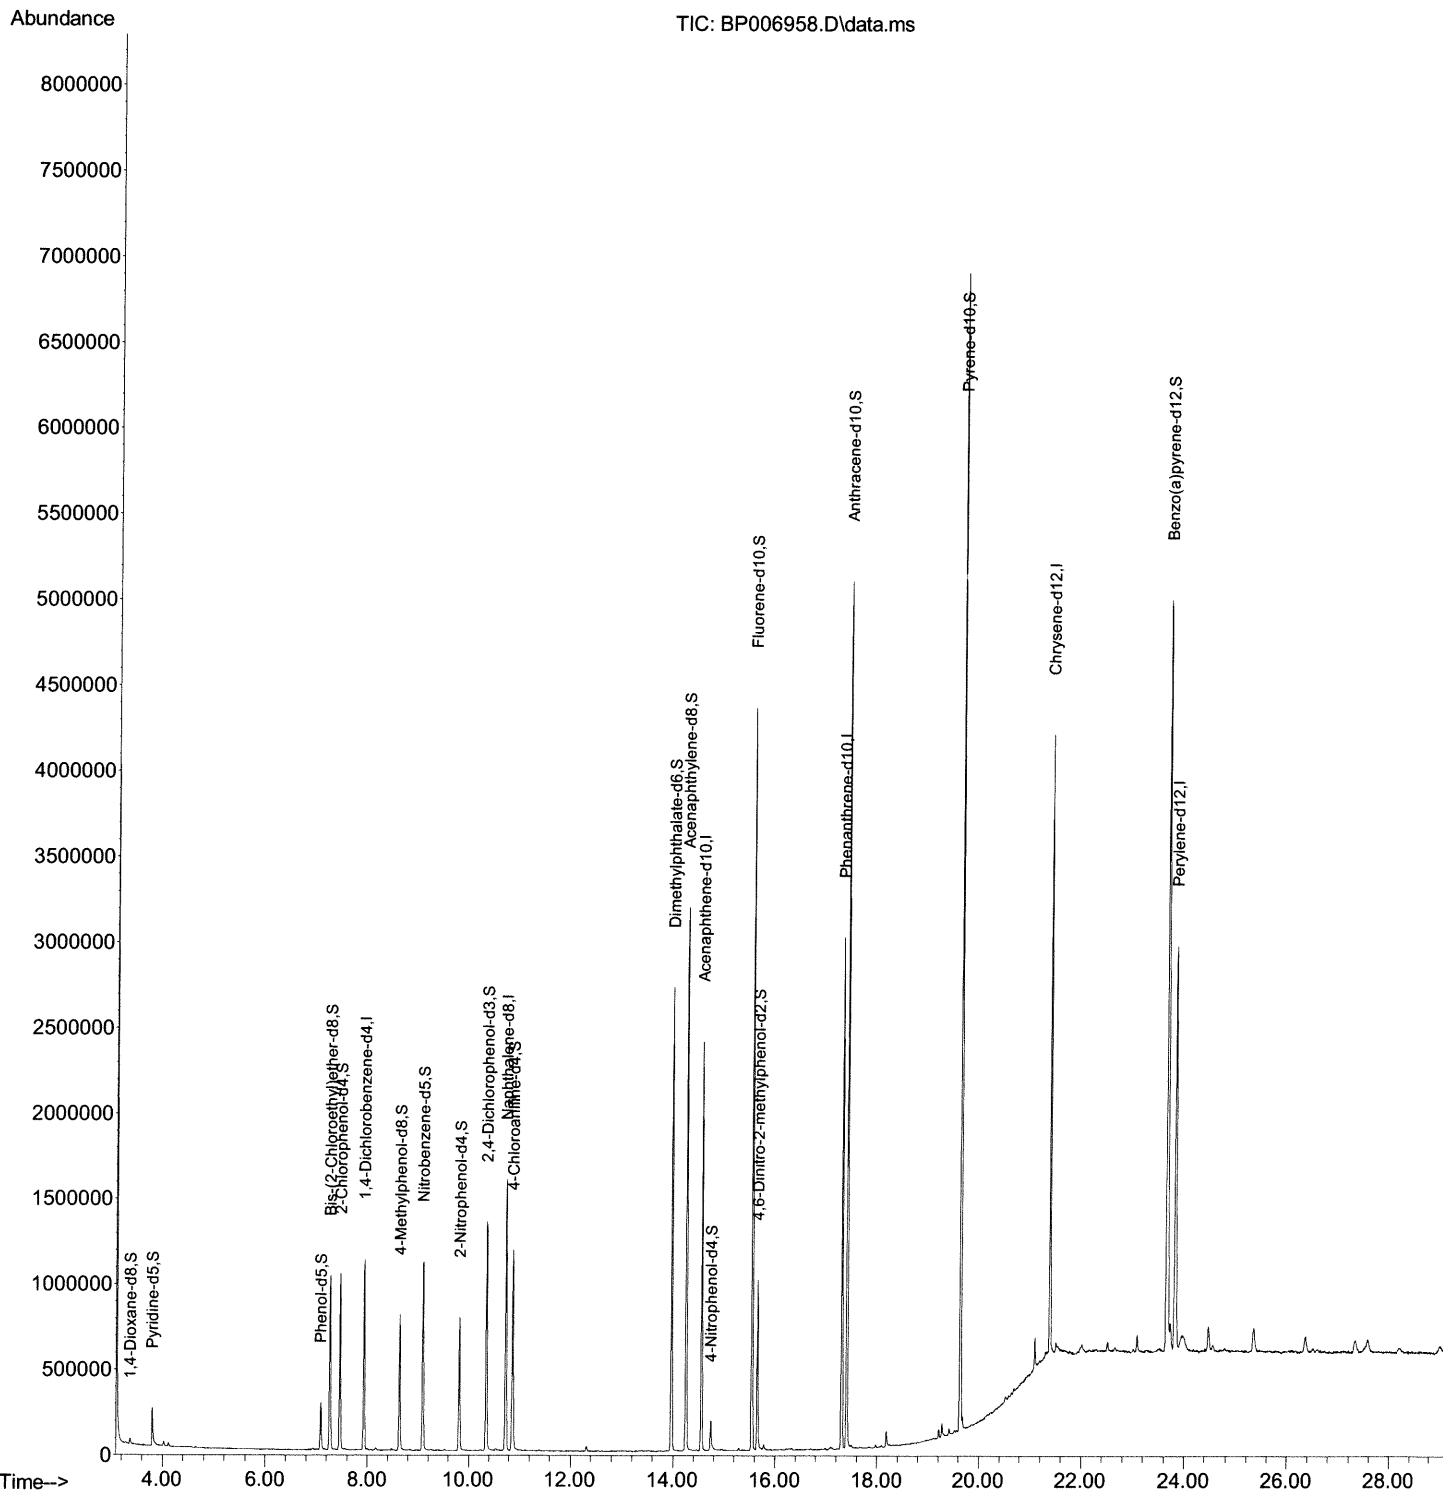

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006958.D
 Acq On : 11 Sep 2021 00:52
 Operator : CG/JU
 Sample : M3651-15
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBKM9

Manual Integrations
 APPROVED

mohammad
 9/13/2021 10:22:36 AM

Quant Time: Sep 11 01:59:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 09 11:07:24 2021
 Response via : Initial Calibration

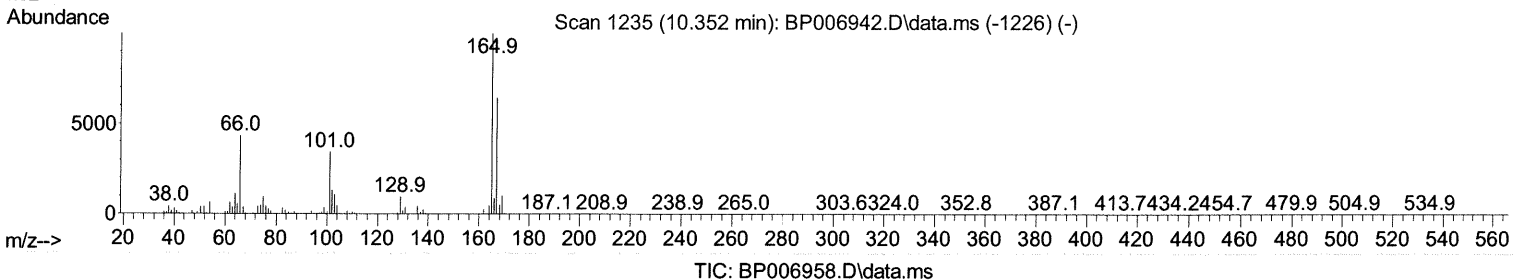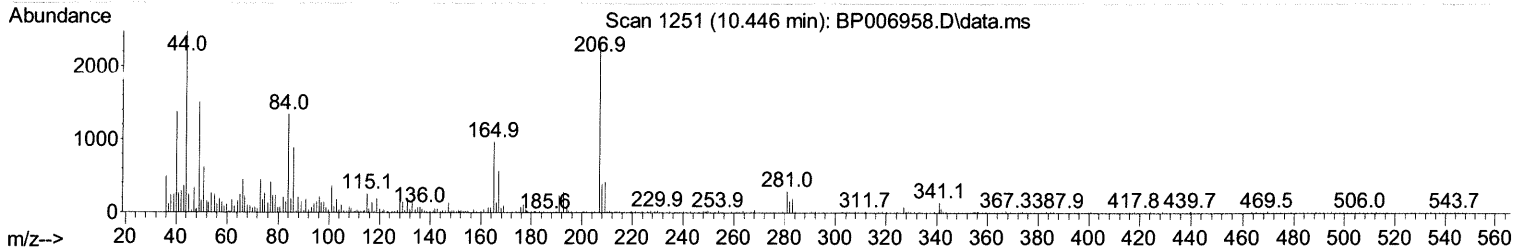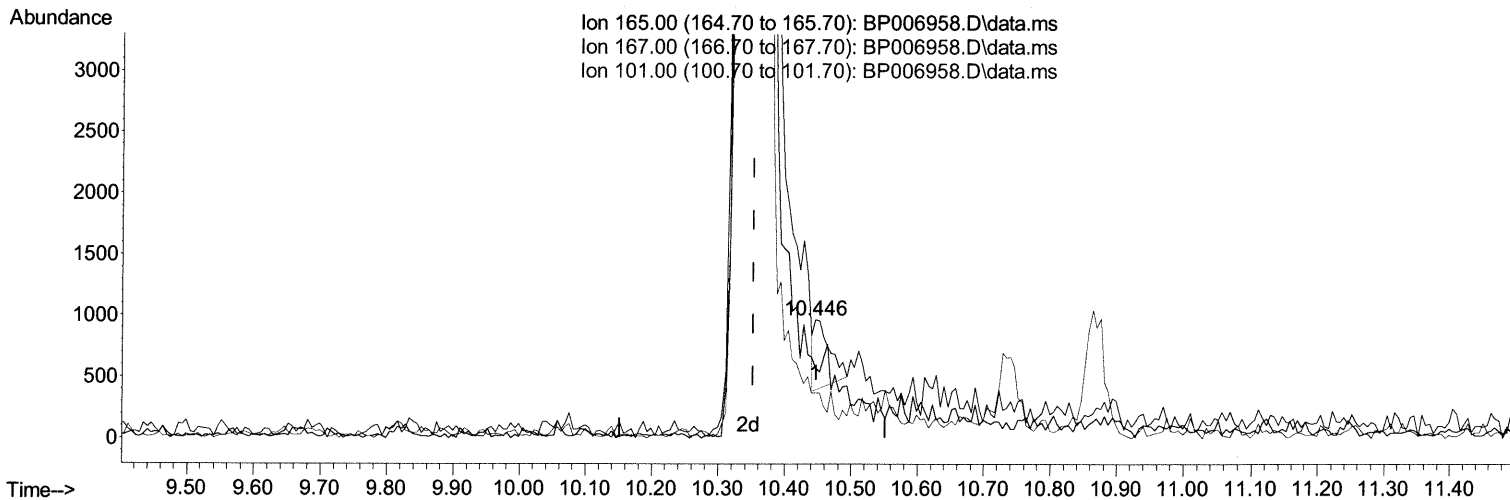

(28) 2,4-Dichlorophenol-d3 (S)

10.446min (+ 0.094) 0.05 ng/ul

response 929

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	62.40	59.52
101.00	40.60	38.20
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006958.D
 Acq On : 11 Sep 2021 00:52
 Operator : CG/JU
 Sample : M3651-15
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBKM9

Manual Integrations
 APPROVED

mohammad
 9/13/2021 10:22:36 AM

Quant Time: Sep 11 01:59:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 09 11:07:24 2021
 Response via : Initial Calibration

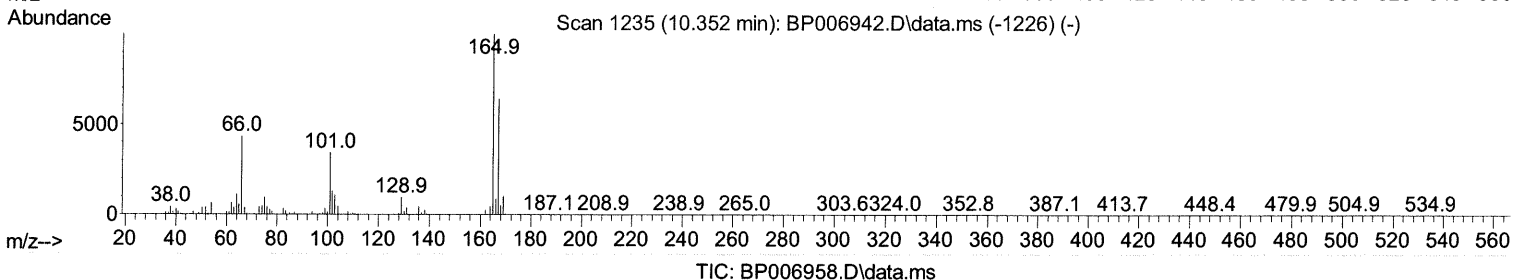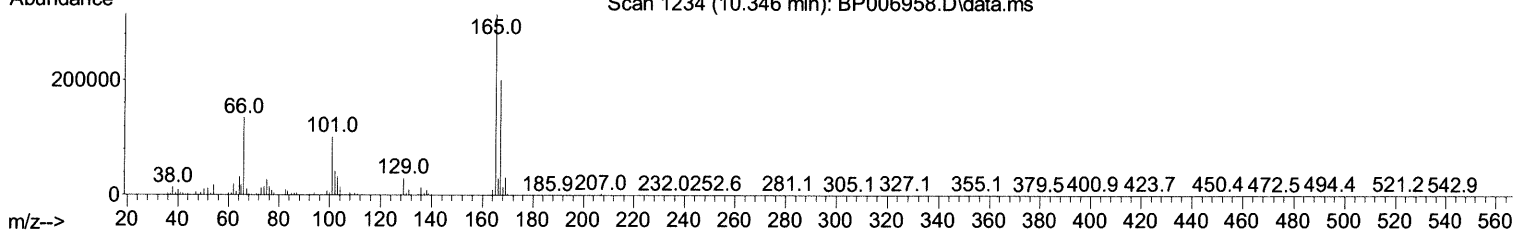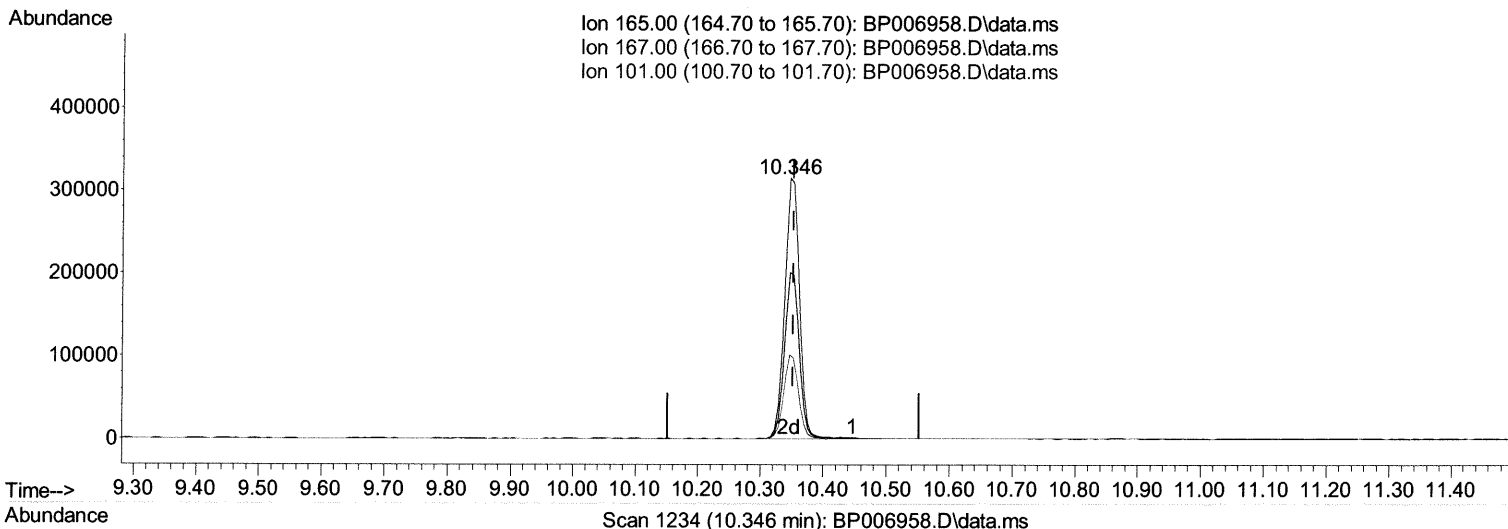

(28) 2,4-Dichlorophenol-d3 (S)

10.346min (-0.006) 28.46 ng/ul m 09/14/21 JU

response 520456

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	62.40	63.72
101.00	40.60	32.25#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006958.D
 Acq On : 11 Sep 2021 00:52
 Operator : CG/JU
 Sample : M3651-15
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBKM9

Manual Integrations
 APPROVED

mohammad
 9/13/2021 10:22:36 AM

Quant Time: Sep 11 01:59:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 09 11:07:24 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	317415	20.000	ng/ul	0.00
20) Naphthalene-d8	10.734	136	1300360	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.557	164	815041	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.304	188	1722717	20.000	ng/ul	#-0.01
79) Chrysene-d12	21.381	240	1714515	20.000	ng/ul	-0.02
88) Perylene-d12	23.816	264	1757105	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	16732	2.098	ng/uL	0.00
4) Pyridine-d5	3.793	84	143565	6.907	ng/ul	0.01
7) Phenol-d5	7.087	99	169750	7.276	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.264	67	445717	33.266	ng/ul	0.00
11) 2-Chlorophenol-d4	7.464	132	487976	25.910	ng/ul	0.00
15) 4-Methylphenol-d8	8.634	113	304590	16.626	ng/ul	0.00
21) Nitrobenzene-d5	9.093	128	280611	35.627	ng/ul	0.00
24) 2-Nitrophenol-d4	9.816	143	265779	34.275	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.346	165	520456m >	28.464	ng/ul >	0.00 Gq//4/17J
31) 4-Chloroaniline-d4	10.863	131	676721	26.763	ng/ul	0.00
46) Dimethylphthalate-d6	13.969	166	1850760	35.060	ng/ul	0.00
49) Acenaphthylene-d8	14.251	160	2225597	33.289	ng/ul	0.00
54) 4-Nitrophenol-d4	14.740	143	46644	5.086	ng/ul	0.00
60) Fluorene-d10	15.546	176	1667072	35.782	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.657	200	211255	27.721	ng/ul	-0.01
73) Anthracene-d10	17.404	188	2861121	40.116	ng/ul	-0.01
81) Pyrene-d10	19.634	212	3397795	42.316	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.657	264	3314359	39.099	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed