

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006898.D
 Acq On : 09 Sep 2021 13:50
 Operator : CG/JU
 Sample : M3573-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ESQK5

Quant Time: Sep 09 16:25:14 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 09 11:07:24 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	248876	20.000	ng/u1	0.00
20) Naphthalene-d8	10.740	136	1020273	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.563	164	646233	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.310	188	1382198	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.392	240	1394121	20.000	ng/u1	0.00
88) Perylene-d12	23.827	264	1459515	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	32034	5.122	ng/uL	0.00
4) Pyridine-d5	3.793	84	150229	9.218	ng/u1	0.01
7) Phenol-d5	7.093	99	134205	7.337	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	350545	33.368	ng/u1	0.00
11) 2-Chlorophenol-d4	7.469	132	383694	25.983	ng/u1	0.00
15) 4-Methylphenol-d8	8.640	113	250222	17.420	ng/u1	0.00
21) Nitrobenzene-d5	9.099	128	222186	35.953	ng/u1	0.00
24) 2-Nitrophenol-d4	9.822	143	211728	34.800	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.357	165	415880	28.989	ng/u1	0.00
31) 4-Chloroaniline-d4	10.869	131	567780	28.619	ng/u1	0.00
46) Dimethylphthalate-d6	13.975	166	1573451	37.593	ng/u1	0.00
49) Acenaphthylene-d8	14.257	160	1791773	33.801	ng/u1	0.00
54) 4-Nitrophenol-d4	14.740	143	38630	5.313	ng/u1	0.00
60) Fluorene-d10	15.551	176	1338829	36.243	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.663	200	182246	29.806	ng/u1	0.00
73) Anthracene-d10	17.410	188	2288269	39.988	ng/u1	0.00
81) Pyrene-d10	19.639	212	2728180	41.785	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.668	264	2656278	37.725	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.405	88	13897	1.997	ng/uL	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006898.D
Acq On : 09 Sep 2021 13:50
Operator : CG/JU
Sample : M3573-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ESQK5

Quant Time: Sep 09 16:25:14 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 09 11:07:24 2021
Response via : Initial Calibration

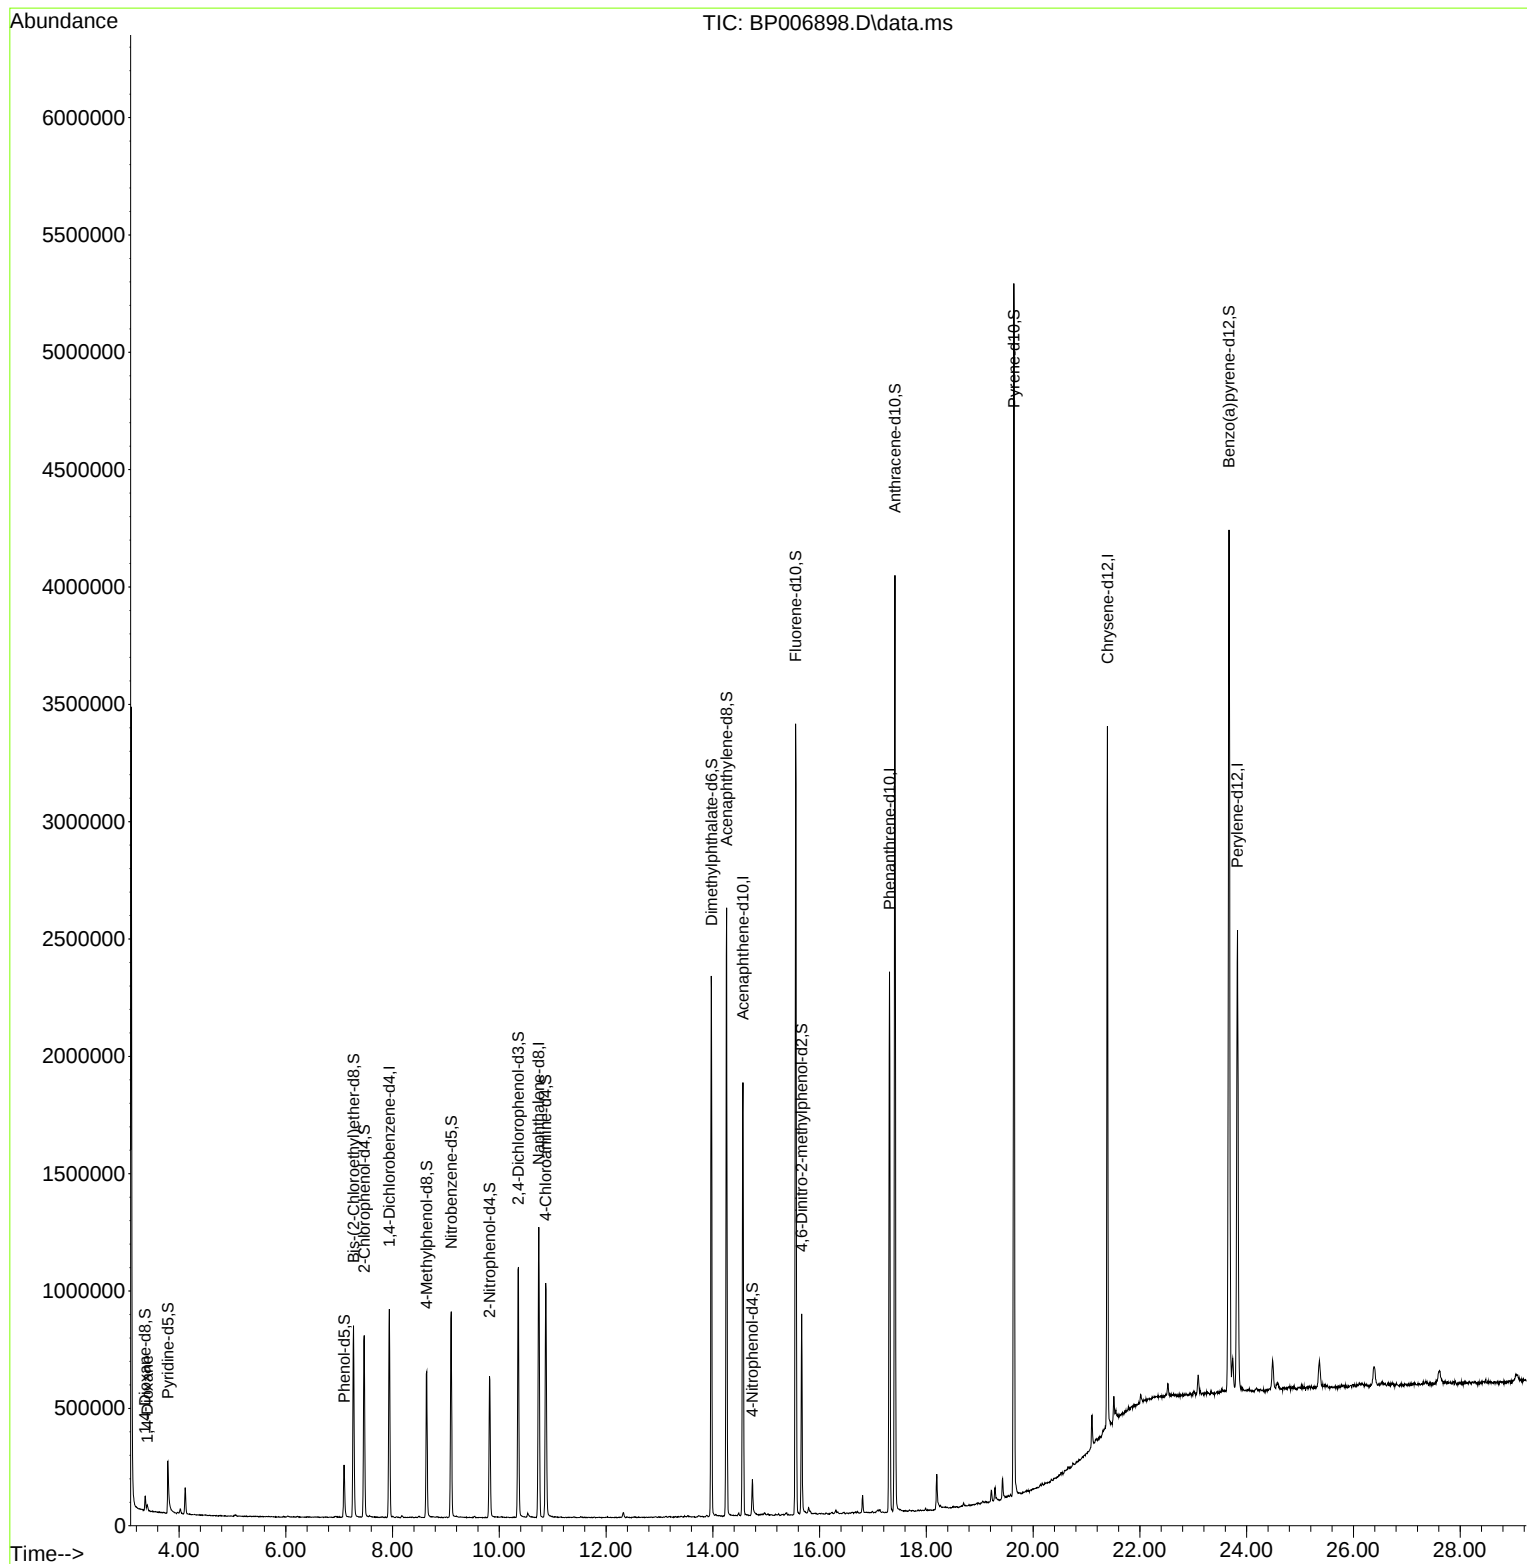

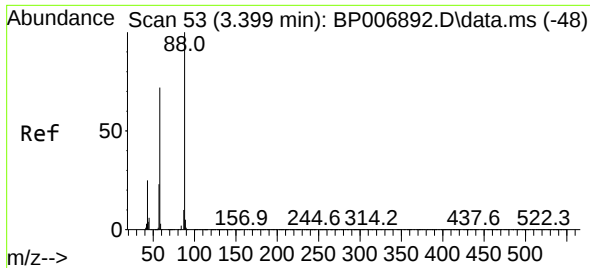

#2
 1,4-Dioxane
 Concen: 1.997 ng/uL
 RT: 3.405 min Scan# 54
 Delta R.T. 0.006 min
 Lab File: BP006898.D
 Acq: 09 Sep 2021 13:50

Instrument :
 BNA_P
 ClientSampleId :
 ESQK5

Tgt Ion: 88 Resp: 13897
 Ion Ratio Lower Upper
 88 100
 43 26.6 20.1 30.1
 58 62.0 48.4 72.6

