

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006893.D
 Acq On : 09 Sep 2021 10:47
 Operator : CG/JU
 Sample : PB138822BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK822

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006893.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	44	47	56	rVB	80551	114295	1.68%	0.174%
2	3.781	116	118	138	rBV	860513	1384369	20.40%	2.110%
3	4.116	171	175	180	rVB	22444	30278	0.45%	0.046%
4	7.093	674	681	693	rBV	1023727	1574600	23.20%	2.400%
5	7.269	704	711	722	rBV	847234	1354832	19.96%	2.065%
6	7.463	738	744	758	rBV	1046449	1677986	24.73%	2.558%
7	7.940	816	825	836	rBV	917225	1485922	21.89%	2.265%
8	8.634	937	943	962	rBV	1218057	2002584	29.51%	3.052%
9	9.093	1014	1021	1033	rBV	881298	1481585	21.83%	2.258%
10	9.816	1137	1144	1153	rBV	592847	1013070	14.93%	1.544%
11	10.210	1206	1211	1215	rVB8	3672	7320	0.11%	0.011%
12	10.351	1227	1235	1252	rBV	1196491	1997953	29.44%	3.045%
13	10.740	1292	1301	1311	rBV	1281511	2112048	31.12%	3.219%
14	10.869	1314	1323	1339	rBV	1196544	2071757	30.53%	3.158%
15	12.322	1565	1570	1576	rVB2	20846	36252	0.53%	0.055%
16	13.292	1731	1735	1739	rBV6	4553	8605	0.13%	0.013%
17	13.539	1773	1777	1783	rVB9	6356	9371	0.14%	0.014%
18	13.969	1844	1850	1865	rBV	2229587	3162466	46.60%	4.820%
19	14.257	1891	1899	1916	rBV	2483281	3705808	54.60%	5.649%
20	14.563	1943	1951	1961	rBV	1951337	2833131	41.75%	4.318%
21	14.739	1974	1981	1999	rBV	856394	1278488	18.84%	1.949%
22	15.551	2112	2119	2130	rBV	3271586	4755914	70.08%	7.249%
23	15.663	2133	2138	2154	rVV	695907	1002198	14.77%	1.528%
24	15.792	2156	2160	2165	rVB2	24590	40601	0.60%	0.062%
25	16.345	2248	2254	2257	rBV7	8075	11947	0.18%	0.018%
26	17.098	2378	2382	2386	rVB3	10559	14683	0.22%	0.022%
27	17.310	2411	2418	2427	rBV	2408343	3390965	49.97%	5.169%
28	17.410	2428	2435	2448	rBV	3825101	5356002	78.92%	8.164%
29	19.216	2739	2742	2747	rBV2	39333	51263	0.76%	0.078%
30	19.286	2750	2754	2758	rVV2	45053	63237	0.93%	0.096%
31	19.639	2808	2814	2820	rBV	4993655	6507828	95.89%	9.919%
32	21.392	3107	3112	3128	rVB	2965118	4140549	61.01%	6.311%
33	23.668	3492	3499	3508	rBV2	3392093	6786582	100.00%	10.344%
34	23.827	3520	3526	3538	rVB2	2022574	4142186	61.03%	6.314%

Sum of corrected areas: 65606675

Instrument :

BNA_P

ClientSampleId :




SBLK822

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006893.D
Acq On : 09 Sep 2021 10:47
Operator : CG/JU
Sample : PB138822BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK822

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

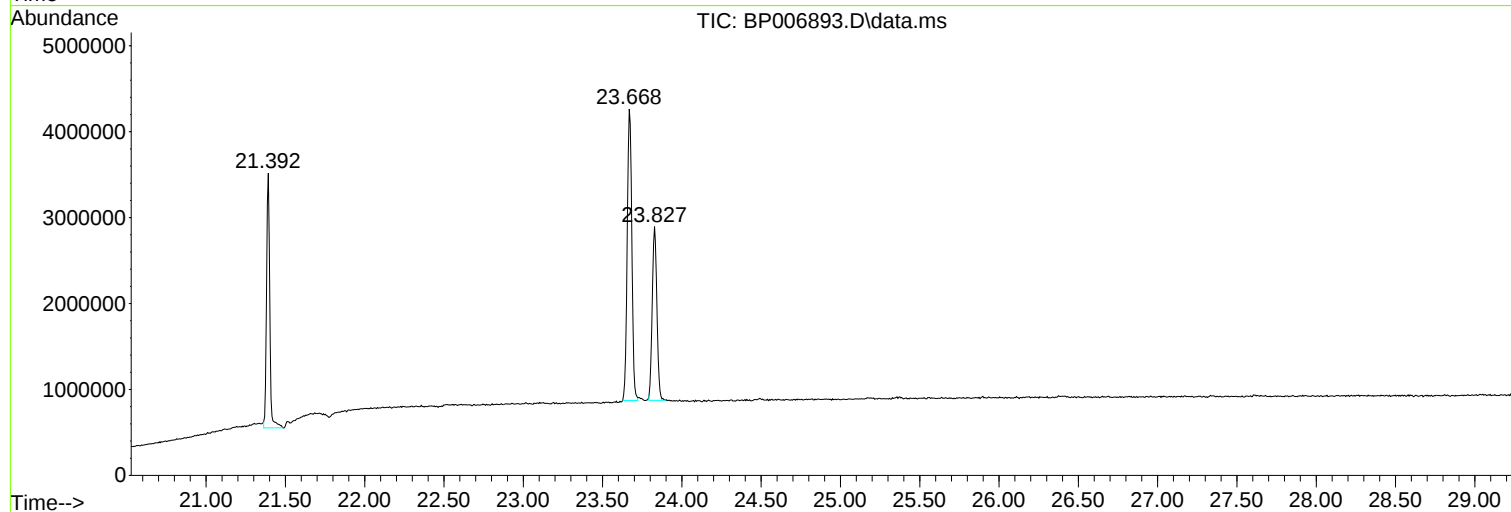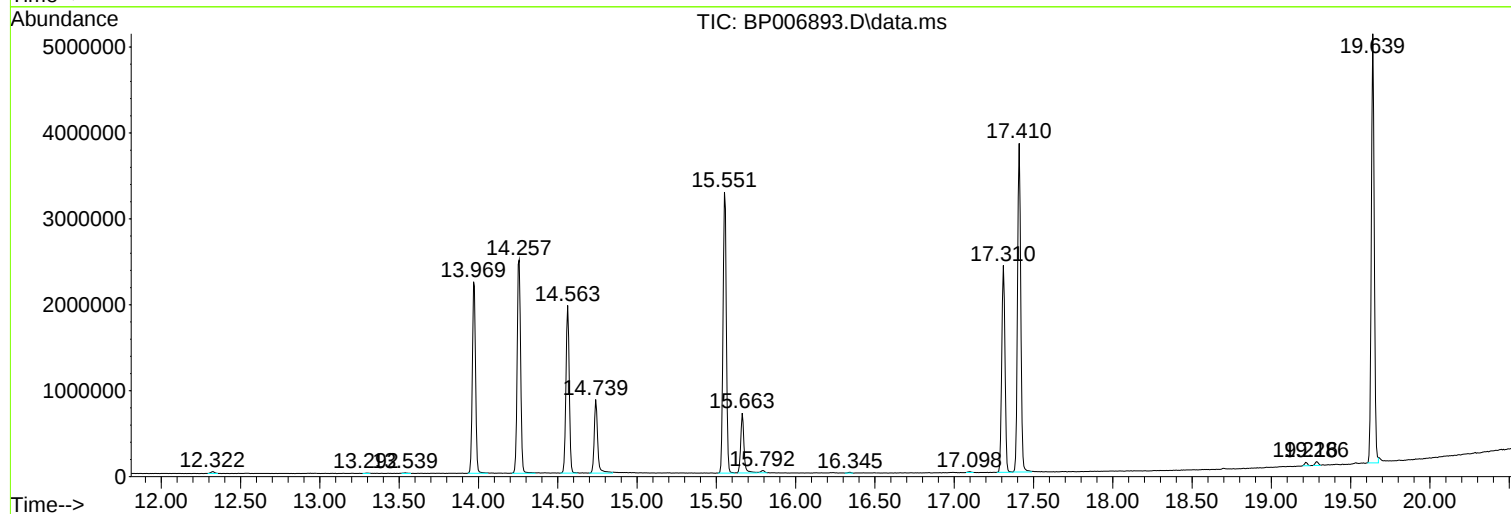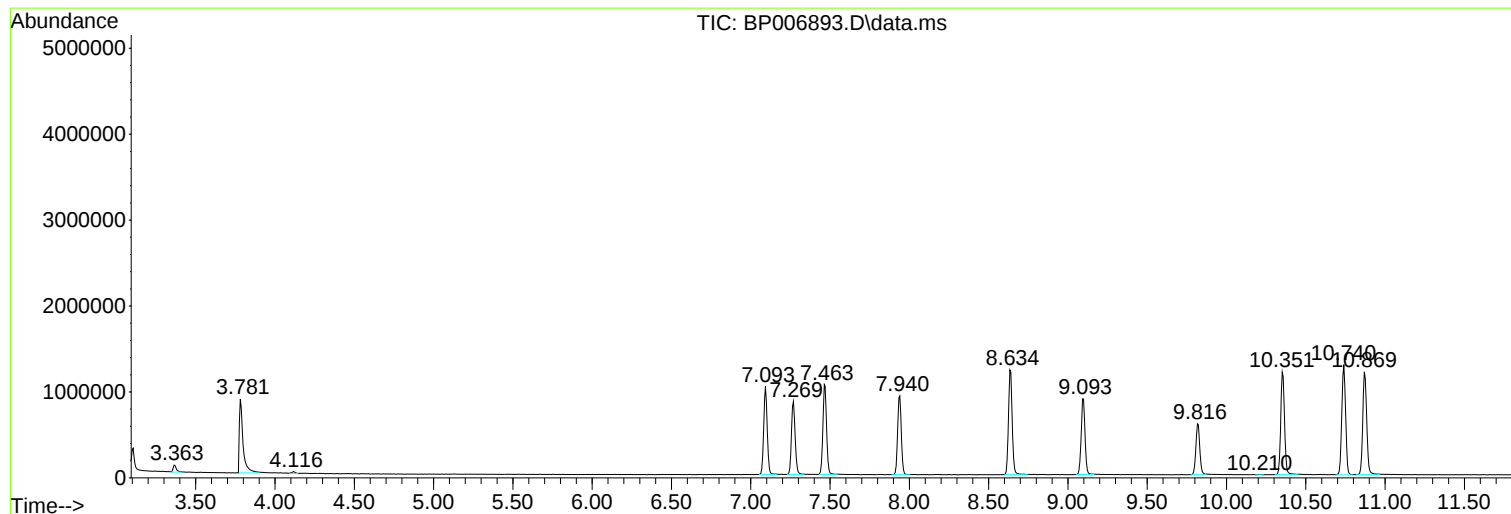

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006893.D
Acq On : 09 Sep 2021 10:47
Operator : CG/JU
Sample : PB138822BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK822

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006893.D
Acq On : 09 Sep 2021 10:47
Operator : CG/JU
Sample : PB138822BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK822

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
