

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006895.D
 Acq On : 09 Sep 2021 12:07
 Operator : CG/JU
 Sample : PB138843BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK843

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006895.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	44	48	61	rVB	90664	136512	2.09%	0.200%
2	3.781	116	118	134	rBV	916966	1593818	24.36%	2.339%
3	4.117	171	175	182	rVB	22383	34777	0.53%	0.051%
4	7.093	674	681	697	rBV	1174818	1803179	27.56%	2.646%
5	7.269	703	711	721	rBV	917253	1496802	22.88%	2.197%
6	7.463	737	744	754	rBV	1162771	1870112	28.59%	2.745%
7	7.940	816	825	835	rBV	1038303	1656761	25.33%	2.431%
8	8.634	936	943	957	rBV	1353029	2217228	33.89%	3.254%
9	9.093	1014	1021	1039	rBV	972035	1649528	25.22%	2.421%
10	9.816	1137	1144	1159	rBV	682222	1161543	17.76%	1.705%
11	10.352	1228	1235	1254	rBV	1302652	2183148	33.37%	3.204%
12	10.740	1293	1301	1309	rBV	1355568	2282454	34.89%	3.350%
13	10.869	1315	1323	1339	rBV	1289164	2247239	34.35%	3.298%
14	12.322	1565	1570	1579	rVB3	22552	41447	0.63%	0.061%
15	12.540	1603	1607	1612	rVB6	3947	6809	0.10%	0.010%
16	13.534	1773	1776	1786	rVB8	6965	15535	0.24%	0.023%
17	13.975	1844	1851	1861	rBV	2246539	3243900	49.59%	4.761%
18	14.257	1892	1899	1911	rBV	2657158	3943826	60.29%	5.788%
19	14.563	1942	1951	1962	rBV	2084011	3004108	45.92%	4.409%
20	14.740	1975	1981	1999	rBV	892123	1345895	20.57%	1.975%
21	15.210	2056	2061	2064	rVB7	4105	7852	0.12%	0.012%
22	15.551	2113	2119	2131	rBV	3484306	4979280	76.12%	7.308%
23	15.663	2132	2138	2154	rVV	732712	1048294	16.02%	1.538%
24	15.792	2156	2160	2167	rVB4	26944	46019	0.70%	0.068%
25	16.345	2249	2254	2256	rVB5	5240	8088	0.12%	0.012%
26	17.098	2377	2382	2388	rBV3	10907	21317	0.33%	0.031%
27	17.310	2412	2418	2428	rBV	2409650	3466893	53.00%	5.088%
28	17.410	2428	2435	2454	rVV	3946338	5540489	84.69%	8.131%
29	18.698	2651	2654	2658	rBV4	14180	23138	0.35%	0.034%
30	19.222	2739	2743	2747	rBV3	36844	55157	0.84%	0.081%
31	19.286	2751	2754	2761	rVB2	44395	58744	0.90%	0.086%
32	19.639	2809	2814	2820	rBV	4944286	6541784	100.00%	9.601%
33	21.392	3107	3112	3128	rVB	3005405	4096699	62.62%	6.012%
34	23.674	3493	3500	3509	rBV2	3175488	6401743	97.86%	9.395%
35	23.833	3521	3527	3537	rVB2	1891910	3908633	59.75%	5.736%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006895.D
Acq On : 09 Sep 2021 12:07
Operator : CG/JU
Sample : PB138843BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK843

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Title : SVOA CALIBRATION




Sum of corrected areas: 68138751

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006895.D
Acq On : 09 Sep 2021 12:07
Operator : CG/JU
Sample : PB138843BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK843

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

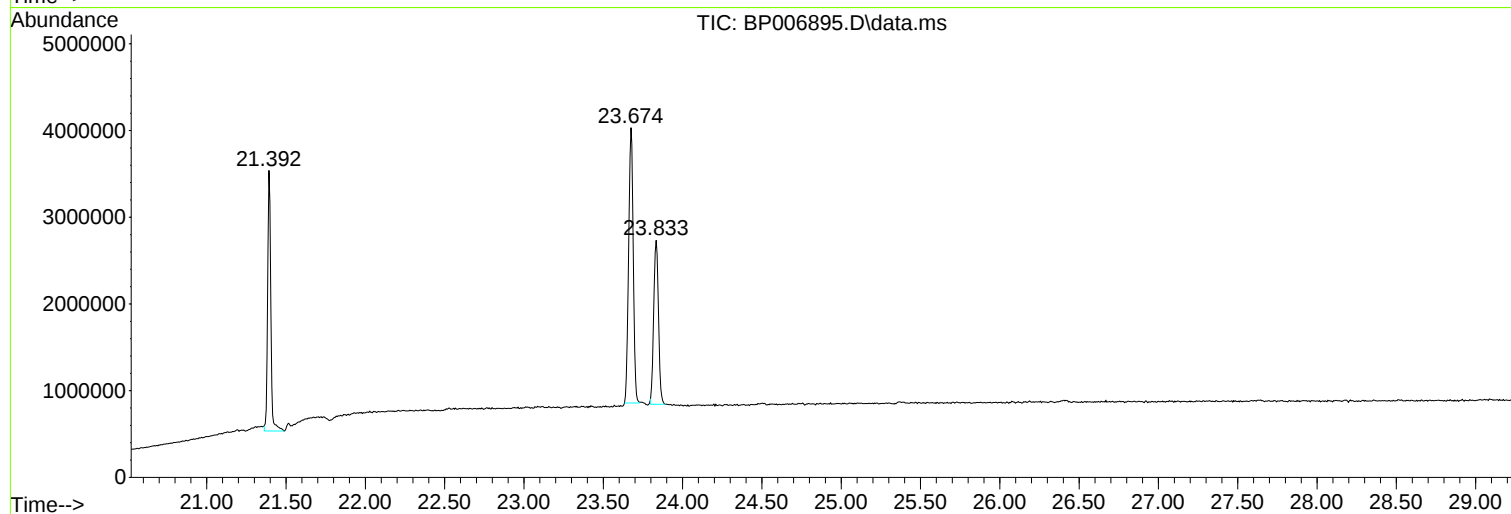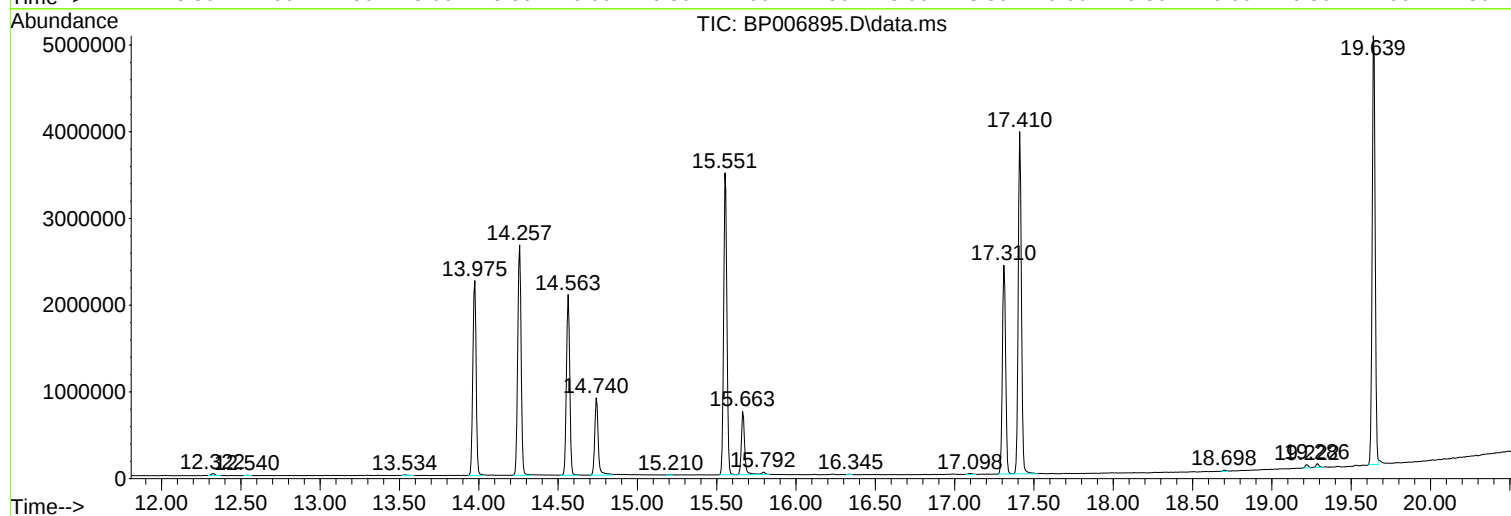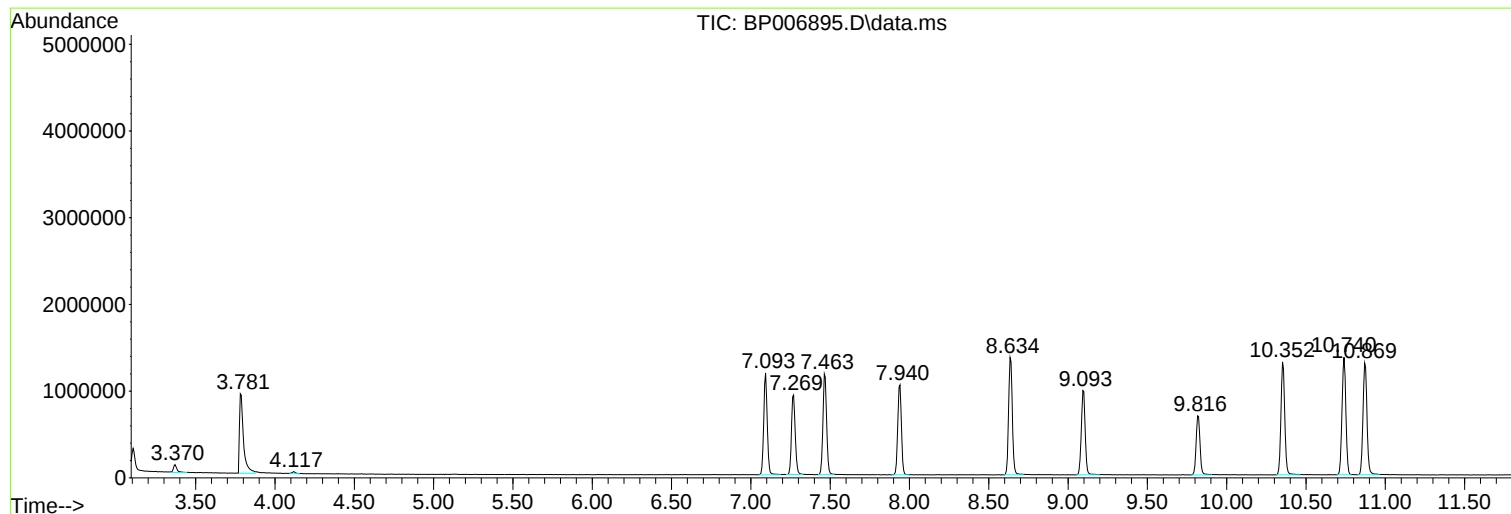

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006895.D
Acq On : 09 Sep 2021 12:07
Operator : CG/JU
Sample : PB138843BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK843

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006895.D
Acq On : 09 Sep 2021 12:07
Operator : CG/JU
Sample : PB138843BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK843

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
