

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006898.D
 Acq On : 09 Sep 2021 13:50
 Operator : CG/JU
 Sample : M3573-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ESQK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006898.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	44	48	51	rBV	60543	80520	1.14%	0.129%
2	3.405	51	54	59	rVB	26242	39573	0.56%	0.063%
3	3.793	116	120	140	rBV	220927	414112	5.84%	0.664%
4	3.975	147	151	154	rBV6	6454	10575	0.15%	0.017%
5	4.022	155	159	163	rVB	18953	27192	0.38%	0.044%
6	4.117	170	175	181	rVB	112413	151839	2.14%	0.244%
7	6.040	497	502	506	rBV8	4689	8483	0.12%	0.014%
8	6.222	529	533	537	rVB3	4924	7391	0.10%	0.012%
9	7.093	675	681	691	rBV	222223	359524	5.07%	0.577%
10	7.269	702	711	728	rBV	816210	1299760	18.34%	2.085%
11	7.469	738	745	756	rBV	772577	1253048	17.68%	2.010%
12	7.569	758	762	768	rVB8	5050	7793	0.11%	0.013%
13	7.940	818	825	832	rBV	887732	1395210	19.68%	2.238%
14	8.005	832	836	842	rVB9	5314	9661	0.14%	0.015%
15	8.175	859	865	871	rBV7	9699	20015	0.28%	0.032%
16	8.499	915	920	928	rVB9	5106	11898	0.17%	0.019%
17	8.640	936	944	955	rBV	621834	1045782	14.75%	1.678%
18	9.099	1014	1022	1035	rBV	876618	1469214	20.73%	2.357%
19	9.540	1093	1097	1100	rVB6	6164	9349	0.13%	0.015%
20	9.816	1136	1144	1155	rBV	602159	1011587	14.27%	1.623%
21	10.357	1228	1236	1247	rBV	1067847	1816825	25.63%	2.914%
22	10.534	1262	1266	1276	rVB3	16455	32288	0.46%	0.052%
23	10.740	1293	1301	1313	rBV	1237088	2035754	28.72%	3.266%
24	10.869	1315	1323	1335	rVV	997414	1731441	24.43%	2.777%
25	12.322	1563	1570	1577	rVB3	21311	41392	0.58%	0.066%
26	12.934	1669	1674	1678	rVB8	3755	7920	0.11%	0.013%
27	13.198	1711	1719	1720	rBV5	4246	8724	0.12%	0.014%
28	13.528	1771	1775	1779	rBV7	5824	9546	0.13%	0.015%
29	13.734	1805	1810	1816	rBV9	5648	13048	0.18%	0.021%
30	13.887	1830	1836	1840	rBV9	6366	12332	0.17%	0.020%
31	13.969	1842	1850	1862	rBV	2303767	3217403	45.39%	5.161%
32	14.057	1862	1865	1868	rVB5	6312	8687	0.12%	0.014%
33	14.257	1890	1899	1911	rBV	2592058	3695239	52.14%	5.927%
34	14.487	1933	1938	1941	rBV7	12277	16387	0.23%	0.026%
35	14.563	1943	1951	1958	rBV	1845786	2757416	38.90%	4.423%
36	14.740	1974	1981	1991	rBV2	153707	261256	3.69%	0.419%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006898.D
 Acq On : 09 Sep 2021 13:50
 Operator : CG/JU
 Sample : M3573-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ESQK5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

37	14.963	2015	2019	2020	rBV4	7193	8552	0.12%	0.014%
38	15.040	2027	2032	2036	rVB5	6158	10149	0.14%	0.016%
39	15.234	2062	2065	2069	rVB4	7564	9749	0.14%	0.016%
40	15.298	2069	2076	2079	rBV9	4811	10361	0.15%	0.017%
41	15.381	2084	2090	2094	rVB5	9647	20040	0.28%	0.032%
42	15.551	2113	2119	2127	rBV	3368286	4893657	69.04%	7.850%
43	15.663	2131	2138	2149	rBV	852362	1162145	16.40%	1.864%
44	15.792	2156	2160	2164	rBV2	20774	31076	0.44%	0.050%
45	16.122	2214	2216	2222	rVB7	5647	9419	0.13%	0.015%
46	16.304	2242	2247	2250	rBV2	13596	20648	0.29%	0.033%
47	16.804	2327	2332	2337	rBV	73758	98992	1.40%	0.159%
48	17.098	2374	2382	2384	rBV5	11635	27146	0.38%	0.044%
49	17.128	2385	2387	2392	rVB5	12600	16304	0.23%	0.026%
50	17.310	2412	2418	2424	rBV	2299584	3305961	46.64%	5.303%
51	17.410	2428	2435	2447	rBV	3988245	5734299	80.90%	9.198%
52	17.986	2530	2533	2538	rVB7	10584	12005	0.17%	0.019%
53	18.192	2563	2568	2578	rBV3	151391	258241	3.64%	0.414%
54	19.216	2739	2742	2748	rVB	45337	60669	0.86%	0.097%
55	19.286	2750	2754	2757	rBV	53764	72173	1.02%	0.116%
56	19.428	2774	2778	2784	rBV3	84586	125498	1.77%	0.201%
57	19.639	2808	2814	2820	rBV	5166207	7078120	99.86%	11.354%
58	21.104	3059	3063	3068	rBV3	138167	206530	2.91%	0.331%
59	21.392	3107	3112	3121	rBV	2977433	3786599	53.42%	6.074%
60	23.668	3492	3499	3507	rBV2	3642332	7087730	100.00%	11.369%
61	23.827	3519	3526	3536	rVB	1954469	3996371	56.38%	6.411%




Sum of corrected areas: 62340618

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006898.D
Acq On : 09 Sep 2021 13:50
Operator : CG/JU
Sample : M3573-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ESQK5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

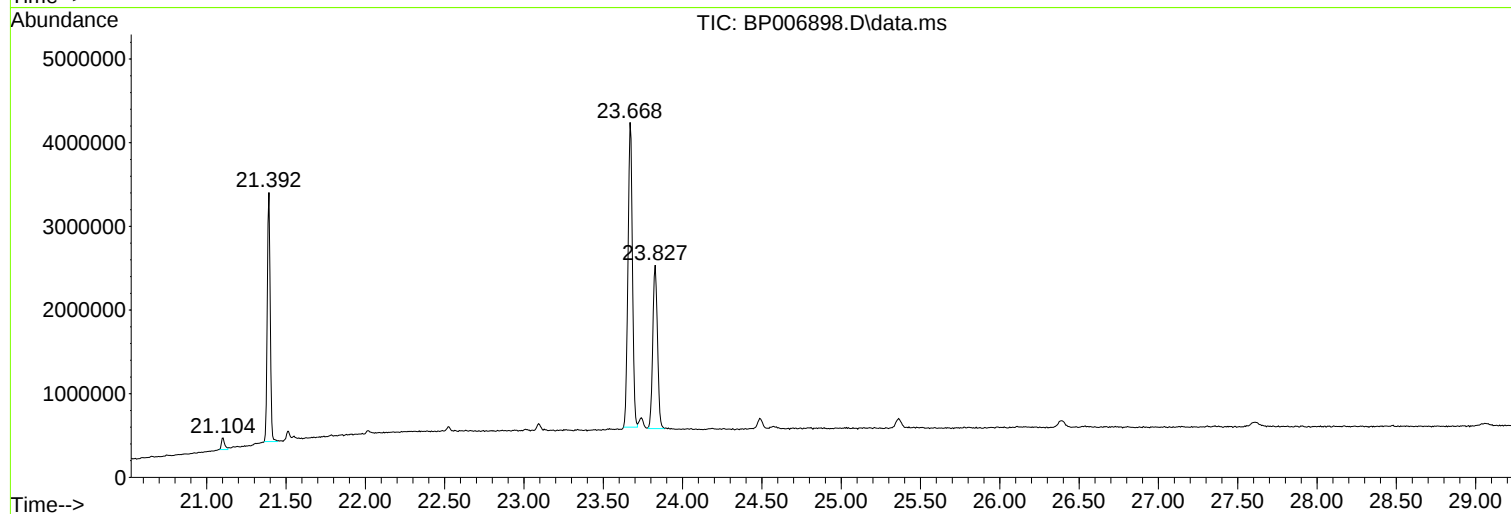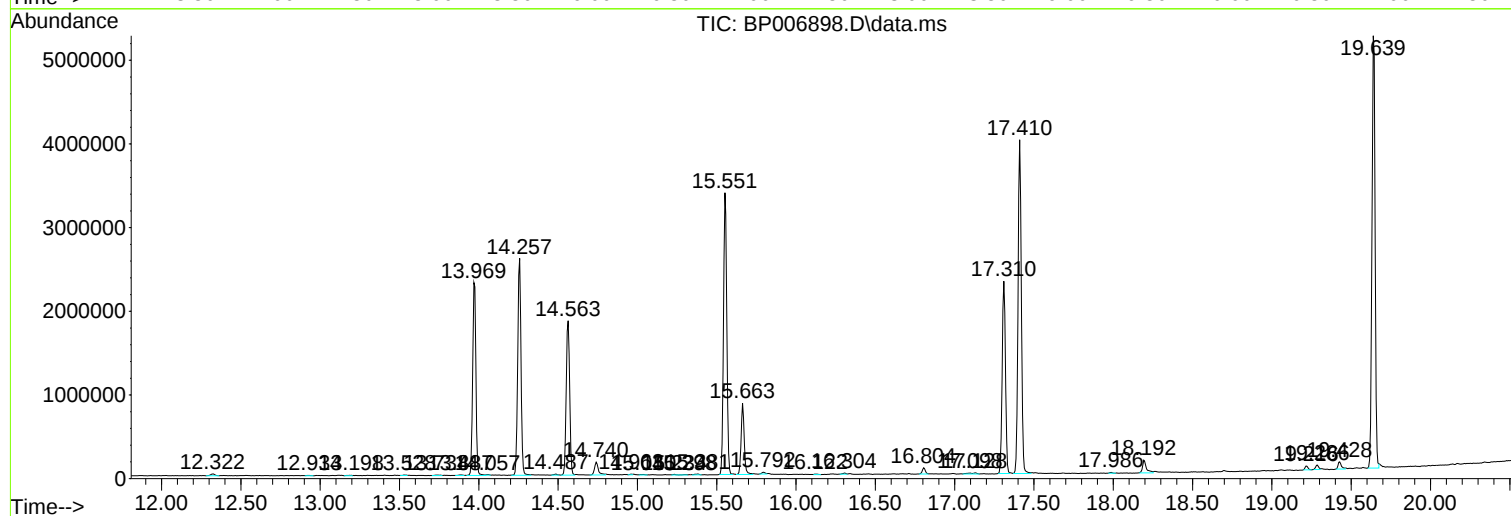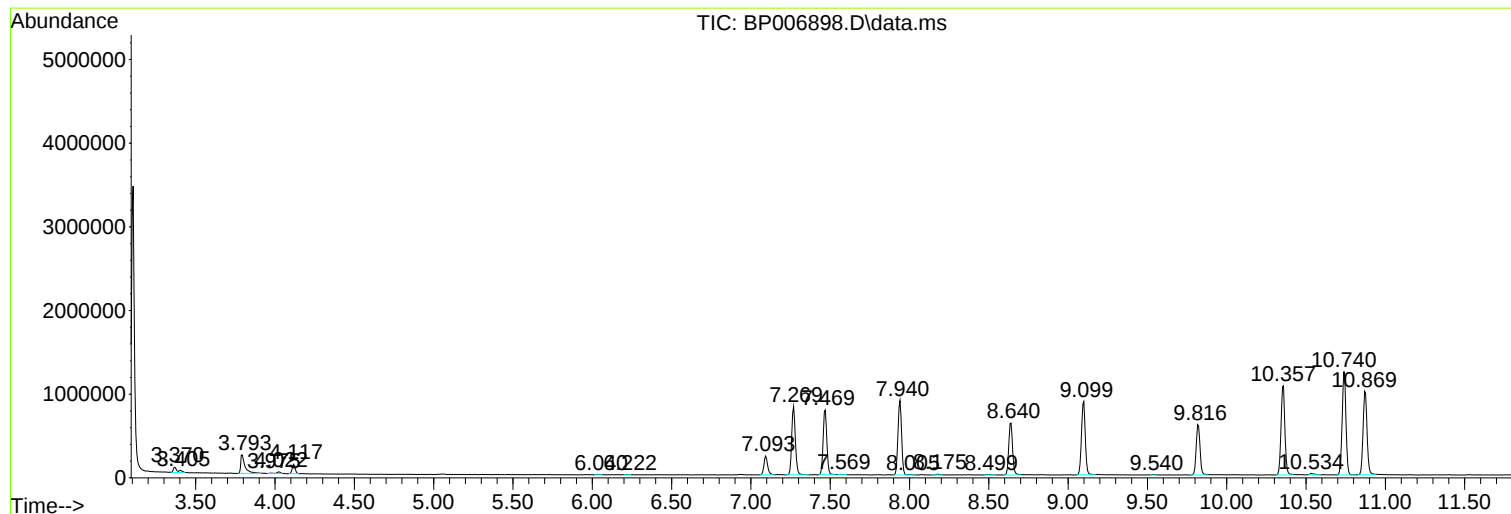

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006898.D
Acq On : 09 Sep 2021 13:50
Operator : CG/JU
Sample : M3573-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ESQK5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006898.D
Acq On : 09 Sep 2021 13:50
Operator : CG/JU
Sample : M3573-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ESQK5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
