

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006904.D
 Acq On : 09 Sep 2021 17:33
 Operator : CG/JU
 Sample : PB138738BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK738

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006904.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	43	48	59	rVB	86660	133228	2.02%	0.197%
2	3.781	115	118	144	rBV	984680	1629871	24.70%	2.407%
3	4.117	171	175	182	rVB	21336	32745	0.50%	0.048%
4	7.087	671	680	692	rBV	1114709	1790748	27.14%	2.644%
5	7.263	704	710	722	rBV	933429	1479127	22.41%	2.184%
6	7.463	737	744	757	rBV	1184894	1851249	28.05%	2.734%
7	7.934	816	824	832	rBV	1026932	1595455	24.18%	2.356%
8	8.634	936	943	953	rBV	1365277	2167398	32.84%	3.200%
9	9.093	1014	1021	1034	rBV	1015546	1640945	24.87%	2.423%
10	9.816	1137	1144	1157	rBV	701337	1158618	17.56%	1.711%
11	10.352	1225	1235	1251	rBV	1291568	2153348	32.63%	3.180%
12	10.740	1292	1301	1309	rBV	1312794	2238845	33.93%	3.306%
13	10.869	1316	1323	1338	rBV	1313321	2213425	33.54%	3.268%
14	12.322	1565	1570	1578	rVB	25275	43084	0.65%	0.064%
15	13.975	1842	1851	1862	rBV	2278768	3231161	48.96%	4.771%
16	14.257	1892	1899	1910	rBV	2641957	3856063	58.43%	5.694%
17	14.563	1944	1951	1961	rBV	1988555	2928402	44.38%	4.324%
18	14.740	1975	1981	1999	rBV	896863	1397359	21.18%	2.063%
19	15.557	2113	2120	2131	rBV	3402222	4917259	74.52%	7.261%
20	15.663	2132	2138	2150	rBV	763646	1102232	16.70%	1.628%
21	15.792	2156	2160	2166	rVB	23550	39023	0.59%	0.058%
22	16.339	2249	2253	2258	rBV8	7496	13523	0.20%	0.020%
23	17.098	2379	2382	2388	rVB3	10875	15639	0.24%	0.023%
24	17.310	2412	2418	2429	rBV	2382223	3434667	52.05%	5.072%
25	17.410	2429	2435	2455	rVV	3827763	5465786	82.83%	8.071%
26	18.204	2566	2570	2575	rBV6	10270	16059	0.24%	0.024%
27	18.704	2651	2655	2660	rBV5	16442	23012	0.35%	0.034%
28	19.222	2739	2743	2748	rBV4	39770	55403	0.84%	0.082%
29	19.286	2750	2754	2758	rBV	42864	56997	0.86%	0.084%
30	19.645	2809	2815	2829	rBV	5108181	6599018	100.00%	9.744%
31	21.392	3107	3112	3122	rBV	2857562	3767267	57.09%	5.563%
32	21.516	3130	3133	3136	rBV	101128	131882	2.00%	0.195%
33	23.674	3493	3500	3509	rBV2	3417609	6571534	99.58%	9.704%
34	23.833	3520	3527	3537	rVB2	1968228	3971831	60.19%	5.865%

Sum of corrected areas: 67722203

Instrument :

BNA_P

ClientSampleId :




SBLK738

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006904.D
Acq On : 09 Sep 2021 17:33
Operator : CG/JU
Sample : PB138738BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK738

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

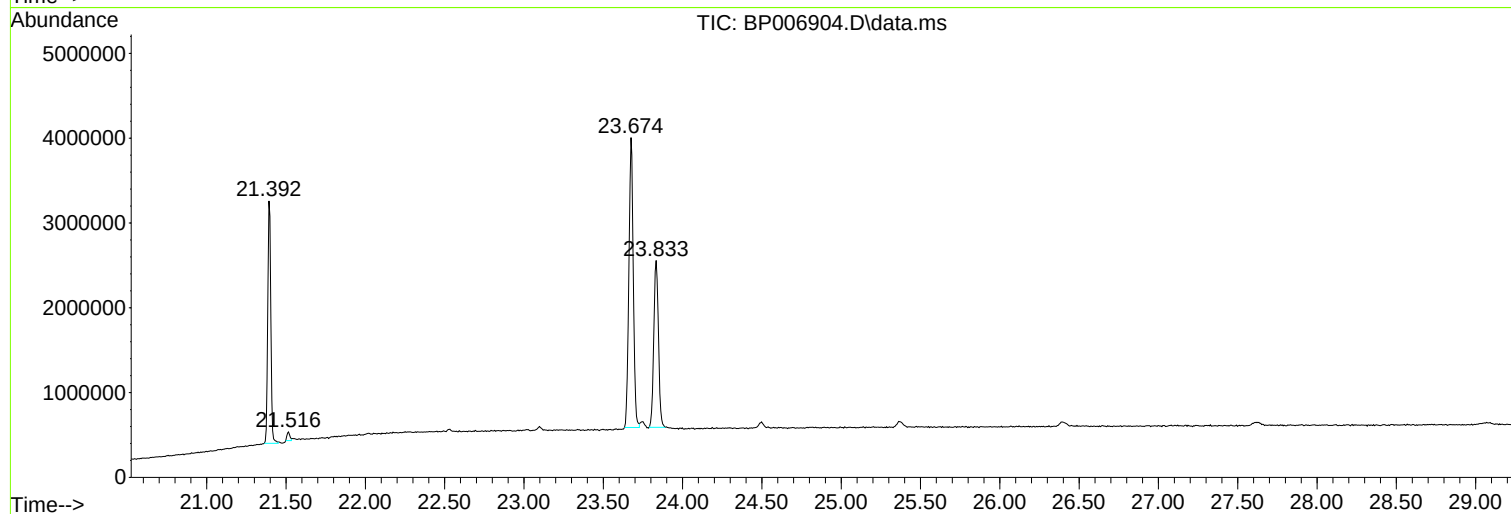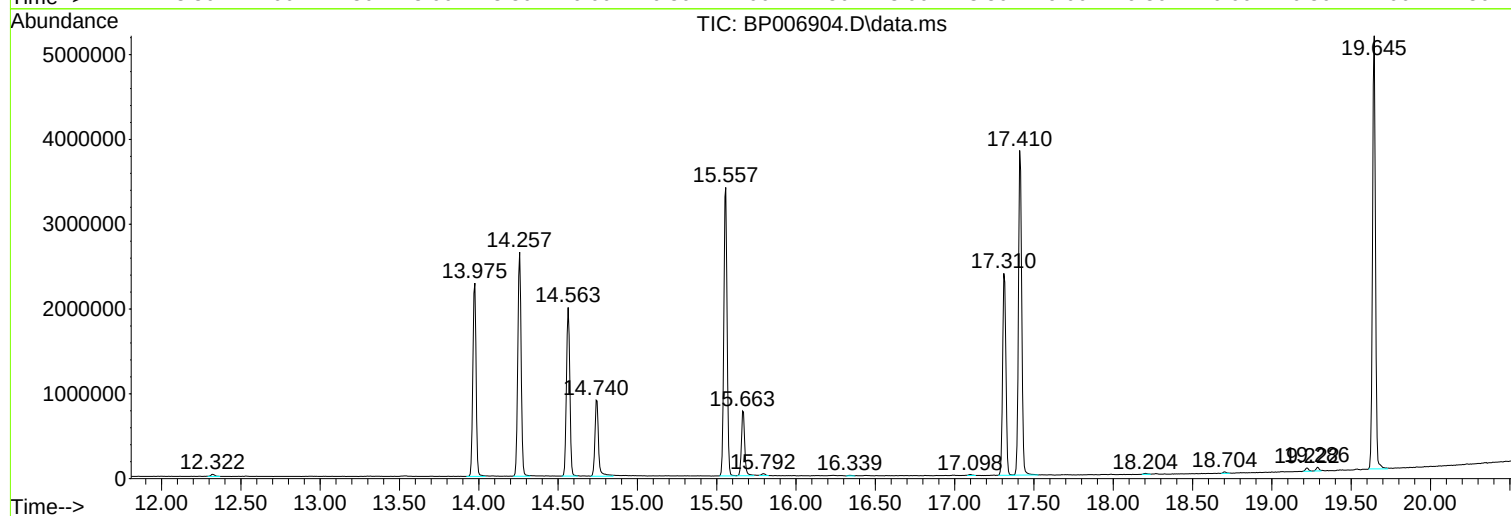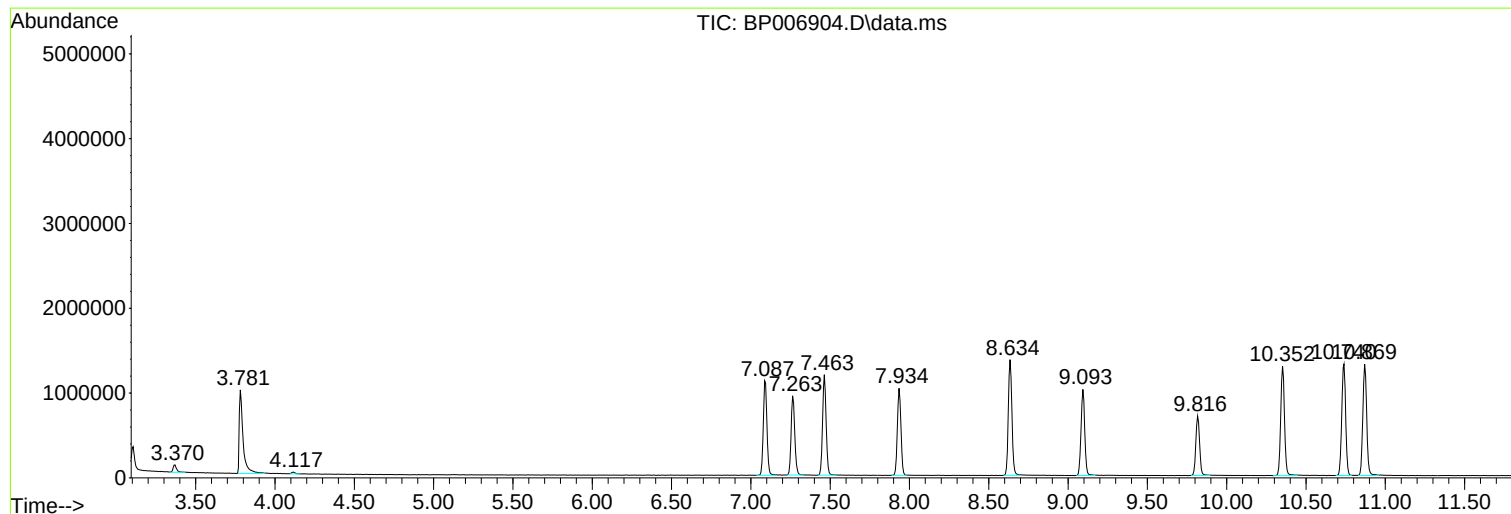

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006904.D
Acq On : 09 Sep 2021 17:33
Operator : CG/JU
Sample : PB138738BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK738

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006904.D
Acq On : 09 Sep 2021 17:33
Operator : CG/JU
Sample : PB138738BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK738

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
