

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006909.D
 Acq On : 09 Sep 2021 20:24
 Operator : CG/JU
 Sample : PB138871BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK871

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006909.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	44	48	54	rBV	92438	125602	1.74%	0.167%
2	3.787	115	119	146	rBV	1059360	1821449	25.28%	2.428%
3	4.122	172	176	186	rVB	26591	40710	0.57%	0.054%
4	7.093	674	681	692	rBV	1298820	2013244	27.94%	2.684%
5	7.269	703	711	721	rBV	1072578	1681984	23.35%	2.242%
6	7.469	738	745	760	rVB	1288818	2079328	28.86%	2.772%
7	7.940	818	825	834	rBV	1148630	1791766	24.87%	2.389%
8	8.634	936	943	962	rBV	1507885	2485767	34.50%	3.314%
9	9.092	1011	1021	1037	rBV	1099635	1870362	25.96%	2.493%
10	9.822	1137	1145	1154	rBV	771049	1297214	18.01%	1.729%
11	10.351	1228	1235	1248	rBV	1471605	2407388	33.41%	3.209%
12	10.739	1293	1301	1309	rBV	1522218	2522967	35.02%	3.363%
13	10.869	1314	1323	1342	rBV	1418642	2523174	35.02%	3.364%
14	12.322	1563	1570	1575	rBV2	24884	43315	0.60%	0.058%
15	13.304	1730	1737	1741	rBV9	4012	8198	0.11%	0.011%
16	13.533	1774	1776	1782	rVB4	6524	10743	0.15%	0.014%
17	13.969	1841	1850	1861	rBV	2551950	3603227	50.01%	4.803%
18	14.257	1891	1899	1911	rBV	2866879	4336054	60.18%	5.780%
19	14.563	1942	1951	1962	rBV	2253018	3282358	45.56%	4.376%
20	14.739	1974	1981	2006	rBV	1028101	1579163	21.92%	2.105%
21	15.551	2113	2119	2131	rBV	3932505	5498673	76.32%	7.330%
22	15.663	2132	2138	2150	rBV	880526	1205588	16.73%	1.607%
23	15.792	2156	2160	2169	rVB	29100	43909	0.61%	0.059%
24	16.233	2229	2235	2239	rBV9	5829	11294	0.16%	0.015%
25	16.339	2248	2253	2256	rBV6	6639	10392	0.14%	0.014%
26	16.992	2360	2364	2367	rVB6	6987	9216	0.13%	0.012%
27	17.092	2378	2381	2387	rVB3	10813	16350	0.23%	0.022%
28	17.310	2411	2418	2428	rBV	2694952	3811793	52.91%	5.081%
29	17.410	2428	2435	2454	rBV	4276940	6073593	84.30%	8.096%
30	17.680	2479	2481	2485	rBV4	4555	7363	0.10%	0.010%
31	17.980	2529	2532	2537	rBV7	6634	7631	0.11%	0.010%
32	18.698	2652	2654	2659	rVB4	7342	7228	0.10%	0.010%
33	19.215	2739	2742	2747	rBV2	39970	49724	0.69%	0.066%
34	19.286	2750	2754	2759	rVB	47429	66979	0.93%	0.089%
35	19.639	2808	2814	2825	rBV	5645132	7204544	100.00%	9.604%
36	21.392	3107	3112	3127	rVB	3250416	4126996	57.28%	5.501%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006909.D
Acq On : 09 Sep 2021 20:24
Operator : CG/JU
Sample : PB138871BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK871

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Title : SVOA CALIBRATION

37	23.668	3492	3499	3507	rBV2	3622521	7084523	98.33%	9.444%
38	23.827	3519	3526	3536	rVB2	2121959	4256169	59.08%	5.674%




Sum of corrected areas: 75015978

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006909.D
Acq On : 09 Sep 2021 20:24
Operator : CG/JU
Sample : PB138871BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK871

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

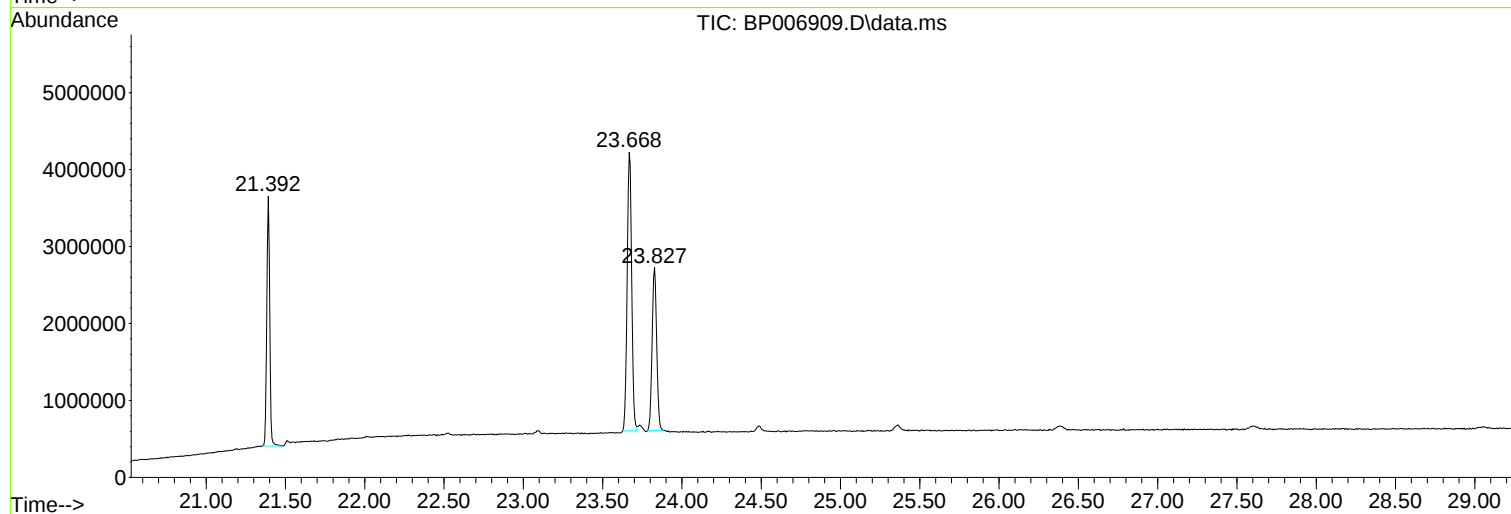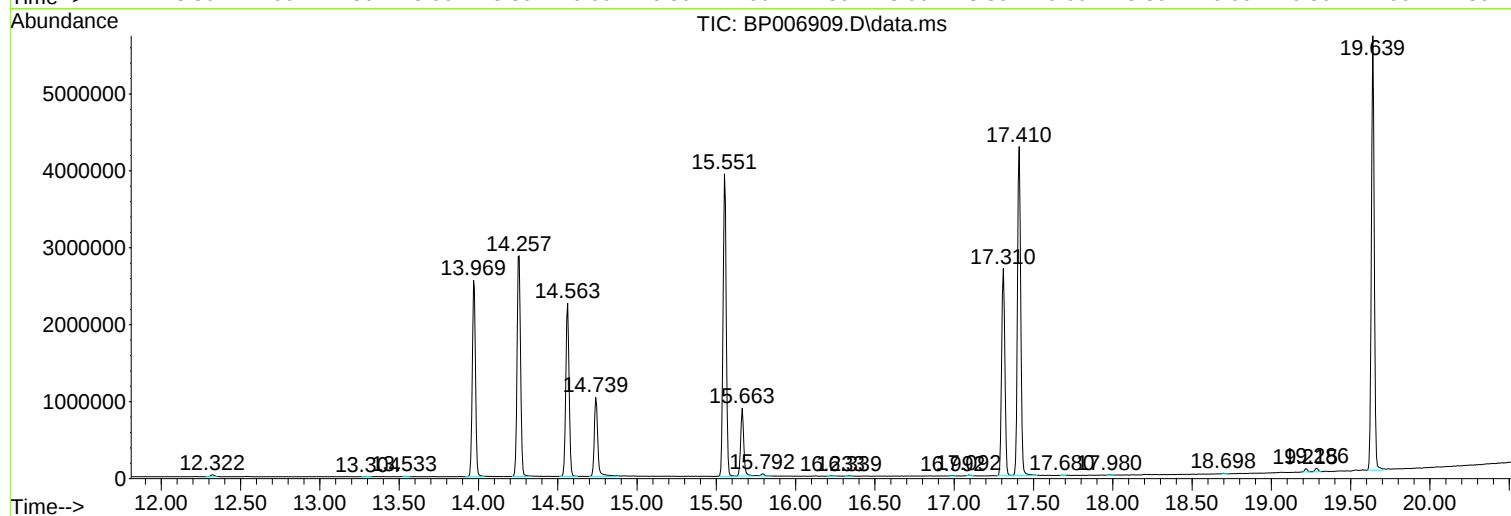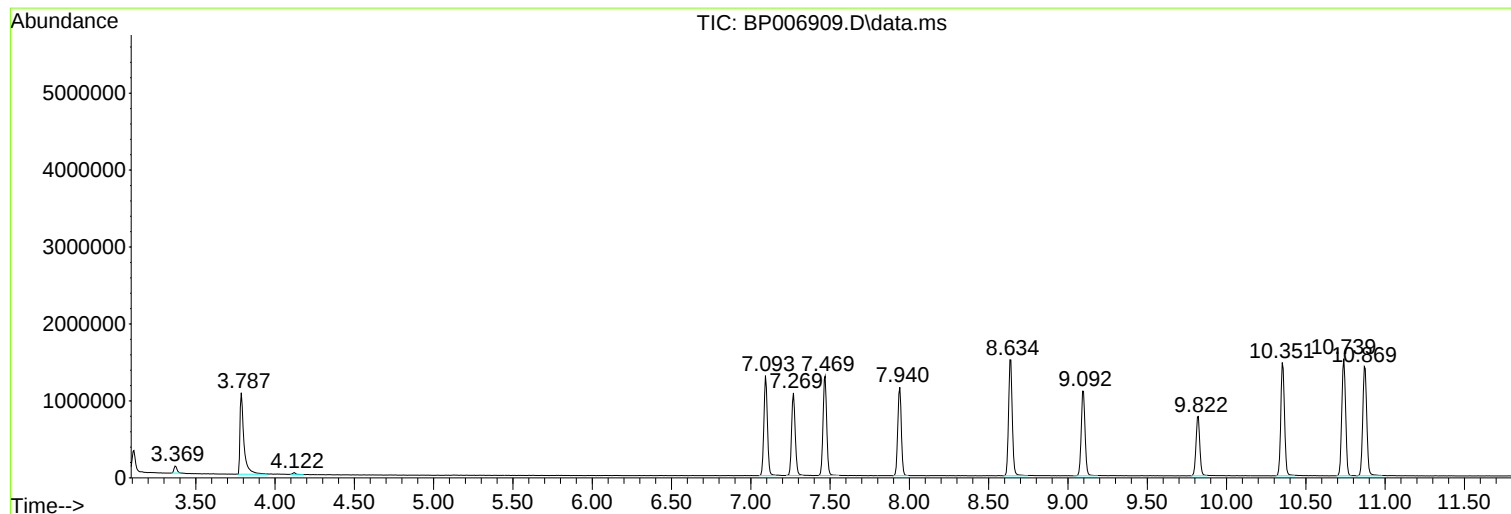

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006909.D
Acq On : 09 Sep 2021 20:24
Operator : CG/JU
Sample : PB138871BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK871

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006909.D
Acq On : 09 Sep 2021 20:24
Operator : CG/JU
Sample : PB138871BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK871

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
