

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006912.D
 Acq On : 09 Sep 2021 22:06
 Operator : CG/JU
 Sample : M3526-16
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW7C6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006912.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	45	48	57	rVB	25004	38756	0.88%	0.103%
2	4.028	154	160	168	rVB	33350	61878	1.41%	0.165%
3	4.116	171	175	184	rVB	22990	35463	0.81%	0.094%
4	5.040	327	332	337	rBV2	13343	23197	0.53%	0.062%
5	5.134	343	348	354	rBV4	9008	16188	0.37%	0.043%
6	5.957	481	488	492	rBV3	18893	29351	0.67%	0.078%
7	6.428	562	568	576	rBV3	7376	17106	0.39%	0.046%
8	6.616	596	600	604	rVB3	7048	10450	0.24%	0.028%
9	6.940	651	655	660	rVB6	6101	10542	0.24%	0.028%
10	7.093	675	681	690	rBV	317778	533080	12.11%	1.420%
11	7.269	705	711	718	rBV	272872	442490	10.05%	1.179%
12	7.463	734	744	754	rBV	315163	527565	11.98%	1.406%
13	7.569	758	762	769	rVB2	24500	45809	1.04%	0.122%
14	7.940	817	825	833	rBV	1060837	1734636	39.40%	4.622%
15	8.004	833	836	841	rVB4	5950	10819	0.25%	0.029%
16	8.057	841	845	852	rVB9	5598	12897	0.29%	0.034%
17	8.175	861	865	871	rBV7	9584	17360	0.39%	0.046%
18	8.498	913	920	927	rBV6	11450	25747	0.58%	0.069%
19	8.634	935	943	954	rBV	348632	604118	13.72%	1.610%
20	8.763	961	965	970	rVB5	10461	15867	0.36%	0.042%
21	8.828	974	976	984	rVB8	6935	11480	0.26%	0.031%
22	9.093	1015	1021	1031	rVV	263419	434115	9.86%	1.157%
23	9.175	1031	1035	1041	rVV	32117	48447	1.10%	0.129%
24	9.269	1045	1051	1053	rBV7	6064	10322	0.23%	0.028%
25	9.298	1054	1056	1064	rVB8	7566	11656	0.26%	0.031%
26	9.528	1088	1095	1099	rBV7	7494	15196	0.35%	0.040%
27	9.657	1109	1117	1123	rBV7	5227	10331	0.23%	0.028%
28	9.816	1135	1144	1151	rBV	161826	286013	6.50%	0.762%
29	10.169	1195	1204	1210	rBV	8808	23786	0.54%	0.063%
30	10.351	1227	1235	1247	rBV	350603	592684	13.46%	1.579%
31	10.528	1260	1265	1275	rBV	35955	79255	1.80%	0.211%
32	10.740	1292	1301	1308	rBV	1427700	2475480	56.23%	6.596%
33	10.869	1317	1323	1338	rVB	292416	546357	12.41%	1.456%
34	11.240	1378	1386	1397	rBV	11912	32574	0.74%	0.087%
35	11.663	1452	1458	1467	rVB	11375	30453	0.69%	0.081%
36	11.775	1471	1477	1486	rVV4	26261	61081	1.39%	0.163%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006912.D
 Acq On : 09 Sep 2021 22:06
 Operator : CG/JU
 Sample : M3526-16
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW7C6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

37	11.934	1499	1504	1508	rVB3	10199	17340	0.39%	0.046%
38	12.028	1517	1520	1525	rVB7	9593	12196	0.28%	0.032%
39	12.163	1538	1543	1550	rBV	76581	120381	2.73%	0.321%
40	12.310	1562	1568	1569	rBV6	7393	11325	0.26%	0.030%
41	12.392	1575	1582	1588	rVB3	24733	44348	1.01%	0.118%
42	12.469	1591	1595	1601	rVB9	7416	12113	0.28%	0.032%
43	12.610	1613	1619	1624	rVV	20923	30970	0.70%	0.083%
44	12.857	1655	1661	1664	rVV7	7791	15906	0.36%	0.042%
45	12.975	1677	1681	1685	rBV	10890	15659	0.36%	0.042%
46	13.010	1685	1687	1692	rVB5	9056	11011	0.25%	0.029%
47	13.116	1700	1705	1710	rVV	30497	45219	1.03%	0.120%
48	13.175	1712	1715	1721	rVB7	8824	13208	0.30%	0.035%
49	13.398	1746	1753	1761	rBV	103524	164205	3.73%	0.438%
50	13.492	1766	1769	1773	rVB4	8364	11165	0.25%	0.030%
51	13.886	1830	1836	1840	rBV3	14950	24939	0.57%	0.066%
52	13.969	1840	1850	1857	rBV	692148	980499	22.27%	2.613%
53	14.051	1860	1864	1869	rVB	52977	70509	1.60%	0.188%
54	14.092	1869	1871	1874	rBV4	10367	11800	0.27%	0.031%
55	14.181	1881	1886	1888	rVB4	9037	12764	0.29%	0.034%
56	14.257	1892	1899	1909	rVB	701103	1062851	24.14%	2.832%
57	14.469	1930	1935	1942	rVB	114719	160294	3.64%	0.427%
58	14.563	1942	1951	1963	rBV	2124740	3144465	71.43%	8.379%
59	14.739	1975	1981	1996	rBV	173914	308229	7.00%	0.821%
60	14.898	2005	2008	2011	rBV5	6369	9853	0.22%	0.026%
61	14.969	2015	2020	2025	rVB7	21499	40489	0.92%	0.108%
62	15.022	2026	2029	2036	rBV8	8533	17150	0.39%	0.046%
63	15.086	2036	2040	2048	rVB5	23455	47110	1.07%	0.126%
64	15.157	2048	2052	2053	rBV3	7195	10125	0.23%	0.027%
65	15.298	2073	2076	2080	rBV3	5988	9546	0.22%	0.025%
66	15.351	2082	2085	2088	rVV5	10517	16344	0.37%	0.044%
67	15.416	2092	2096	2101	rVB	108988	131233	2.98%	0.350%
68	15.551	2113	2119	2125	rBV	1081607	1530764	34.77%	4.079%
69	15.598	2125	2127	2130	rVB3	20870	21675	0.49%	0.058%
70	15.657	2132	2137	2145	rBV	164938	241670	5.49%	0.644%
71	15.822	2154	2165	2171	rBV2	53325	97259	2.21%	0.259%
72	15.975	2187	2191	2197	rBV8	12354	27863	0.63%	0.074%
73	16.039	2198	2202	2209	rVB8	24832	40738	0.93%	0.109%
74	16.280	2238	2243	2245	rBV	123190	178044	4.04%	0.474%
75	16.304	2245	2247	2260	rVB	136058	176611	4.01%	0.471%
76	16.416	2260	2266	2267	rBV6	5465	9909	0.23%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006912.D
 Acq On : 09 Sep 2021 22:06
 Operator : CG/JU
 Sample : M3526-16
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW7C6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

77	16.786	2325	2329	2333	rBV6	6470	12915	0.29%	0.034%
78	16.845	2335	2339	2344	rBV6	15271	31452	0.71%	0.084%
79	17.075	2373	2378	2383	rBV2	91071	126904	2.88%	0.338%
80	17.127	2383	2387	2393	rVB	60071	83694	1.90%	0.223%
81	17.310	2411	2418	2424	rBV	2476294	3645363	82.81%	9.714%
82	17.404	2429	2434	2446	rVV	1134553	1716607	39.00%	4.574%
83	17.498	2446	2450	2456	rVB9	14845	27368	0.62%	0.073%
84	17.604	2465	2468	2474	rVB7	14054	24354	0.55%	0.065%
85	17.733	2488	2490	2495	rVB5	12426	16304	0.37%	0.043%
86	17.816	2499	2504	2508	rBV	92141	118834	2.70%	0.317%
87	17.980	2529	2532	2536	rVB4	17563	22741	0.52%	0.061%
88	18.192	2564	2568	2571	rBV2	99864	131401	2.98%	0.350%
89	18.392	2600	2602	2607	rVB2	21958	28315	0.64%	0.075%
90	18.486	2614	2618	2621	rBV	85935	100849	2.29%	0.269%
91	19.092	2717	2721	2727	rVB	86336	100471	2.28%	0.268%
92	19.310	2756	2758	2764	rVB	29890	35704	0.81%	0.095%
93	19.421	2774	2777	2782	rBV5	49547	67092	1.52%	0.179%
94	19.639	2808	2814	2828	rBV	1657849	2453932	55.74%	6.539%
95	20.168	2901	2904	2908	rVB	80780	78726	1.79%	0.210%
96	20.651	2983	2986	2989	rBV	82871	91298	2.07%	0.243%
97	21.098	3059	3062	3070	rBV3	172916	245978	5.59%	0.655%
98	21.386	3106	3111	3117	rBV	3252253	4158996	94.48%	11.082%
99	23.662	3492	3498	3505	rBV2	1043944	2016956	45.82%	5.374%
100	23.821	3518	3525	3536	rVB2	2086609	4402105	100.00%	11.730%




Sum of corrected areas: 37528687

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP006912\
Data File : BP006912.D
Acq On : 09 Sep 2021 22:06
Operator : CG/JU
Sample : M3526-16
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW7C6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP006912.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

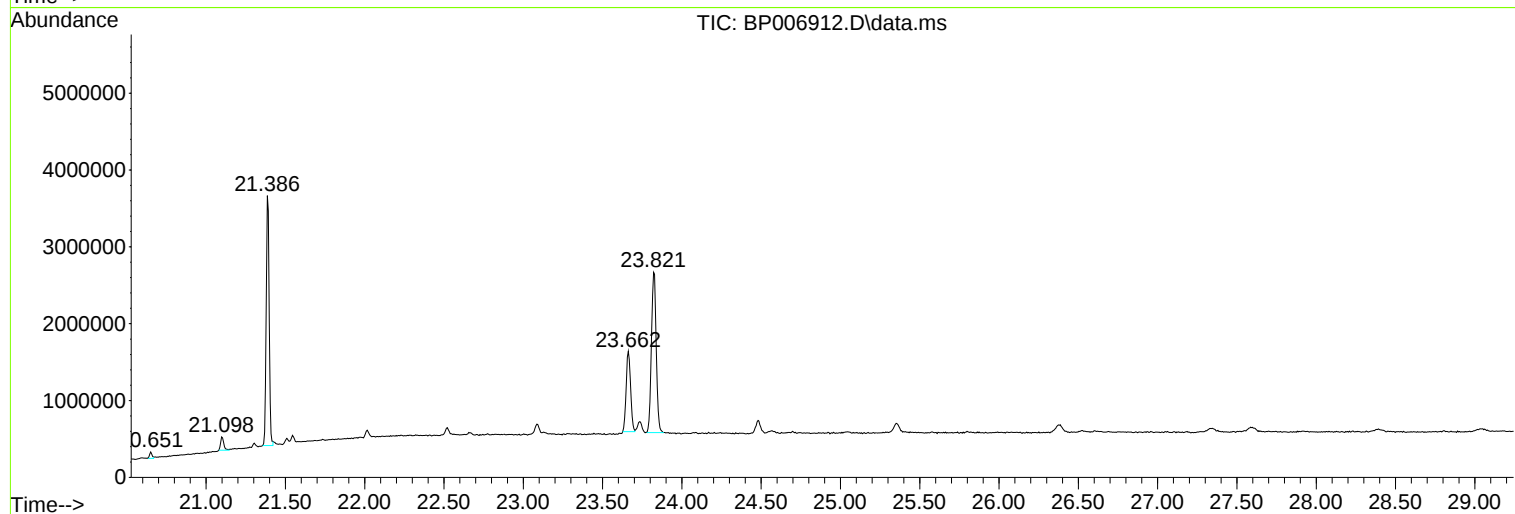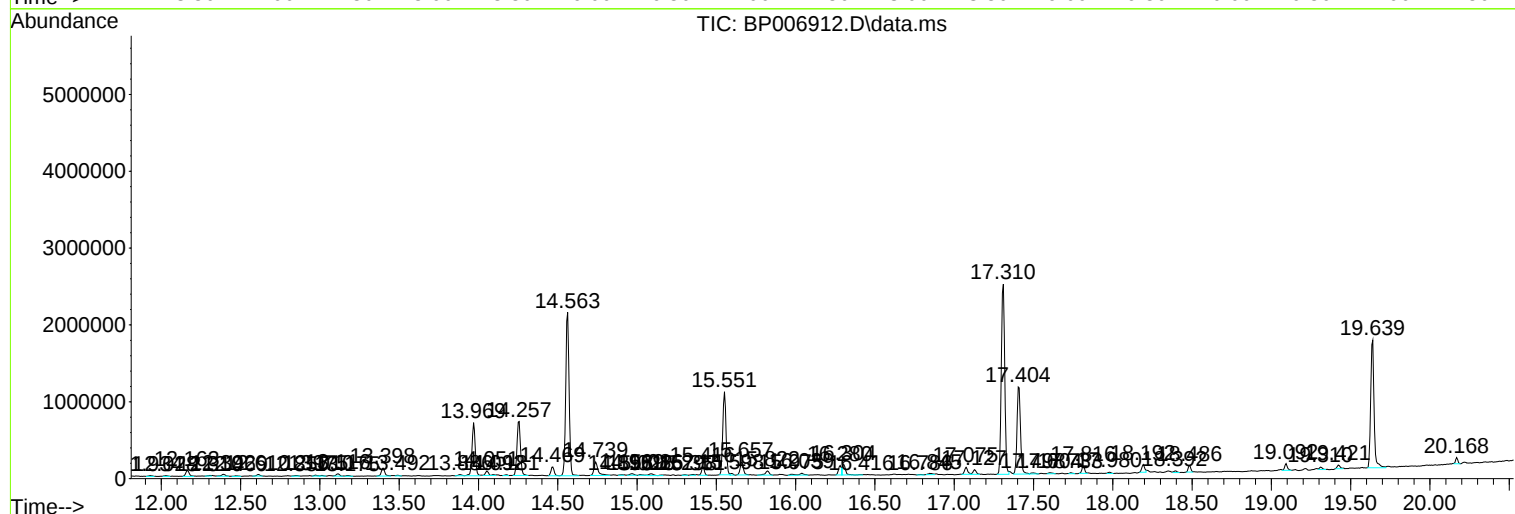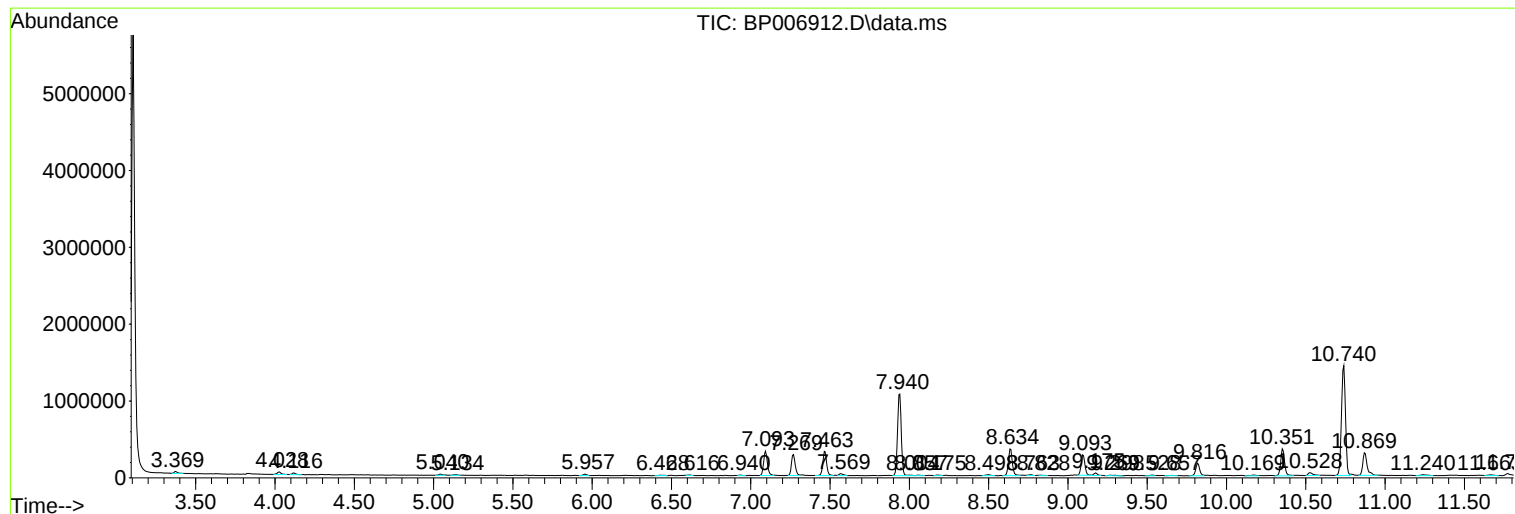

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006912.D
Acq On : 09 Sep 2021 22:06
Operator : CG/JU
Sample : M3526-16
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW7C6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006912.D
Acq On : 09 Sep 2021 22:06
Operator : CG/JU
Sample : M3526-16
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW7C6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
