

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006913.D
 Acq On : 09 Sep 2021 22:41
 Operator : CG/JU
 Sample : M3608-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBKL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006913.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	45	49	53	rBV	31035	44400	0.54%	0.062%
2	3.793	118	120	140	rBV	213570	418901	5.14%	0.588%
3	4.028	154	160	166	rVB	23990	39212	0.48%	0.055%
4	4.122	172	176	184	rVB	26374	39456	0.48%	0.055%
5	5.063	330	336	343	rVB7	9366	23434	0.29%	0.033%
6	6.940	651	655	658	rBV3	6002	8602	0.11%	0.012%
7	7.093	675	681	690	rBV	304565	502520	6.16%	0.705%
8	7.269	704	711	724	rBV	909649	1476930	18.11%	2.072%
9	7.463	737	744	755	rBV	939759	1531469	18.78%	2.148%
10	7.569	759	762	765	rVB5	6126	8581	0.11%	0.012%
11	7.940	817	825	832	rBV	1134871	1821645	22.34%	2.556%
12	8.004	833	836	842	rVB7	7076	10345	0.13%	0.015%
13	8.181	861	866	870	rVB4	11069	18374	0.23%	0.026%
14	8.487	913	918	924	rBV4	8485	14178	0.17%	0.020%
15	8.634	935	943	957	rBV	818656	1314817	16.12%	1.845%
16	9.093	1014	1021	1034	rBV	974968	1627098	19.95%	2.283%
17	9.534	1091	1096	1102	rVB4	9853	14402	0.18%	0.020%
18	9.816	1137	1144	1152	rBV	650445	1079900	13.24%	1.515%
19	10.351	1227	1235	1245	rBV	1262375	2038059	24.99%	2.859%
20	10.528	1259	1265	1278	rBV2	28469	67013	0.82%	0.094%
21	10.740	1293	1301	1312	rBV	1538999	2575533	31.58%	3.613%
22	10.869	1314	1323	1338	rBV	1117849	1930422	23.67%	2.708%
23	12.322	1564	1570	1575	rBV2	24044	39666	0.49%	0.056%
24	12.534	1600	1606	1614	rVB2	3765	8517	0.10%	0.012%
25	13.398	1748	1753	1758	rVB3	14082	20910	0.26%	0.029%
26	13.534	1771	1776	1783	rVB8	11012	18838	0.23%	0.026%
27	13.875	1830	1834	1840	rBV9	4105	10229	0.13%	0.014%
28	13.969	1844	1850	1861	rVV	2477159	3358075	41.18%	4.711%
29	14.251	1891	1898	1913	rBV	2671110	3978224	48.78%	5.581%
30	14.563	1942	1951	1961	rBV	2294202	3424386	41.99%	4.804%
31	14.739	1974	1981	1997	rBV	210855	360302	4.42%	0.505%
32	14.975	2016	2021	2024	rBV6	5489	8760	0.11%	0.012%
33	15.298	2072	2076	2081	rBV	18863	26093	0.32%	0.037%
34	15.416	2092	2096	2103	rVB2	14114	20790	0.25%	0.029%
35	15.551	2112	2119	2132	rBV	3878899	5508955	67.55%	7.728%
36	15.663	2132	2138	2154	rVV	992263	1364230	16.73%	1.914%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006913.D
 Acq On : 09 Sep 2021 22:41
 Operator : CG/JU
 Sample : M3608-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBKL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

37	15.792	2155	2160	2169	rVB3	28345	51547	0.63%	0.072%
38	16.228	2228	2234	2239	rBV10	6912	15376	0.19%	0.022%
39	16.339	2249	2253	2258	rVB4	13714	19309	0.24%	0.027%
40	17.086	2374	2380	2381	rBV4	12641	21461	0.26%	0.030%
41	17.310	2410	2418	2427	rBV	2761562	3984007	48.85%	5.589%
42	17.410	2428	2435	2449	rVV	4785472	6743093	82.69%	9.460%
43	17.933	2521	2524	2528	rBV6	6079	9353	0.11%	0.013%
44	17.980	2529	2532	2536	rVB6	10144	15416	0.19%	0.022%
45	18.192	2563	2568	2576	rBV	103519	154798	1.90%	0.217%
46	18.480	2615	2617	2622	rBV6	7161	10028	0.12%	0.014%
47	18.698	2651	2654	2660	rBV7	8589	16731	0.21%	0.023%
48	19.216	2738	2742	2747	rBV	44064	57641	0.71%	0.081%
49	19.286	2749	2754	2760	rBV	60519	96867	1.19%	0.136%
50	19.422	2774	2777	2785	rBV3	55978	80334	0.99%	0.113%
51	19.527	2793	2795	2798	rVB2	16264	12976	0.16%	0.018%
52	19.639	2808	2814	2826	rBV	6309387	8153976	99.99%	11.439%
53	21.098	3059	3062	3066	rBV3	105598	131867	1.62%	0.185%
54	21.386	3106	3111	3120	rBV	3265138	4334354	53.15%	6.081%
55	23.668	3491	3499	3507	rBV2	3964790	8154790	100.00%	11.440%
56	23.821	3519	3525	3535	rVB2	2171322	4464310	54.74%	6.263%




Sum of corrected areas: 71281500

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP0090921\
Data File : BP006913.D
Acq On : 09 Sep 2021 22:41
Operator : CG/JU
Sample : M3608-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP0090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

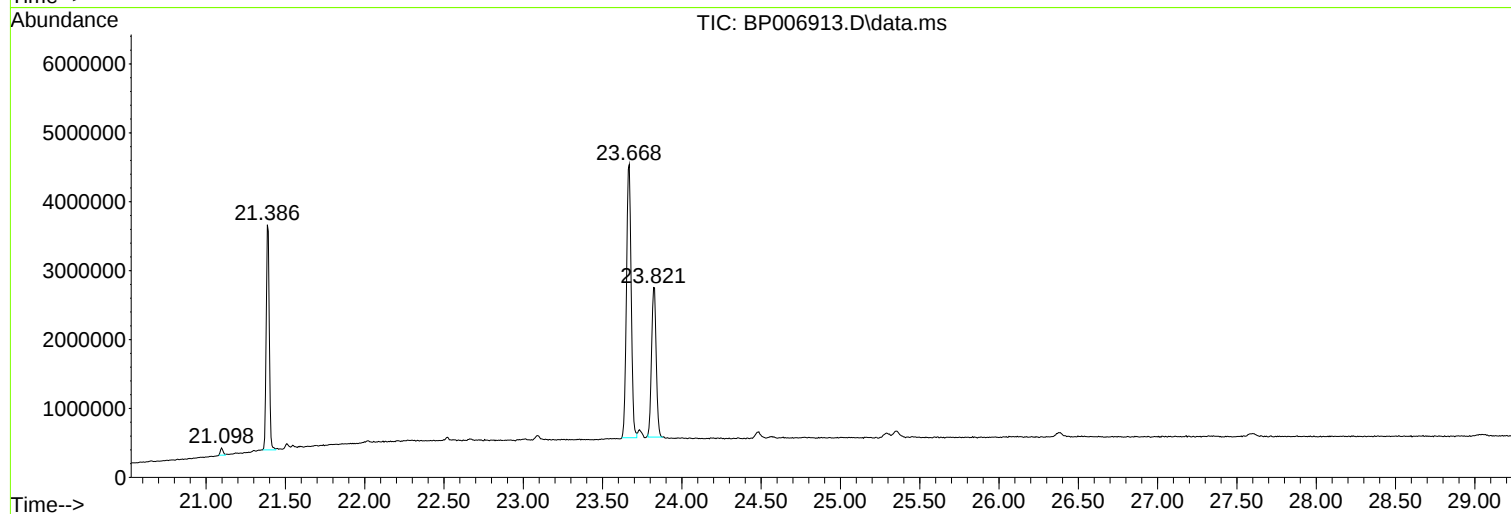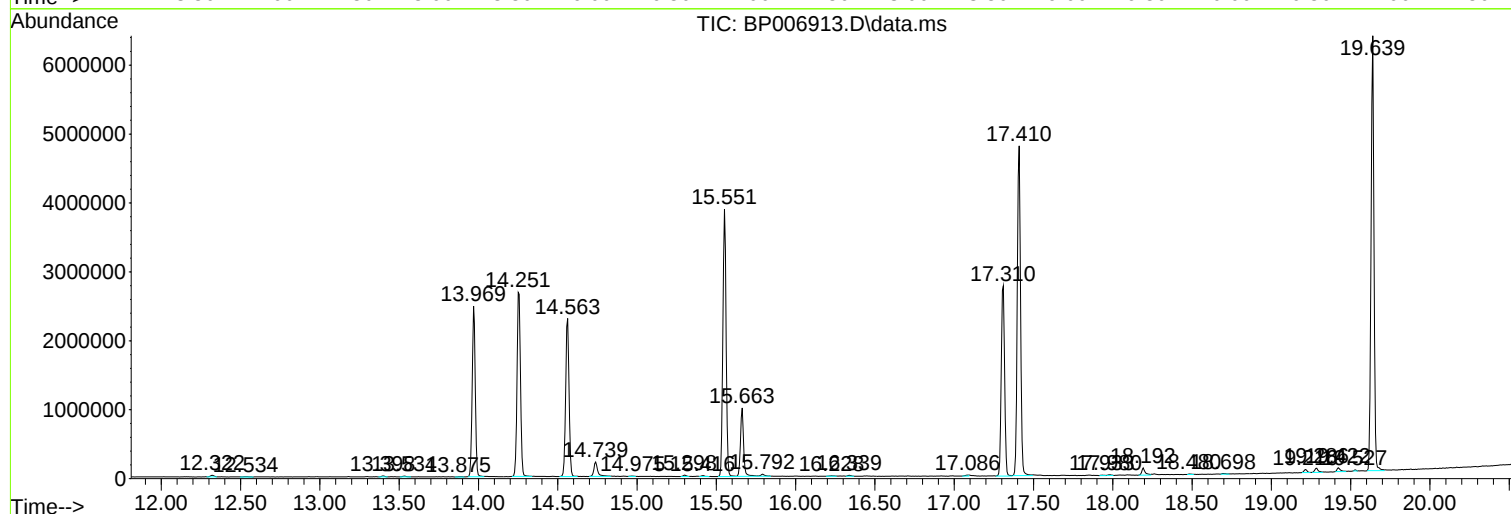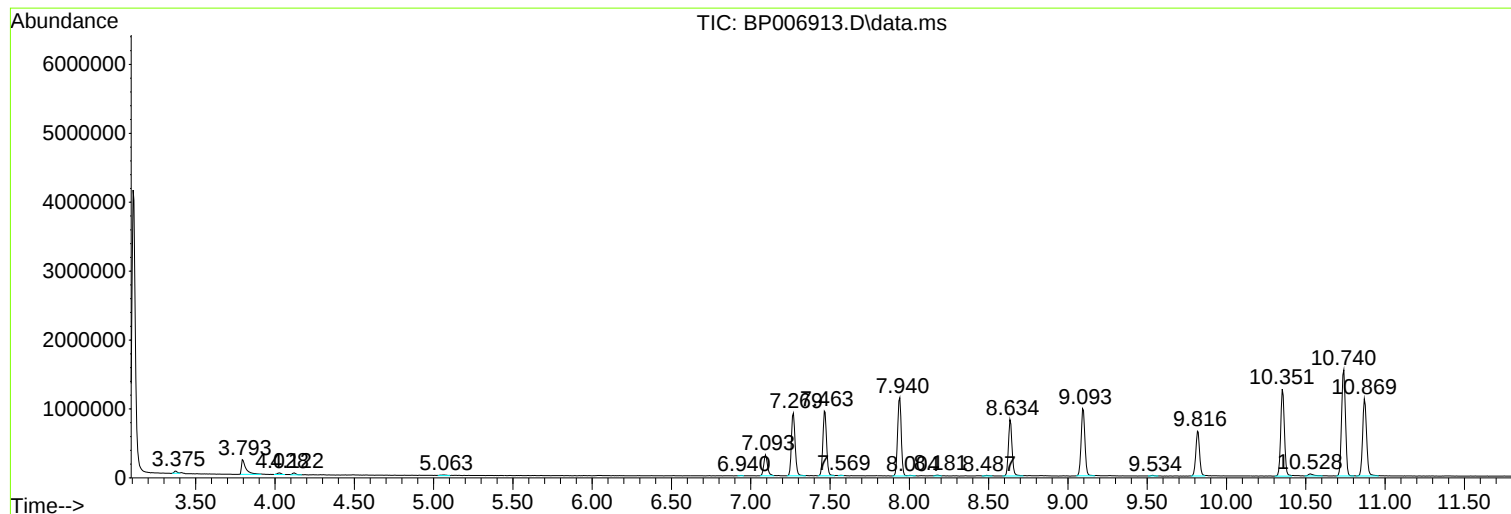

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006913.D
Acq On : 09 Sep 2021 22:41
Operator : CG/JU
Sample : M3608-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006913.D
Acq On : 09 Sep 2021 22:41
Operator : CG/JU
Sample : M3608-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
