

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006916.D
 Acq On : 10 Sep 2021 00:23
 Operator : CG/JU
 Sample : M3651-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBKM7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006916.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	45	49	55	rVB	30033	44343	0.53%	0.063%
2	3.793	117	120	140	rBV	218859	417921	4.95%	0.597%
3	4.022	155	159	166	rVB	23096	38991	0.46%	0.056%
4	4.116	172	175	180	rVB	20706	30180	0.36%	0.043%
5	5.057	329	335	342	rBV	21339	35790	0.42%	0.051%
6	6.034	497	501	505	rBV5	5884	9904	0.12%	0.014%
7	6.940	652	655	662	rVB	9090	12515	0.15%	0.018%
8	7.092	672	681	691	rBV	250366	425060	5.03%	0.607%
9	7.269	704	711	727	rBV	921463	1485042	17.58%	2.121%
10	7.463	737	744	756	rBV	867523	1390917	16.47%	1.987%
11	7.939	817	825	833	rBV	1092133	1757272	20.81%	2.510%
12	8.004	833	836	843	rVB5	10530	16310	0.19%	0.023%
13	8.075	843	848	855	rBV7	4534	9321	0.11%	0.013%
14	8.175	859	865	872	rVB5	13811	27893	0.33%	0.040%
15	8.487	913	918	922	rBV3	9984	16325	0.19%	0.023%
16	8.634	936	943	955	rBV	669829	1115490	13.21%	1.593%
17	9.092	1014	1021	1035	rBV	990228	1665535	19.72%	2.379%
18	9.263	1045	1050	1056	rVB9	6782	12927	0.15%	0.018%
19	9.534	1091	1096	1101	rVB6	6644	11150	0.13%	0.016%
20	9.816	1137	1144	1157	rBV	606506	1018904	12.06%	1.455%
21	10.351	1227	1235	1252	rBV	1140636	1892373	22.41%	2.703%
22	10.528	1259	1265	1282	rBV2	47252	108771	1.29%	0.155%
23	10.739	1293	1301	1314	rBV	1462647	2480922	29.38%	3.543%
24	10.869	1316	1323	1338	rVV	1105915	1899014	22.49%	2.712%
25	12.322	1565	1570	1574	rBV	23794	35494	0.42%	0.051%
26	13.533	1772	1776	1781	rVB7	5198	8603	0.10%	0.012%
27	13.969	1844	1850	1860	rBV	2388359	3293151	38.99%	4.704%
28	14.257	1888	1899	1907	rBV	2684135	3970324	47.01%	5.671%
29	14.563	1944	1951	1961	rBV	2129735	3194931	37.83%	4.563%
30	14.739	1973	1981	1987	rBV	153898	259344	3.07%	0.370%
31	15.304	2070	2077	2083	rBV	112064	162194	1.92%	0.232%
32	15.374	2084	2089	2093	rVB5	9009	15181	0.18%	0.022%
33	15.551	2112	2119	2129	rBV	3940595	5587091	66.16%	7.980%
34	15.663	2132	2138	2150	rBV	920802	1254063	14.85%	1.791%
35	15.792	2156	2160	2165	rVB3	26281	38707	0.46%	0.055%
36	16.121	2210	2216	2220	rVB9	4553	11415	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006916.D
 Acq On : 10 Sep 2021 00:23
 Operator : CG/JU
 Sample : M3651-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBKM7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

37	16.227	2230	2234	2241	rBV9	6531	11170	0.13%	0.016%
38	16.339	2250	2253	2260	rVB9	10296	18806	0.22%	0.027%
39	17.092	2374	2381	2384	rBV2	13341	23449	0.28%	0.033%
40	17.310	2411	2418	2427	rBV	2540584	3669636	43.45%	5.241%
41	17.410	2428	2435	2446	rBV	4858610	6913580	81.86%	9.874%
42	17.980	2527	2532	2539	rBV8	16470	28268	0.33%	0.040%
43	18.092	2549	2551	2555	rVB5	7333	8817	0.10%	0.013%
44	18.192	2564	2568	2577	rBV2	153703	228837	2.71%	0.327%
45	18.692	2651	2653	2656	rBV4	8951	12080	0.14%	0.017%
46	19.215	2738	2742	2746	rBV2	42086	61180	0.72%	0.087%
47	19.286	2750	2754	2758	rVV	55271	76186	0.90%	0.109%
48	19.421	2774	2777	2784	rBV2	92853	128367	1.52%	0.183%
49	19.639	2808	2814	2828	rBV	6355778	8270916	97.94%	11.813%
50	21.098	3059	3062	3067	rBV3	120042	164490	1.95%	0.235%
51	21.392	3107	3112	3122	rBV	3066121	3967564	46.98%	5.667%
52	23.668	3491	3499	3507	rBV	4298315	8445157	100.00%	12.062%
53	23.827	3519	3526	3536	rVB2	2001020	4232756	50.12%	6.046%




Sum of corrected areas: 70014627

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006916.D
Acq On : 10 Sep 2021 00:23
Operator : CG/JU
Sample : M3651-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKM7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

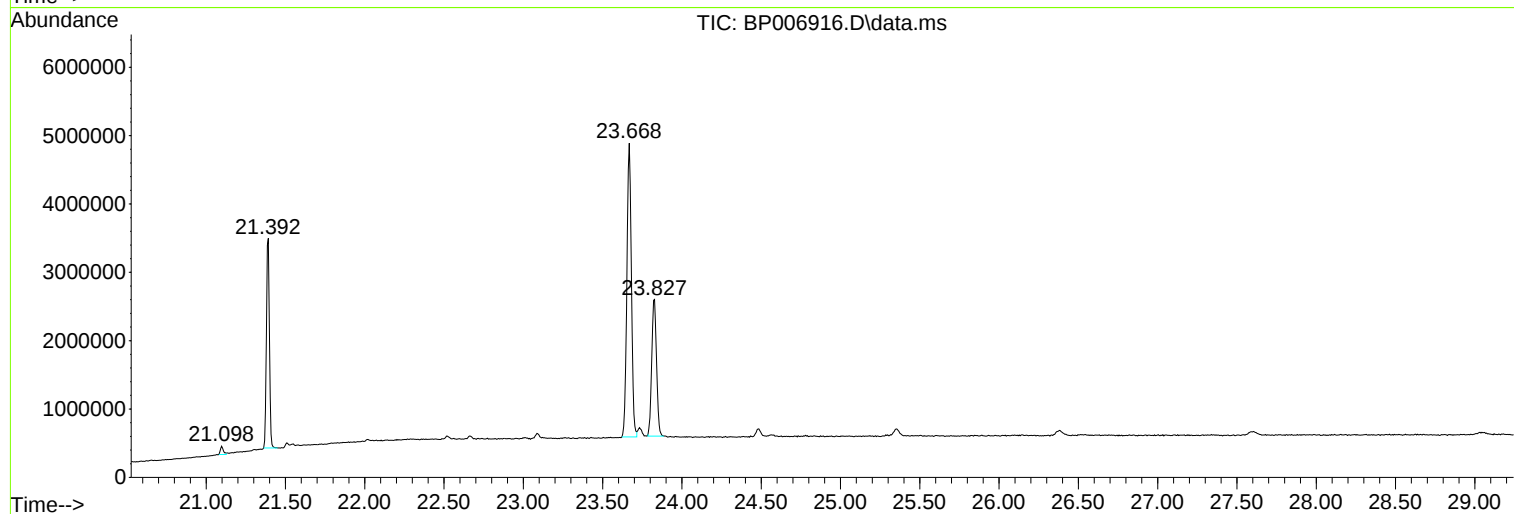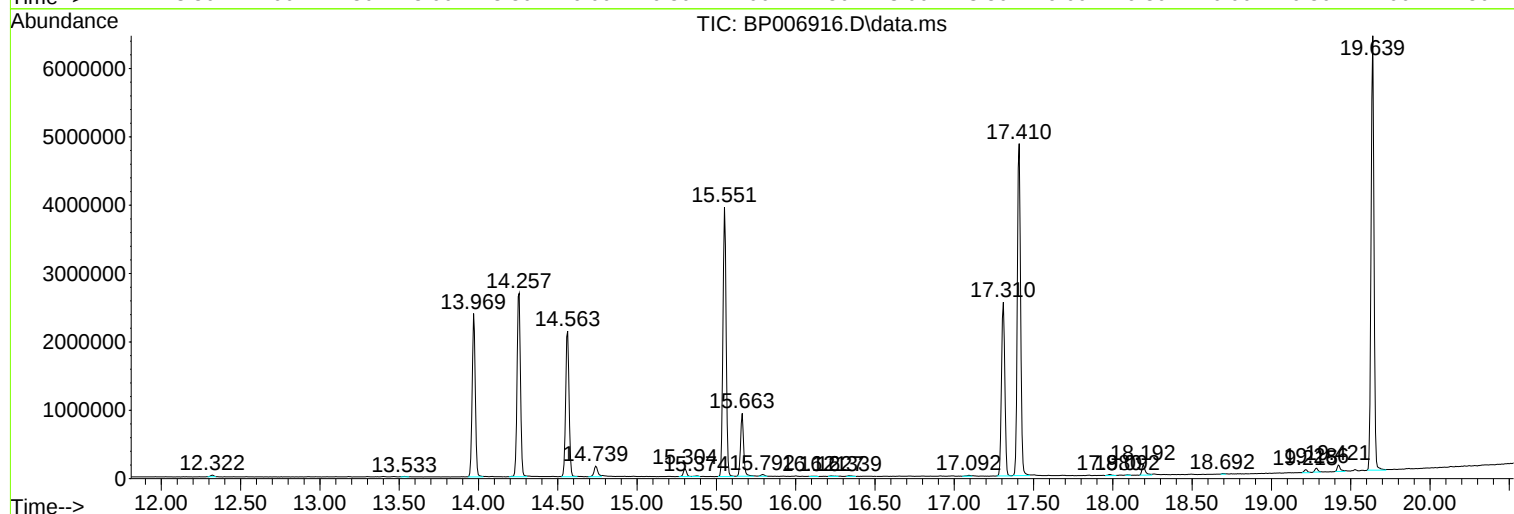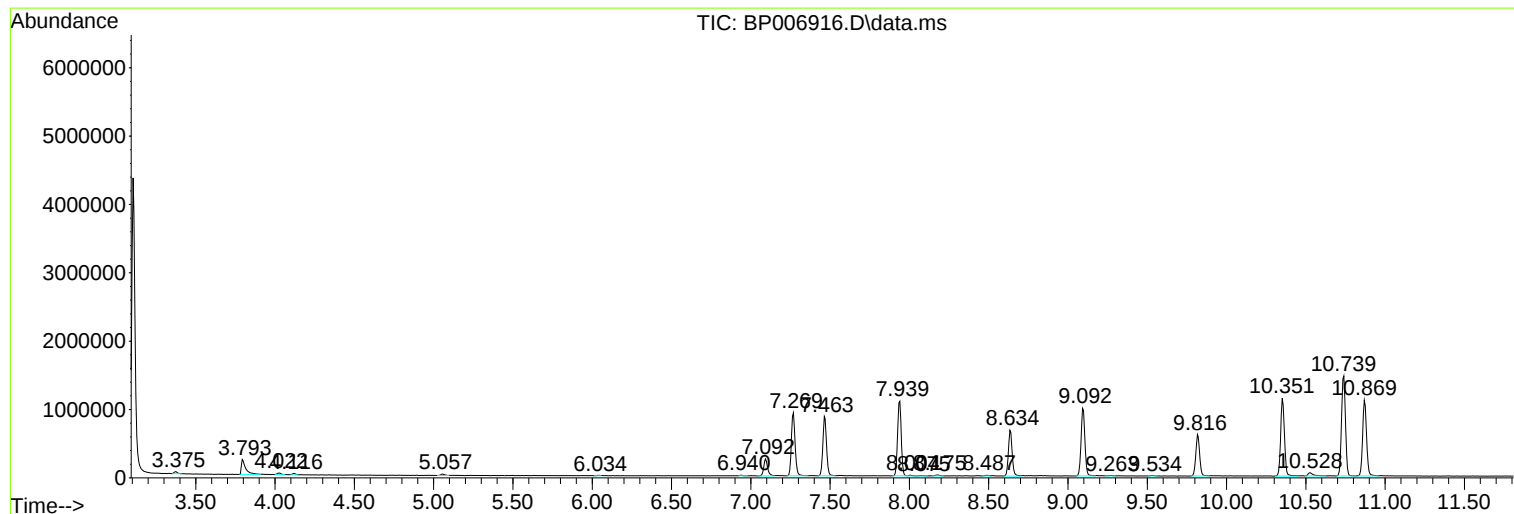

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006916.D
Acq On : 10 Sep 2021 00:23
Operator : CG/JU
Sample : M3651-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKM7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006916.D
Acq On : 10 Sep 2021 00:23
Operator : CG/JU
Sample : M3651-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKM7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
