

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006917.D
 Acq On : 10 Sep 2021 00:57
 Operator : CG/JU
 Sample : M3651-16
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBKN0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006917.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	45	48	54	rVB	40476	50467	0.59%	0.062%
2	3.793	116	120	143	rBV	384217	713997	8.37%	0.882%
3	4.028	155	160	166	rVB2	27757	44539	0.52%	0.055%
4	4.117	171	175	183	rVB	24067	35759	0.42%	0.044%
5	7.093	674	681	691	rBV	342339	545589	6.39%	0.674%
6	7.269	702	711	727	rBV	1014910	1702124	19.95%	2.103%
7	7.463	736	744	757	rBV	1076049	1715044	20.10%	2.118%
8	7.934	816	824	833	rBV	1092722	1787617	20.95%	2.208%
9	8.005	833	836	844	rVV2	13121	22197	0.26%	0.027%
10	8.169	859	864	873	rBV7	10639	24664	0.29%	0.030%
11	8.634	936	943	959	rBV	917266	1486125	17.42%	1.836%
12	9.093	1014	1021	1031	rVB	1140979	1865501	21.86%	2.304%
13	9.299	1049	1056	1062	rVB2	15675	32603	0.38%	0.040%
14	9.816	1137	1144	1155	rBV	788784	1278160	14.98%	1.579%
15	10.034	1176	1181	1186	rVB7	9468	17823	0.21%	0.022%
16	10.140	1194	1199	1205	rVV2	23044	36525	0.43%	0.045%
17	10.352	1228	1235	1246	rBV	1454412	2407277	28.21%	2.974%
18	10.522	1258	1264	1272	rBV	101177	187380	2.20%	0.231%
19	10.740	1291	1301	1307	rBV	1551556	2540645	29.78%	3.138%
20	10.799	1307	1311	1315	rVB3	26272	39377	0.46%	0.049%
21	10.869	1315	1323	1331	rBV	1416276	2415294	28.31%	2.983%
22	10.981	1339	1342	1347	rVB	17722	26350	0.31%	0.033%
23	11.093	1356	1361	1367	rBV7	11209	18981	0.22%	0.023%
24	11.157	1367	1372	1378	rVB4	9873	18004	0.21%	0.022%
25	11.399	1407	1413	1420	rBV8	10088	22023	0.26%	0.027%
26	11.516	1428	1433	1439	rVB7	11351	20601	0.24%	0.025%
27	11.846	1483	1489	1498	rBV7	8762	20999	0.25%	0.026%
28	12.287	1559	1564	1567	rBV	33320	57667	0.68%	0.071%
29	12.322	1567	1570	1574	rVV	28512	42132	0.49%	0.052%
30	12.369	1574	1578	1582	rVB5	11053	18209	0.21%	0.022%
31	12.593	1610	1616	1623	rVB4	18936	39994	0.47%	0.049%
32	12.698	1630	1634	1641	rBV6	9888	20510	0.24%	0.025%
33	12.904	1665	1669	1677	rBV8	13320	28249	0.33%	0.035%
34	13.081	1693	1699	1704	rBV2	14492	25612	0.30%	0.032%
35	13.298	1730	1736	1742	rVB10	12758	27714	0.32%	0.034%
36	13.398	1748	1753	1760	rVV7	23717	52515	0.62%	0.065%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006917.D
 Acq On : 10 Sep 2021 00:57
 Operator : CG/JU
 Sample : M3651-16
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBKN0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

37	13.569	1779	1782	1786	rVV3	18421	30040	0.35%	0.037%
38	13.610	1786	1789	1797	rVB4	23828	50228	0.59%	0.062%
39	13.698	1797	1804	1807	rBV9	9779	17388	0.20%	0.021%
40	13.740	1807	1811	1819	rVB5	16366	31231	0.37%	0.039%
41	13.898	1831	1838	1844	rBV10	9518	27746	0.33%	0.034%
42	13.969	1844	1850	1863	rBV	2972297	4079835	47.82%	5.040%
43	14.151	1878	1881	1887	rVB4	15016	24129	0.28%	0.030%
44	14.251	1892	1898	1913	rVV	3235527	4787459	56.11%	5.914%
45	14.381	1913	1920	1925	rVB	8856	23413	0.27%	0.029%
46	14.557	1939	1950	1957	rBV	2283933	3429135	40.19%	4.236%
47	14.622	1957	1961	1967	rVV	309321	451918	5.30%	0.558%
48	14.740	1975	1981	1992	rBV	224775	372854	4.37%	0.461%
49	14.869	1998	2003	2008	rBV	102902	139343	1.63%	0.172%
50	15.298	2072	2076	2081	rVB	38630	58558	0.69%	0.072%
51	15.551	2112	2119	2132	rBV	4276740	6284067	73.65%	7.762%
52	15.663	2132	2138	2146	rBV	1021036	1387145	16.26%	1.713%
53	15.734	2146	2150	2153	rBV2	46906	75639	0.89%	0.093%
54	15.763	2153	2155	2159	rVB	38506	45012	0.53%	0.056%
55	15.857	2168	2171	2175	rBV4	16510	26853	0.31%	0.033%
56	15.904	2175	2179	2184	rVB4	37158	57668	0.68%	0.071%
57	16.004	2192	2196	2199	rBV2	46529	68294	0.80%	0.084%
58	16.039	2199	2202	2211	rVB2	121520	216618	2.54%	0.268%
59	16.139	2211	2219	2224	rBV4	26488	57812	0.68%	0.071%
60	16.275	2238	2242	2245	rBV2	20359	28374	0.33%	0.035%
61	16.404	2258	2264	2269	rBV2	66320	111936	1.31%	0.138%
62	16.469	2269	2275	2279	rVV8	25319	47478	0.56%	0.059%
63	16.569	2287	2292	2296	rBV3	48644	93223	1.09%	0.115%
64	16.681	2305	2311	2318	rBV3	17444	43042	0.50%	0.053%
65	16.763	2321	2325	2329	rVB3	25221	38487	0.45%	0.048%
66	16.845	2335	2339	2341	rBV5	15669	20747	0.24%	0.026%
67	17.092	2377	2381	2386	rVB3	17602	26530	0.31%	0.033%
68	17.198	2396	2399	2402	rBV	32638	37245	0.44%	0.046%
69	17.257	2406	2409	2412	rVV	32835	35882	0.42%	0.044%
70	17.310	2412	2418	2424	rVB	2711712	3936910	46.14%	4.863%
71	17.410	2428	2435	2445	rBV	4864774	6874201	80.57%	8.491%
72	17.675	2477	2480	2483	rBV5	12104	19909	0.23%	0.025%
73	17.710	2483	2486	2492	rVB4	28558	44659	0.52%	0.055%
74	17.957	2525	2528	2534	rBV4	32425	69970	0.82%	0.086%
75	18.010	2534	2537	2540	rVV	47555	58332	0.68%	0.072%
76	18.045	2540	2543	2548	rVB6	21377	34736	0.41%	0.043%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006917.D
 Acq On : 10 Sep 2021 00:57
 Operator : CG/JU
 Sample : M3651-16
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBKN0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

77	18.098	2548	2552	2555	rBV3	47113	65400	0.77%	0.081%
78	18.133	2555	2558	2563	rVB	61655	79523	0.93%	0.098%
79	18.192	2563	2568	2576	rBV2	154253	242072	2.84%	0.299%
80	18.363	2591	2597	2604	rBV2	153051	242750	2.85%	0.300%
81	18.433	2606	2609	2613	rBV	45308	61233	0.72%	0.076%
82	18.539	2624	2627	2629	rBV3	21438	25020	0.29%	0.031%
83	18.645	2641	2645	2650	rVB2	46671	65470	0.77%	0.081%
84	18.692	2650	2653	2657	rBV4	28406	32113	0.38%	0.040%
85	18.745	2659	2662	2666	rVV3	35831	44501	0.52%	0.055%
86	18.851	2677	2680	2686	rBV	38872	51378	0.60%	0.063%
87	18.916	2688	2691	2695	rVB5	29706	34960	0.41%	0.043%
88	19.280	2749	2753	2756	rBV	75920	116998	1.37%	0.145%
89	19.310	2756	2758	2765	rVB	75539	100025	1.17%	0.124%
90	19.422	2774	2777	2785	rVB3	109151	143528	1.68%	0.177%
91	19.639	2808	2814	2826	rBV	6319006	8532039	100.00%	10.539%
92	20.033	2875	2881	2886	rBV	165913	270915	3.18%	0.335%
93	20.086	2887	2890	2897	rVV	60513	87289	1.02%	0.108%
94	20.186	2904	2907	2911	rVB3	50396	64403	0.75%	0.080%
95	20.686	2989	2992	2995	rBV	60587	80754	0.95%	0.100%
96	20.727	2996	2999	3006	rVB2	89213	128922	1.51%	0.159%
97	21.098	3059	3062	3068	rBV2	202550	263078	3.08%	0.325%
98	21.386	3106	3111	3118	rBV	3419821	4533078	53.13%	5.599%
99	23.668	3491	3499	3507	rBV	4293506	8364983	98.04%	10.333%
100	23.821	3518	3525	3536	rVB2	2293287	4673815	54.78%	5.773%




Sum of corrected areas: 80956560

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP006917\
Data File : BP006917.D
Acq On : 10 Sep 2021 00:57
Operator : CG/JU
Sample : M3651-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKN0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP006917.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

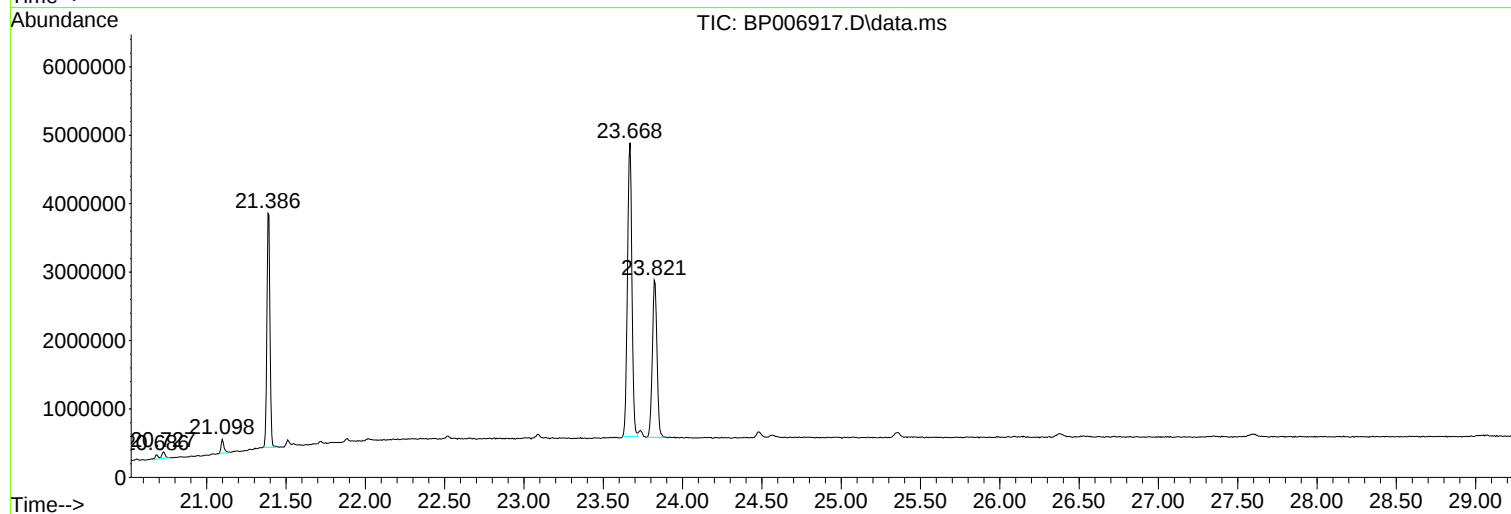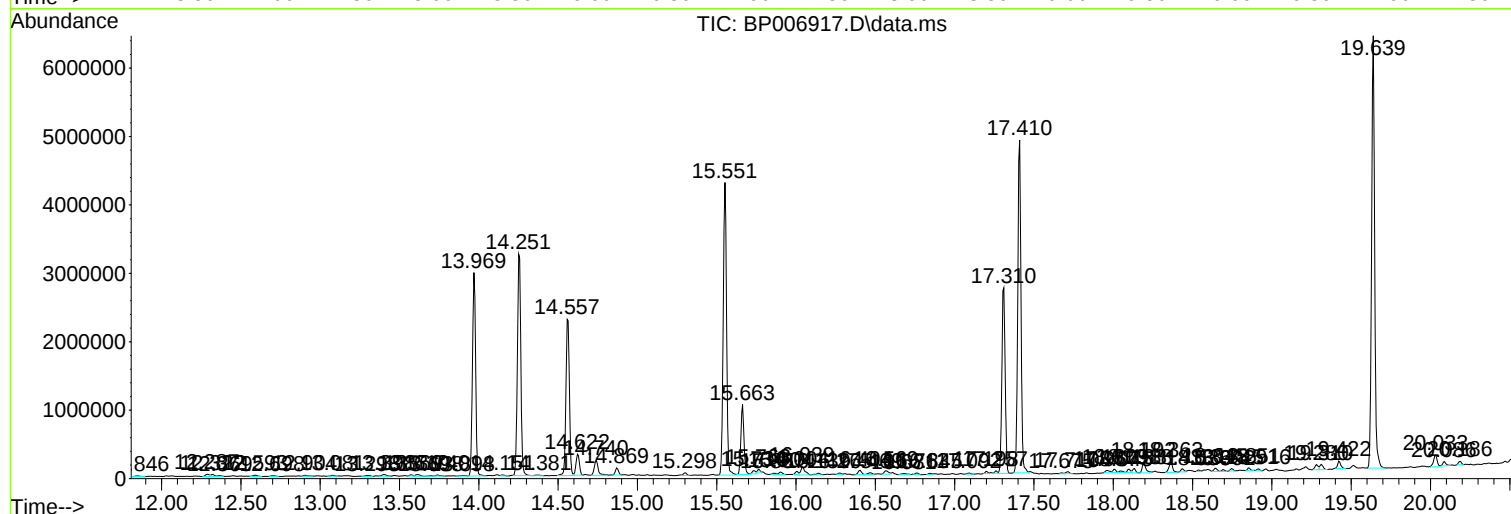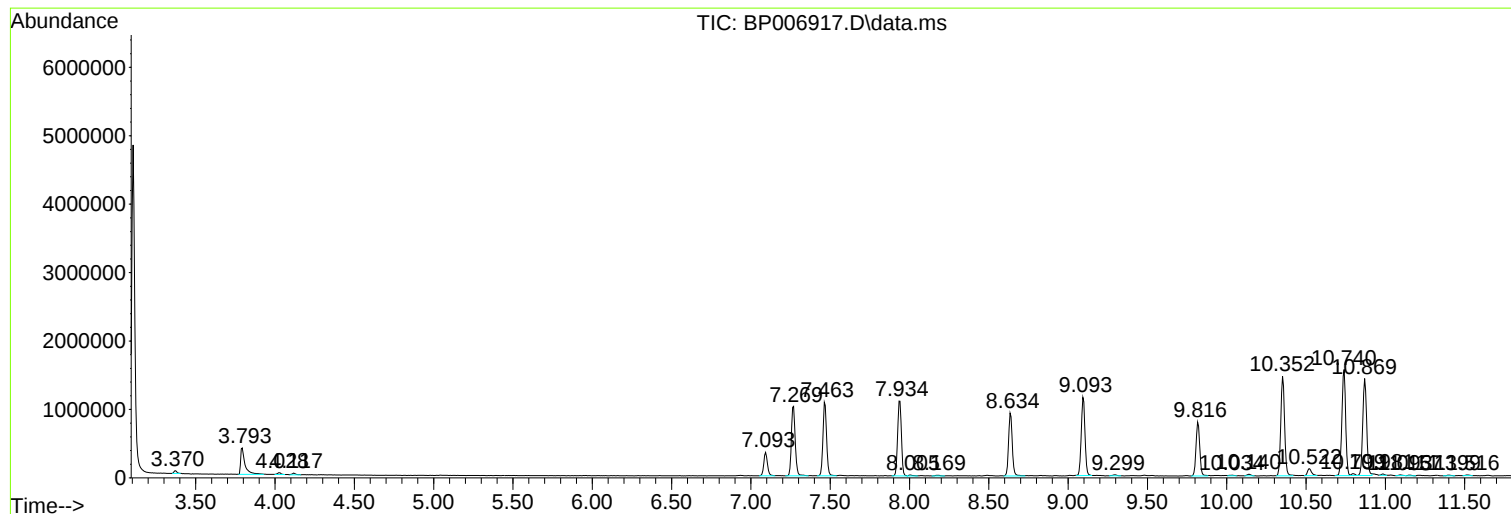

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006917.D
Acq On : 10 Sep 2021 00:57
Operator : CG/JU
Sample : M3651-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKN0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006917.D
Acq On : 10 Sep 2021 00:57
Operator : CG/JU
Sample : M3651-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKN0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
