

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP006921\
 Data File : BP006921.D
 Acq On : 10 Sep 2021 03:47
 Operator : CG/JU
 Sample : PB138947BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK947

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP006921.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006921.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	44	48	58	rVB	109071	154820	1.82%	0.178%
2	3.787	115	119	144	rBV	1180492	2078373	24.38%	2.391%
3	4.117	171	175	180	rVB	24060	35740	0.42%	0.041%
4	7.093	674	681	691	rBV	1478647	2290676	26.87%	2.635%
5	7.263	704	710	727	rVB	1182719	1895095	22.23%	2.180%
6	7.463	737	744	757	rBV	1490395	2367028	27.77%	2.723%
7	7.934	817	824	834	rBV	1281695	2026853	23.78%	2.332%
8	8.634	936	943	960	rBV	1762543	2831629	33.22%	3.258%
9	9.093	1010	1021	1036	rBV	1296493	2135247	25.05%	2.457%
10	9.816	1136	1144	1159	rBV	925668	1511539	17.73%	1.739%
11	10.351	1227	1235	1253	rBV	1692974	2766579	32.46%	3.183%
12	10.740	1291	1301	1311	rBV	1669029	2864510	33.60%	3.296%
13	10.869	1315	1323	1345	rVV	1650096	2882388	33.81%	3.316%
14	12.322	1563	1570	1576	rBV2	27989	50322	0.59%	0.058%
15	13.534	1771	1776	1781	rVB5	5528	10643	0.12%	0.012%
16	13.969	1843	1850	1866	rBV	2988567	4135142	48.51%	4.757%
17	14.251	1890	1898	1912	rBV	3414678	4987072	58.50%	5.737%
18	14.563	1943	1951	1962	rBV	2518888	3753968	44.04%	4.319%
19	14.739	1974	1981	1996	rBV	1269561	1846387	21.66%	2.124%
20	15.551	2111	2119	2128	rBV	4372988	6297533	73.88%	7.245%
21	15.663	2131	2138	2154	rVV	1066947	1479244	17.35%	1.702%
22	15.792	2155	2160	2166	rVB	30771	51964	0.61%	0.060%
23	16.228	2229	2234	2239	rBV9	5271	10846	0.13%	0.012%
24	16.334	2249	2252	2256	rVB5	7151	9751	0.11%	0.011%
25	17.092	2378	2381	2388	rVB3	13984	23728	0.28%	0.027%
26	17.310	2411	2418	2428	rBV	3042618	4404555	51.67%	5.067%
27	17.404	2428	2434	2445	rBV	4752538	6981620	81.90%	8.032%
28	18.198	2565	2569	2574	rBV8	11237	21814	0.26%	0.025%
29	19.216	2738	2742	2746	rBV2	47664	72190	0.85%	0.083%
30	19.280	2749	2753	2760	rVV	54975	83134	0.98%	0.096%
31	19.639	2808	2814	2827	rBV	6336758	8396579	98.50%	9.660%
32	21.386	3106	3111	3127	rVB	3558383	4873849	57.18%	5.607%
33	23.668	3491	3499	3507	rBV2	4196156	8524330	100.00%	9.807%
34	23.821	3518	3525	3534	rVB2	2499812	5066370	59.43%	5.829%

Sum of corrected areas: 86921518

Instrument :

BNA_P

ClientSampleId :




SBLK947

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006921.D
Acq On : 10 Sep 2021 03:47
Operator : CG/JU
Sample : PB138947BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK947

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

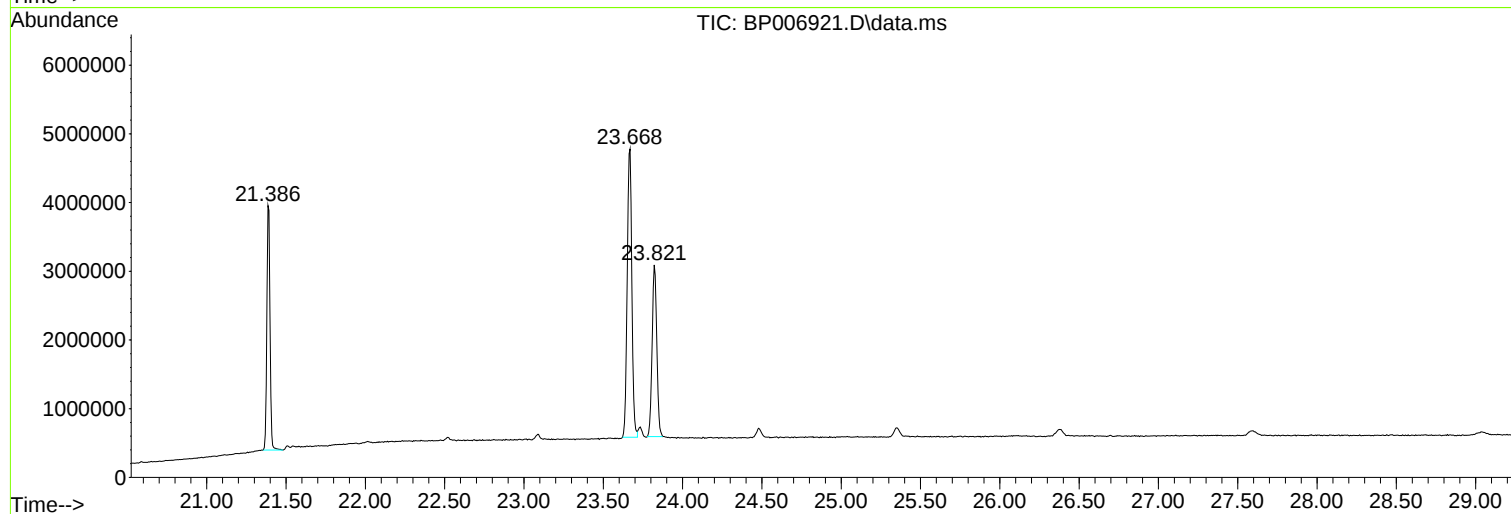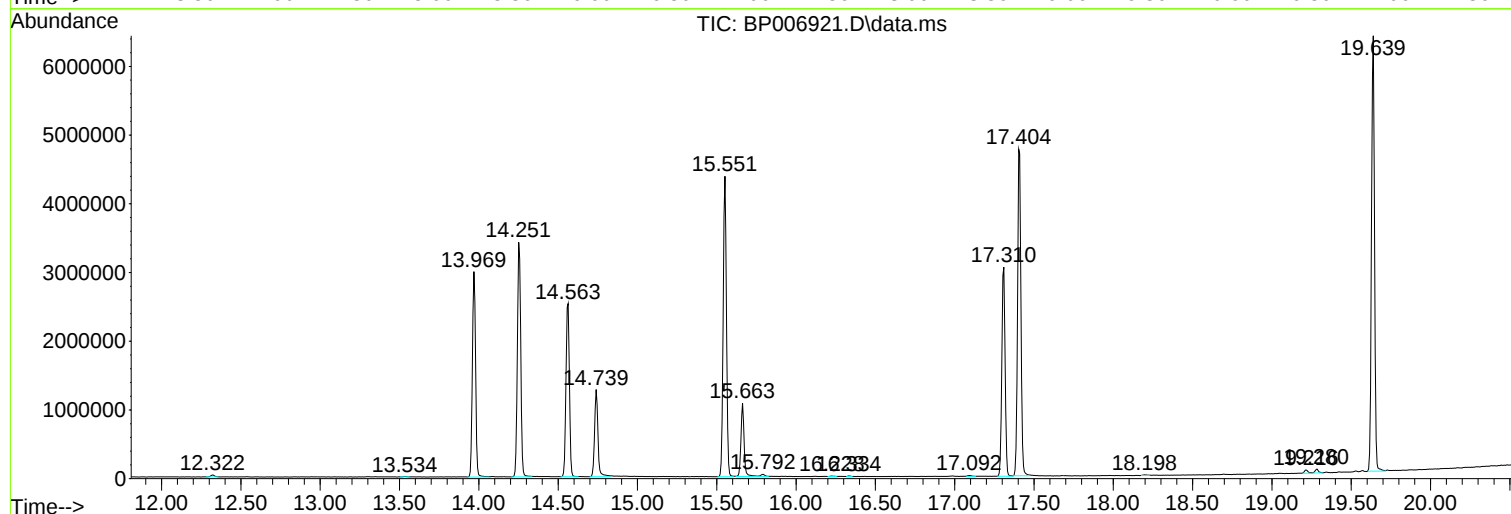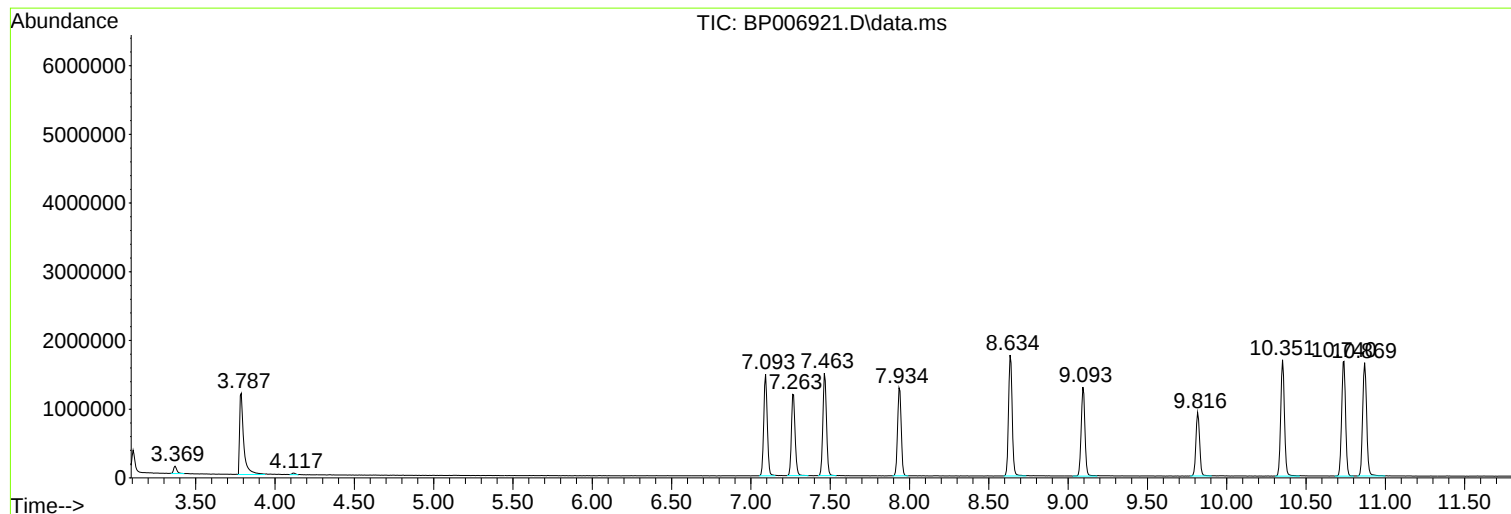

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006921.D
Acq On : 10 Sep 2021 03:47
Operator : CG/JU
Sample : PB138947BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK947

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006921.D
Acq On : 10 Sep 2021 03:47
Operator : CG/JU
Sample : PB138947BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK947

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
