

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006922.D
 Acq On : 10 Sep 2021 04:21
 Operator : CG/JU
 Sample : PB138976BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK976

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006922.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	44	48	57	rVB	108456	150205	1.75%	0.173%
2	3.781	116	118	141	rBV	1230418	1992357	23.19%	2.298%
3	4.117	171	175	181	rVB	27319	40550	0.47%	0.047%
4	7.093	674	681	694	rBV	1411871	2250242	26.19%	2.595%
5	7.264	704	710	722	rBV	1176411	1859893	21.65%	2.145%
6	7.464	737	744	757	rBV	1494592	2322781	27.04%	2.679%
7	7.934	817	824	835	rBV	1245529	1976265	23.00%	2.279%
8	8.634	936	943	956	rBV	1728962	2763075	32.16%	3.187%
9	9.093	1014	1021	1035	rBV	1298827	2078525	24.19%	2.397%
10	9.816	1137	1144	1153	rBV	916797	1476406	17.19%	1.703%
11	10.352	1227	1235	1248	rBV	1643244	2721038	31.67%	3.138%
12	10.734	1293	1300	1312	rVB	1633295	2806491	32.67%	3.237%
13	10.869	1315	1323	1337	rBV	1657928	2825979	32.89%	3.259%
14	12.316	1563	1569	1579	rBV	27670	53094	0.62%	0.061%
15	13.534	1770	1776	1780	rBV3	7008	11923	0.14%	0.014%
16	13.969	1843	1850	1863	rBV	2988628	4121334	47.97%	4.753%
17	14.251	1891	1898	1917	rBV	3343953	4945161	57.56%	5.703%
18	14.557	1943	1950	1962	rBV	2478106	3733858	43.46%	4.306%
19	14.740	1974	1981	1996	rBV	1270508	1854088	21.58%	2.138%
20	14.916	2009	2011	2018	rVB8	7153	10778	0.13%	0.012%
21	15.551	2112	2119	2129	rBV	4345905	6275779	73.05%	7.238%
22	15.663	2132	2138	2154	rVV	1098862	1505669	17.53%	1.736%
23	15.793	2155	2160	2168	rVB	33053	56556	0.66%	0.065%
24	16.222	2229	2233	2239	rBV9	5683	10231	0.12%	0.012%
25	16.334	2248	2252	2257	rBV6	7773	14159	0.16%	0.016%
26	16.987	2359	2363	2367	rVB7	7254	10006	0.12%	0.012%
27	17.092	2375	2381	2384	rBV3	13421	22380	0.26%	0.026%
28	17.310	2410	2418	2428	rBV	3107803	4438055	51.66%	5.118%
29	17.404	2428	2434	2447	rBV	4751976	7015445	81.66%	8.091%
30	18.192	2564	2568	2572	rBV4	16177	27128	0.32%	0.031%
31	19.216	2738	2742	2748	rBV2	46915	62410	0.73%	0.072%
32	19.281	2749	2753	2759	rVV	55059	75415	0.88%	0.087%
33	19.339	2761	2763	2769	rVB4	15523	17513	0.20%	0.020%
34	19.569	2800	2802	2807	rVB3	18682	20320	0.24%	0.023%
35	19.639	2808	2814	2826	rBV	6406393	8502148	98.96%	9.806%
36	21.386	3106	3111	3125	rVB	3738169	4910743	57.16%	5.664%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006922.D
Acq On : 10 Sep 2021 04:21
Operator : CG/JU
Sample : PB138976BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK976

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Title : SVOA CALIBRATION

37	23.669	3491	3499	3507	rBV2	4238074	8591107	100.00%	9.908%
38	23.822	3518	3525	3537	rVB2	2515361	5158125	60.04%	5.949%




Sum of corrected areas: 86707232

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006922.D
Acq On : 10 Sep 2021 04:21
Operator : CG/JU
Sample : PB138976BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK976

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

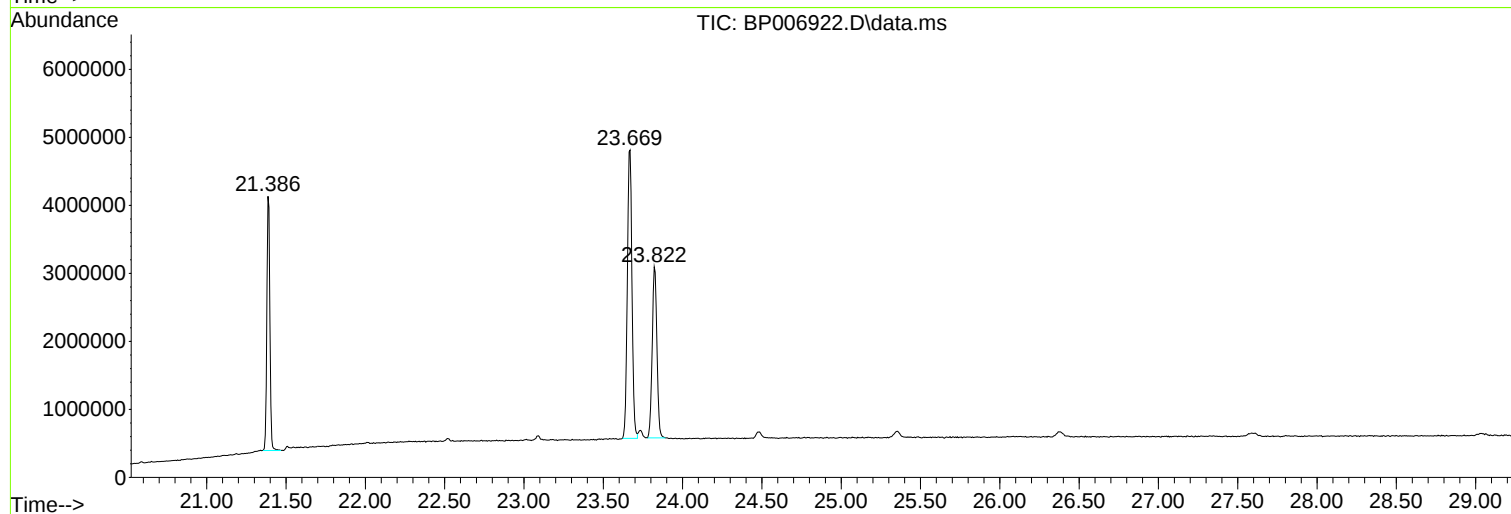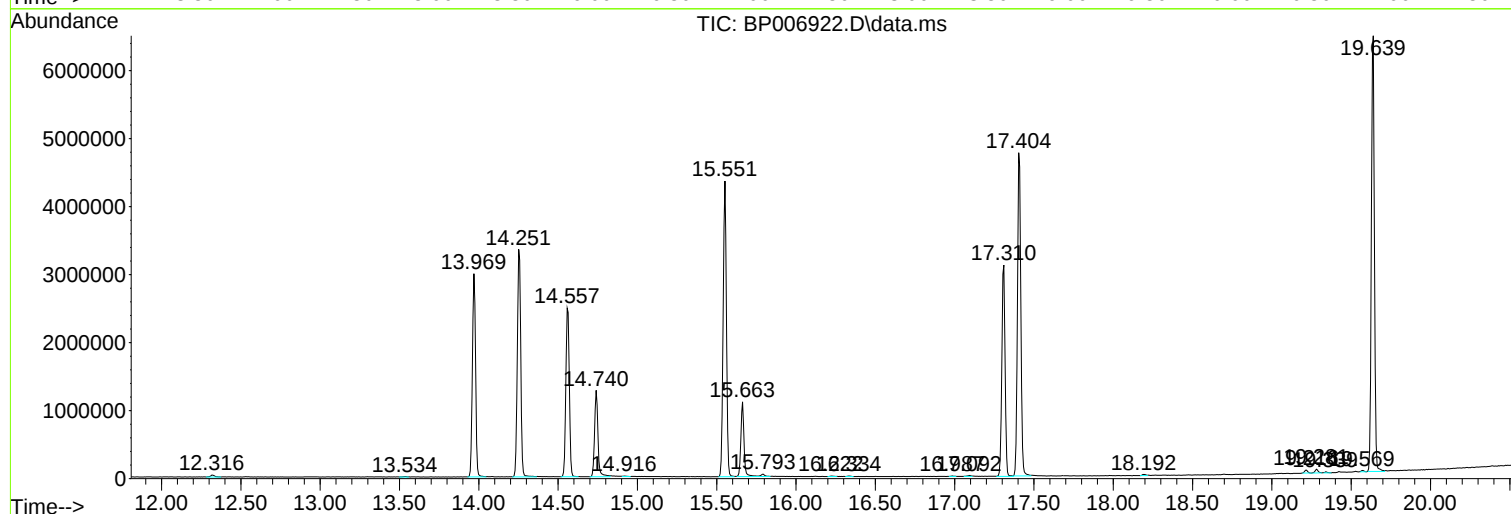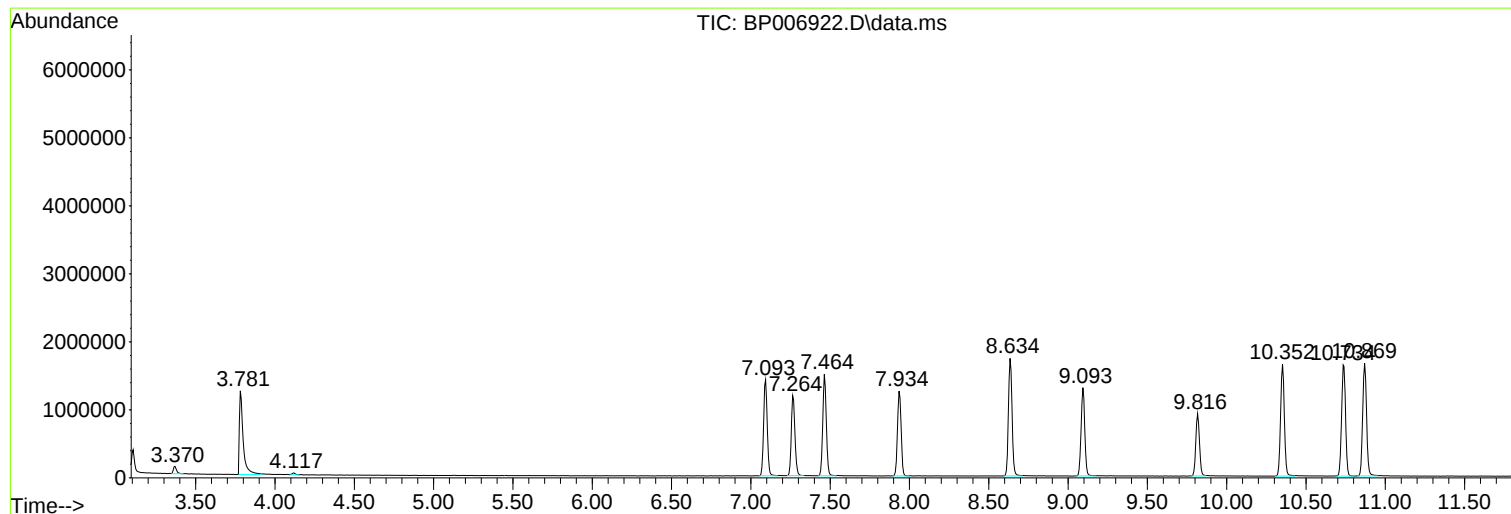

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006922.D
Acq On : 10 Sep 2021 04:21
Operator : CG/JU
Sample : PB138976BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK976

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006922.D
Acq On : 10 Sep 2021 04:21
Operator : CG/JU
Sample : PB138976BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK976

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
