

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006928.D
 Acq On : 10 Sep 2021 07:45
 Operator : CG/JU
 Sample : M3608-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBKK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006928.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	45	48	54	rVB	42264	59387	0.66%	0.074%
2	3.793	118	120	139	rBV	258147	488906	5.45%	0.610%
3	4.022	155	159	166	rVB2	30154	47254	0.53%	0.059%
4	4.122	171	176	183	rVB	26129	43650	0.49%	0.054%
5	7.093	675	681	690	rBV	365094	583690	6.51%	0.729%
6	7.263	704	710	727	rBV	1108307	1791424	19.97%	2.236%
7	7.463	737	744	758	rBV	1183064	1870101	20.85%	2.334%
8	7.563	758	761	769	rVB8	8151	15937	0.18%	0.020%
9	7.934	818	824	832	rBV	1147897	1822792	20.32%	2.275%
10	8.075	844	848	856	rVB10	5121	10256	0.11%	0.013%
11	8.169	859	864	871	rBV6	10125	20246	0.23%	0.025%
12	8.487	913	918	922	rBV5	7471	14242	0.16%	0.018%
13	8.634	935	943	957	rBV	1006127	1580011	17.61%	1.972%
14	9.093	1014	1021	1033	rBV	1242684	2027286	22.60%	2.530%
15	9.528	1091	1095	1102	rVB6	7462	10520	0.12%	0.013%
16	9.816	1135	1144	1160	rBV	895820	1457280	16.25%	1.819%
17	10.351	1226	1235	1252	rBV	1543320	2526749	28.17%	3.154%
18	10.534	1260	1266	1275	rBV3	14932	35851	0.40%	0.045%
19	10.734	1293	1300	1312	rBV	1547688	2622066	29.23%	3.273%
20	10.869	1315	1323	1341	rBV	1428594	2429612	27.09%	3.032%
21	12.322	1564	1570	1575	rBV	28483	47477	0.53%	0.059%
22	12.934	1669	1674	1677	rBV7	6159	9083	0.10%	0.011%
23	13.181	1712	1716	1720	rVB6	8188	10557	0.12%	0.013%
24	13.534	1772	1776	1784	rVB4	7974	13065	0.15%	0.016%
25	13.969	1843	1850	1862	rBV	2981079	4083121	45.52%	5.096%
26	14.251	1891	1898	1910	rBV	3434474	4941666	55.09%	6.168%
27	14.557	1943	1950	1959	rBV	2416407	3532291	39.38%	4.409%
28	14.740	1972	1981	1990	rBV	237920	400987	4.47%	0.500%
29	14.975	2017	2021	2027	rVB9	7590	11515	0.13%	0.014%
30	15.369	2084	2088	2094	rVB7	5476	10365	0.12%	0.013%
31	15.551	2112	2119	2131	rBV	4647291	6521240	72.70%	8.139%
32	15.663	2131	2138	2153	rVV	1097548	1573560	17.54%	1.964%
33	15.787	2155	2159	2166	rVB2	30640	49528	0.55%	0.062%
34	16.004	2192	2196	2200	rVB7	8347	11358	0.13%	0.014%
35	16.334	2249	2252	2258	rVB6	12266	18278	0.20%	0.023%
36	17.092	2372	2381	2385	rBV3	15838	30545	0.34%	0.038%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006928.D
 Acq On : 10 Sep 2021 07:45
 Operator : CG/JU
 Sample : M3608-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBKK0

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

37	17.304	2410	2417	2427	rBV	2852054	4181027	46.61%	5.218%
38	17.404	2428	2434	2446	rBV	5171544	7519222	83.82%	9.385%
39	17.980	2529	2532	2538	rVB6	13541	16538	0.18%	0.021%
40	18.192	2563	2568	2576	rBV	118762	182037	2.03%	0.227%
41	19.022	2706	2709	2715	rBV6	24517	31123	0.35%	0.039%
42	19.216	2738	2742	2746	rBV2	48072	60577	0.68%	0.076%
43	19.280	2750	2753	2761	rVB	61730	88991	0.99%	0.111%
44	19.422	2774	2777	2785	rBV4	52644	72780	0.81%	0.091%
45	19.639	2808	2814	2825	rBV	6788309	8970180	100.00%	11.196%
46	21.098	3059	3062	3066	rBV2	124358	150195	1.67%	0.187%
47	21.304	3093	3097	3101	rBV	156430	202228	2.25%	0.252%
48	21.386	3106	3111	3121	rVV	3429701	4526268	50.46%	5.649%
49	23.668	3491	3499	3506	rBV2	4492767	8743844	97.48%	10.913%
50	23.821	3518	3525	3538	rVB2	2218897	4654023	51.88%	5.809%




Sum of corrected areas: 80120929

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP006921\
Data File : BP006928.D
Acq On : 10 Sep 2021 07:45
Operator : CG/JU
Sample : M3608-04
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKK0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP006921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

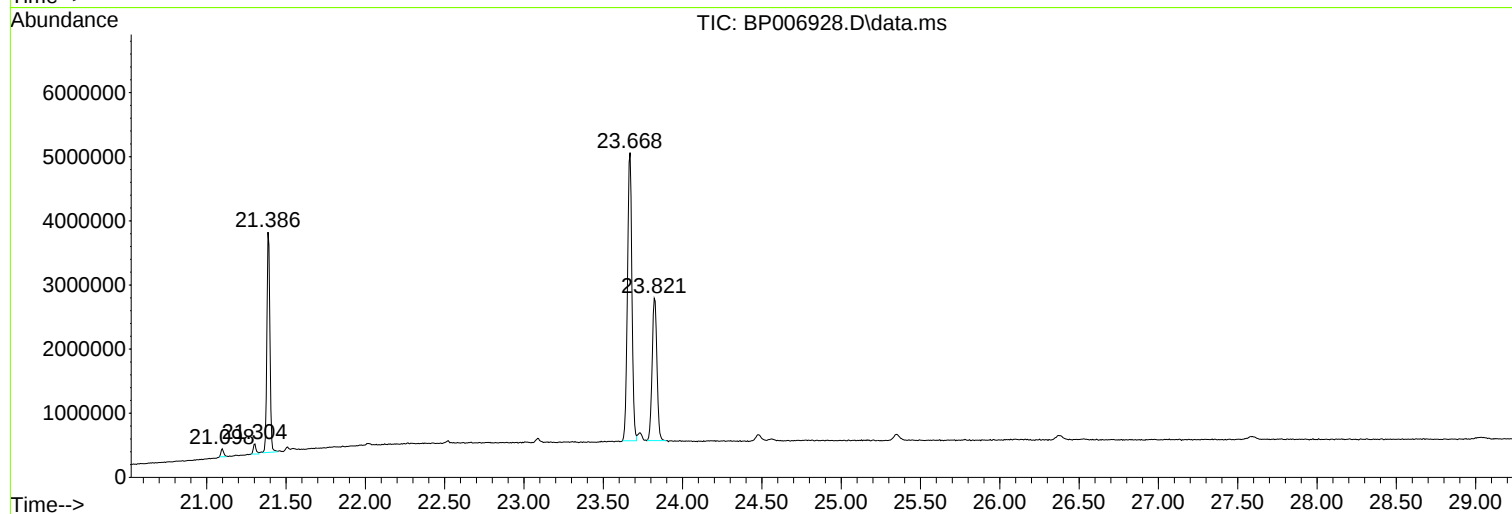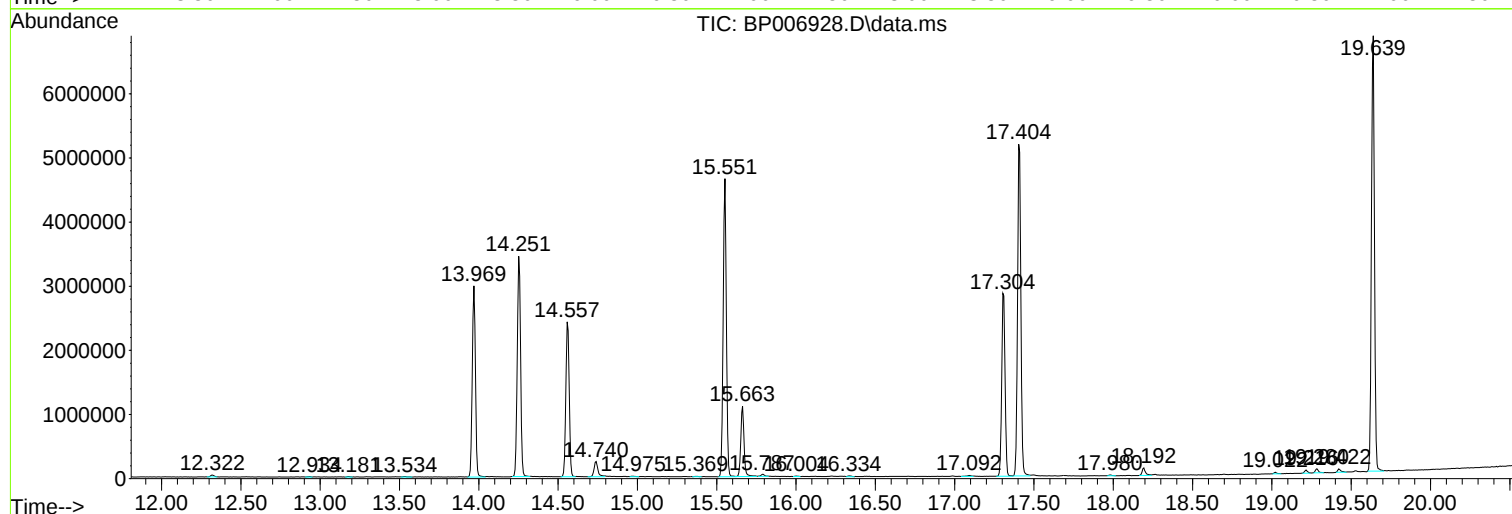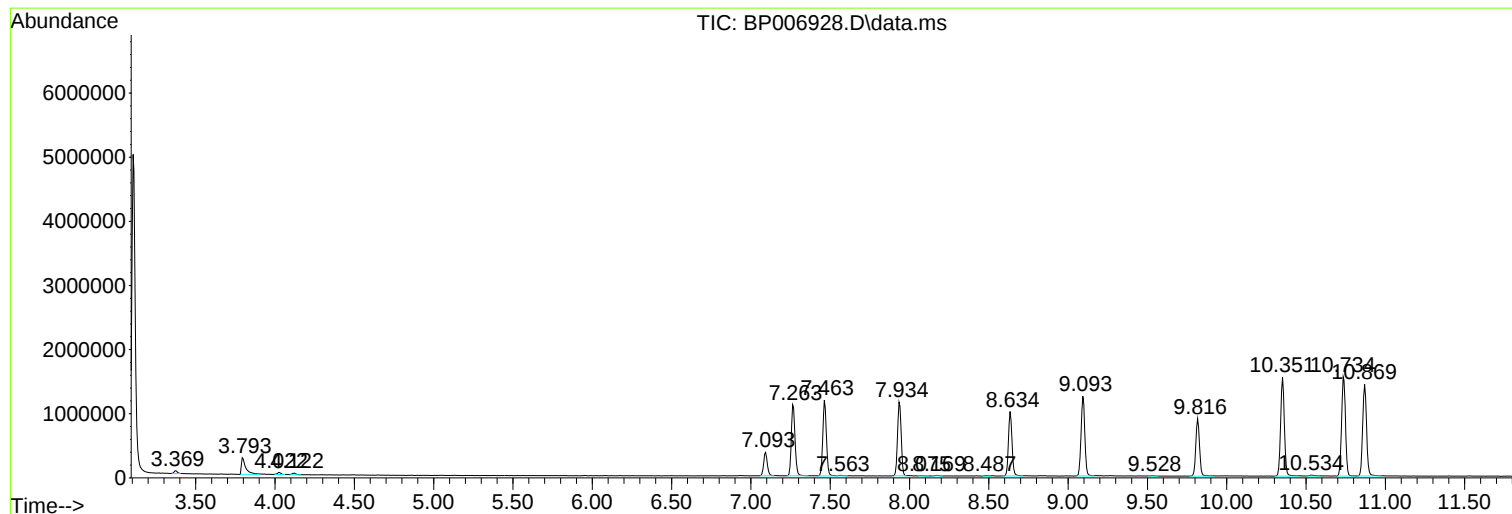

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006928.D
Acq On : 10 Sep 2021 07:45
Operator : CG/JU
Sample : M3608-04
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKK0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006928.D
Acq On : 10 Sep 2021 07:45
Operator : CG/JU
Sample : M3608-04
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKK0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
