

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006930.D
 Acq On : 10 Sep 2021 08:55
 Operator : CG/JU
 Sample : PB138946BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK946

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006930.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	44	48	58	rVB	88987	136137	2.00%	0.186%
2	3.787	116	119	152	rVB	990373	1750640	25.77%	2.396%
3	4.117	171	175	181	rVB	19054	30983	0.46%	0.042%
4	7.093	673	681	694	rBV	1161231	1879431	27.67%	2.572%
5	7.263	704	710	725	rVB	978391	1558497	22.95%	2.133%
6	7.463	735	744	759	rBV	1256035	1976474	29.10%	2.705%
7	7.934	817	824	835	rBV	1214821	1856614	27.34%	2.541%
8	8.634	936	943	953	rBV	1478151	2323521	34.21%	3.180%
9	9.093	1013	1021	1030	rBV	1091794	1747004	25.72%	2.391%
10	9.816	1136	1144	1158	rBV	772900	1274967	18.77%	1.745%
11	10.351	1226	1235	1253	rBV	1392274	2312994	34.05%	3.165%
12	10.734	1292	1300	1310	rBV	1547454	2614202	38.49%	3.578%
13	10.869	1313	1323	1335	rBV	1426860	2394153	35.25%	3.276%
14	12.322	1565	1570	1579	rVB	25868	45280	0.67%	0.062%
15	13.540	1772	1777	1781	rBV7	5278	8649	0.13%	0.012%
16	13.969	1843	1850	1864	rBV	2483563	3451447	50.82%	4.723%
17	14.251	1888	1898	1912	rBV	2906033	4209291	61.97%	5.760%
18	14.557	1942	1950	1961	rBV	2304607	3447738	50.76%	4.718%
19	14.739	1973	1981	1993	rBV	993030	1462017	21.53%	2.001%
20	15.551	2112	2119	2130	rBV	3764182	5316597	78.28%	7.276%
21	15.663	2131	2138	2150	rBV	836865	1168100	17.20%	1.599%
22	15.792	2155	2160	2167	rVB2	25349	42992	0.63%	0.059%
23	16.222	2230	2233	2237	rBV5	4378	7584	0.11%	0.010%
24	16.334	2248	2252	2258	rVB10	6483	11121	0.16%	0.015%
25	16.986	2359	2363	2368	rBV6	5523	9715	0.14%	0.013%
26	17.092	2377	2381	2387	rVB	11856	17885	0.26%	0.024%
27	17.310	2411	2418	2428	rBV	2741440	3979265	58.59%	5.446%
28	17.410	2428	2435	2448	rBV	3923394	5742813	84.55%	7.859%
29	19.216	2739	2742	2747	rVB2	33665	42217	0.62%	0.058%
30	19.286	2750	2754	2761	rVV	43632	62358	0.92%	0.085%
31	19.639	2808	2814	2827	rBV	5352409	6792064	100.00%	9.295%
32	21.392	3107	3112	3126	rVB	3314935	4289110	63.15%	5.870%
33	23.668	3492	3499	3508	rBV2	3463765	6620257	97.47%	9.060%
34	23.827	3519	3526	3539	rVB2	2204661	4491091	66.12%	6.146%

Sum of corrected areas: 73073208

Instrument :

BNA_P

ClientSampleId :




SBLK946

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006930.D
Acq On : 10 Sep 2021 08:55
Operator : CG/JU
Sample : PB138946BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK946

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

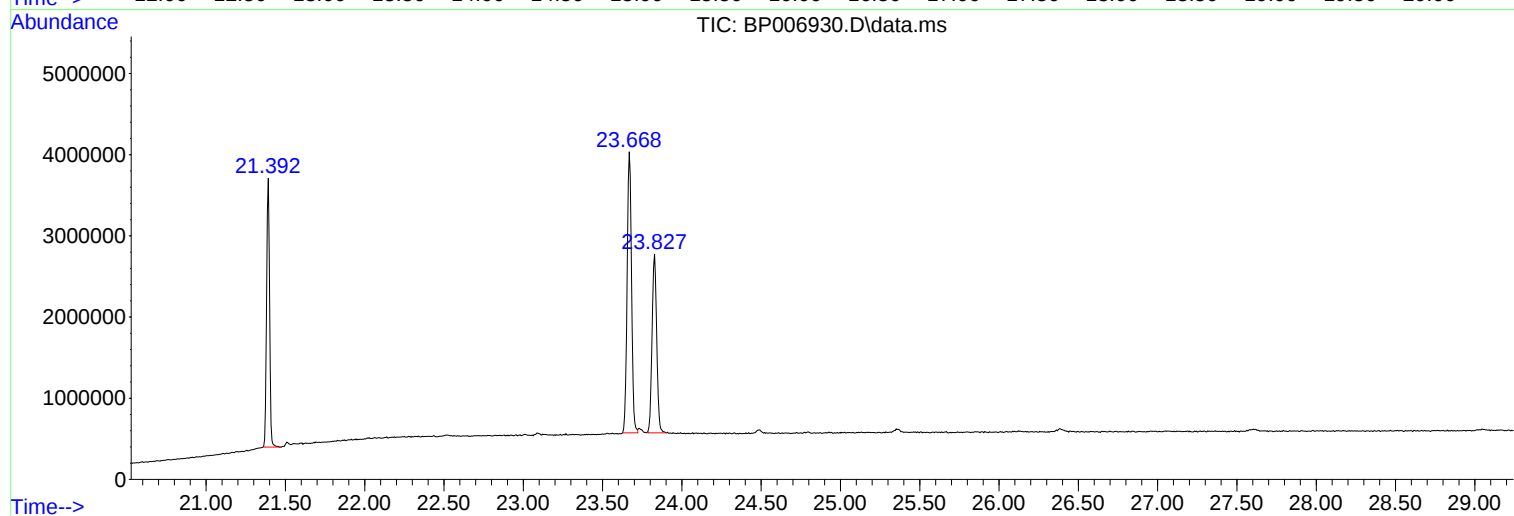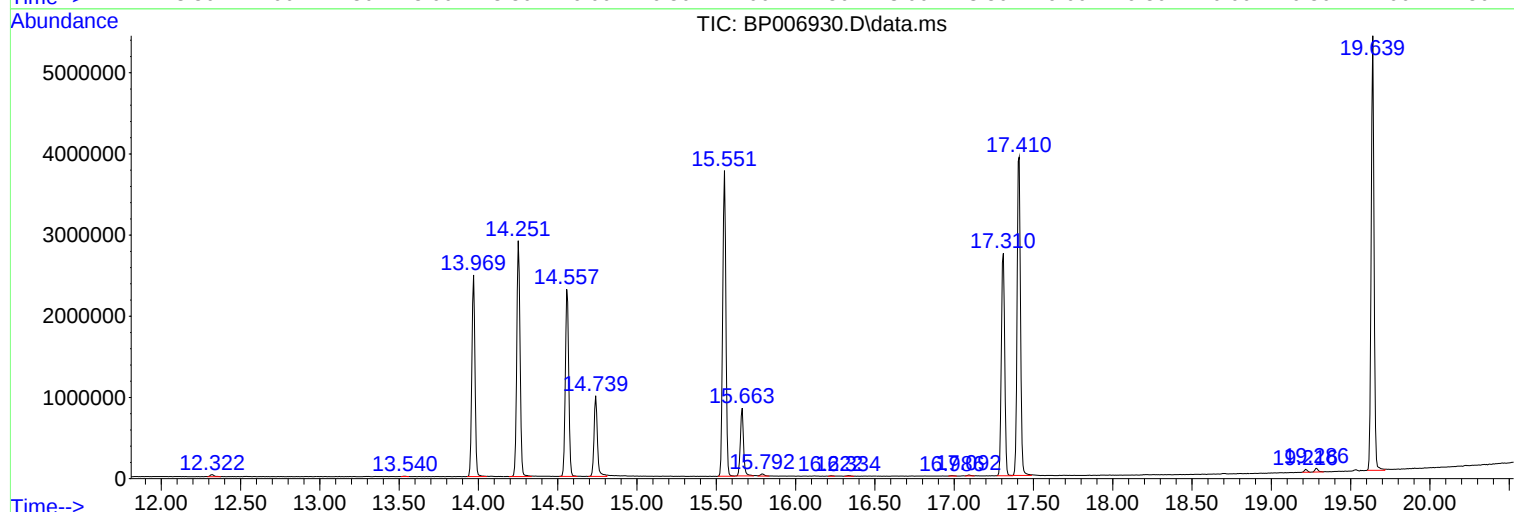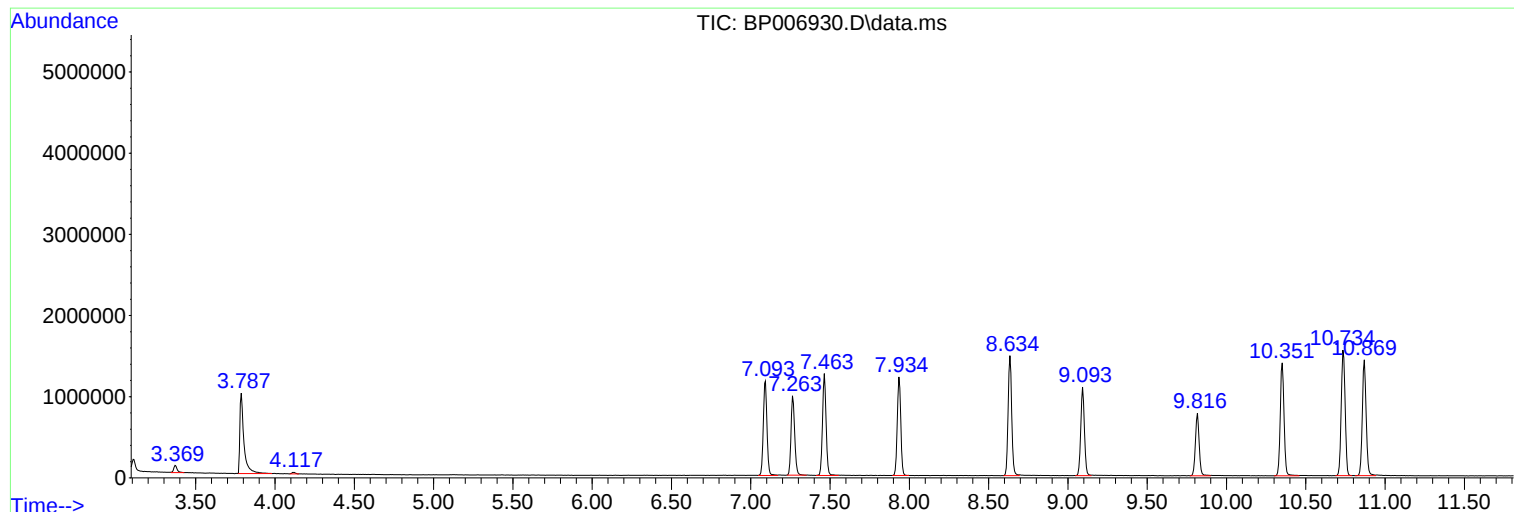

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006930.D
Acq On : 10 Sep 2021 08:55
Operator : CG/JU
Sample : PB138946BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK946

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006930.D
Acq On : 10 Sep 2021 08:55
Operator : CG/JU
Sample : PB138946BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK946

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
