

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006939.D
 Acq On : 10 Sep 2021 14:02
 Operator : CG/JU
 Sample : M3651-11
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBKM5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006939.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	45	49	58	rVB	35009	57134	0.73%	0.084%
2	3.799	119	121	139	rBV	128970	272138	3.48%	0.399%
3	4.028	155	160	166	rVB	26243	44369	0.57%	0.065%
4	4.117	171	175	184	rVB	18234	31935	0.41%	0.047%
5	6.034	496	501	506	rBV5	9857	16567	0.21%	0.024%
6	6.940	646	655	660	rBV6	10788	23785	0.30%	0.035%
7	7.093	674	681	693	rBV	280665	476866	6.10%	0.700%
8	7.269	704	711	722	rBV	957682	1557798	19.93%	2.287%
9	7.464	737	744	754	rBV	978842	1567385	20.05%	2.301%
10	7.569	759	762	766	rVB5	5577	8432	0.11%	0.012%
11	7.934	817	824	832	rBV	968812	1576398	20.16%	2.314%
12	8.005	832	836	841	rVB4	7015	12933	0.17%	0.019%
13	8.175	859	865	871	rBV3	14944	28173	0.36%	0.041%
14	8.487	913	918	922	rBV3	10160	16906	0.22%	0.025%
15	8.634	935	943	956	rBV	760311	1279890	16.37%	1.879%
16	8.834	970	977	979	rBV8	4092	9272	0.12%	0.014%
17	9.093	1009	1021	1033	rBV	1076952	1781317	22.79%	2.615%
18	9.263	1046	1050	1056	rVB9	6004	12179	0.16%	0.018%
19	9.528	1090	1095	1100	rVB7	7321	12272	0.16%	0.018%
20	9.816	1136	1144	1154	rBV	761604	1257434	16.08%	1.846%
21	10.352	1227	1235	1247	rBV	1320518	2163600	27.68%	3.176%
22	10.522	1257	1264	1274	rBV	62870	126131	1.61%	0.185%
23	10.740	1293	1301	1311	rBV	1335779	2235946	28.60%	3.282%
24	10.869	1315	1323	1338	rBV	1275653	2176506	27.84%	3.195%
25	12.322	1559	1570	1575	rBV2	25942	47418	0.61%	0.070%
26	13.181	1712	1716	1722	rBV8	5148	9331	0.12%	0.014%
27	13.398	1749	1753	1758	rVB8	5092	7873	0.10%	0.012%
28	13.534	1770	1776	1779	rBV6	6008	7893	0.10%	0.012%
29	13.969	1842	1850	1867	rBV	2503327	3486006	44.59%	5.117%
30	14.251	1892	1898	1915	rVB	2812468	4218197	53.96%	6.192%
31	14.563	1944	1951	1959	rBV	1992802	2950289	37.74%	4.331%
32	14.745	1975	1982	1999	rBV	168713	322376	4.12%	0.473%
33	14.922	2008	2012	2015	rVB6	4429	7883	0.10%	0.012%
34	15.304	2071	2077	2082	rBV	186660	262734	3.36%	0.386%
35	15.375	2086	2089	2093	rVB3	11237	14911	0.19%	0.022%
36	15.551	2112	2119	2130	rBV	3921092	5588573	71.49%	8.204%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006939.D
 Acq On : 10 Sep 2021 14:02
 Operator : CG/JU
 Sample : M3651-11
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBKM5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

37	15.663	2132	2138	2148	rBV	893025	1240264	15.86%	1.821%
38	15.792	2156	2160	2170	rVB	30927	48574	0.62%	0.071%
39	16.228	2229	2234	2241	rBV10	6711	13198	0.17%	0.019%
40	16.340	2249	2253	2260	rVB9	8580	14037	0.18%	0.021%
41	16.992	2360	2364	2367	rVB6	6041	9050	0.12%	0.013%
42	17.092	2375	2381	2383	rBV3	11856	19055	0.24%	0.028%
43	17.310	2411	2418	2427	rBV	2422518	3388664	43.35%	4.975%
44	17.410	2428	2435	2449	rBV	4735082	6598459	84.40%	9.687%
45	17.851	2506	2510	2513	rBV6	6758	10041	0.13%	0.015%
46	17.981	2529	2532	2537	rBV7	11957	16442	0.21%	0.024%
47	18.092	2549	2551	2556	rVB6	8609	10513	0.13%	0.015%
48	18.192	2564	2568	2576	rBV	116239	167983	2.15%	0.247%
49	19.216	2738	2742	2748	rBV2	44666	65266	0.83%	0.096%
50	19.286	2750	2754	2758	rVV	51010	69900	0.89%	0.103%
51	19.422	2774	2777	2781	rBV4	42758	55930	0.72%	0.082%
52	19.639	2808	2814	2827	rBV	5960282	7817742	100.00%	11.476%
53	21.098	3059	3062	3066	rBV2	155670	178654	2.29%	0.262%
54	21.386	3107	3111	3122	rVB	2680990	3570593	45.67%	5.242%
55	23.669	3492	3499	3507	rBV2	3764883	7432082	95.07%	10.910%
56	23.827	3519	3526	3538	rVB2	1767319	3724583	47.64%	5.468%




Sum of corrected areas: 68119880

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006939.D
Acq On : 10 Sep 2021 14:02
Operator : CG/JU
Sample : M3651-11
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKM5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

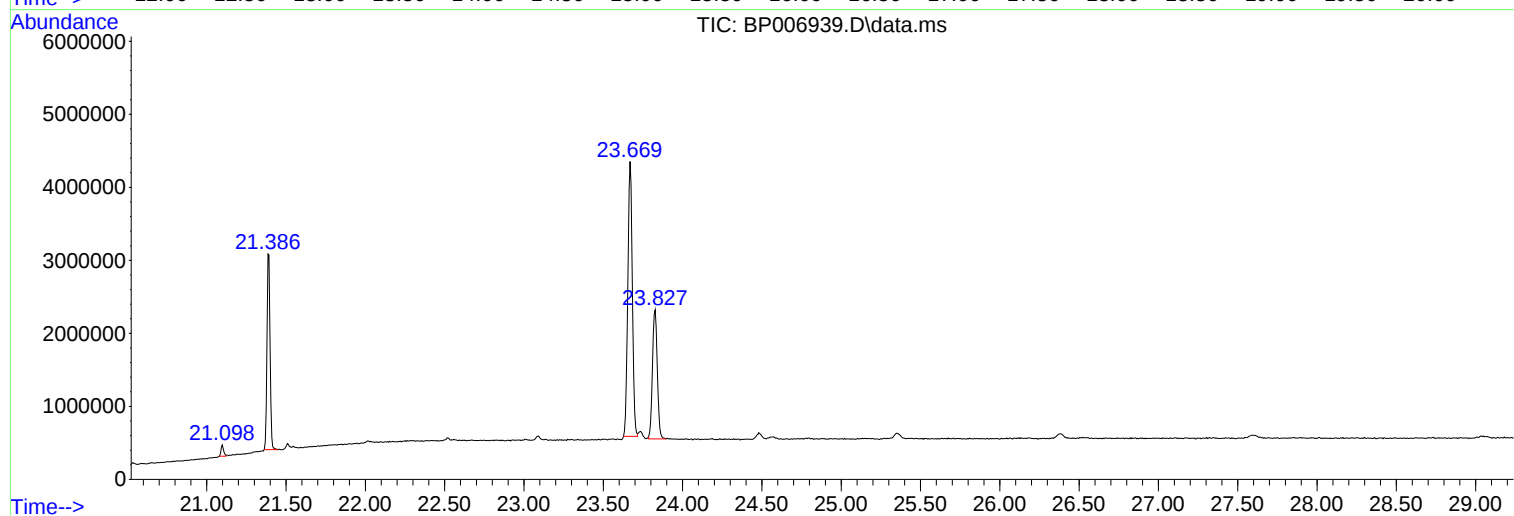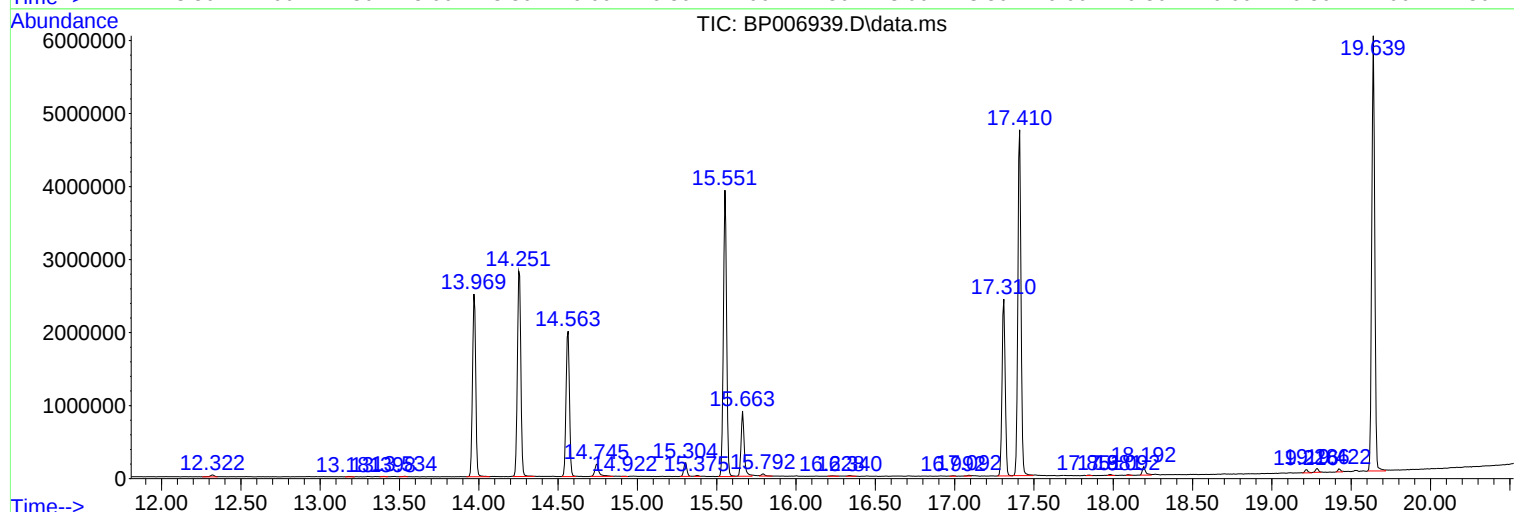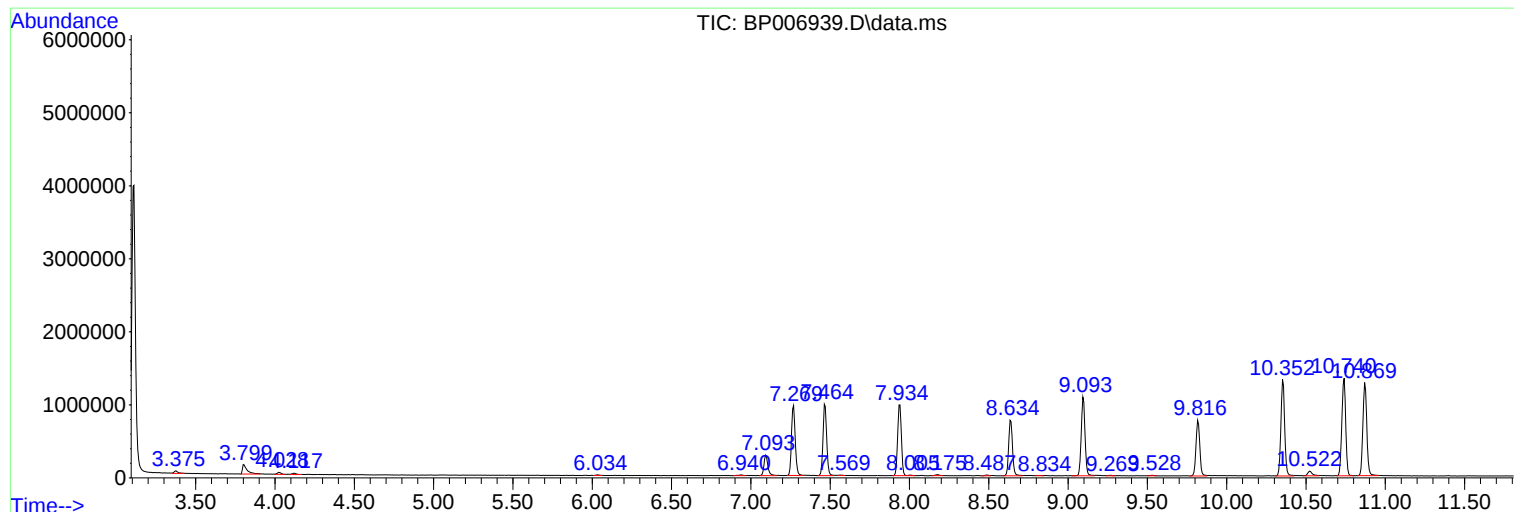

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006939.D
Acq On : 10 Sep 2021 14:02
Operator : CG/JU
Sample : M3651-11
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKM5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006939.D
Acq On : 10 Sep 2021 14:02
Operator : CG/JU
Sample : M3651-11
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKM5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
