

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006948.D
 Acq On : 10 Sep 2021 19:11
 Operator : CG/JU
 Sample : M3608-02DL2 100X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBKJ8DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006948.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.116	170	175	180	rVB	44995	65307	1.43%	0.187%
2	5.446	395	401	406	rBV	119668	173226	3.80%	0.496%
3	5.575	418	423	432	rVB	31038	62963	1.38%	0.180%
4	5.946	477	486	491	rBV	22620	40847	0.89%	0.117%
5	7.022	665	669	674	rBV3	10765	17254	0.38%	0.049%
6	7.087	676	680	686	rVV6	9942	21519	0.47%	0.062%
7	7.163	688	693	697	rVB4	10096	17490	0.38%	0.050%
8	7.269	707	711	717	rBV2	10999	17110	0.37%	0.049%
9	7.457	739	743	748	rBV6	7879	15906	0.35%	0.046%
10	7.587	759	765	772	rVV2	30555	49846	1.09%	0.143%
11	7.657	772	777	785	rVB	48500	81103	1.78%	0.232%
12	7.934	816	824	838	rBV	1216049	1959671	42.94%	5.614%
13	8.051	840	844	848	rVB	13911	19210	0.42%	0.055%
14	8.310	881	888	895	rBV	583180	922318	20.21%	2.642%
15	8.375	895	899	905	rVB4	21088	35965	0.79%	0.103%
16	8.475	910	916	926	rVB	141297	240251	5.26%	0.688%
17	8.704	950	955	961	rBV2	16401	27921	0.61%	0.080%
18	8.781	963	968	976	rVB2	14148	25896	0.57%	0.074%
19	9.298	1050	1056	1061	rBV4	11578	20574	0.45%	0.059%
20	9.357	1061	1066	1070	rBV4	16106	29394	0.64%	0.084%
21	9.416	1070	1076	1082	rVV	30431	65513	1.44%	0.188%
22	9.481	1082	1087	1091	rVB3	12258	20404	0.45%	0.058%
23	9.904	1152	1159	1163	rBV	47031	84428	1.85%	0.242%
24	9.992	1169	1174	1184	rVB2	19360	40402	0.89%	0.116%
25	10.139	1184	1199	1207	rBV5	33549	110031	2.41%	0.315%
26	10.210	1207	1211	1220	rVB	35132	59833	1.31%	0.171%
27	10.369	1230	1238	1244	rBV	83679	154436	3.38%	0.442%
28	10.592	1267	1276	1292	rBV3	52579	160337	3.51%	0.459%
29	10.734	1292	1300	1304	rVV	1651835	2771774	60.73%	7.940%
30	10.787	1304	1309	1320	rVV	2313919	3844085	84.23%	11.012%
31	10.904	1320	1329	1339	rVB	123029	254190	5.57%	0.728%
32	11.104	1357	1363	1368	rVB6	7763	14721	0.32%	0.042%
33	11.269	1386	1391	1396	rBV	11214	18998	0.42%	0.054%
34	11.563	1436	1441	1447	rBV2	22298	37881	0.83%	0.109%
35	11.757	1468	1474	1479	rBV5	10432	20353	0.45%	0.058%
36	11.810	1479	1483	1487	rVV3	13374	26071	0.57%	0.075%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006948.D
 Acq On : 10 Sep 2021 19:11
 Operator : CG/JU
 Sample : M3608-02DL2 100X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBKJ8DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

37	11.845	1487	1489	1495	rVV7	10730	18904	0.41%	0.054%
38	11.934	1498	1504	1513	rVB7	7564	17624	0.39%	0.050%
39	12.122	1531	1536	1542	rVB3	14452	28837	0.63%	0.083%
40	12.286	1558	1564	1569	rBV3	18649	30565	0.67%	0.088%

41	12.392	1575	1582	1590	rBV	544708	868277	19.02%	2.487%
42	12.516	1593	1603	1609	rVV2	61231	126384	2.77%	0.362%
43	12.610	1609	1619	1628	rVB	309057	529352	11.60%	1.516%
44	12.763	1640	1645	1651	rBV5	11540	26075	0.57%	0.075%
45	12.975	1678	1681	1686	rVB4	10719	13599	0.30%	0.039%

46	13.063	1686	1696	1702	rBV9	17909	48043	1.05%	0.138%
47	13.257	1722	1729	1733	rBV	59800	100940	2.21%	0.289%
48	13.398	1746	1753	1762	rVB	99308	167588	3.67%	0.480%
49	13.563	1776	1781	1794	rVB2	51892	133067	2.92%	0.381%
50	13.739	1800	1811	1817	rBV7	31119	91244	2.00%	0.261%

51	13.828	1819	1826	1829	rBV9	7126	14044	0.31%	0.040%
52	13.880	1829	1835	1840	rVV2	44466	80907	1.77%	0.232%
53	13.933	1840	1844	1847	rVV	21869	32761	0.72%	0.094%
54	13.969	1847	1850	1855	rVB	27264	39578	0.87%	0.113%
55	14.116	1866	1875	1880	rBV5	17025	33826	0.74%	0.097%

56	14.251	1890	1898	1900	rBV	27202	48196	1.06%	0.138%
57	14.275	1900	1902	1909	rVB2	33493	49928	1.09%	0.143%
58	14.363	1909	1917	1924	rBV2	8594	19776	0.43%	0.057%
59	14.557	1942	1950	1956	rBV	2450083	3594080	78.75%	10.296%
60	14.622	1956	1961	1967	rVV	460834	672114	14.73%	1.925%

61	14.686	1967	1972	1977	rVV	93669	139498	3.06%	0.400%
62	14.733	1977	1980	1986	rVB3	17584	27177	0.60%	0.078%
63	14.827	1992	1996	2006	rBV3	32812	61395	1.35%	0.176%
64	14.957	2012	2018	2025	rVB2	196043	319127	6.99%	0.914%
65	15.275	2068	2072	2077	rVB5	12069	17513	0.38%	0.050%

66	15.551	2108	2119	2123	rBV	45276	79738	1.75%	0.228%
67	15.604	2123	2128	2134	rVV2	163482	235593	5.16%	0.675%
68	15.669	2134	2139	2146	rVV	207676	329902	7.23%	0.945%
69	15.733	2146	2150	2158	rVV4	45193	117882	2.58%	0.338%
70	15.827	2161	2166	2173	rVV8	23893	69019	1.51%	0.198%

71	15.898	2174	2178	2186	rVV7	14703	30840	0.68%	0.088%
72	15.980	2186	2192	2196	rVV6	10125	23169	0.51%	0.066%
73	16.039	2200	2202	2209	rVV4	11338	20168	0.44%	0.058%
74	16.274	2234	2242	2251	rBV4	27563	61022	1.34%	0.175%
75	16.398	2257	2263	2269	rBV9	14885	31424	0.69%	0.090%

76	16.486	2271	2278	2286	rVV2	29274	68320	1.50%	0.196%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006948.D
 Acq On : 10 Sep 2021 19:11
 Operator : CG/JU
 Sample : M3608-02DL2 100X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBKJ8DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

77	16.557	2286	2290	2296	rVV	31661	52827	1.16%	0.151%
78	16.604	2296	2298	2302	rVV5	10361	15678	0.34%	0.045%
79	16.657	2305	2307	2313	rVB6	10893	14071	0.31%	0.040%
80	16.774	2322	2327	2330	rBV6	14115	25014	0.55%	0.072%
81	17.086	2374	2380	2384	rBV3	39741	64809	1.42%	0.186%
82	17.127	2384	2387	2392	rVB	13883	19949	0.44%	0.057%
83	17.216	2394	2402	2406	rBV6	11907	28557	0.63%	0.082%
84	17.304	2411	2417	2422	rVV	2960149	4218325	92.43%	12.084%
85	17.345	2422	2424	2430	rVV	167741	237573	5.21%	0.681%
86	17.404	2430	2434	2438	rVB2	45223	64872	1.42%	0.186%
87	17.504	2446	2451	2456	rVB9	10159	18338	0.40%	0.053%
88	17.668	2475	2479	2481	rBV3	23801	33872	0.74%	0.097%
89	17.710	2481	2486	2493	rVV	428429	599992	13.15%	1.719%
90	17.798	2496	2501	2508	rBV3	39608	84017	1.84%	0.241%
91	17.863	2508	2512	2518	rVB	48599	68259	1.50%	0.196%
92	18.127	2554	2557	2563	rBV	22572	30289	0.66%	0.087%
93	18.216	2566	2572	2578	rVV2	49528	91160	2.00%	0.261%
94	18.286	2580	2584	2589	rVB	31520	45028	0.99%	0.129%
95	18.439	2607	2610	2613	rBV4	9567	15483	0.34%	0.044%
96	18.592	2633	2636	2641	rVB6	14237	20577	0.45%	0.059%
97	19.633	2809	2813	2817	rBV2	58391	85030	1.86%	0.244%
98	20.080	2886	2889	2894	rBV2	31658	52885	1.16%	0.151%
99	21.386	3106	3111	3120	rVB	3585801	4563961	100.00%	13.074%
100	23.821	3518	3525	3538	rVB2	2213797	4513058	98.88%	12.928%




Sum of corrected areas: 34908348

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP006948\
Data File : BP006948.D
Acq On : 10 Sep 2021 19:11
Operator : CG/JU
Sample : M3608-02DL2 100X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKJ8DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP006948.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

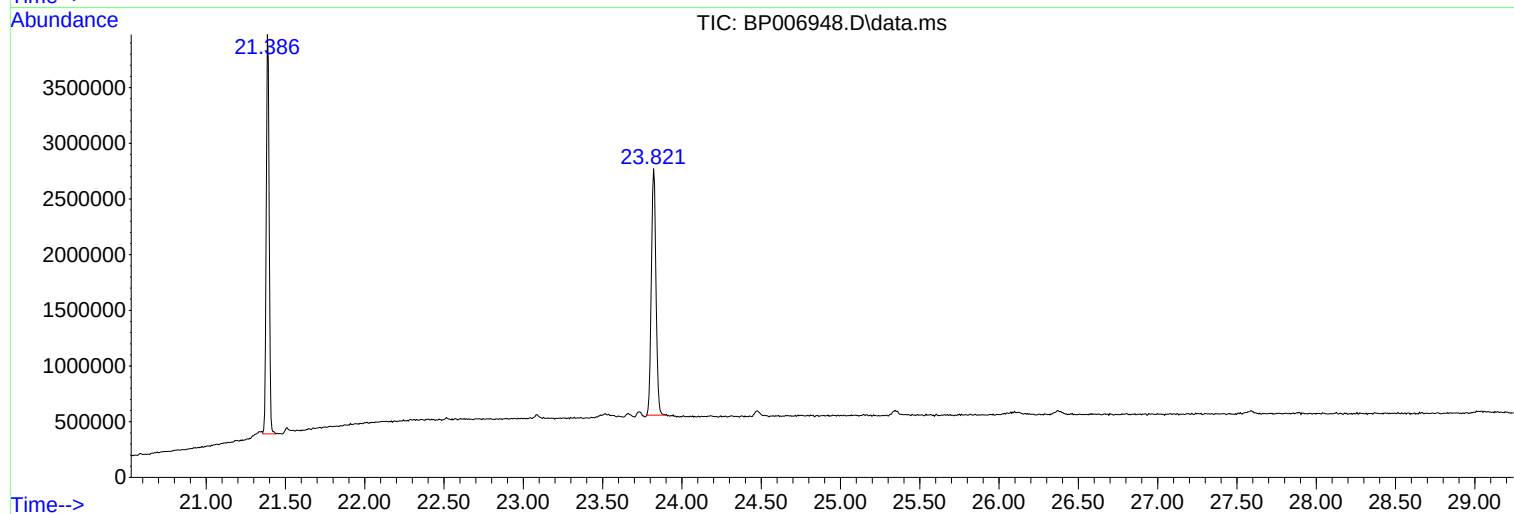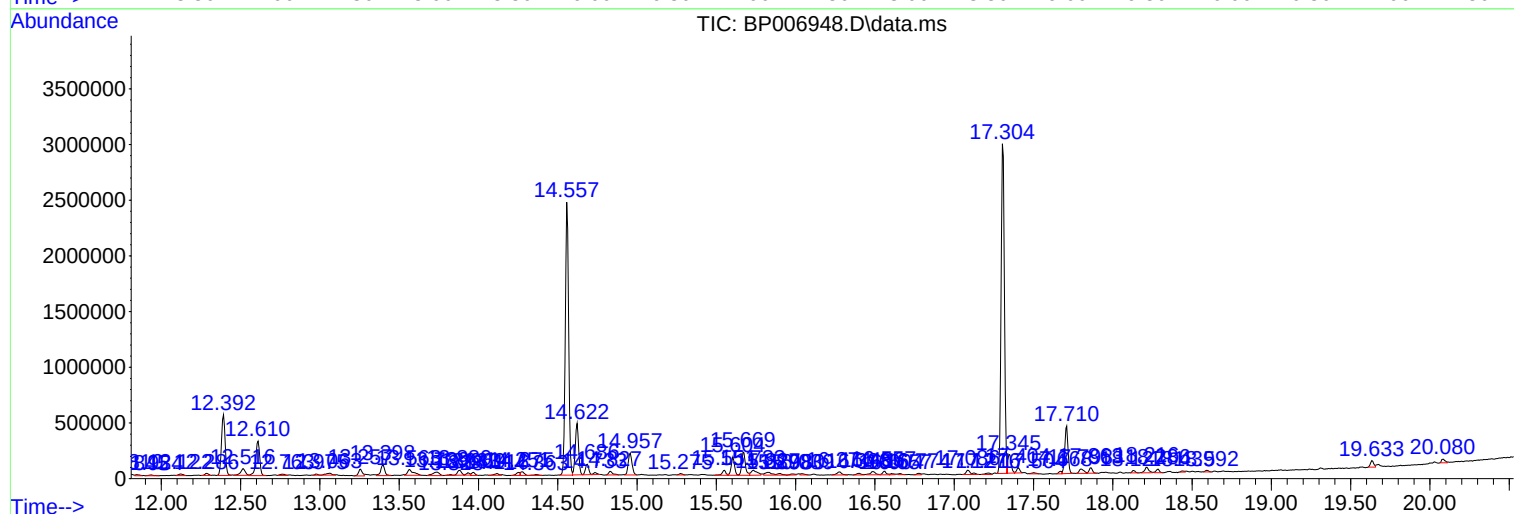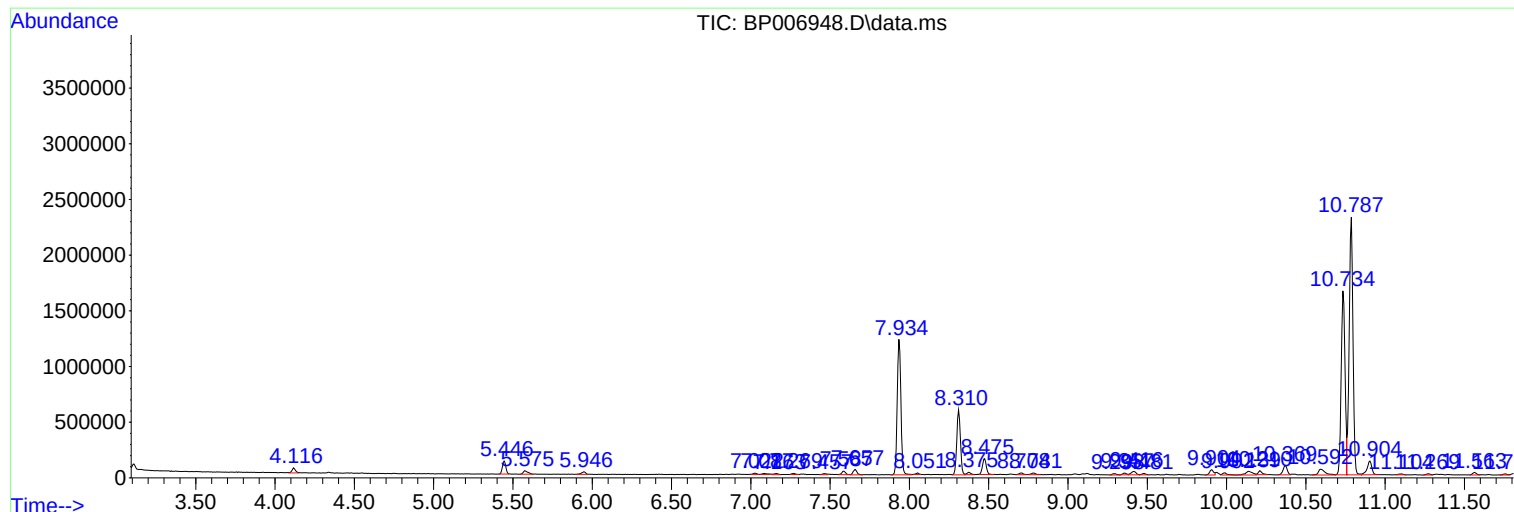

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006948.D
Acq On : 10 Sep 2021 19:11
Operator : CG/JU
Sample : M3608-02DL2 100X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKJ8DL2










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Indane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.310	9.41 ng/ul	922318	1,4-Dichlorobenzene-d4	7.934

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Indane			118	C9H10	000496-11-7	93
2	Indane			118	C9H10	000496-11-7	90
3	Indane			118	C9H10	000496-11-7	83
4	Deltacyclene			118	C9H10	007785-10-6	72
5	Benzene, cyclopropyl-			118	C9H10	000873-49-4	64

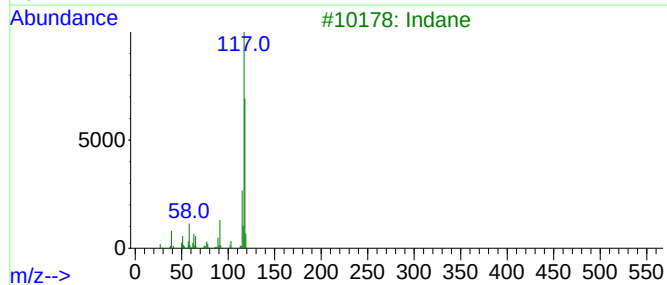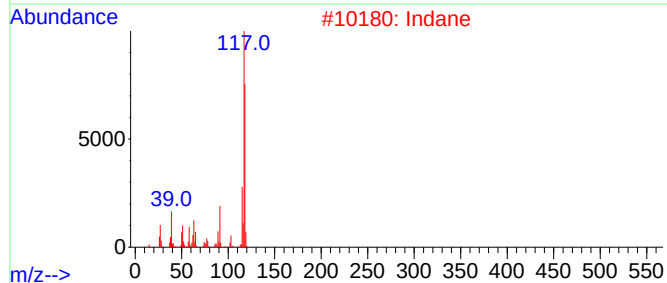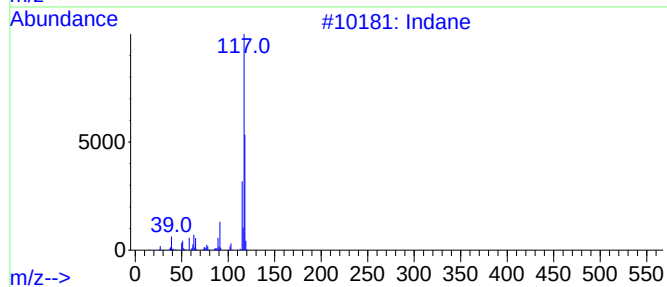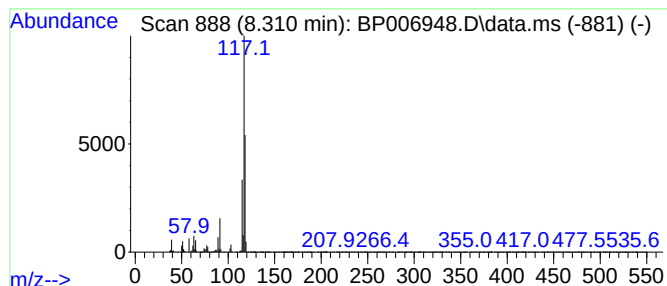

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006948.D
Acq On : 10 Sep 2021 19:11
Operator : CG/JU
Sample : M3608-02DL2 100X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKJ8DL2










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Benzene, 1-propynyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.475	2.45 ng/ul	240251	1,4-Dichlorobenzene-d4	7.934

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1-propynyl-	116	C9H8	000673-32-5	94
2			Indene	116	C9H8	000095-13-6	93
3			3-Methylphenylacetylene	116	C9H8	000766-82-5	91
4			Benzene, 1-propynyl-	116	C9H8	000673-32-5	91
5			Benzene, 1,2-propadienyl-	116	C9H8	002327-99-3	91

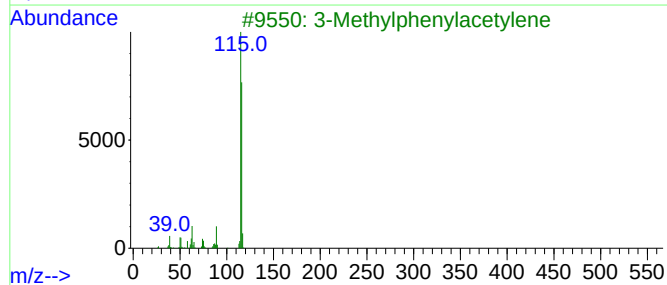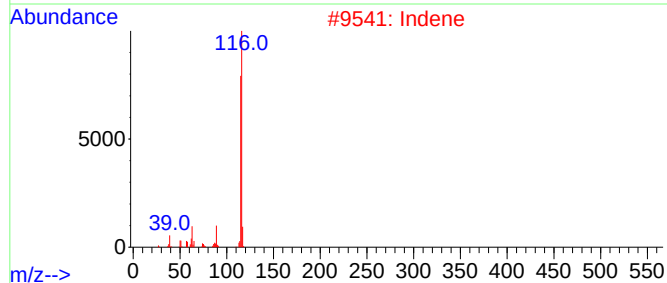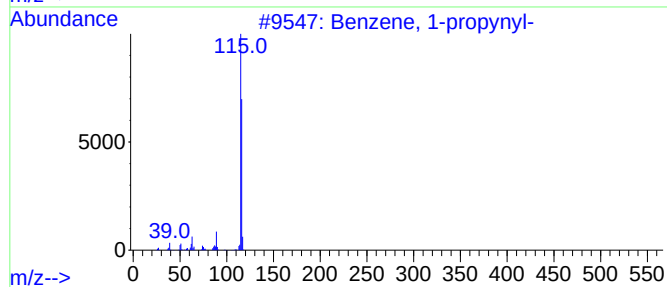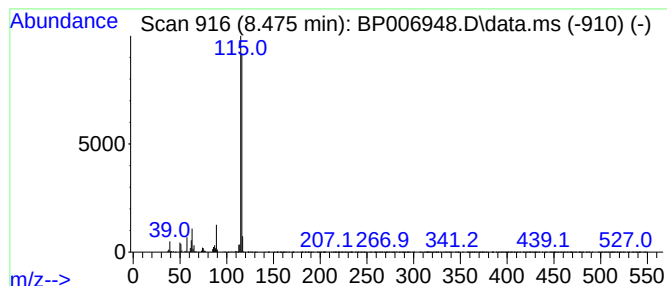

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006948.D
Acq On : 10 Sep 2021 19:11
Operator : CG/JU
Sample : M3608-02DL2 100X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKJ8DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Indane	8.310	9.4	ng/u1	922318	1	7.934	1959670	20.0
Benzene, 1-prop...	8.475	2.5	ng/u1	240251	1	7.934	1959670	20.0