

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006953.D
 Acq On : 10 Sep 2021 22:01
 Operator : CG/JU
 Sample : M3651-07
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBKM3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006953.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	45	49	58	rVB	37701	60496	0.66%	0.077%
2	3.799	118	121	139	rBV	210886	418466	4.59%	0.532%
3	4.028	155	160	168	rVB	29715	50146	0.55%	0.064%
4	4.117	171	175	182	rVB	19927	33408	0.37%	0.042%
5	6.934	650	654	660	rVB3	9722	15337	0.17%	0.019%
6	7.093	674	681	691	rBV	323933	544206	5.96%	0.692%
7	7.263	703	710	726	rBV	1093864	1740590	19.07%	2.212%
8	7.463	737	744	757	rBV	1135371	1765732	19.35%	2.244%
9	7.558	758	760	769	rVB8	6964	13406	0.15%	0.017%
10	7.934	814	824	832	rBV	1199663	1888765	20.70%	2.400%
11	8.069	844	847	852	rVB2	6897	10134	0.11%	0.013%
12	8.175	859	865	870	rBV3	15495	26957	0.30%	0.034%
13	8.481	913	917	928	rVB3	11652	25859	0.28%	0.033%
14	8.634	933	943	954	rBV	918862	1457128	15.97%	1.852%
15	9.093	1013	1021	1034	rBV	1193998	1951868	21.39%	2.481%
16	9.257	1046	1049	1055	rVB8	5910	9190	0.10%	0.012%
17	9.528	1090	1095	1100	rVB8	6000	10184	0.11%	0.013%
18	9.816	1136	1144	1158	rBV	823877	1377630	15.10%	1.751%
19	10.352	1226	1235	1248	rBV	1443690	2407079	26.38%	3.059%
20	10.528	1258	1265	1272	rBV3	17594	39616	0.43%	0.050%
21	10.734	1292	1300	1313	rBV	1642394	2676185	29.33%	3.401%
22	10.869	1314	1323	1338	rBV	1317096	2301642	25.22%	2.925%
23	11.387	1404	1411	1419	rVB8	5074	12653	0.14%	0.016%
24	12.316	1563	1569	1577	rVB2	27245	47953	0.53%	0.061%
25	13.534	1770	1776	1781	rVB8	7495	12035	0.13%	0.015%
26	13.969	1842	1850	1861	rBV	2855848	3853896	42.23%	4.898%
27	14.251	1886	1898	1909	rBV	3216180	4669108	51.16%	5.934%
28	14.557	1943	1950	1962	rBV	2481718	3529267	38.67%	4.485%
29	14.740	1975	1981	1999	rBV	222509	404159	4.43%	0.514%
30	14.969	2017	2020	2024	rVB6	6483	9468	0.10%	0.012%
31	15.298	2070	2076	2083	rBV	110809	155230	1.70%	0.197%
32	15.357	2083	2086	2092	rVB7	5035	9736	0.11%	0.012%
33	15.551	2109	2119	2131	rBV	4227045	6340181	69.47%	8.057%
34	15.663	2131	2138	2152	rVV	1045994	1531825	16.79%	1.947%
35	15.787	2155	2159	2168	rVB2	32461	63042	0.69%	0.080%
36	16.216	2226	2232	2239	rBV2	9479	24434	0.27%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006953.D
 Acq On : 10 Sep 2021 22:01
 Operator : CG/JU
 Sample : M3651-07
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBKM3

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

37	16.339	2248	2253	2259	rVB8	11804	21131	0.23%	0.027%
38	16.981	2358	2362	2367	rBV8	6503	12901	0.14%	0.016%
39	17.092	2376	2381	2383	rBV	12117	17944	0.20%	0.023%
40	17.304	2411	2417	2427	rBV	2920690	4083353	44.74%	5.189%
41	17.404	2427	2434	2447	rBV	5361653	7675426	84.11%	9.754%
42	17.969	2528	2530	2537	rVB8	11782	17200	0.19%	0.022%
43	18.186	2563	2567	2576	rBV2	89969	137197	1.50%	0.174%
44	19.210	2737	2741	2746	rBV	48844	72513	0.79%	0.092%
45	19.280	2749	2753	2759	rBV	70576	105324	1.15%	0.134%
46	19.416	2773	2776	2781	rBV5	35679	51483	0.56%	0.065%
47	19.633	2807	2813	2819	rBV	6992549	9125907	100.00%	11.598%
48	21.092	3058	3061	3067	rBV	159879	207694	2.28%	0.264%
49	21.386	3106	3111	3121	rVB	3376031	4325261	47.40%	5.497%
50	23.663	3490	3498	3506	rBV2	4540152	8903868	97.57%	11.316%
51	23.816	3517	3524	3535	rVB2	2130720	4442965	48.69%	5.646%


Sum of corrected areas: 78687178

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006953.D
Acq On : 10 Sep 2021 22:01
Operator : CG/JU
Sample : M3651-07
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKM3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

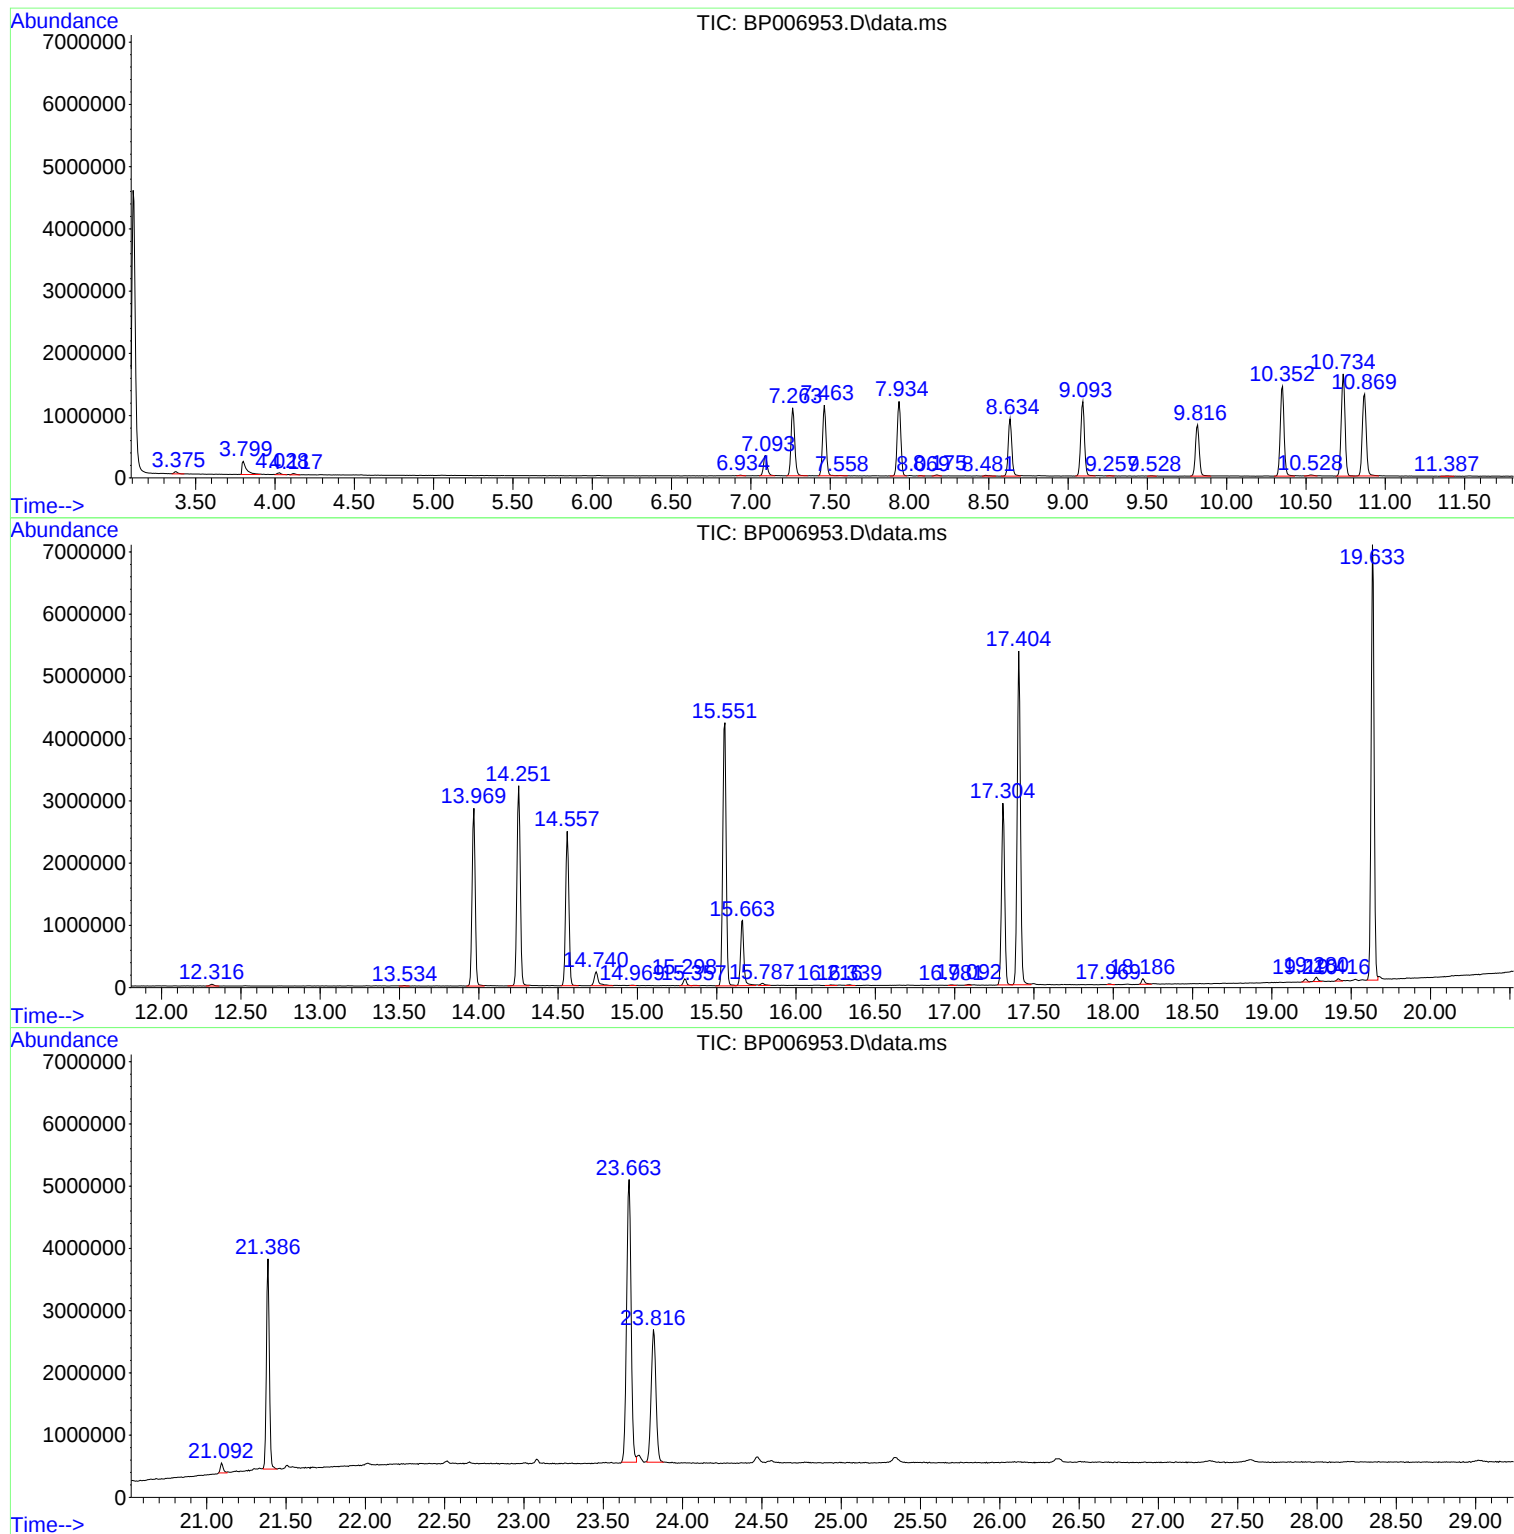

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006953.D
Acq On : 10 Sep 2021 22:01
Operator : CG/JU
Sample : M3651-07
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKM3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006953.D
Acq On : 10 Sep 2021 22:01
Operator : CG/JU
Sample : M3651-07
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKM3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
