

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006958.D
 Acq On : 11 Sep 2021 00:52
 Operator : CG/JU
 Sample : M3651-15
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBKM9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006958.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	44	48	55	rVB	32876	46787	0.52%	0.061%
2	3.793	118	120	138	rBV	219499	405785	4.51%	0.529%
3	4.023	155	159	166	rVB	24744	40248	0.45%	0.053%
4	4.117	171	175	179	rVB	19544	25898	0.29%	0.034%
5	4.646	261	265	271	rBV9	8219	15647	0.17%	0.020%
6	6.934	650	654	658	rVB	7542	12219	0.14%	0.016%
7	7.087	672	680	691	rBV	278935	471857	5.24%	0.615%
8	7.264	703	710	725	rBV	1019130	1627317	18.07%	2.123%
9	7.464	736	744	756	rBV	1030375	1620462	18.00%	2.114%
10	7.934	816	824	832	rBV	1116687	1799197	19.98%	2.347%
11	7.999	833	835	842	rVV6	8079	13418	0.15%	0.018%
12	8.069	842	847	854	rVB10	6471	13984	0.16%	0.018%
13	8.169	859	864	870	rBV4	13221	25379	0.28%	0.033%
14	8.481	913	917	921	rBV4	8879	14096	0.16%	0.018%
15	8.634	935	943	951	rBV	795913	1287076	14.30%	1.679%
16	9.093	1013	1021	1031	rBV	1103982	1862258	20.68%	2.429%
17	9.258	1046	1049	1056	rVB9	6955	11659	0.13%	0.015%
18	9.522	1090	1094	1102	rVB6	8415	16130	0.18%	0.021%
19	9.816	1136	1144	1156	rBV	781500	1303786	14.48%	1.701%
20	10.346	1226	1234	1247	rBV	1340155	2244569	24.93%	2.928%
21	10.540	1261	1267	1272	rBV6	11094	20351	0.23%	0.027%
22	10.734	1292	1300	1308	rBV	1583608	2570959	28.56%	3.354%
23	10.863	1314	1322	1337	rBV	1174429	2090529	23.22%	2.727%
24	11.399	1406	1413	1416	rBV8	5486	10638	0.12%	0.014%
25	12.316	1563	1569	1576	rBV	29073	46696	0.52%	0.061%
26	13.352	1739	1745	1750	rBV10	4055	9798	0.11%	0.013%
27	13.969	1843	1850	1861	rBV	2709136	3762487	41.79%	4.908%
28	14.251	1891	1898	1913	rVB	3175266	4576679	50.83%	5.970%
29	14.557	1942	1950	1958	rBV	2394287	3461857	38.45%	4.516%
30	14.740	1973	1981	1994	rBV	172306	336053	3.73%	0.438%
31	14.957	2015	2018	2023	rVB6	5786	10316	0.11%	0.013%
32	15.298	2070	2076	2080	rBV	16158	21668	0.24%	0.028%
33	15.546	2111	2118	2131	rBV	4341573	6119398	67.97%	7.982%
34	15.657	2131	2137	2153	rVV	998029	1419189	15.76%	1.851%
35	15.787	2155	2159	2169	rVB3	31300	59072	0.66%	0.077%
36	16.334	2248	2252	2257	rVB8	11505	19252	0.21%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
 Data File : BP006958.D
 Acq On : 11 Sep 2021 00:52
 Operator : CG/JU
 Sample : M3651-15
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBKM9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

37	16.704	2313	2315	2321	rVB7	6416	10111	0.11%	0.013%
38	16.910	2344	2350	2355	rBV9	5625	9108	0.10%	0.012%
39	16.981	2360	2362	2367	rVB5	7496	9841	0.11%	0.013%
40	17.093	2374	2381	2384	rBV2	13327	28329	0.31%	0.037%
41	17.234	2400	2405	2409	rBV8	5340	11277	0.13%	0.015%
42	17.304	2410	2417	2424	rBV	2993025	4139833	45.98%	5.400%
43	17.404	2427	2434	2446	rBV	5064870	7170473	79.64%	9.353%
44	17.975	2527	2531	2537	rVB7	16801	21779	0.24%	0.028%
45	18.087	2548	2550	2558	rVB9	10168	14184	0.16%	0.019%
46	18.187	2562	2567	2575	rBV3	89368	149752	1.66%	0.195%
47	19.210	2737	2741	2747	rBV3	50066	80435	0.89%	0.105%
48	19.275	2749	2752	2763	rVV	75700	125345	1.39%	0.164%
49	19.416	2773	2776	2781	rBV2	35307	48435	0.54%	0.063%
50	19.634	2807	2813	2818	rBV	6760556	8785138	97.58%	11.460%
51	19.675	2818	2820	2824	rVB4	65060	78476	0.87%	0.102%
52	21.092	3058	3061	3067	rBV2	162602	177782	1.97%	0.232%
53	21.381	3106	3110	3123	rVB	3608710	4631080	51.44%	6.041%
54	23.657	3489	3497	3505	rBV2	4379984	9003275	100.00%	11.744%
55	23.816	3517	3524	3535	rVB2	2344001	4775103	53.04%	6.229%




Sum of corrected areas: 76662470

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006958.D
Acq On : 11 Sep 2021 00:52
Operator : CG/JU
Sample : M3651-15
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKM9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

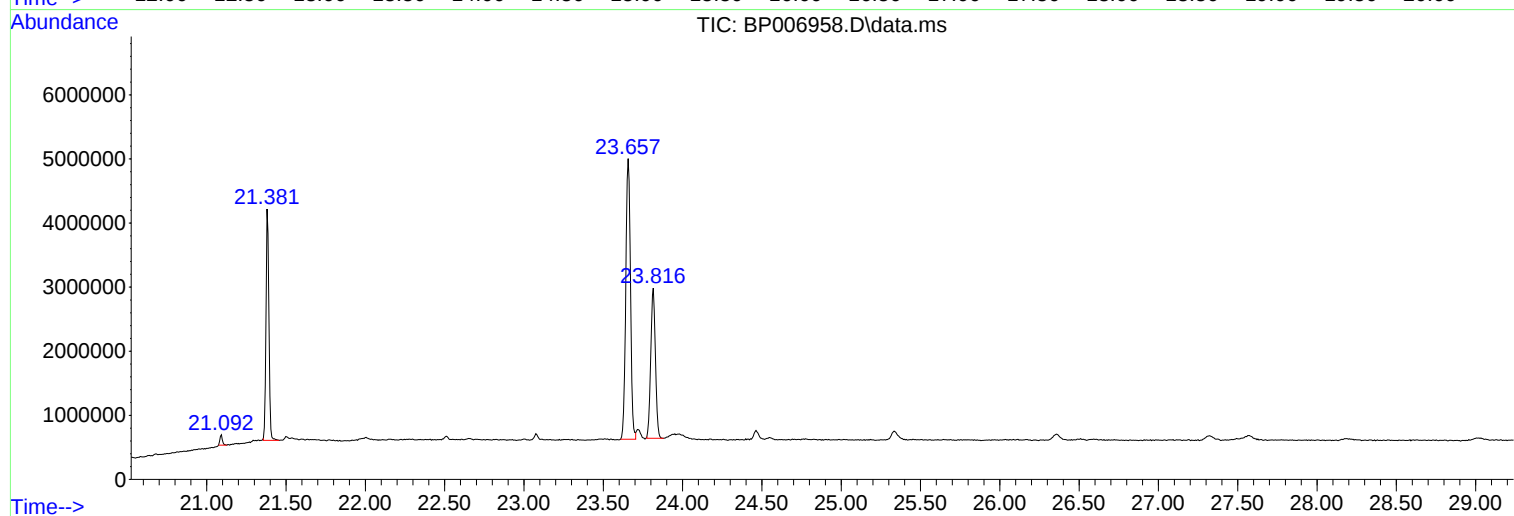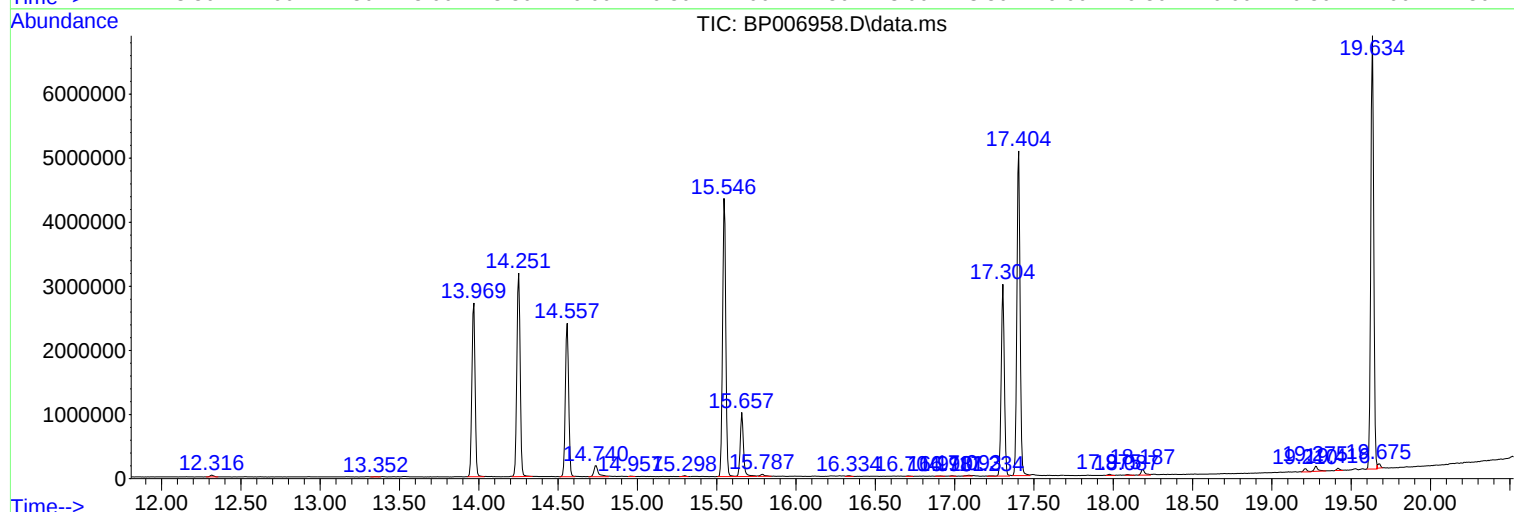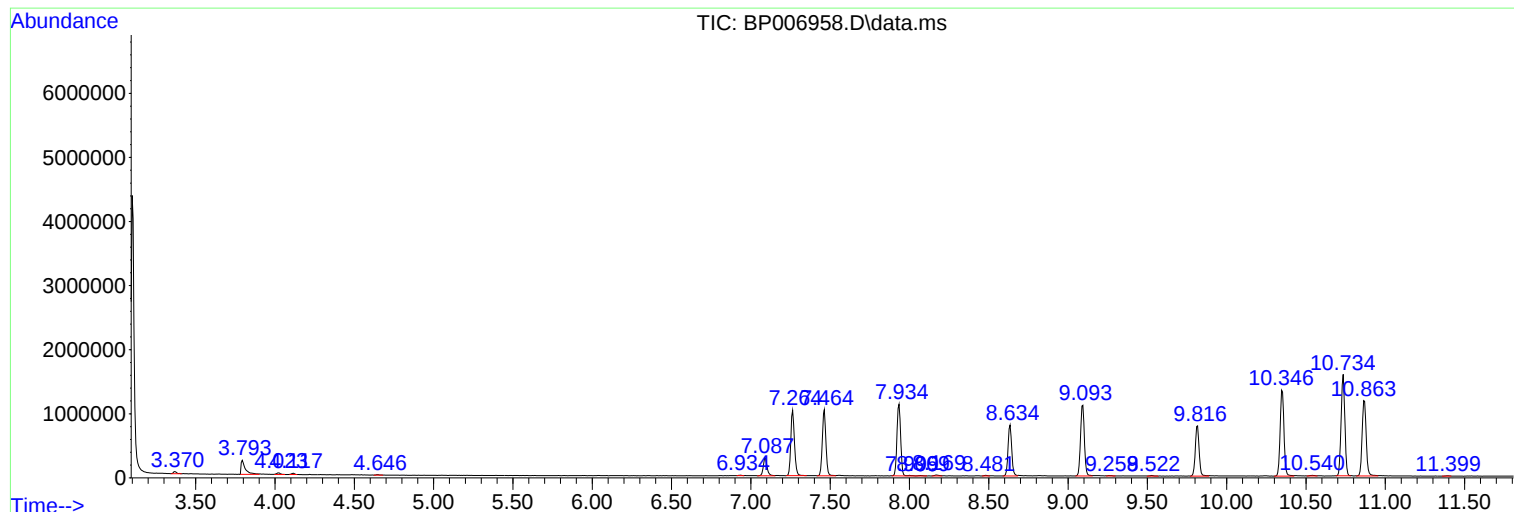

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006958.D
Acq On : 11 Sep 2021 00:52
Operator : CG/JU
Sample : M3651-15
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKM9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090921\
Data File : BP006958.D
Acq On : 11 Sep 2021 00:52
Operator : CG/JU
Sample : M3651-15
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBKM9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
