
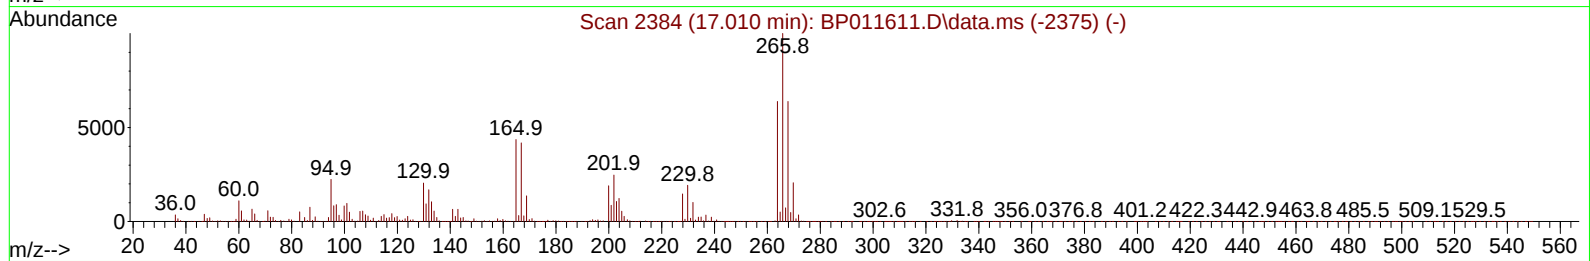
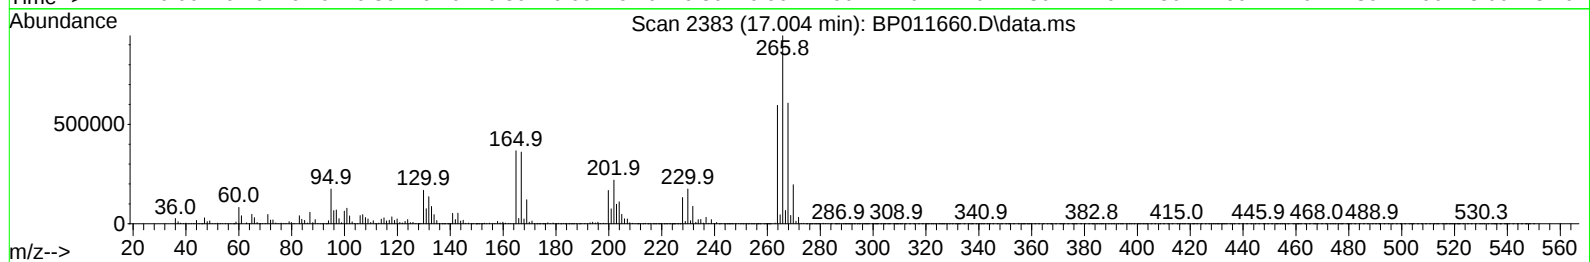


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090922\
Data File : BP011660.D
Acq On : 09 Sep 2022 11:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 04:56:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 10 00:48:09 2022
Response via : Initial Calibration

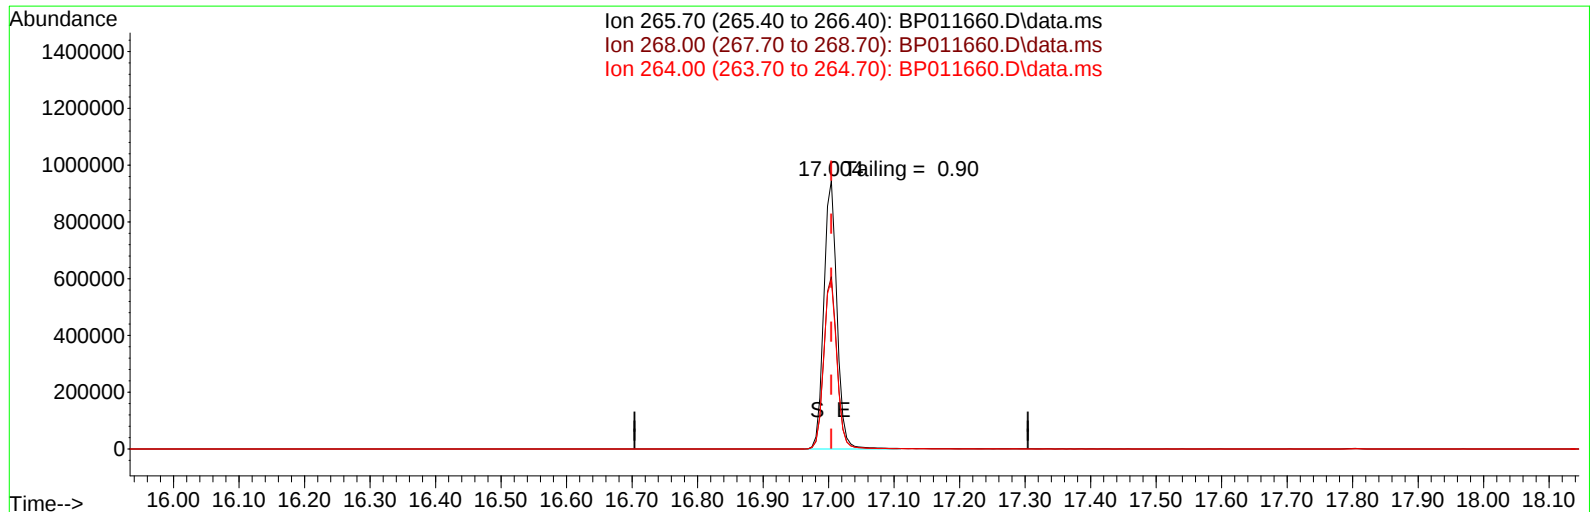

TIC: BP011660.D\data.ms

(70) Pentachlorophenol (C)




17.004min (-0.000) 1022382.80 ng

response 1325818

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.16
264.00	63.00	63.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090922\
 Data File : BP011660.D
 Acq On : 09 Sep 2022 11:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 04:56:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 10 00:48:09 2022
 Response via : Initial Calibration

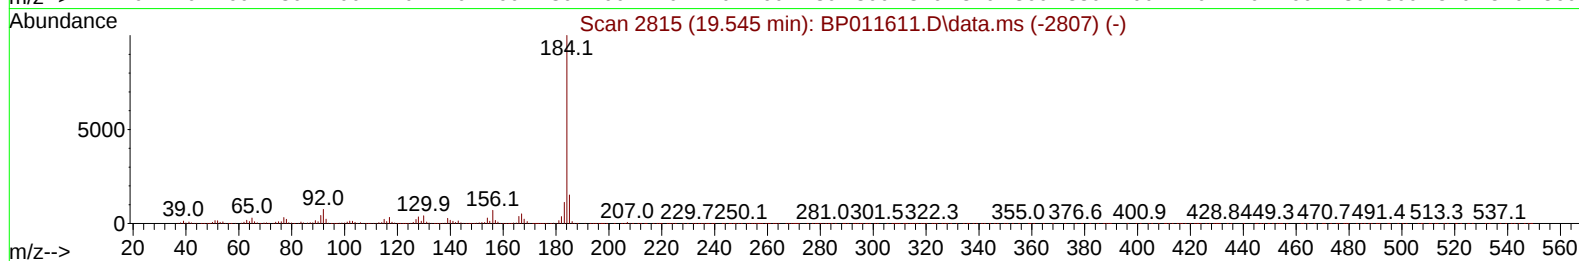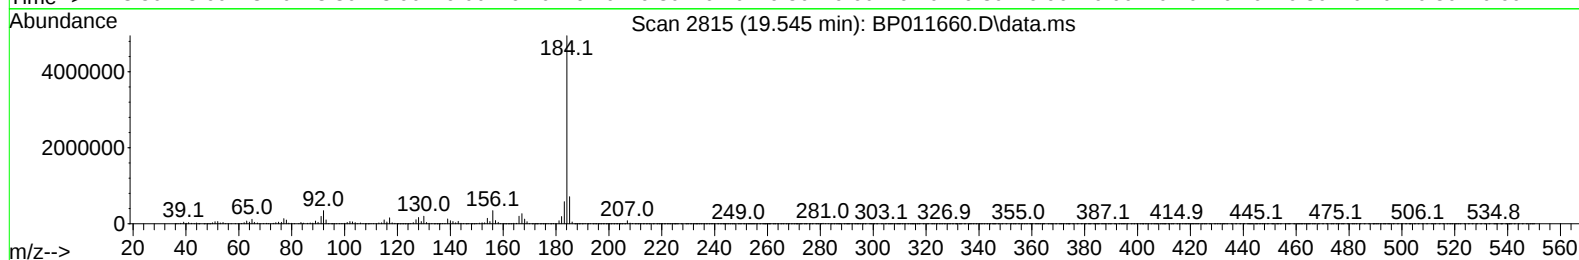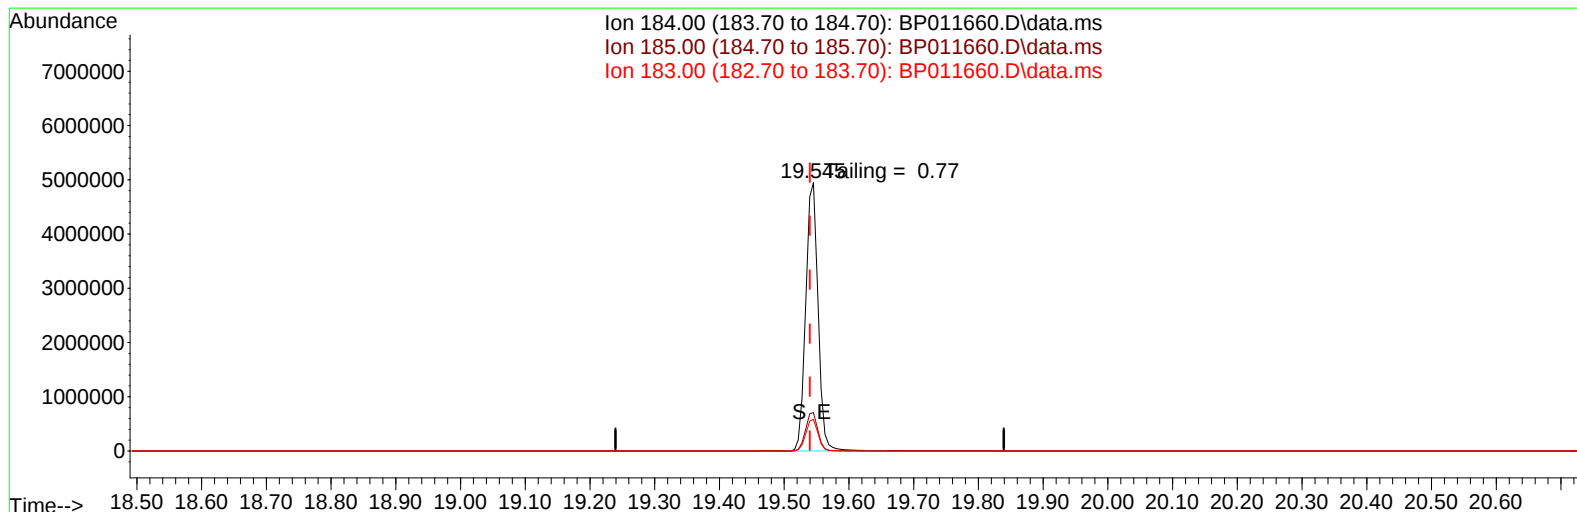

TIC: BP011660.D\data.ms

(77) Benzidine**19.545min (+ 0.006) 302473.39 ng****response 6614037**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.35
183.00	11.30	11.74
0.00	0.00	0.00