

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090922\
 Data File : BP011669.D
 Acq On : 09 Sep 2022 18:31
 Operator : CG/JU
 Sample : N4549-13
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 MW-57

Quant Time: Sep 10 00:55:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 10 00:48:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	413251	20.000	ng	0.00
21) Naphthalene-d8	10.775	136	1645432	20.000	ng	# 0.00
39) Acenaphthene-d10	14.598	164	978096	20.000	ng	0.00
64) Phenanthrene-d10	17.357	188	2047101	20.000	ng	0.00
76) Chrysene-d12	21.433	240	2030492	20.000	ng	0.00
86) Perylene-d12	23.904	264	2237676	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.516	112	1818946	77.846	ng	0.00
7) Phenol-d6	7.111	99	1422006	45.993	ng	0.00
23) Nitrobenzene-d5	9.128	82	2597085	96.886	ng	0.00
42) 2,4,6-Tribromophenol	16.092	330	1967862	178.072	ng	0.00
45) 2-Fluorobiphenyl	13.228	172	6580100	96.203	ng	0.00
79) Terphenyl-d14	19.910	244	10550391	108.829	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090922\
Data File : BP011669.D
Acq On : 09 Sep 2022 18:31
Operator : CG/JU
Sample : N4549-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MW-57

Quant Time: Sep 10 00:55:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 10 00:48:09 2022
Response via : Initial Calibration




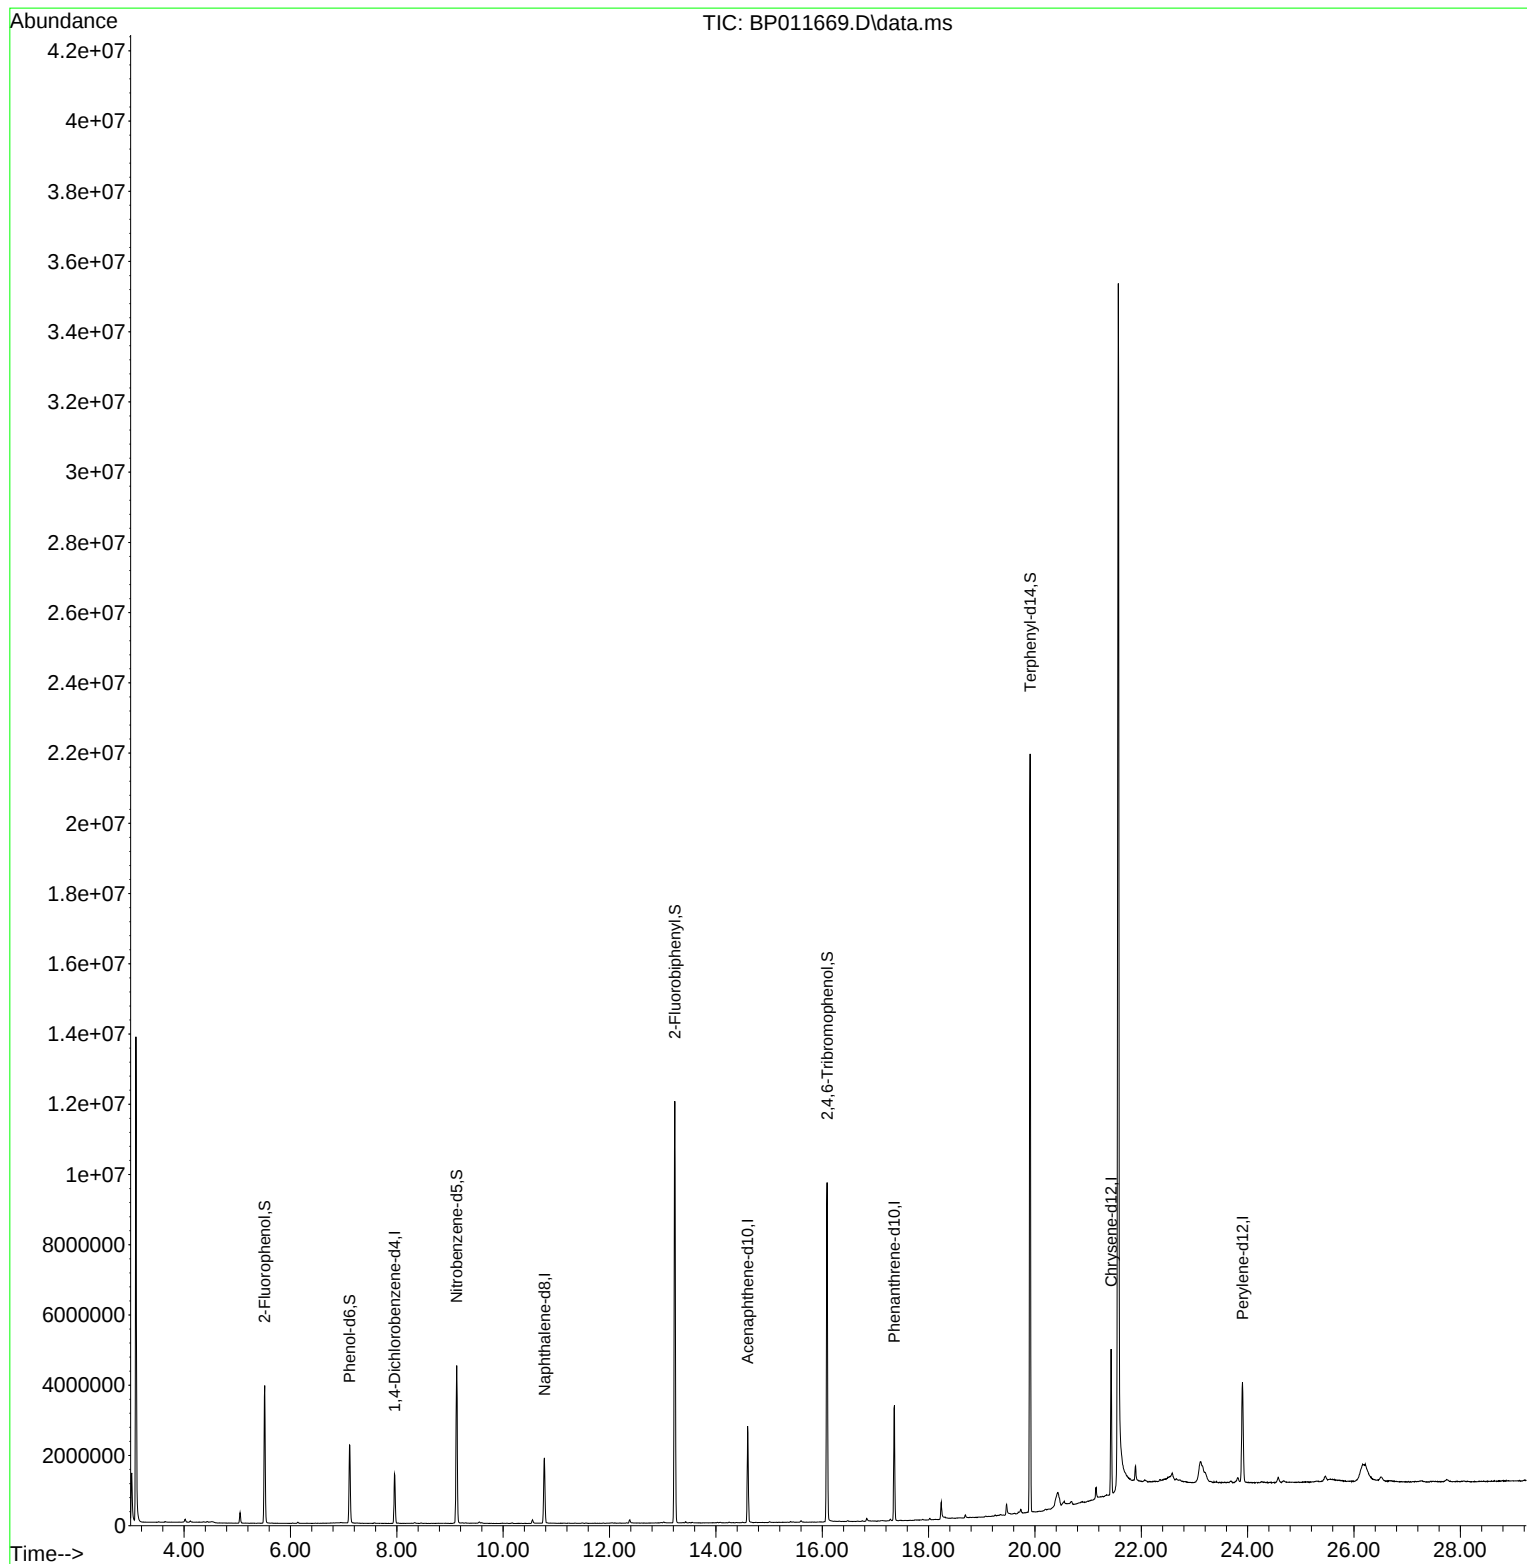


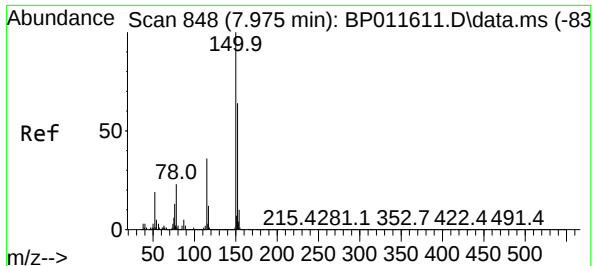

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.957 min Scan# 84
Delta R.T. -0.007 min
Lab File: BP011669.D
Acq: 09 Sep 2022 18:31




Instrument :
BNA_P
ClientSampleId :
MW-57


Tgt Ion:152 Resp: 413251
Ion Ratio Lower Upper
152 100
150 157.8 123.4 185.2
115 58.0 51.3 76.9

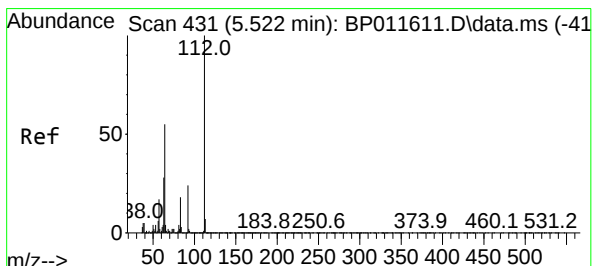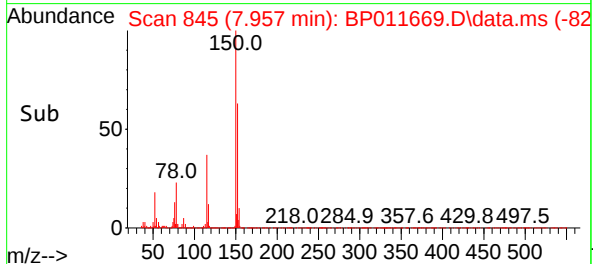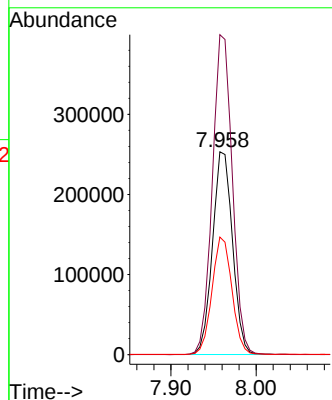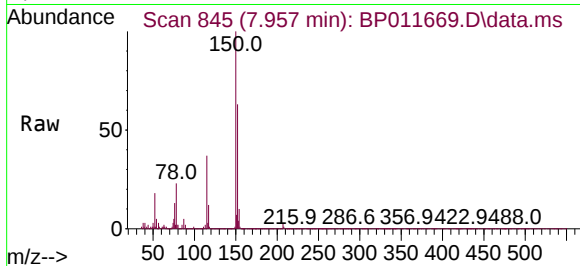

#5
2-Fluorophenol
Concen: 77.846 ng
RT: 5.516 min Scan# 430
Delta R.T. -0.000 min
Lab File: BP011669.D
Acq: 09 Sep 2022 18:31

Tgt Ion:112 Resp: 1818946
Ion Ratio Lower Upper
112 100
64 52.6 56.9 85.3#
63 27.0 31.2 46.8#


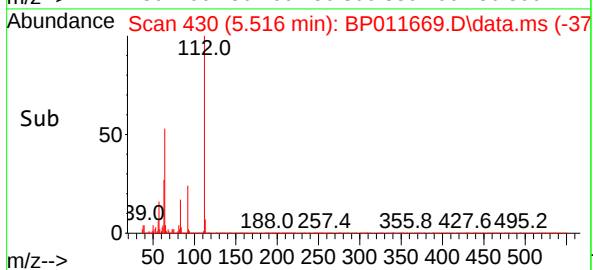
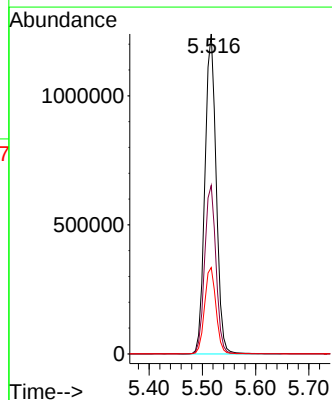
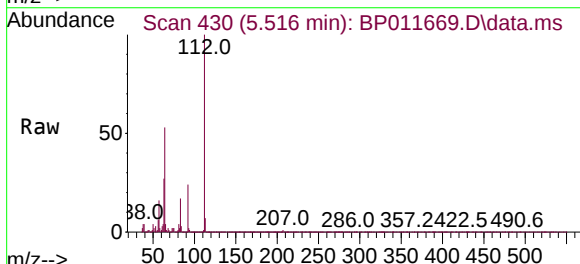


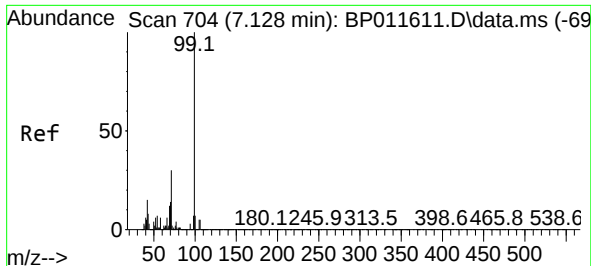

#7
Phenol-d6
Concen: 45.993 ng
RT: 7.111 min Scan# 704
Delta R.T. -0.006 min
Lab File: BP011669.D
Acq: 09 Sep 2022 18:31




Instrument :
BNA_P
ClientSampleId :
MW-57


Tgt Ion: 99 Resp: 1422006
Ion Ratio Lower Upper
99 100
42 14.4 20.3 30.5#
71 30.0 33.9 50.9#

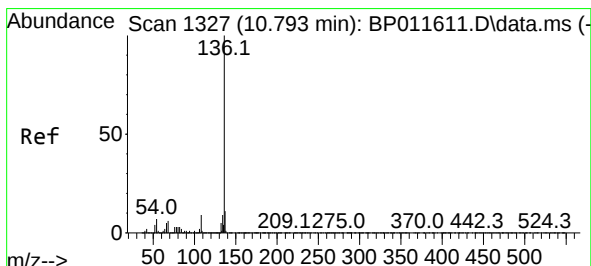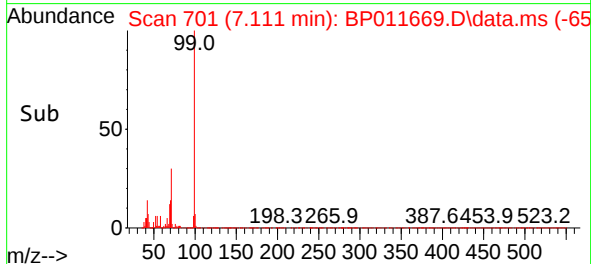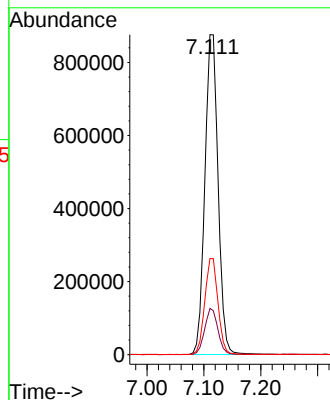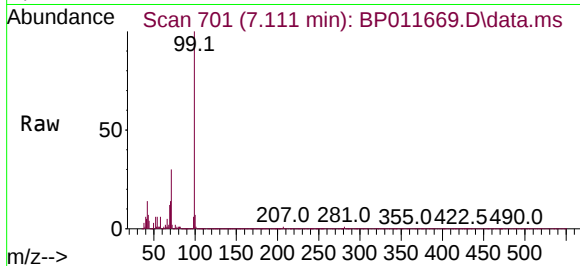

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.775 min Scan# 1324
Delta R.T. -0.000 min
Lab File: BP011669.D
Acq: 09 Sep 2022 18:31

Tgt Ion:136 Resp: 1645432
Ion Ratio Lower Upper
136 100
137 10.6 9.0 13.4
54 6.7 8.7 13.1#
68 5.4 4.8 7.2


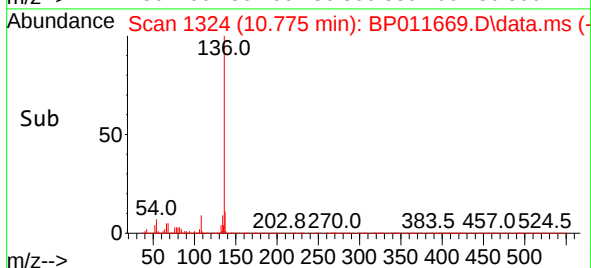
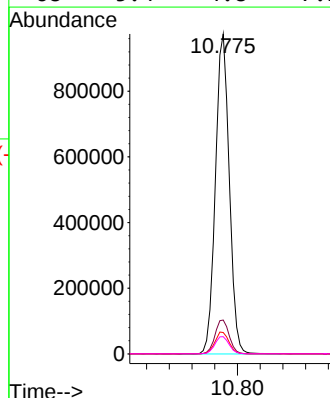
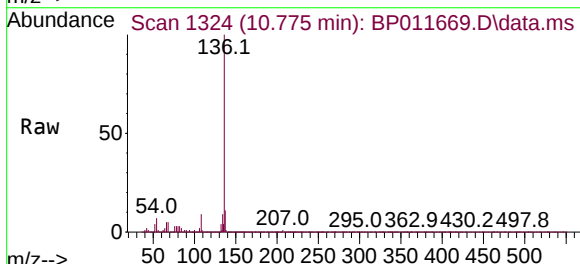


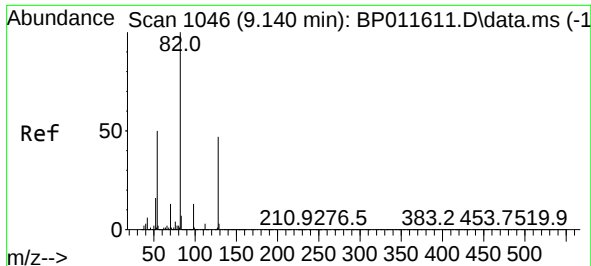

#23
Nitrobenzene-d5
Concen: 96.886 ng
RT: 9.128 min Scan# 1044
Delta R.T. -0.000 min
Lab File: BP011669.D
Acq: 09 Sep 2022 18:31




Instrument :
BNA_P
ClientSampleId :
MW-57


Tgt Ion: 82 Resp: 2597085
Ion Ratio Lower Upper
82 100
128 48.5 31.3 46.9#
54 45.3 49.8 74.8#

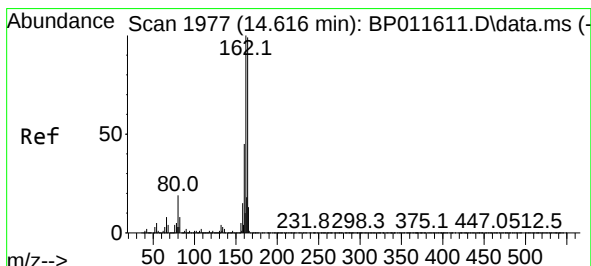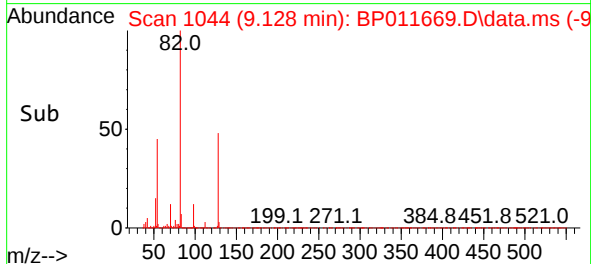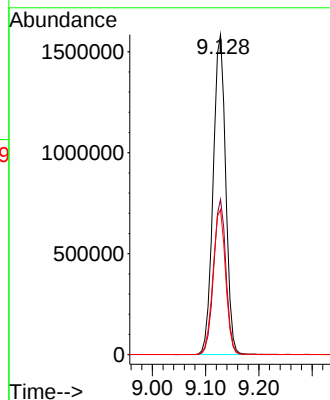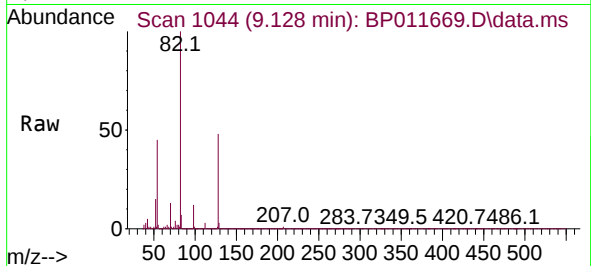

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.598 min Scan# 1974
Delta R.T. -0.006 min
Lab File: BP011669.D
Acq: 09 Sep 2022 18:31

Tgt Ion: 164 Resp: 978096
Ion Ratio Lower Upper
164 100
162 99.3 81.9 122.9
160 44.6 34.6 51.8


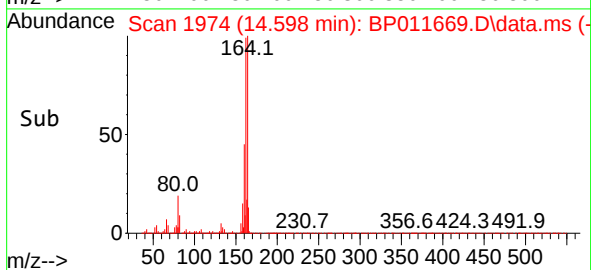
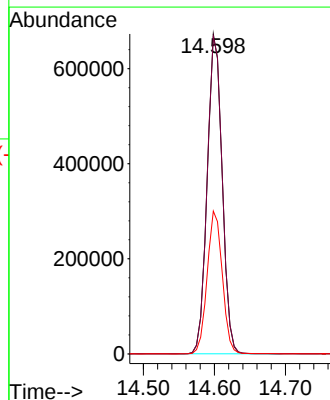
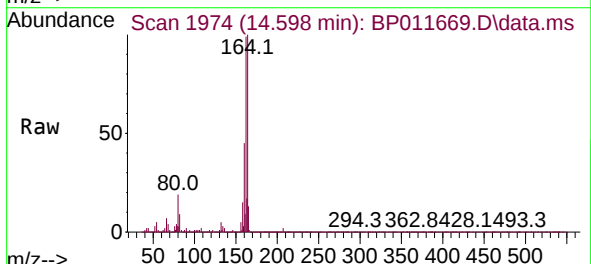


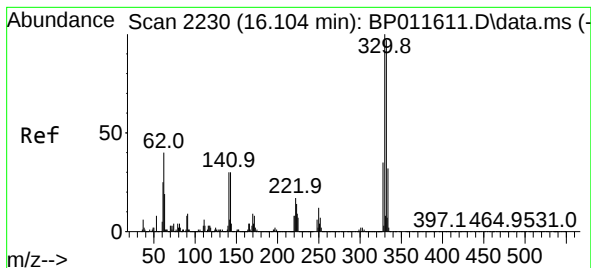

#42
2,4,6-Tribromophenol
Concen: 178.072 ng
RT: 16.092 min Scan# 21
Delta R.T. -0.000 min
Lab File: BP011669.D
Acq: 09 Sep 2022 18:31




Instrument :
BNA_P
ClientSampleId :
MW-57


Tgt Ion:330 Resp: 1967862
Ion Ratio Lower Upper
330 100
332 96.1 78.1 117.1
141 29.4 31.4 47.2#

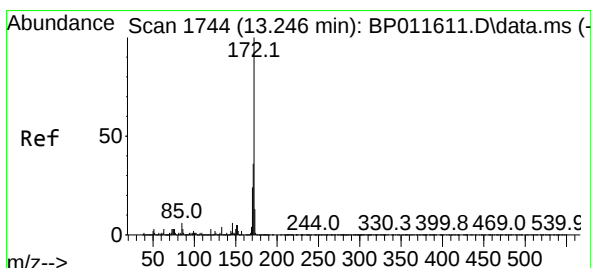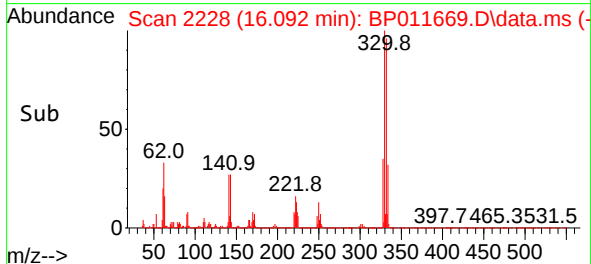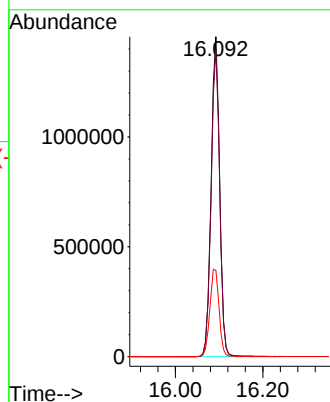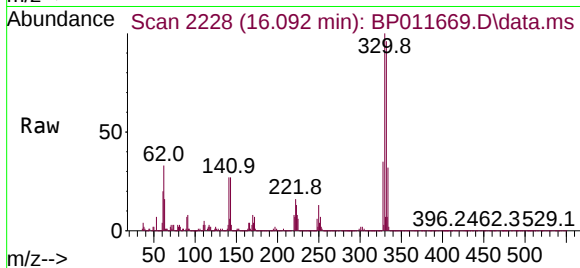

#45
2-Fluorobiphenyl
Concen: 96.203 ng
RT: 13.228 min Scan# 1741
Delta R.T. -0.000 min
Lab File: BP011669.D
Acq: 09 Sep 2022 18:31

Tgt Ion:172 Resp: 6580100
Ion Ratio Lower Upper
172 100
171 35.5 27.9 41.9
170 23.9 18.2 27.2


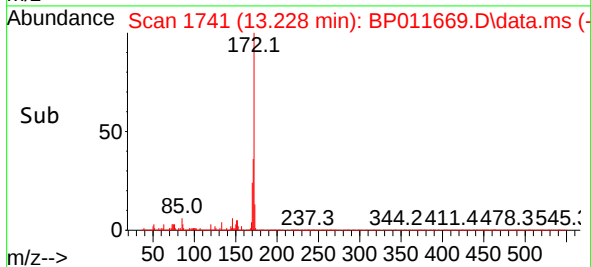
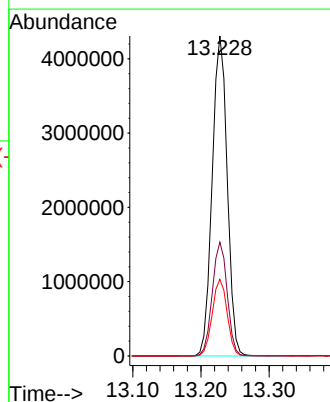
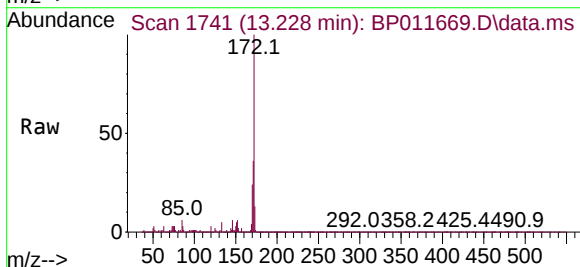


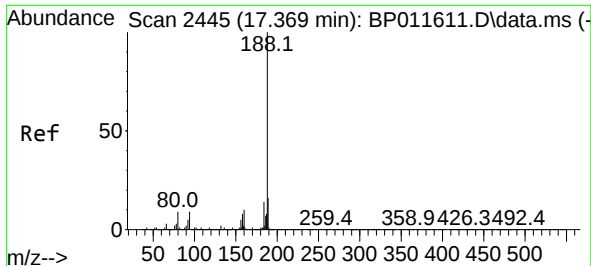

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.357 min Scan# 2443
Delta R.T. -0.000 min
Lab File: BP011669.D
Acq: 09 Sep 2022 18:31




Instrument :
BNA_P
ClientSampleId :
MW-57


Tgt Ion:188 Resp: 2047101
Ion Ratio Lower Upper
188 100
94 8.3 6.6 10.0
80 8.7 8.0 12.0

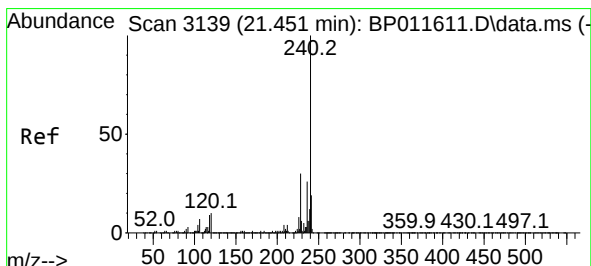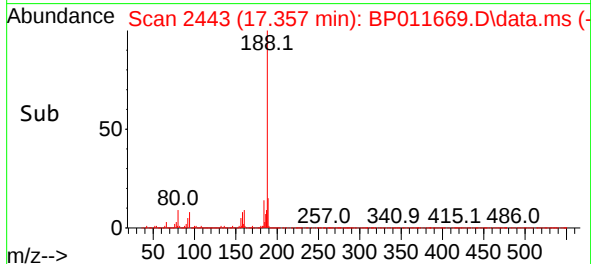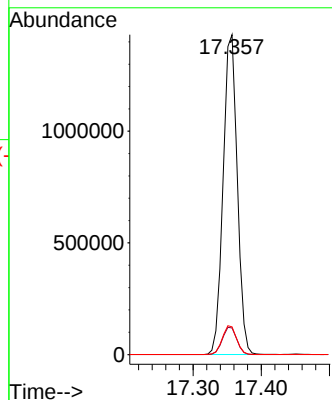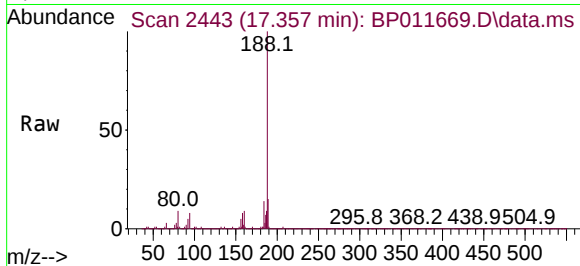

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.433 min Scan# 3136
Delta R.T. -0.006 min
Lab File: BP011669.D
Acq: 09 Sep 2022 18:31

Tgt Ion:240 Resp: 2030492
Ion Ratio Lower Upper
240 100
120 10.0 8.6 12.8
236 26.0 19.8 29.6

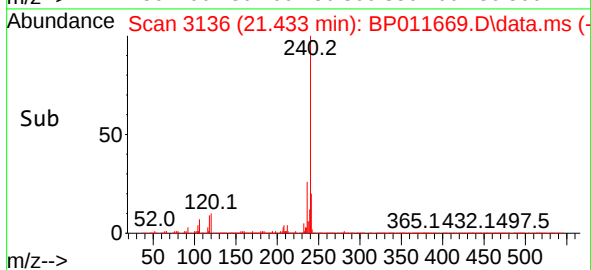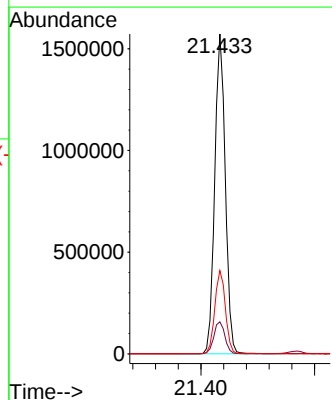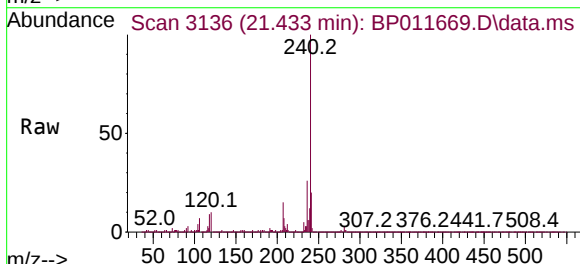

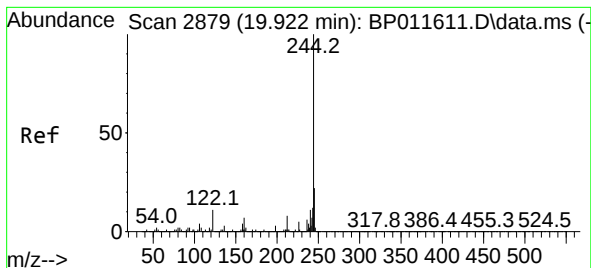

#79

Terphenyl-d14

Concen: 108.829 ng

RT: 19.910 min Scan# 2879

Delta R.T. -0.000 min

Lab File: BP011669.D

Acq: 09 Sep 2022 18:31

Instrument :

BNA_P

ClientSampleId :

MW-57





Tgt Ion:244 Resp:10550391

Ion Ratio Lower Upper

244 100

212 7.2 5.8 8.8

122 10.2 7.6 11.4

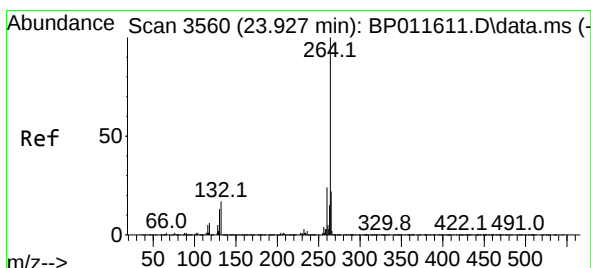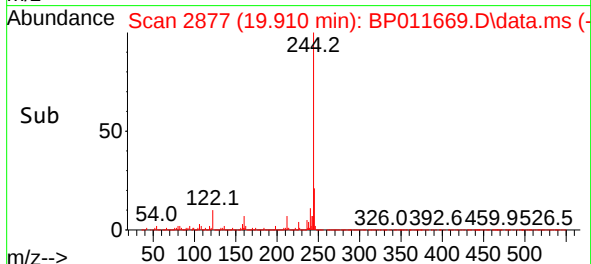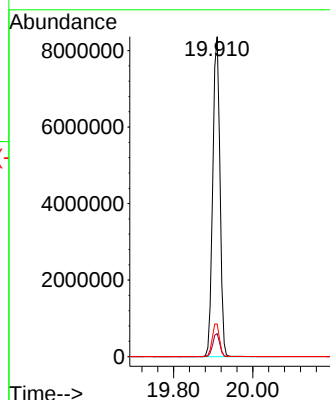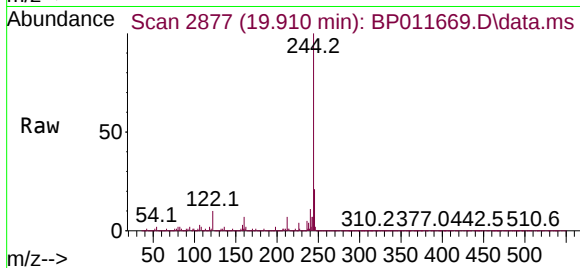

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.904 min Scan# 3556

Delta R.T. -0.006 min

Lab File: BP011669.D

Acq: 09 Sep 2022 18:31

Tgt Ion:264 Resp: 2237676

Ion Ratio Lower Upper

264 100

260 24.3 19.3 28.9

265 21.9 18.0 27.0

