
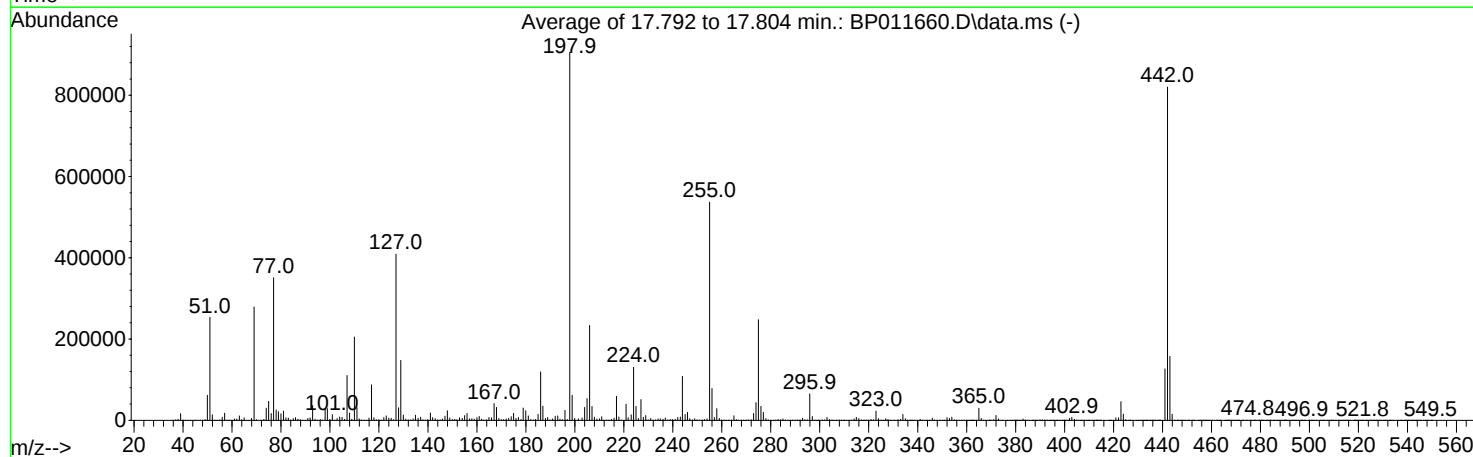


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090922\
 Data File : BP011660.D
 Acq On : 09 Sep 2022 11:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 10 00:48:09 2022

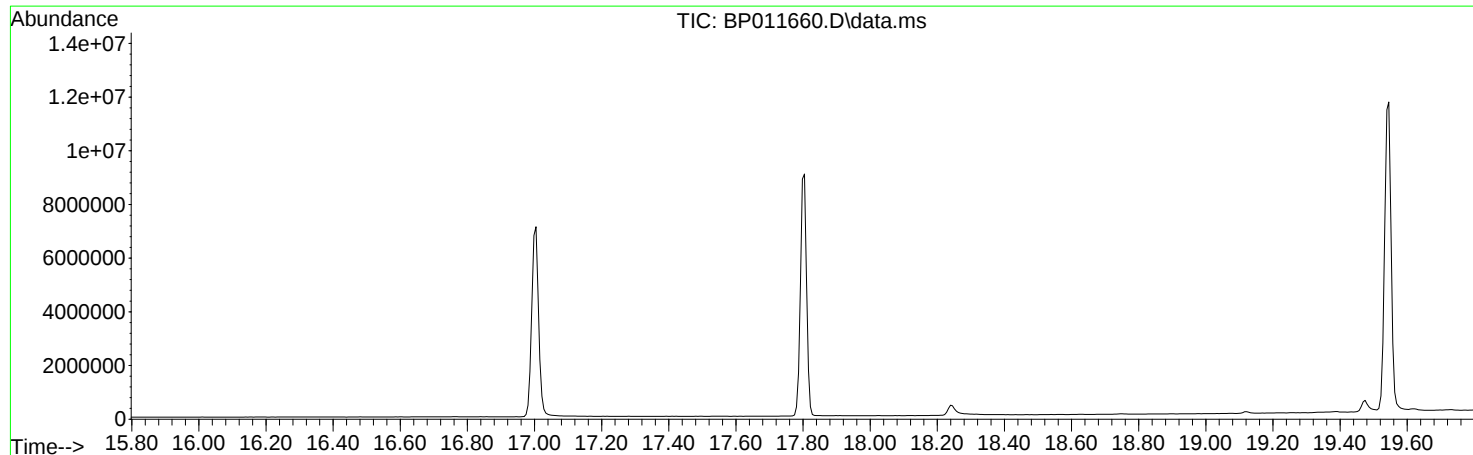




AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.0	253434	PASS
68	69	0.00	2	1.6	4362	PASS
69	198	0.00	100	30.8	279157	PASS
70	69	0.00	2	0.5	1422	PASS
127	198	10	80	45.2	408944	PASS
197	198	0.00	2	0.2	1411	PASS
198	198	100	100	100.0	905413	PASS
199	198	5	9	6.8	61624	PASS
275	198	10	60	27.4	247648	PASS
365	198	1	100	3.3	29608	PASS
441	198	0.01	100	14.0	126727	PASS
442	442	100	100	100.0	820138	PASS
443	442	15	24	19.2	157528	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090922\
 Data File : BP011660.D
 Acq On : 09 Sep 2022 11:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 10 04:56:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 10 00:48:09 2022
 Response via : Initial Calibration

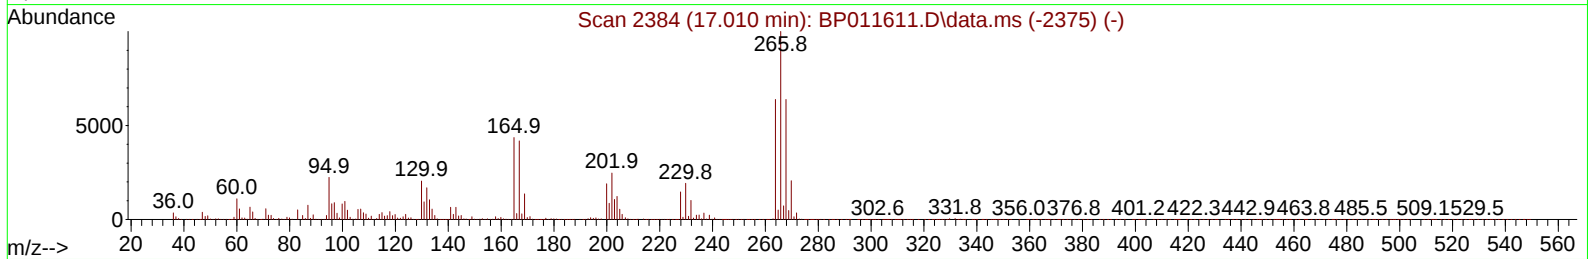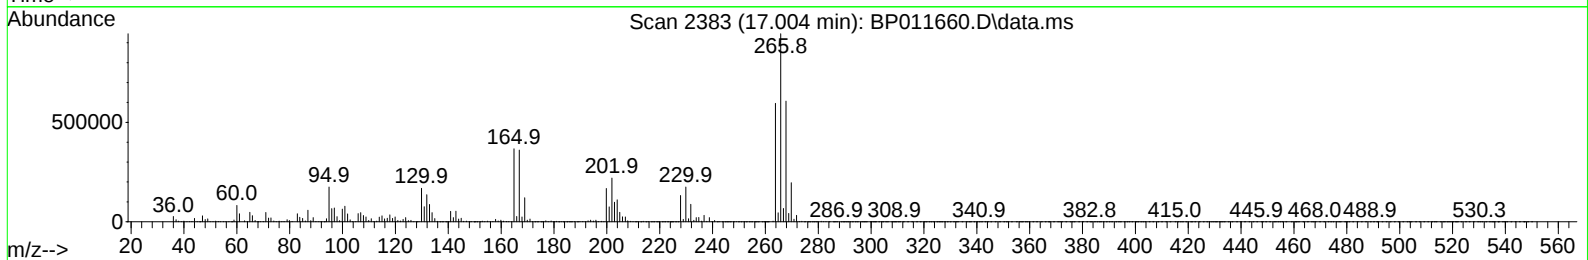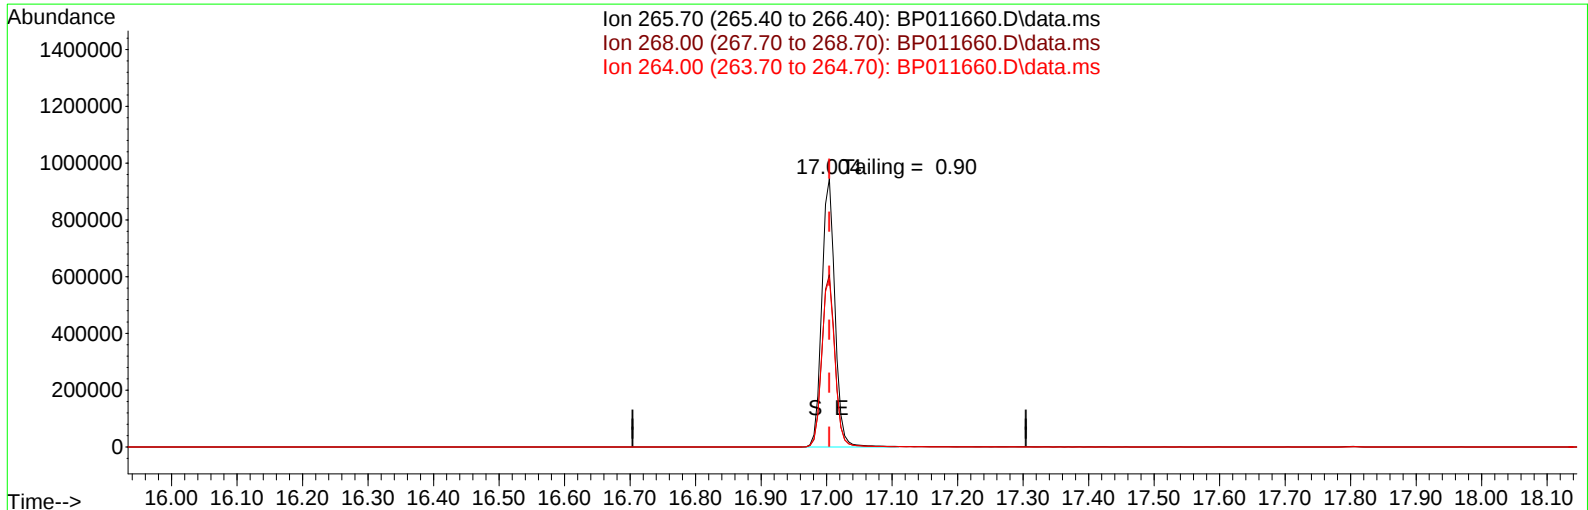

TIC: BP011660.D\data.ms

(70) Pentachlorophenol (C)

17.004min (-0.000) 1022382.80 ng




response 1325818

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.16
264.00	63.00	63.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090922\
 Data File : BP011660.D
 Acq On : 09 Sep 2022 11:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 10 04:56:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 10 00:48:09 2022
 Response via : Initial Calibration

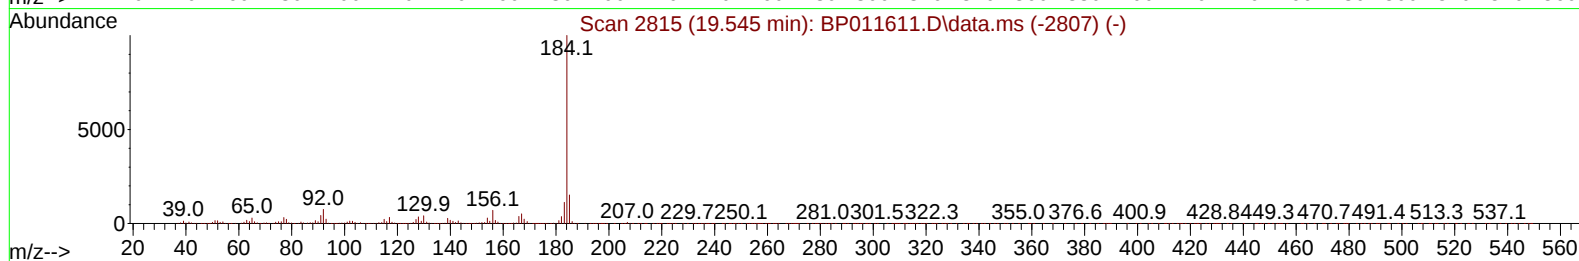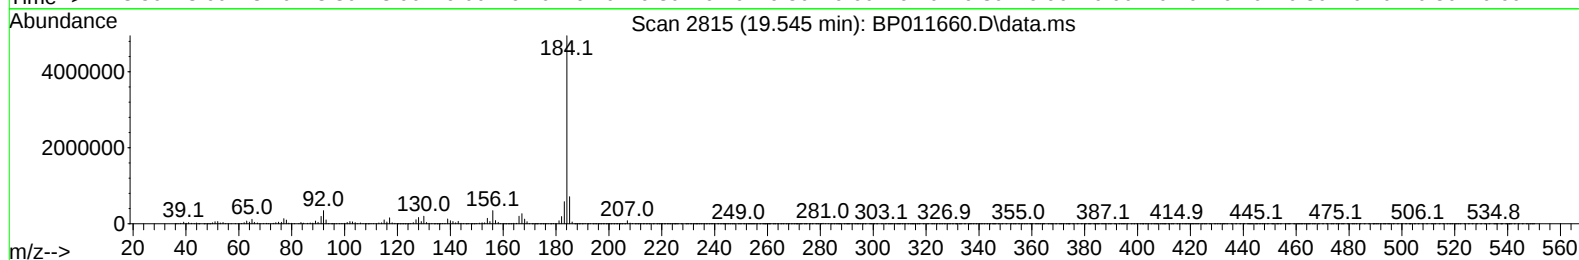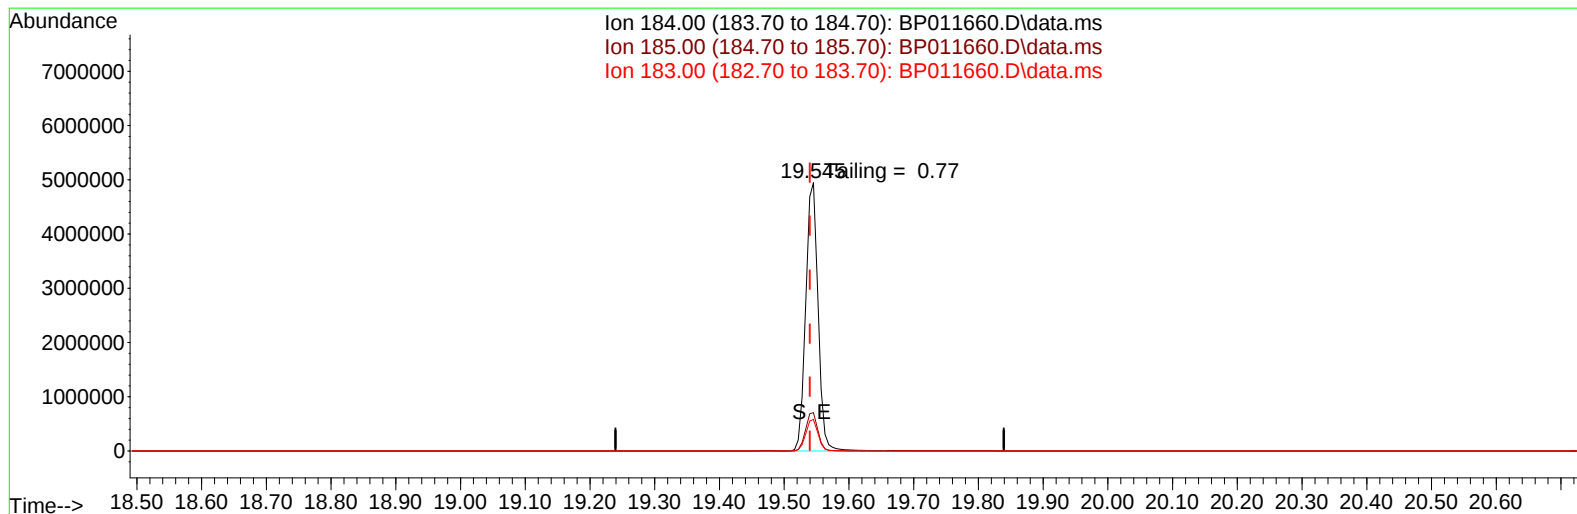

TIC: BP011660.D\data.ms

(77) Benzidine

19.545min (+ 0.006) 302473.39 ng

response 6614037

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.35
183.00	11.30	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/9/2022	BNA_P	<u>BP011660.D</u>
Compound Name	Response	Retention Time
DDT	3190446	20.745
DDD	33814	20.316
DDE	1559	19.816
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
35373	3225819	1.10

Instrument :
BNA_P
ClientSampleId :
DFTPP