

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091019\
 Data File : BP000175.D
 Acq On : 10 Sep 2019 19:24
 Operator : HP/JU
 Sample : K4780-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Sep 11 01:58:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 02:43:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	438268	20.00	ng/ul	0.00
18) Naphthalene-d8	8.17	136	1729049	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.95	164	940848	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.45	188	1713076	20.00	ng/ul	0.00
78) Chrysene-d12	14.14	240	1304634	20.00	ng/ul	0.00
86) Perylene-d12	15.69	264	1310579	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.61	96	52923	4.28	ng/uL	0.00
5) Phenol-d5	6.50	99	232101	6.22	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.57	67	480010	24.59	ng/ul	0.00
9) 2-Chlorophenol-d4	6.66	132	635600	21.05	ng/ul	0.00
13) 4-Methylphenol-d8	7.26	113	414857	14.79	ng/ul	0.00
19) Nitrobenzene-d5	7.45	128	369609	28.15	ng/ul	0.00
22) 2-Nitrophenol-d4	7.77	143	395289	30.93	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	8.01	165	659076	24.29	ng/ul	0.00
29) 4-Chloroaniline-d4	8.23	131	168356	5.02	ng/ul	0.00
44) Dimethylphthalate-d6	9.63	166	2103815	30.28	ng/ul	0.00
47) Acenaphthylene-d8	9.79	160	2446077	28.49	ng/ul	0.00
52) 4-Nitrophenol-d4	10.03	143	80647	6.50	ng/ul	0.00
58) Fluorene-d10	10.47	176	1687196	28.60	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.53	200	220278	27.98	ng/ul	0.00
71) Anthracene-d10	11.50	188	2439150	29.40	ng/ul	0.00
79) Pyrene-d10	12.90	212	2611727	33.66	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.59	264	2241634	33.00	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	9.65	163	186477	2.660	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091019\
Data File : BP000175.D
Acq On : 10 Sep 2019 19:24
Operator : HP/JU
Sample : K4780-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Sep 11 01:58:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 02:43:18 2019
Response via : Initial Calibration

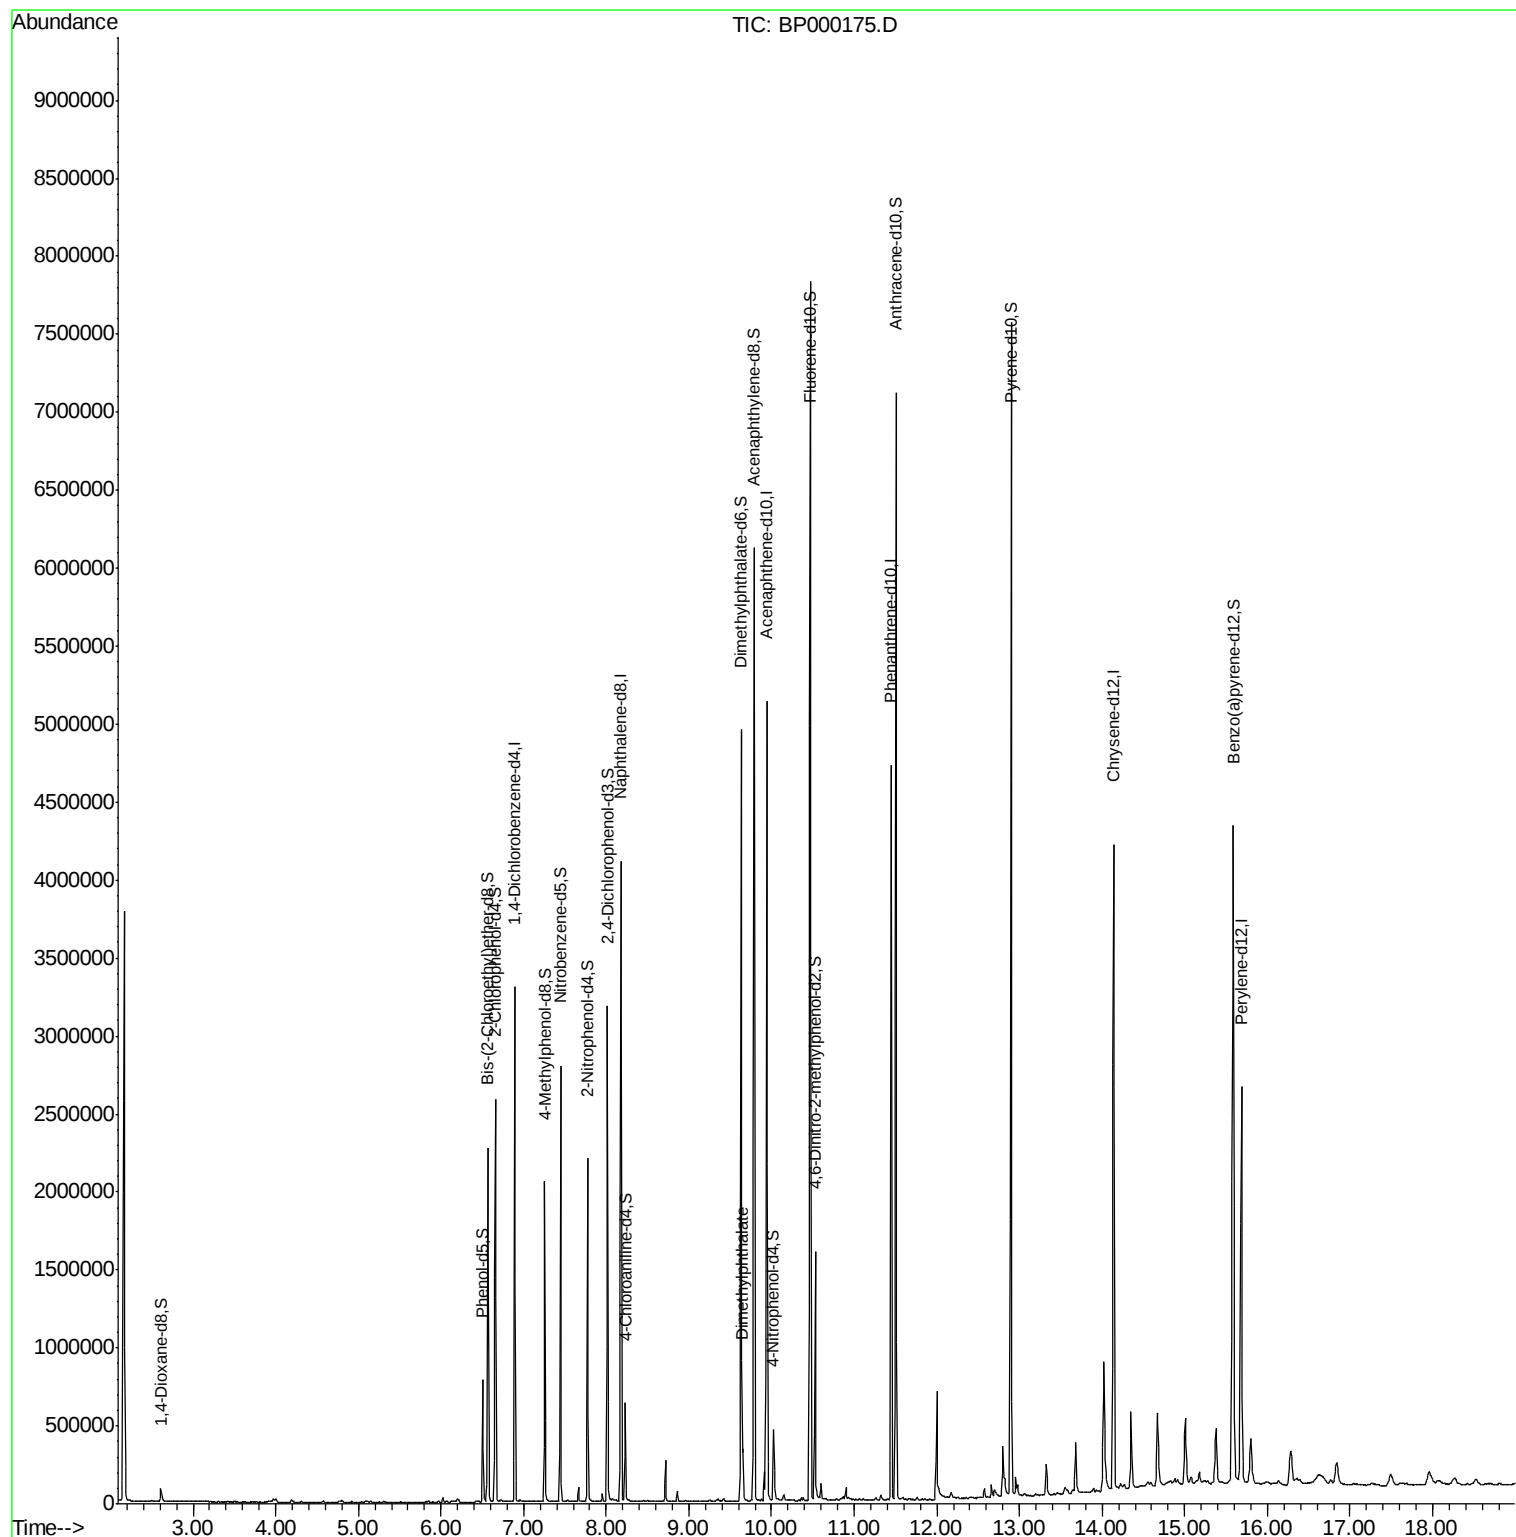

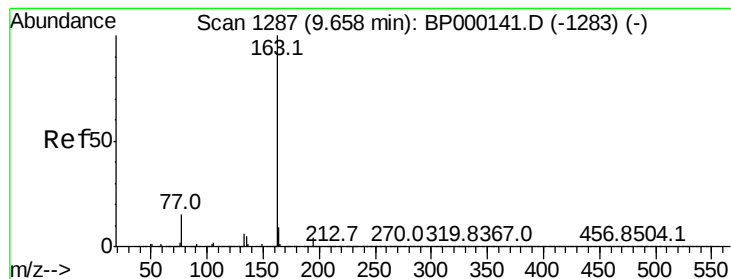

#45

Dimethylphthalate

Concen: 2.660 ng/ul

RT: 9.65 min Scan# 1286

Delta R.T. -0.01 min

Lab File: BP000175.D

Acq: 10 Sep 2019 19:24

Instrument :

BNA_P

ClientSampleId :


Tot Ion:163 Resp: 186477

Ion Ratio Lower Upper

163 100

194 4.0 3.2 4.8

164 9.9 8.4 12.6

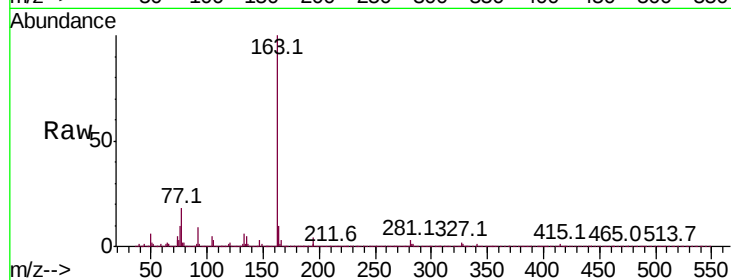

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

