

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091019\
 Data File : BP000172.D
 Acq On : 10 Sep 2019 18:11
 Operator : HP/JU
 Sample : K4780-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0BN8

Quant Time: Sep 11 01:57:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 02:43:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	389525	20.00	ng/ul	0.00
18) Naphthalene-d8	8.18	136	1526574	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.95	164	845510	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.45	188	1536194	20.00	ng/ul	0.00
78) Chrysene-d12	14.14	240	1244559	20.00	ng/ul	0.00
86) Perylene-d12	15.68	264	1245628	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.60	96	49898	4.54	ng/uL	0.00
5) Phenol-d5	6.50	99	221566	6.68	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.57	67	450744	25.98	ng/ul	0.00
9) 2-Chlorophenol-d4	6.66	132	615024	22.92	ng/ul	0.00
13) 4-Methylphenol-d8	7.26	113	384343	15.42	ng/ul	0.00
19) Nitrobenzene-d5	7.45	128	345212	29.78	ng/ul	0.00
22) 2-Nitrophenol-d4	7.78	143	367097	32.53	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	8.01	165	605233	25.27	ng/ul	0.00
29) 4-Chloroaniline-d4	8.23	131	148493	5.01	ng/ul	0.00
44) Dimethylphthalate-d6	9.63	166	1847181	29.59	ng/ul	0.00
47) Acenaphthylene-d8	9.79	160	2231407	28.92	ng/ul	0.00
52) 4-Nitrophenol-d4	10.02	143	81362	7.29	ng/ul	-0.01
58) Fluorene-d10	10.47	176	1529293	28.84	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.53	200	203170	28.77	ng/ul	0.00
71) Anthracene-d10	11.50	188	2349994	31.59	ng/ul	0.00
79) Pyrene-d10	12.90	212	2511658	33.93	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.59	264	2190305	33.92	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	9.65	163	337151	5.352	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091019\
Data File : BP000172.D
Acq On : 10 Sep 2019 18:11
Operator : HP/JU
Sample : K4780-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0BN8

Quant Time: Sep 11 01:57:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 02:43:18 2019
Response via : Initial Calibration

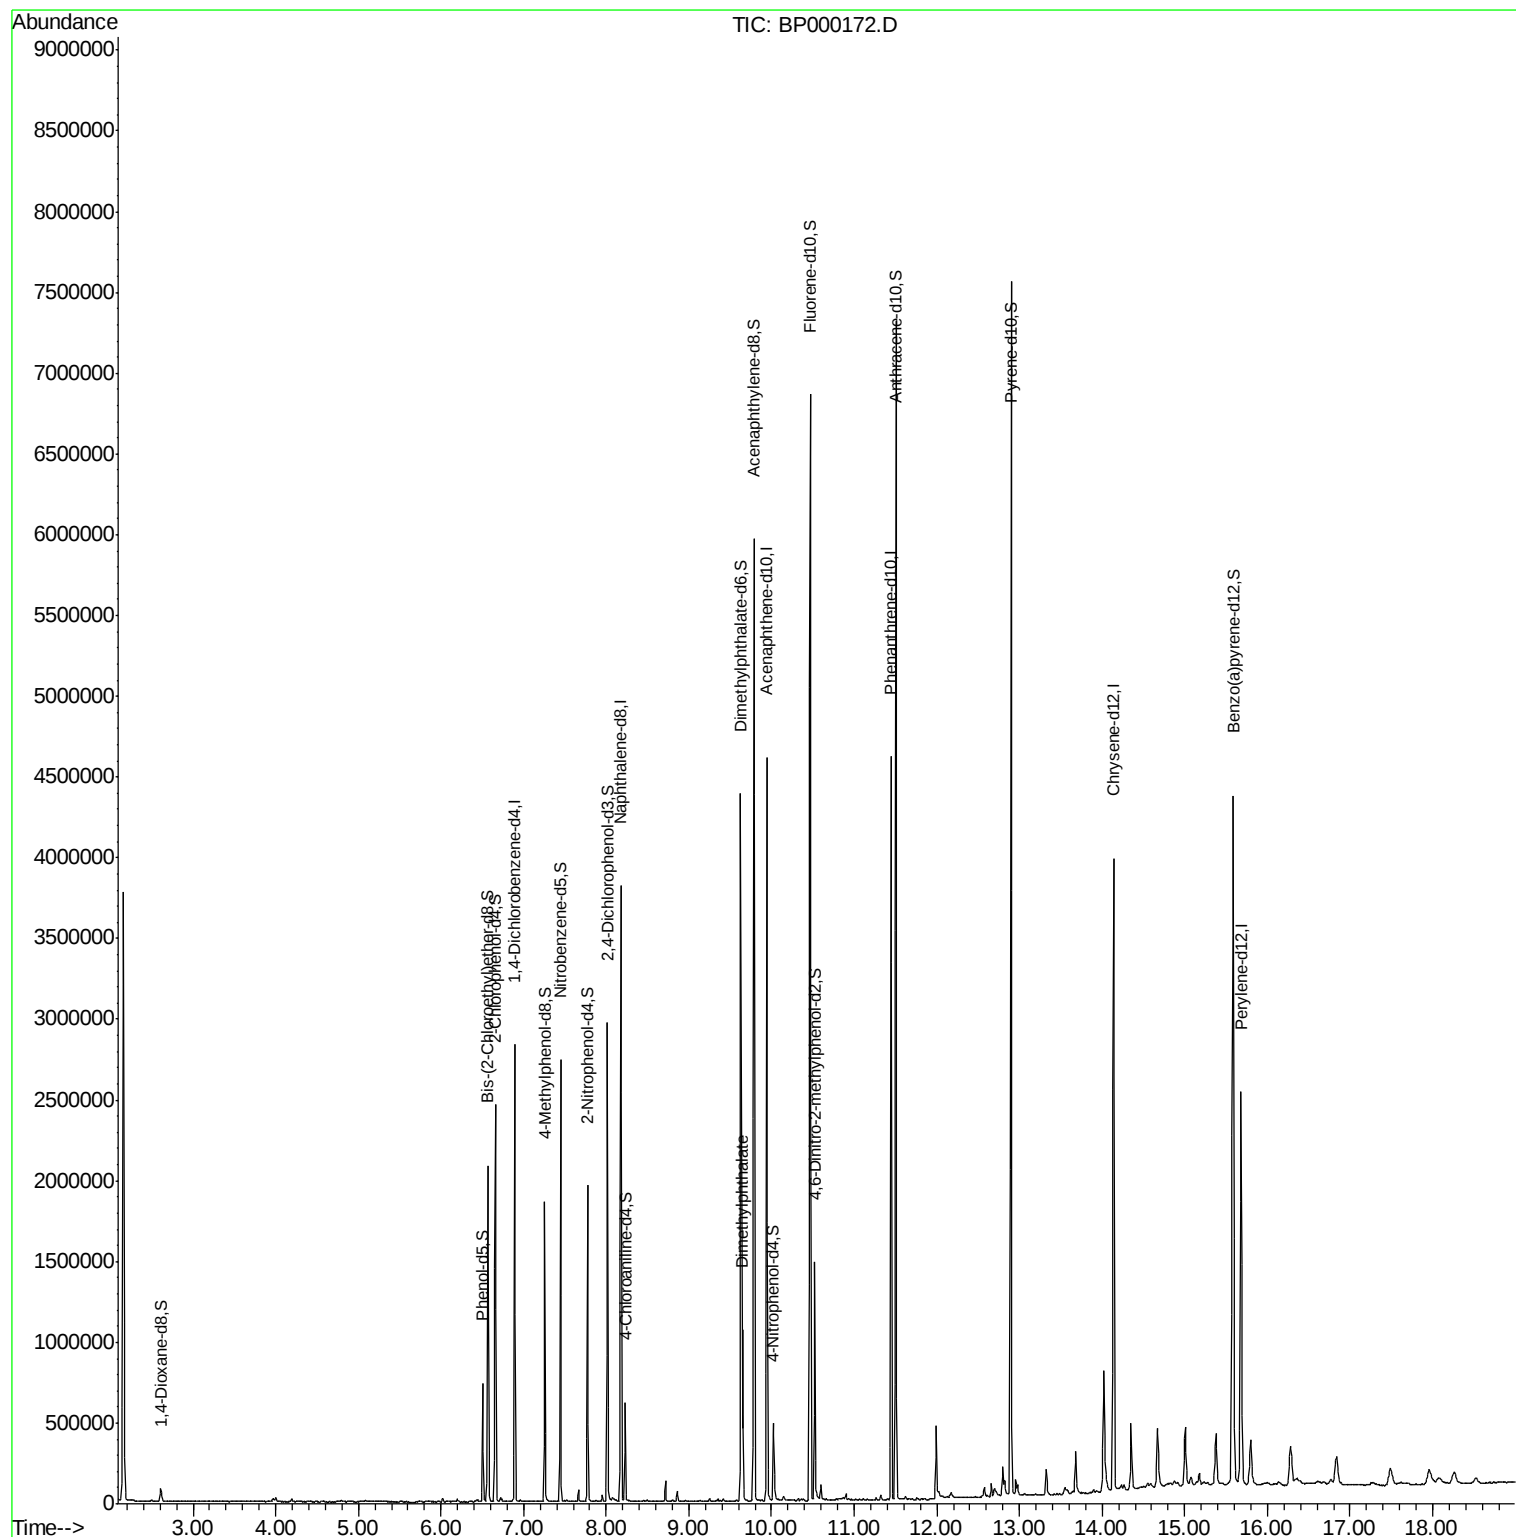

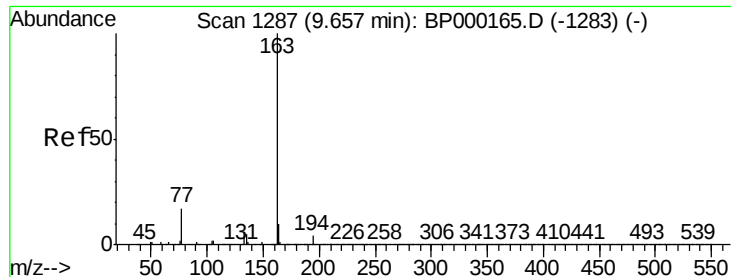

#45
 Dimethylphthalate
 Concen: 5.352 ng/ul
 RT: 9.65 min Scan# 1286
 Delta R.T. -0.01 min
 Lab File: BP000172.D
 Acq: 10 Sep 2019 18:11

Instrument :
 BNA_P
 ClientSampleId :
 H0BN8

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.2	4.8
164	10.0	8.4	12.6

