

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091019\
 Data File : BP000173.D
 Acq On : 10 Sep 2019 18:36
 Operator : HP/JU
 Sample : K4780-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0BM4

Quant Time: Sep 11 01:58:04 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 02:43:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	435556	20.00	ng/ul	0.00
18) Naphthalene-d8	8.17	136	1707811	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.95	164	957739	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.45	188	1688123	20.00	ng/ul	0.00
78) Chrysene-d12	14.14	240	1287471	20.00	ng/ul	0.00
86) Perylene-d12	15.69	264	1319092	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.61	96	45342	3.69	ng/uL	0.00
5) Phenol-d5	6.50	99	234590	6.32	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.57	67	472246	24.34	ng/ul	0.00
9) 2-Chlorophenol-d4	6.66	132	625501	20.85	ng/ul	0.00
13) 4-Methylphenol-d8	7.26	113	419974	15.07	ng/ul	0.00
19) Nitrobenzene-d5	7.45	128	360452	27.80	ng/ul	0.00
22) 2-Nitrophenol-d4	7.77	143	383626	30.39	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	8.02	165	653141	24.38	ng/ul	0.00
29) 4-Chloroaniline-d4	8.23	131	188277	5.68	ng/ul	0.00
44) Dimethylphthalate-d6	9.63	166	2093068	29.60	ng/ul	0.00
47) Acenaphthylene-d8	9.79	160	2379037	27.22	ng/ul	0.00
52) 4-Nitrophenol-d4	10.02	143	83386	6.60	ng/ul	-0.01
58) Fluorene-d10	10.47	176	1696667	28.25	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.53	200	214655	27.66	ng/ul	0.00
71) Anthracene-d10	11.50	188	2478532	30.32	ng/ul	0.00
79) Pyrene-d10	12.90	212	2484144	32.44	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.59	264	2241752	32.79	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	9.65	163	196936	2.760	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091019\
Data File : BP000173.D
Acq On : 10 Sep 2019 18:36
Operator : HP/JU
Sample : K4780-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0BM4

Quant Time: Sep 11 01:58:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 02:43:18 2019
Response via : Initial Calibration

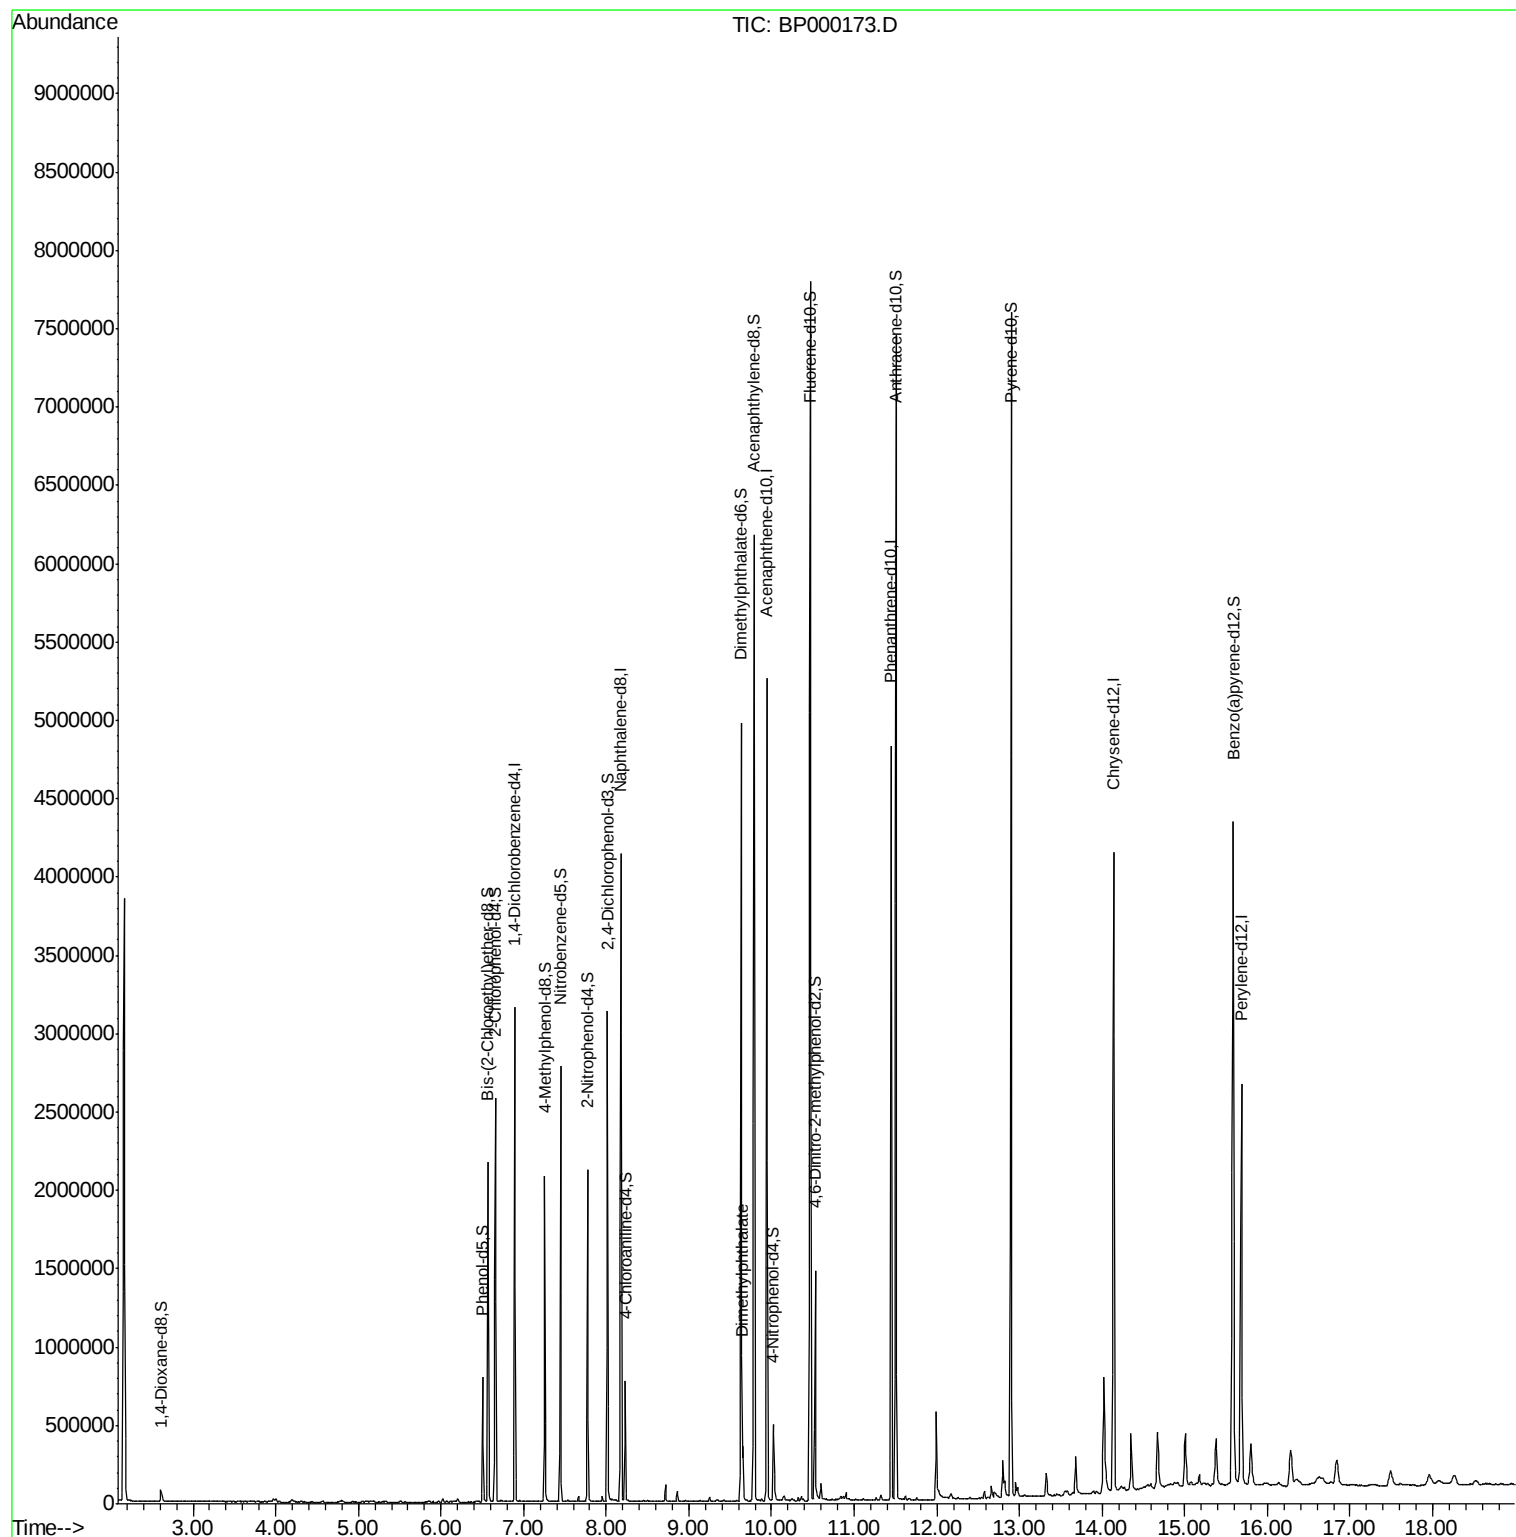

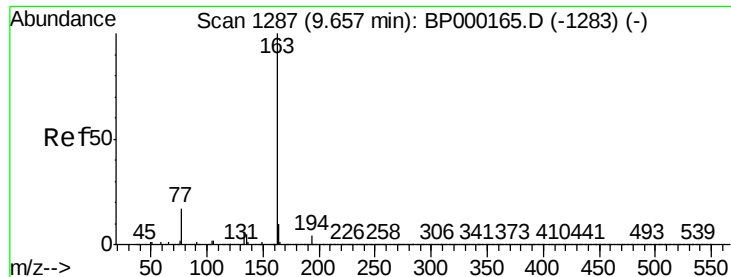

#45
 Dimethylphthalate
 Concen: 2.760 ng/ul
 RT: 9.65 min Scan# 1286
 Delta R.T. -0.01 min
 Lab File: BP000173.D
 Acq: 10 Sep 2019 18:36

Instrument :
 BNA_P
 ClientSampleId :
 H0BM4

Tot Ion:163	Resp:	196936
Ion Ratio	Lower	Upper
163	100	
194	4.2	3.2 4.8
164	10.1	8.4 12.6

