

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091019\
 Data File : BP000184.D
 Acq On : 10 Sep 2019 23:03
 Operator : HP/JU
 Sample : K4633-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F2D03

Manual Integrations
 APPROVED

mohammad
 9/12/2019 9:29:59 AM

Quant Time: Sep 11 04:05:37 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 02:43:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	462941	20.00	ng/ul	0.00
18) Naphthalene-d8	8.17	136	1756497	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.95	164	920135	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.45	188	1577123	20.00	ng/ul	0.00
78) Chrysene-d12	14.15	240	1031024	20.00	ng/ul	0.00
86) Perylene-d12	15.70	264	1175005	20.00	ng/ul	0.01


System Monitoring Compounds

3) 1,4-Dioxane-d8	2.62	96	53178	4.07	ng/uL	0.01
5) Phenol-d5	6.51	99	988000	25.06	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.58	67	507779	24.63	ng/ul	0.00
9) 2-Chlorophenol-d4	6.66	132	814778	25.55	ng/ul	0.00
13) 4-Methylphenol-d8	7.26	113	768034	25.93	ng/ul	0.00
19) Nitrobenzene-d5	7.45	128	392528	29.43	ng/ul	0.00
22) 2-Nitrophenol-d4	7.77	143	421054	32.43	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	8.02	165	720634	26.15	ng/ul	0.00
29) 4-Chloroaniline-d4	8.23	131	781827	22.94	ng/ul	0.00
44) Dimethylphthalate-d6	9.63	166	1957664	28.81	ng/ul	0.00
47) Acenaphthylene-d8	9.79	160	2323607	27.67	ng/ul	0.00
52) 4-Nitrophenol-d4	10.03	143	265787	21.89	ng/ul	0.00
58) Fluorene-d10	10.47	176	1547918	26.83	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.53	200	100354	13.84	ng/ul	0.00
71) Anthracene-d10	11.50	188	2041599	26.73	ng/ul	0.00
79) Pyrene-d10	12.90	212	2007708	32.74	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.60	264	1785268	29.31	ng/ul	0.02

Target Compounds

					Ovalue	
6) Phenol	6.52	94	165914	4.037	ng/ul	99
28) Naphthalene	8.20	128	198868	2.079	ng/ul	99
45) Dimethylphthalate	9.66	163	706835	10.310	ng/ul	98
50) Acenaphthene	9.97	153	431724	7.103	ng/ul	100
54) Dibenzofuran	10.15	168	141630	1.698	ng/ul	98
59) Fluorene	10.50	166	202614	3.141	ng/ul	99
70) Phenanthrene	11.47	178	2843321	30.486	ng/ul	99
72) Anthracene	11.53	178	608458	6.630	ng/ul	99
75) Carbazole	11.67	167	439770	5.604	ng/ul	100
77) Fluoranthene	12.69	202	4765179	50.656	ng/ul	97
80) Pyrene	12.92	202	4236533	54.464	ng/ul	96
83) Benzo(a)anthracene	14.14	228	2797093	37.478	ng/ul	95
85) Chrysene	14.18	228	3015601	44.033	ng/ul	98
88) Benzo(b)fluoranthene	15.25	252	4793521	61.553	ng/ul	97
89) Benzo(k)fluoranthene	15.27	252	812098m	11.063	ng/ul	
91) Benzo(a)pyrene	15.64	252	3106297	42.513	ng/ul	98
92) Indeno(1,2,3-cd)pyrene	17.28	276	2334257	27.769	ng/ul	99
93) Dibenzo(a,h)anthracene	17.29	278	610825	8.773	ng/ul	98
94) Benzo(g,h,i)perylene	17.75	276	1958345	27.942	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#6

Phenol

Concen: 4.037 ng/ul

RT: 6.52 min Scan# 754

Delta R.T. -0.00 min

Lab File: BP000184.D

Acq: 10 Sep 2019 23:03

Instrument :

BNA_P





ClientSampleId :

F2D03

Tot Ion:	94	Resp:	165914
Ion Ratio	Lower	Upper	
94	100		
65	23.4	18.8	28.2
66	31.5	24.2	36.2

Manual Integrations
APPROVED

mohammad
9/12/2019 9:29:59 AM

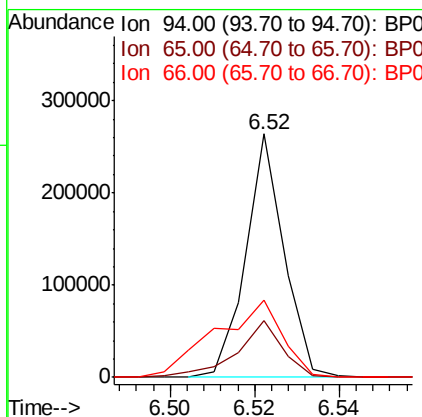

#28

Naphthalene

Concen: 2.079 ng/ul




RT: 8.20 min Scan# 1039


Delta R.T. -0.00 min

Lab File: BP000184.D

Acq: 10 Sep 2019 23:03

Tgt Ion:	128	Resp:	198868
Ion Ratio	Lower	Upper	
128	100		
129	11.0	9.1	13.7
127	13.4	10.7	16.1

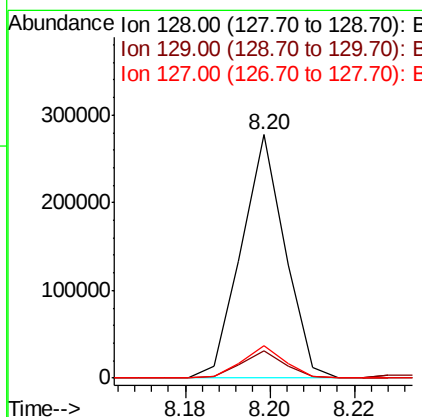







#45
Dimethylphthalate
Concen: 10.310 ng/ul
RT: 9.66 min Scan# 1287
Delta R.T. 0.00 min
Lab File: BP000184.D
Acq: 10 Sep 2019 23:03

Instrument :
BNA_P
ClientSampled :
F2D03

Tot Ion	Ratio	Resp Lower	Upper
163	100		
194	4.3	3.2	4.8
164	9.8	8.4	12.6




Manual Integrations
APPROVED


mohammad
9/12/2019 9:29:59 AM

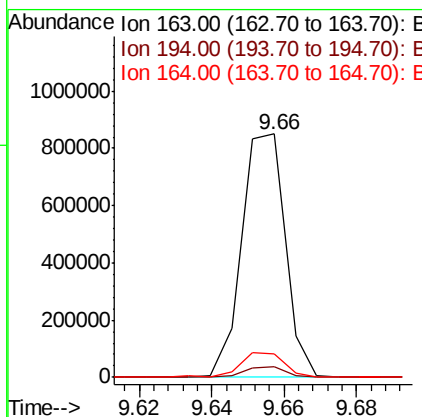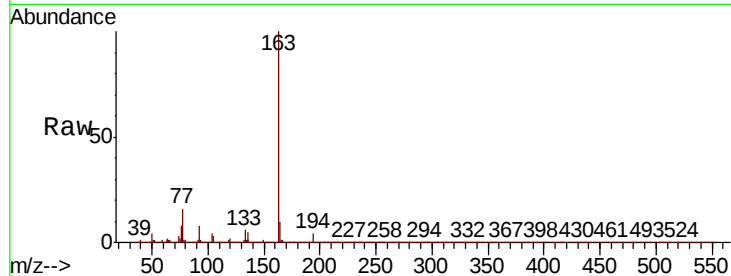

#50
Acenaphthene
Concen: 7.103 ng/ul
RT: 9.97 min Scan# 1341
Delta R.T. -0.01 min
Lab File: BP000184.D
Acq: 10 Sep 2019 23:03

Tgt Ion	Ratio	Resp Lower	Upper
153	100		
152	47.5	38.0	57.0
154	90.4	72.6	108.8

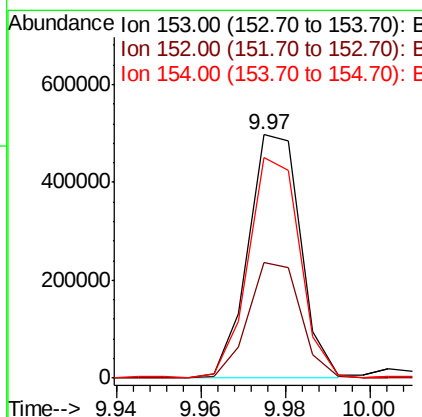







#54
Dibenzofuran
Concen: 1.698 ng/ul
RT: 10.15 min Scan# 1371
Delta R.T. -0.00 min
Lab File: BP000184.D
Acq: 10 Sep 2019 23:03

Instrument :
BNA_P
ClientSampleId :
F2D03

Tot Ion	Ratio	Lower	Upper
168	100		
139	36.1	30.0	45.0




Manual Integrations
APPROVED


mohammad
9/12/2019 9:29:59 AM

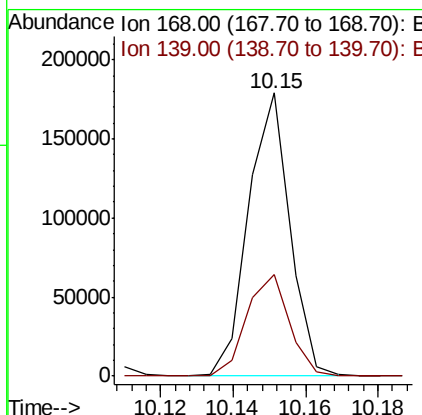

#59
Fluorene
Concen: 3.141 ng/ul
RT: 10.50 min Scan# 1430
Delta R.T. 0.00 min
Lab File: BP000184.D
Acq: 10 Sep 2019 23:03

Tgt Ion	Ratio	Lower	Upper
166	100		
165	96.5	77.8	116.8
167	13.5	10.9	16.3

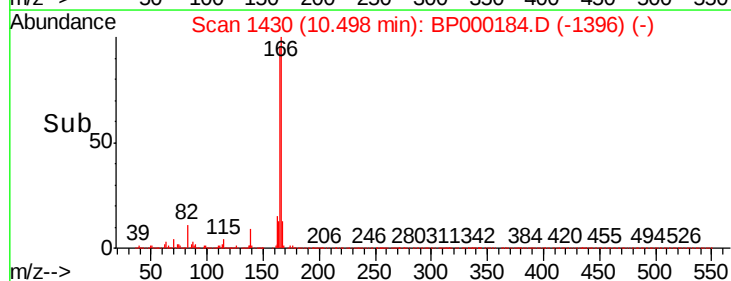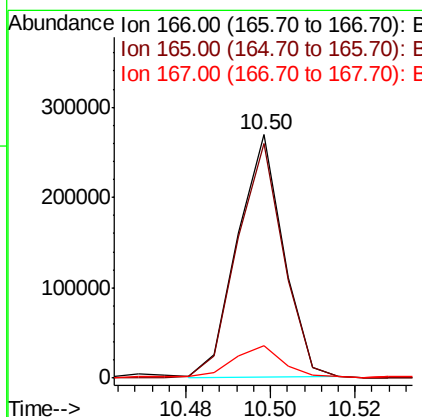







#70
Phenanthrene
Concen: 30.486 ng/ul
RT: 11.47 min Scan# 1596
Delta R.T. 0.00 min
Lab File: BP000184.D
Acq: 10 Sep 2019 23:03

Instrument :
BNA_P
ClientSampleId :
F2D03

Tot Ion	Ratio	Lower	Upper
178	100		
179	16.2	12.5	18.7
176	20.2	15.7	23.5




Manual Integrations
APPROVED


mohammad
9/12/2019 9:29:59 AM

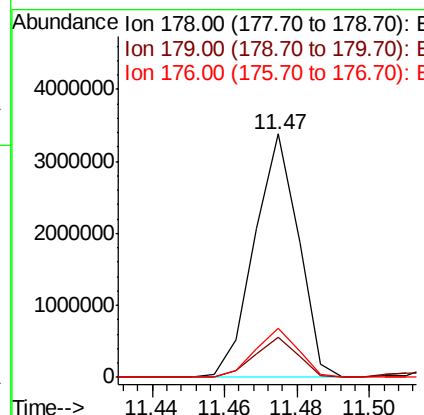

#72
Anthracene
Concen: 6.630 ng/ul
RT: 11.53 min Scan# 1605
Delta R.T. -0.00 min
Lab File: BP000184.D
Acq: 10 Sep 2019 23:03

Tgt Ion	Ratio	Lower	Upper
178	100		
179	15.6	12.3	18.5
176	18.6	15.1	22.7

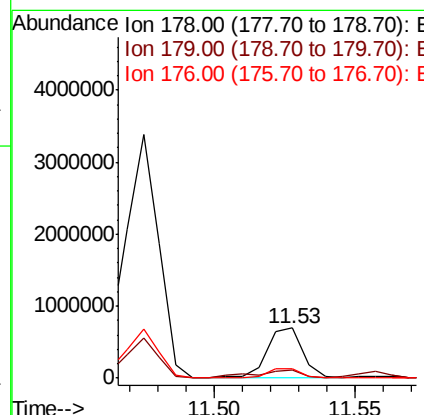







#75
 Carbazole
 Concen: 5.604 ng/ul
 RT: 11.67 min Scan# 1630
 Delta R.T. -0.01 min
 Lab File: BP000184.D
 Acq: 10 Sep 2019 23:03

Instrument :
 BNA_P
 ClientSampleId :
 F2D03

Tot Ion	Ratio	Lower	Upper
167	100		
166	21.4	17.3	25.9
139	13.2	10.6	15.8




Manual Integrations
 APPROVED


mohammad
 9/12/2019 9:29:59 AM

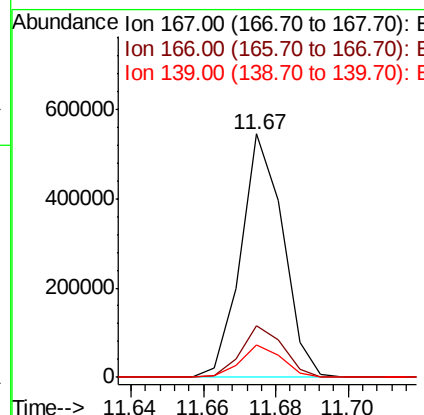

#77
 Fluoranthene
 Concen: 50.656 ng/ul
 RT: 12.69 min Scan# 1803
 Delta R.T. 0.01 min
 Lab File: BP000184.D
 Acq: 10 Sep 2019 23:03

Tgt Ion	Ratio	Lower	Upper
202	100		
101	11.1	10.0	15.0
100	8.4	7.4	11.2

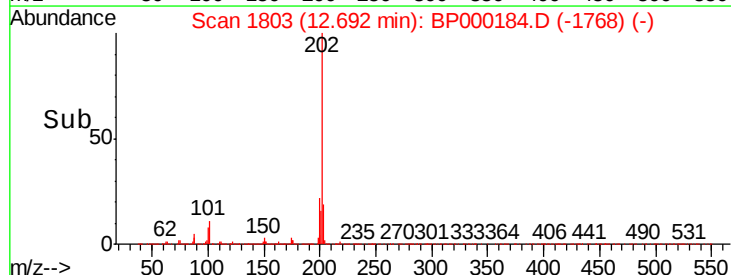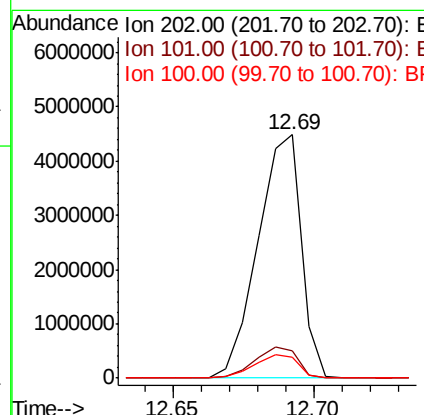







#80
Pvrene
Concen: 54.464 ng/ul
RT: 12.92 min Scan# 1842
Delta R.T. 0.01 min
Lab File: BP000184.D
Acq: 10 Sep 2019 23:03

Instrument :
BNA_P
ClientSampled :
F2D03

Tot Ion	Ratio	Lower	Upper
202	100		
101	14.8	13.4	20.0
100	12.0	10.8	16.2




Manual Integrations
APPROVED


mohammad
9/12/2019 9:29:59 AM

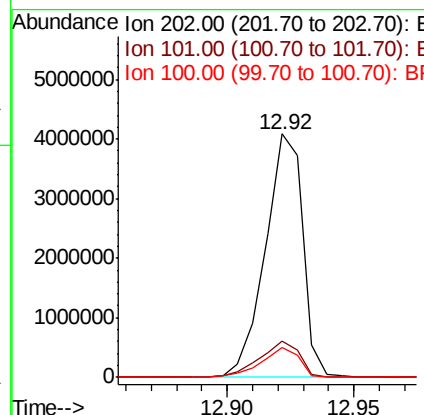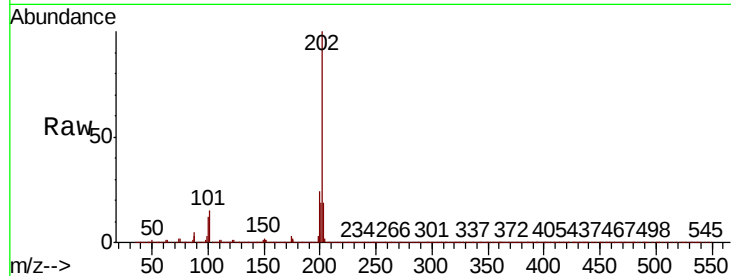

#83
Benzo(a)anthracene
Concen: 37.478 ng/ul
RT: 14.14 min Scan# 2049
Delta R.T. 0.01 min
Lab File: BP000184.D
Acq: 10 Sep 2019 23:03

Tgt Ion	Ratio	Lower	Upper
228	100		
229	22.8	15.9	23.9
226	29.5	22.1	33.1

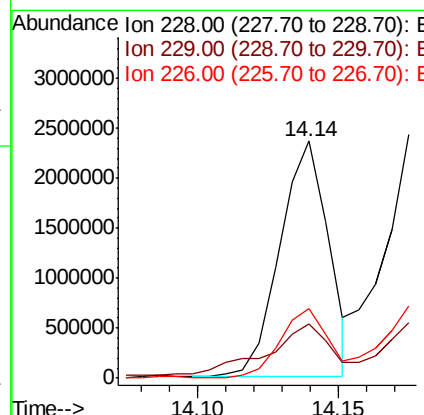







#85
Chrysene
Concen: 44.033 ng/ul
RT: 14.18 min Scan# 2056
Delta R.T. 0.01 min
Lab File: BP000184.D
Acq: 10 Sep 2019 23:03

Instrument :
BNA_P
ClientSampleId :
F2D03

Tot Ion	Ratio	Lower	Upper
228	100		
226	31.2	24.4	36.6
229	21.1	16.0	24.0




Manual Integrations
APPROVED


mohammad
9/12/2019 9:29:59 AM

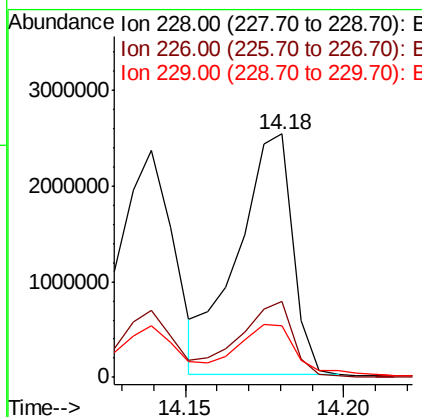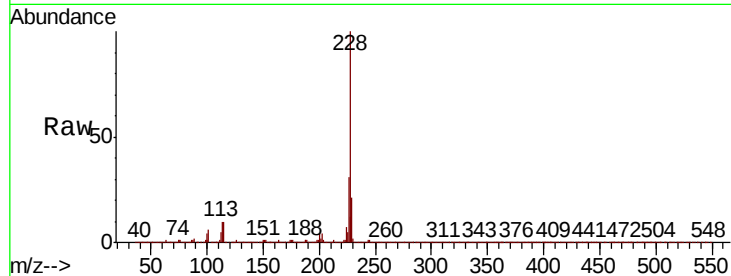

#88
Benzo(b)fluoranthene
Concen: 61.553 ng/ul
RT: 15.25 min Scan# 2238
Delta R.T. 0.02 min
Lab File: BP000184.D
Acq: 10 Sep 2019 23:03

Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.2	17.5	26.3
125	12.8	9.9	14.9

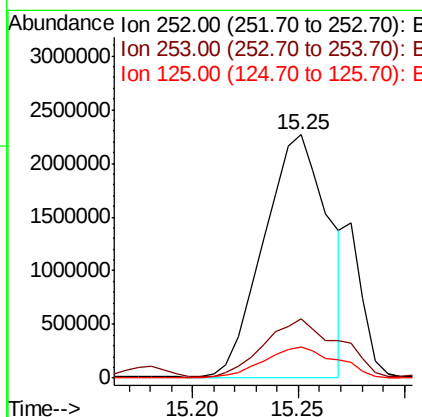







#89
Benzo(k)fluoranthene
Concen: 11.063 ng/ul m
RT: 15.27 min Scan# 2242
Delta R.T. 0.02 min
Lab File: BP000184.D
Acq: 10 Sep 2019 23:03

Instrument :
BNA_P
ClientSampleId :
F2D03

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.2	18.0	27.0
125	10.5	10.2	15.2




Manual Integrations
APPROVED


mohammad
9/12/2019 9:29:59 AM

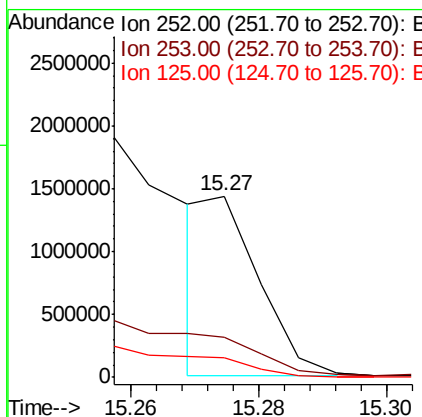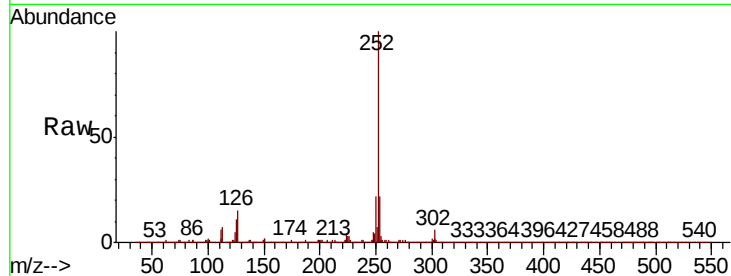

#91
Benzo(a)pyrene
Concen: 42.513 ng/ul
RT: 15.64 min Scan# 2304
Delta R.T. 0.02 min
Lab File: BP000184.D
Acq: 10 Sep 2019 23:03

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.3	17.5	26.3
125	12.1	10.2	15.2

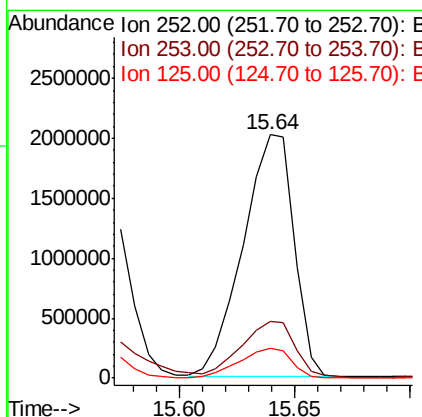







#92
 Indeno(1,2,3-cd)pyrene
 Concen: 27.769 ng/uL
 RT: 17.28 min Scan# 2583
 Delta R.T. 0.03 min
 Lab File: BP000184.D
 Acq: 10 Sep 2019 23:03

Instrument :
 BNA_P
 ClientSampleId :
 F2D03

Tot Ion	Ratio	Lower	Upper
276	100		
138	24.4	20.0	30.0
277	23.7	19.4	29.0




Manual Integrations
 APPROVED


mohammad
 9/12/2019 9:29:59 AM

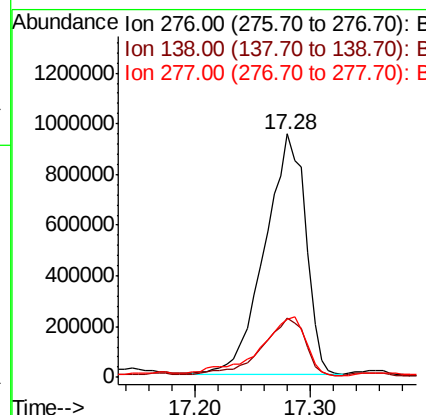

#93
 Dibenzo(a,h)anthracene
 Concen: 8.773 ng/uL
 RT: 17.29 min Scan# 2585
 Delta R.T. 0.02 min
 Lab File: BP000184.D
 Acq: 10 Sep 2019 23:03

Tgt Ion	Ratio	Lower	Upper
278	100		
139	18.2	15.1	22.7
279	25.3	19.2	28.8

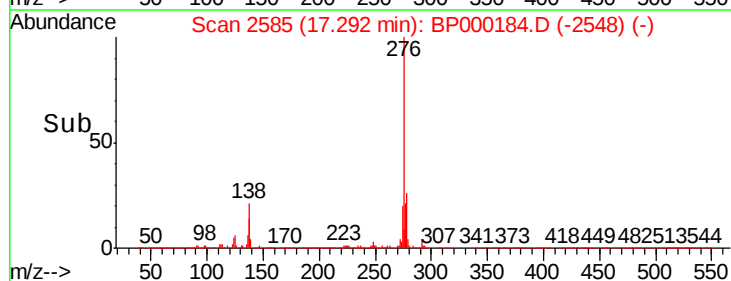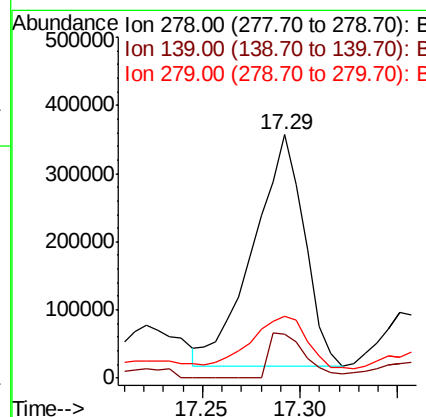



#94
 Benzo(a,h,i)perylene
 Concen: 27.942 ng/ul
 RT: 17.75 min Scan# 2663
 Delta R.T. 0.03 min
 Lab File: BP000184.D
 Acq: 10 Sep 2019 23:03

Instrument :
 BNA_P
 ClientSampleId :
 F2D03

Tot Ion:	276	Resp:	1958345
Ion Ratio	Lower	Upper	
276	100		
138	24.4	20.0	30.0
277	23.2	19.1	28.7

Manual Integrations
 APPROVED

mohammad
 9/12/2019 9:29:59 AM

