

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091019\
 Data File : BP000187.D
 Acq On : 11 Sep 2019 00:16
 Operator : HP/JU
 Sample : K4633-18
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F2D17

Manual Integrations
 APPROVED

mohammad
 9/12/2019 10:25:53 AM

Quant Time: Sep 11 04:26:19 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 11 02:03:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	458670	20.00	ng/ul	0.00
18) Naphthalene-d8	8.18	136	1689255	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.95	164	864941	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.45	188	1473768	20.00	ng/ul	0.00
78) Chrysene-d12	14.15	240	1043166	20.00	ng/ul	0.00
86) Perylene-d12	15.70	264	1157074	20.00	ng/ul	0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.62	96	54157	4.19	ng/uL	0.01
5) Phenol-d5	6.51	99	1011290	25.89	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.58	67	537040	26.29	ng/ul	0.00
9) 2-Chlorophenol-d4	6.66	132	834461	26.41	ng/ul	0.00
13) 4-Methylphenol-d8	7.26	113	743838	25.35	ng/ul	0.00
19) Nitrobenzene-d5	7.45	128	413100	32.21	ng/ul	0.00
22) 2-Nitrophenol-d4	7.78	143	437864	35.06	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	8.02	165	736948	27.80	ng/ul	0.00
29) 4-Chloroaniline-d4	8.23	131	305029	9.31	ng/ul	0.00
44) Dimethylphthalate-d6	9.63	166	1910673	29.92	ng/ul	0.00
47) Acenaphthylene-d8	9.79	160	2267807	28.73	ng/ul	0.00
52) 4-Nitrophenol-d4	10.03	143	283209	24.82	ng/ul	0.00
58) Fluorene-d10	10.47	176	1500945	27.67	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.53	200	117130	17.29	ng/ul	0.00
71) Anthracene-d10	11.50	188	1972031	27.63	ng/ul	0.00
79) Pyrene-d10	12.90	212	1880053	30.30	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.60	264	1746169	29.11	ng/ul	0.01

Target Compounds

					Ovalue	
6) Phenol	6.52	94	183412	4.505	ng/ul	95
45) Dimethylphthalate	9.66	163	656397	10.185	ng/ul	99
70) Phenanthrene	11.47	178	347428	3.986	ng/ul	99
77) Fluoranthene	12.68	202	942335	10.720	ng/ul	99
80) Pyrene	12.92	202	824735	10.479	ng/ul	97
83) Benzo(a)anthracene	14.13	228	476372	6.309	ng/ul	97
85) Chrysene	14.17	228	468433	6.760	ng/ul	97
88) Benzo(b)fluoranthene	15.23	252	781031	10.184	ng/ul	97
89) Benzo(k)fluoranthene	15.26	252	248236m	3.434	ng/ul	
91) Benzo(a)pyrene	15.63	252	474256	6.591	ng/ul	98
92) Indeno(1,2,3-cd)pyrene	17.26	276	351562	4.247	ng/ul	99
93) Dibenzo(a,h)anthracene	17.27	278	92452	1.348	ng/ul#	90
94) Benzo(g,h,i)perylene	17.73	276	305148	4.421	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091019\
Data File : BP000187.D
Acq On : 11 Sep 2019 00:16
Operator : HP/JU
Sample : K4633-18
Misc :
ALS Vial : 23 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
F2D17

Manual Integrations
APPROVED

mohammad
9/12/2019 10:25:53 AM

Quant Time: Sep 11 04:26:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 11 02:03:45 2019
Response via : Initial Calibration

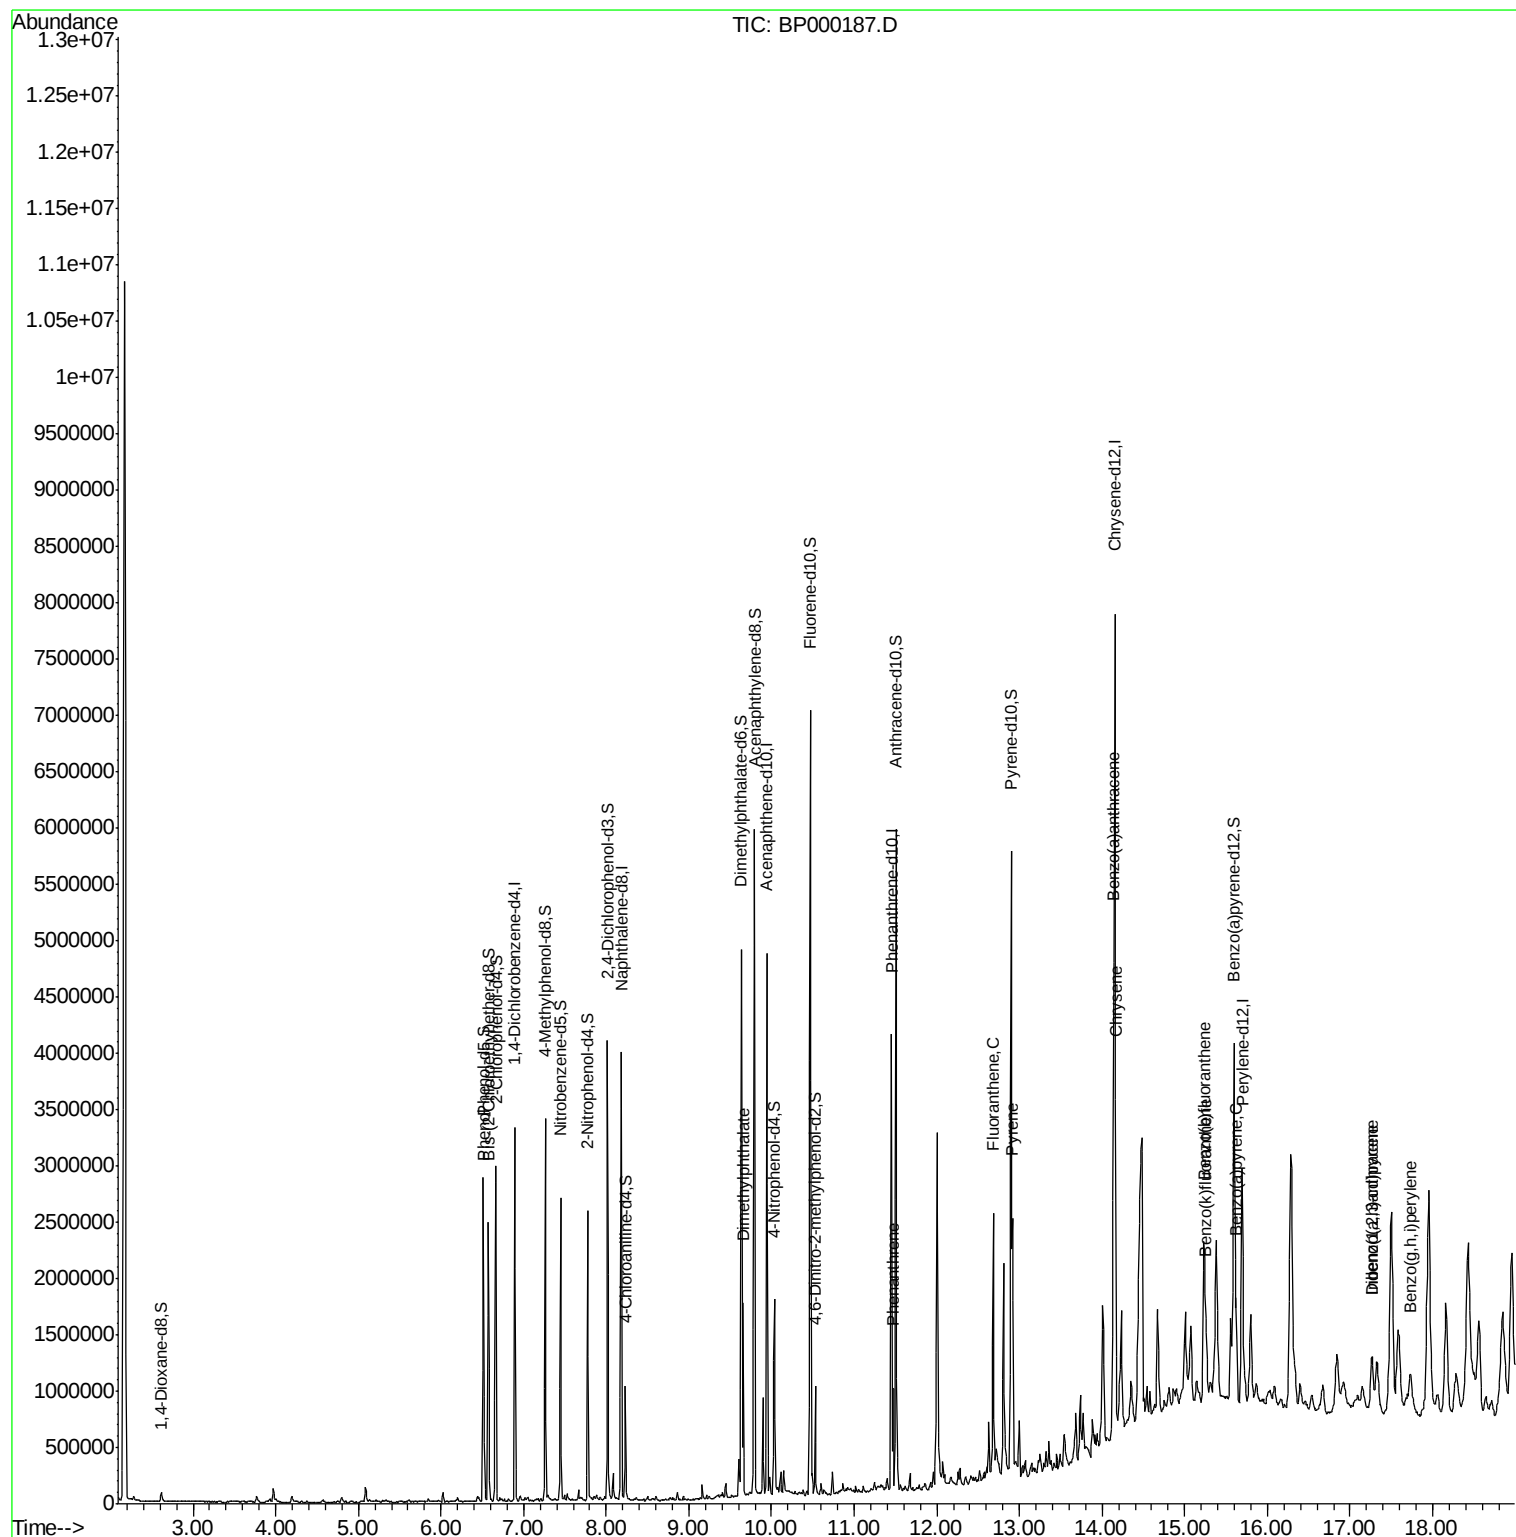

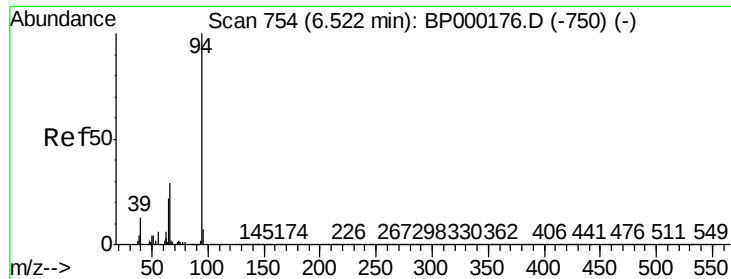

#6

Phenol

Concen: 4.505 ng/ul

RT: 6.52 min Scan# 754

Delta R.T. 0.00 min

Lab File: BP000187.D

Acq: 11 Sep 2019 00:16

Instrument :

BNA_P





ClientSampleId :

F2D17

Tot Ion:	94	Resp:	183412
Ion Ratio	Lower	Upper	
94	100		
65	24.8	18.8	28.2
66	34.1	24.2	36.2

Manual Integrations
APPROVED

mohammad
9/12/2019 10:25:53 AM

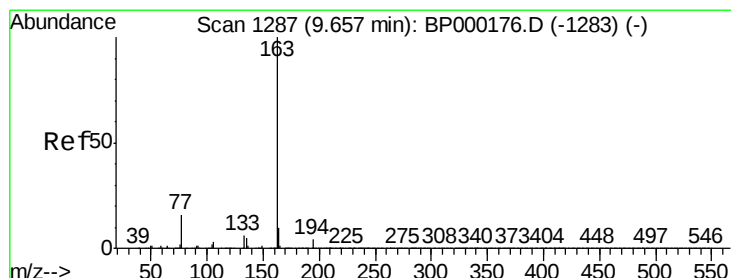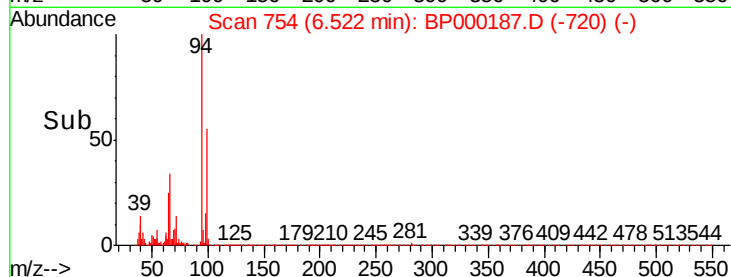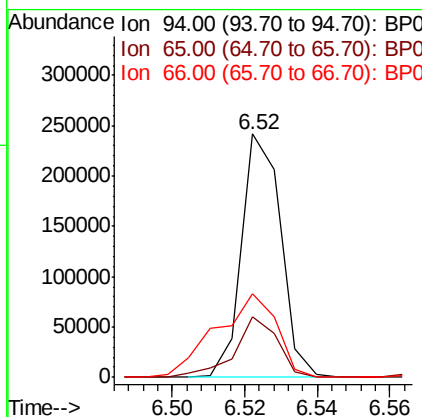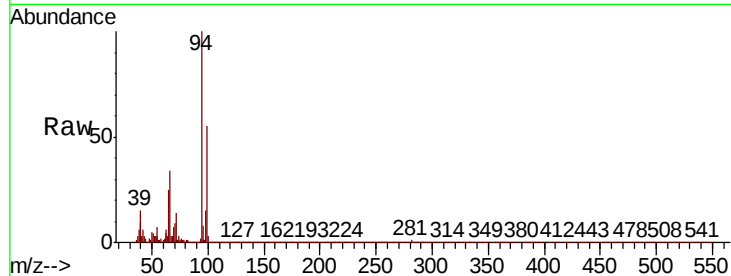

#45

Dimethylphthalate

Concen: 10.185 ng/ul




RT: 9.66 min Scan# 1287


Delta R.T. 0.00 min

Lab File: BP000187.D

Acq: 11 Sep 2019 00:16

Tgt Ion:	163	Resp:	656397
Ion Ratio	Lower	Upper	
163	100		
194	4.2	3.2	4.8
164	9.9	8.4	12.6

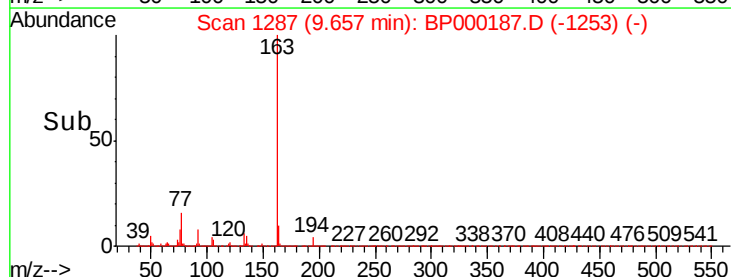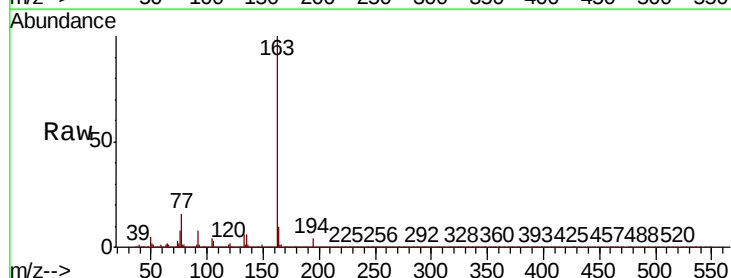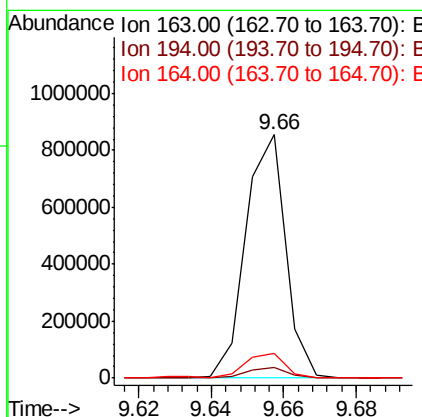

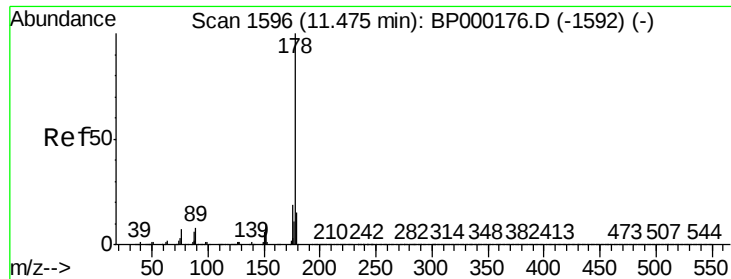





#70
Phenanthrene
Concen: 3.986 ng/ul
RT: 11.47 min Scan# 1596
Delta R.T. 0.00 min
Lab File: BP000187.D
Acq: 11 Sep 2019 00:16

Instrument :
BNA_P
ClientSampleId :
F2D17

Tot Ion	Ratio	Lower	Upper
178	100		
179	15.4	12.5	18.7
176	19.0	15.7	23.5




Manual Integrations
APPROVED


mohammad
9/12/2019 10:25:53 AM

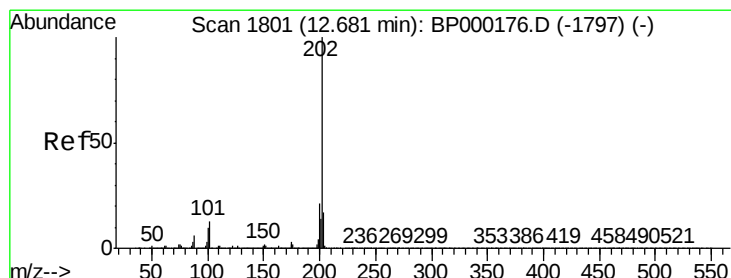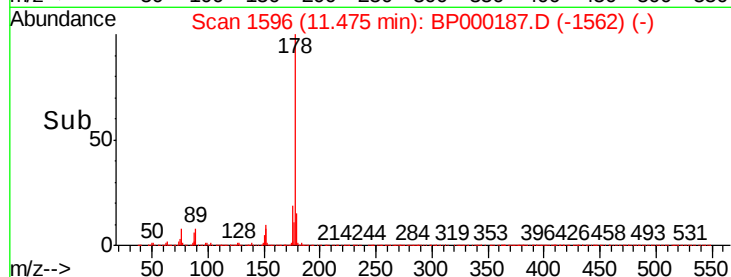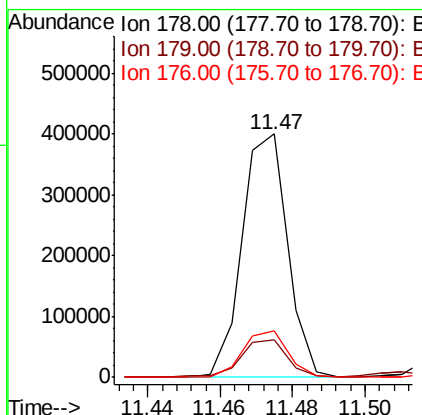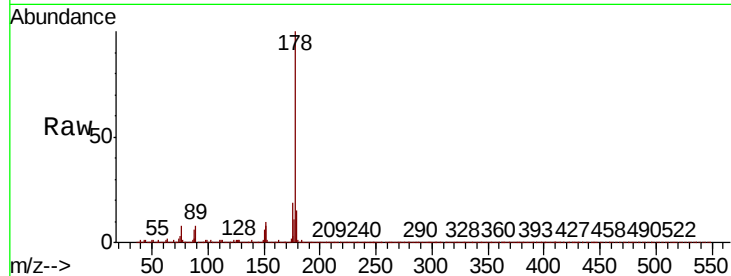

#77
Fluoranthene
Concen: 10.720 ng/ul
RT: 12.68 min Scan# 1801
Delta R.T. -0.01 min
Lab File: BP000187.D
Acq: 11 Sep 2019 00:16

Tgt Ion	Ratio	Lower	Upper
202	100		
101	12.9	10.0	15.0
100	9.7	7.4	11.2

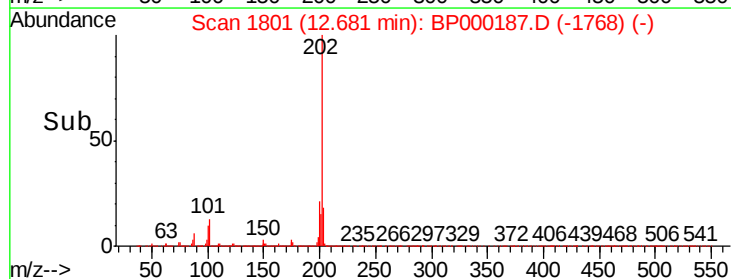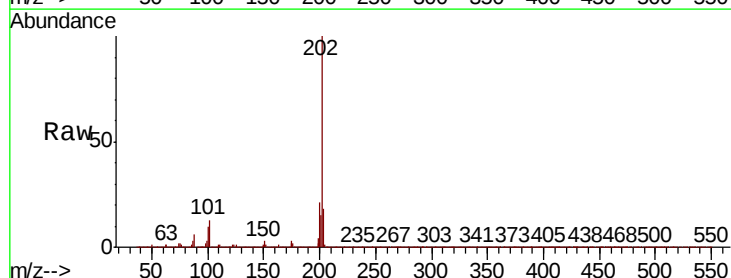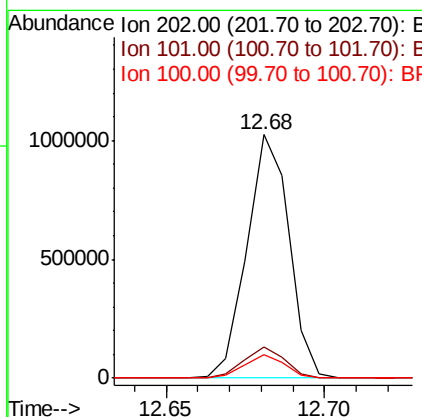

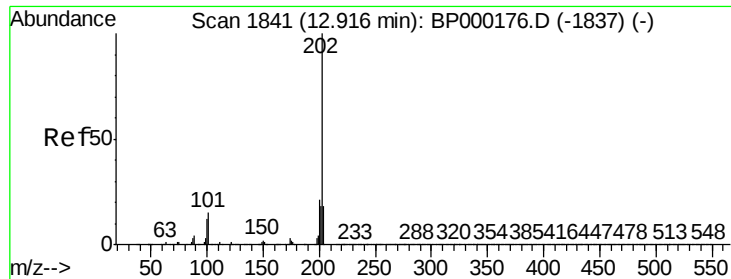





#80
Pvrene
Concen: 10.479 ng/ul
RT: 12.92 min Scan# 1841
Delta R.T. 0.00 min
Lab File: BP000187.D
Acq: 11 Sep 2019 00:16

Instrument :
BNA_P
ClientSampleId :
F2D17

Tot Ion	Ratio	Resp	Lower	Upper
202	100	824735		
101	15.4		13.4	20.0
100	12.4		10.8	16.2




Manual Integrations
APPROVED


mohammad
9/12/2019 10:25:53 AM

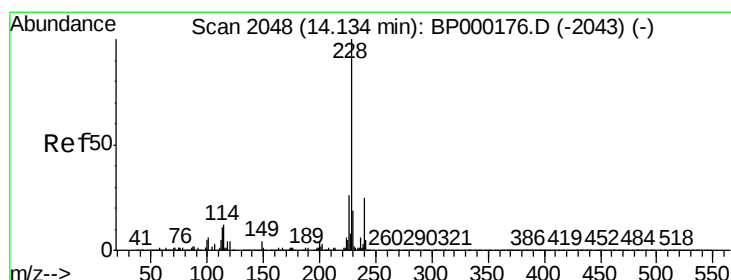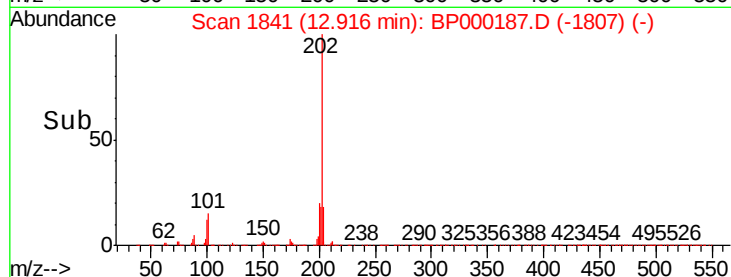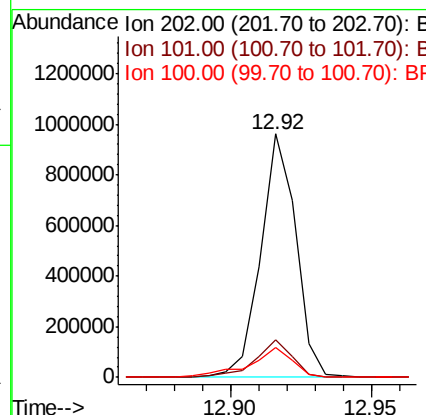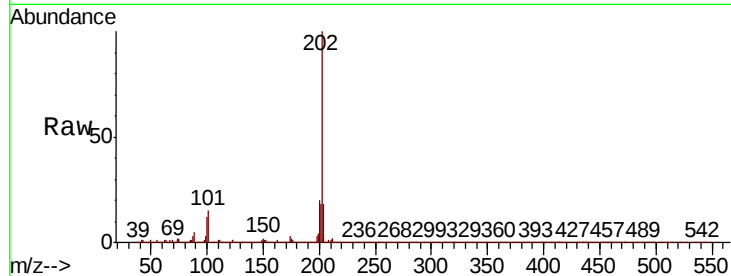

#83
Benzo(a)anthracene
Concen: 6.309 ng/ul
RT: 14.13 min Scan# 2048
Delta R.T. 0.00 min
Lab File: BP000187.D
Acq: 11 Sep 2019 00:16

Tgt Ion	Ratio	Resp	Lower	Upper
228	100	476372		
229	20.7		15.9	23.9
226	29.8		22.1	33.1

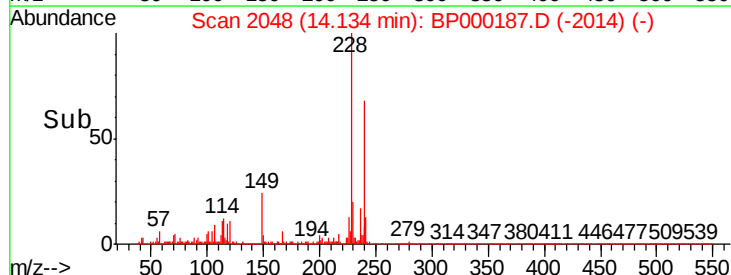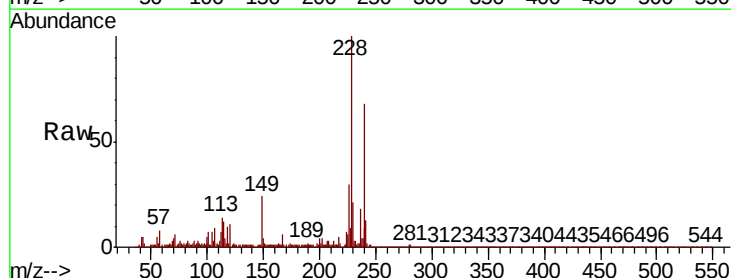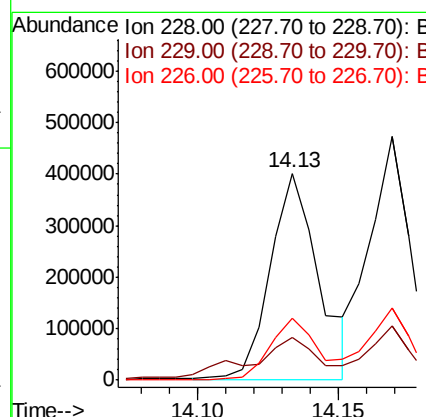

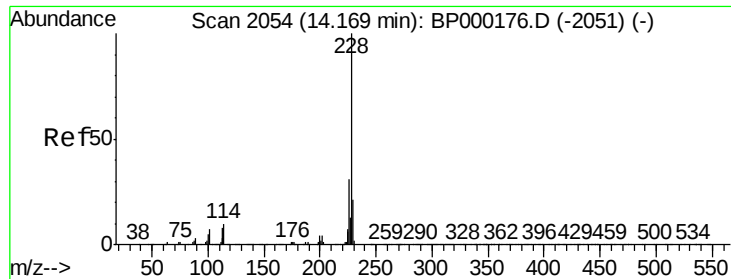





#85
Chrysene
Concen: 6.760 ng/ul
RT: 14.17 min Scan# 2054
Delta R.T. 0.00 min
Lab File: BP000187.D
Acq: 11 Sep 2019 00:16

Instrument :
BNA_P
ClientSampleId :
F2D17

Tot Ion	Ratio	Lower	Upper
228	100		
226	29.7	24.4	36.6
229	22.0	16.0	24.0




Manual Integrations
APPROVED


mohammad
9/12/2019 10:25:53 AM

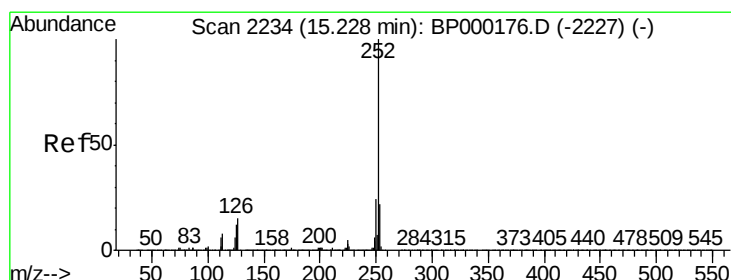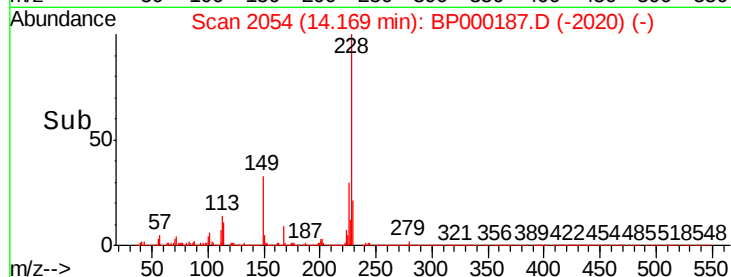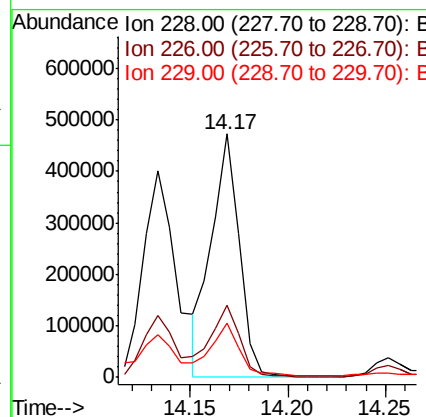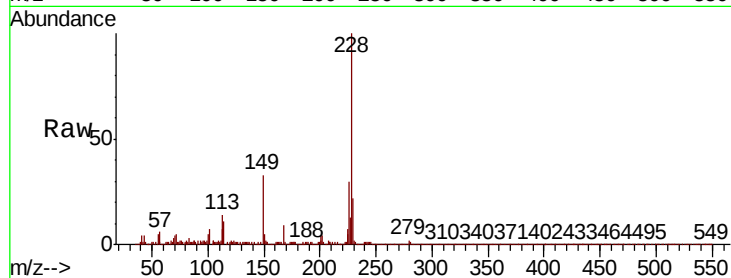

#88
Benzo(b)fluoranthene
Concen: 10.184 ng/ul
RT: 15.23 min Scan# 2235
Delta R.T. 0.01 min
Lab File: BP000187.D
Acq: 11 Sep 2019 00:16

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.4	17.5	26.3
125	13.5	9.9	14.9

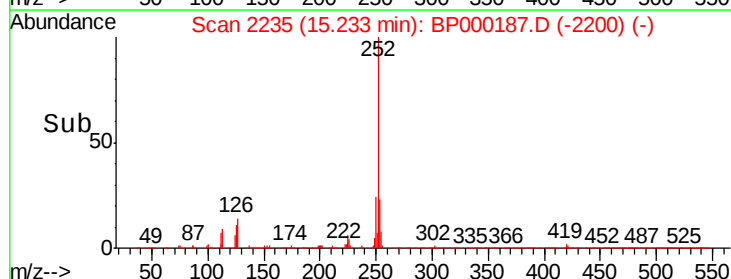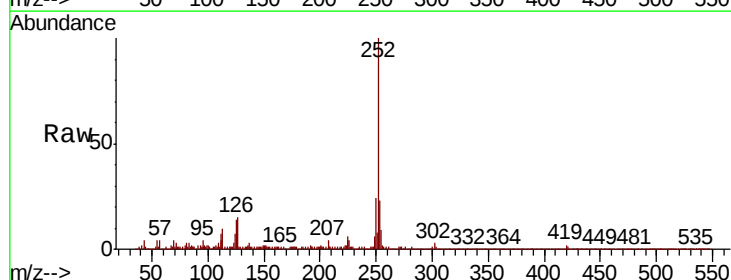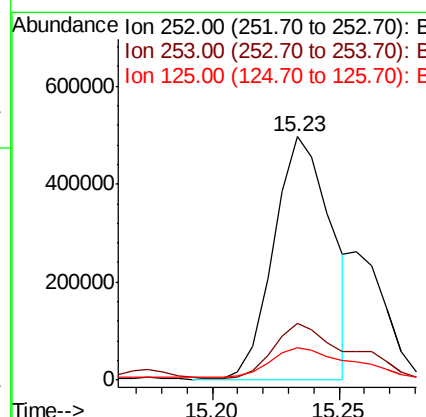

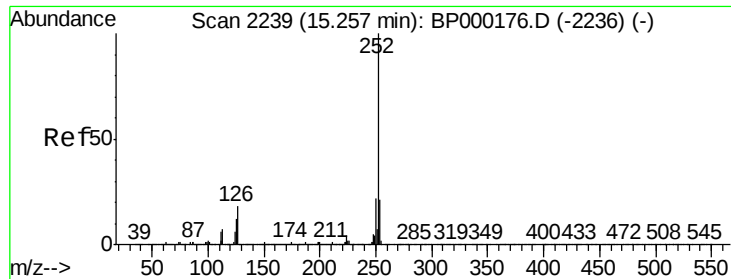





#89
Benzo(k)fluoranthene
Concen: 3.434 ng/ul m
RT: 15.26 min Scan# 2239
Delta R.T. 0.00 min
Lab File: BP000187.D
Acq: 11 Sep 2019 00:16

Instrument :
BNA_P
ClientSampleId :
F2D17

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.7	18.0	27.0
125	14.6	10.2	15.2




Manual Integrations
APPROVED


mohammad
9/12/2019 10:25:53 AM

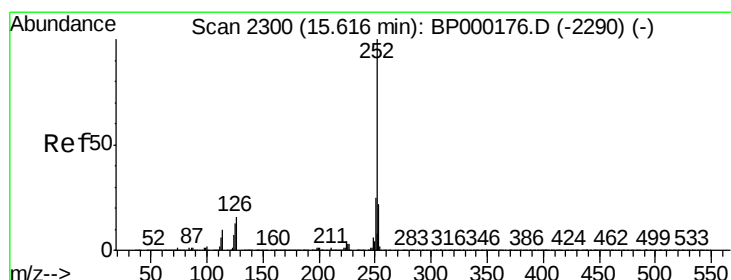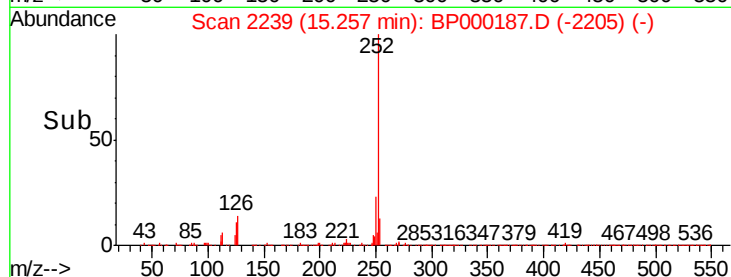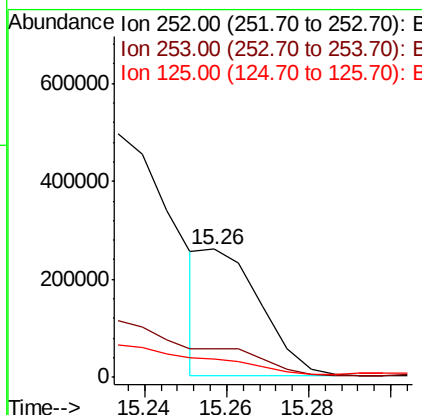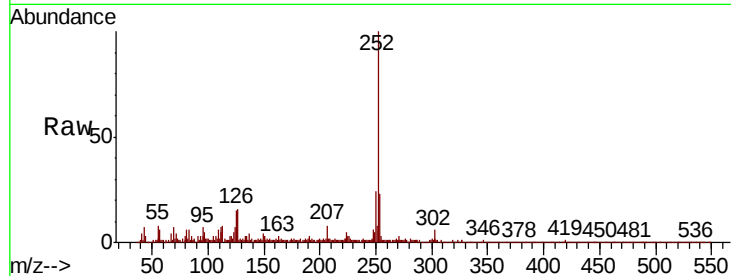

#91
Benzo(a)pyrene
Concen: 6.591 ng/ul
RT: 15.63 min Scan# 2302
Delta R.T. 0.01 min
Lab File: BP000187.D
Acq: 11 Sep 2019 00:16

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.8	17.5	26.3
125	12.1	10.2	15.2

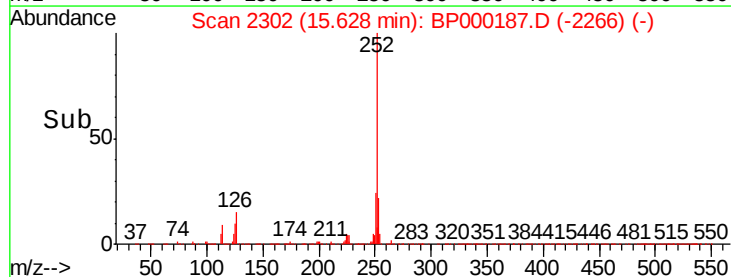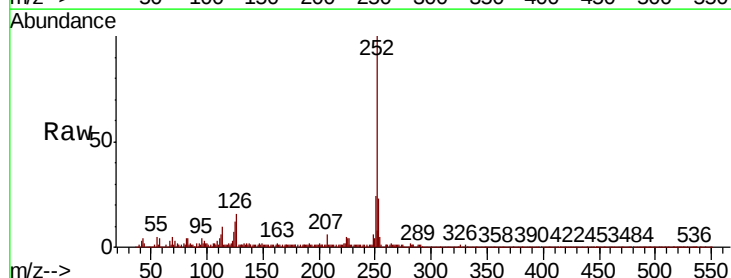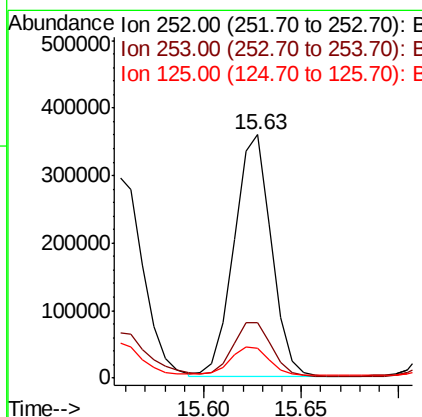

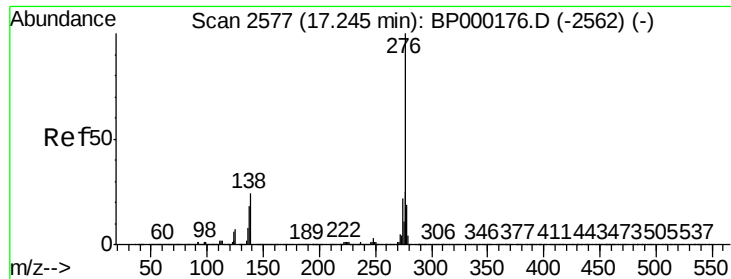


#92
Indeno(1,2,3-cd)pyrene
Concen: 4.247 ng/ul
RT: 17.26 min Scan# 2580
Delta R.T. 0.01 min
Lab File: BP000187.D
Acq: 11 Sep 2019 00:16

Instrument :
BNA_P
ClientSampleId :
F2D17

Tot Ion	Ratio	Lower	Upper
276	100		
138	24.4	20.0	30.0
277	24.4	19.4	29.0

Manual Integrations
APPROVED

mohammad
9/12/2019 10:25:53 AM



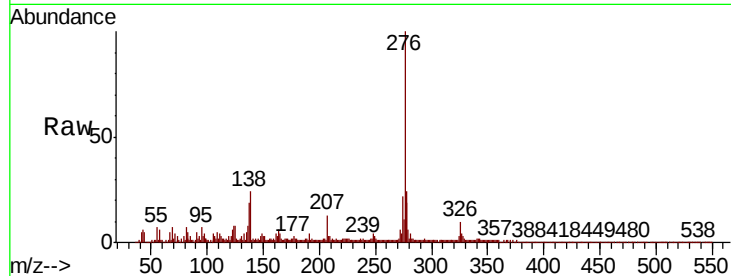


Abundance

Ion 276.00 (275.70 to 276.70): E


Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

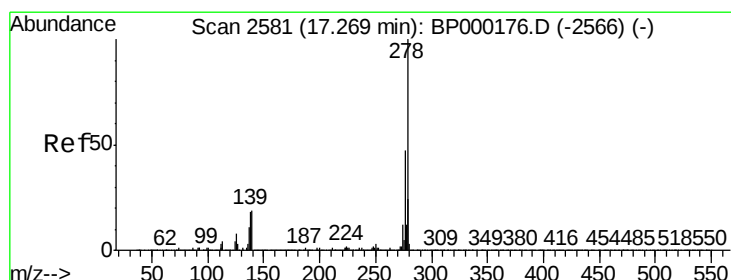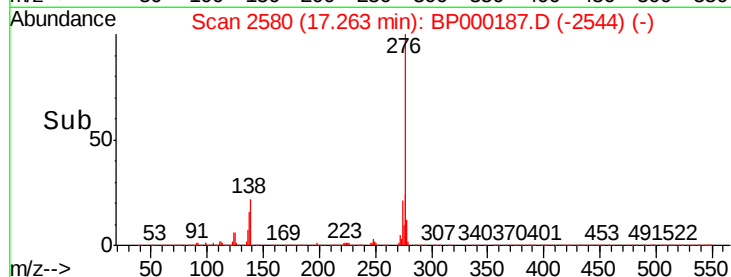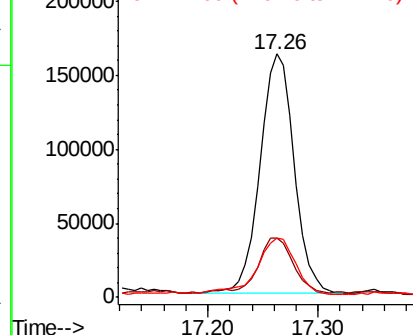

#93
Dibenzo(a,h)anthracene
Concen: 1.348 ng/ul
RT: 17.27 min Scan# 2582
Delta R.T. 0.00 min
Lab File: BP000187.D
Acq: 11 Sep 2019 00:16

Tgt Ion	Ratio	Lower	Upper
278	100		
139	20.7	15.1	22.7
279	30.8	19.2	28.8#


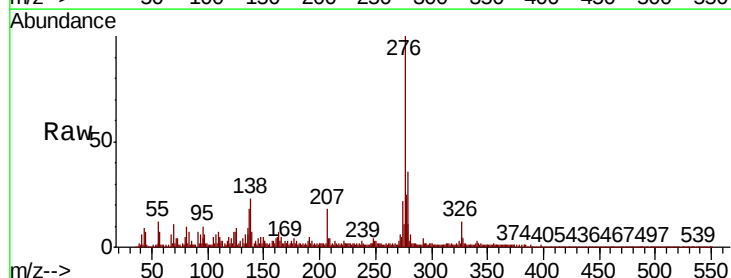



Abundance

Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

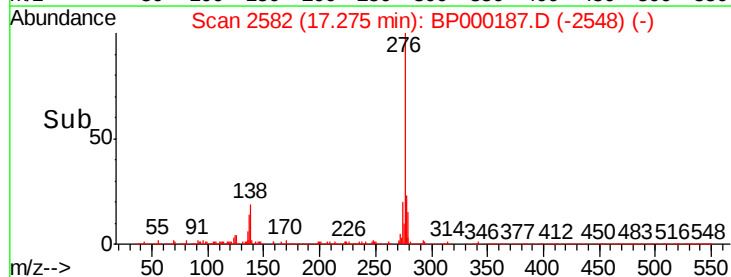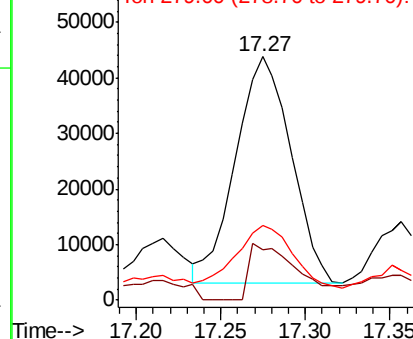

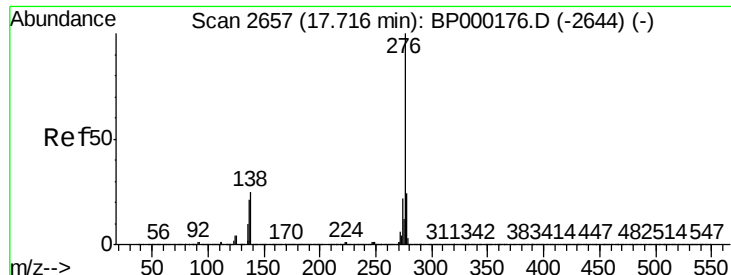

#94
 Benzo(a,h,i)perylene
 Concen: 4.421 ng/ul
 RT: 17.73 min Scan# 2660
 Delta R.T. 0.01 min
 Lab File: BP000187.D
 Acq: 11 Sep 2019 00:16

Instrument :
 BNA_P
 ClientSampleId :
 F2D17

Tot Ion:	276	Resp:	305148
Ion Ratio	Lower	Upper	
276	100		
138	23.9	20.0	30.0
277	24.9	19.1	28.7

Manual Integrations
 APPROVED

mohammad
 9/12/2019 10:25:53 AM

