

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091023\
 Data File : BP017089.D
 Acq On : 11 Sep 2023 04:46
 Operator : MA/JU
 Sample : SSTD08047
 Misc :
 ALS Vial : 105 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD080607

Quant Time: Sep 11 05:47:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 11 05:32:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.963	152	319900	20.000	ng/u1	0.00
20) Naphthalene-d8	10.787	136	1435973	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.622	164	880939	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.392	188	1873229	20.000	ng/u1	0.00
79) Chrysene-d12	21.492	240	1616037	20.000	ng/u1	0.00
88) Perylene-d12	24.021	264	1352290	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.317	96	277687	32.834	ng/uL	0.00
4) Pyridine-d5	3.752	84	2193620	90.776	ng/u1	0.00
7) Phenol-d5	7.116	99	2604754	89.125	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.305	67	1672405	91.483	ng/u1	0.00
11) 2-Chlorophenol-d4	7.487	132	1944158	91.913	ng/u1	0.00
15) 4-Methylphenol-d8	8.681	113	2053568	92.231	ng/u1	0.01
21) Nitrobenzene-d5	9.163	128	980084	87.976	ng/u1	0.00
24) 2-Nitrophenol-d4	9.881	143	1074255	88.955	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.405	165	1912532	85.782	ng/u1	0.00
31) 4-Chloroaniline-d4	10.952	131	2843342	88.395	ng/u1	0.00
46) Dimethylphthalate-d6	14.040	166	5598110	85.370	ng/u1	0.00
49) Acenaphthylene-d8	14.322	160	6598100	87.187	ng/u1	0.00
54) 4-Nitrophenol-d4	14.851	143	1176415	91.842	ng/u1	0.02
60) Fluorene-d10	15.622	176	4751914	84.637	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	1018112	90.314	ng/u1	0.01
73) Anthracene-d10	17.492	188	7301248	84.872	ng/u1	0.00
81) Pyrene-d10	19.728	212	8140969	82.706	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.857	264	6224697	90.733	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.352	88	301322	32.999	ng/uL	98
5) Pyridine	3.770	79	2295007	89.212	ng/u1	98
6) Benzaldehyde	7.122	77	1231034	92.935	ng/u1	96
8) Phenol	7.146	94	2734046	90.040	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.399	93	2123140	87.680	ng/u1	99
12) 2-Chlorophenol	7.516	128	1972678	87.541	ng/u1	99
13) 2-Methylphenol	8.405	108	1989569	89.326	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.475	45	1964195	57.613	ng/u1	100
16) Acetophenone	8.822	105	3233651	89.999	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.805	70	1804255	94.003	ng/u1	97
18) 4-Methylphenol	8.752	108	2147370	88.404	ng/u1	99
19) Hexachloroethane	9.028	117	809839	86.752	ng/u1	97
22) Nitrobenzene	9.210	77	2602485	87.489	ng/u1	98
23) Isophorone	9.734	82	4940371	88.402	ng/u1	98
25) 2-Nitrophenol	9.910	139	1151842	86.631	ng/u1	96
26) 2,4-Dimethylphenol	9.952	107	2261638	83.309	ng/u1	99
27) Bis(2-Chloroethoxy)met...	10.210	93	2889647	83.434	ng/u1	99
29) 2,4-Dichlorophenol	10.434	162	1896442	83.465	ng/u1	98
30) Naphthalene	10.840	128	6338040	80.888	ng/u1	99
32) 4-Chloroaniline	10.981	127	2798138	83.587	ng/u1	100
33) Hexachlorobutadiene	11.069	225	1027318	75.646	ng/u1	98
34) Caprolactam	11.834	113	398041	52.896	ng/u1	96
35) 4-Chloro-3-methylphenol	12.087	107	2169478	87.130	ng/u1	99
36) 2-Methylnaphthalene	12.446	142	4385387	84.691	ng/u1	99


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091023\
 Data File : BP017089.D
 Acq On : 11 Sep 2023 04:46
 Operator : MA/JU
 Sample : SSTD08047
 Misc :
 ALS Vial : 105 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD080607

Quant Time: Sep 11 05:47:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 11 05:32:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.663	142	4427556	84.928	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.799	216	2057405	79.268	ng/ul	99
40) Hexachlorocyclopentadiene	12.746	237	1253825	74.556	ng/ul	100
41) 2,4,6-Trichlorophenol	13.051	196	1472493	83.354	ng/ul	100
42) 2,4,5-Trichlorophenol	13.122	196	1584331	82.427	ng/ul	99
43) 1,1'-Biphenyl	13.457	154	5638678	80.862	ng/ul	99
44) 2-Chloronaphthalene	13.504	162	4460581	81.472	ng/ul	99
45) 2-Nitroaniline	13.746	65	1605693	98.478	ng/ul	94
47) Dimethylphthalate	14.087	163	5612669	81.574	ng/ul	99
48) 2,6-Dinitrotoluene	14.234	165	1188375	88.936	ng/ul	95
50) Acenaphthylene	14.351	152	7441331	87.816	ng/ul	97
51) 3-Nitroaniline	14.575	138	1132948	84.959	ng/ul	92
52) Acenaphthene	14.687	153	4909917	83.047	ng/ul	99
53) 2,4-Dinitrophenol	14.769	184	740961	89.436	ng/ul	94
55) 4-Nitrophenol	14.869	109	941338	91.821	ng/ul	96
56) Dibenzofuran	15.028	168	6582351	80.971	ng/ul	100
57) 2,4-Dinitrotoluene	15.016	165	1807103	94.214	ng/ul	85
58) 2,3,4,6-Tetrachlorophenol	15.240	232	1264467	81.594	ng/ul	96
59) Diethylphthalate	15.445	149	5778757	84.047	ng/ul	99
61) Fluorene	15.681	166	5562183	82.990	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.669	204	2684637	82.885	ng/ul	95
63) 4-Nitroaniline	15.751	138	1069205	91.194	ng/ul	94
66) 4,6-Dinitro-2-methylph...	15.775	198	1092191	92.476	ng/ul#	86
67) N-Nitrosodiphenylamine	15.892	169	4607805	81.577	ng/ul	99
68) 4-Bromophenyl-phenylether	16.569	248	1497703	80.364	ng/ul	98
69) Hexachlorobenzene	16.651	284	1599891	78.315	ng/ul	94
70) Atrazine	16.851	200	1564768	80.912	ng/ul	97
71) Pentachlorophenol	17.016	266	1105713	82.999	ng/ul	98
72) Phenanthrene	17.439	178	8538435	82.030	ng/ul	99
74) Anthracene	17.528	178	8673796	82.895	ng/ul	97
75) 1,2,3,4-Tetrachloroben...	13.410	216	2191391	82.126	ng/uL	100
76) Pentachlorobenzene	14.916	250	1852429	72.072	ng/uL	98
77) Carbazole	17.816	167	8018668	85.278	ng/ul	99
78) Di-n-butylphthalate	18.322	149	9757896	84.707	ng/ul	99
80) Fluoranthene	19.398	202	9642044	78.451	ng/ul	96
82) Pyrene	19.757	202	9876263	77.394	ng/ul	96
83) Butylbenzylphthalate	20.616	149	4673717	88.561	ng/ul	94
84) 3,3'-Dichlorobenzidine	21.416	252	2844054	79.300	ng/ul	99
85) Benzo(a)anthracene	21.475	228	9506045	83.522	ng/ul	96
86) Bis(2-ethylhexyl)phtha...	21.351	149	6487989	88.990	ng/ul#	95
87) Chrysene	21.533	228	8626994	81.031	ng/ul	95
89) Di-n-octyl phthalate	22.316	149	10731008	94.663	ng/ul	100
90) Benzo(b)fluoranthene	23.239	252	8079789	85.517	ng/ul	99
91) Benzo(k)fluoranthene	23.292	252	8058392	88.076	ng/ul	99
93) Benzo(a)pyrene	23.916	252	7248789	91.985	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.715	276	6918551	79.090	ng/ul	99
95) Dibenzo(a,h)anthracene	26.739	278	5818038	80.582	ng/ul	99
96) Benzo(g,h,i)perylene	27.557	276	5093911	73.894	ng/ul	99





(#) = qualifier out of range (m) = manual integration (+) = signals summed

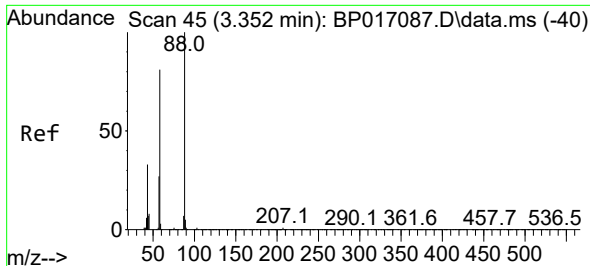

#2
1,4-Dioxane
Concen: 32.999 ng/uL
RT: 3.352 min Scan# 41
Delta R.T. 0.000 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion: 88 Resp: 301322
Ion Ratio Lower Upper
88 100
43 32.7 27.3 40.9
58 78.5 63.7 95.5

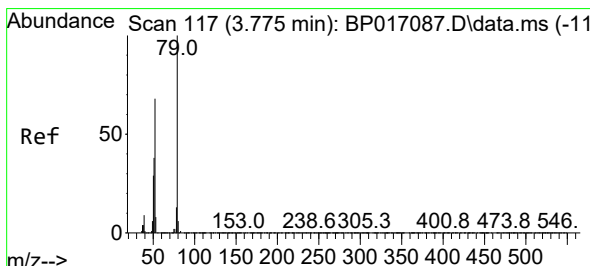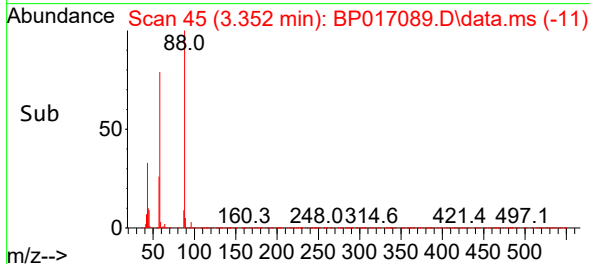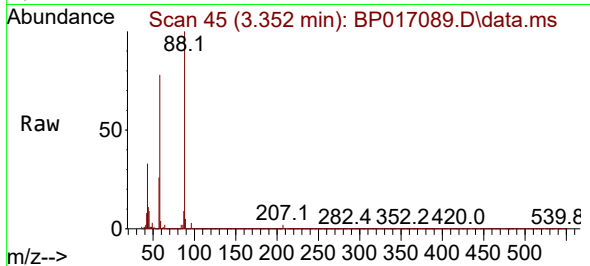

#5
Pyridine
Concen: 89.212 ng/uL
RT: 3.770 min Scan# 116
Delta R.T. -0.006 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion: 79 Resp: 2295007
Ion Ratio Lower Upper
79 100
52 78.6 61.6 92.4
51 37.6 30.9 46.3


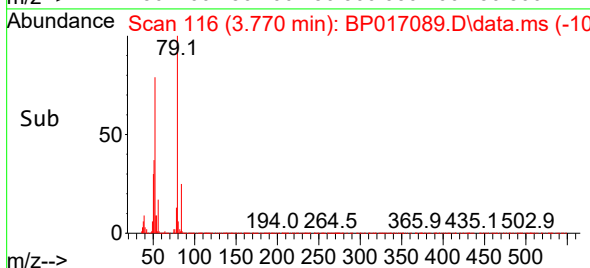
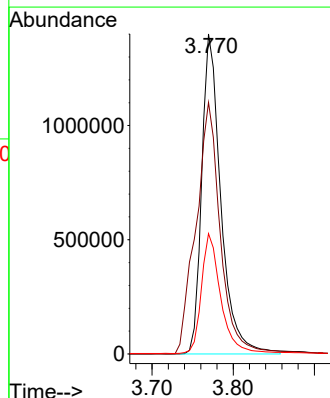
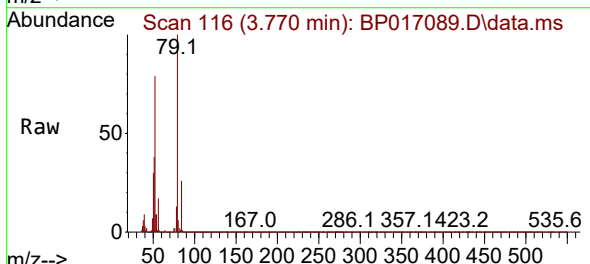




#6
Benzaldehyde
Concen: 92.935 ng/ul
RT: 7.122 min Scan# 61
Delta R.T. 0.006 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion: 77 Resp: 1231034
Ion Ratio Lower Upper
77 100
105 93.3 70.3 105.5
106 89.2 69.0 103.6



#8
Phenol
Concen: 90.040 ng/ul
RT: 7.146 min Scan# 690
Delta R.T. 0.006 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion: 94 Resp: 2734046
Ion Ratio Lower Upper
94 100
65 29.9 25.4 38.0
66 37.7 30.6 46.0









#10
Bis(2-Chloroethyl)ether
Concen: 87.680 ng/ul
RT: 7.399 min Scan# 710
Delta R.T. 0.006 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion: 93 Resp: 2123140
Ion Ratio Lower Upper
93 100
63 81.1 65.4 98.0
95 32.1 25.1 37.7



#12
2-Chlorophenol
Concen: 87.541 ng/ul
RT: 7.516 min Scan# 753
Delta R.T. 0.000 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion:128 Resp: 1972678
Ion Ratio Lower Upper
128 100
64 53.3 42.2 63.4
130 32.8 25.3 37.9





#13

2-Methylphenol

Concen: 89.326 ng/ul

RT: 8.405 min Scan# 904

Delta R.T. 0.006 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46

Instrument :

BNA_P

ClientSampleId :





SSTD080607

Tgt Ion:108 Resp: 1989569

Ion Ratio Lower Upper

108 100

107 89.3 72.3 108.5



#14

2,2'-oxybis(1-Chloropropane)

Concen: 57.613 ng/ul

RT: 8.475 min Scan# 916

Delta R.T. 0.000 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46




Tgt Ion: 45 Resp: 1964195


Ion Ratio Lower Upper

45 100

77 13.7 11.0 16.4

79 9.8 7.8 11.6









#16
Acetophenone
Concen: 89.999 ng/ul
RT: 8.822 min Scan# 91
Delta R.T. 0.012 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion:105 Resp: 3233651
Ion Ratio Lower Upper
105 100
77 82.1 67.0 100.4
51 30.0 25.4 38.0



#17
N-Nitroso-di-n-propylamine
Concen: 94.003 ng/ul
RT: 8.805 min Scan# 972
Delta R.T. 0.024 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion: 70 Resp: 1804255
Ion Ratio Lower Upper
70 100
42 60.9 50.9 76.3
101 9.3 6.7 10.1
130 19.6 14.8 22.2



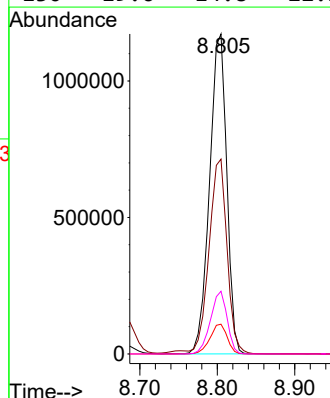





#18
4-Methylphenol
Concen: 88.404 ng/ul
RT: 8.752 min Scan# 960
Delta R.T. 0.018 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion:108 Resp: 2147370
Ion Ratio Lower Upper
108 100
107 111.5 90.2 135.4



#19
Hexachloroethane
Concen: 86.752 ng/ul
RT: 9.028 min Scan# 1010
Delta R.T. 0.000 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion:117 Resp: 809839
Ion Ratio Lower Upper
117 100
201 90.8 69.9 104.9
199 56.5 43.9 65.9









#22
Nitrobenzene
Concen: 87.489 ng/ul
RT: 9.210 min Scan# 1130
Delta R.T. 0.006 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion: 77 Resp: 2602485
Ion Ratio Lower Upper
77 100
123 42.5 32.8 49.2
65 13.7 11.0 16.4



#23
Isophorone
Concen: 88.402 ng/ul
RT: 9.734 min Scan# 1130
Delta R.T. 0.018 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion: 82 Resp: 4940371
Ion Ratio Lower Upper
82 100
95 6.8 5.2 7.8
138 16.7 12.6 19.0









#25
2-Nitrophenol
Concen: 86.631 ng/ul
RT: 9.910 min Scan# 1159
Delta R.T. 0.006 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion:139 Resp: 1151842
Ion Ratio Lower Upper
139 100
65 58.2 49.9 74.9
109 31.2 25.3 37.9



#26
2,4-Dimethylphenol
Concen: 83.309 ng/ul
RT: 9.952 min Scan# 1167
Delta R.T. 0.006 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion:107 Resp: 2261638
Ion Ratio Lower Upper
107 100
121 50.1 39.1 58.7
122 84.0 66.6 100.0





#27

Bis(2-Chloroethoxy)methane

Concen: 83.434 ng/ul

RT: 10.210 min Scan# 1210

Delta R.T. 0.006 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46

Instrument :

BNA_P

ClientSampleId :

SSTD080607





Tgt Ion: 93 Resp: 2889647

Ion Ratio Lower Upper

93 100

95 32.3 26.6 39.8

123 10.6 8.8 13.2

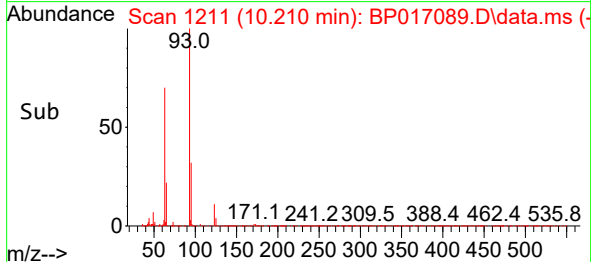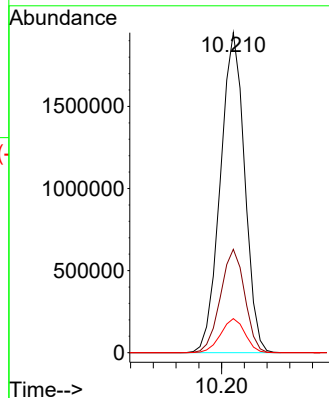

#29

2,4-Dichlorophenol

Concen: 83.465 ng/ul

RT: 10.434 min Scan# 1249

Delta R.T. 0.012 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46




Tgt Ion:162 Resp: 1896442


Ion Ratio Lower Upper

162 100

164 64.9 51.0 76.6

98 37.1 30.7 46.1


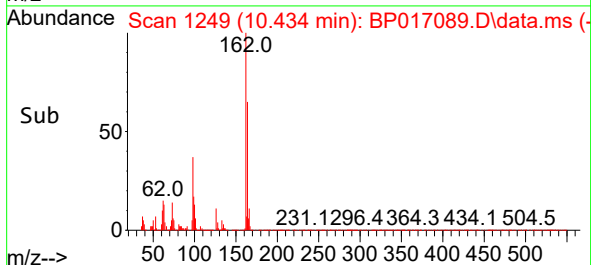
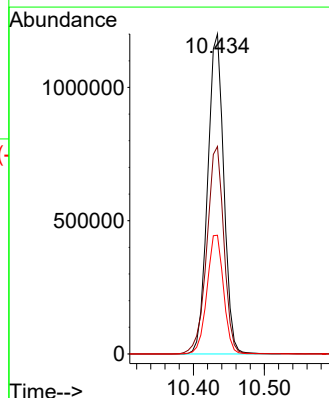
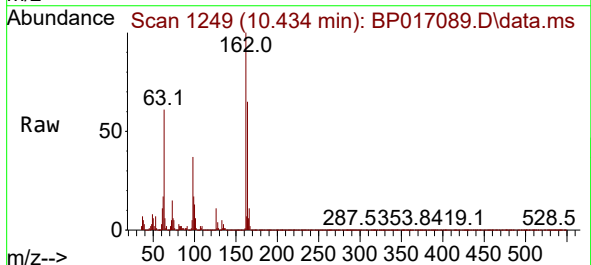




#30
Naphthalene
Concen: 80.888 ng/ul
RT: 10.840 min Scan# 1318
Delta R.T. 0.000 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion:128 Resp: 6338040
Ion Ratio Lower Upper
128 100
129 11.4 8.9 13.3
127 13.6 10.4 15.6

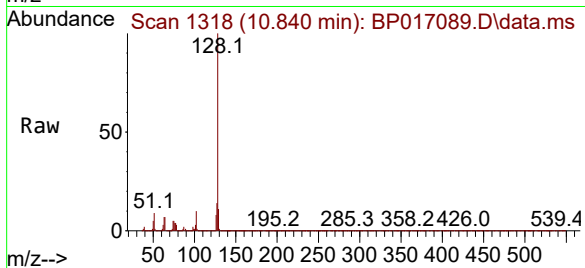

#32
4-Chloroaniline
Concen: 83.587 ng/ul
RT: 10.981 min Scan# 1342
Delta R.T. 0.006 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion:127 Resp: 2798138
Ion Ratio Lower Upper
127 100
129 32.6 25.9 38.9


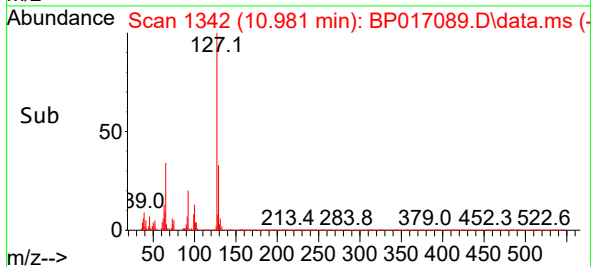

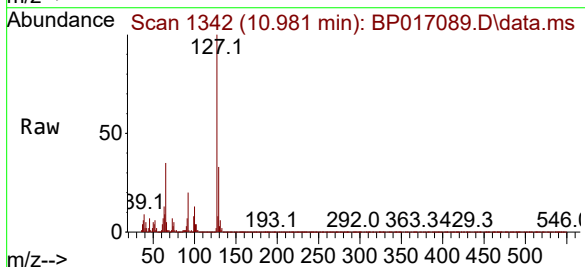




#33
Hexachlorobutadiene
Concen: 75.646 ng/ul
RT: 11.069 min Scan# 11
Delta R.T. 0.000 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion:225 Resp: 1027318
Ion Ratio Lower Upper
225 100
223 62.3 51.6 77.4
227 64.0 51.8 77.8



#34
Caprolactam
Concen: 52.896 ng/ul
RT: 11.834 min Scan# 1487
Delta R.T. 0.041 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion:113 Resp: 398041
Ion Ratio Lower Upper
113 100
55 196.4 160.4 240.6
56 141.0 118.5 177.7



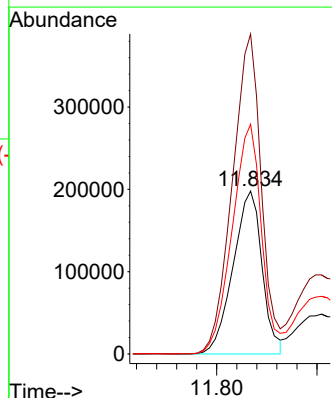



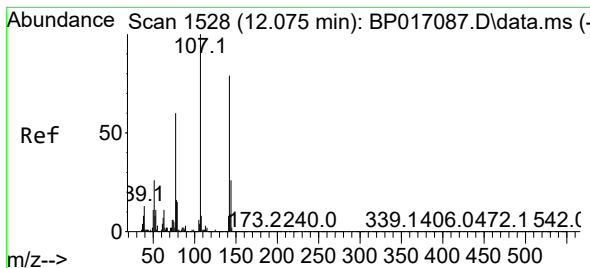

#35
4-Chloro-3-methylphenol
Concen: 87.130 ng/ul
RT: 12.087 min Scan# 1528
Delta R.T. 0.012 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion:107 Resp: 2169478
Ion Ratio Lower Upper
107 100
144 26.2 20.9 31.3
142 79.6 63.2 94.8

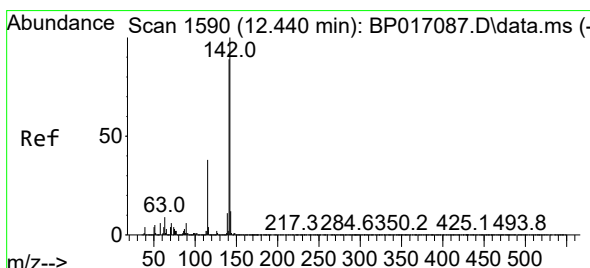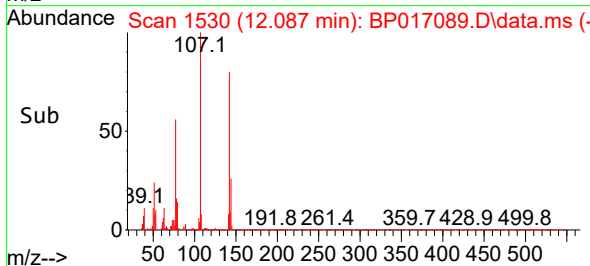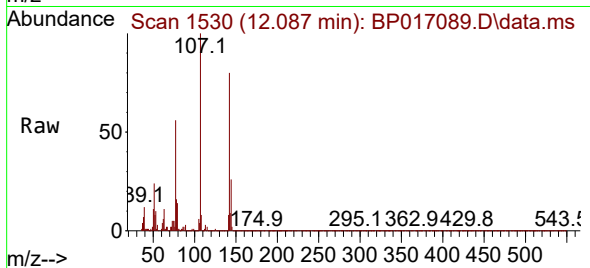

#36
2-Methylnaphthalene
Concen: 84.691 ng/ul
RT: 12.446 min Scan# 1591
Delta R.T. 0.006 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion:142 Resp: 4385387
Ion Ratio Lower Upper
142 100
141 89.9 71.4 107.0

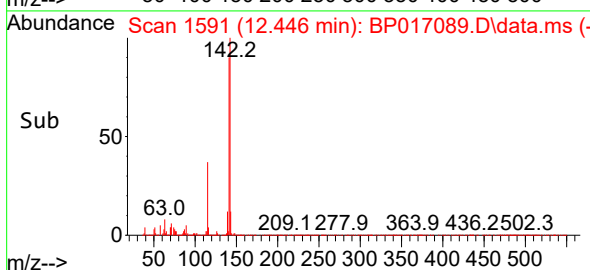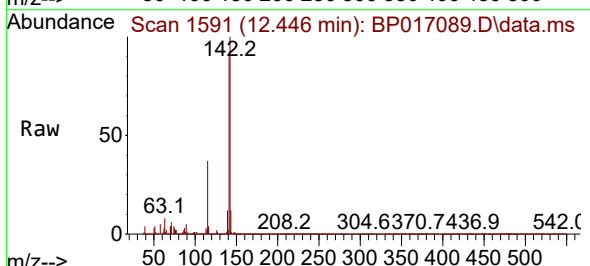



#37

1-Methylnaphthalene

Concen: 84.928 ng/ul

RT: 12.663 min Scan# 1

Delta R.T. 0.000 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46

Instrument :

BNA_P

ClientSampleId :

SSTD080607





Tgt Ion:142 Resp: 4427556

Ion Ratio Lower Upper

142 100

141 92.1 73.1 109.7

116 4.0 3.2 4.8

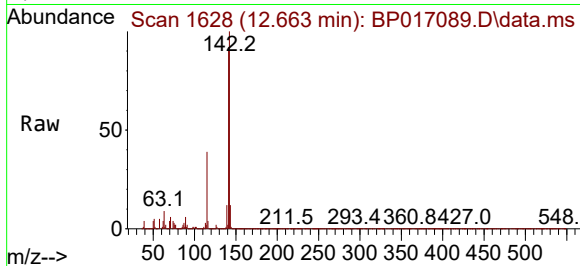

#39

1,2,4,5-Tetrachlorobenzene

Concen: 79.268 ng/ul

RT: 12.799 min Scan# 1651

Delta R.T. 0.006 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46

Tgt Ion:216 Resp: 2057405




Ion Ratio Lower Upper


216 100

214 78.0 62.2 93.2

179 22.2 18.2 27.4

108 19.0 17.0 25.6

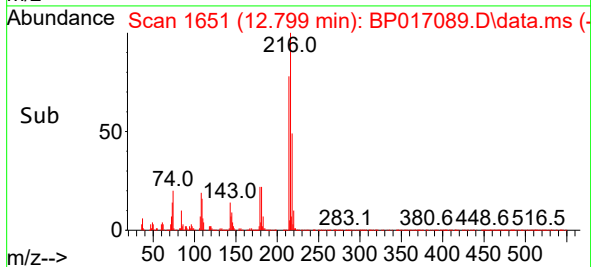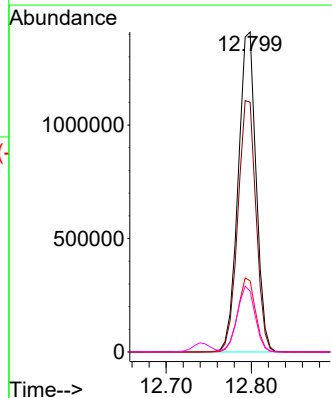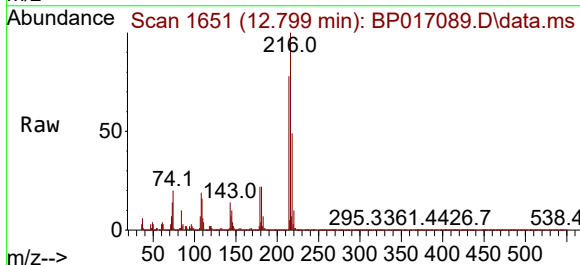



#40

Hexachlorocyclopentadiene

Concen: 74.556 ng/ul

RT: 12.746 min Scan# 1

Delta R.T. 0.006 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46

Instrument :

BNA_P

ClientSampleId :

SSTD080607





Tgt Ion:237 Resp: 1253825

Ion Ratio Lower Upper

237 100

235 63.6 50.9 76.3

272 12.0 8.8 13.2

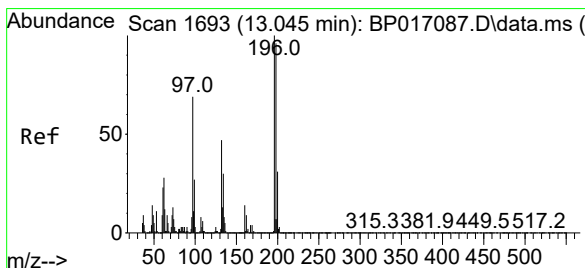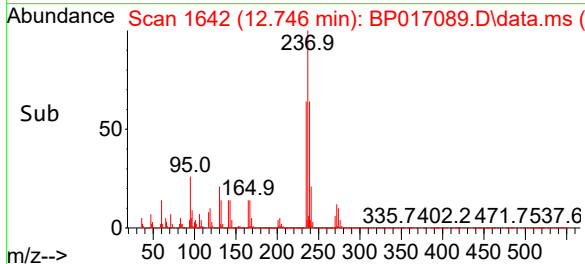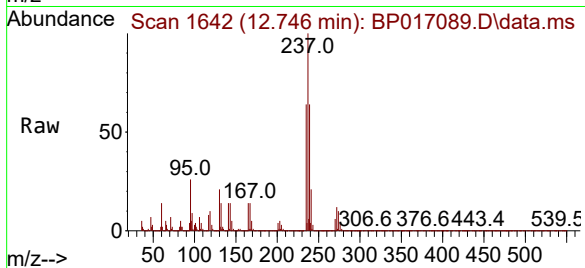

#41

2,4,6-Trichlorophenol

Concen: 83.354 ng/ul

RT: 13.051 min Scan# 1694

Delta R.T. 0.006 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46




Tgt Ion:196 Resp: 1472493


Ion Ratio Lower Upper

196 100

198 95.4 76.7 115.1

200 30.5 24.4 36.6


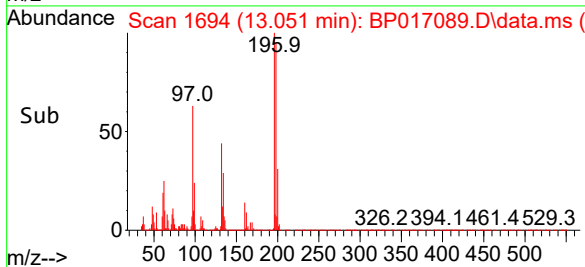

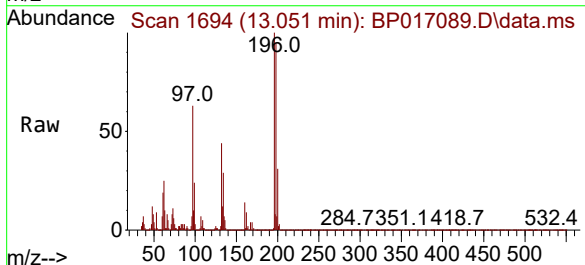




#42
2,4,5-Trichlorophenol
Concen: 82.427 ng/ul
RT: 13.122 min Scan# 1706
Delta R.T. 0.006 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion:196 Resp: 1584331
Ion Ratio Lower Upper
196 100
198 94.8 76.6 115.0
200 30.9 23.8 35.8

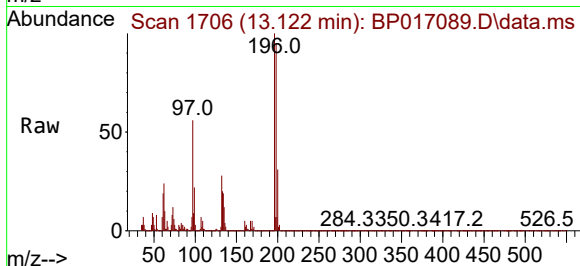

#43
1,1'-Biphenyl
Concen: 80.862 ng/ul
RT: 13.457 min Scan# 1763
Delta R.T. 0.006 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion:154 Resp: 5638678
Ion Ratio Lower Upper
154 100
153 41.3 32.6 49.0
76 15.2 12.2 18.4









#44
2-Chloronaphthalene
Concen: 81.472 ng/ul
RT: 13.504 min Scan# 11
Delta R.T. 0.006 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion:162 Resp: 4460581
Ion Ratio Lower Upper
162 100
164 33.4 26.0 39.0
127 39.7 31.8 47.8



#45
2-Nitroaniline
Concen: 98.478 ng/ul
RT: 13.746 min Scan# 1812
Delta R.T. 0.012 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion: 65 Resp: 1605693
Ion Ratio Lower Upper
65 100
92 66.4 52.5 78.7
138 98.2 71.8 107.6









#47
Dimethylphthalate
Concen: 81.574 ng/ul
RT: 14.087 min Scan# 1869
Delta R.T. 0.006 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion:163 Resp: 5612669
Ion Ratio Lower Upper
163 100
194 3.9 2.9 4.3
164 10.5 7.9 11.9



#48
2,6-Dinitrotoluene
Concen: 88.936 ng/ul
RT: 14.234 min Scan# 1895
Delta R.T. 0.006 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion:165 Resp: 1188375
Ion Ratio Lower Upper
165 100
89 65.8 55.6 83.4
121 22.2 20.0 30.0



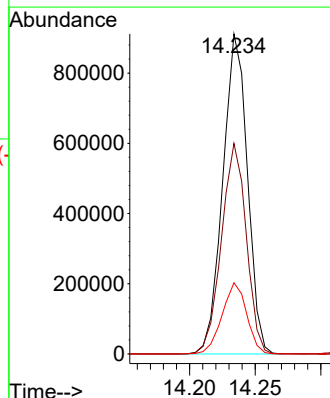





#50
Acenaphthylene
Concen: 87.816 ng/ul
RT: 14.351 min Scan# 1915
Delta R.T. 0.000 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion:152 Resp: 7441331
Ion Ratio Lower Upper
152 100
151 20.6 15.5 23.3
153 13.8 10.2 15.4



#51
3-Nitroaniline
Concen: 84.959 ng/ul
RT: 14.575 min Scan# 1953
Delta R.T. 0.012 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion:138 Resp: 1132948
Ion Ratio Lower Upper
138 100
108 10.0 8.5 12.7
92 119.3 103.3 154.9









#52
Acenaphthene
Concen: 83.047 ng/ul
RT: 14.687 min Scan# 1972
Delta R.T. 0.000 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion:153 Resp: 4909917
Ion Ratio Lower Upper
153 100
152 48.3 38.9 58.3
154 87.9 69.0 103.6



#53
2,4-Dinitrophenol
Concen: 89.436 ng/ul
RT: 14.769 min Scan# 1986
Delta R.T. 0.006 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion:184 Resp: 740961
Ion Ratio Lower Upper
184 100
63 84.2 74.5 111.7
154 66.1 53.8 80.8









#55
4-Nitrophenol
Concen: 91.821 ng/ul
RT: 14.869 min Scan# 2000
Delta R.T. 0.018 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion:109 Resp: 941338
Ion Ratio Lower Upper
109 100
139 129.4 98.6 147.8
65 143.0 117.0 175.4

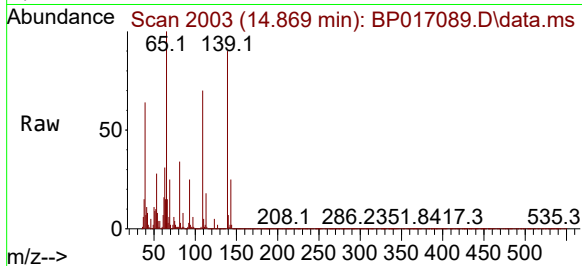

#56
Dibenzofuran
Concen: 80.971 ng/ul
RT: 15.028 min Scan# 2030
Delta R.T. 0.006 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion:168 Resp: 6582351
Ion Ratio Lower Upper
168 100
139 38.3 30.6 45.8




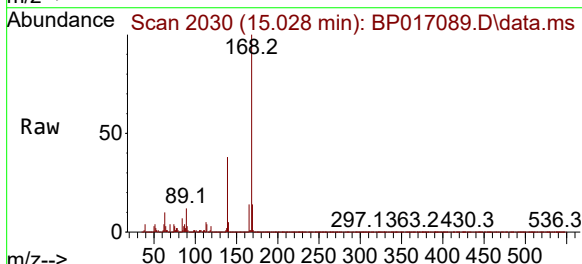




#57
2,4-Dinitrotoluene
Concen: 94.214 ng/ul
RT: 15.016 min Scan# 2027
Delta R.T. 0.006 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion:165 Resp: 1807103
Ion Ratio Lower Upper
165 100
63 59.4 57.7 86.5
182 2.7 2.2 3.4

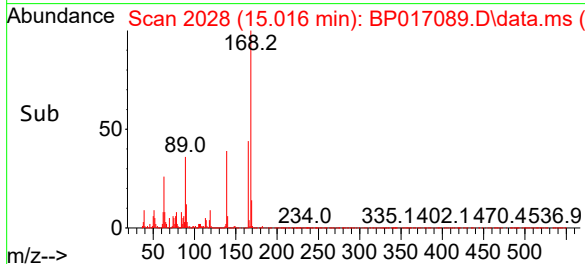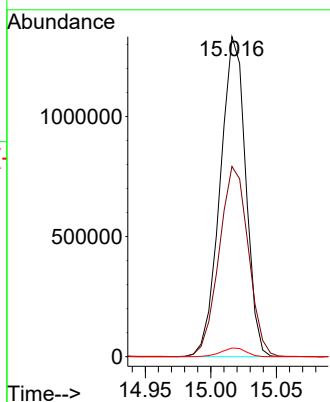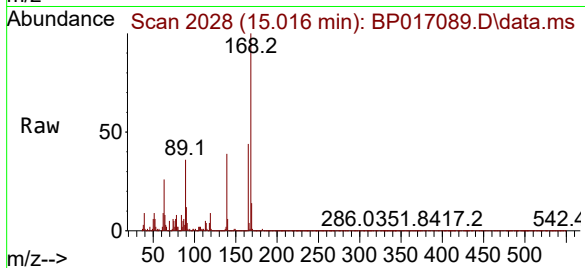

#58
2,3,4,6-Tetrachlorophenol
Concen: 81.594 ng/ul
RT: 15.240 min Scan# 2066
Delta R.T. 0.006 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion:232 Resp: 1264467
Ion Ratio Lower Upper
232 100
131 53.8 46.9 70.3
130 3.0 2.4 3.6
166 36.4 29.6 44.4


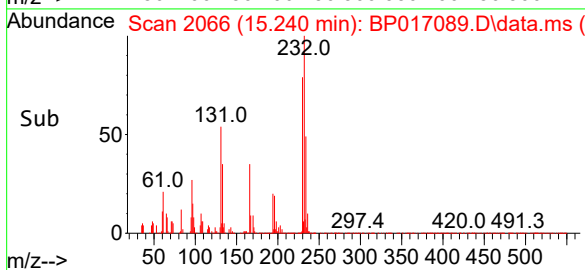

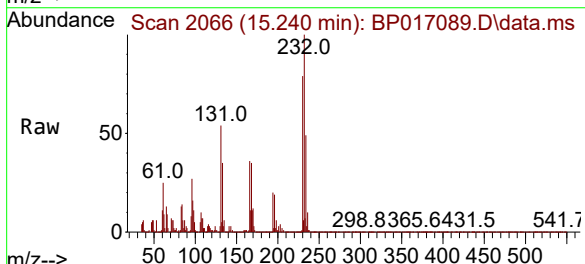




#59
Diethylphthalate
Concen: 84.047 ng/ul
RT: 15.445 min Scan# 2100
Delta R.T. 0.006 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion:149 Resp: 5778757
Ion Ratio Lower Upper
149 100
177 22.1 17.4 26.0
150 12.7 9.5 14.3



#61
Fluorene
Concen: 82.990 ng/ul
RT: 15.681 min Scan# 2141
Delta R.T. 0.012 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion:166 Resp: 5562183
Ion Ratio Lower Upper
166 100
165 97.6 78.8 118.2
167 13.5 10.9 16.3









#62
4-Chlorophenyl-phenylether
Concen: 82.885 ng/ul
RT: 15.669 min Scan# 2138
Delta R.T. 0.006 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion:204 Resp: 2684637
Ion Ratio Lower Upper
204 100
206 33.7 26.6 40.0
141 58.0 50.6 76.0

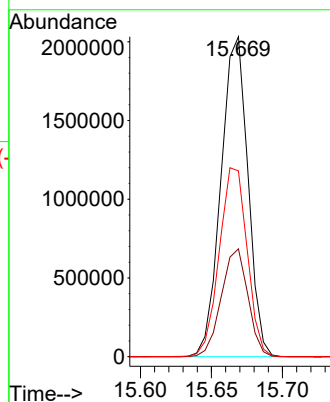

#63
4-Nitroaniline
Concen: 91.194 ng/ul
RT: 15.751 min Scan# 2153
Delta R.T. 0.018 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion:138 Resp: 1069205
Ion Ratio Lower Upper
138 100
92 55.8 45.0 67.6
108 105.0 77.2 115.8









#66
4,6-Dinitro-2-methylphenol
Concen: 92.476 ng/ul
RT: 15.775 min Scan# 2154
Delta R.T. 0.018 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion:198 Resp: 1092191
Ion Ratio Lower Upper
198 100
182 3.4 4.7 7.1#
77 28.0 29.6 44.4#

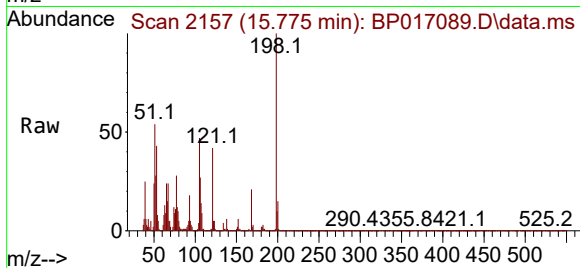

#67
N-Nitrosodiphenylamine
Concen: 81.577 ng/ul
RT: 15.892 min Scan# 2177
Delta R.T. 0.006 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion:169 Resp: 4607805
Ion Ratio Lower Upper
169 100
168 68.6 54.5 81.7
167 38.3 30.4 45.6




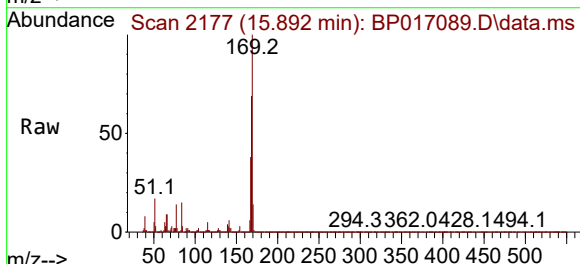




#68
4-Bromophenyl-phenylether
Concen: 80.364 ng/ul
RT: 16.569 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion:248 Resp: 1497703
Ion Ratio Lower Upper
248 100
250 97.3 78.9 118.3
141 81.7 67.9 101.9



#69
Hexachlorobenzene
Concen: 78.315 ng/ul
RT: 16.651 min Scan# 2306
Delta R.T. 0.006 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion:284 Resp: 1599891
Ion Ratio Lower Upper
284 100
142 44.1 38.9 58.3
249 35.1 26.1 39.1





#70

Atrazine

Concen: 80.912 ng/ul

RT: 16.851 min Scan# 21

Delta R.T. 0.006 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46

Instrument :

BNA_P

ClientSampleId :

SSTD080607





Tgt Ion:200 Resp: 1564768

Ion Ratio Lower Upper

200 100

173 27.8 21.0 31.4

215 46.7 35.9 53.9

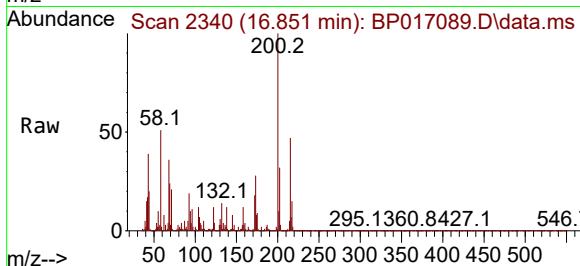

#71

Pentachlorophenol

Concen: 82.999 ng/ul

RT: 17.016 min Scan# 2368

Delta R.T. 0.006 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46




Tgt Ion:266 Resp: 1105713


Ion Ratio Lower Upper

266 100

264 64.8 49.8 74.8

268 64.5 50.9 76.3

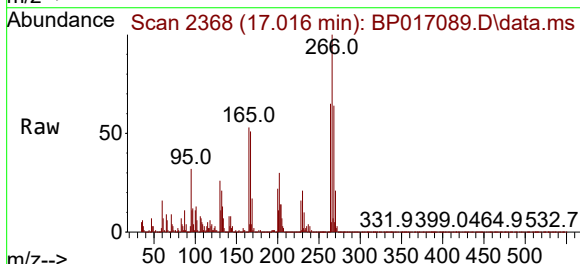



#72

Phenanthrene

Concen: 82.030 ng/ul

RT: 17.439 min Scan# 2439

Delta R.T. 0.006 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46

Instrument :

BNA_P

ClientSampleId :

SSTD080607





Tgt Ion:178 Resp: 8538435

Ion Ratio Lower Upper

178 100

179 15.9 12.3 18.5

176 20.4 15.8 23.8



#74

Anthracene

Concen: 82.895 ng/ul

RT: 17.528 min Scan# 2455

Delta R.T. 0.000 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46




Tgt Ion:178 Resp: 8673796


Ion Ratio Lower Upper

178 100

179 16.6 12.2 18.2

176 20.2 15.4 23.2





#75

1,2,3,4-Tetrachlorobenzene

Concen: 82.126 ng/uL

RT: 13.410 min Scan# 1755

Delta R.T. 0.006 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46

Instrument :

BNA_P

ClientSampleId :

SSTD080607





Tgt Ion:216 Resp: 2191391

Ion Ratio Lower Upper

216 100

214 79.2 63.8 95.6

218 47.7 38.1 57.1



#76

Pentachlorobenzene

Concen: 72.072 ng/uL

RT: 14.916 min Scan# 2011

Delta R.T. 0.006 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46




Tgt Ion:250 Resp: 1852429


Ion Ratio Lower Upper

250 100

248 65.0 49.9 74.9

252 64.8 51.4 77.0

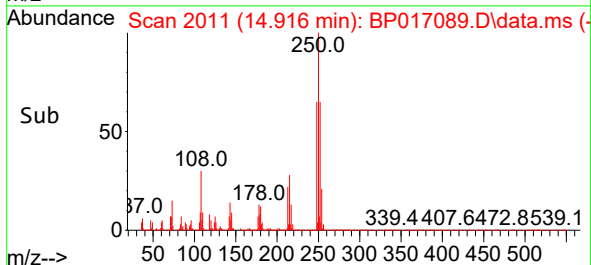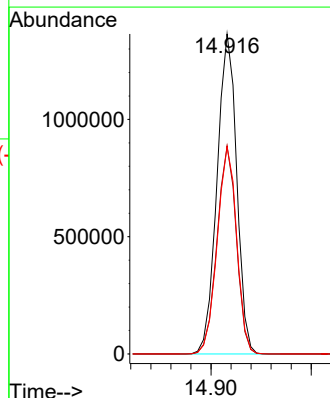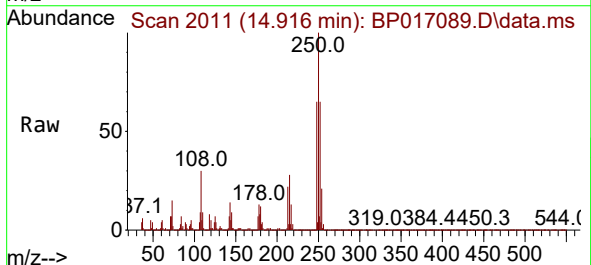




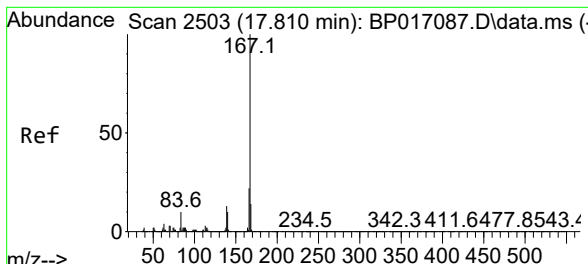


#77
 Carbazole
 Concen: 85.278 ng/ul
 RT: 17.816 min Scan# 2504
 Delta R.T. 0.006 min
 Lab File: BP017089.D
 Acq: 11 Sep 2023 04:46

Instrument :
 BNA_P
 ClientSampleId :
 SSTD080607

Tgt Ion:167 Resp: 8018668




Ion	Ratio	Lower	Upper
167	100		
166	22.6	17.7	26.5
139	13.8	10.8	16.2

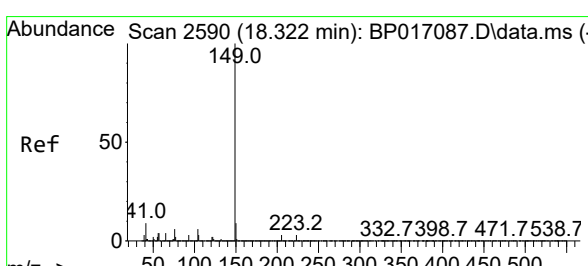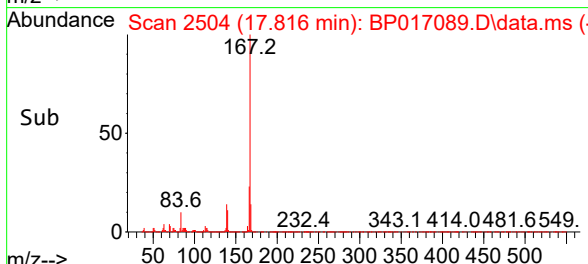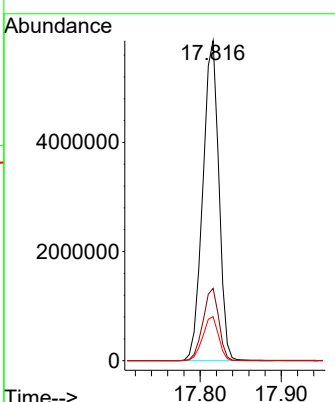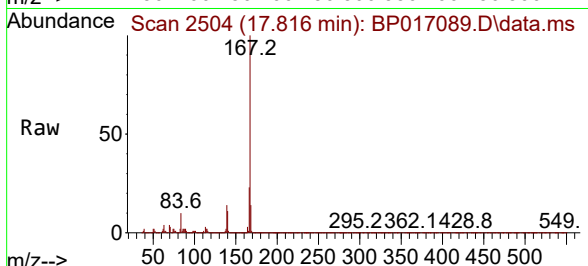


#78
 Di-n-butylphthalate
 Concen: 84.707 ng/ul
 RT: 18.322 min Scan# 2590
 Delta R.T. 0.000 min
 Lab File: BP017089.D
 Acq: 11 Sep 2023 04:46

Tgt Ion:149 Resp: 9757896

Ion	Ratio	Lower	Upper
149	100		
150	10.0	7.3	10.9
104	5.9	4.7	7.1


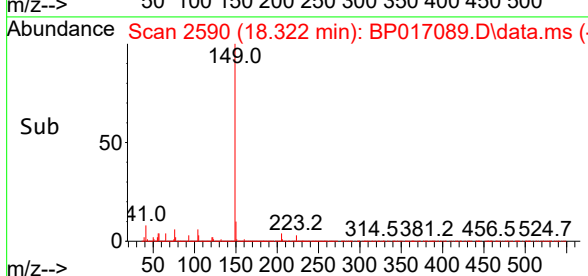
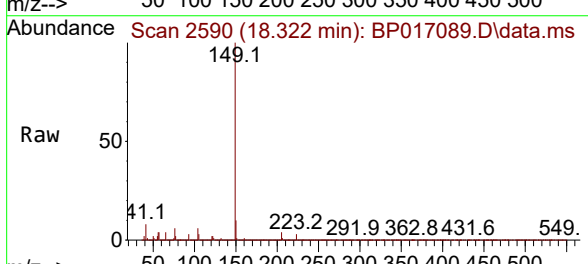
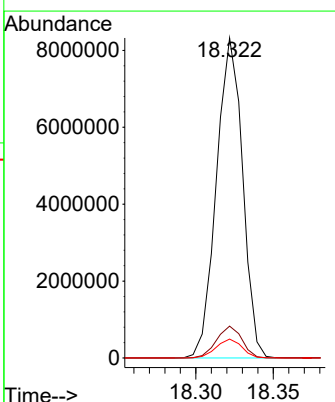




#80
Fluoranthene
Concen: 78.451 ng/ul
RT: 19.398 min Scan# 2773
Delta R.T. 0.000 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion:202 Resp: 9642044
Ion Ratio Lower Upper
202 100
101 14.0 9.9 14.9
100 10.8 7.8 11.8



#82
Pyrene
Concen: 77.394 ng/ul
RT: 19.757 min Scan# 2834
Delta R.T. 0.000 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion:202 Resp: 9876263
Ion Ratio Lower Upper
202 100
101 16.6 11.9 17.9
100 13.6 9.8 14.6





#83

Butylbenzylphthalate

Concen: 88.561 ng/ul

RT: 20.616 min Scan# 2980

Delta R.T. 0.000 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46

Instrument :

BNA_P

ClientSampleId :

SSTD080607





Tgt Ion:149 Resp: 4673717

Ion Ratio Lower Upper

149 100

91 75.6 64.6 96.8

206 20.5 14.6 22.0

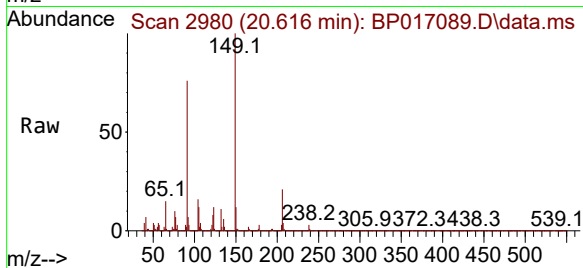

#84

3,3'-Dichlorobenzidine

Concen: 79.300 ng/ul

RT: 21.416 min Scan# 3116

Delta R.T. 0.006 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46




Tgt Ion:252 Resp: 2844054


Ion Ratio Lower Upper

252 100

254 64.4 51.7 77.5

126 12.6 11.5 17.3

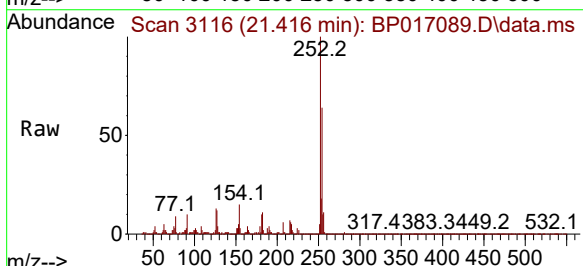



#85

Benzo(a)anthracene

Concen: 83.522 ng/ul

RT: 21.475 min Scan# 3125

Delta R.T. 0.006 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46

Instrument :

BNA_P

ClientSampleId :

SSTD080607





Tgt Ion:228 Resp: 9506045

Ion Ratio Lower Upper

228 100

229 21.1 16.0 24.0

226 31.0 22.9 34.3



#86

Bis(2-ethylhexyl)phthalate

Concen: 88.990 ng/ul

RT: 21.351 min Scan# 3105

Delta R.T. 0.000 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46




Tgt Ion:149 Resp: 6487989


Ion Ratio Lower Upper

149 100

167 28.4 20.8 31.2

279 4.1 2.6 3.8#



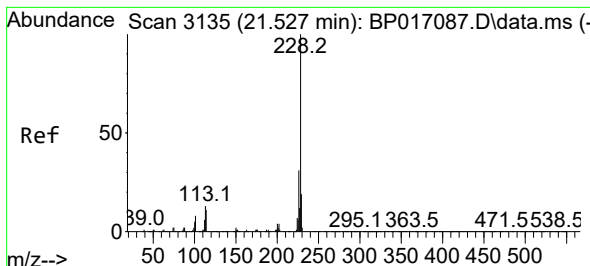

#87

Chrysene

Concen: 81.031 ng/ul

RT: 21.533 min Scan# 3135

Delta R.T. 0.006 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46

Instrument :

BNA_P

ClientSampleId :

SSTD080607





Tgt Ion:228 Resp: 8626994

Ion Ratio Lower Upper

228 100

226 33.9 24.6 36.8

229 20.7 15.6 23.4

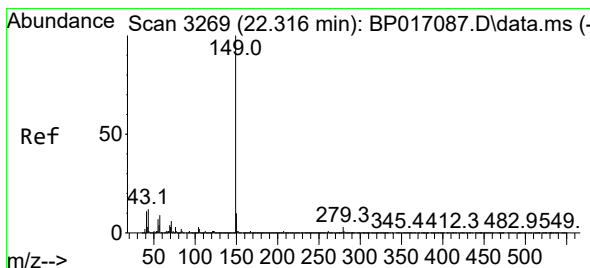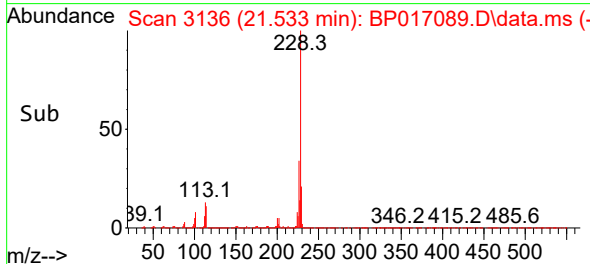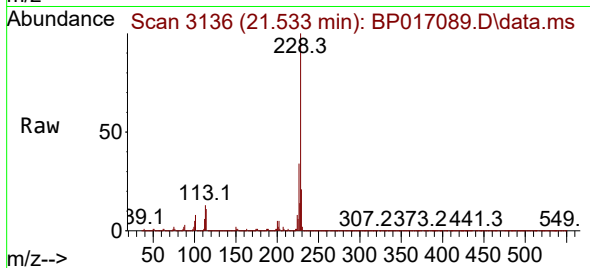

#89

Di-n-octyl phthalate

Concen: 94.663 ng/ul




RT: 22.316 min Scan# 3269


Delta R.T. 0.000 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46

Tgt Ion:149 Resp:10731008


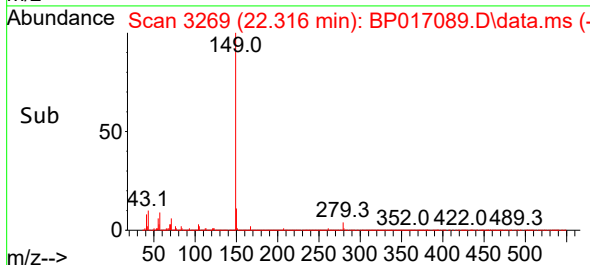
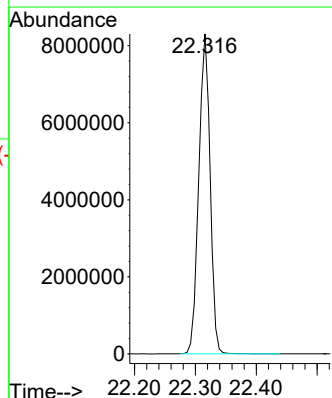
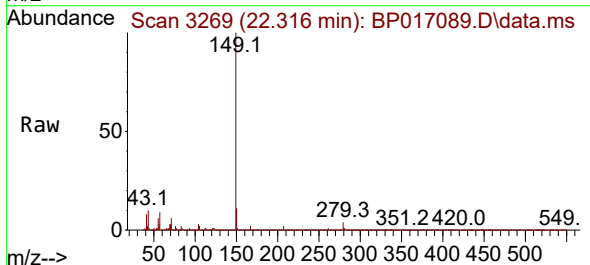




#90
Benzo(b)fluoranthene
Concen: 85.517 ng/ul
RT: 23.239 min Scan# 3424
Delta R.T. 0.012 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46




Instrument :
BNA_P
ClientSampleId :
SSTD080607


Tgt Ion:252 Resp: 8079789
Ion Ratio Lower Upper
252 100
253 22.8 17.9 26.9
125 12.0 10.3 15.5



#91
Benzo(k)fluoranthene
Concen: 88.076 ng/ul
RT: 23.292 min Scan# 3435
Delta R.T. 0.012 min
Lab File: BP017089.D
Acq: 11 Sep 2023 04:46

Tgt Ion:252 Resp: 8058392
Ion Ratio Lower Upper
252 100
253 22.7 17.7 26.5
125 12.2 10.0 15.0





#93

Benzo(a)pyrene

Concen: 91.985 ng/ul

RT: 23.916 min Scan# 3

Delta R.T. 0.012 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46

Instrument :

BNA_P

ClientSampleId :

SSTD080607





Tgt Ion:252 Resp: 7248789

Ion Ratio Lower Upper

252 100

253 22.3 17.6 26.4

125 13.4 11.3 16.9



#94

Indeno(1,2,3-cd)pyrene

Concen: 79.090 ng/ul

RT: 26.715 min Scan# 4017

Delta R.T. 0.018 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46




Tgt Ion:276 Resp: 6918551


Ion Ratio Lower Upper

276 100

138 29.7 23.4 35.2

277 25.4 20.1 30.1

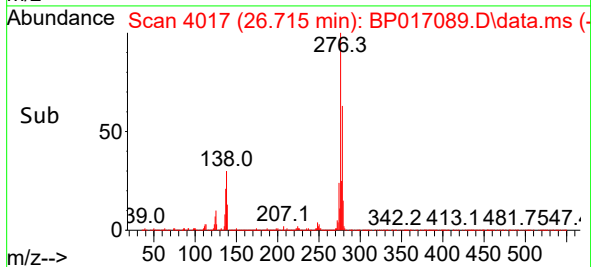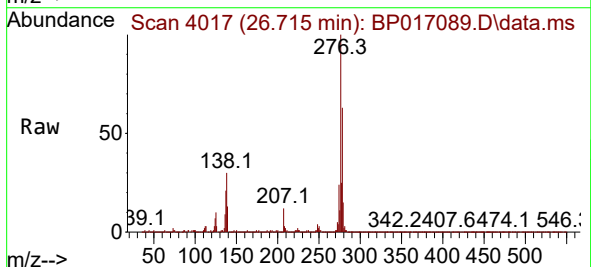



#95

Dibenzo(a,h)anthracene

Concen: 80.582 ng/ul

RT: 26.739 min Scan# 4018

Delta R.T. 0.018 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46

Instrument :

BNA_P

ClientSampleId :

SSTD080607





Tgt Ion:278 Resp: 5818038

Ion Ratio Lower Upper

278 100

139 19.8 16.5 24.7

279 24.3 19.2 28.8

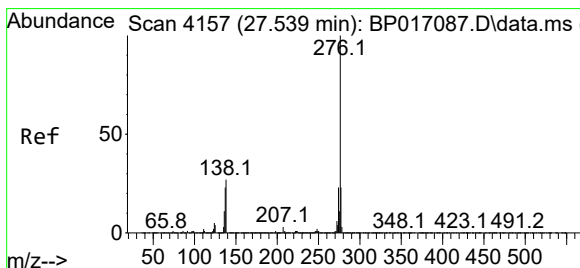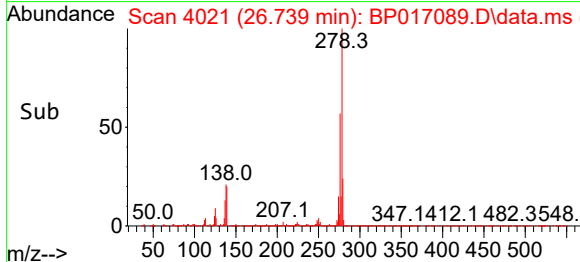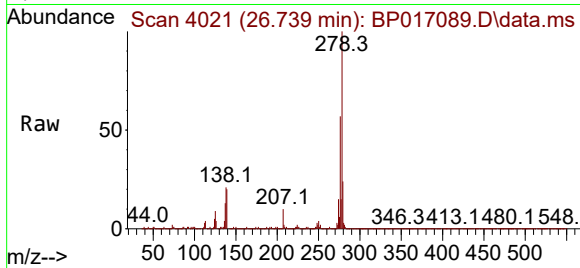

#96

Benzo(g,h,i)perylene

Concen: 73.894 ng/ul

RT: 27.557 min Scan# 4160

Delta R.T. 0.018 min

Lab File: BP017089.D

Acq: 11 Sep 2023 04:46

Tgt Ion:276 Resp: 5093911

Ion Ratio Lower Upper

276 100

138 27.4 22.0 33.0

277 24.1 18.7 28.1

