

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091023\
 Data File : BP017095.D
 Acq On : 11 Sep 2023 09:17
 Operator : MA/JU
 Sample : 04262-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJ75

Quant Time: Sep 12 02:26:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 11 06:13:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	288217	20.000	ng/u1	0.00
20) Naphthalene-d8	10.787	136	1329938	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.616	164	846992	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.387	188	1879649	20.000	ng/u1	0.00
79) Chrysene-d12	21.486	240	1560578	20.000	ng/u1	0.00
88) Perylene-d12	24.016	264	1595704	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.317	96	41394	5.482	ng/uL	0.00
4) Pyridine-d5	3.752	84	215438	9.461	ng/u1	0.00
7) Phenol-d5	7.111	99	175124	6.684	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.299	67	526739	29.977	ng/u1	0.00
11) 2-Chlorophenol-d4	7.481	132	445515	23.528	ng/u1	0.00
15) 4-Methylphenol-d8	8.669	113	325743	15.717	ng/u1	0.00
21) Nitrobenzene-d5	9.158	128	279631	29.533	ng/u1	0.00
24) 2-Nitrophenol-d4	9.869	143	290862	29.764	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.393	165	488267	26.350	ng/u1	0.00
31) 4-Chloroaniline-d4	10.946	131	656904	22.108	ng/u1	0.00
46) Dimethylphthalate-d6	14.034	166	2013646	33.412	ng/u1	0.00
49) Acenaphthylene-d8	14.316	160	2092707	30.494	ng/u1	0.00
54) 4-Nitrophenol-d4	14.834	143	60524	4.868	ng/u1	0.00
60) Fluorene-d10	15.616	176	1686454	32.975	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.740	200	258500	24.370	ng/u1	0.00
73) Anthracene-d10	17.487	188	2788146	34.606	ng/u1	0.00
81) Pyrene-d10	19.722	212	3150692	38.338	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.845	264	2669508	34.848	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.352	88	25587	3.122 ng/uL	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091023\
Data File : BP017095.D
Acq On : 11 Sep 2023 09:17
Operator : MA/JU
Sample : 04262-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ75


Quant Time: Sep 12 02:26:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 11 06:13:29 2023
Response via : Initial Calibration

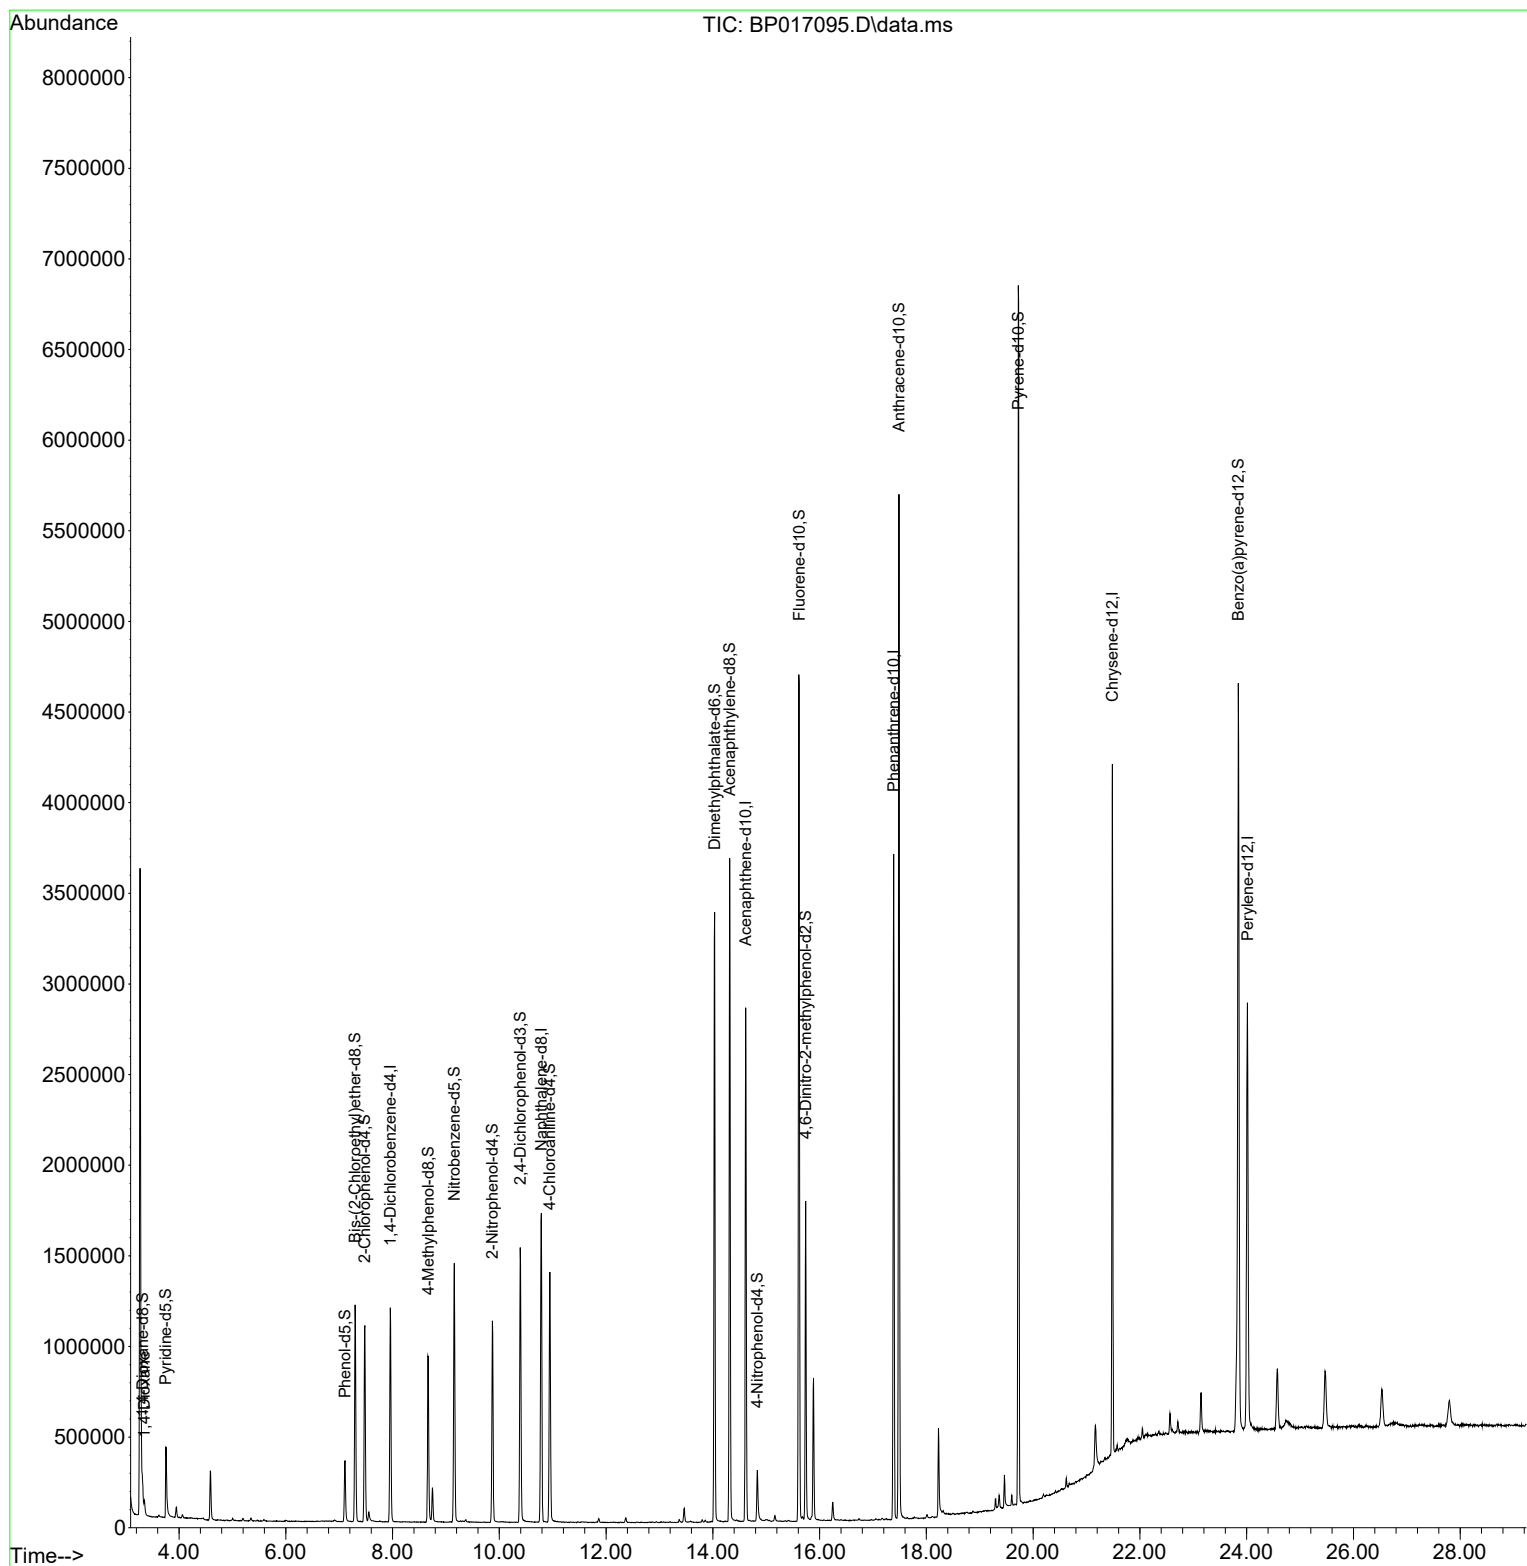

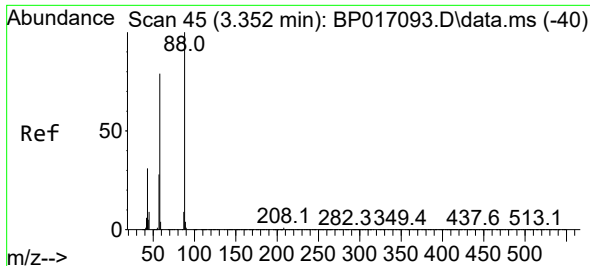

#2
 1,4-Dioxane
 Concen: 3.122 ng/uL
 RT: 3.352 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BP017095.D
 Acq: 11 Sep 2023 09:17

Instrument :
 BNA_P
 ClientSampleId :
 BBJ75

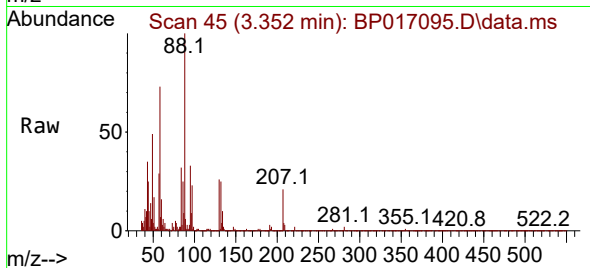

Tgt Ion: 88 Resp: 25587
 Ion Ratio Lower Upper
 88 100
 43 35.2 27.3 40.9
 58 72.9 63.7 95.5

