

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091023\
 Data File : BP017111.D
 Acq On : 11 Sep 2023 19:22
 Operator : MA/JU
 Sample : 04247-10
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJ83

Quant Time: Sep 12 02:31:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 11 06:13:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	259279	20.000	ng/u1	0.00
20) Naphthalene-d8	10.781	136	1284483	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.616	164	903910	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.386	188	1965677	20.000	ng/u1	0.00
79) Chrysene-d12	21.486	240	1626470	20.000	ng/u1	0.00
88) Perylene-d12	24.015	264	1690581	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.316	96	46767	6.885	ng/uL	0.00
4) Pyridine-d5	3.752	84	287879	14.053	ng/u1	0.00
7) Phenol-d5	7.104	99	266862	11.323	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.298	67	691718	43.760	ng/u1	0.00
11) 2-Chlorophenol-d4	7.481	132	614313	36.063	ng/u1	0.00
15) 4-Methylphenol-d8	8.669	113	451306	24.206	ng/u1	0.00
21) Nitrobenzene-d5	9.157	128	371888	40.667	ng/u1	0.00
24) 2-Nitrophenol-d4	9.869	143	387532	41.060	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.392	165	635129	35.489	ng/u1	0.00
31) 4-Chloroaniline-d4	10.945	131	837479	29.183	ng/u1	0.00
46) Dimethylphthalate-d6	14.033	166	2432073	37.813	ng/u1	0.00
49) Acenaphthylene-d8	14.316	160	2638476	36.026	ng/u1	0.00
54) 4-Nitrophenol-d4	14.833	143	104327	7.862	ng/u1	0.00
60) Fluorene-d10	15.616	176	2086668	38.231	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.739	200	347849	31.358	ng/u1	0.00
73) Anthracene-d10	17.486	188	3543370	42.055	ng/u1	0.00
81) Pyrene-d10	19.727	212	3999645	46.696	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.850	264	3473654	42.801	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.352	88	17214	2.335	ng/uL	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091023\
Data File : BP017111.D
Acq On : 11 Sep 2023 19:22
Operator : MA/JU
Sample : 04247-10
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ83

Quant Time: Sep 12 02:31:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 11 06:13:29 2023
Response via : Initial Calibration

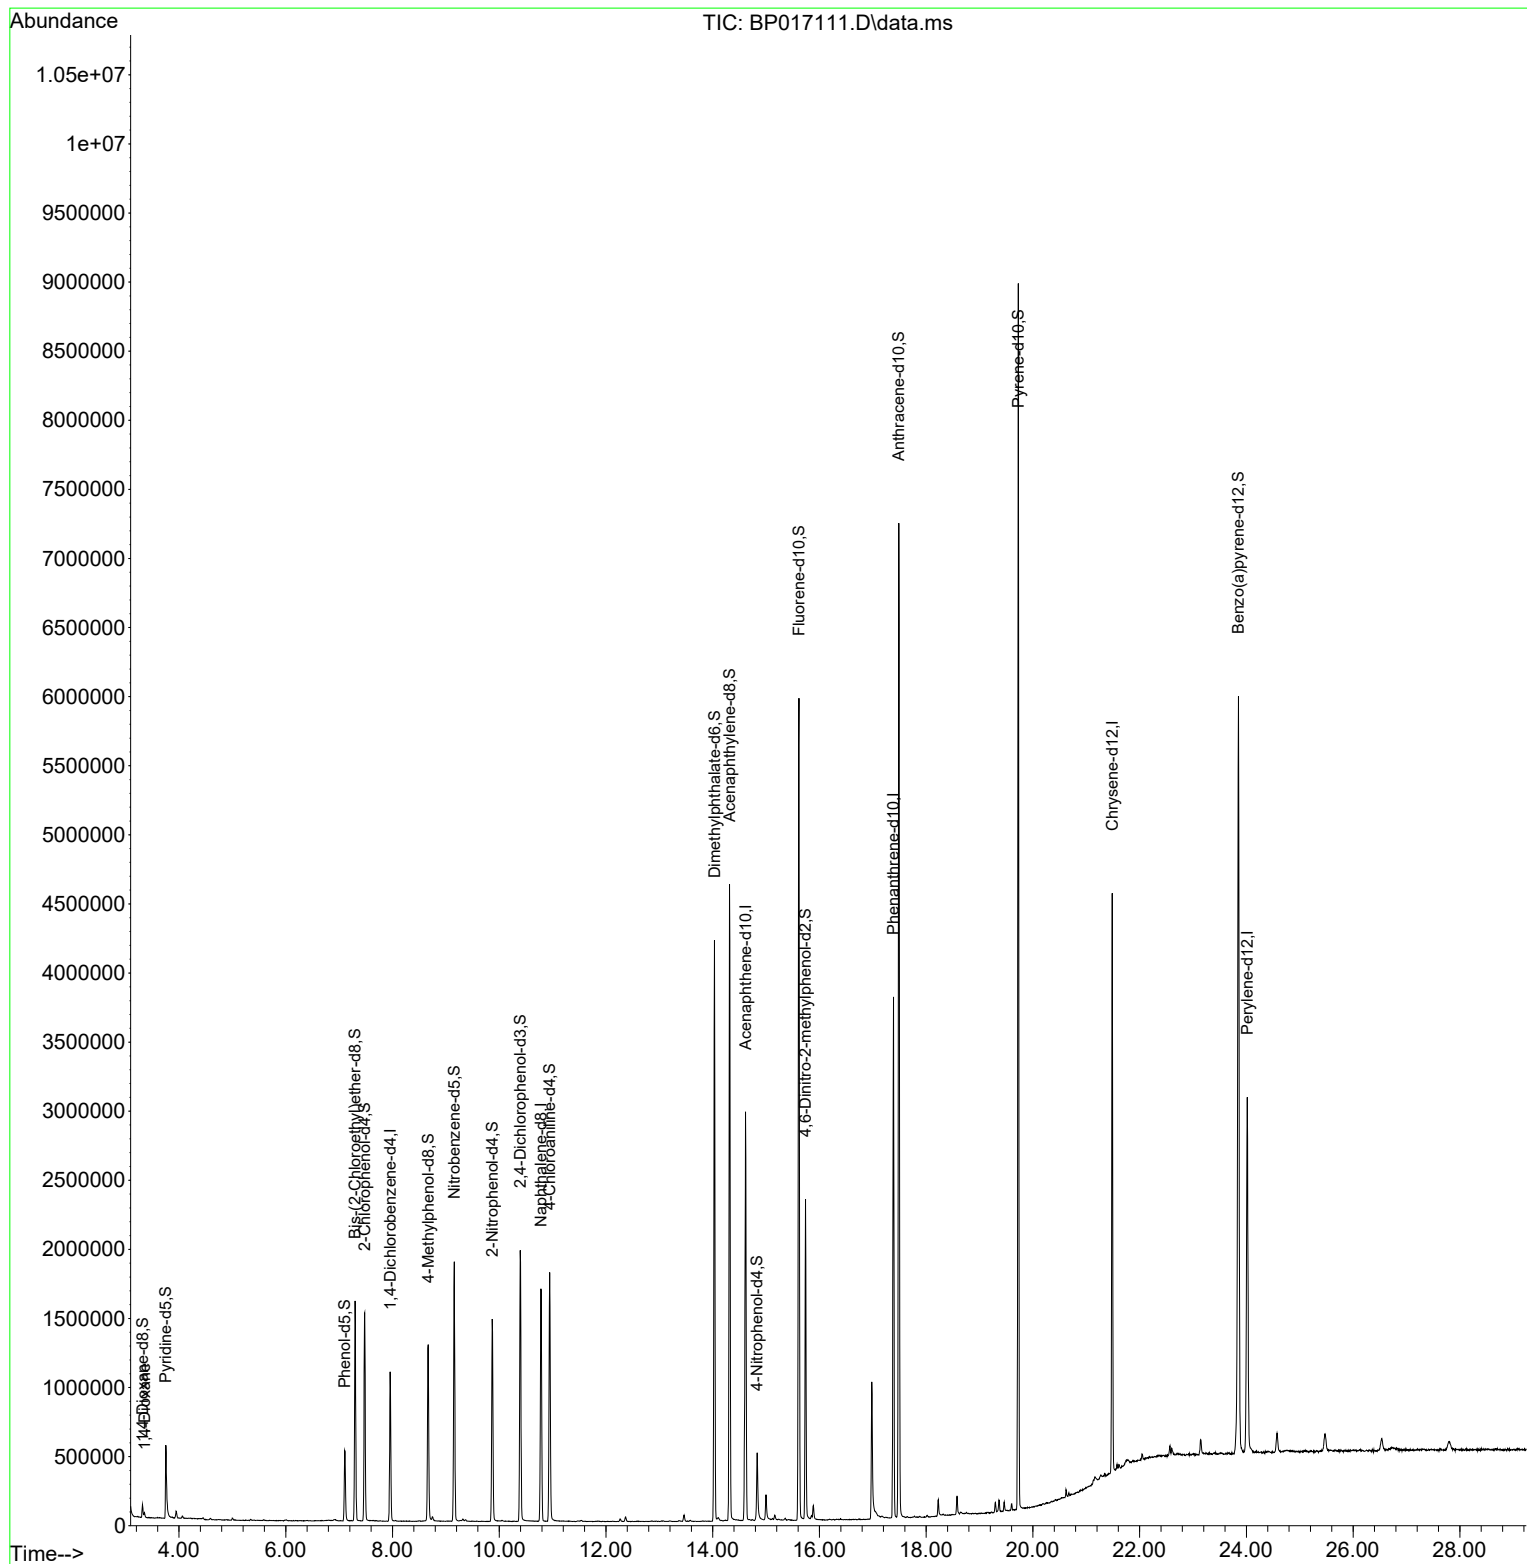

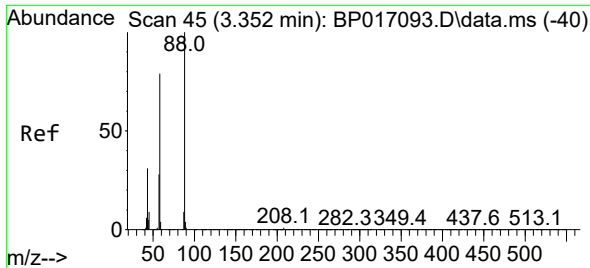

#2
 1,4-Dioxane
 Concen: 2.335 ng/uL
 RT: 3.352 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BP017111.D
 Acq: 11 Sep 2023 19:22

Instrument :
 BNA_P
 ClientSampleId :
 BBJ83

Tgt Ion: 88 Resp: 17214
 Ion Ratio Lower Upper
 88 100
 43 36.9 27.3 40.9
 58 71.0 63.7 95.5

