

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091023\
 Data File : BP017112.D
 Acq On : 11 Sep 2023 19:56
 Operator : MA/JU
 Sample : 04247-11
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA05

Quant Time: Sep 12 02:31:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 11 06:13:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	262748	20.000	ng/u1	0.00
20) Naphthalene-d8	10.787	136	1371172	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.616	164	876283	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.386	188	1914839	20.000	ng/u1	0.00
79) Chrysene-d12	21.486	240	1681550	20.000	ng/u1	0.00
88) Perylene-d12	24.015	264	1815539	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.317	96	42133	6.121	ng/uL	0.00
4) Pyridine-d5	3.752	84	221061	10.649	ng/u1	0.00
7) Phenol-d5	7.110	99	213626	8.944	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.299	67	731285	45.652	ng/u1	0.00
11) 2-Chlorophenol-d4	7.475	132	619278	35.875	ng/u1	0.00
15) 4-Methylphenol-d8	8.669	113	415582	21.996	ng/u1	0.00
21) Nitrobenzene-d5	9.157	128	400874	41.065	ng/u1	0.00
24) 2-Nitrophenol-d4	9.869	143	413718	41.063	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.399	165	709901	37.159	ng/u1	0.00
31) 4-Chloroaniline-d4	10.946	131	680606	22.217	ng/u1	0.00
46) Dimethylphthalate-d6	14.034	166	2423164	38.863	ng/u1	0.00
49) Acenaphthylene-d8	14.316	160	2776031	39.100	ng/u1	0.00
54) 4-Nitrophenol-d4	14.857	143	83310	6.476	ng/u1	0.02
60) Fluorene-d10	15.616	176	2109874	39.875	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.739	200	341040	31.560	ng/u1	0.00
73) Anthracene-d10	17.486	188	3320530	40.457	ng/u1	0.00
81) Pyrene-d10	19.727	212	3799468	42.906	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.851	264	3495665	40.108	ng/u1	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.352	88	91767	12.281	ng/uL	96
10) Bis(2-Chloroethyl)ether	7.393	93	48976	2.420	ng/u1	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091023\
Data File : BP017112.D
Acq On : 11 Sep 2023 19:56
Operator : MA/JU
Sample : 04247-11
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA05

Quant Time: Sep 12 02:31:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 11 06:13:29 2023
Response via : Initial Calibration




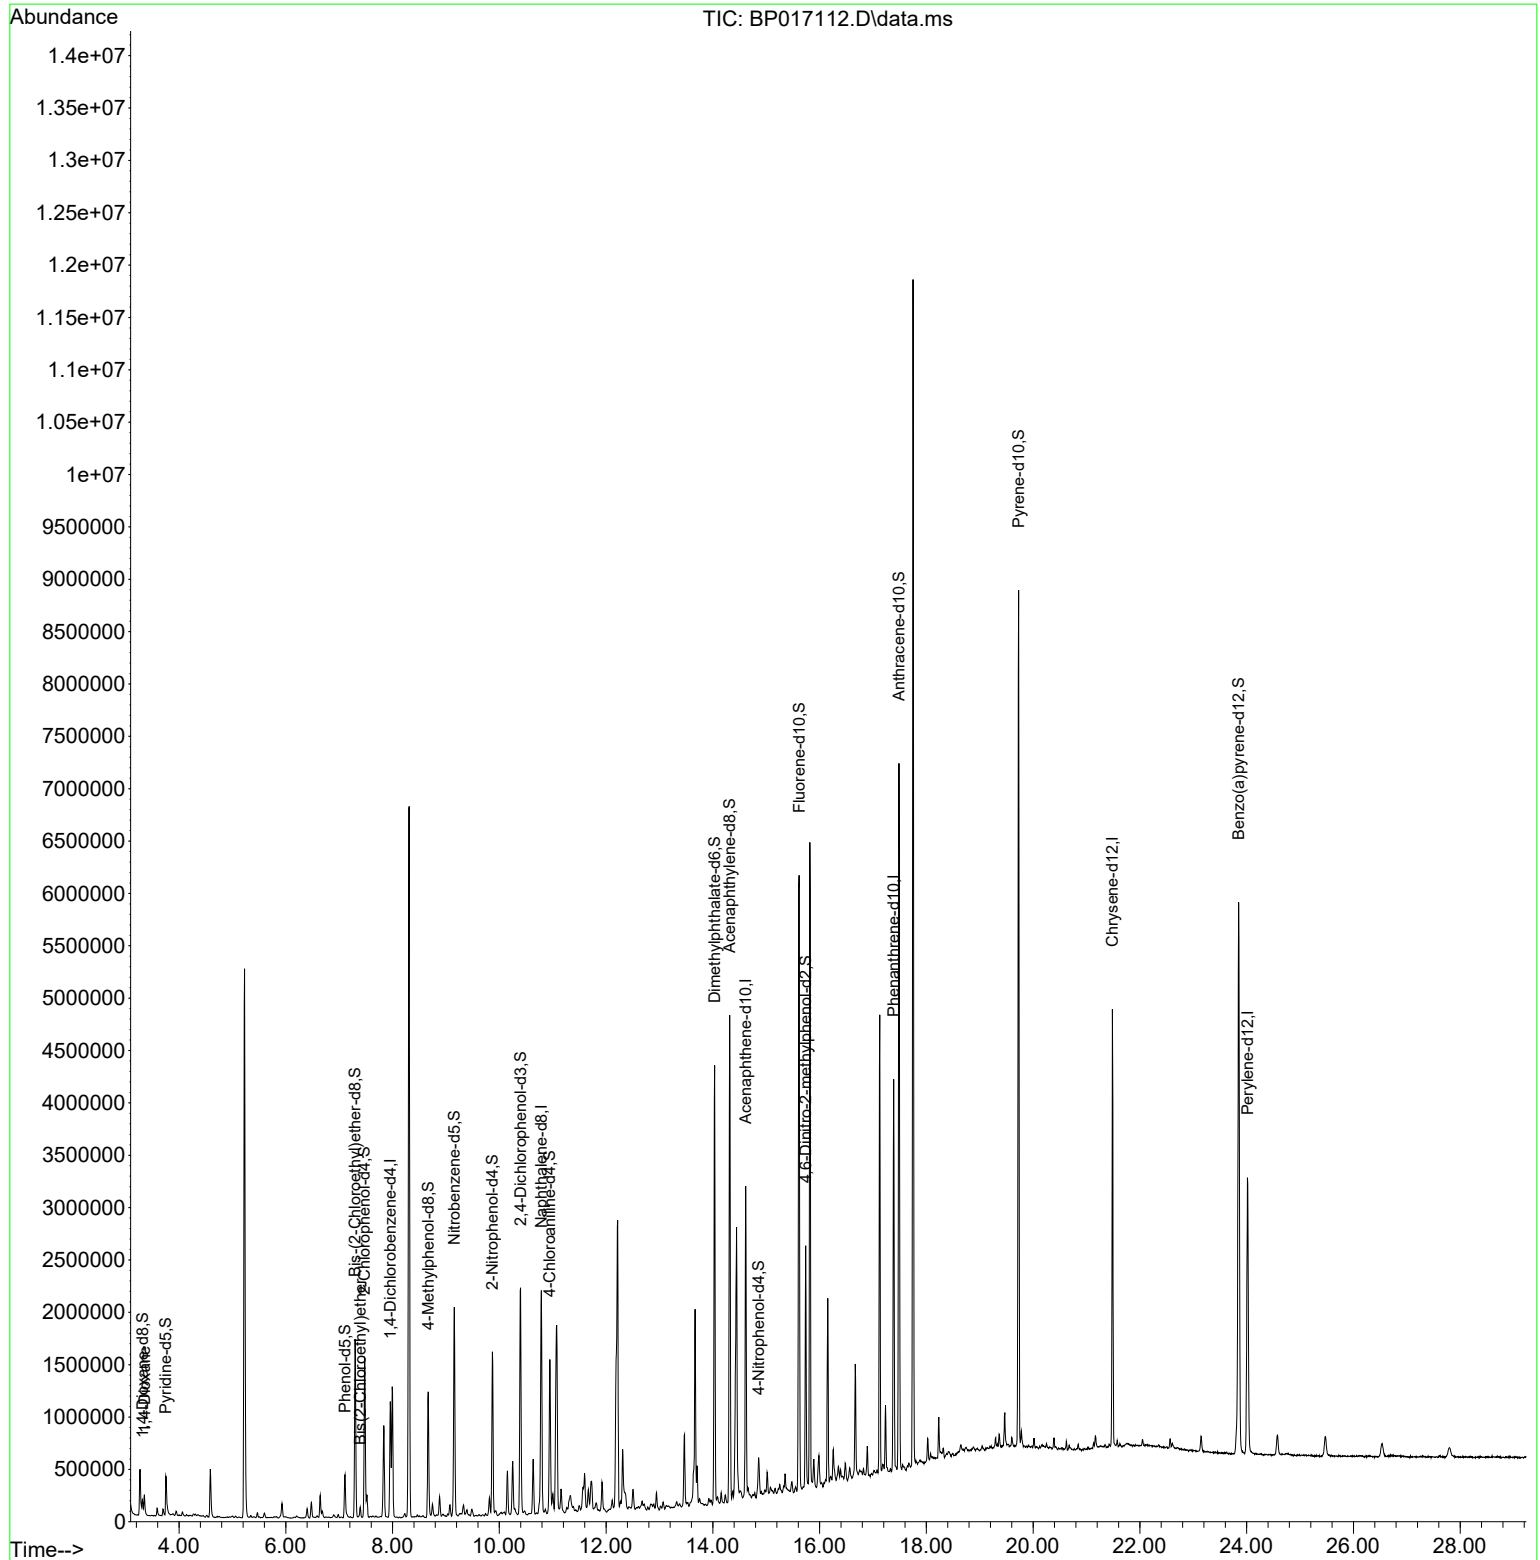


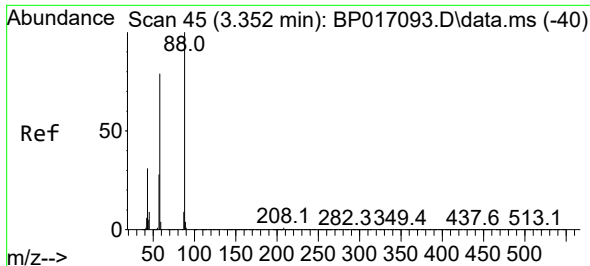

#2
 1,4-Dioxane
 Concen: 12.281 ng/uL
 RT: 3.352 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BP017112.D
 Acq: 11 Sep 2023 19:56

Instrument :
 BNA_P
 ClientSampleId :
 BHA05

Tgt Ion: 88 Resp: 91767
 Ion Ratio Lower Upper
 88 100
 43 34.6 27.3 40.9
 58 75.1 63.7 95.5

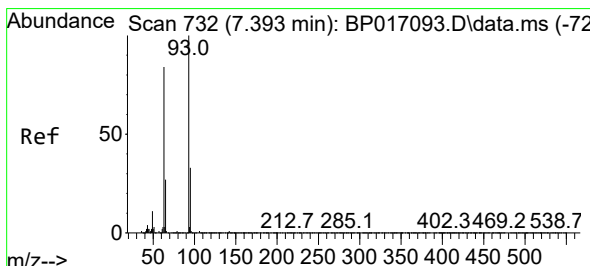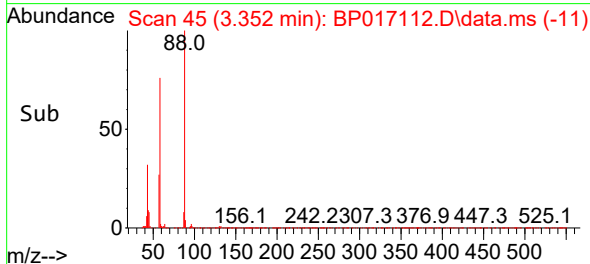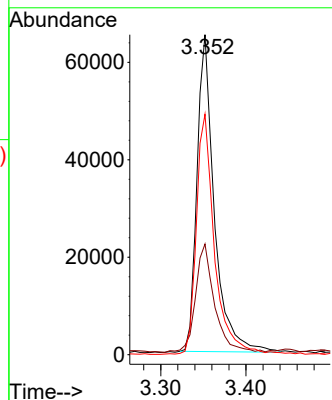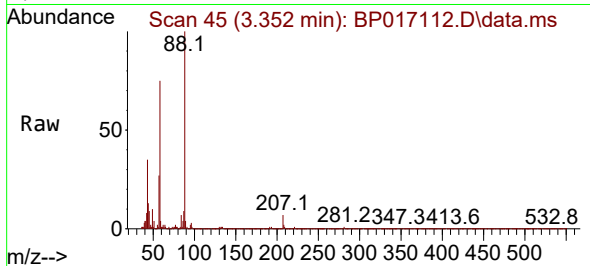

#10
 Bis(2-Chloroethyl)ether
 Concen: 2.420 ng/uL
 RT: 7.393 min Scan# 732
 Delta R.T. 0.000 min
 Lab File: BP017112.D
 Acq: 11 Sep 2023 19:56

Tgt Ion: 93 Resp: 48976
 Ion Ratio Lower Upper
 93 100
 63 86.6 65.4 98.0
 95 33.3 25.1 37.7

