

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091219\
 Data File : BP000230.D
 Acq On : 12 Sep 2019 21:47
 Operator : HP/JU
 Sample : K4634-20DL 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Sep 13 01:52:28 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 02:43:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	274594	20.00	ng/ul	0.00
18) Naphthalene-d8	8.18	136	1033773	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.95	164	558936	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.46	188	1042381	20.00	ng/ul	0.00
78) Chrysene-d12	14.17	240	785218	20.00	ng/ul	0.02
86) Perylene-d12	15.65	264	159651	20.00	ng/ul	-0.04

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.62	96	4364	0.56	ng/uL	0.02
5) Phenol-d5	6.52	99	87548	3.74	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.58	67	44356	3.63	ng/ul	0.00
9) 2-Chlorophenol-d4	6.66	132	72061	3.81	ng/ul	0.00
13) 4-Methylphenol-d8	7.26	113	65026	3.70	ng/ul	0.00
19) Nitrobenzene-d5	7.45	128	30157	3.84	ng/ul	0.00
22) 2-Nitrophenol-d4	7.78	143	32245	4.22	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	8.02	165	60832	3.75	ng/ul	0.00
29) 4-Chloroaniline-d4	8.24	131	20670	1.03	ng/ul	0.00
44) Dimethylphthalate-d6	9.63	166	179697	4.35	ng/ul	0.00
47) Acenaphthylene-d8	9.79	160	221053	4.33	ng/ul	0.00
52) 4-Nitrophenol-d4	10.04	143	15951	2.16	ng/ul	0.00
58) Fluorene-d10	10.47	176	146986	4.19	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.55	200	8438	1.76	ng/ul	0.02
71) Anthracene-d10	11.51	188	221095	4.38	ng/ul	0.00
79) Pyrene-d10	12.91	212	210489	4.51	ng/ul	0.01
90) Benzo(a)pyrene-d12	15.65	264	159651	19.29	ng/ul	0.06

Target Compounds


					Ovalue	
50) Acenaphthene	9.98	153	158363	4.289	ng/ul	99
70) Phenanthrene	11.48	178	624630	10.133	ng/ul	99
72) Anthracene	11.53	178	145190	2.394	ng/ul	98
75) Carbazole	11.69	167	82451	1.590	ng/ul	96
77) Fluoranthene	12.70	202	1267579	20.387	ng/ul	99
80) Pyrene	12.93	202	1542557	26.039	ng/ul#	91
83) Benzo(a)anthracene	14.16	228	1075293	18.918	ng/ul	98
85) Chrysene	14.20	228	1524213	29.223	ng/ul	97
88) Benzo(b)fluoranthene	15.29	252	1909007	180.413	ng/ul	98
89) Benzo(k)fluoranthene	15.29	252	1930935	193.589	ng/ul	98
91) Benzo(a)pyrene	15.68	252	1147660	115.600	ng/ul	96
92) Indeno(1,2,3-cd)pyrene	17.36	276	434567	38.049	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091219\
Data File : BP000230.D
Acq On : 12 Sep 2019 21:47
Operator : HP/JU
Sample : K4634-20DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Sep 13 01:52:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 02:43:18 2019
Response via : Initial Calibration

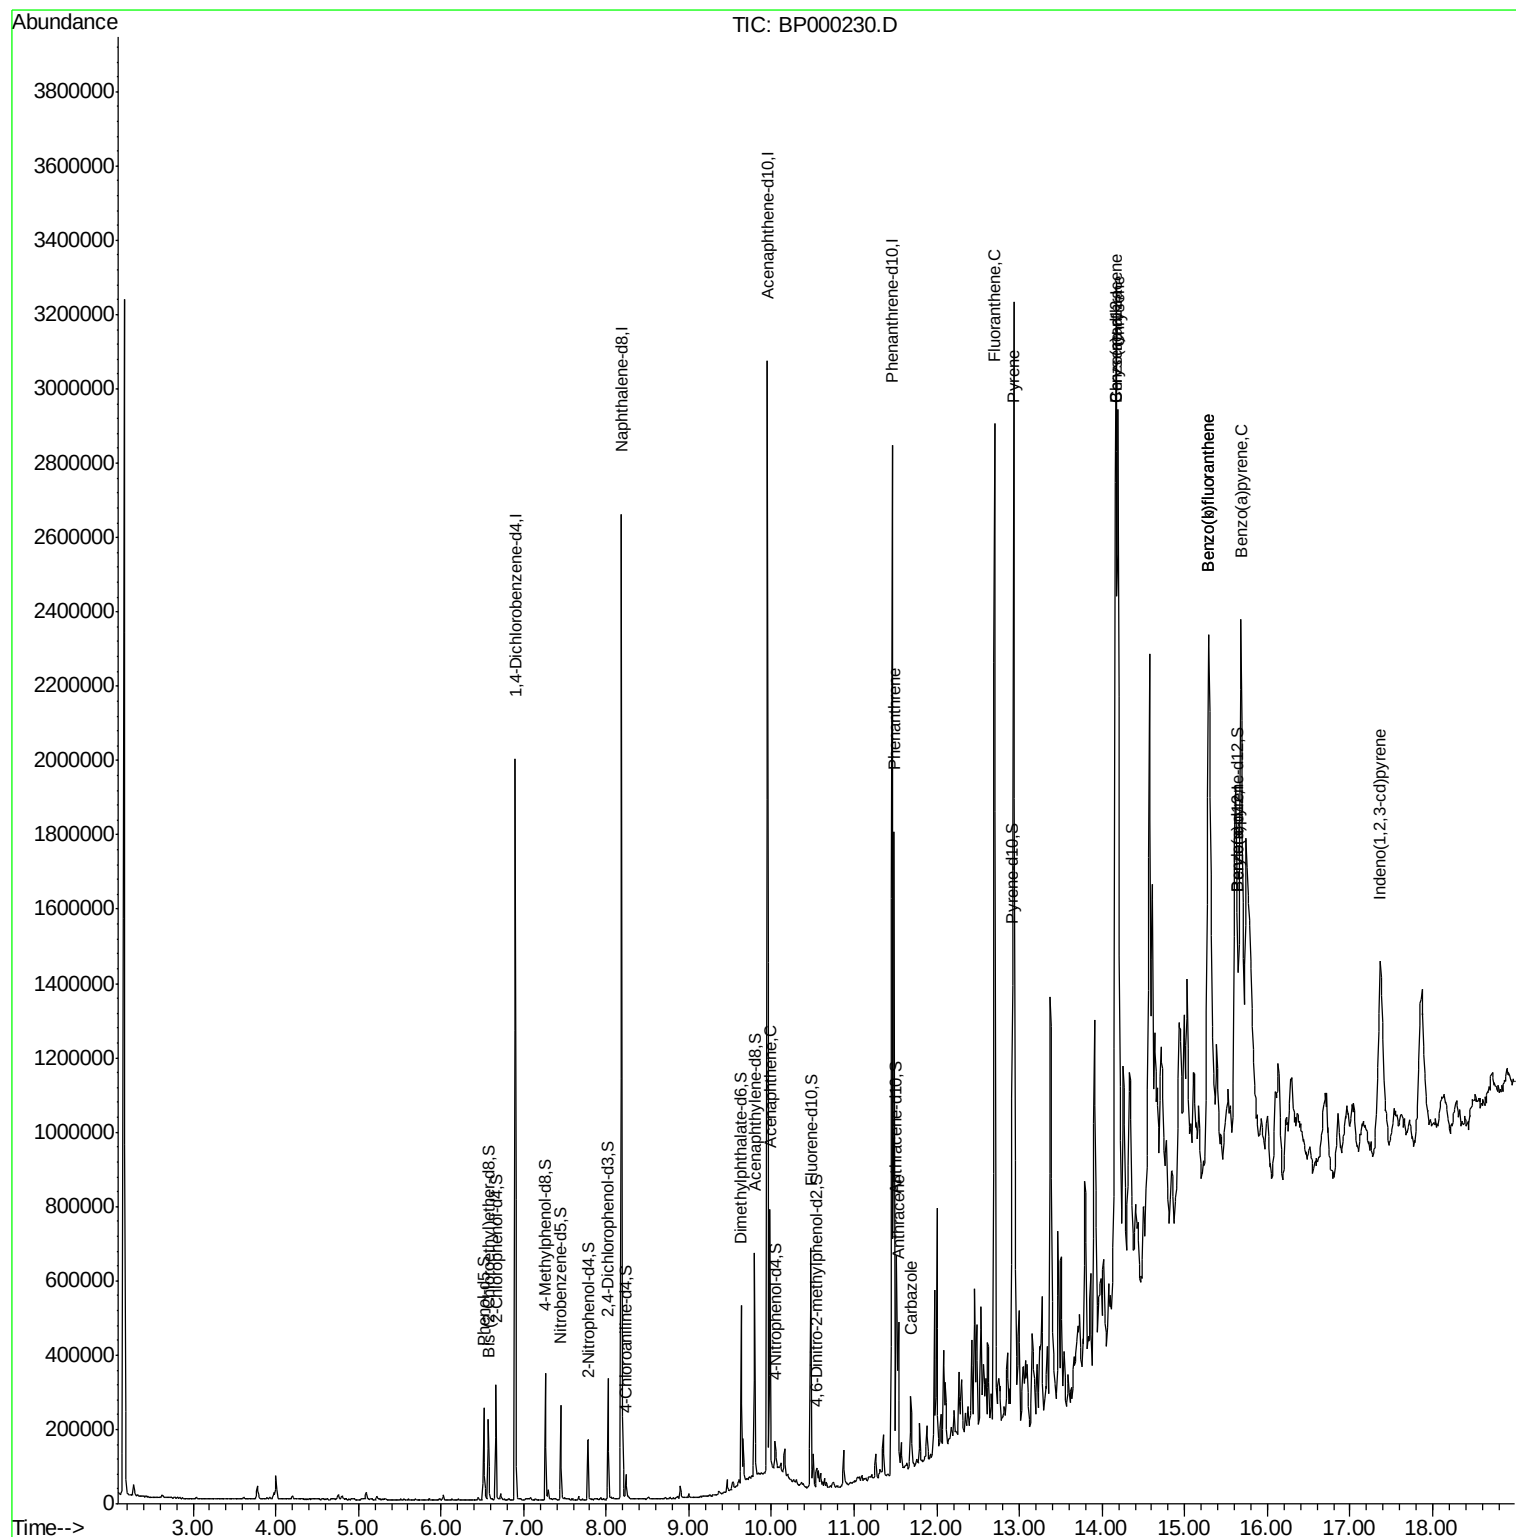

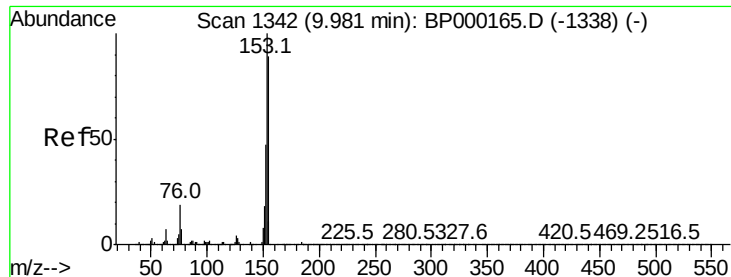

#50

Acenaphthene

Concen: 4.289 ng/ul

RT: 9.98 min Scan# 1342

Delta R.T. 0.00 min

Lab File: BP000230.D

Acq: 12 Sep 2019 21:47

Instrument :

BNA_P

ClientSampled :


Tot Ion:153 Resp: 158363

Ion Ratio Lower Upper

153 100

152 47.1 38.0 57.0




154 92.1 72.6 108.8

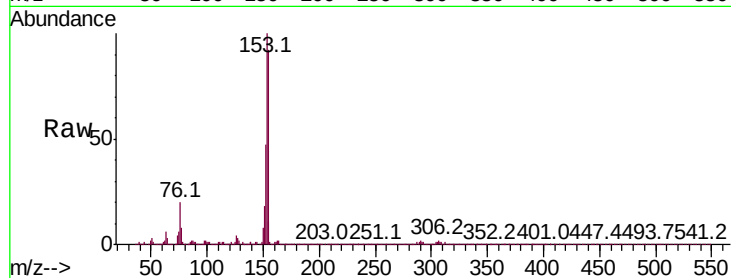

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

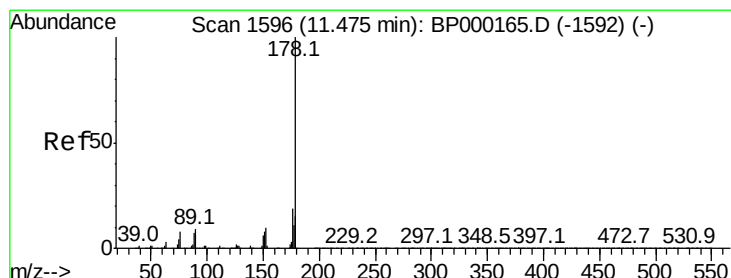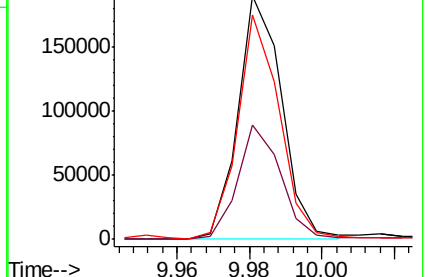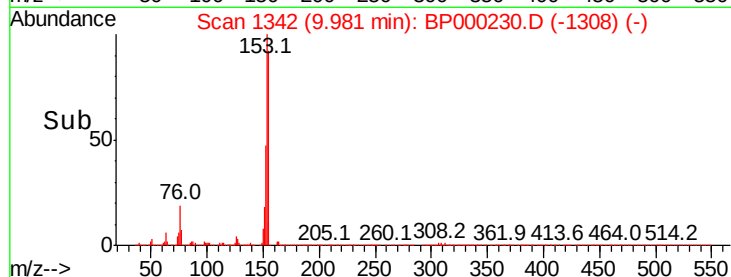

#70

Phenanthrene

Concen: 10.133 ng/ul

RT: 11.48 min Scan# 1597

Delta R.T. 0.01 min

Lab File: BP000230.D

Acq: 12 Sep 2019 21:47


Tgt Ion:178 Resp: 624630

Ion Ratio Lower Upper

178 100

179 16.1 12.5 18.7



176 19.6 15.7 23.5

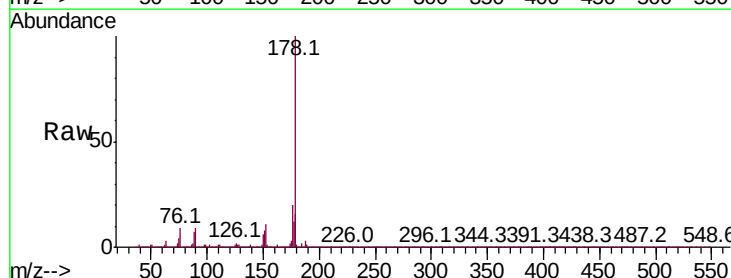


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

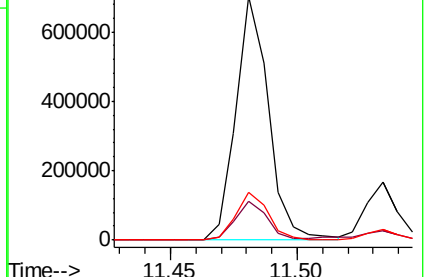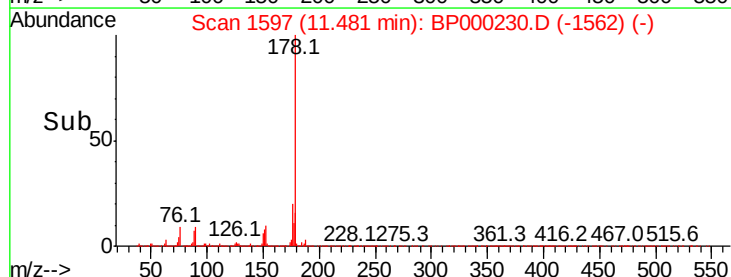

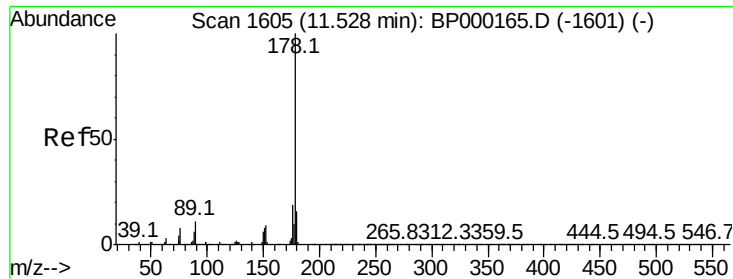

#72

Anthracene

Concen: 2.394 ng/ul

RT: 11.53 min Scan# 1606

Delta R.T. 0.01 min

Lab File: BP000230.D

Acq: 12 Sep 2019 21:47





Instrument :

BNA_P

ClientSampleId :

Tot Ion:178 Resp: 145190

Ion	Ratio	Lower	Upper
178	100		
179	16.7	12.3	18.5
176	19.2	15.1	22.7

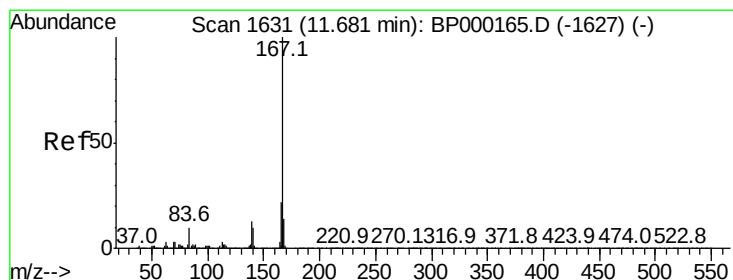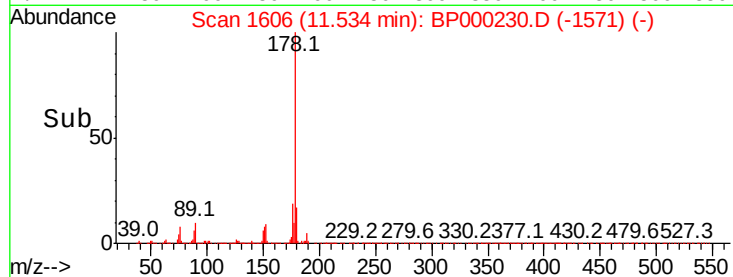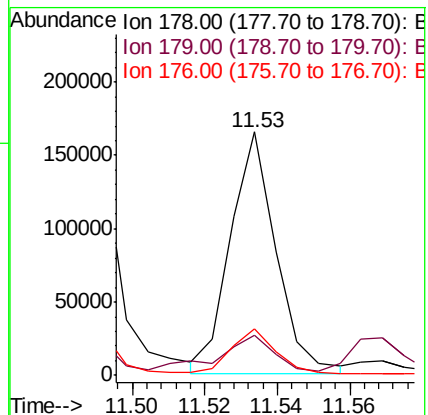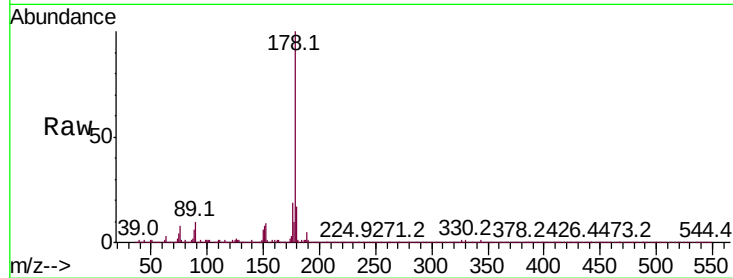

#75

Carbazole

Concen: 1.590 ng/ul

RT: 11.69 min Scan# 1632




Delta R.T. 0.01 min


Lab File: BP000230.D

Acq: 12 Sep 2019 21:47

Tgt Ion:167 Resp: 82451

Ion	Ratio	Lower	Upper
167	100		
166	23.5	17.3	25.9
139	14.4	10.6	15.8

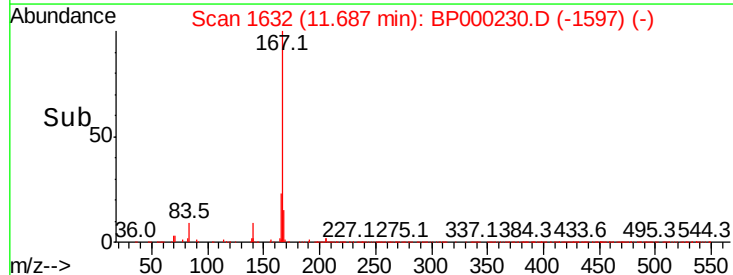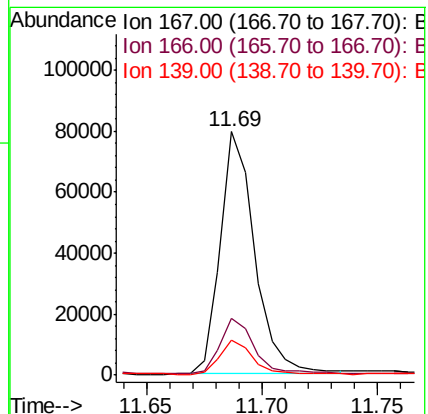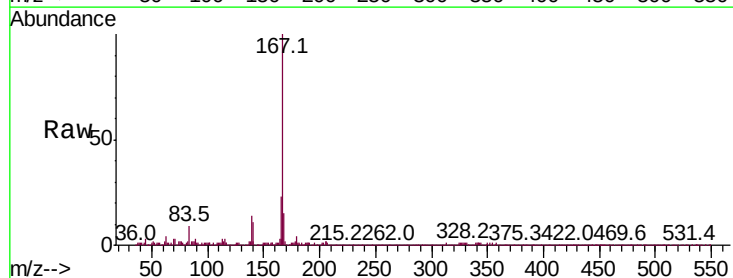




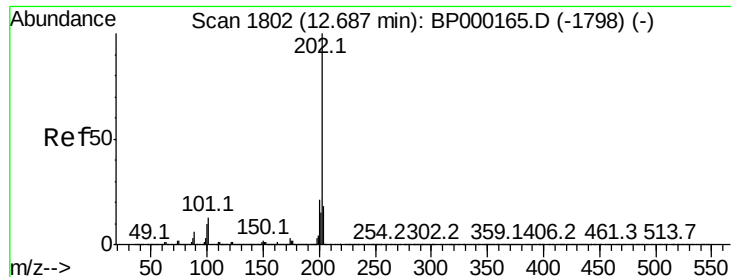


#77
 Fluoranthene
 Concen: 20.387 ng/ul
 RT: 12.70 min Scan# 1804
 Delta R.T. 0.01 min
 Lab File: BP000230.D
 Acq: 12 Sep 2019 21:47

Instrument :
 BNA_P
 ClientSampleId :

Tot Ion:202 Resp: 1267579




Ion	Ratio	Lower	Upper
202	100		
101	11.9	10.0	15.0
100	8.9	7.4	11.2

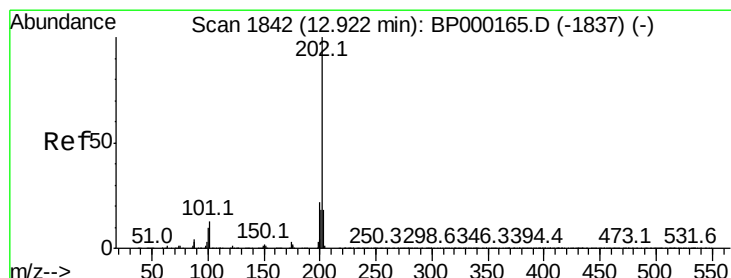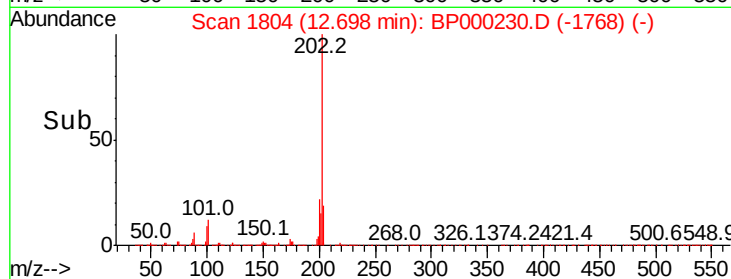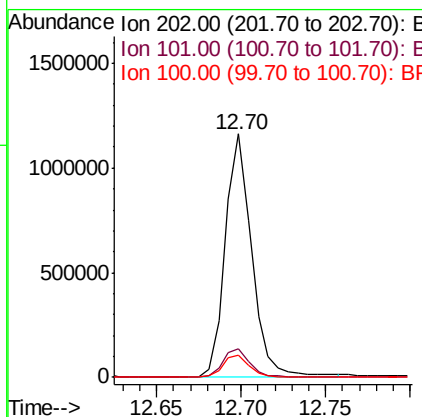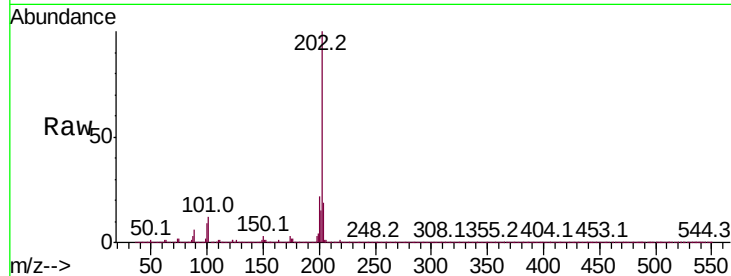


#80
 Pyrene
 Concen: 26.039 ng/ul
 RT: 12.93 min Scan# 1844
 Delta R.T. 0.02 min
 Lab File: BP000230.D
 Acq: 12 Sep 2019 21:47

Tgt Ion:202 Resp: 1542557

Ion	Ratio	Lower	Upper
202	100		
101	12.6	13.4	20.0#
100	10.3	10.8	16.2#

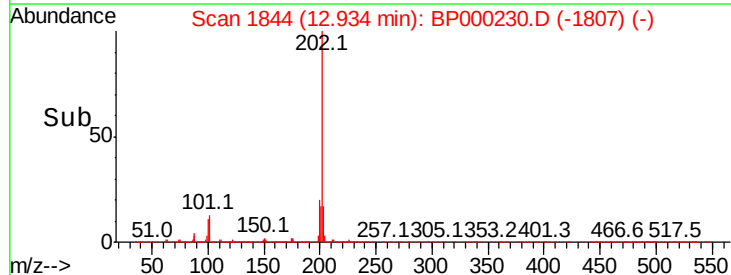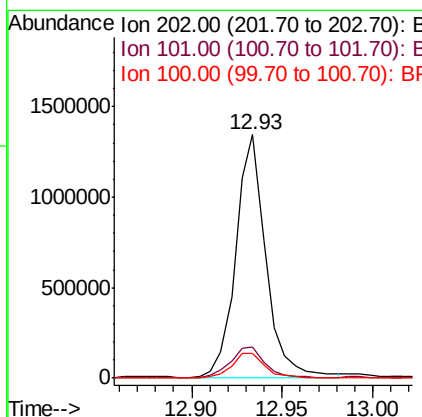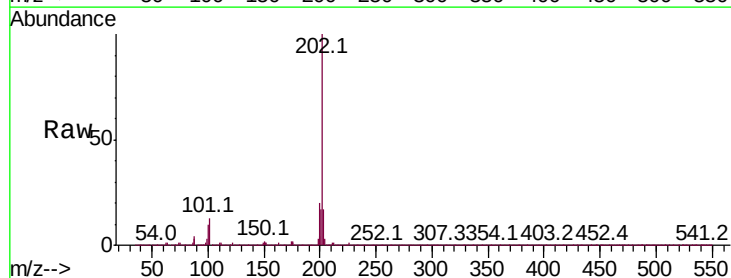

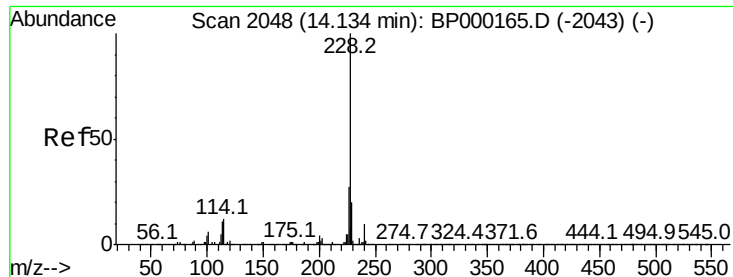

#83

Benzo(a)anthracene

Concen: 18.918 ng/ul

RT: 14.16 min Scan# 2052

Delta R.T. 0.02 min

Lab File: BP000230.D

Acq: 12 Sep 2019 21:47

Instrument :

BNA_P

ClientSampled :


Tot Ion:228 Resp: 1075293

Ion Ratio Lower Upper

228 100

229 21.6 15.9 23.9




226 27.6 22.1 33.1

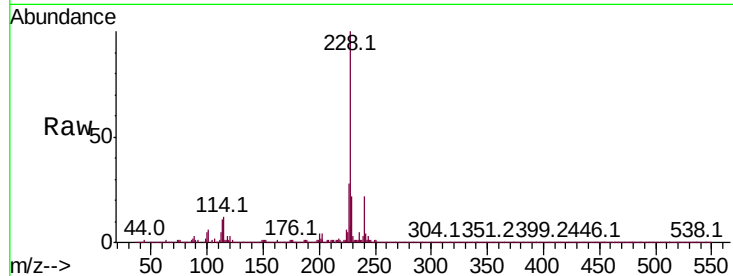

Abundance Ion 228.00 (227.70 to 228.70): E

1200000 Ion 229.00 (228.70 to 229.70): E

1000000 Ion 226.00 (225.70 to 226.70): E

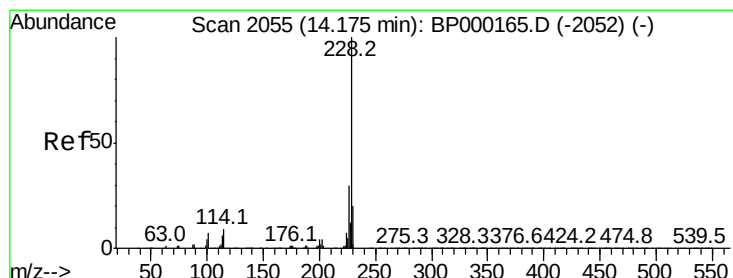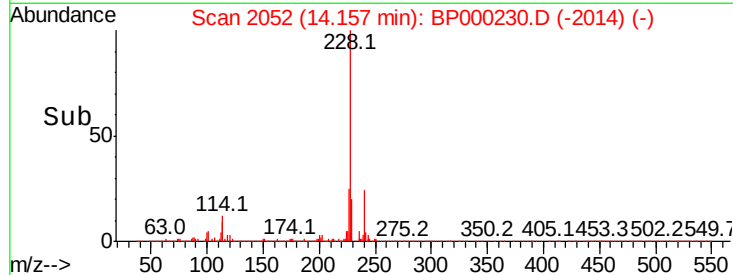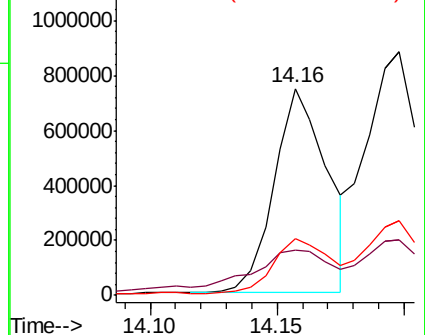

#85

Chrysene

Concen: 29.223 ng/ul

RT: 14.20 min Scan# 2059

Delta R.T. 0.03 min

Lab File: BP000230.D

Acq: 12 Sep 2019 21:47


Tgt Ion:228 Resp: 1524213

Ion Ratio Lower Upper

228 100

226 30.7 24.4 36.6



229 22.8 16.0 24.0

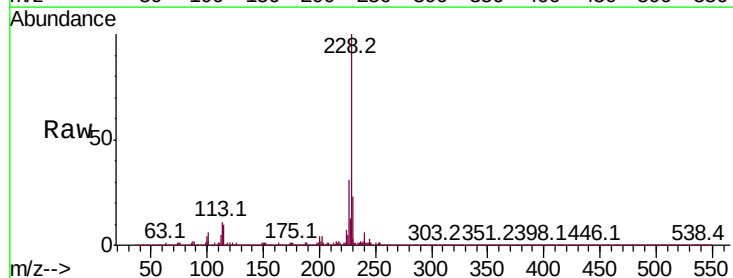


Abundance Ion 228.00 (227.70 to 228.70): E

1200000 Ion 226.00 (225.70 to 226.70): E

1000000 Ion 229.00 (228.70 to 229.70): E



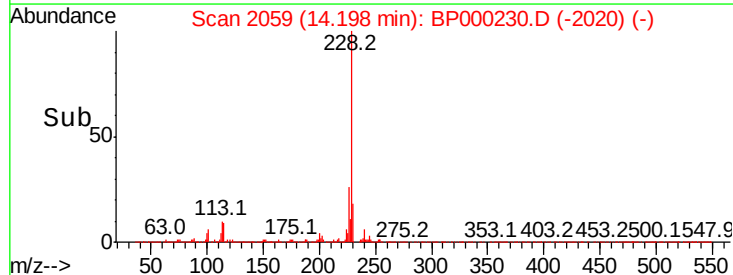
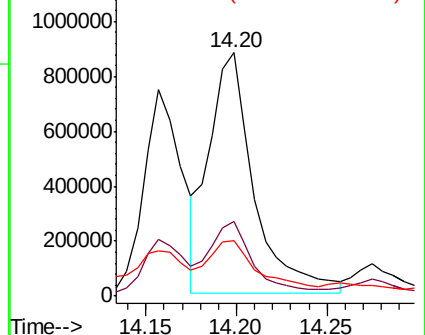


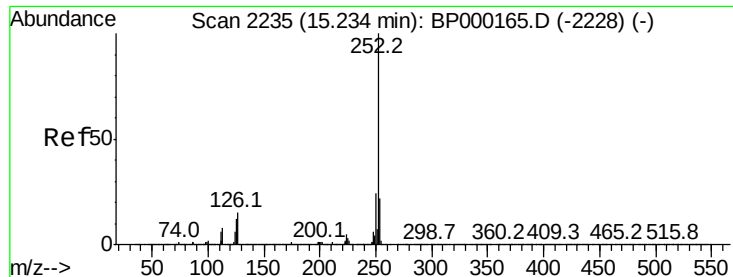

#88
Benzo(b)fluoranthene
Concen: 180.413 ng/ul
RT: 15.29 min Scan# 2244
Delta R.T. 0.06 min
Lab File: BP000230.D
Acq: 12 Sep 2019 21:47




Instrument :
BNA_P
ClientSampleId :


Tot Ion:252 Resp: 1909007
Ion Ratio Lower Upper
252 100
253 22.9 17.5 26.3
125 11.3 9.9 14.9

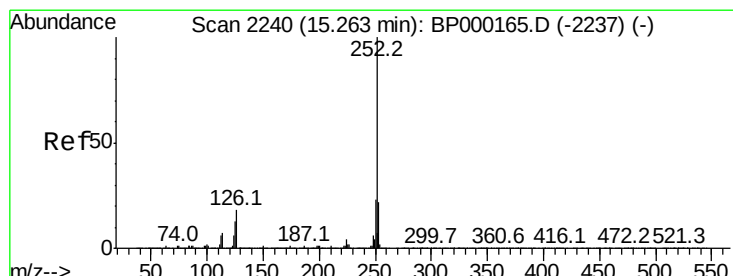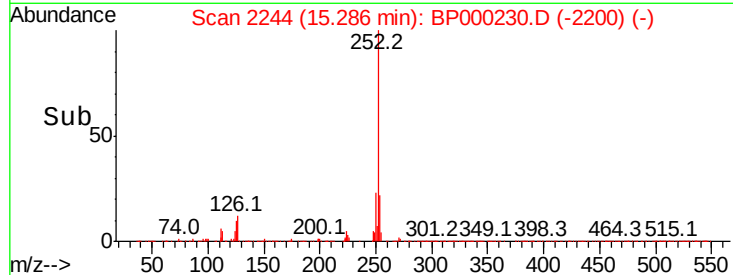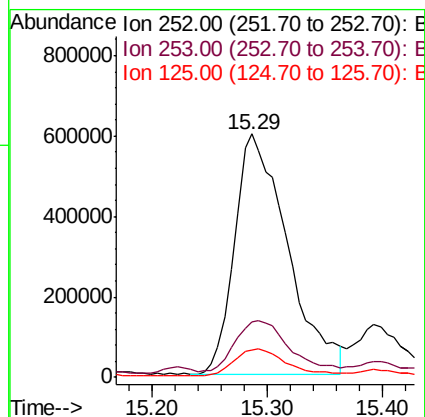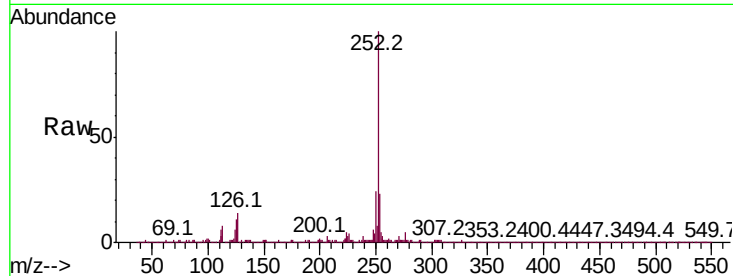

#89
Benzo(k)fluoranthene
Concen: 193.589 ng/ul
RT: 15.29 min Scan# 2244
Delta R.T. 0.03 min
Lab File: BP000230.D
Acq: 12 Sep 2019 21:47

Tgt Ion:252 Resp: 1930935
Ion Ratio Lower Upper
252 100
253 22.9 18.0 27.0
125 11.3 10.2 15.2


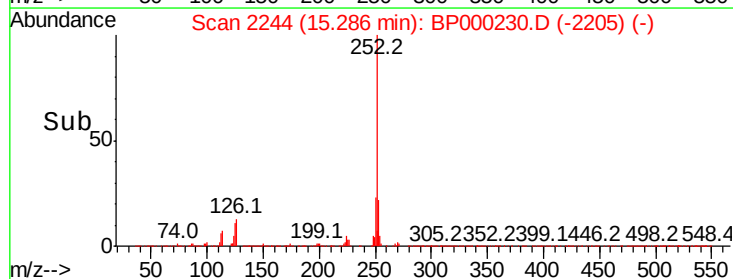
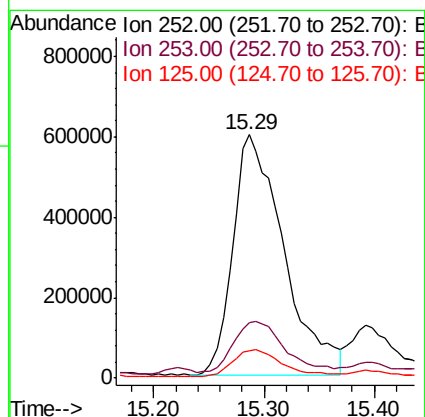
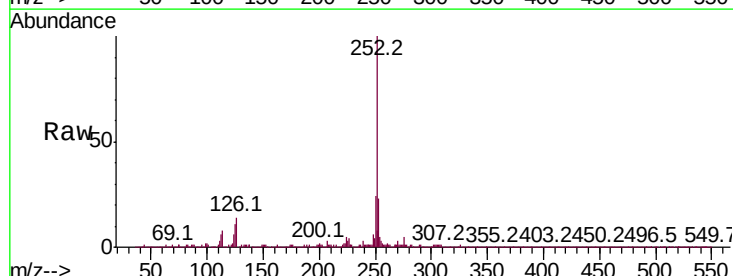


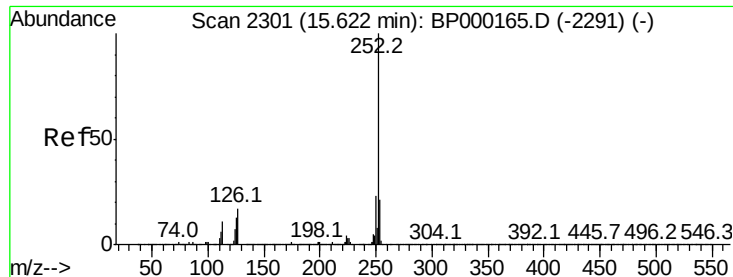

#91
Benzo(a)pyrene
Concen: 115.600 ng/ul
RT: 15.68 min Scan# 2311
Delta R.T. 0.06 min
Lab File: BP000230.D
Acq: 12 Sep 2019 21:47

Instrument :
BNA_P
ClientSampleId :

Tot Ion:252 Resp: 1147660
Ion Ratio Lower Upper
252 100
253 24.3 17.5 26.3
125 11.8 10.2 15.2

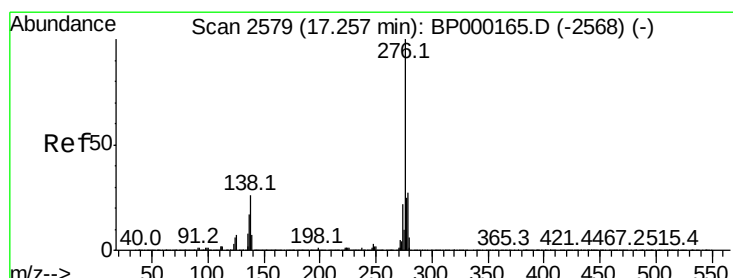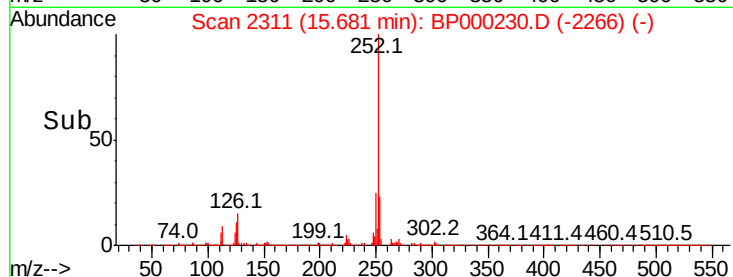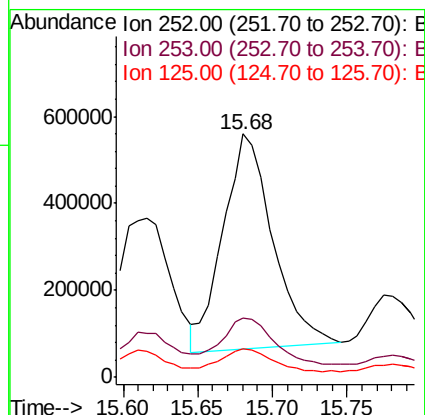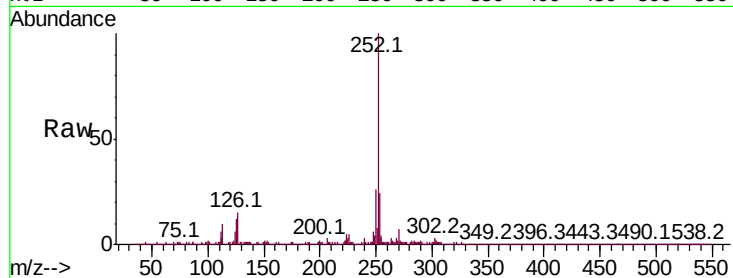

#92
Indeno(1,2,3-cd)pyrene
Concen: 38.049 ng/ul
RT: 17.36 min Scan# 2597
Delta R.T. 0.11 min
Lab File: BP000230.D
Acq: 12 Sep 2019 21:47

Tgt Ion:276 Resp: 434567
Ion Ratio Lower Upper
276 100
138 26.6 20.0 30.0
277 27.5 19.4 29.0

