


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091219\
Data File : BP000225.D
Acq On : 12 Sep 2019 19:45
Operator : HP/JU
Sample : K4633-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampled :
F2D12

Manual Integrations
APPROVED

mohammad
9/16/2019 9:09:36 AM

Quant Time: Sep 13 14:28:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 02:43:18 2019
Response via : Initial Calibration

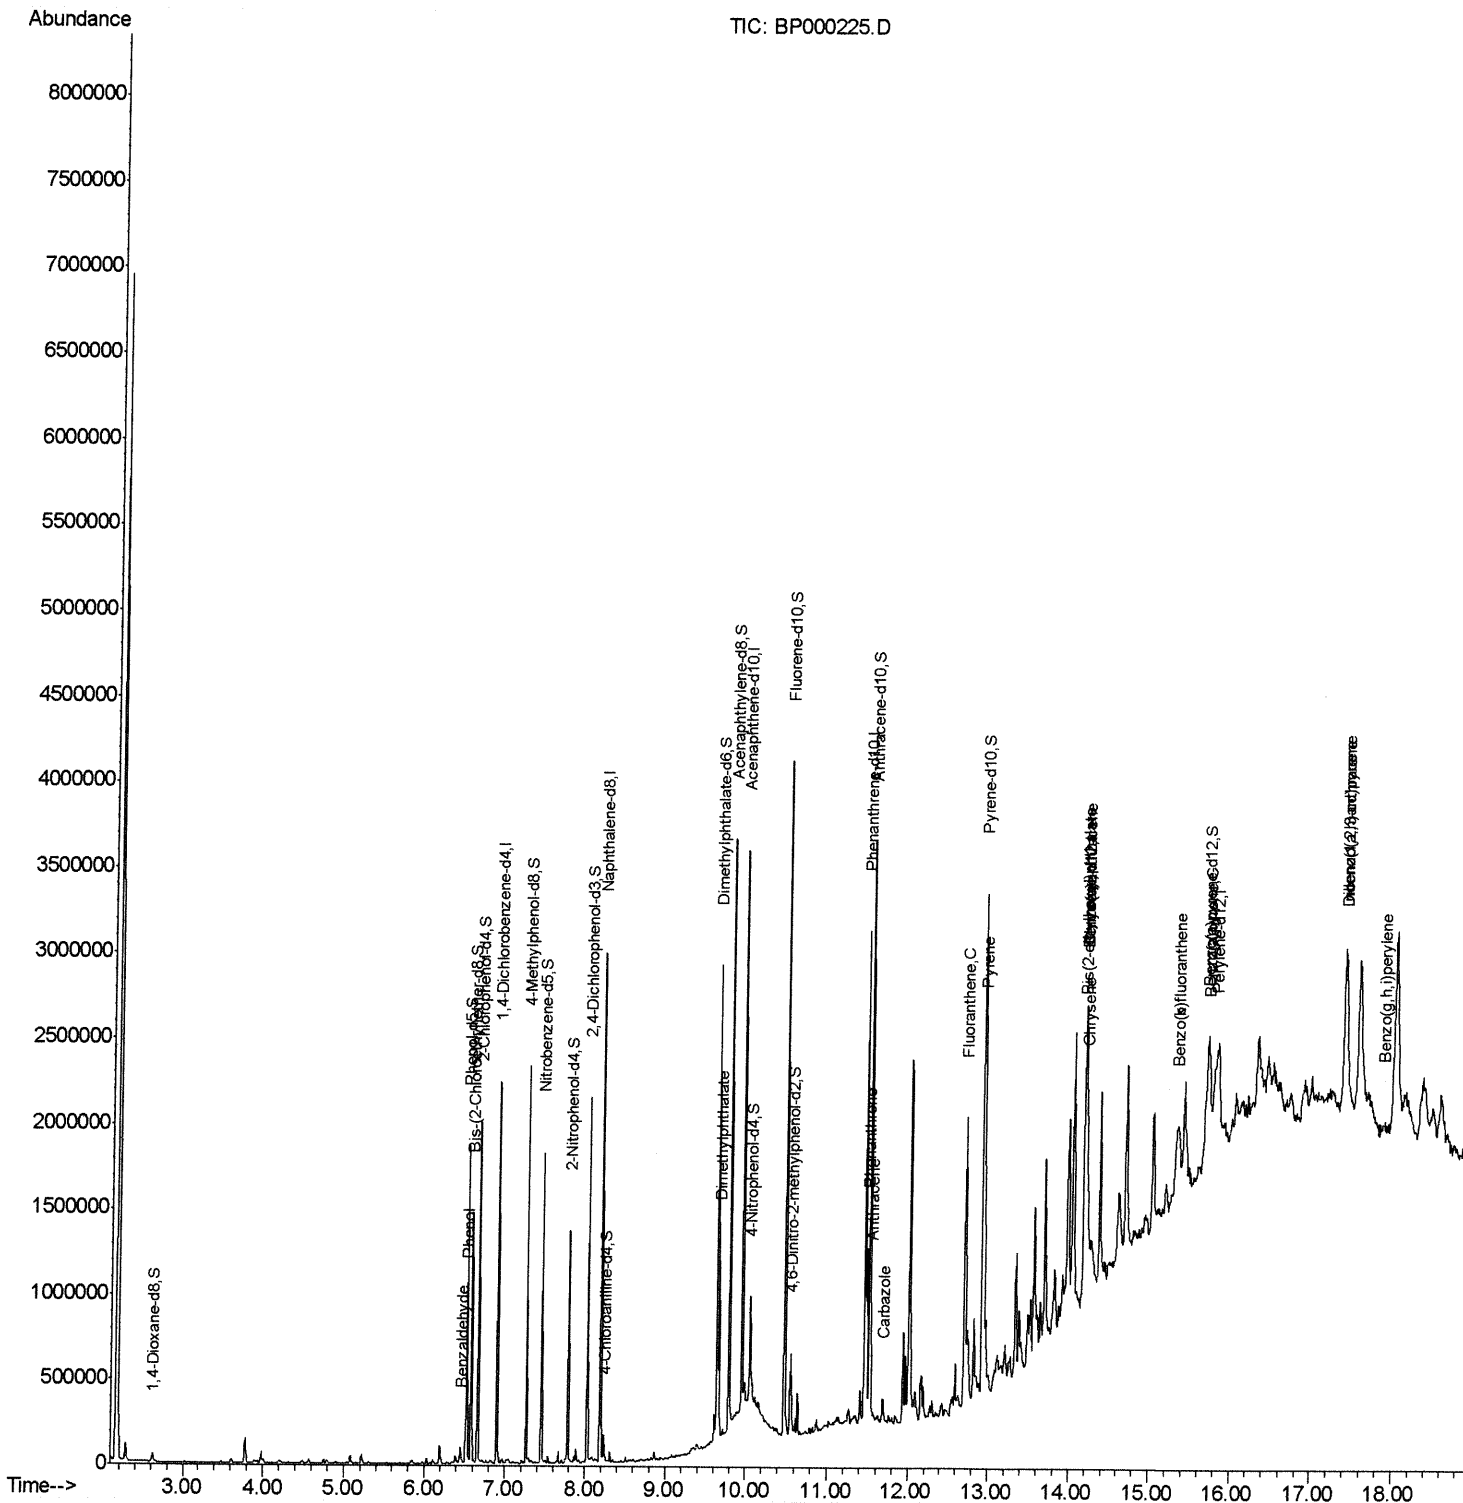



Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091219\
Data File : BP000225.D
Acq On : 12 Sep 2019 19:45
Operator : HP/JU
Sample : K4633-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F2D12

Manual Integrations
APPROVED

mohammad
9/16/2019 9:09:36 AM

Quant Time: Sep 13 01:51:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 02:43:18 2019
Response via : Initial Calibration

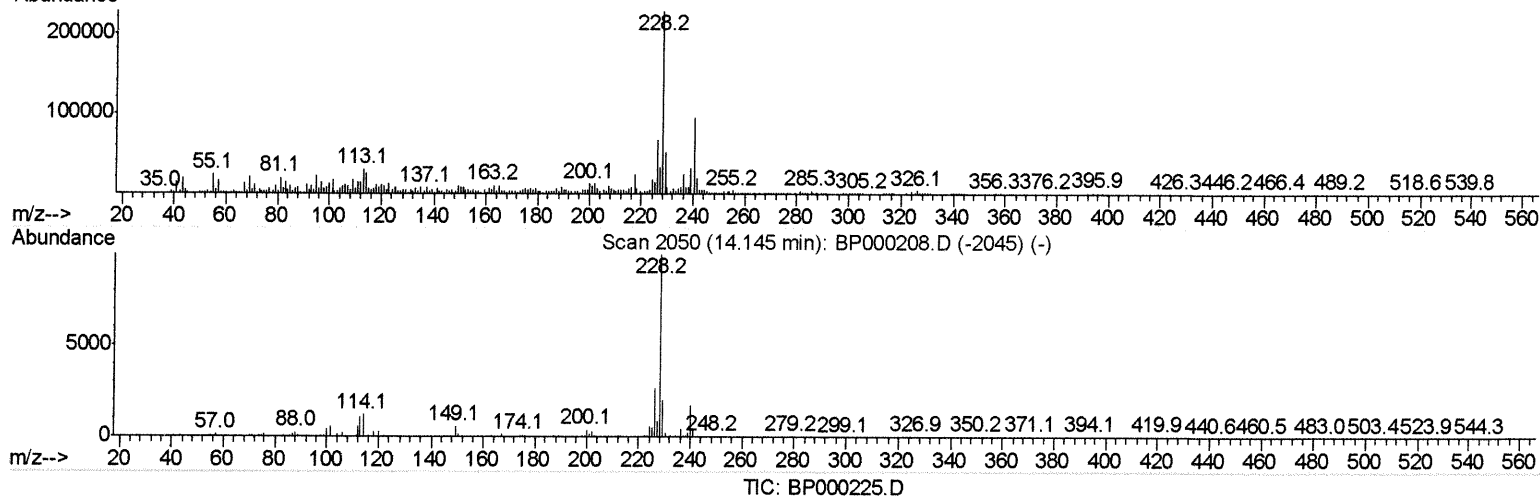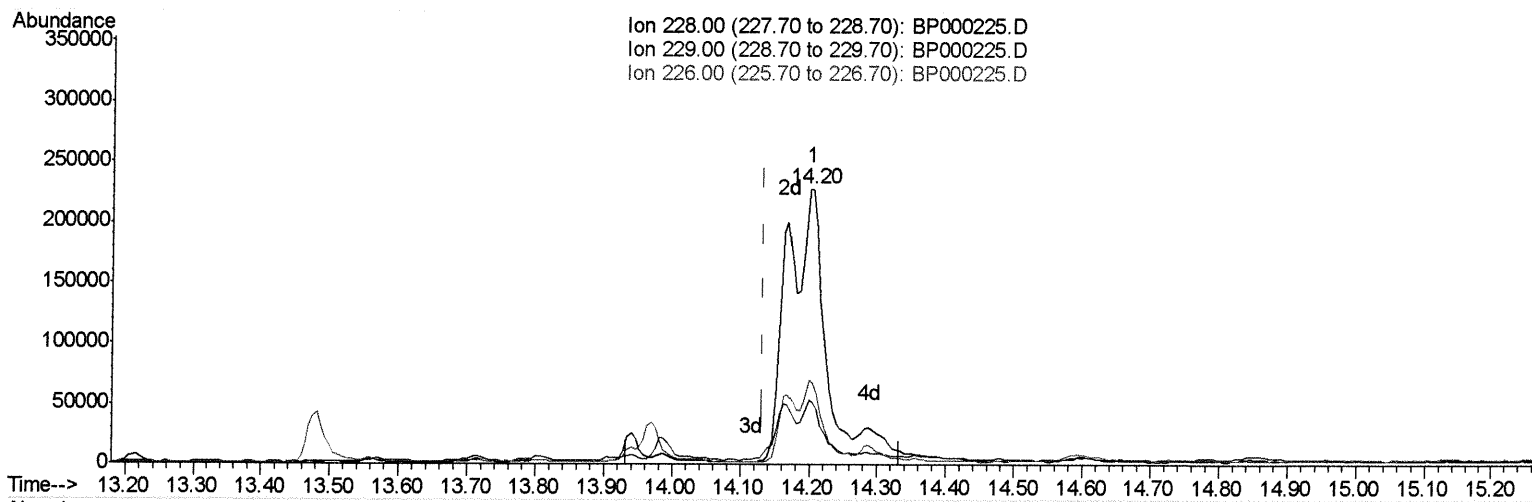

(83) Benzo(a)anthracene

14.204min (+0.071) 7.25ng/ul

response 477350

Ion	Exp%	Act%
228.00	100	100
229.00	19.90	22.95
226.00	27.60	29.42
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091219\
 Data File : BP000225.D
 Acq On : 12 Sep 2019 19:45
 Operator : HP/JU
 Sample : K4633-13
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F2D12

Manual Integrations
 APPROVED

mohammad
 9/16/2019 9:09:36 AM

Quant Time: Sep 13 01:51:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 02:43:18 2019
 Response via : Initial Calibration

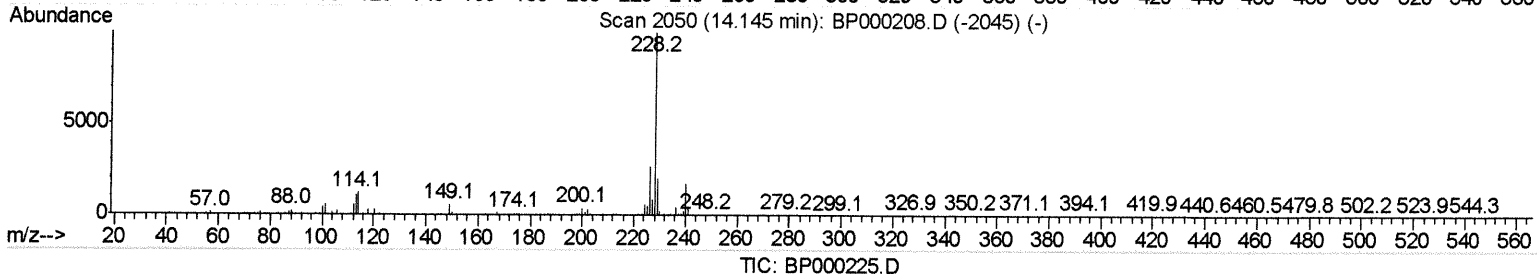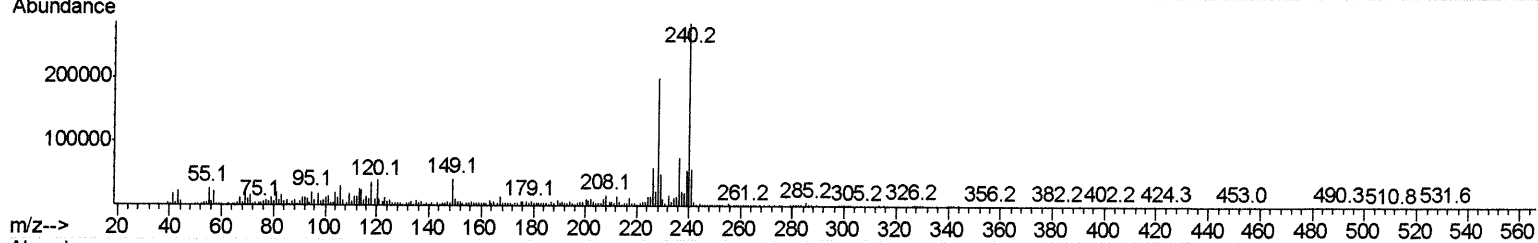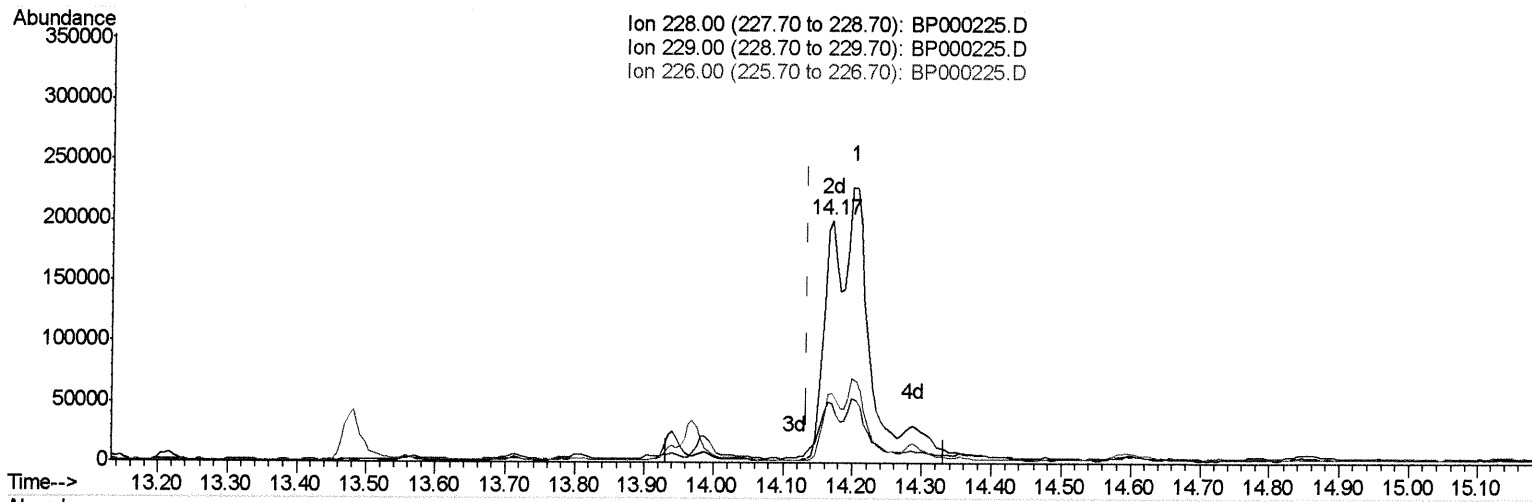

(83) Benzo(a)anthracene

14.169min (+0.035) 4.78ng/ul m *JU 09/17/19*

response 314962

Ion	Exp%	Act%
228.00	100	100
229.00	19.90	24.63#
226.00	27.60	29.05
0.00	0.00	0.00



Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091219\
Data File : BP000225.D
Acq On : 12 Sep 2019 19:45
Operator : HP/JU
Sample : K4633-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F2D12


Manual Integrations
APPROVED

mohammad
9/16/2019 9:09:36 AM

Quant Time: Sep 13 01:51:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 02:43:18 2019
Response via : Initial Calibration

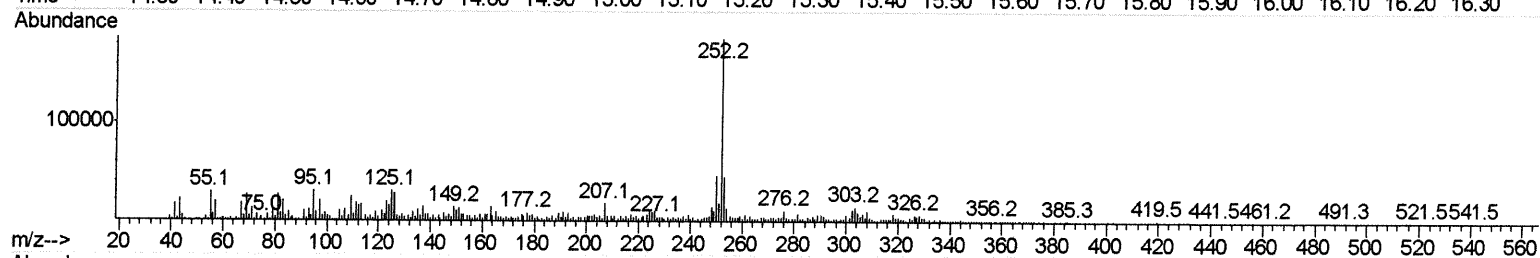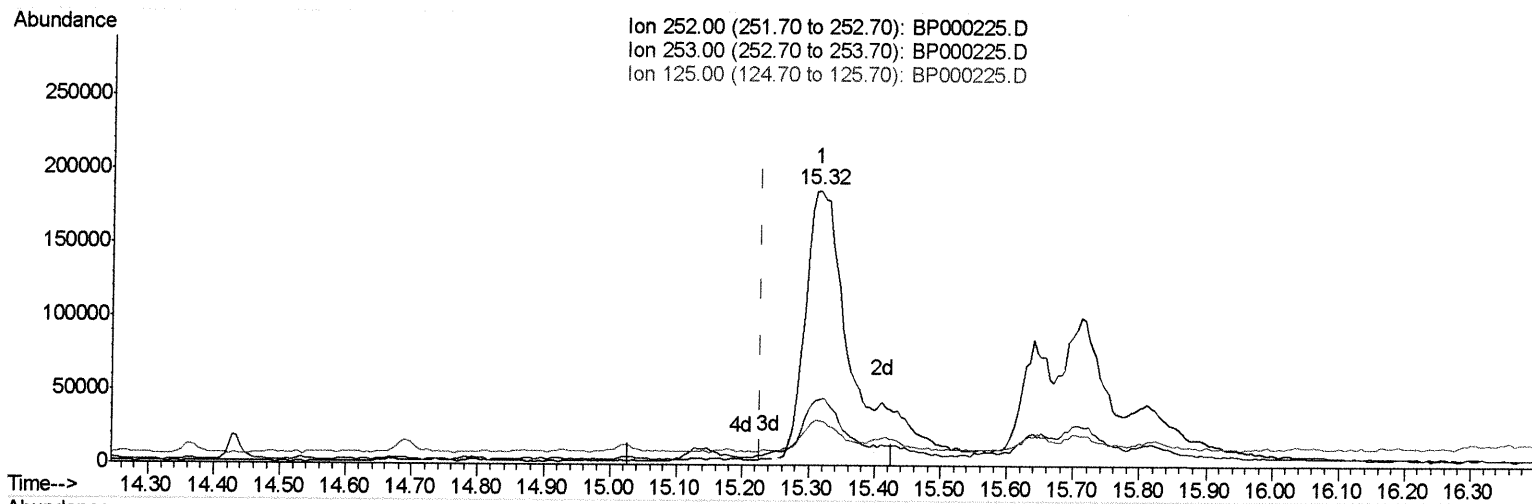

Scan 2238 (15.251 min): BP000208.D (-2230) (-)

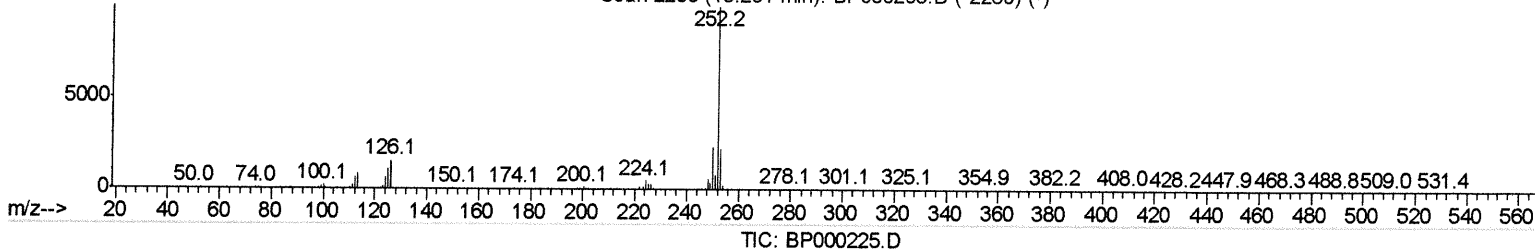

(88) Benzo(b)fluoranthene

15.316min (+0.088) 13.52ng/ul

response 756646

Ion	Exp%	Act%
252.00	100	100
253.00	21.90	23.92
125.00	12.40	16.33#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP091219\

Data File : BP000225.D

Acq On : 12 Sep 2019 19:45

Operator : HP/JU

Sample : K4633-13

Misc :

ALS Vial : 18 Sample Multiplier: 1

Quant Time: Sep 13 14:28:28 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Sep 10 02:43:18 2019




Response via : Initial Calibration

Instrument :

BNA_P

ClientSampleId :

F2D12

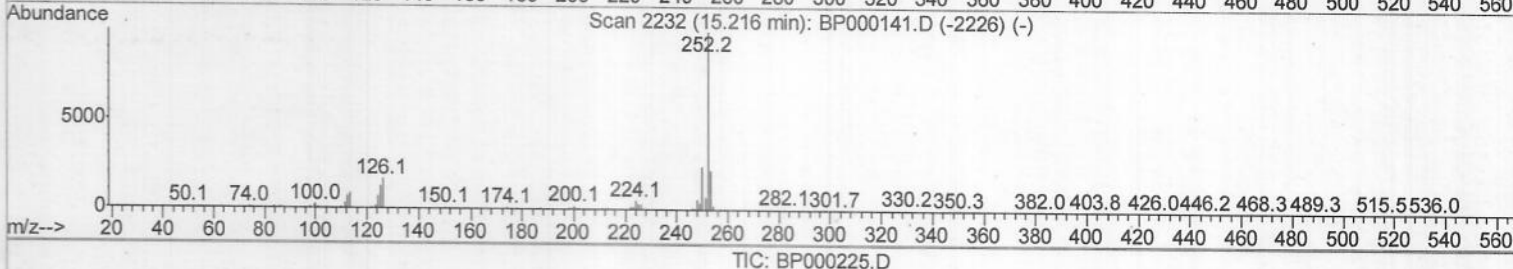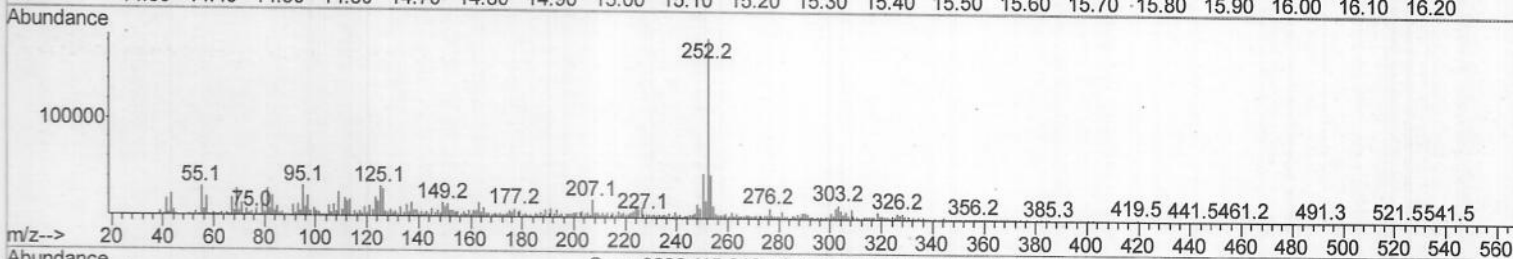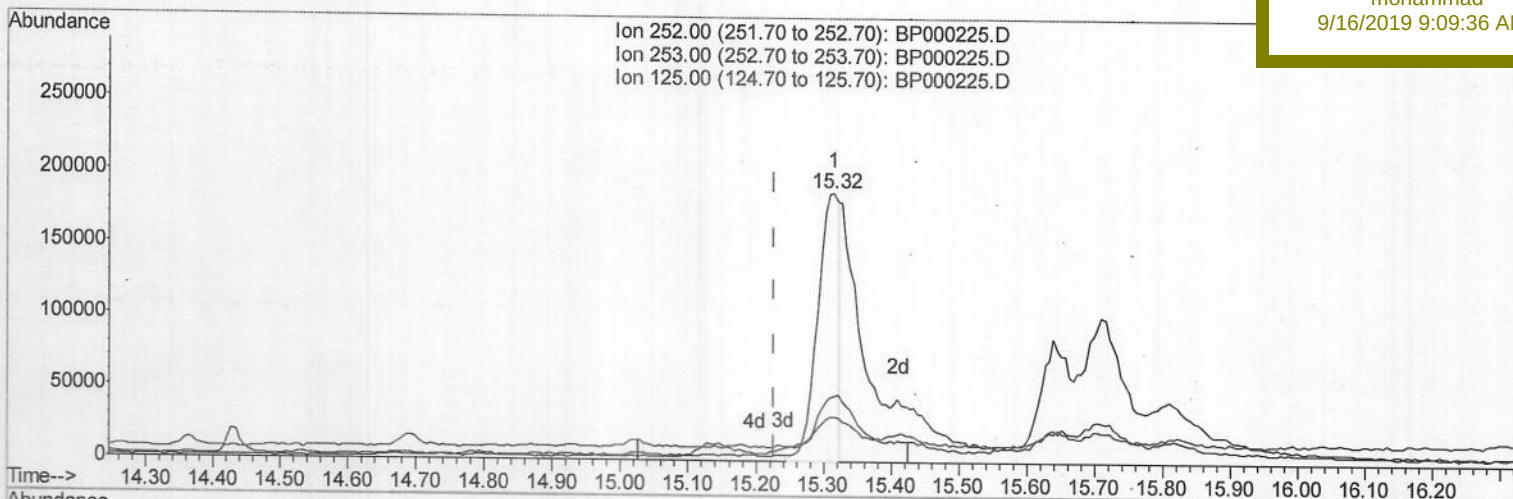Manual Integrations
APPROVEDmohammad
9/16/2019 9:09:36 AM

(88) Benzo(b)fluoranthene

15.316min (+0.088) 7.31ng/ul m

response 408829

Ion	Exp%	Act%
252.00	100	100
253.00	21.90	23.92
125.00	12.40	16.33#
0.00	0.00	0.00

JU
09/17/19



Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091219\
Data File : BP000225.D
Acq On : 12 Sep 2019 19:45
Operator : HP/JU
Sample : K4633-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F2D12

Manual Integrations
APPROVED

mohammad
9/16/2019 9:09:36 AM

Quant Time: Sep 13 01:51:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 02:43:18 2019
Response via : Initial Calibration

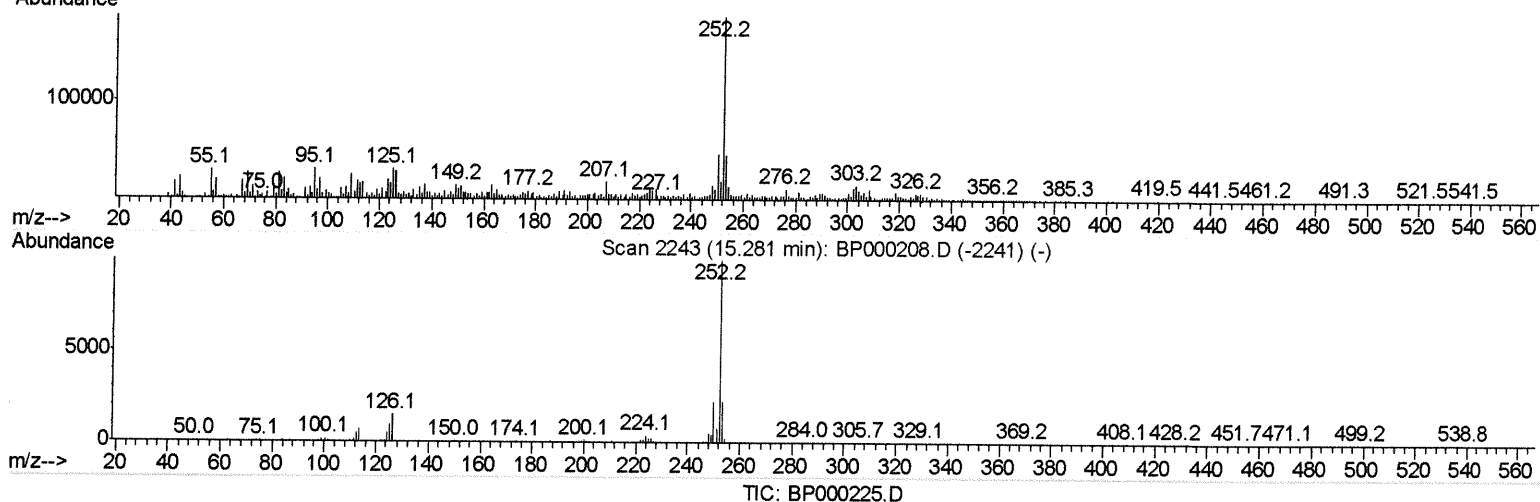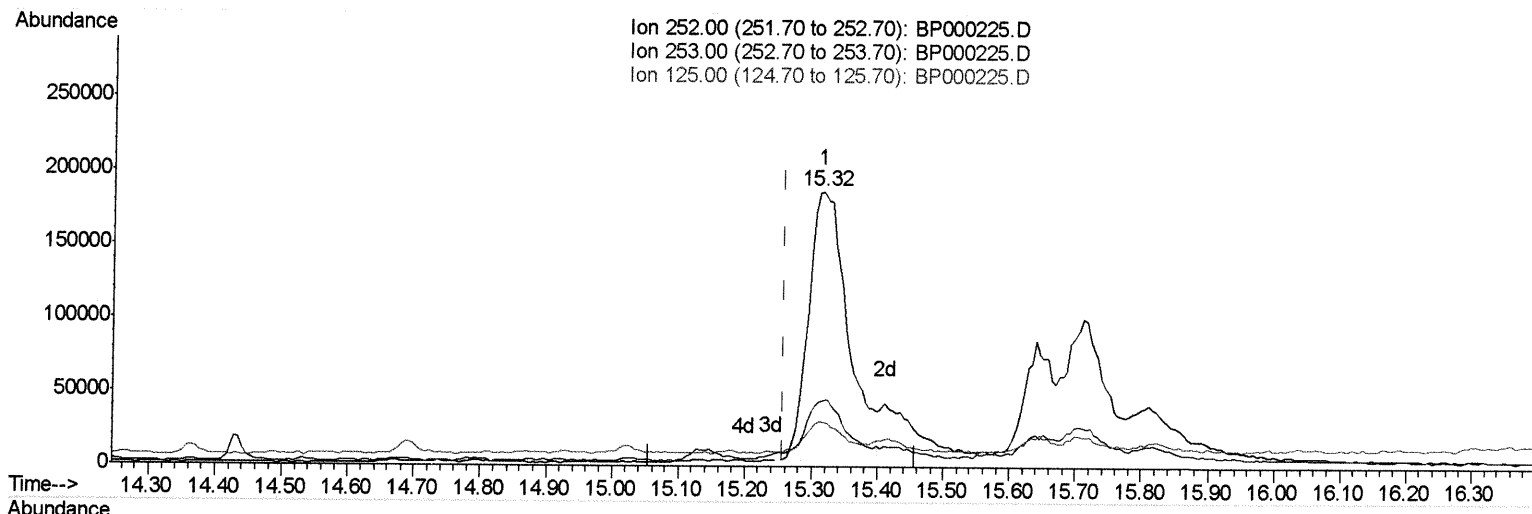

(89) Benzo(k)fluoranthene

15.316min (+0.059) 14.34ng/ul

response 756646

Ion	Exp%	Act%
252.00	100	100
253.00	22.50	23.92
125.00	12.70	16.33#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091219\
 Data File : BP000225.D
 Acq On : 12 Sep 2019 19:45
 Operator : HP/JU
 Sample : K4633-13
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F2D12

Manual Integrations
 APPROVED

mohammad
 9/16/2019 9:09:36 AM

Quant Time: Sep 13 01:51:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 02:43:18 2019
 Response via : Initial Calibration

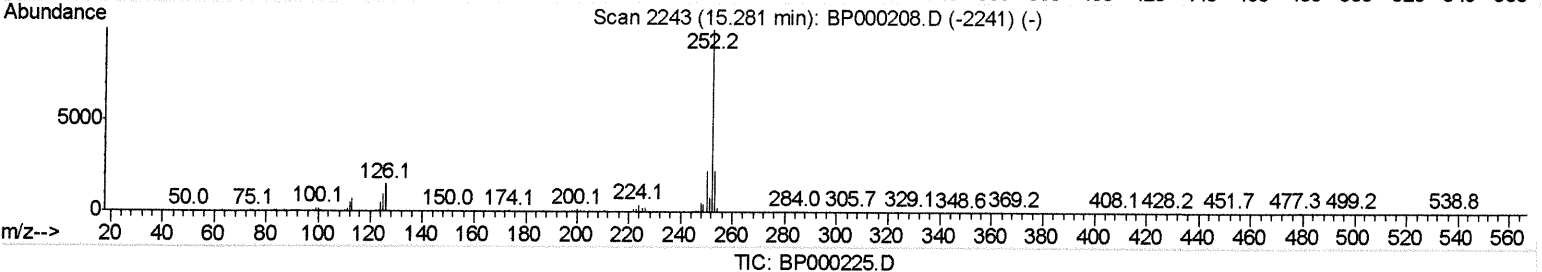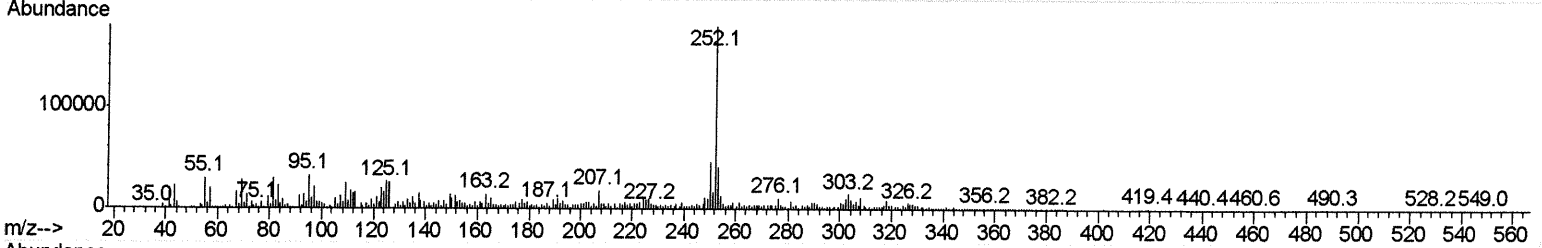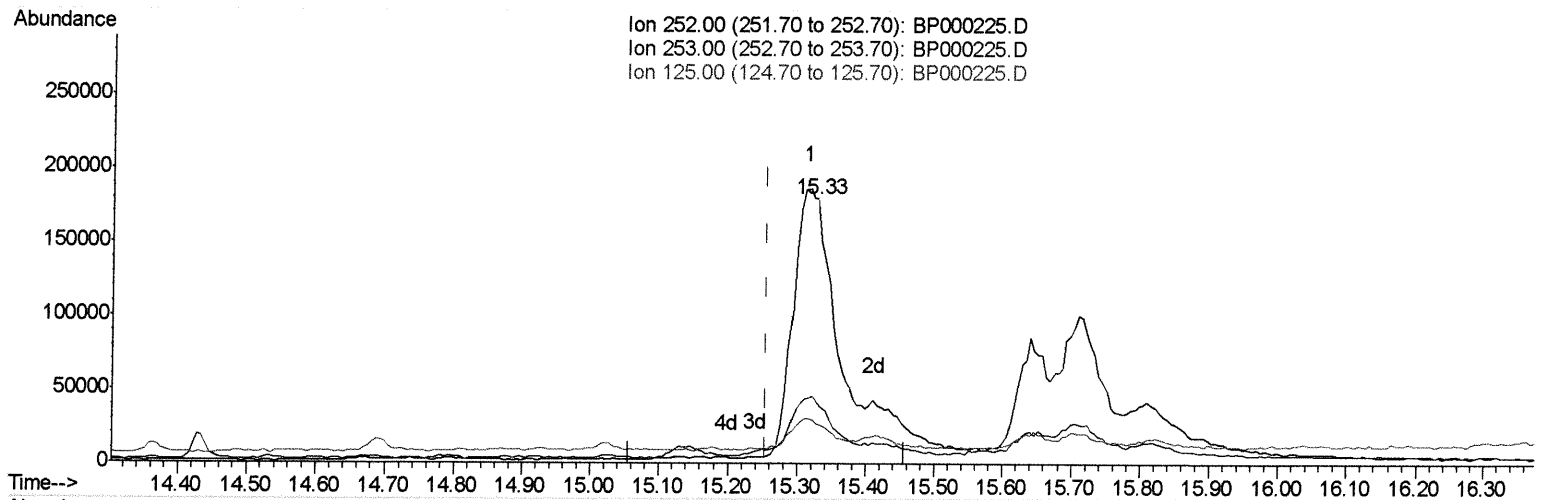

(89) Benzo(k)fluoranthene

15.328min (+0.071) 2.71ng/ul m

JU
 09/17/19

response 142793

Ion	Exp%	Act%
252.00	100	100
253.00	22.50	22.97
125.00	12.70	14.95
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091219\
 Data File : BP000225.D
 Acq On : 12 Sep 2019 19:45
 Operator : HP/JU
 Sample : K4633-13
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F2D12

Manual Integrations
 APPROVED

mohammad
 9/16/2019 9:09:36 AM

Quant Time: Sep 13 01:51:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 02:43:18 2019
 Response via : Initial Calibration

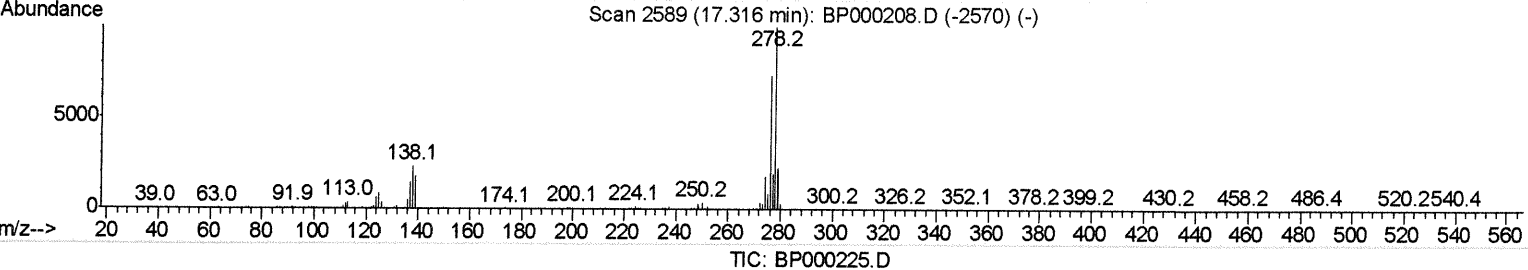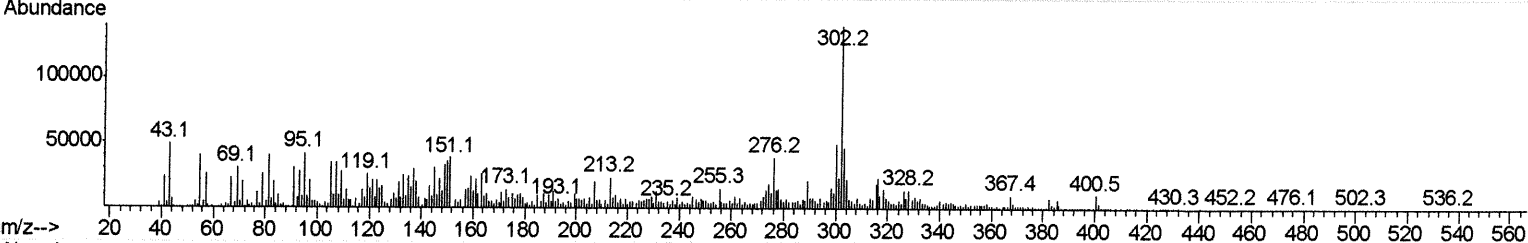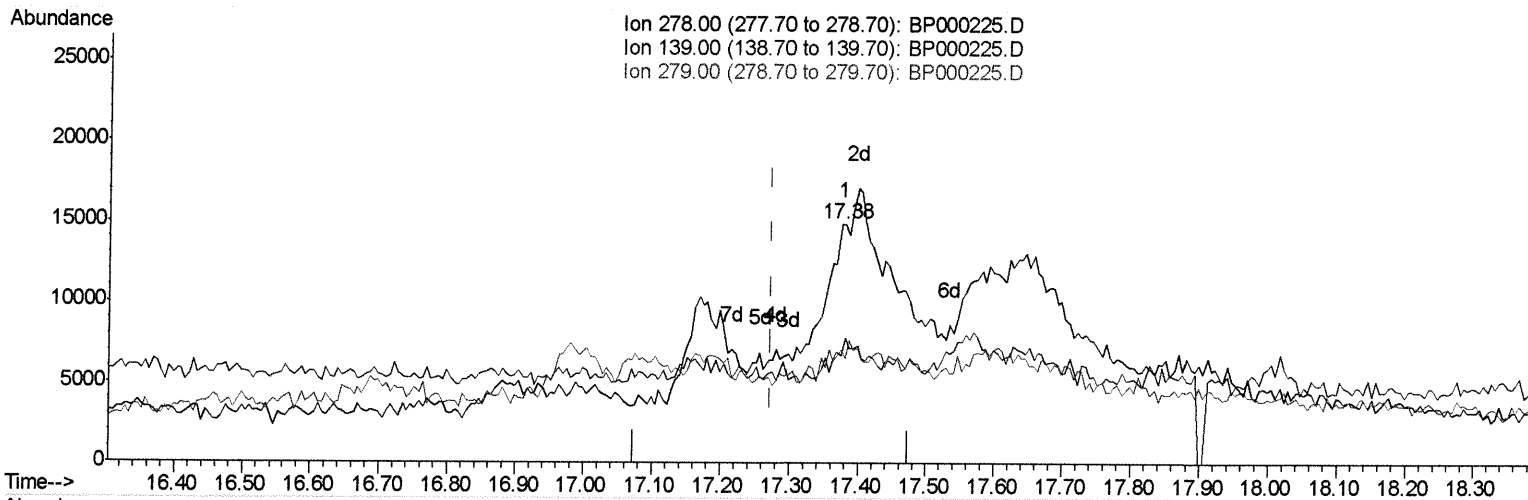

(93) Dibenzo(a,h)anthracene

17.381min (+0.106) 0.40ng/ul

response 19863

Ion	Exp%	Act%
278.00	100	100
139.00	18.90	52.02#
279.00	24.00	43.72#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091219\
Data File : BP000225.D
Acq On : 12 Sep 2019 19:45
Operator : HP/JU
Sample : K4633-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F2D12

Manual Integrations
APPROVED

mohammad
9/16/2019 9:09:36 AM

Quant Time: Sep 13 01:51:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 02:43:18 2019
Response via : Initial Calibration

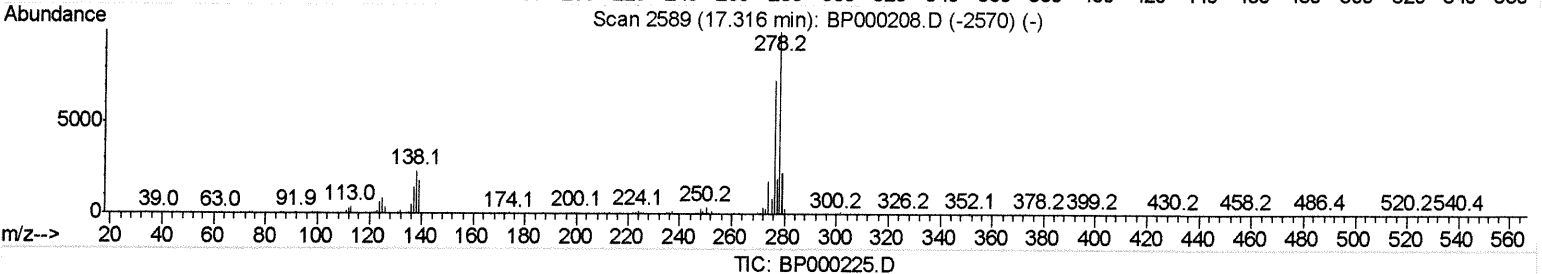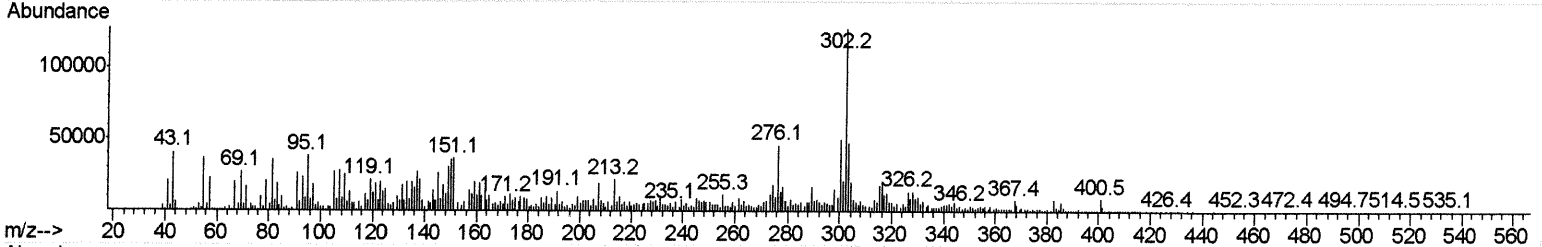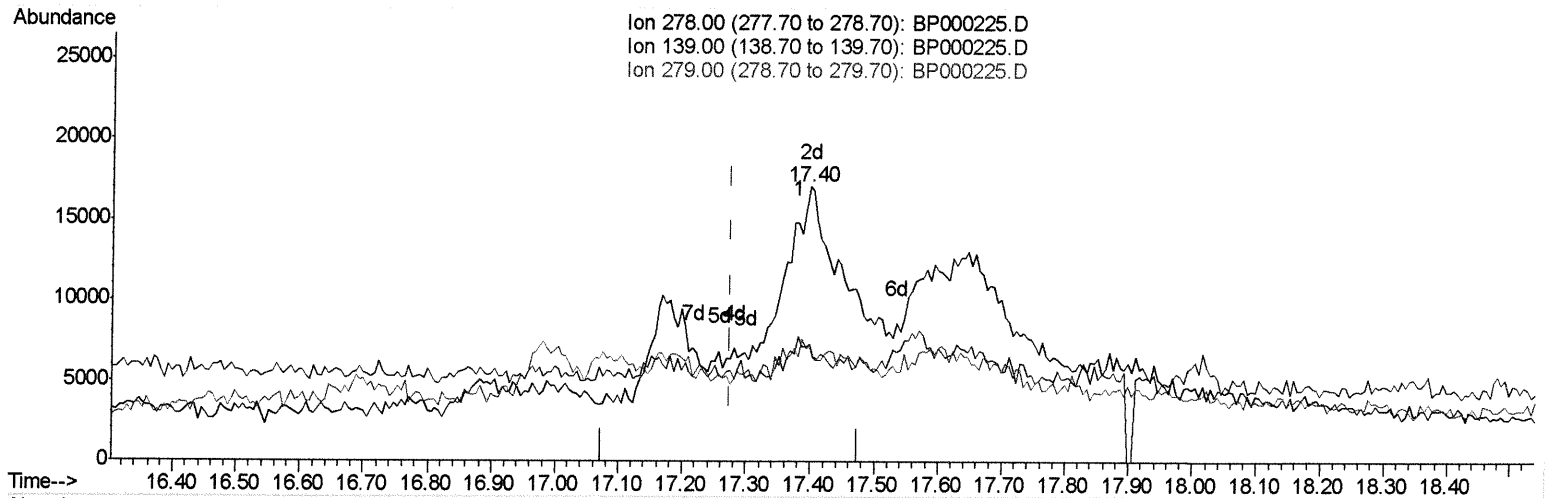

(93) Dibenzo(a,h)anthracene

17.398min (+0.124) 1.29ng/ul m

JU
09/17/19

response 64321

Ion	Exp%	Act%
278.00	100	100
139.00	18.90	42.76#
279.00	24.00	41.93#
0.00	0.00	0.00



Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091219\
Data File : BP000225.D
Acq On : 12 Sep 2019 19:45
Operator : HP/JU
Sample : K4633-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampled :
F2D12


Manual Integrations
APPROVED

mohammad
9/16/2019 9:09:36 AM

Quant Time: Sep 13 01:51:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 02:43:18 2019
Response via : Initial Calibration

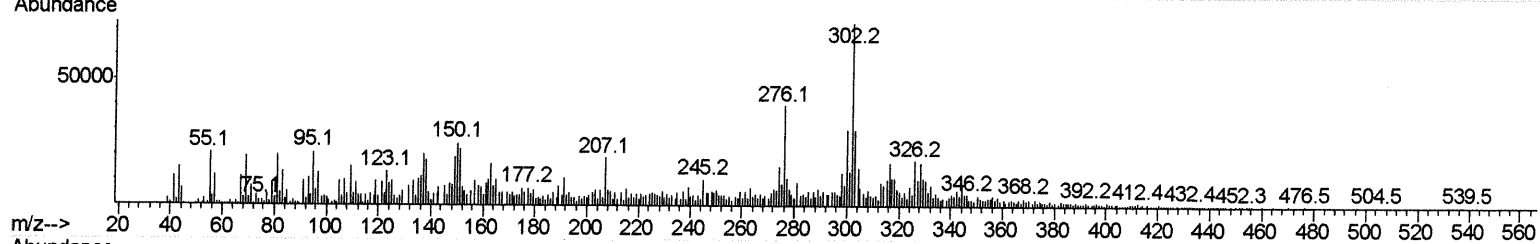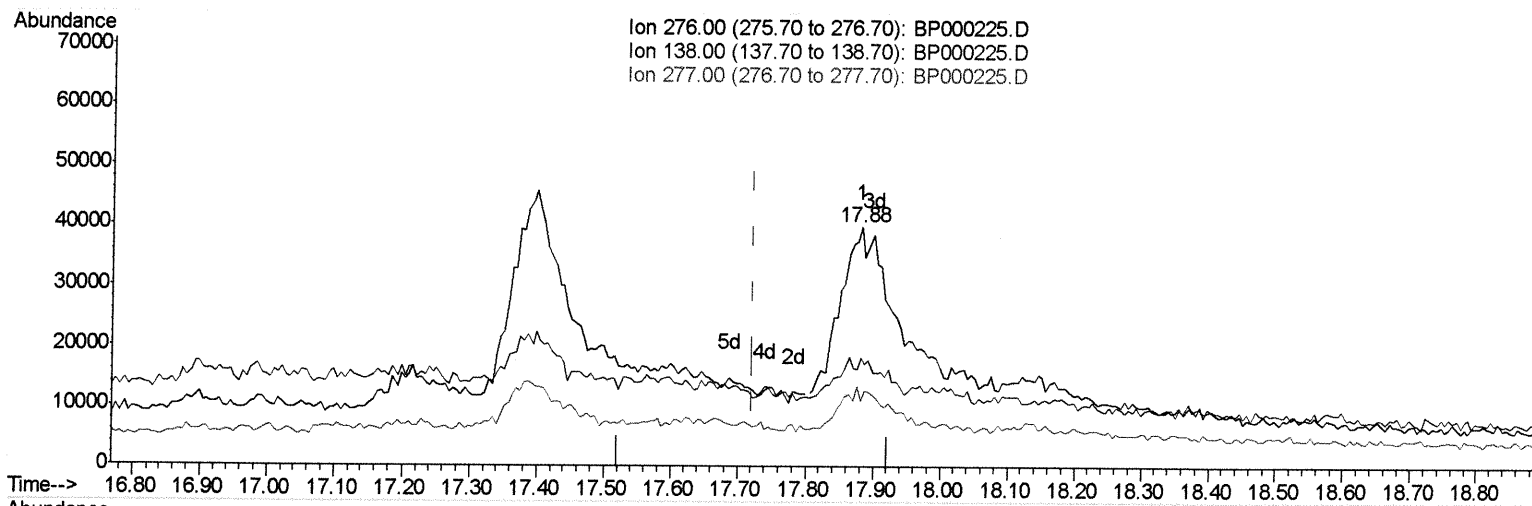

Scan 2666 (17.769 min): BP000208.D (-2650) (-)

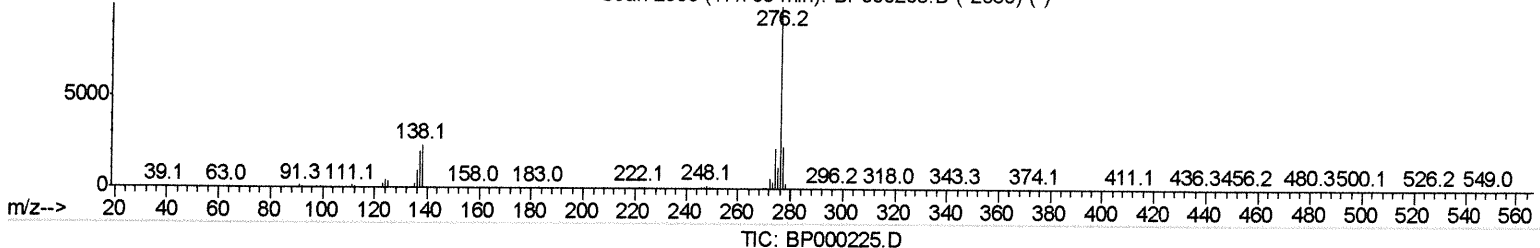

(94) Benzo(g,h,i)perylene

17.880min (+0.159) 1.44ng/ul

response 72474

Ion	Exp%	Act%
276.00	100	100
138.00	25.00	45.24#
277.00	23.90	27.78
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091219\
Data File : BP000225.D
Acq On : 12 Sep 2019 19:45
Operator : HP/JU
Sample : K4633-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleID :
F2D12

Manual Integrations
APPROVED

mohammad
9/16/2019 9:09:36 AM

Quant Time: Sep 13 01:51:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 02:43:18 2019
Response via : Initial Calibration

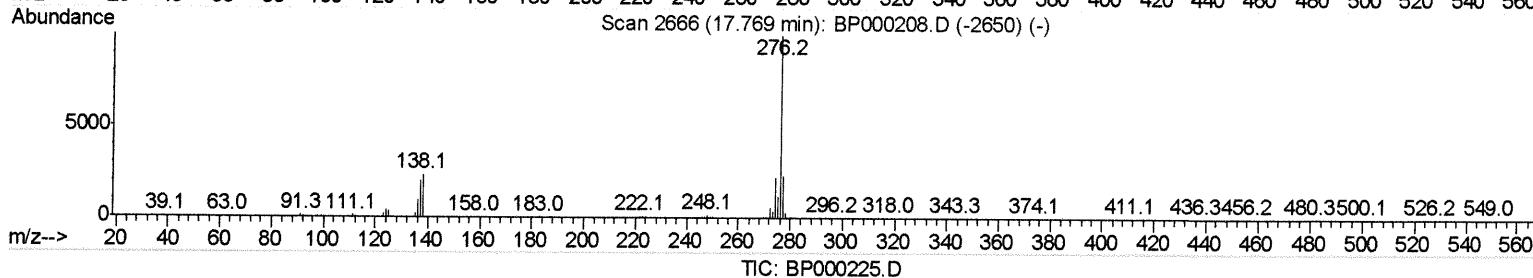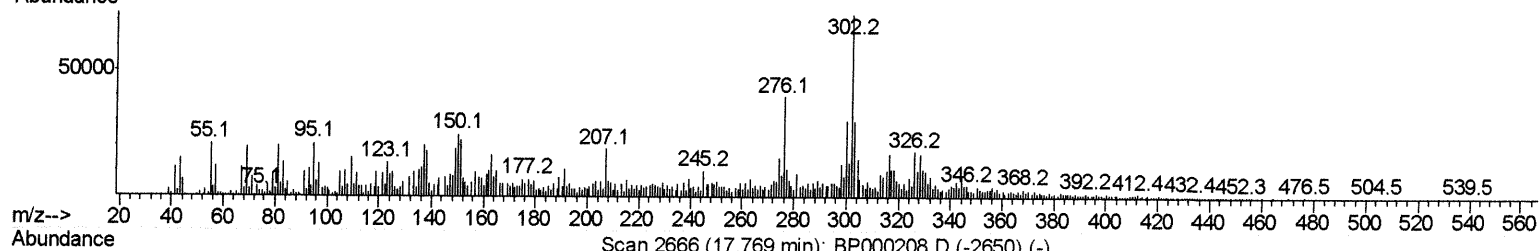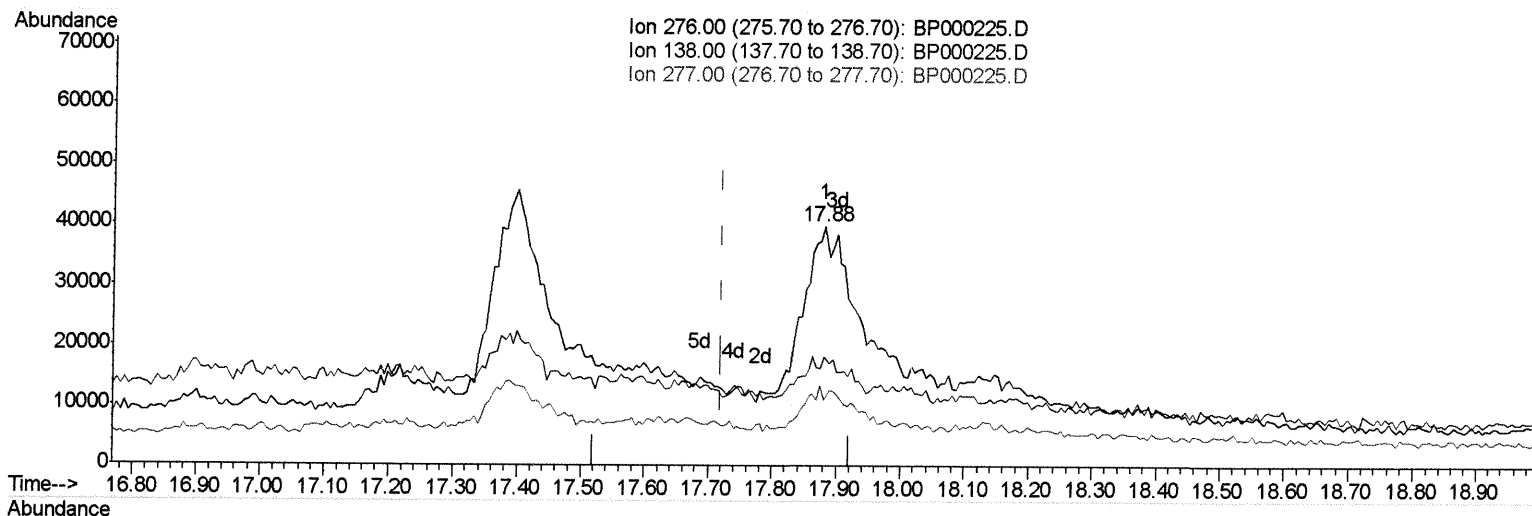

(94) Benzo(g,h,i)perylene

17.880min (+0.159) 3.67ng/ul m *JU* 09/17/19

response 184622

Ion	Exp%	Act%
276.00	100	100
138.00	25.00	45.24#
277.00	23.90	27.78
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091219\
 Data File : BP000225.D
 Acq On : 12 Sep 2019 19:45
 Operator : HP/JU
 Sample : K4633-13
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F2D12

Manual Integrations
 APPROVED

mohammad
 9/16/2019 9:09:36 AM

Quant Time: Sep 13 05:55:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 02:43:18 2019
 Response via : Initial Calibration

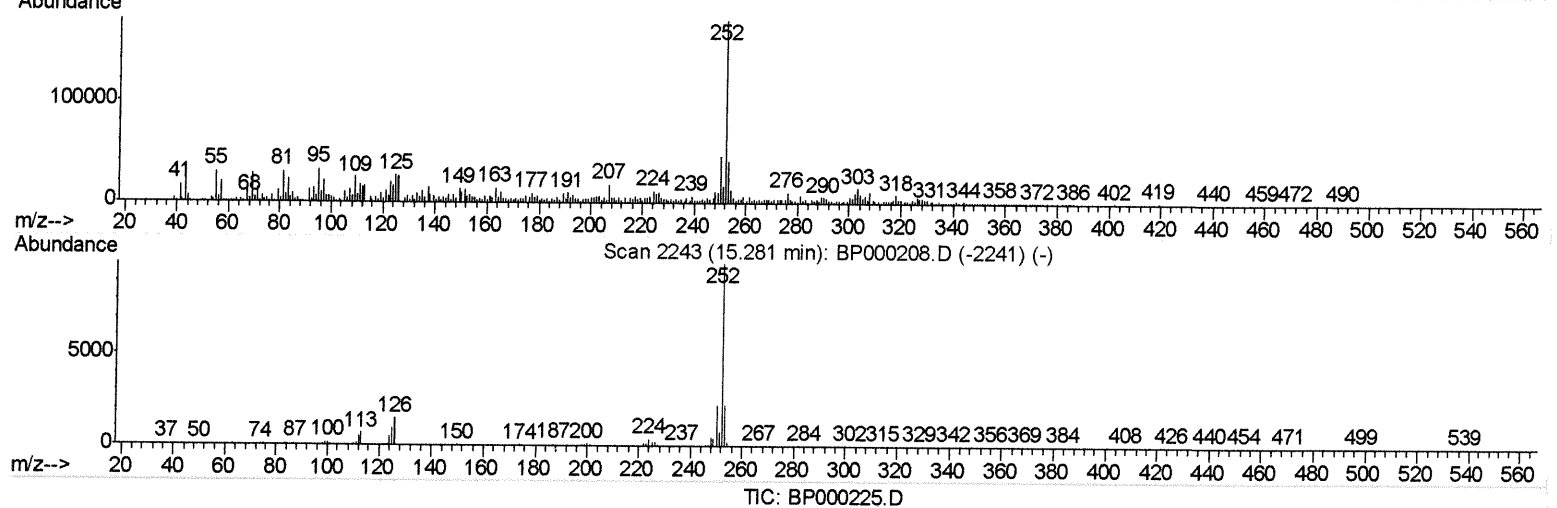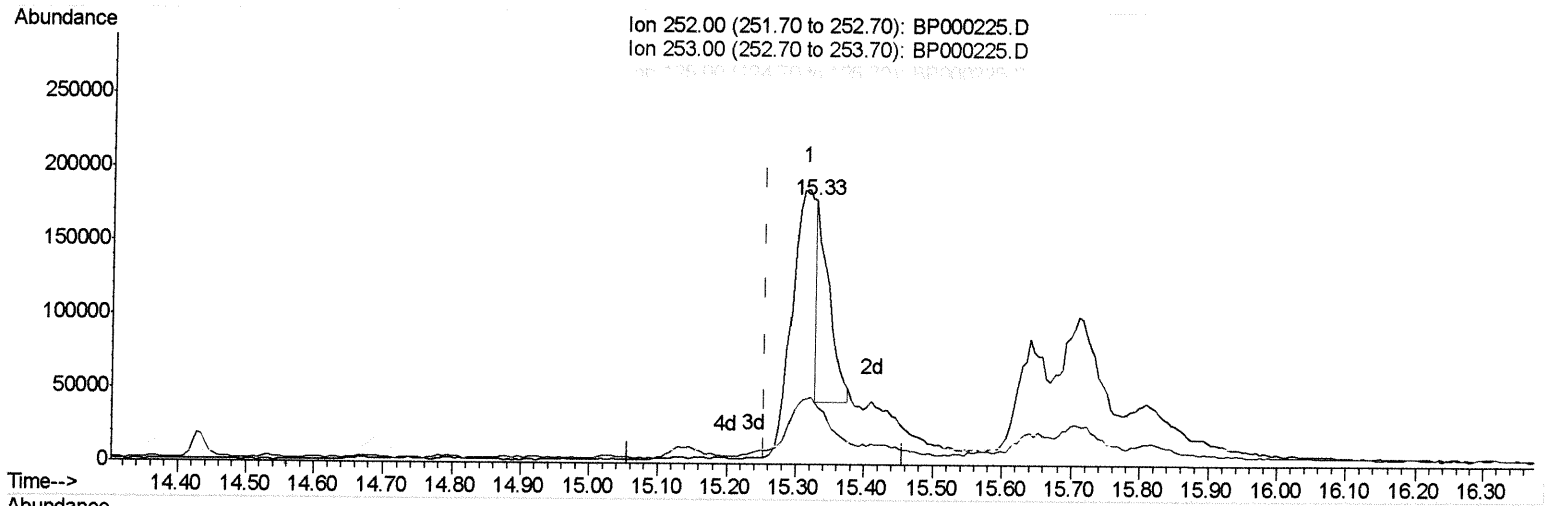

(89) Benzo(k)fluoranthene

15.328min (+0.071) 2.71ng/ul m *JU 09/17/19*

response 142793

Ion	Exp%	Act%
252.00	100	100
253.00	22.50	22.97
125.00	12.70	14.95
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091219\
 Data File : BP000225.D
 Acq On : 12 Sep 2019 19:45
 Operator : HP/JU
 Sample : K4633-13
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F2D12

Manual Integrations
 APPROVED

mohammad
 9/16/2019 9:09:36 AM

Quant Time: Sep 13 05:55:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 02:43:18 2019
 Response via : Initial Calibration

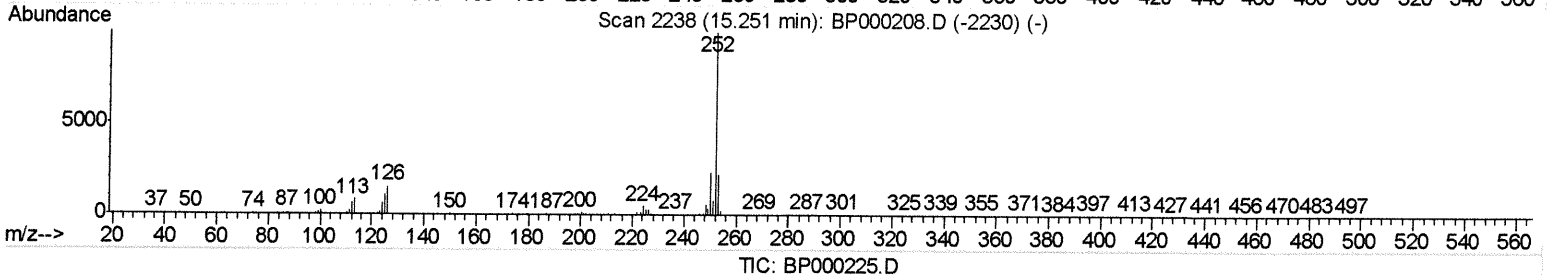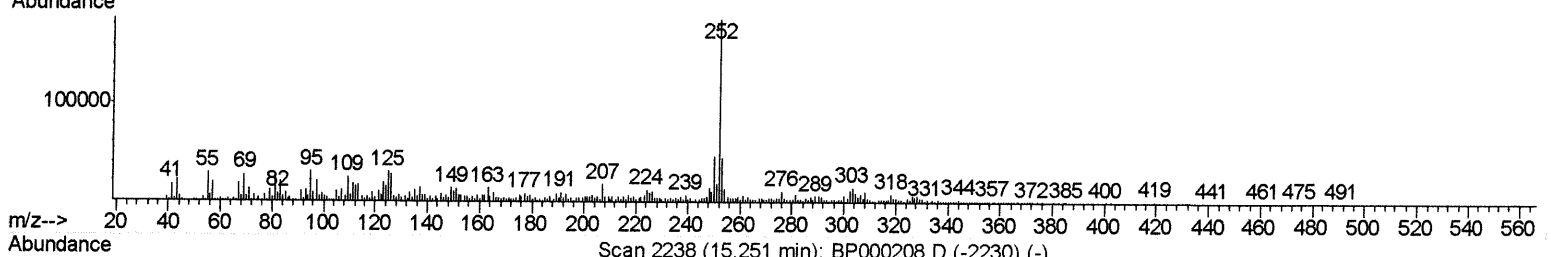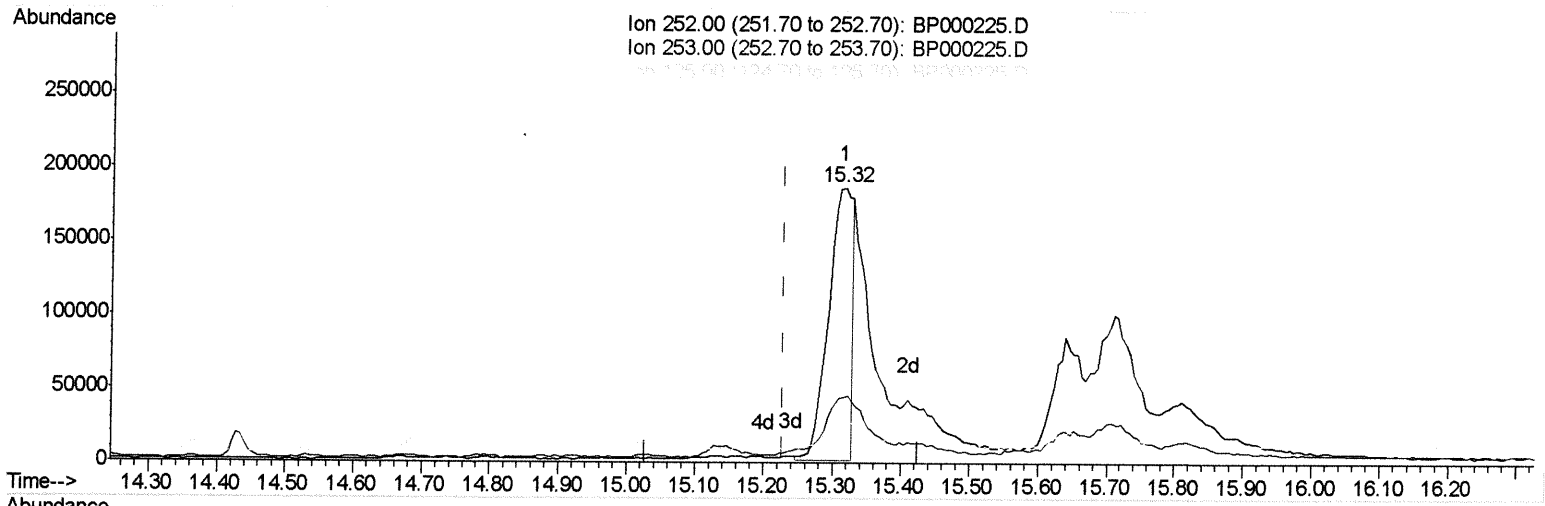

(88) Benzo(b)fluoranthene

15.316min (+0.088) 8.29ng/ul m *JU 09/17/19*

response 463904

Ion	Exp%	Act%
252.00	100	100
253.00	21.90	23.92
125.00	12.40	16.33#
0.00	0.00	0.00



Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091219\
Data File : BP000225.D
Acq On : 12 Sep 2019 19:45
Operator : HP/JU
Sample : K4633-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F2D12


Manual Integrations
APPROVED

mohammad
9/16/2019 9:09:36 AM

Quant Time: Sep 13 05:55:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 02:43:18 2019
Response via : Initial Calibration

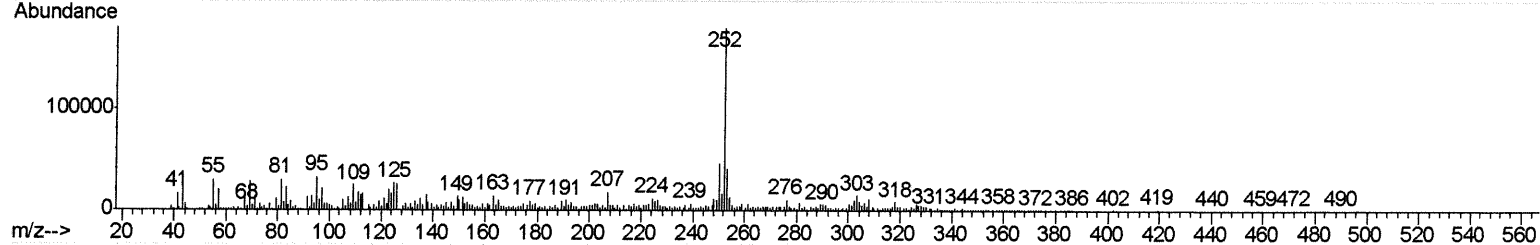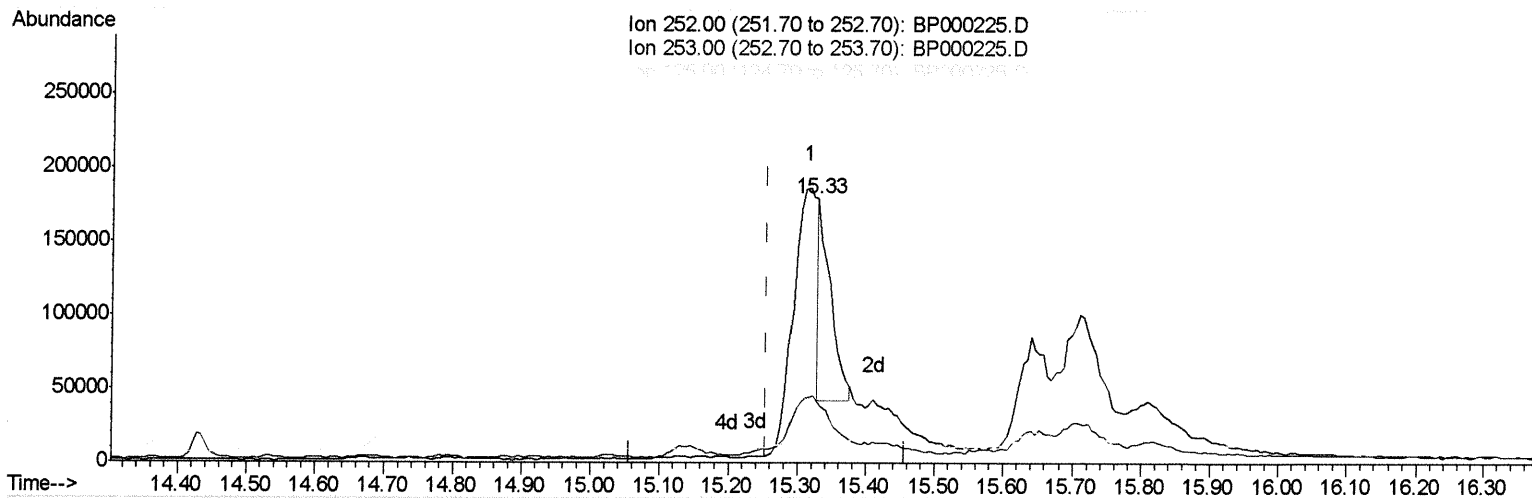

Scan 2243 (15.281 min): BP000208.D (-2241) (-)

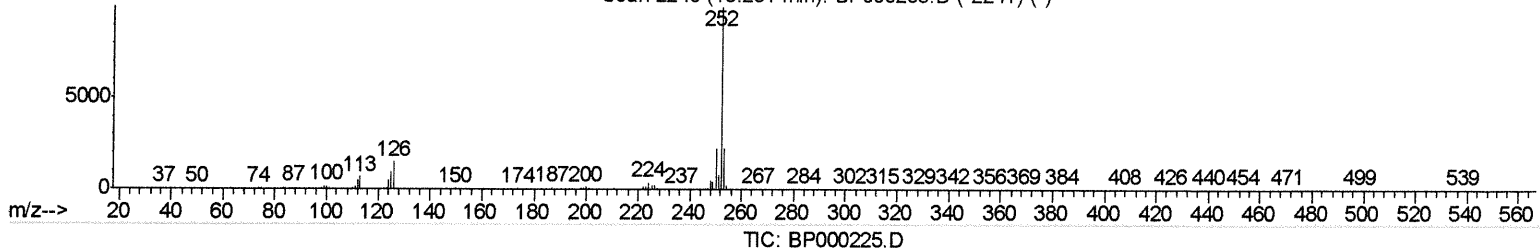

(89) Benzo(k)fluoranthene

15.328min (+0.071) 2.71ng/ul m *JU 9/17/19*

response 142793

Ion	Exp%	Act%
252.00	100	100
253.00	22.50	22.97
125.00	12.70	14.95
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091219\
 Data File : BP000225.D
 Acq On : 12 Sep 2019 19:45
 Operator : HP/JU
 Sample : K4633-13
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F2D12

Manual Integrations
 APPROVED

mohammad
 9/16/2019 9:09:36 AM

Quant Time: Sep 13 05:55:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 02:43:18 2019
 Response via : Initial Calibration

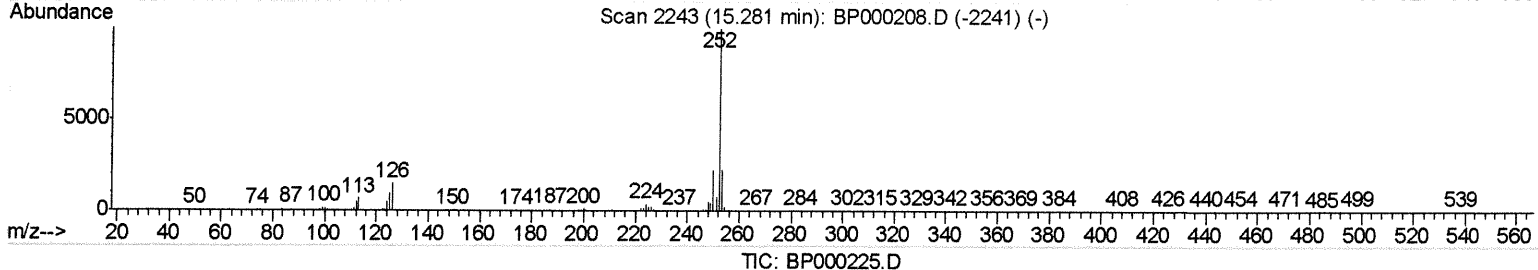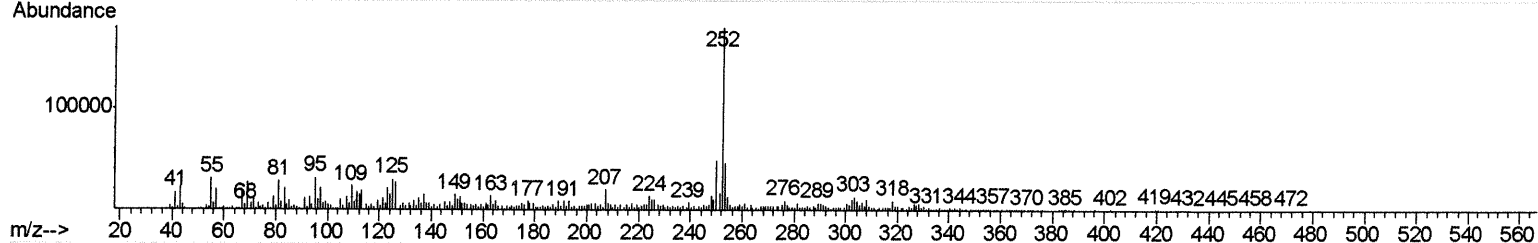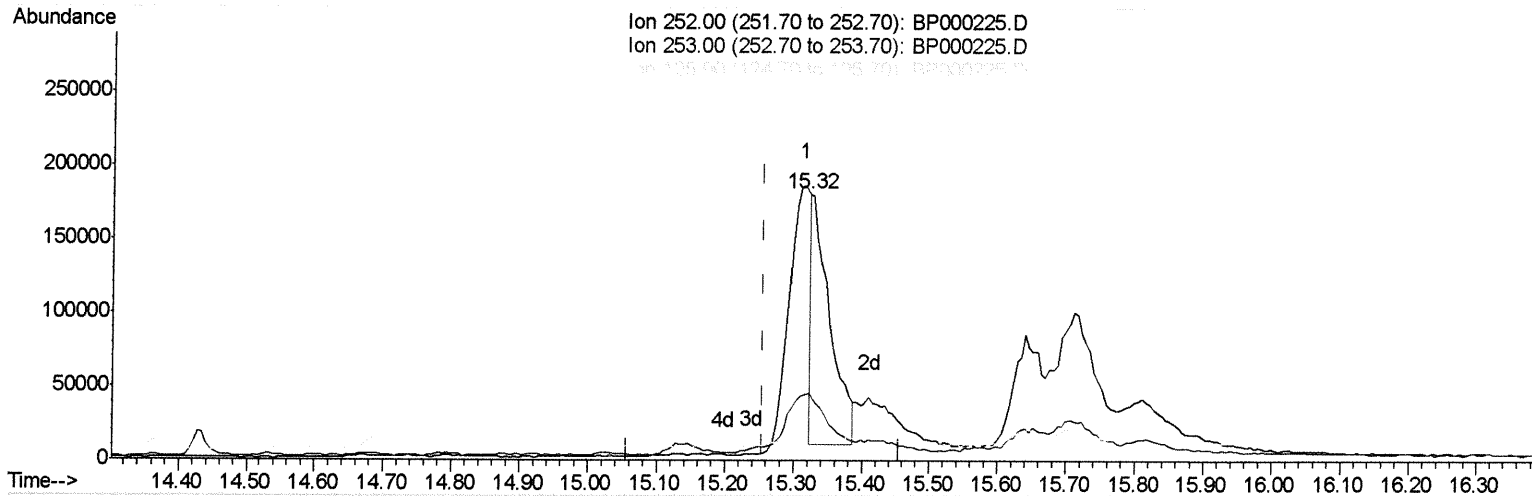

(89) Benzo(k)fluoranthene

15.322min (+0.065) 5.94ng/ul m

JU
 09/17/19

response 313276

Ion	Exp%	Act%
252.00	100	100
253.00	22.50	25.33
125.00	12.70	16.55#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091219\
 Data File : BP000225.D
 Acq On : 12 Sep 2019 19:45
 Operator : HP/JU
 Sample : K4633-13
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F2D12

Manual Integrations
 APPROVED

mohammad
 9/16/2019 9:09:36 AM

Quant Time: Sep 13 14:28:28 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 02:43:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	312341	20.00	ng/ul	0.00
18) Naphthalene-d8	8.18	136	1178712	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.95	164	618869	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.46	188	1109520	20.00	ng/ul	0.00
78) Chrysene-d12	14.18	240	910141	20.00	ng/ul	0.04
86) Perylene-d12	15.79	264	844356	20.00	ng/ul	0.10

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.62	96	31497	3.58	ng/uL	0.01
5) Phenol-d5	6.52	99	588686	22.13	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	6.58	67	305317	21.95	ng/ul	0.00
9) 2-Chlorophenol-d4	6.66	132	494423	22.98	ng/ul	0.00
13) 4-Methylphenol-d8	7.26	113	443037	22.17	ng/ul	0.00
19) Nitrobenzene-d5	7.45	128	231927	25.91	ng/ul	0.00
22) 2-Nitrophenol-d4	7.78	143	253127	29.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	8.02	165	429694	23.23	ng/ul	0.00
29) 4-Chloroaniline-d4	8.23	131	47495	2.08	ng/ul	0.00
44) Dimethylphthalate-d6	9.63	166	1162206	25.43	ng/ul	0.00
47) Acenaphthylene-d8	9.79	160	1368039	24.22	ng/ul	0.00
52) 4-Nitrophenol-d4	10.04	143	158080	19.36	ng/ul	0.00
58) Fluorene-d10	10.48	176	928285	23.92	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.55	200	95709	18.77	ng/ul	0.02
71) Anthracene-d10	11.52	188	1287733	23.97	ng/ul	0.00
79) Pyrene-d10	12.92	212	1300676	24.03	ng/ul	0.02
90) Benzo(a)pyrene-d12	15.67	264	921890	21.06	ng/ul	0.09

Target Compounds

					Qvalue
4) Benzaldehyde	6.45	77	17867	1.329	ng/ul 98
6) Phenol	6.53	94	112325	4.051	ng/ul 97
45) Dimethylphthalate	9.66	163	348115	7.549	ng/ul 100
70) Phenanthrene	11.48	178	371755	5.666	ng/ul 99
72) Anthracene	11.53	178	73372	1.136	ng/ul 98
75) Carbazole	11.69	167	73856	1.338	ng/ul 100
77) Fluoranthene	12.70	202	893826	13.506	ng/ul 99
80) Pyrene	12.93	202	727386	10.593	ng/ul 95
83) Benzo(a)anthracene	14.17	228	314962m →	4.781	ng/ul > 2 Ju 09/17/19
84) Bis(2-ethylhexyl)phthalate	14.16	149	61277	1.638	ng/ul# 96
85) Chrysene	14.20	228	477350	7.896	ng/ul 96
88) Benzo(b)fluoranthene	15.32	252	408829m →	7.305	ng/ul > 2 Ju 09/17/19
89) Benzo(k)fluoranthene	15.32	252	313276m →	5.939	ng/ul > 2 Ju 09/17/19
91) Benzo(a)pyrene	15.71	252	213996	4.076	ng/ul# 86
92) Indeno(1,2,3-cd)pyrene	17.40	276	168319	2.787	ng/ul# 72
93) Dibenzo(a,h)anthracene	17.40	278	64321m →	1.286	ng/ul > 2 Ju 09/17/19
94) Benzo(g,h,i)perylene	17.88	276	184622m →	3.666	ng/ul > 2 Ju 09/17/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed