

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091219\
 Data File : BP000211.D
 Acq On : 12 Sep 2019 12:25
 Operator : HP/JU
 Sample : K4634-15
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F2D33

Manual Integrations
 APPROVED

mohammad
 9/16/2019 9:09:02 AM

Quant Time: Sep 13 13:08:29 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 02:43:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	398752	20.00	ng/ul	0.00
18) Naphthalene-d8	8.18	136	1506293	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.95	164	777149	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.46	188	1305960	20.00	ng/ul	0.00
78) Chrysene-d12	14.18	240	820252	20.00	ng/ul	0.04
86) Perylene-d12	15.76	264	932125m	20.00	ng/ul	0.07

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.62	96	30126	2.68	ng/uL	0.01
5) Phenol-d5	6.51	99	570045	16.78	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.57	67	307651	17.32	ng/ul	0.00
9) 2-Chlorophenol-d4	6.66	132	482533	17.57	ng/ul	0.00
13) 4-Methylphenol-d8	7.26	113	429625	16.84	ng/ul	0.00
19) Nitrobenzene-d5	7.45	128	229030	20.02	ng/ul	0.00
22) 2-Nitrophenol-d4	7.77	143	245083	22.01	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	8.02	165	431589	18.26	ng/ul	0.00
29) 4-Chloroaniline-d4	8.23	131	254941	8.72	ng/ul	0.00
44) Dimethylphthalate-d6	9.63	166	1178193	20.53	ng/ul	0.00
47) Acenaphthylene-d8	9.79	160	1386164	19.55	ng/ul	0.00
52) 4-Nitrophenol-d4	10.04	143	138452	13.50	ng/ul	0.00
58) Fluorene-d10	10.47	176	936310	19.21	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.54	200	60479	10.08	ng/ul	0.01
71) Anthracene-d10	11.52	188	1246517	19.71	ng/ul	0.00
79) Pyrene-d10	12.92	212	1127964	23.12	ng/ul	0.02
90) Benzo(a)pyrene-d12	15.66	264	977779	20.24	ng/ul	0.07

Target Compounds

					Ovalue	
6) Phenol	6.52	94	105531	2.981	ng/ul	97
14) Acetophenone	7.29	105	51371	1.342	ng/ul	99
45) Dimethylphthalate	9.66	163	271977	4.697	ng/ul	99
50) Acenaphthene	9.98	153	108982	2.123	ng/ul	99
70) Phenanthrene	11.49	178	2569537	33.271	ng/ul	99
72) Anthracene	11.53	178	566628	7.456	ng/ul	99
75) Carbazole	11.69	167	451411	6.947	ng/ul	99
77) Fluoranthene	12.72	202	7324733	94.032	ng/ul	97
80) Pyrene	12.95	202	6835658	110.458	ng/ul	94
83) Benzo(a)anthracene	14.17	228	4957115	83.487	ng/ul	97
84) Bis(2-ethylhexyl)phthalate	14.17	149	56446	1.674	ng/ul#	86
85) Chrysene	14.21	228	4663611	85.594	ng/ul	98
88) Benzo(b)fluoranthene	15.31	252	4150884m	67.189	ng/ul	
89) Benzo(k)fluoranthene	15.32	252	3814570m	65.502	ng/ul	
91) Benzo(a)pyrene	15.70	252	3654287m	63.044	ng/ul	
92) Indeno(1,2,3-cd)pyrene	17.37	276	2363897m	35.449	ng/ul	
93) Dibenzo(a,h)anthracene	17.37	278	630880	11.422	ng/ul	95
94) Benzo(g,h,i)perylene	17.85	276	2310581m	41.558	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091219\
Data File : BP000211.D
Acq On : 12 Sep 2019 12:25
Operator : HP/JU
Sample : K4634-15
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampled :
F2D33

Manual Integrations
APPROVED

mohammad
9/16/2019 9:09:02 AM

Quant Time: Sep 13 13:08:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 02:43:18 2019
Response via : Initial Calibration

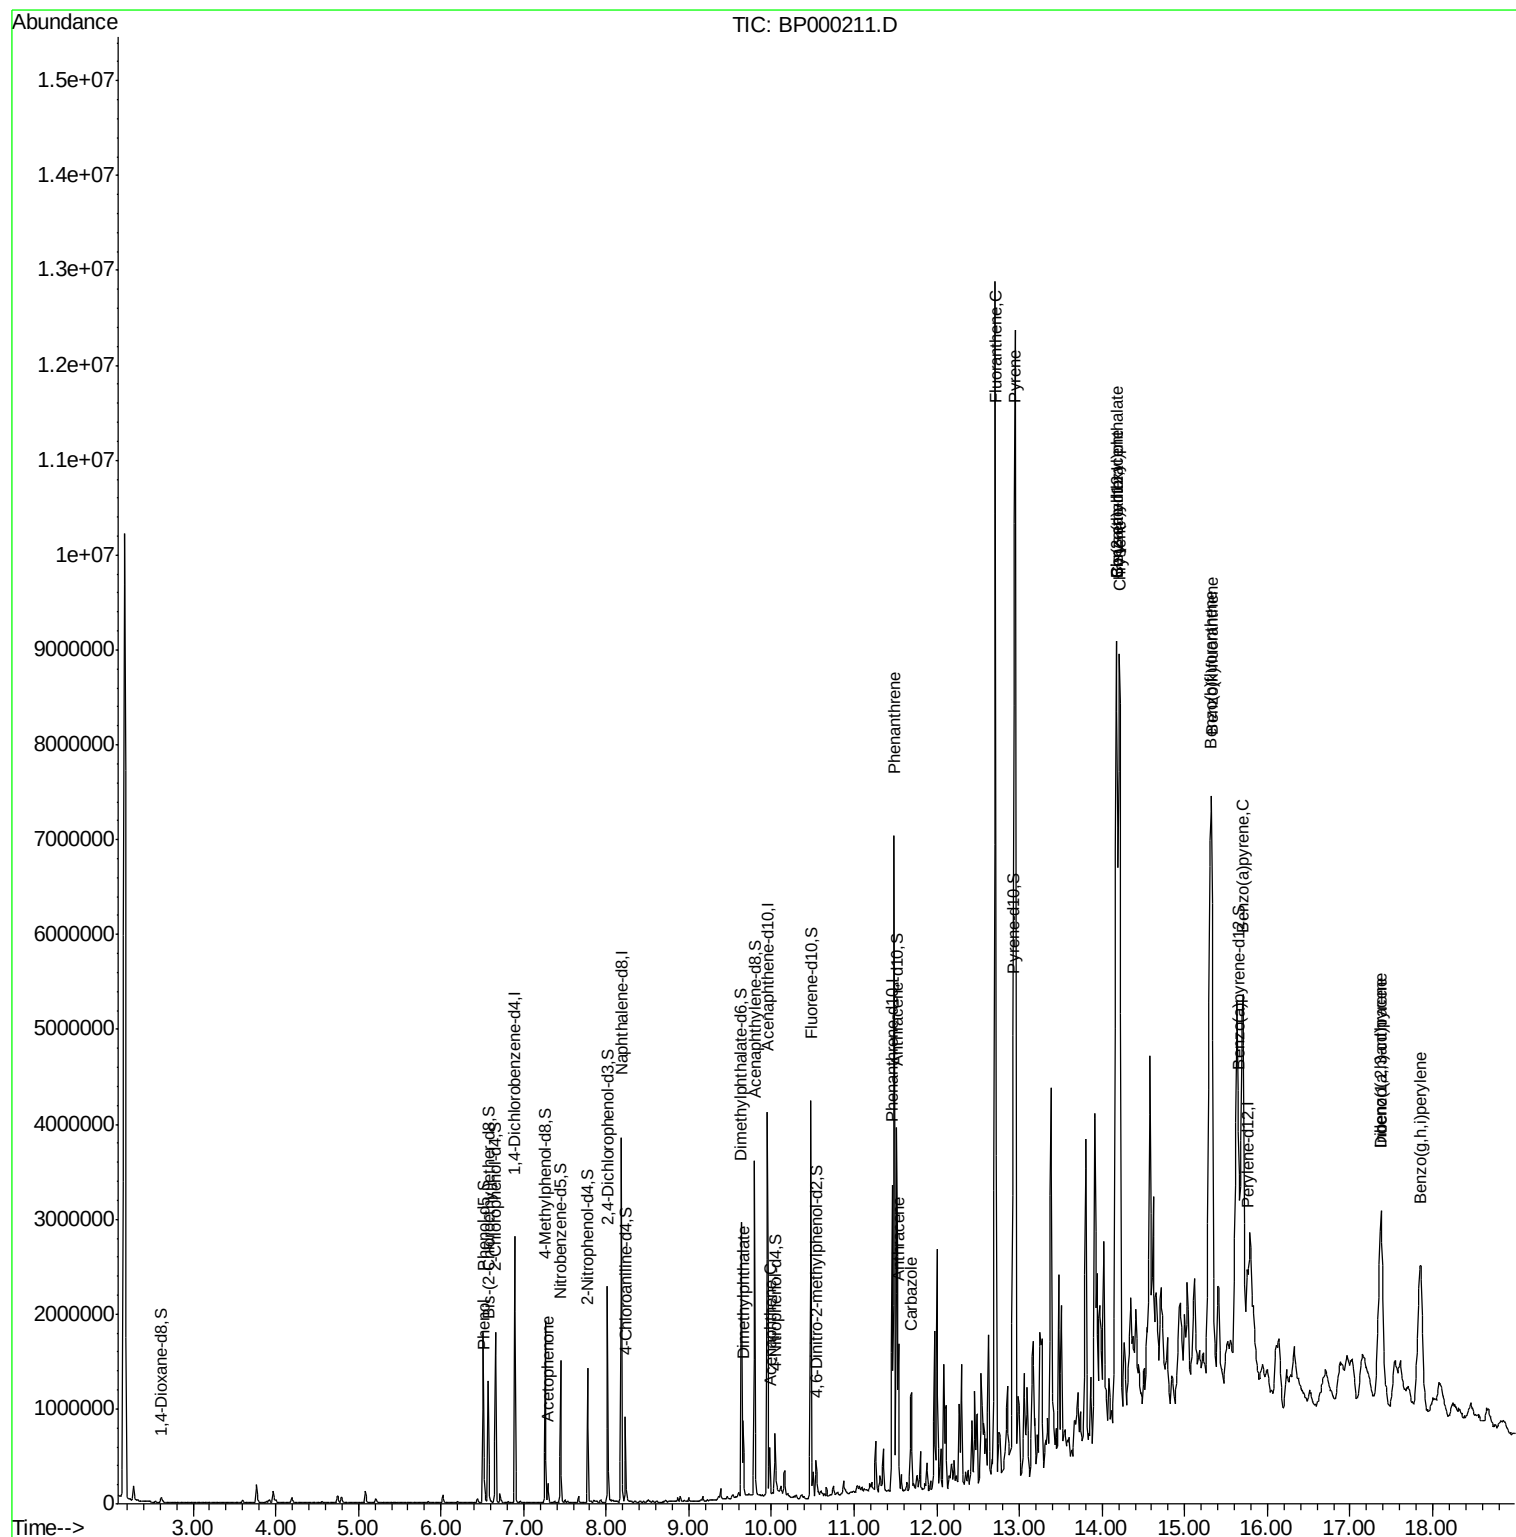

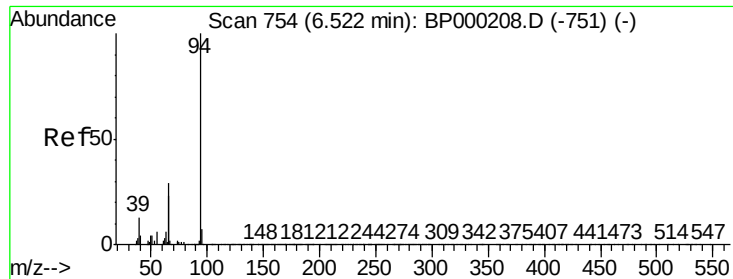

#6

Phenol

Concen: 2.981 ng/ul

RT: 6.52 min Scan# 754

Delta R.T. 0.00 min

Lab File: BP000211.D

Acq: 12 Sep 2019 12:25

Instrument :

BNA_P





ClientSampleId :

F2D33

Tot Ion:	94	Resp:	105531
Ion	Ratio	Lower	Upper
94	100		
65	23.1	18.8	28.2
66	32.7	24.2	36.2

Manual Integrations
APPROVED

mohammad
9/16/2019 9:09:02 AM

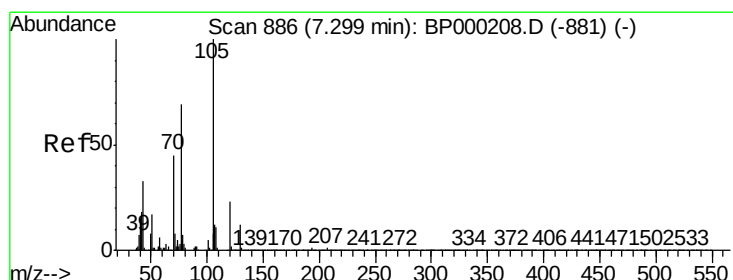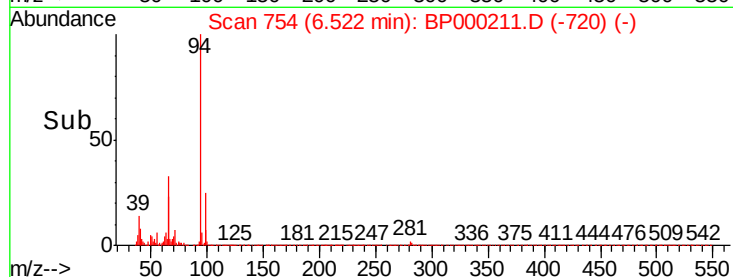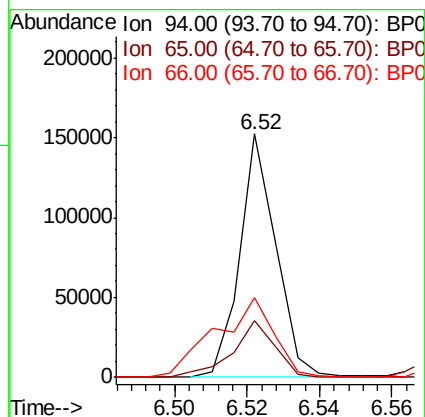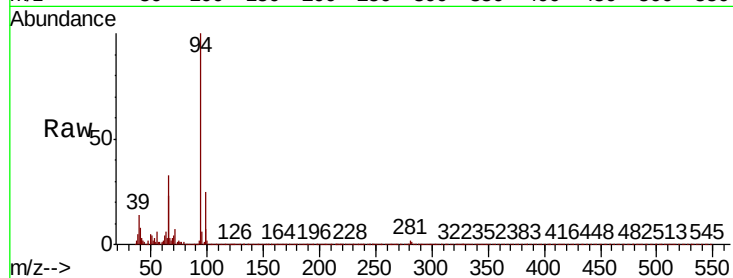

#14

Acetophenone

Concen: 1.342 ng/ul




RT: 7.29 min Scan# 885


Delta R.T. -0.01 min

Lab File: BP000211.D

Acq: 12 Sep 2019 12:25

Tgt Ion:	105	Resp:	51371
Ion	Ratio	Lower	Upper
105	100		
77	70.7	57.2	85.8
51	19.0	14.7	22.1

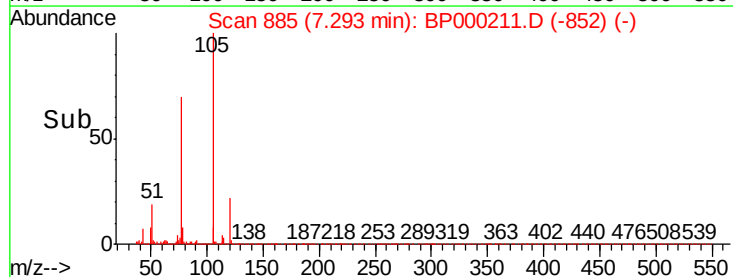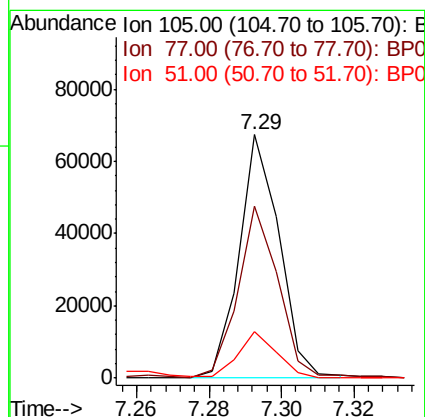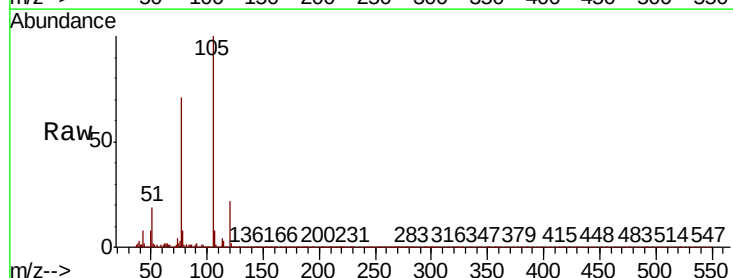







#45
Dimethylphthalate
Concen: 4.697 ng/ul
RT: 9.66 min Scan# 1287
Delta R.T. 0.00 min
Lab File: BP000211.D
Acq: 12 Sep 2019 12:25

Instrument :
BNA_P
ClientSampleId :
F2D33

Tot Ion	Ratio	Resp	Lower	Upper
163	100	271977		
194	4.0		3.2	4.8
164	9.9		8.4	12.6




Manual Integrations
APPROVED


mohammad
9/16/2019 9:09:02 AM

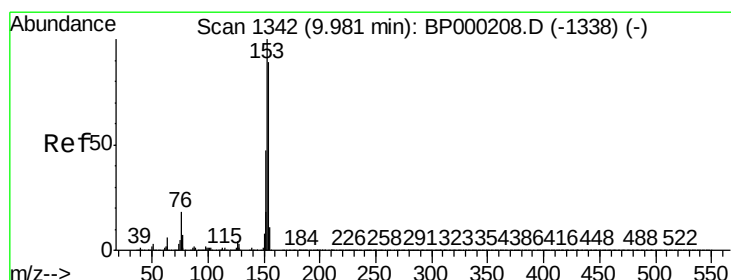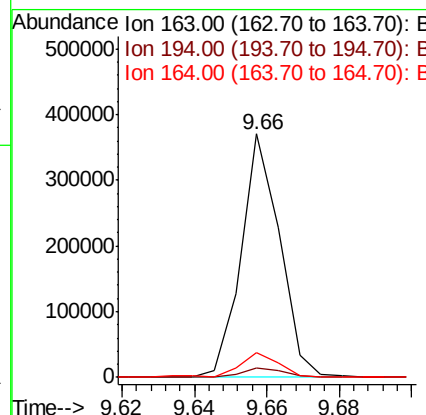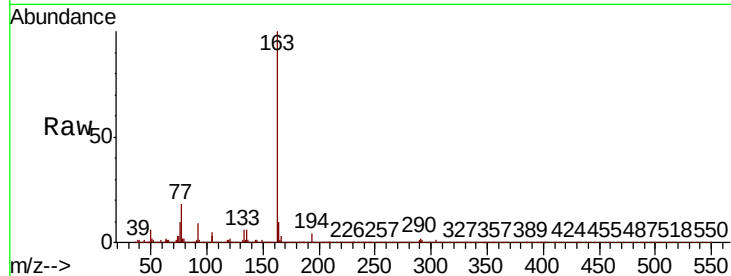

#50
Acenaphthene
Concen: 2.123 ng/ul
RT: 9.98 min Scan# 1342
Delta R.T. 0.00 min
Lab File: BP000211.D
Acq: 12 Sep 2019 12:25

Tgt Ion	Ratio	Resp	Lower	Upper
153	100	108982		
152	48.0		38.0	57.0
154	89.6		72.6	108.8

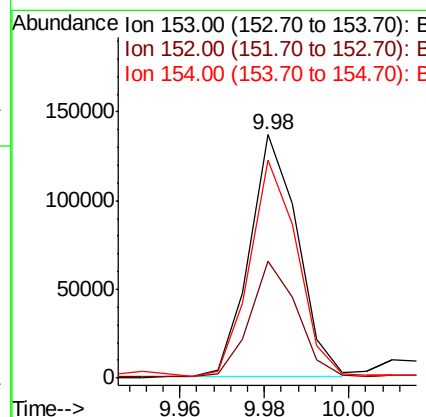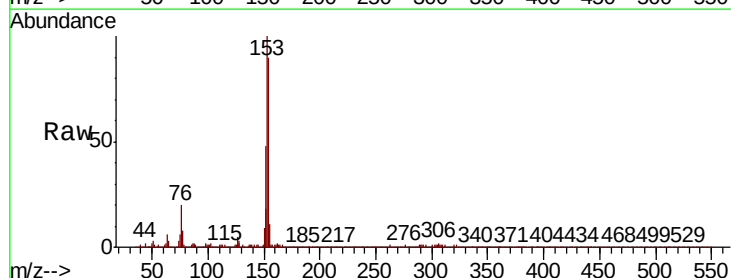

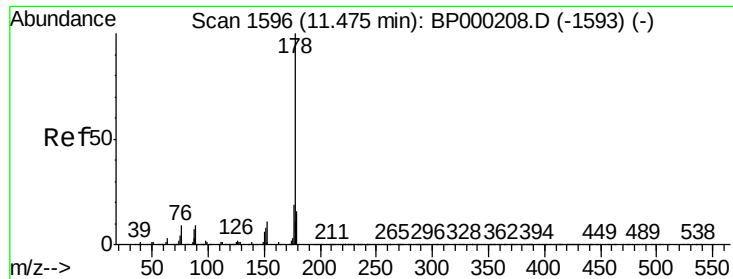





#70
Phenanthrene
Concen: 33.271 ng/ul
RT: 11.49 min Scan# 1598
Delta R.T. 0.01 min
Lab File: BP000211.D
Acq: 12 Sep 2019 12:25

Instrument :
BNA_P
ClientSampleId :
F2D33

Tot Ion	Ratio	Lower	Upper
178	100		
179	15.6	12.5	18.7
176	20.0	15.7	23.5




Manual Integrations
APPROVED


mohammad
9/16/2019 9:09:02 AM

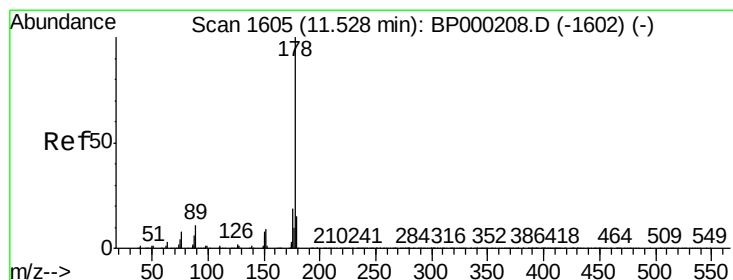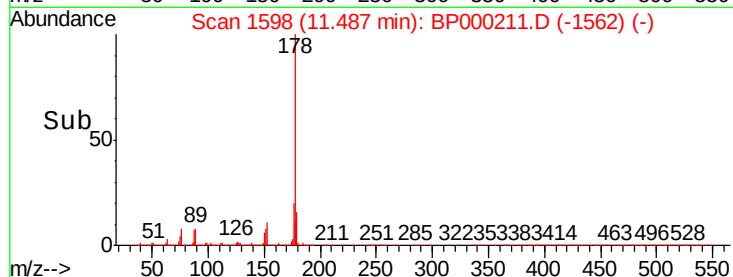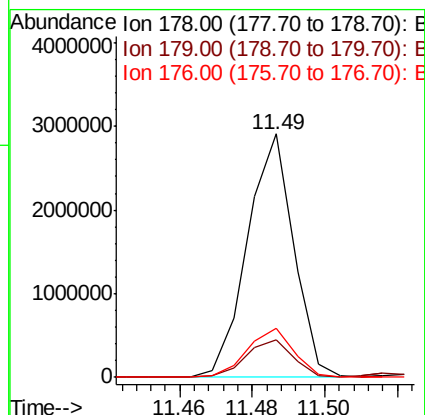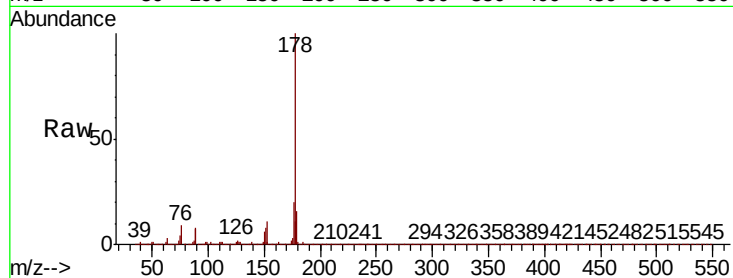

#72
Anthracene
Concen: 7.456 ng/ul
RT: 11.53 min Scan# 1606
Delta R.T. 0.01 min
Lab File: BP000211.D
Acq: 12 Sep 2019 12:25

Tgt Ion	Ratio	Lower	Upper
178	100		
179	16.1	12.3	18.5
176	18.9	15.1	22.7

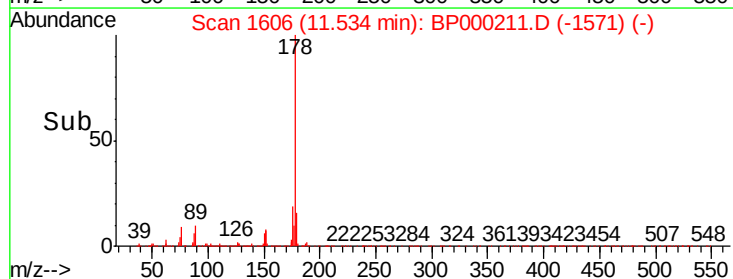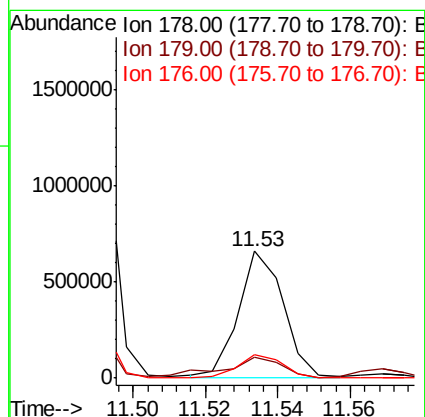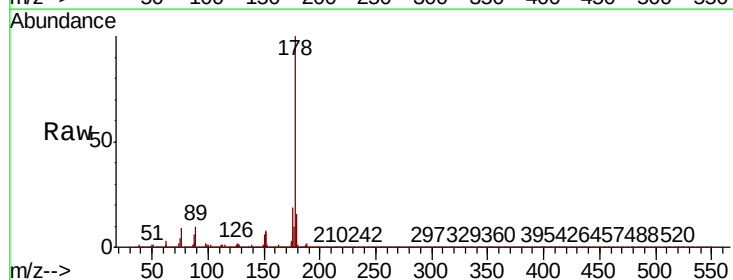



#75

Carbazole

Concen: 6.947 ng/ul

RT: 11.69 min Scan# 1633

Delta R.T. 0.01 min

Lab File: BP000211.D

Acq: 12 Sep 2019 12:25

Instrument :

BNA_P





ClientSampleId :

F2D33

Tot Ion:	167	Resp:	451411
Ion Ratio	Lower	Upper	
167	100		
166	22.1	17.3	25.9
139	12.8	10.6	15.8

Manual Integrations
APPROVED

mohammad
9/16/2019 9:09:02 AM

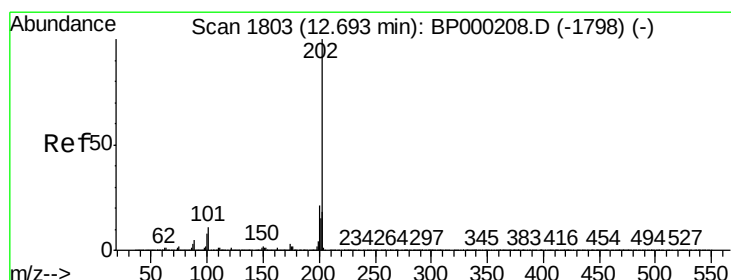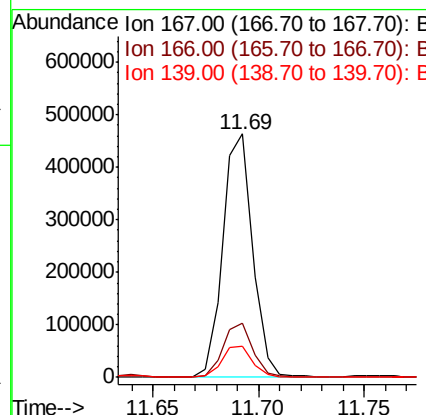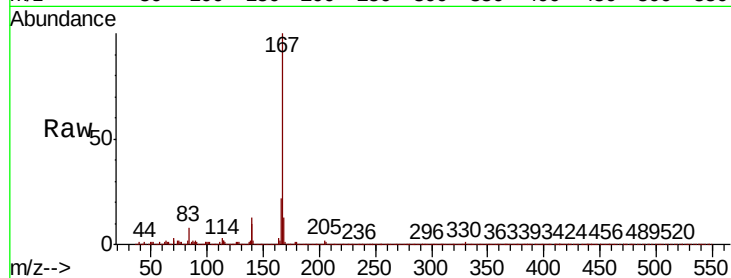

#77

Fluoranthene

Concen: 94.032 ng/ul




RT: 12.72 min Scan# 1807


Delta R.T. 0.03 min

Lab File: BP000211.D

Acq: 12 Sep 2019 12:25

Tgt Ion:	202	Resp:	7324733
Ion Ratio	Lower	Upper	
202	100		
101	11.0	10.0	15.0
100	8.3	7.4	11.2

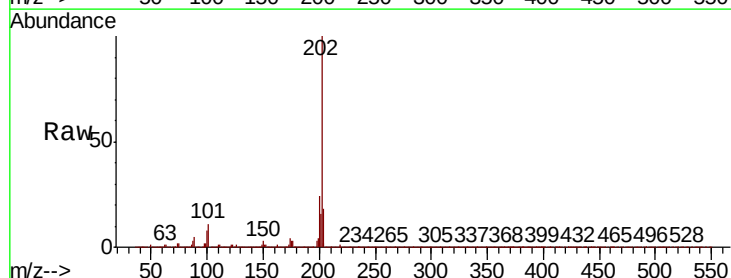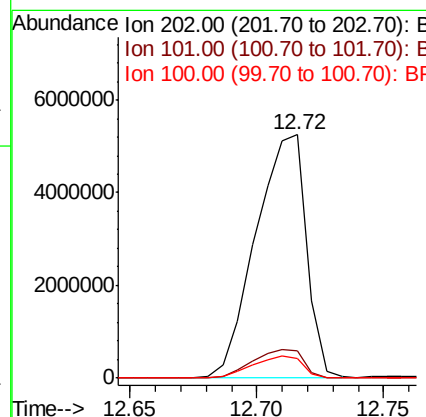







#80
Pvrene
Concen: 110.458 ng/ul
RT: 12.95 min Scan# 1846
Delta R.T. 0.03 min
Lab File: BP000211.D
Acq: 12 Sep 2019 12:25

Instrument :
BNA_P
ClientSampleId :
F2D33

Tot Ion	Ratio	Lower	Upper
202	100		
101	13.7	13.4	20.0
100	11.3	10.8	16.2




Manual Integrations
APPROVED


mohammad
9/16/2019 9:09:02 AM

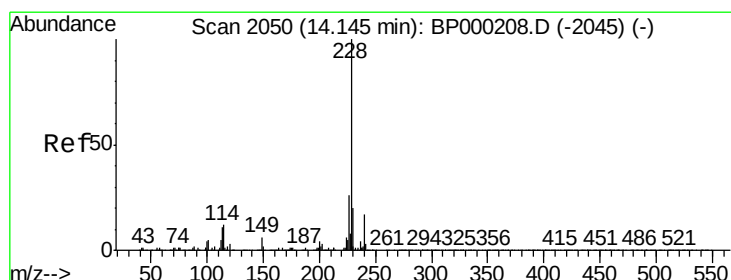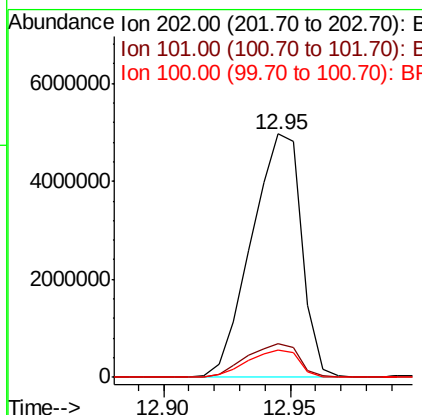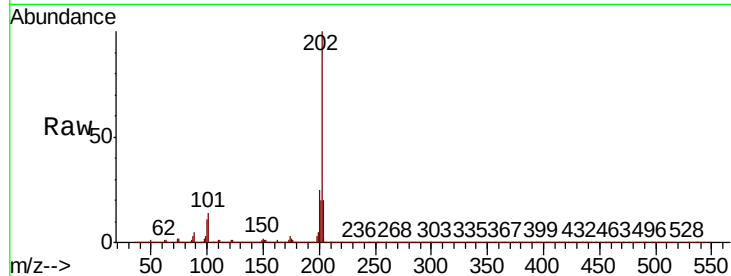

#83
Benzo(a)anthracene
Concen: 83.487 ng/ul
RT: 14.17 min Scan# 2054
Delta R.T. 0.04 min
Lab File: BP000211.D
Acq: 12 Sep 2019 12:25

Tgt Ion	Ratio	Lower	Upper
228	100		
229	20.6	15.9	23.9
226	30.0	22.1	33.1

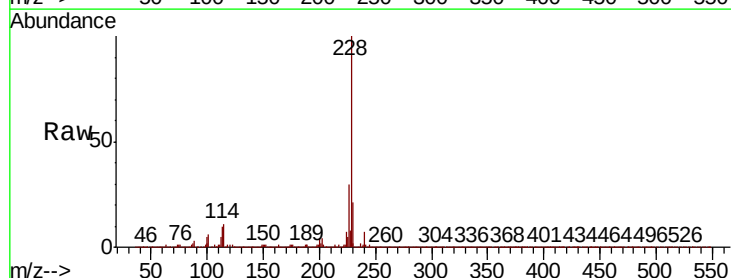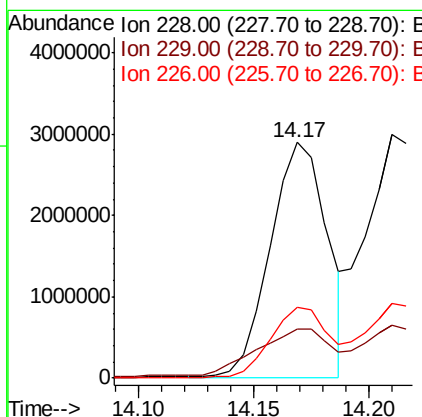



#84

Bis(2-ethylhexyl)phthalate

Concen: 1.674 ng/ul

RT: 14.17 min Scan# 2055

Delta R.T. 0.02 min

Lab File: BP000211.D

Acq: 12 Sep 2019 12:25

Instrument :

BNA_P





ClientSampleId :

F2D33

Tot Ion:	149	Resp:	56446
Ion Ratio	Lower	Upper	
149	100		
167	18.9	21.8	32.8#
279	3.5	3.0	4.4

Manual Integrations
APPROVED

mohammad
9/16/2019 9:09:02 AM

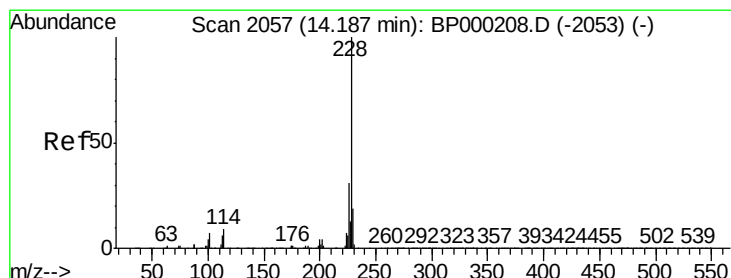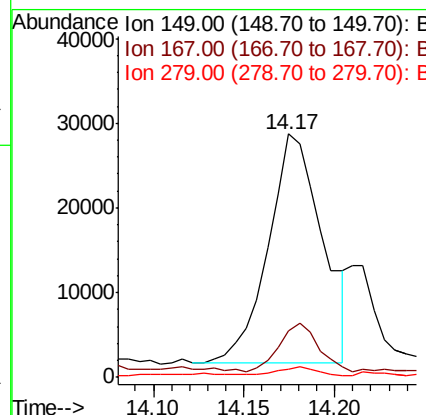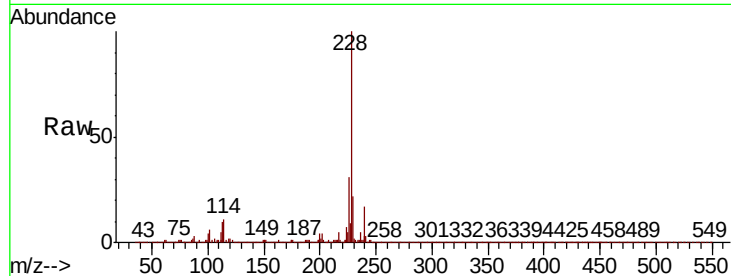

#85

Chrysene

Concen: 85.594 ng/ul




RT: 14.21 min Scan# 2061


Delta R.T. 0.04 min

Lab File: BP000211.D

Acq: 12 Sep 2019 12:25

Tgt Ion:	228	Resp:	4663611
Ion Ratio	Lower	Upper	
228	100		
226	30.9	24.4	36.6
229	21.9	16.0	24.0

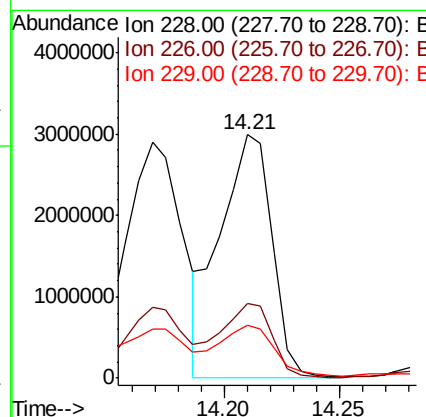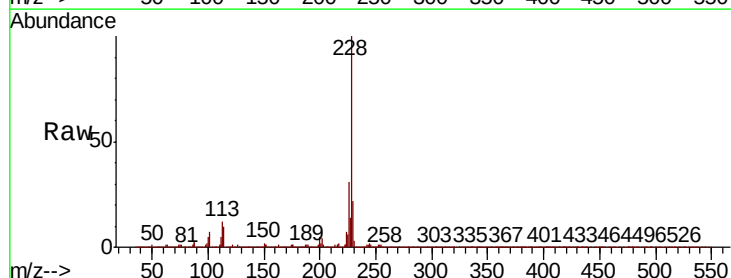







#88
Benzo(b)fluoranthene
Concen: 67.189 ng/ul m
RT: 15.31 min Scan# 2248
Delta R.T. 0.08 min
Lab File: BP000211.D
Acq: 12 Sep 2019 12:25

Instrument :
BNA_P
ClientSampleId :
F2D33

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.0	17.5	26.3
125	12.1	9.9	14.9




Manual Integrations
APPROVED


mohammad
9/16/2019 9:09:02 AM

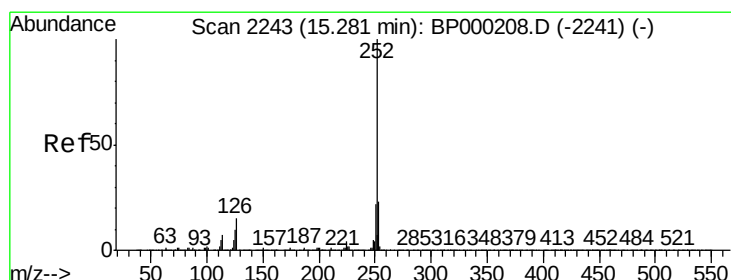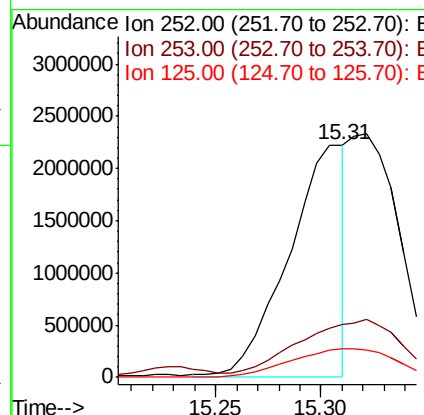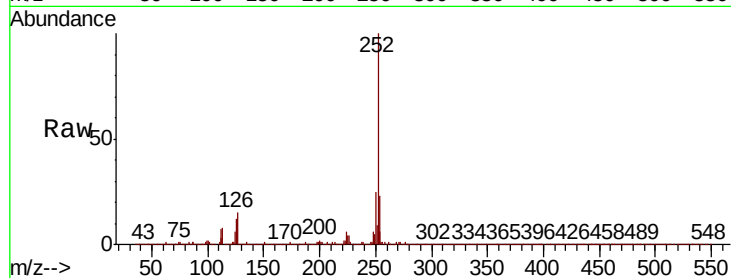

#89
Benzo(k)fluoranthene
Concen: 65.502 ng/ul m
RT: 15.32 min Scan# 2250
Delta R.T. 0.06 min
Lab File: BP000211.D
Acq: 12 Sep 2019 12:25

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.6	18.0	27.0
125	11.3	10.2	15.2

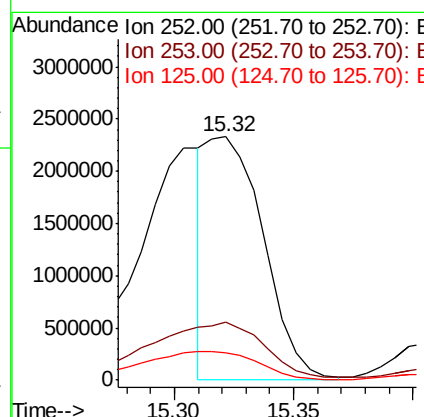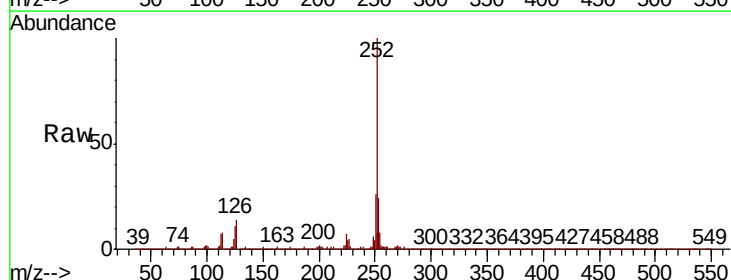







#91
Benzo(a)pyrene
Concen: 63.044 ng/ul m
RT: 15.70 min Scan# 2315
Delta R.T. 0.09 min
Lab File: BP000211.D
Acq: 12 Sep 2019 12:25

Instrument :
BNA_P
ClientSampleId :
F2D33

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.3	17.5	26.3
125	11.4	10.2	15.2




Manual Integrations
APPROVED


mohammad
9/16/2019 9:09:02 AM

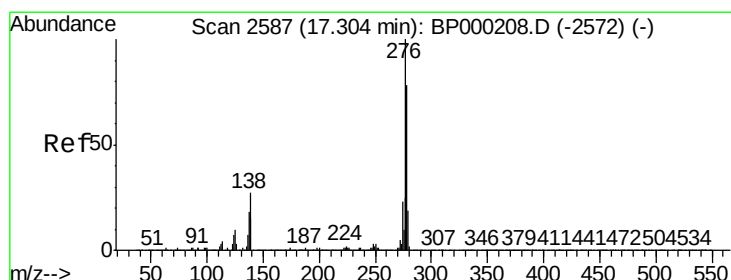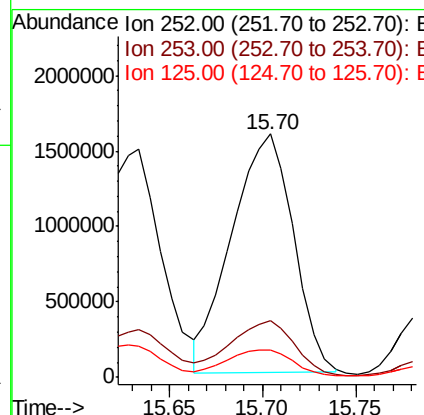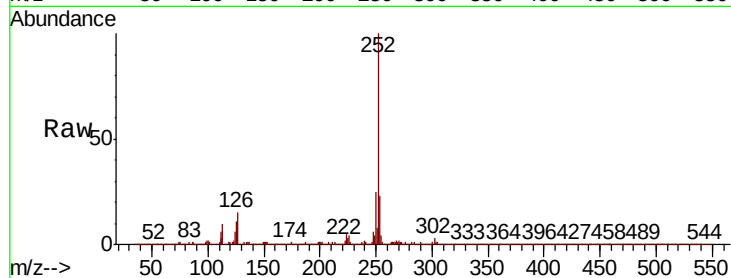

#92
Indeno(1,2,3-cd)pyrene
Concen: 35.449 ng/ul m
RT: 17.37 min Scan# 2598
Delta R.T. 0.12 min
Lab File: BP000211.D
Acq: 12 Sep 2019 12:25

Tgt Ion	Ratio	Lower	Upper
276	100		
138	24.6	20.0	30.0
277	24.9	19.4	29.0

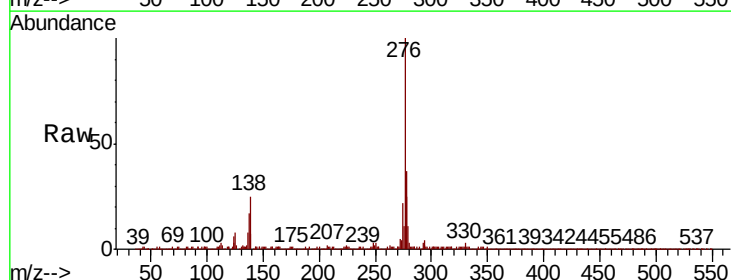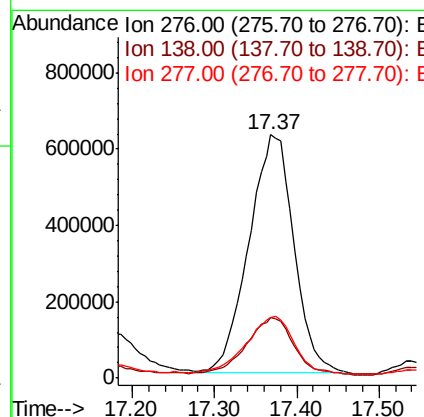







#93
Dibenzo(a,h)anthracene
Concen: 11.422 ng/ul
RT: 17.37 min Scan# 2599
Delta R.T. 0.10 min
Lab File: BP000211.D
Acq: 12 Sep 2019 12:25

Instrument :
BNA_P
ClientSampleId :
F2D33

Tot Ion	Ratio	Lower	Upper
278	100		
139	18.8	15.1	22.7
279	28.6	19.2	28.8

Manual Integrations
APPROVED

mohammad
9/16/2019 9:09:02 AM

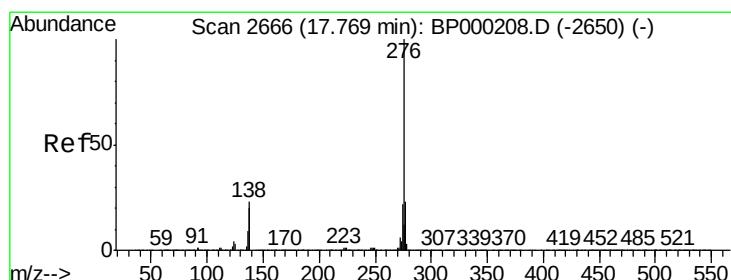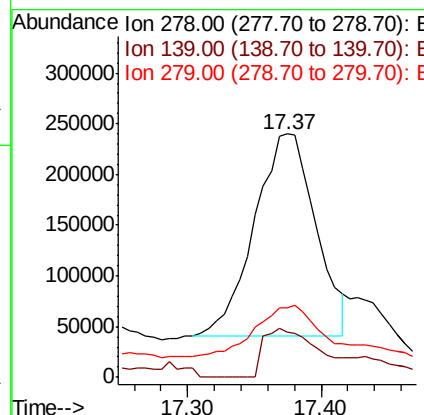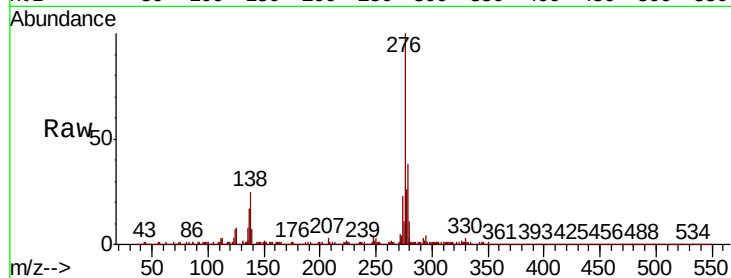

#94
Benzo(g,h,i)perylene
Concen: 41.558 ng/ul m
RT: 17.85 min Scan# 2680
Delta R.T. 0.13 min
Lab File: BP000211.D
Acq: 12 Sep 2019 12:25

Tgt Ion	Ratio	Lower	Upper
276	100		
138	24.6	20.0	30.0
277	25.0	19.1	28.7

