

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091219\
 Data File : BP000216.D
 Acq On : 12 Sep 2019 14:27
 Operator : HP/JU
 Sample : K4634-19DL 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F2D37DL

Manual Integrations
 APPROVED

mohammad
 9/16/2019 9:09:08 AM

Quant Time: Sep 13 04:43:09 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 10 02:43:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	447670	20.00	ng/ul	0.00
18) Naphthalene-d8	8.18	136	1678804	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.95	164	855632	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.46	188	1516150	20.00	ng/ul	0.00
78) Chrysene-d12	14.17	240	1158130	20.00	ng/ul	0.03
86) Perylene-d12	15.76	264	1188272	20.00	ng/ul	0.07

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.62	96	5985	0.47	ng/uL	0.02
5) Phenol-d5	6.51	99	118613	3.11	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.57	67	63630	3.19	ng/ul	0.00
9) 2-Chlorophenol-d4	6.66	132	102531	3.32	ng/ul	0.00
13) 4-Methylphenol-d8	7.26	113	94377	3.29	ng/ul	0.00
19) Nitrobenzene-d5	7.45	128	44911	3.52	ng/ul	0.00
22) 2-Nitrophenol-d4	7.78	143	44075	3.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	8.02	165	85989	3.26	ng/ul	0.00
29) 4-Chloroaniline-d4	8.23	131	44118	1.35	ng/ul	0.00
44) Dimethylphthalate-d6	9.63	166	250307	3.96	ng/ul	0.00
47) Acenaphthylene-d8	9.79	160	297779	3.81	ng/ul	0.00
52) 4-Nitrophenol-d4	10.04	143	24622	2.18	ng/ul	0.00
58) Fluorene-d10	10.47	176	202176	3.77	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.54	200	5623	0.81	ng/ul	0.01
71) Anthracene-d10	11.51	188	282479	3.85	ng/ul	0.00
79) Pyrene-d10	12.91	212	272339	3.95	ng/ul	0.01
90) Benzo(a)pyrene-d12	15.66	264	212897	3.46	ng/ul	0.07

Target Compounds

					Ovalue
70) Phenanthrene	11.48	178	876159	9.772 ng/ul	99
72) Anthracene	11.53	178	153898	1.744 ng/ul	99
75) Carbazole	11.69	167	104855	1.390 ng/ul	98
77) Fluoranthene	12.70	202	2641086	29.205 ng/ul	99
80) Pyrene	12.93	202	2681677	30.691 ng/ul	94
83) Benzo(a)anthracene	14.16	228	2135041	25.468 ng/ul	95
85) Chrysene	14.20	228	2118669	27.541 ng/ul	100
88) Benzo(b)fluoranthene	15.31	252	1770017m	22.475 ng/ul	
89) Benzo(k)fluoranthene	15.31	252	915422m	12.331 ng/ul	
91) Benzo(a)pyrene	15.69	252	1488928	20.150 ng/ul	98
92) Indeno(1,2,3-cd)pyrene	17.35	276	700683	8.243 ng/ul	94
93) Dibenzo(a,h)anthracene	17.36	278	238552	3.388 ng/ul#	83
94) Benzo(g,h,i)perylene	17.84	276	789927m	11.145 ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091219\
Data File : BP000216.D
Acq On : 12 Sep 2019 14:27
Operator : HP/JU
Sample : K4634-19DL 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampled :
F2D37DL

Manual Integrations
APPROVED

mohammad
9/16/2019 9:09:08 AM

Quant Time: Sep 13 04:43:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 10 02:43:18 2019
Response via : Initial Calibration

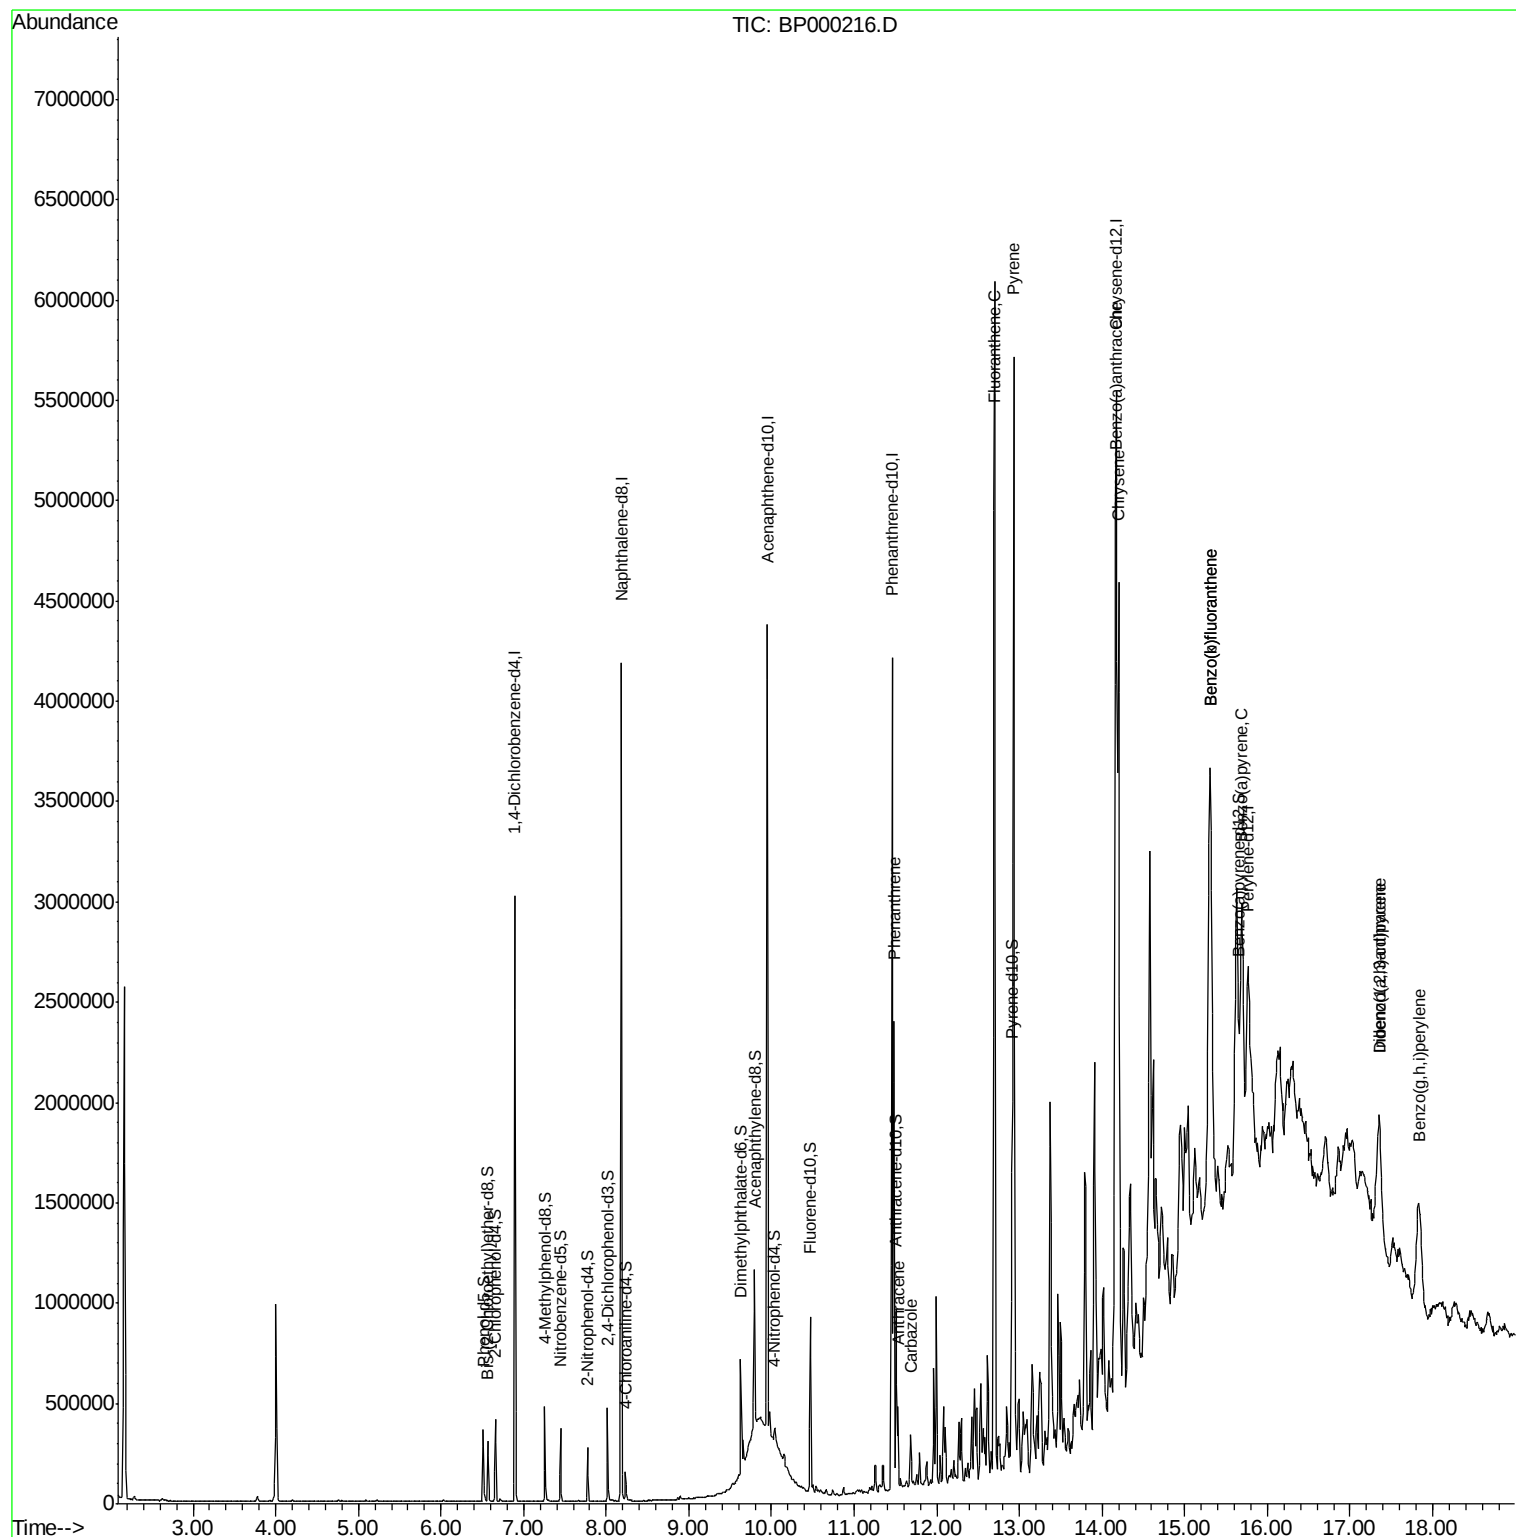

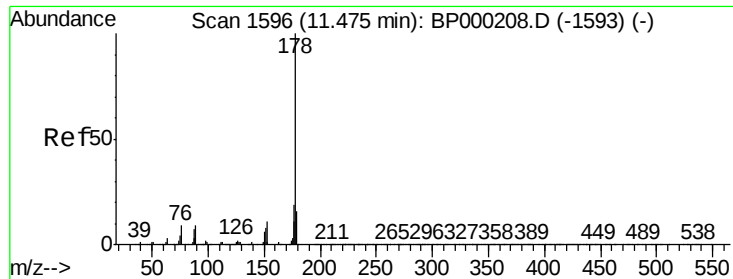





#70
Phenanthrene
Concen: 9.772 ng/ul
RT: 11.48 min Scan# 1597
Delta R.T. 0.01 min
Lab File: BP000216.D
Acq: 12 Sep 2019 14:27

Instrument :
BNA_P
ClientSampleID :
F2D37DL

Tot Ion	Ratio	Lower	Upper
178	100		
179	15.9	12.5	18.7
176	20.3	15.7	23.5




Manual Integrations
APPROVED


mohammad
9/16/2019 9:09:08 AM

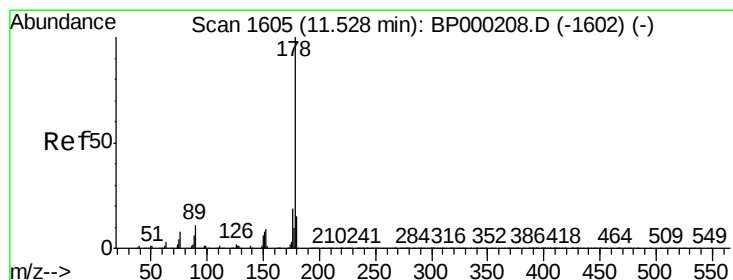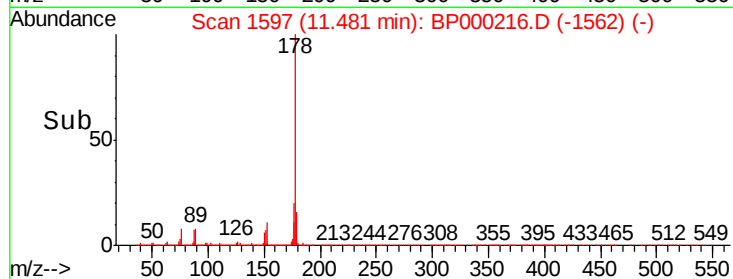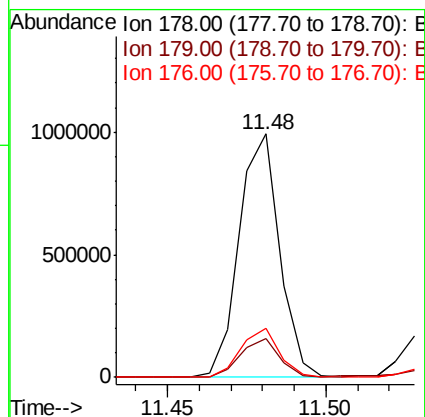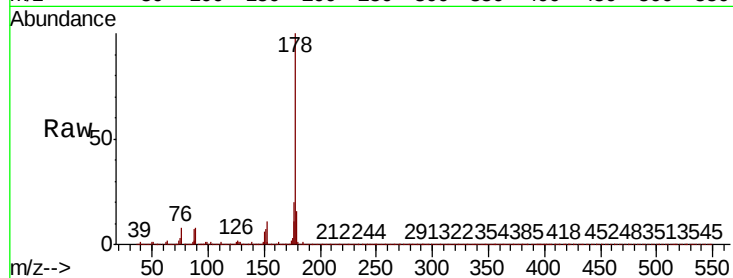

#72
Anthracene
Concen: 1.744 ng/ul
RT: 11.53 min Scan# 1605
Delta R.T. 0.00 min
Lab File: BP000216.D
Acq: 12 Sep 2019 14:27

Tgt Ion	Ratio	Lower	Upper
178	100		
179	16.0	12.3	18.5
176	18.9	15.1	22.7

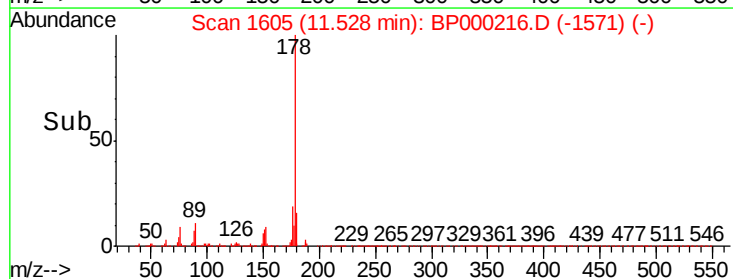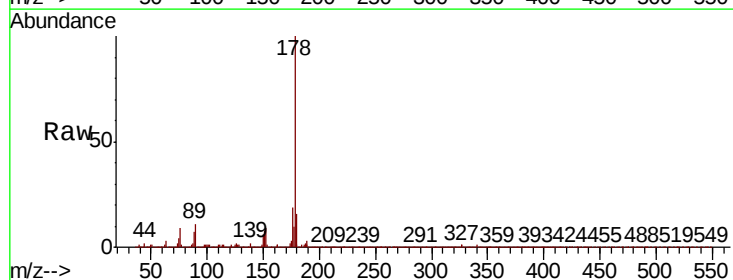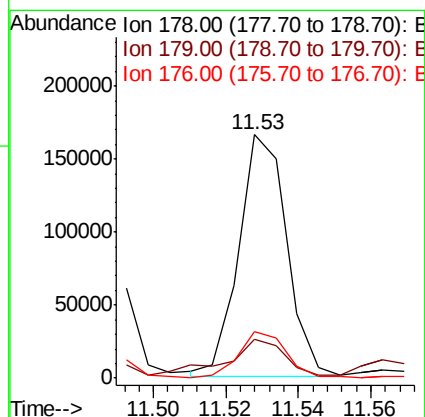

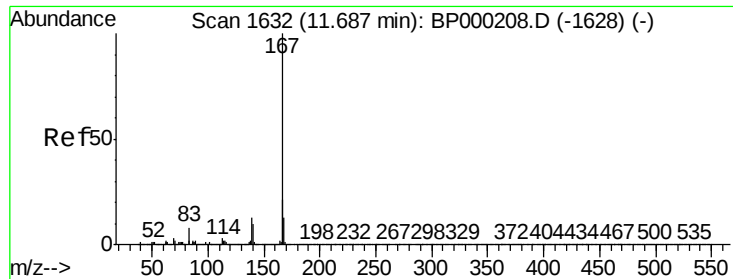

#75

Carbazole

Concen: 1.390 ng/ul

RT: 11.69 min Scan# 1632

Delta R.T. 0.01 min

Lab File: BP000216.D

Acq: 12 Sep 2019 14:27

Instrument :

BNA_P





ClientSampled :

F2D37DL

Tot Ion:	167	Resp:	104855
Ion Ratio	Lower	Upper	
167	100		
166	22.9	17.3	25.9
139	12.7	10.6	15.8

Manual Integrations
APPROVED

mohammad
9/16/2019 9:09:08 AM

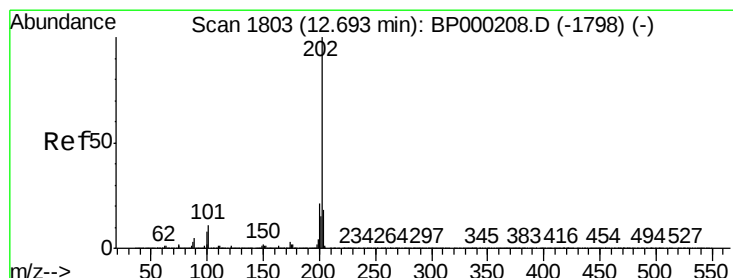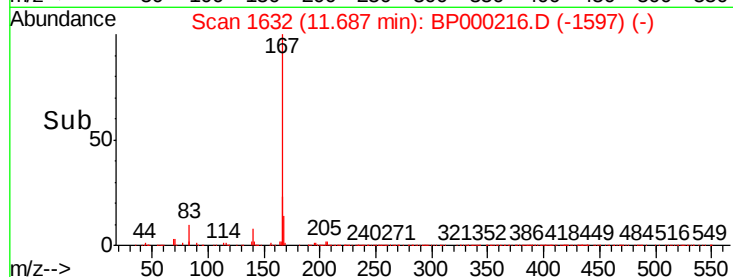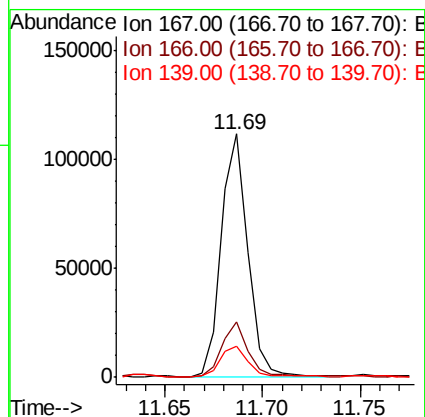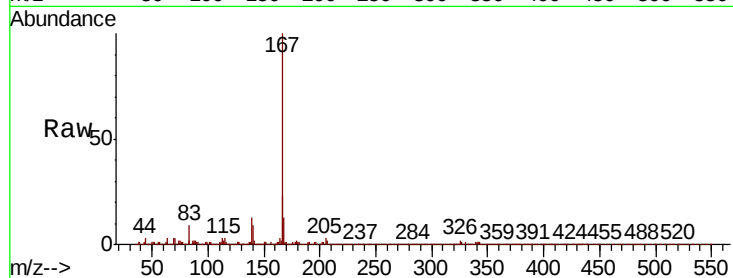

#77

Fluoranthene

Concen: 29.205 ng/ul




RT: 12.70 min Scan# 1804


Delta R.T. 0.01 min

Lab File: BP000216.D

Acq: 12 Sep 2019 14:27

Tgt Ion:	202	Resp:	2641086
Ion Ratio	Lower	Upper	
202	100		
101	12.2	10.0	15.0
100	8.9	7.4	11.2

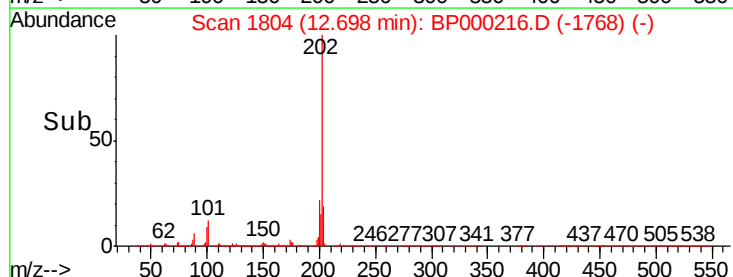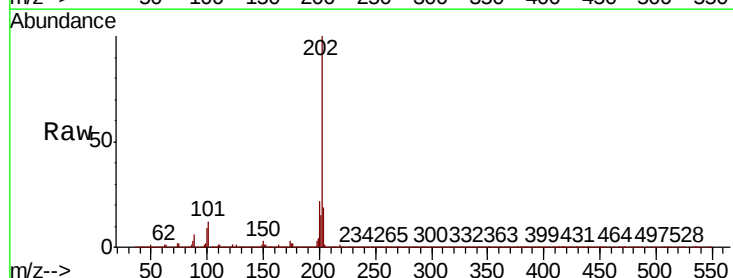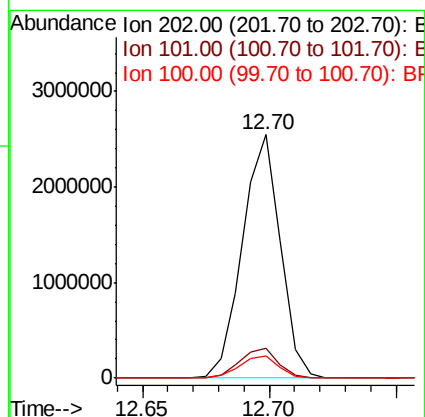

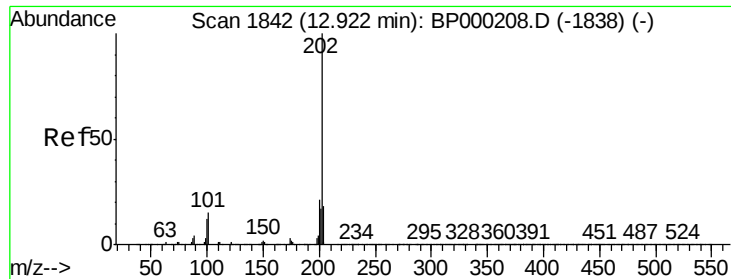





#80
Pvrene
Concen: 30.691 ng/ul
RT: 12.93 min Scan# 1844
Delta R.T. 0.02 min
Lab File: BP000216.D
Acq: 12 Sep 2019 14:27

Instrument :
BNA_P
ClientSampleId :
F2D37DL

Tot Ion	Ratio	Lower	Upper
202	100		
101	14.1	13.4	20.0
100	11.1	10.8	16.2




Manual Integrations
APPROVED


mohammad
9/16/2019 9:09:08 AM

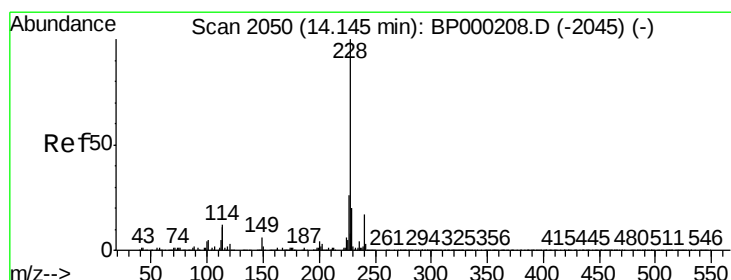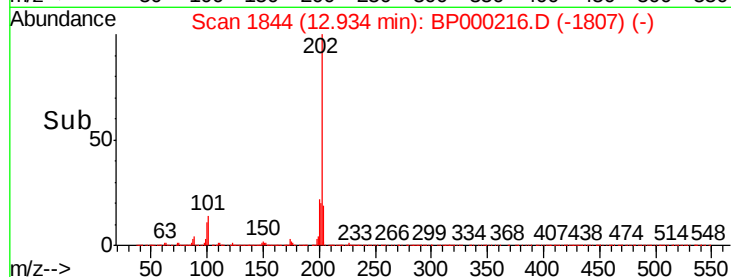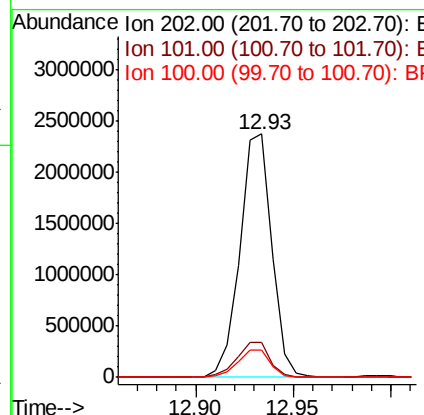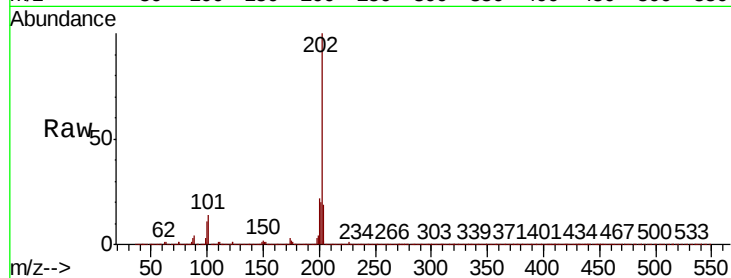

#83
Benzo(a)anthracene
Concen: 25.468 ng/ul
RT: 14.16 min Scan# 2052
Delta R.T. 0.02 min
Lab File: BP000216.D
Acq: 12 Sep 2019 14:27

Tgt Ion	Ratio	Lower	Upper
228	100		
229	22.5	15.9	23.9
226	30.0	22.1	33.1

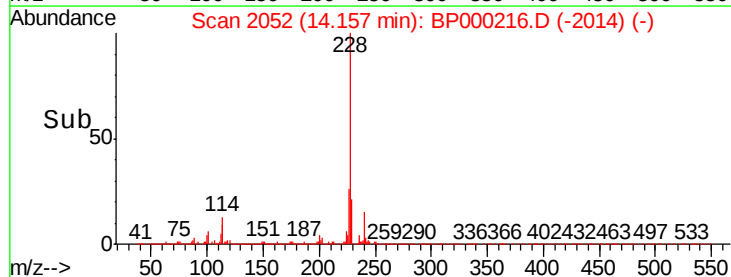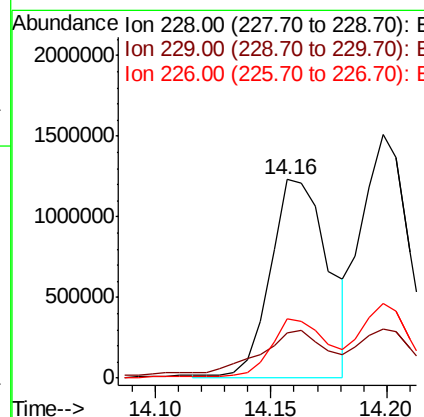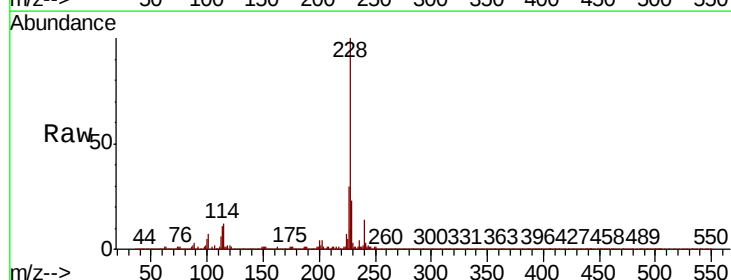

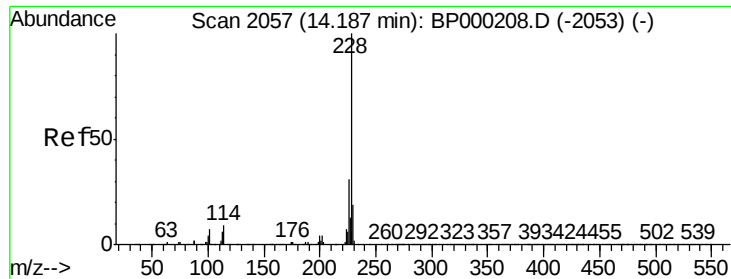





#85
Chrysene
Concen: 27.541 ng/ul
RT: 14.20 min Scan# 2059
Delta R.T. 0.03 min
Lab File: BP000216.D
Acq: 12 Sep 2019 14:27

Instrument :
BNA_P
ClientSampleID :
F2D37DL

Tot Ion	Ratio	Lower	Upper
228	100		
226	30.5	24.4	36.6
229	20.4	16.0	24.0




Manual Integrations
APPROVED


mohammad
9/16/2019 9:09:08 AM

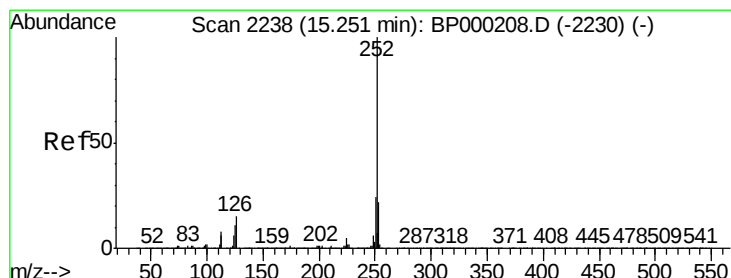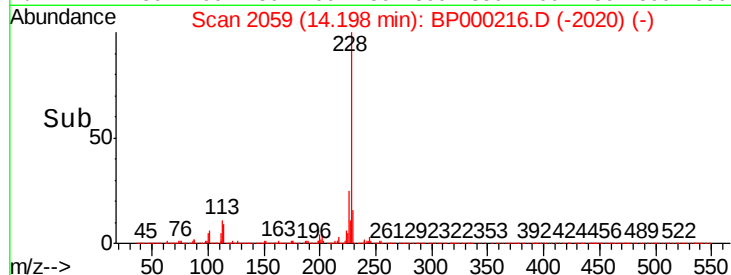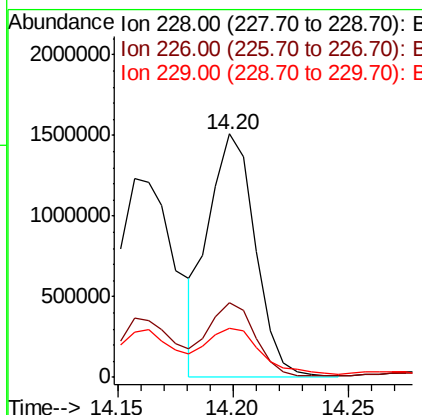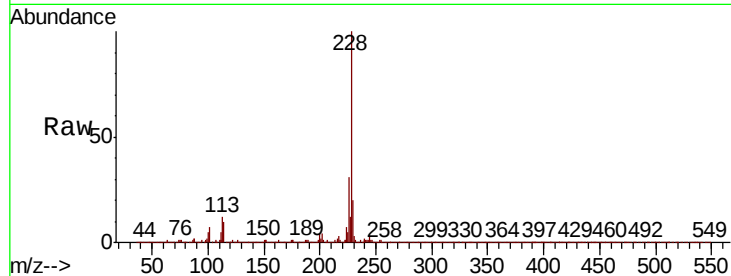

#88
Benzo(b)fluoranthene
Concen: 22.475 ng/ul m
RT: 15.31 min Scan# 2248
Delta R.T. 0.08 min
Lab File: BP000216.D
Acq: 12 Sep 2019 14:27

Tgt Ion	Ratio	Lower	Upper
252	100		
253	21.3	17.5	26.3
125	10.9	9.9	14.9

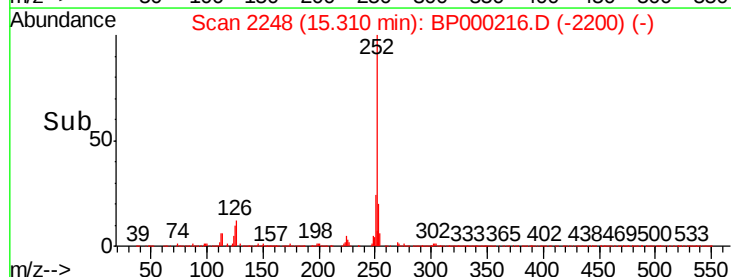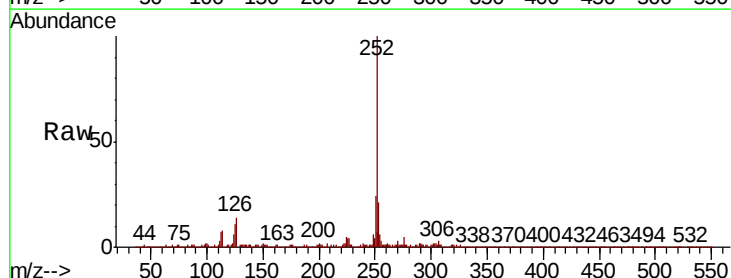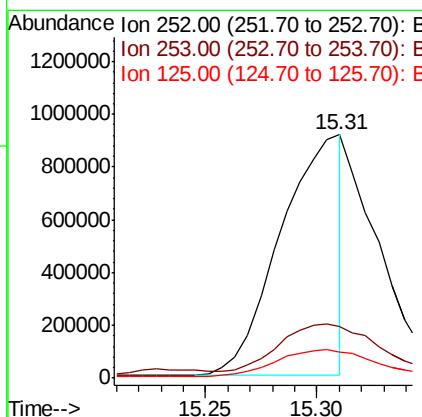

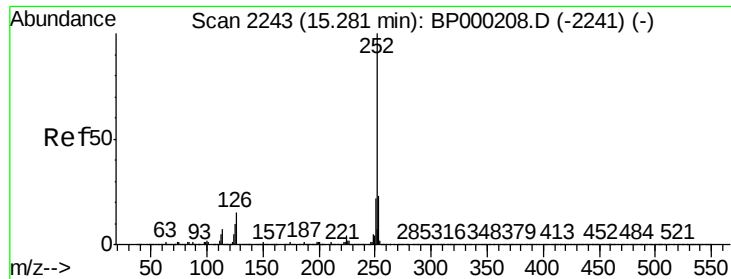





#89
Benzo(k)fluoranthene
Concen: 12.331 ng/ul m
RT: 15.31 min Scan# 2248
Delta R.T. 0.05 min
Lab File: BP000216.D
Acq: 12 Sep 2019 14:27

Instrument :
BNA_P
ClientSampleId :
F2D37DL

Tot Ion	Ratio	Lower	Upper
252	100		
253	21.3	18.0	27.0
125	10.9	10.2	15.2




Manual Integrations
APPROVED


mohammad
9/16/2019 9:09:08 AM

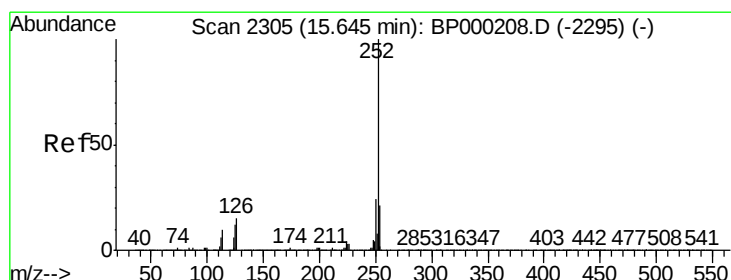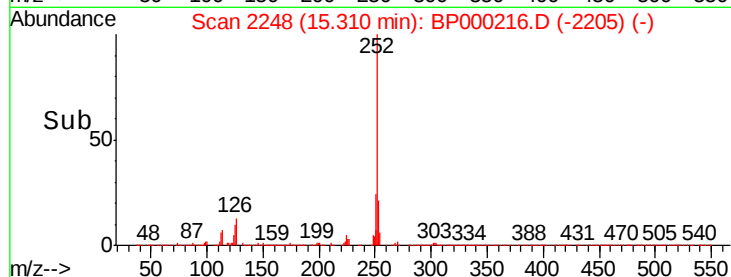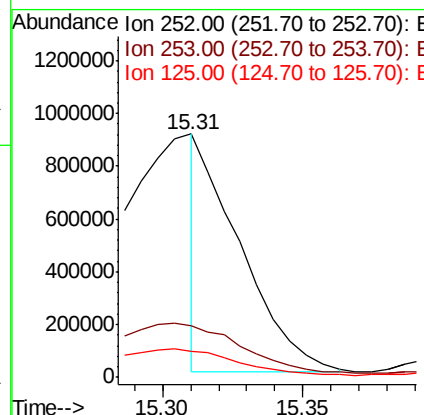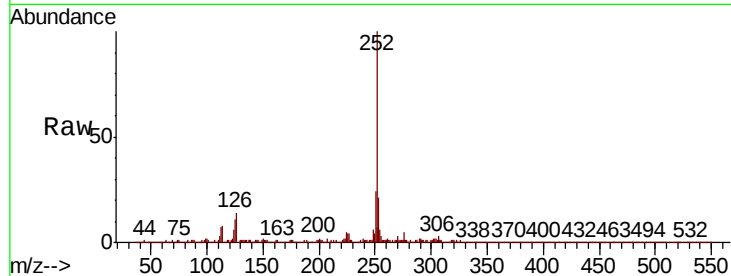

#91
Benzo(a)pyrene
Concen: 20.150 ng/ul
RT: 15.69 min Scan# 2313
Delta R.T. 0.08 min
Lab File: BP000216.D
Acq: 12 Sep 2019 14:27

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.6	17.5	26.3
125	11.9	10.2	15.2

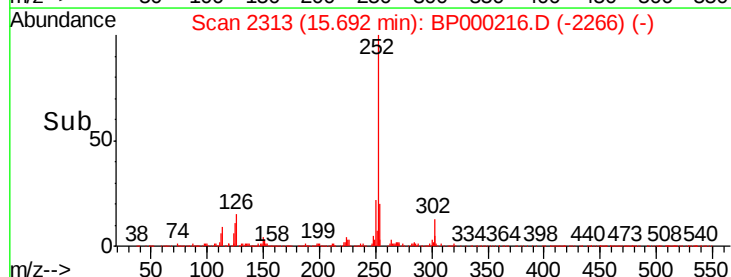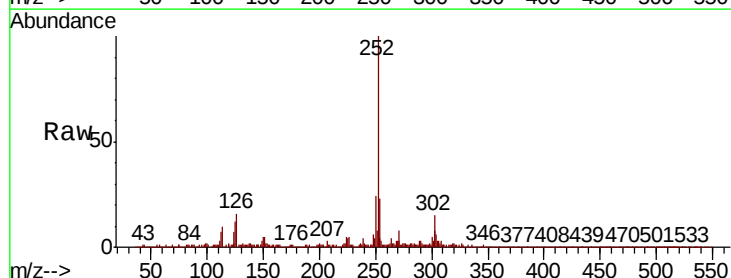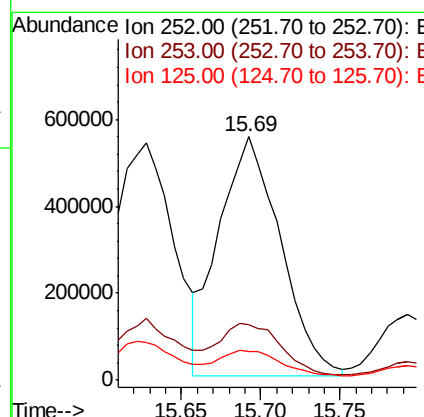

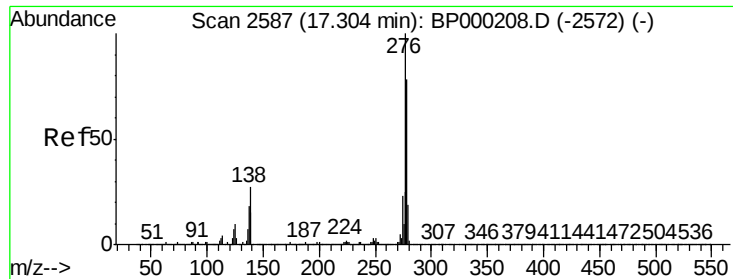





#92
 Indeno(1,2,3-cd)pyrene
 Concen: 8.243 ng/ul
 RT: 17.35 min Scan# 2595
 Delta R.T. 0.10 min
 Lab File: BP000216.D
 Acq: 12 Sep 2019 14:27

Instrument :
 BNA_P
 ClientSampled :
 F2D37DL

Tot Ion	Ratio	Lower	Upper
276	100		
138	29.6	20.0	30.0
277	25.9	19.4	29.0




Manual Integrations
 APPROVED


mohammad
 9/16/2019 9:09:08 AM

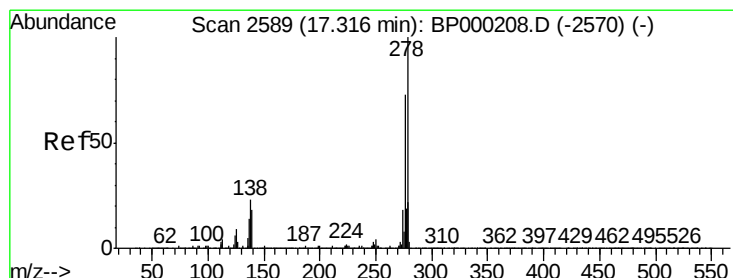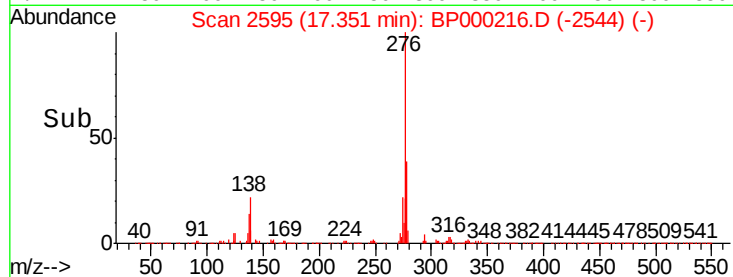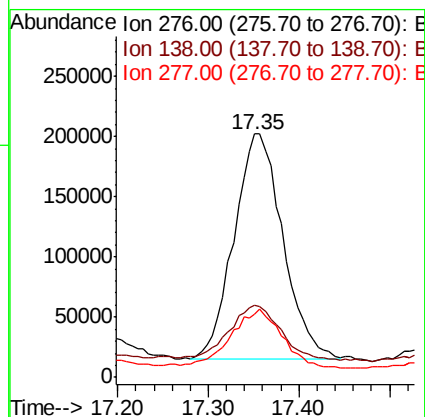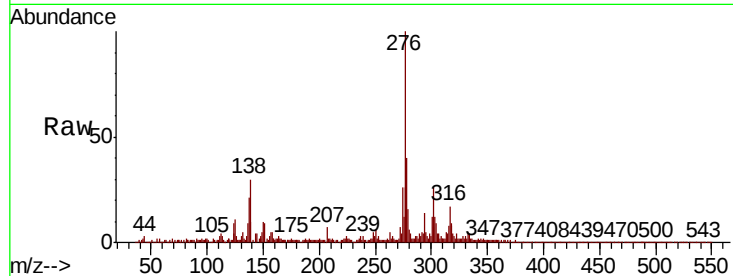

#93
 Dibenzo(a,h)anthracene
 Concen: 3.388 ng/ul
 RT: 17.36 min Scan# 2597
 Delta R.T. 0.09 min
 Lab File: BP000216.D
 Acq: 12 Sep 2019 14:27

Tgt Ion	Ratio	Lower	Upper
278	100		
139	21.8	15.1	22.7
279	36.2	19.2	28.8#

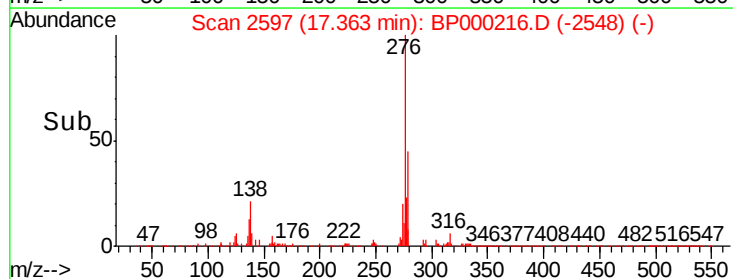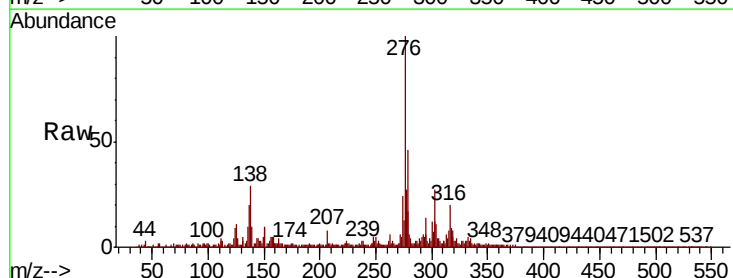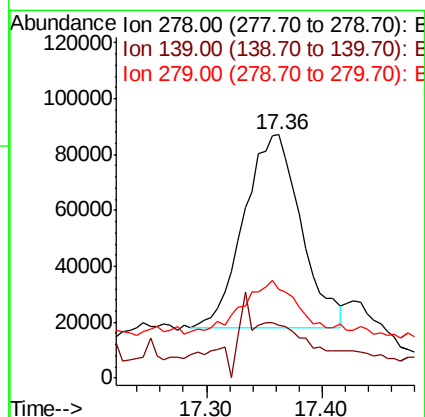

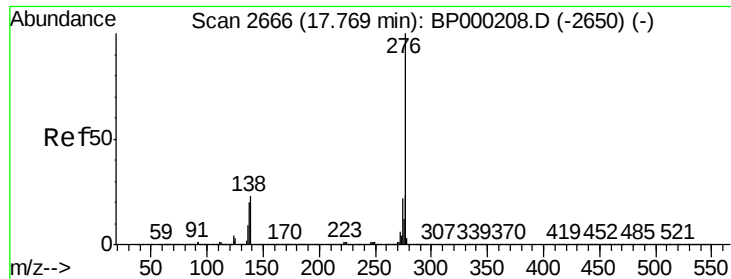

#94

Benzo(a,h,i)perylene

Concen: 11.145 ng/ul m

RT: 17.84 min Scan# 2678

Delta R.T. 0.12 min

Lab File: BP000216.D

Acq: 12 Sep 2019 14:27

Instrument :

BNA_P

ClientSampleId :

F2D37DL

Tot Ion:	276	Resp:	789927
Ion Ratio	Lower	Upper	
276	100		
138	25.0	20.0	30.0
277	23.7	19.1	28.7

Manual Integrations
APPROVED

mohammad
9/16/2019 9:09:08 AM

