

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091223\
 Data File : BM041812.D
 Acq On : 12 Sep 2023 14:58
 Operator : MA/JU
 Sample : PB155326BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Sep 13 03:10:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 04:50:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	10114	0.400	ng/ul	0.00
4) Naphthalene-d8	10.790	136	26251	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.620	164	14338	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.371	188	28956	0.400	ng/ul	0.00
17) Chrysene-d12	21.542	240	14362	0.400	ng/ul #	0.00
23) Perylene-d12	23.962	264	15073	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	62051	4.014	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.374	152	9265	0.274	ng/ul	0.00
18) Fluoranthene-d10	19.389	212	15722	0.226	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.614	166	4173	0.054	ng/ul#	13
20) Pyrene	19.761	202	3699	0.022	ng/ul#	1
26) Benzo(a)pyrene	23.807	252	5916	0.054	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091223\
Data File : BM041812.D
Acq On : 12 Sep 2023 14:58
Operator : MA/JU
Sample : PB155326BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Sep 13 03:10:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 04:50:34 2023
Response via : Initial Calibration

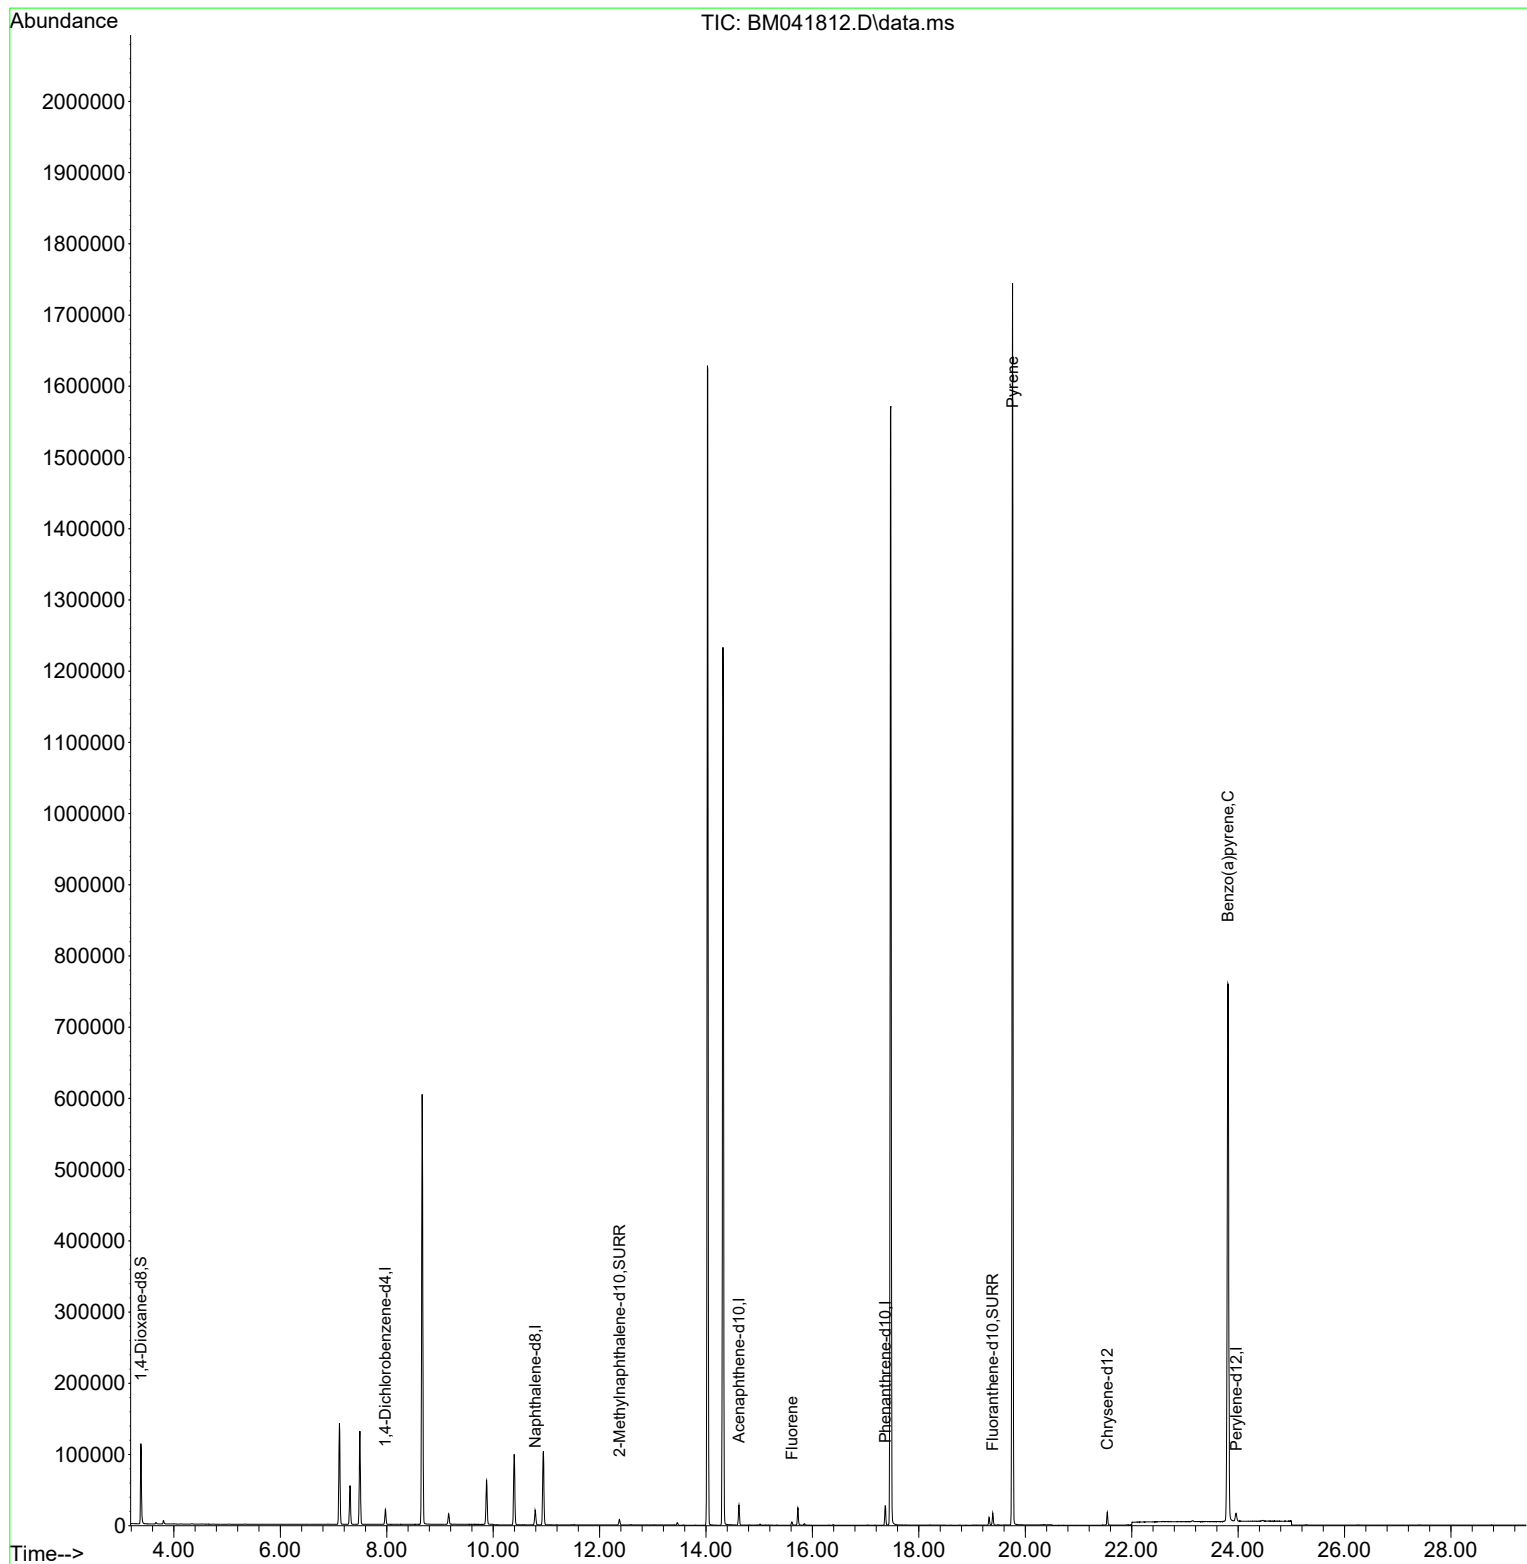

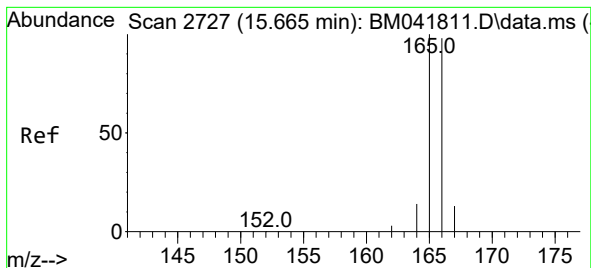

#12

Fluorene

Concen: 0.054 ng/ul

RT: 15.614 min Scan# 21

Delta R.T. -0.056 min

Lab File: BM041812.D





Acq: 12 Sep 2023 14:58

Instrument :

BNA_P

ClientSampleId :

Tgt Ion:166	Resp:	4173
Ion	Ratio	Lower Upper
166	100	
165	6.7	79.4 119.2#
167	33.4	11.3 16.9#

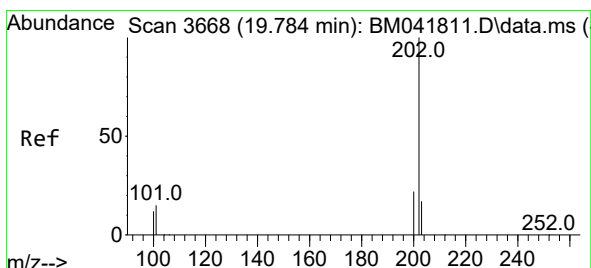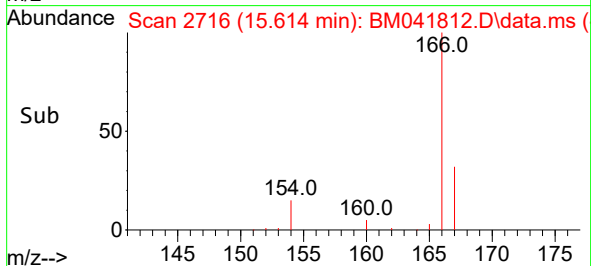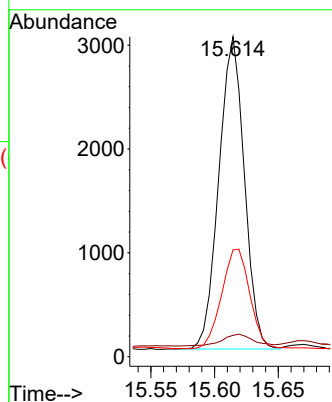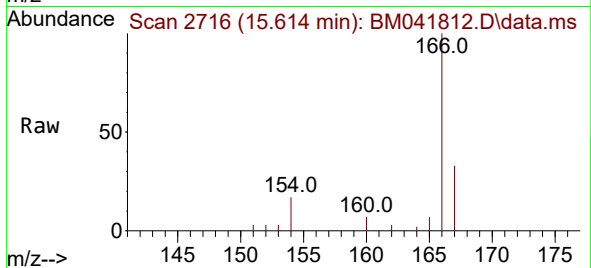

#20

Pyrene

Concen: 0.022 ng/ul




RT: 19.761 min Scan# 3663


Delta R.T. -0.028 min

Lab File: BM041812.D

Acq: 12 Sep 2023 14:58


Tgt Ion:202	Resp:	3699
Ion	Ratio	Lower Upper
202	100	
101	163.4	11.8 17.8#
100	1207.8	9.8 14.6#

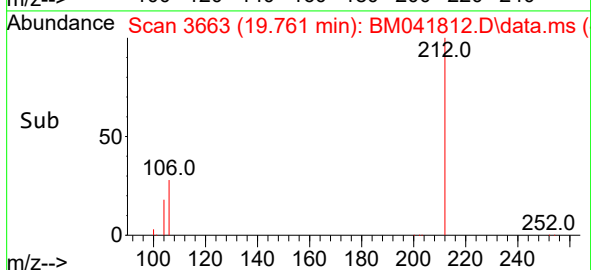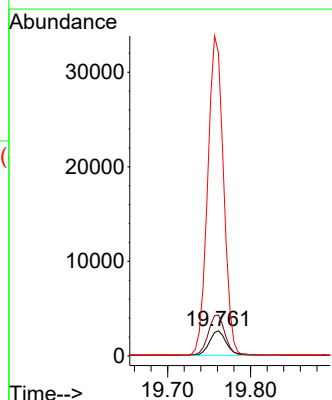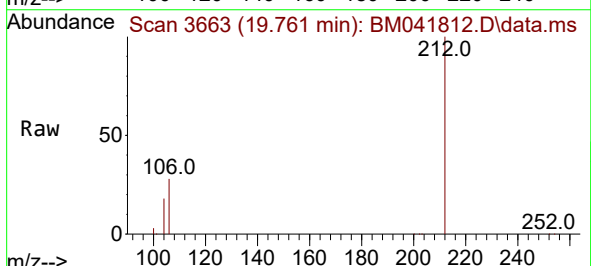

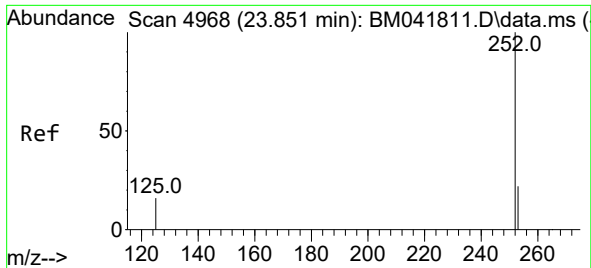

#26
Benzo(a)pyrene
Concen: 0.054 ng/ul
RT: 23.807 min Scan# 49
Delta R.T. -0.047 min
Lab File: BM041812.D
Acq: 12 Sep 2023 14:58

Instrument :
BNA_P
ClientSampleId :

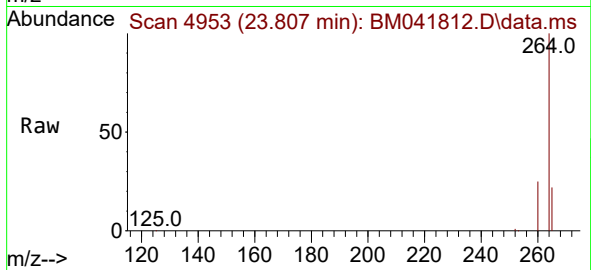

Tgt Ion:252 Resp: 5916
Ion Ratio Lower Upper
252 100
253 45.3 22.4 33.6#
125 44.1 21.0 31.4#

