

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017144.D
 Acq On : 13 Sep 2023 12:14
 Operator : MA/JU
 Sample : 04324-14
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBKA8

Quant Time: Sep 13 23:17:38 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 12 23:27:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	142917	20.000	ng/ul	0.00
20) Naphthalene-d8	10.781	136	613365	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.610	164	404072	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.380	188	969129	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	978315	20.000	ng/ul	0.00
88) Perylene-d12	24.010	264	1072960	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	18964	5.576	ng/uL	0.00
4) Pyridine-d5	3.752	84	82265	8.456	ng/ul	0.00
7) Phenol-d5	7.105	99	116090	9.990	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.293	67	296686	40.847	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	295118	31.833	ng/ul	0.00
15) 4-Methylphenol-d8	8.663	113	206888	21.481	ng/ul	0.00
21) Nitrobenzene-d5	9.152	128	179497	41.793	ng/ul	0.00
24) 2-Nitrophenol-d4	9.869	143	174719	38.105	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.393	165	331088	37.337	ng/ul	0.00
31) 4-Chloroaniline-d4	10.940	131	275110	20.583	ng/ul	0.00
46) Dimethylphthalate-d6	14.028	166	1277586	44.431	ng/ul	0.00
49) Acenaphthylene-d8	14.310	160	1367146	41.902	ng/ul	0.00
54) 4-Nitrophenol-d4	14.834	143	35423	6.374	ng/ul	0.00
60) Fluorene-d10	15.610	176	1140172	45.859	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.739	200	152493	28.164	ng/ul	0.00
73) Anthracene-d10	17.480	188	2194732	53.301	ng/ul	0.00
81) Pyrene-d10	19.722	212	2731186	53.232	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.845	264	2785358	55.001	ng/ul	0.00
Target Compounds						
					Qvalue	
6) Benzaldehyde	7.110	77	8674	1.341	ng/ul	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017144.D
Acq On : 13 Sep 2023 12:14
Operator : MA/JU
Sample : 04324-14
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBKA8

Quant Time: Sep 13 23:17:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 12 23:27:27 2023
Response via : Initial Calibration

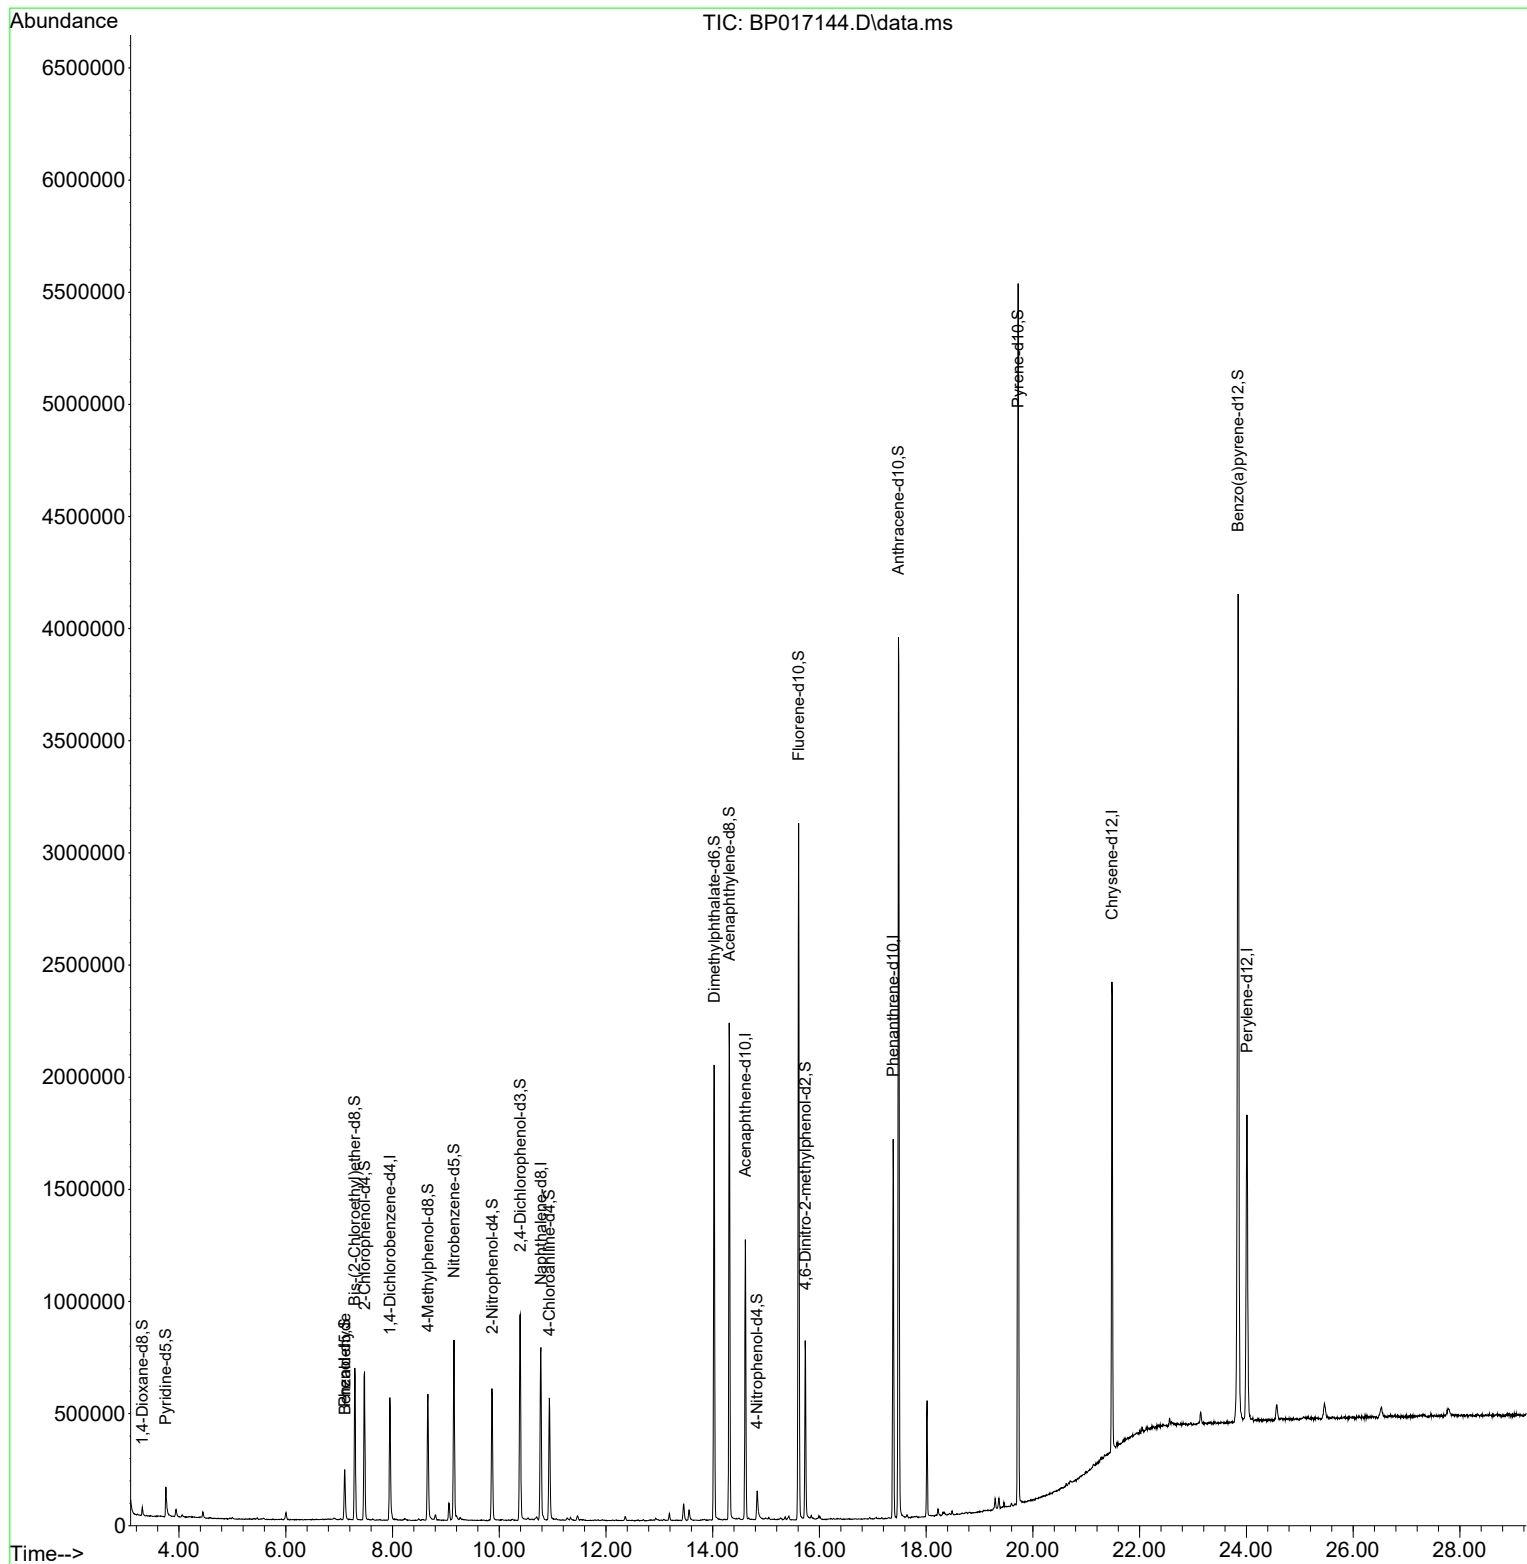

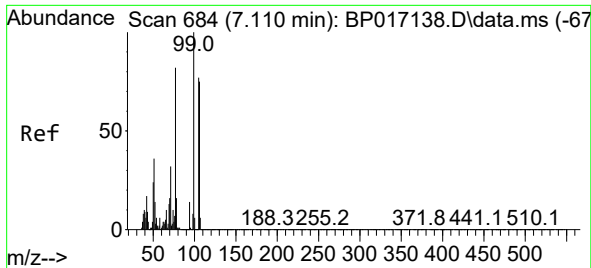

#6
Benzaldehyde
Concen: 1.341 ng/ul
RT: 7.110 min Scan# 61
Delta R.T. -0.006 min
Lab File: BP017144.D
Acq: 13 Sep 2023 12:14

Instrument :
BNA_P
ClientSampleId :
BBKA8

Tgt Ion: 77 Resp: 8674
Ion Ratio Lower Upper
77 100
105 77.9 75.3 112.9
106 85.3 74.6 111.8

