

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017145.D
 Acq On : 13 Sep 2023 12:49
 Operator : MA/JU
 Sample : 04330-03
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZYP2

Quant Time: Sep 13 23:17:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 12 23:27:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	185742	20.000	ng/ul	0.00
20) Naphthalene-d8	10.781	136	763630	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.610	164	485469	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.381	188	1099196	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	984633	20.000	ng/ul	0.00
88) Perylene-d12	24.010	264	973179	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.317	96	26465	5.988	ng/uL	0.00
4) Pyridine-d5	3.752	84	175053	13.845	ng/ul	0.00
7) Phenol-d5	7.105	99	142955	9.465	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.293	67	402831	42.673	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	392226	32.553	ng/ul	0.00
15) 4-Methylphenol-d8	8.663	113	256807	20.517	ng/ul	0.00
21) Nitrobenzene-d5	9.152	128	238680	44.637	ng/ul	0.00
24) 2-Nitrophenol-d4	9.863	143	253910	44.479	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.393	165	434551	39.362	ng/ul	0.00
31) 4-Chloroaniline-d4	10.940	131	397838	23.908	ng/ul	0.00
46) Dimethylphthalate-d6	14.028	166	1589003	45.996	ng/ul	0.00
49) Acenaphthylene-d8	14.310	160	1736558	44.300	ng/ul	0.00
54) 4-Nitrophenol-d4	14.834	143	40662	6.090	ng/ul	0.00
60) Fluorene-d10	15.610	176	1400686	46.891	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.739	200	231032	37.620	ng/ul	0.00
73) Anthracene-d10	17.486	188	2428934	52.009	ng/ul	0.00
81) Pyrene-d10	19.722	212	2894187	56.046	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.845	264	2434273	52.997	ng/ul	0.00


Target Compounds					Qvalue
6) Benzaldehyde	7.110	77	9889	1.176 ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017145.D
Acq On : 13 Sep 2023 12:49
Operator : MA/JU
Sample : 04330-03
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZIP2

Quant Time: Sep 13 23:17:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 12 23:27:27 2023
Response via : Initial Calibration

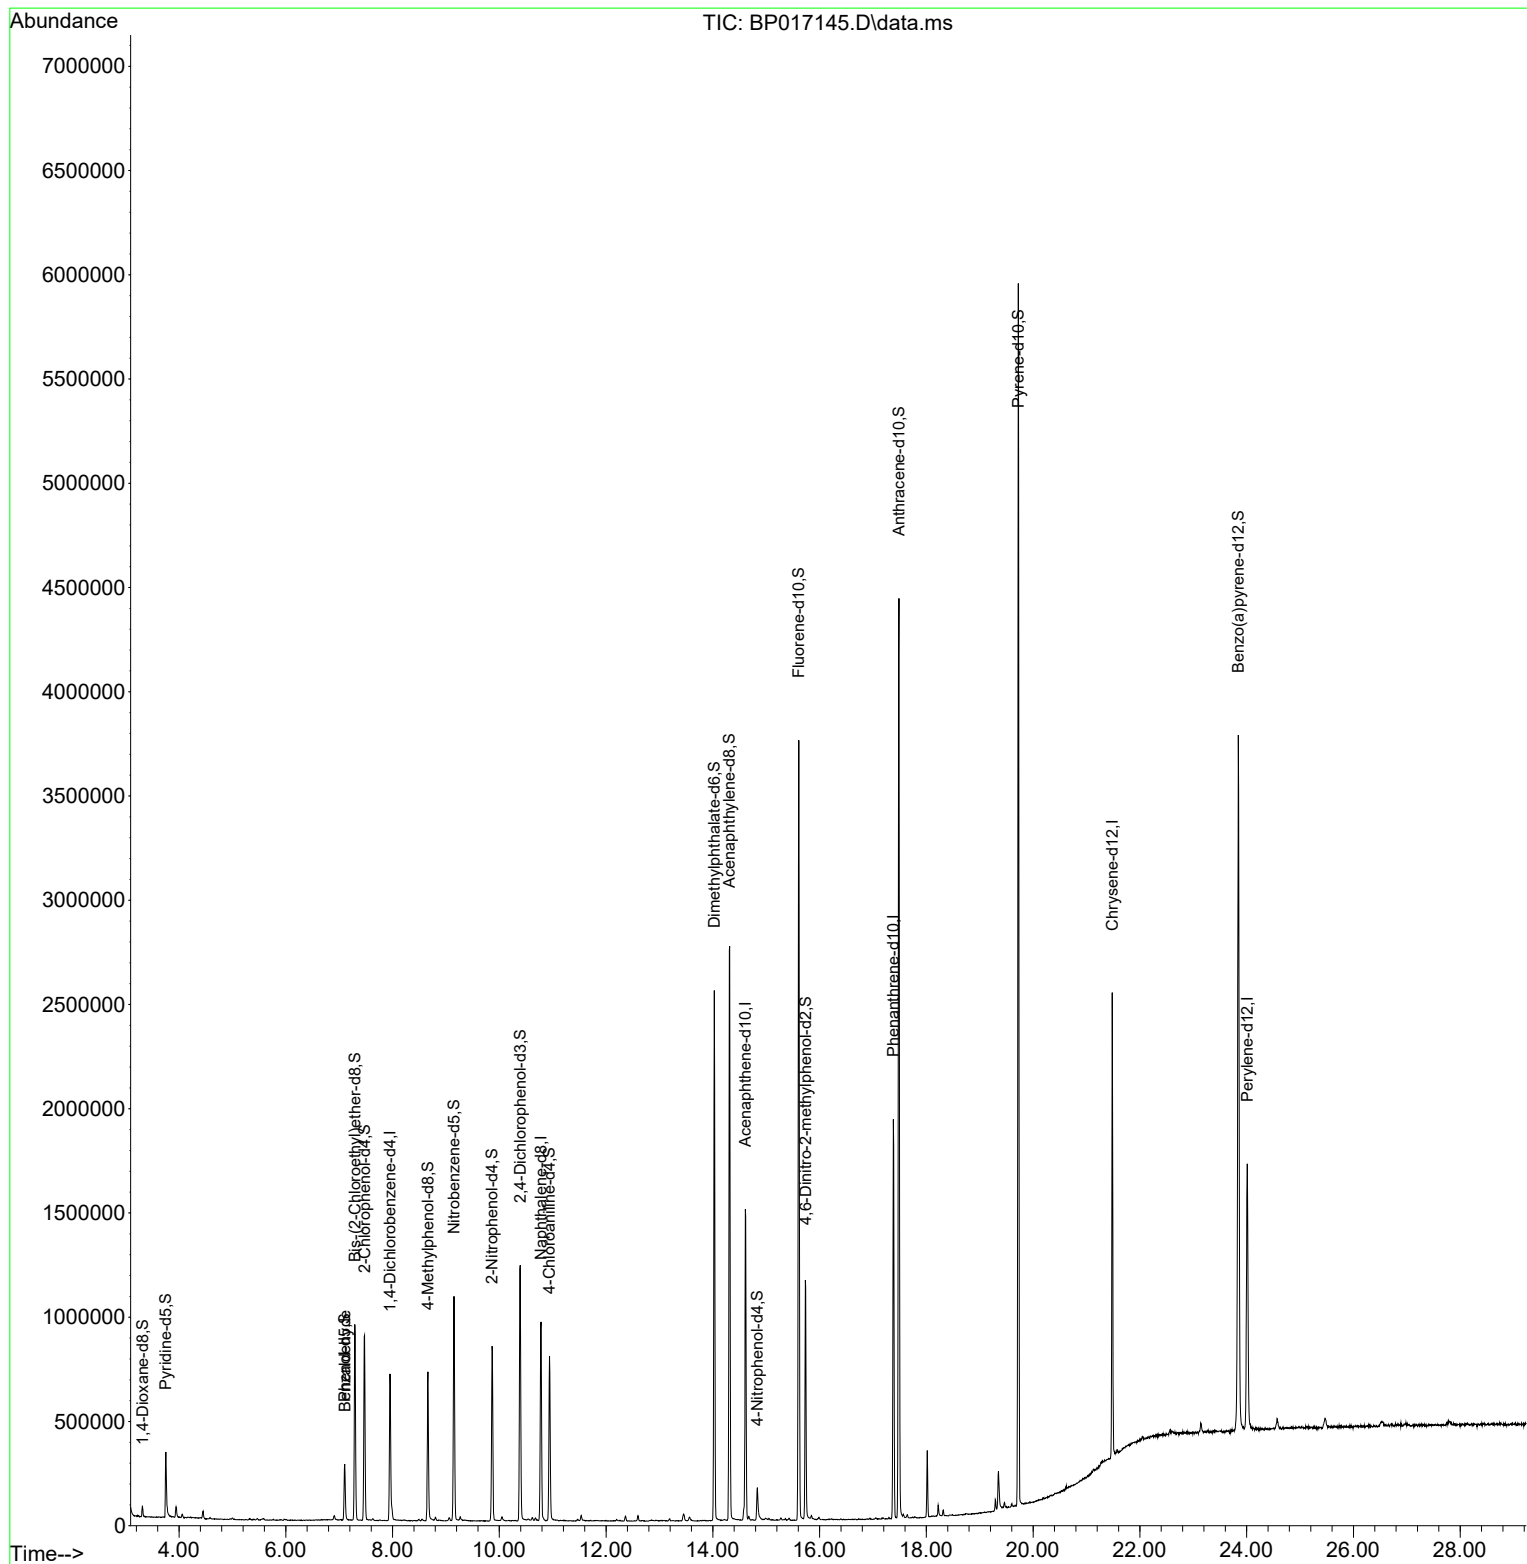

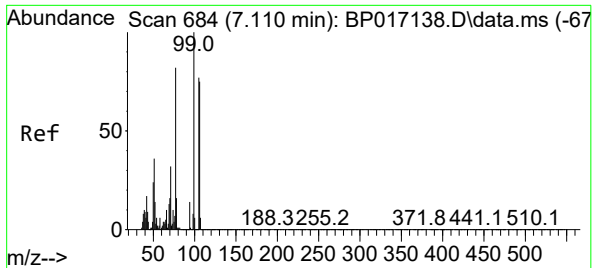

#6
Benzaldehyde
Concen: 1.176 ng/ul
RT: 7.110 min Scan# 61
Delta R.T. -0.006 min
Lab File: BP017145.D
Acq: 13 Sep 2023 12:49

Instrument :
BNA_P
ClientSampleId :
EZYP2

Tgt Ion:	77	Resp:	9889
Ion	Ratio	Lower	Upper
77	100		
105	90.1	75.3	112.9
106	73.6	74.6	111.8#

