

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017147.D
 Acq On : 13 Sep 2023 13:58
 Operator : MA/JU
 Sample : 04324-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHF8

Quant Time: Sep 13 23:18:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 12 23:27:27 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	168844	20.000	ng/ul	0.00
20) Naphthalene-d8	10.775	136	635991	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.610	164	356786	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.381	188	764257	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	759974	20.000	ng/ul	0.00
88) Perylene-d12	24.010	264	898663	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.317	96	25925	6.452	ng/uL	0.00
4) Pyridine-d5	3.752	84	112217	9.763	ng/ul	0.00
7) Phenol-d5	7.105	99	133002	9.688	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.293	67	379831	44.264	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	378766	34.582	ng/ul	0.00
15) 4-Methylphenol-d8	8.663	113	234466	20.606	ng/ul	0.00
21) Nitrobenzene-d5	9.152	128	217777	48.901	ng/ul	0.00
24) 2-Nitrophenol-d4	9.863	143	225560	47.443	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	389705	42.384	ng/ul	0.00
31) 4-Chloroaniline-d4	10.940	131	271271	19.574	ng/ul	0.00
46) Dimethylphthalate-d6	14.028	166	1247477	49.133	ng/ul	0.00
49) Acenaphthylene-d8	14.310	160	1383817	48.034	ng/ul	0.00
54) 4-Nitrophenol-d4	14.834	143	32363	6.595	ng/ul	0.00
60) Fluorene-d10	15.610	176	1086033	49.470	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.734	200	167355	39.194	ng/ul	-0.01
73) Anthracene-d10	17.481	188	1776541	54.711	ng/ul	0.00
81) Pyrene-d10	19.722	212	2240223	56.207	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.845	264	2453258	57.839	ng/ul	0.00
Target Compounds						
34) Caprolactam	11.775	113	27173	9.288	ng/ul	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017147.D
Acq On : 13 Sep 2023 13:58
Operator : MA/JU
Sample : 04324-07
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHF8

Quant Time: Sep 13 23:18:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 12 23:27:27 2023
Response via : Initial Calibration

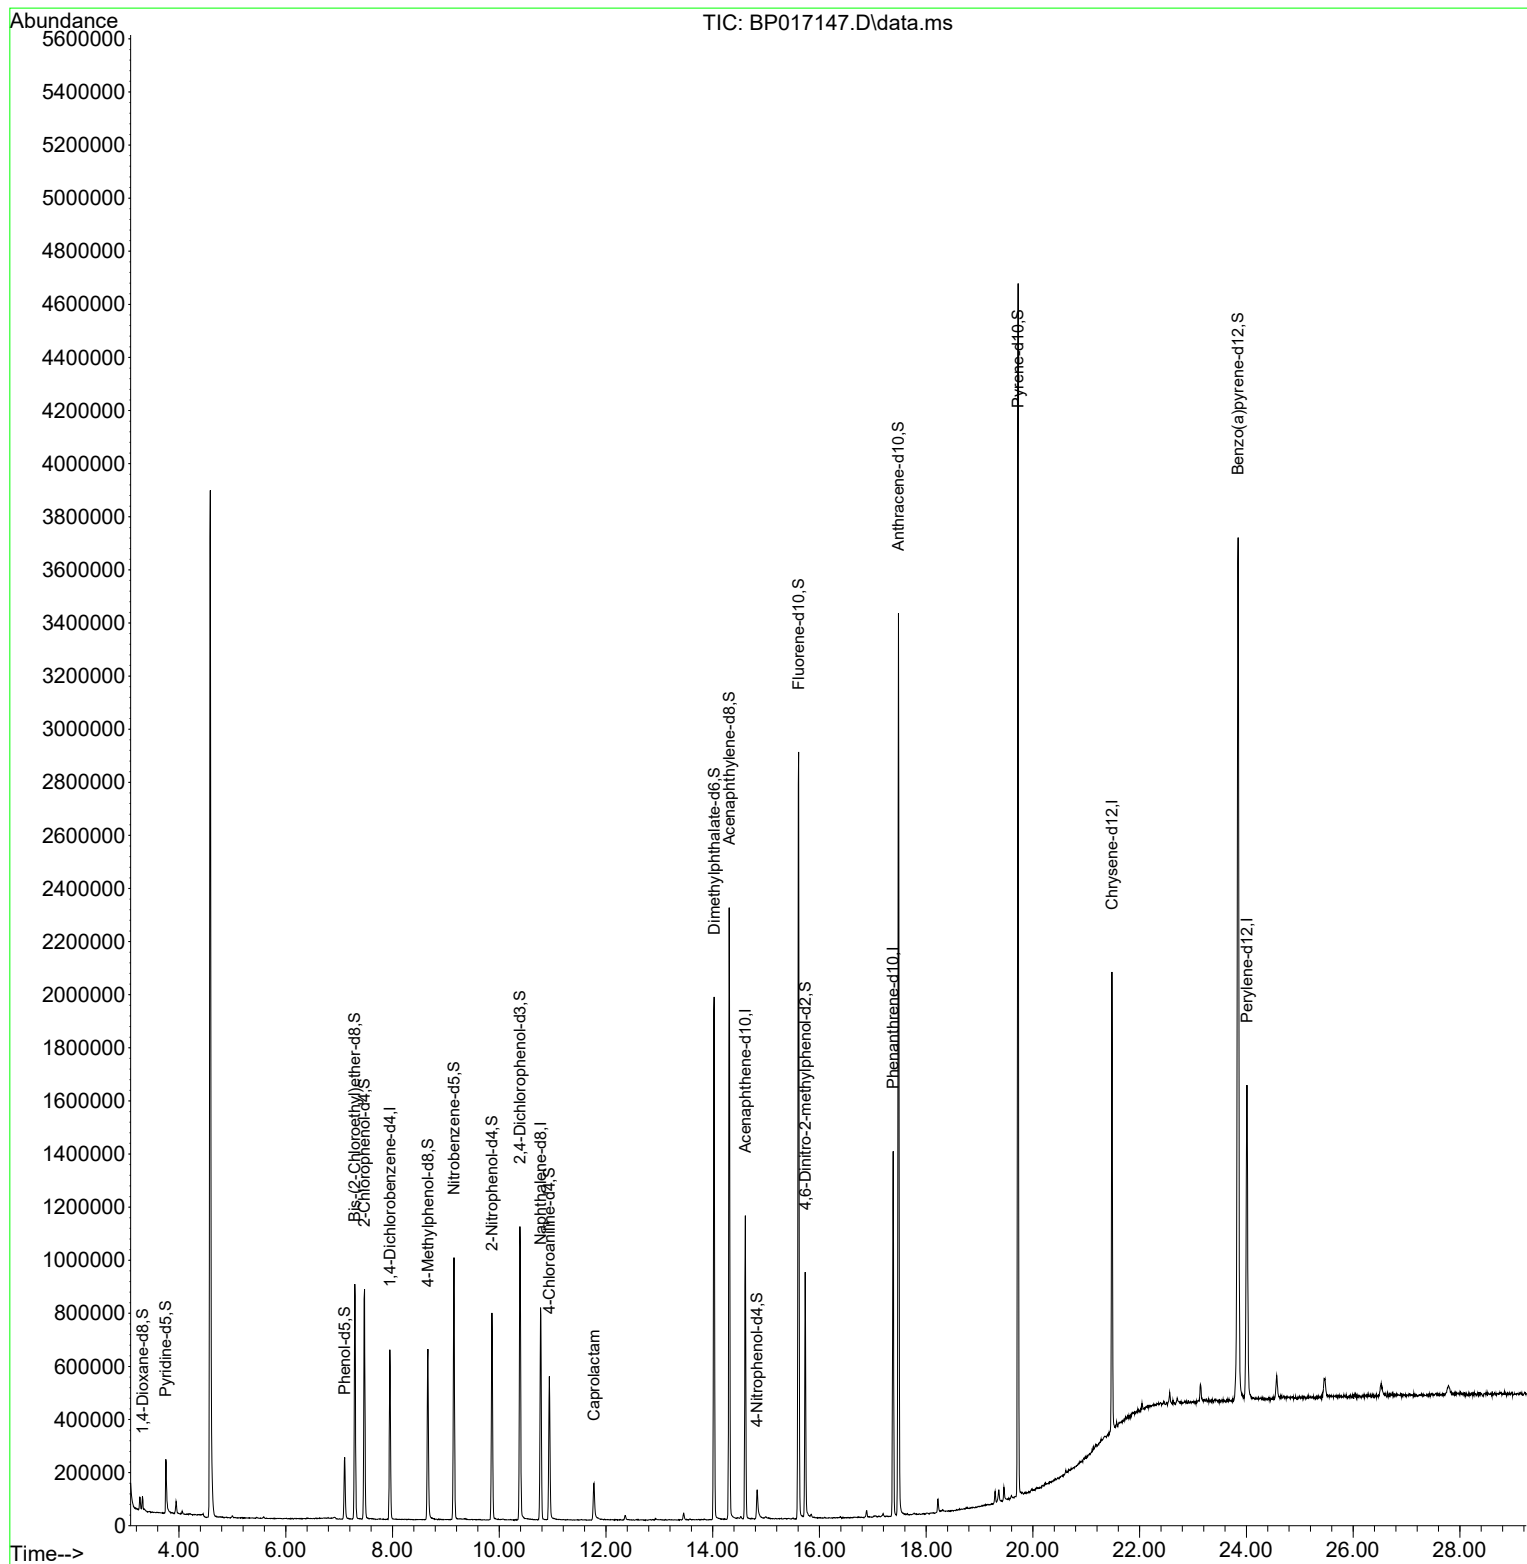

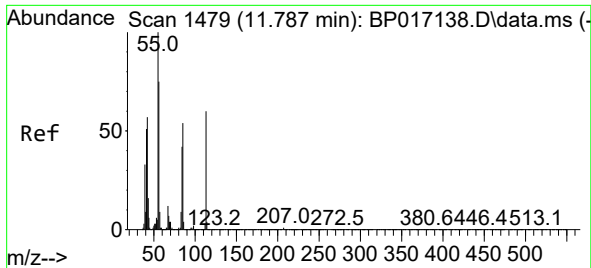

#34
 Caprolactam
 Concen: 9.288 ng/ul
 RT: 11.775 min Scan# 14
 Delta R.T. -0.023 min
 Lab File: BP017147.D
 Acq: 13 Sep 2023 13:58

Instrument :
 BNA_P
 ClientSampleId :
 BBHF8

Tgt Ion:113 Resp: 27173
 Ion Ratio Lower Upper
 113 100
 55 166.6 130.7 196.1
 56 126.2 96.8 145.2

