

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017156.D
 Acq On : 13 Sep 2023 19:09
 Operator : MA/JU
 Sample : 04324-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHW8

Quant Time: Sep 13 23:20:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 12 23:27:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	169127	20.000	ng/ul	0.00
20) Naphthalene-d8	10.781	136	716542	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.610	164	453516	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.380	188	1041882	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	969447	20.000	ng/ul	0.00
88) Perylene-d12	24.004	264	978203	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	23643	5.875	ng/uL	0.00
4) Pyridine-d5	3.752	84	141184	12.263	ng/ul	0.00
7) Phenol-d5	7.104	99	115628	8.408	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.293	67	316023	36.766	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	309403	28.202	ng/ul	0.00
15) 4-Methylphenol-d8	8.663	113	209658	18.395	ng/ul	0.00
21) Nitrobenzene-d5	9.151	128	186045	37.080	ng/ul	0.00
24) 2-Nitrophenol-d4	9.863	143	190639	35.590	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	352344	34.013	ng/ul	0.00
31) 4-Chloroaniline-d4	10.940	131	275418	17.639	ng/ul	0.00
46) Dimethylphthalate-d6	14.028	166	1264332	39.176	ng/ul	0.00
49) Acenaphthylene-d8	14.310	160	1357497	37.070	ng/ul	0.00
54) 4-Nitrophenol-d4	14.834	143	36918	5.919	ng/ul	0.00
60) Fluorene-d10	15.610	176	1113650	39.909	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.733	200	183126	31.460	ng/ul	-0.01
73) Anthracene-d10	17.480	188	1942978	43.892	ng/ul	0.00
81) Pyrene-d10	19.721	212	2467406	48.530	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.839	264	2167814	46.953	ng/ul	-0.01
Target Compounds						
					Qvalue	
34) Caprolactam	11.775	113	29967	9.092	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017156.D
Acq On : 13 Sep 2023 19:09
Operator : MA/JU
Sample : 04324-17
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHW8

Quant Time: Sep 13 23:20:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 12 23:27:27 2023
Response via : Initial Calibration

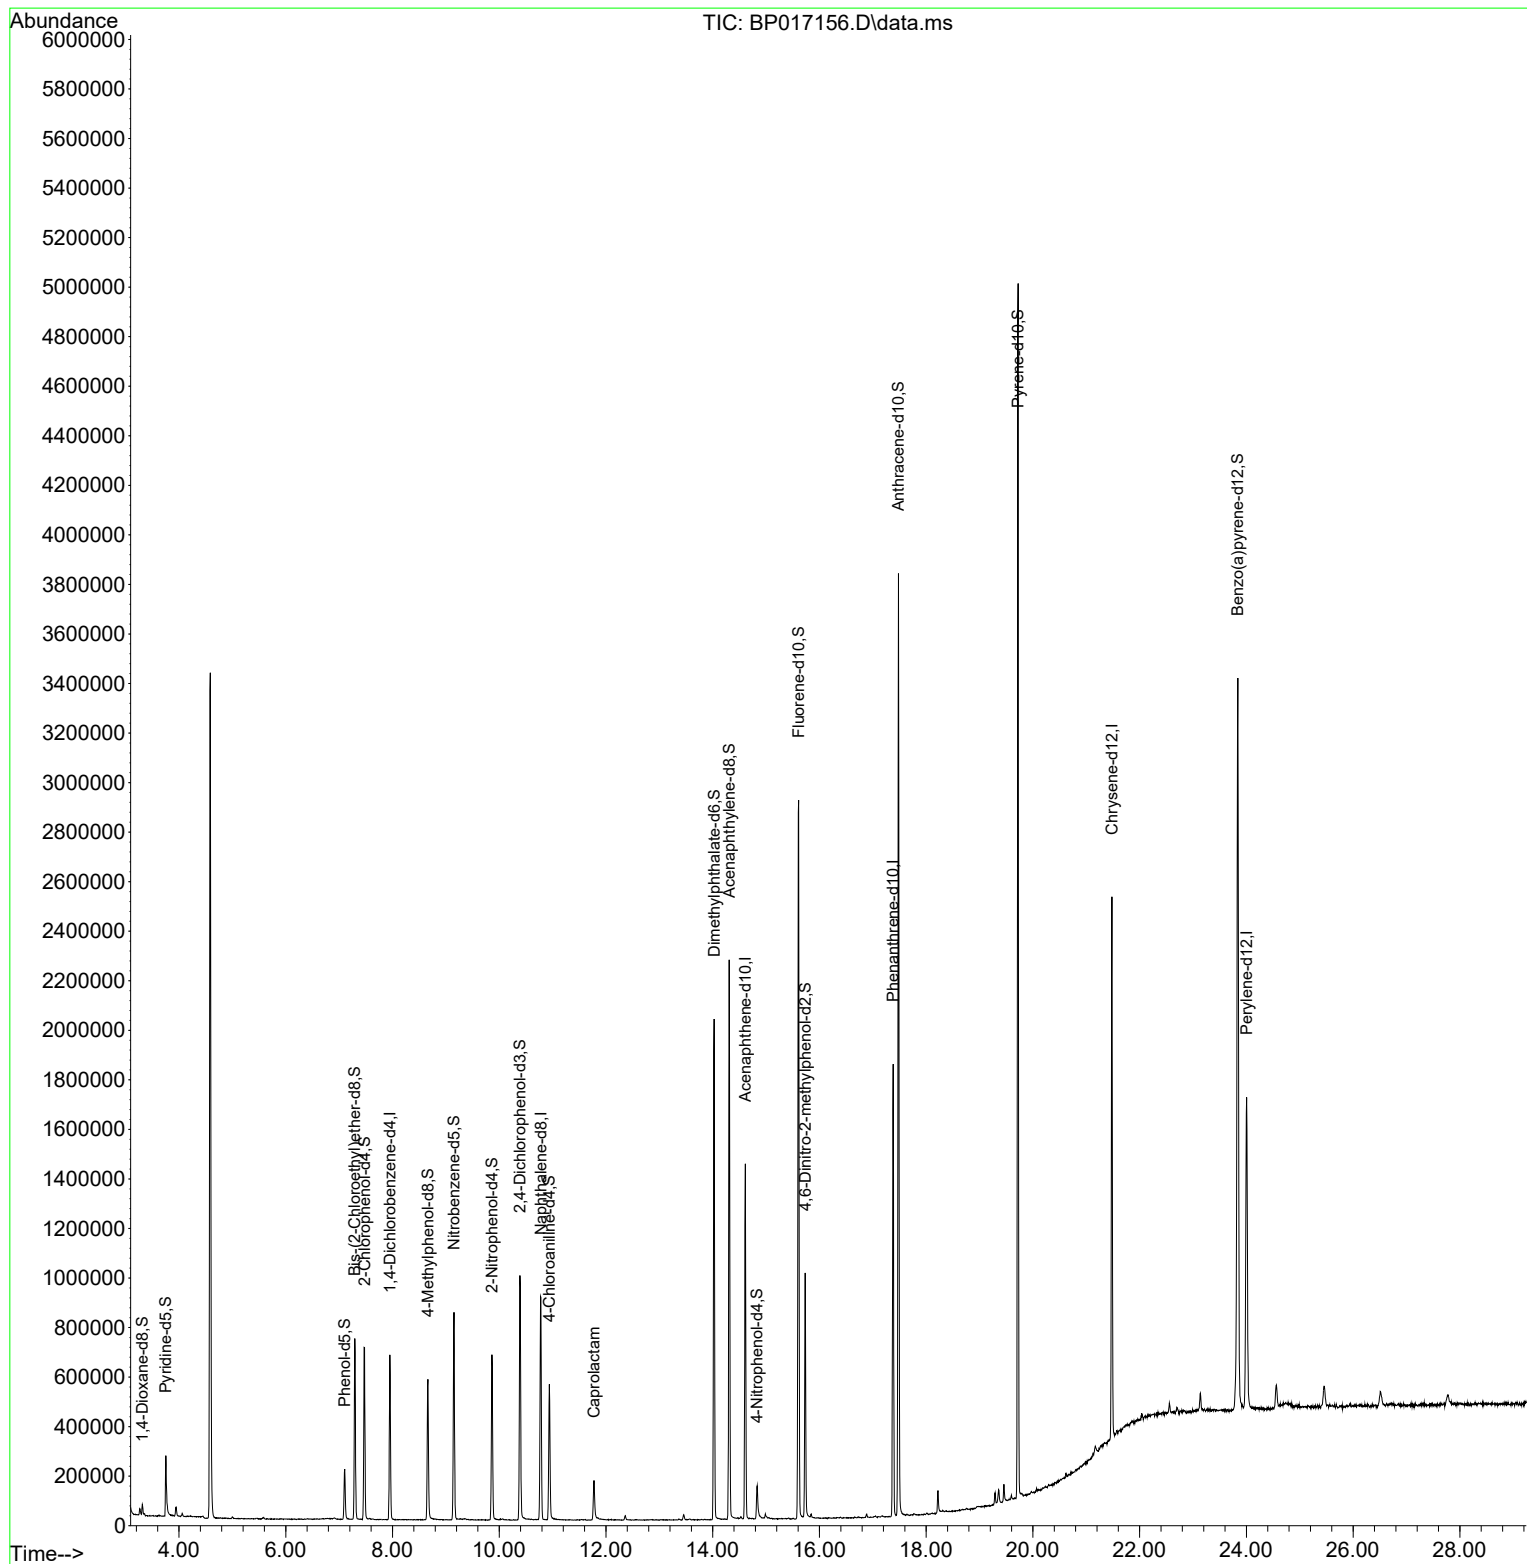

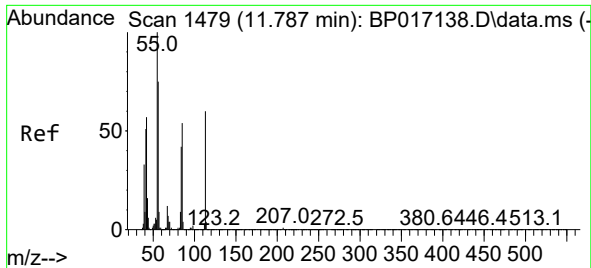

#34
 Caprolactam
 Concen: 9.092 ng/ul
 RT: 11.775 min Scan# 14
 Delta R.T. -0.024 min
 Lab File: BP017156.D
 Acq: 13 Sep 2023 19:09

Instrument :
 BNA_P
 ClientSampleId :
 BBHW8

Tgt Ion:113 Resp: 29967
 Ion Ratio Lower Upper
 113 100
 55 161.4 130.7 196.1
 56 121.9 96.8 145.2

