

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017174.D
 Acq On : 14 Sep 2023 13:25
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020734

Quant Time: Sep 14 22:47:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 12 23:27:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	227487	20.000	ng/u1	0.00
20) Naphthalene-d8	10.775	136	912601	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.610	164	530437	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.381	188	1120999	20.000	ng/u1	0.00
79) Chrysene-d12	21.486	240	1049616	20.000	ng/u1	0.00
88) Perylene-d12	24.010	264	1172897	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	45856	8.471	ng/uL	0.00
4) Pyridine-d5	3.746	84	302711	19.548	ng/u1	0.00
7) Phenol-d5	7.105	99	344806	18.641	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.293	67	227988	19.720	ng/u1	0.00
11) 2-Chlorophenol-d4	7.469	132	291133	19.729	ng/u1	0.00
15) 4-Methylphenol-d8	8.663	113	274763	17.923	ng/u1	0.00
21) Nitrobenzene-d5	9.152	128	135031	21.131	ng/u1	0.00
24) 2-Nitrophenol-d4	9.863	143	143894	21.092	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	270950	20.536	ng/u1	0.00
31) 4-Chloroaniline-d4	10.940	131	377386	18.977	ng/u1	0.00
46) Dimethylphthalate-d6	14.028	166	766794	20.314	ng/u1	0.00
49) Acenaphthylene-d8	14.310	160	894552	20.886	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	126431	17.330	ng/u1	0.00
60) Fluorene-d10	15.610	176	657503	20.145	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.739	200	113069	18.053	ng/u1	0.00
73) Anthracene-d10	17.480	188	986718	20.717	ng/u1	0.00
81) Pyrene-d10	19.722	212	1131292	20.551	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.845	264	1147401	20.727	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.346	88	47941	8.236	ng/uL	93
5) Pyridine	3.764	79	321672	20.054	ng/u1	98
6) Benzaldehyde	7.110	77	232100	22.538	ng/u1	99
8) Phenol	7.128	94	369643	18.947	ng/u1	100
10) Bis(2-Chloroethyl)ether	7.387	93	305211	19.615	ng/u1	99
12) 2-Chlorophenol	7.505	128	294176	19.640	ng/u1	99
13) 2-Methylphenol	8.393	108	267074	18.363	ng/u1	100
14) 2,2'-oxybis(1-Chloropr...	8.463	45	252454	11.972	ng/u1	99
16) Acetophenone	8.804	105	449318	18.726	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.769	70	225412	18.281	ng/u1	96
18) 4-Methylphenol	8.728	108	291690	18.128	ng/u1	97
19) Hexachloroethane	9.016	117	123215	20.002	ng/u1	96
22) Nitrobenzene	9.193	77	345359	20.753	ng/u1	99
23) Isophorone	9.704	82	601168	19.277	ng/u1	99
25) 2-Nitrophenol	9.899	139	159676	21.059	ng/u1	98
26) 2,4-Dimethylphenol	9.934	107	304115	19.680	ng/u1	96
27) Bis(2-Chloroethoxy)met...	10.193	93	390736	19.991	ng/u1	99
29) 2,4-Dichlorophenol	10.416	162	273083	20.448	ng/u1	98
30) Naphthalene	10.828	128	937708	20.305	ng/u1	100
32) 4-Chloroaniline	10.963	127	372481	19.194	ng/u1	97
33) Hexachlorobutadiene	11.057	225	194714	21.471	ng/u1	99
34) Caprolactam	11.787	113	68710	16.367	ng/u1	97
35) 4-Chloro-3-methylphenol	12.063	107	268073	18.552	ng/u1	99
36) 2-Methylnaphthalene	12.434	142	618583	19.851	ng/u1	97


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017174.D
 Acq On : 14 Sep 2023 13:25
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020734

Quant Time: Sep 14 22:47:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 12 23:27:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.651	142	619076	19.627	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.781	216	351370	22.241	ng/ul	98
40) Hexachlorocyclopentadiene	12.734	237	213880	21.728	ng/ul	98
41) 2,4,6-Trichlorophenol	13.040	196	212022	21.126	ng/ul	99
42) 2,4,5-Trichlorophenol	13.110	196	223261	20.924	ng/ul	99
43) 1,1'-Biphenyl	13.445	154	800251	21.039	ng/ul	99
44) 2-Chloronaphthalene	13.492	162	643381	21.300	ng/ul	98
45) 2-Nitroaniline	13.728	65	163987	20.043	ng/ul	99
47) Dimethylphthalate	14.075	163	769702	20.087	ng/ul	100
48) 2,6-Dinitrotoluene	14.216	165	138496	19.770	ng/ul	96
50) Acenaphthylene	14.339	152	1021867	20.652	ng/ul	99
51) 3-Nitroaniline	14.557	138	140352	18.728	ng/ul	98
52) Acenaphthene	14.675	153	666395	20.352	ng/ul	99
53) 2,4-Dinitrophenol	14.757	184	77155	15.724	ng/ul	100
55) 4-Nitrophenol	14.845	109	103134	17.663	ng/ul	98
56) Dibenzofuran	15.010	168	924078	20.423	ng/ul	99
57) 2,4-Dinitrotoluene	14.998	165	201963	19.361	ng/ul#	95
58) 2,3,4,6-Tetrachlorophenol	15.228	232	189356	20.229	ng/ul	99
59) Diethylphthalate	15.428	149	747048	19.746	ng/ul	100
61) Fluorene	15.663	166	754347	20.165	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.657	204	399390	20.999	ng/ul	97
63) 4-Nitroaniline	15.728	138	135497	19.448	ng/ul	98
66) 4,6-Dinitro-2-methylph...	15.751	198	126306	18.791	ng/ul	97
67) N-Nitrosodiphenylamine	15.881	169	608005	20.859	ng/ul	97
68) 4-Bromophenyl-phenylether	16.557	248	228924	21.424	ng/ul	98
69) Hexachlorobenzene	16.639	284	265478	20.990	ng/ul	99
70) Atrazine	16.839	200	222685	21.106	ng/ul	99
71) Pentachlorophenol	17.004	266	153314	18.652	ng/ul	99
72) Phenanthrene	17.428	178	1159057	20.575	ng/ul	99
74) Anthracene	17.516	178	1169288	20.493	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.398	216	365010	23.550	ng/ul	99
76) Pentachlorobenzene	14.904	250	316975	22.538	ng/ul	98
77) Carbazole	17.804	167	1012137	20.202	ng/ul	100
78) Di-n-butylphthalate	18.316	149	1200134	21.022	ng/ul	100
80) Fluoranthene	19.392	202	1321184	20.534	ng/ul	99
82) Pyrene	19.751	202	1397203	20.552	ng/ul	99
83) Butylbenzylphthalate	20.610	149	509114	20.997	ng/ul	96
84) 3,3'-Dichlorobenzidine	21.410	252	428464	19.911	ng/ul	97
85) Benzo(a)anthracene	21.469	228	1425742	20.746	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.345	149	742410	21.812	ng/ul	98
87) Chrysene	21.521	228	1319864	20.646	ng/ul	98
89) Di-n-octyl phthalate	22.310	149	1271664	19.553	ng/ul	100
90) Benzo(b)fluoranthene	23.221	252	1394017	20.163	ng/ul	99
91) Benzo(k)fluoranthene	23.274	252	1399523	20.363	ng/ul	99
93) Benzo(a)pyrene	23.898	252	1322316	20.616	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.686	276	1643719	23.142	ng/ul	100
95) Dibenzo(a,h)anthracene	26.715	278	1374735	23.041	ng/ul	99
96) Benzo(g,h,i)perylene	27.527	276	1298067	23.635	ng/ul	100





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 8.236 ng/uL
RT: 3.346 min Scan# 44
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25




Instrument :
BNA_P
ClientSampleId :
SSTD020734


Tgt Ion: 88 Resp: 47941
Ion Ratio Lower Upper
88 100
43 26.6 21.9 32.9
58 70.5 50.8 76.2

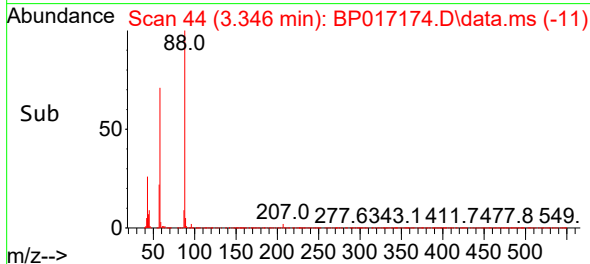

#5
Pyridine
Concen: 20.054 ng/uL
RT: 3.764 min Scan# 115
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25

Tgt Ion: 79 Resp: 321672
Ion Ratio Lower Upper
79 100
52 66.4 54.5 81.7
51 33.3 27.0 40.6


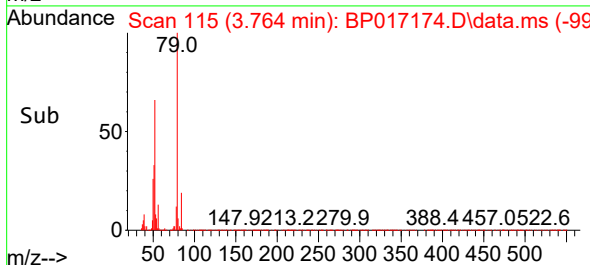
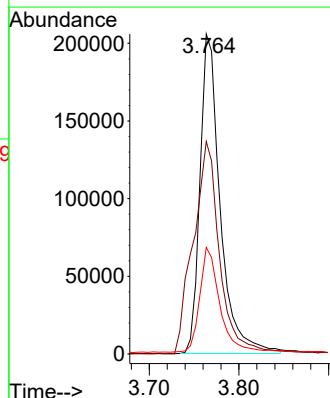
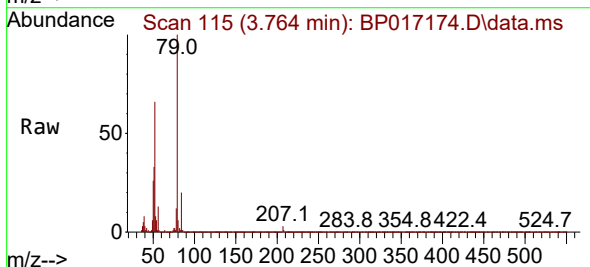




#6
Benzaldehyde
Concen: 22.538 ng/ul
RT: 7.110 min Scan# 684
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25




Instrument :
BNA_P
ClientSampleId :
SSTD020734


Tgt Ion: 77 Resp: 232100
Ion Ratio Lower Upper
77 100
105 93.9 75.3 112.9
106 90.8 74.6 111.8



#8
Phenol
Concen: 18.947 ng/ul
RT: 7.128 min Scan# 687
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25

Tgt Ion: 94 Resp: 369643
Ion Ratio Lower Upper
94 100
65 28.4 22.7 34.1
66 36.6 29.6 44.4









#10
Bis(2-Chloroethyl)ether
Concen: 19.615 ng/ul
RT: 7.387 min Scan# 731
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25




Instrument :
BNA_P
ClientSampleId :
SSTD020734


Tgt Ion: 93 Resp: 305211
Ion Ratio Lower Upper
93 100
63 73.2 59.5 89.3
95 32.0 25.8 38.6



#12
2-Chlorophenol
Concen: 19.640 ng/ul
RT: 7.505 min Scan# 751
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25

Tgt Ion:128 Resp: 294176
Ion Ratio Lower Upper
128 100
64 47.1 36.8 55.2
130 32.8 26.3 39.5









#13
2-Methylphenol
Concen: 18.363 ng/ul
RT: 8.393 min Scan# 902
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25




Instrument :
BNA_P
ClientSampleId :
SSTD020734


Tgt Ion:108 Resp: 267074
Ion Ratio Lower Upper
108 100
107 90.3 72.2 108.4

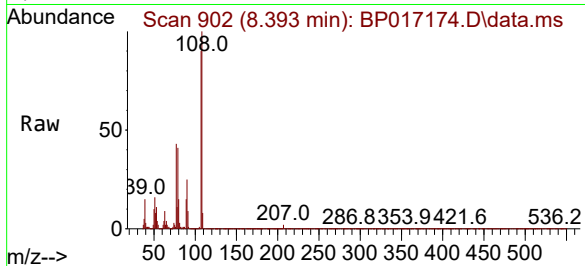

#14
2,2'-oxybis(1-Chloropropane)
Concen: 11.972 ng/ul
RT: 8.463 min Scan# 914
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25

Tgt Ion: 45 Resp: 252454
Ion Ratio Lower Upper
45 100
77 14.9 12.5 18.7
79 10.7 8.8 13.2




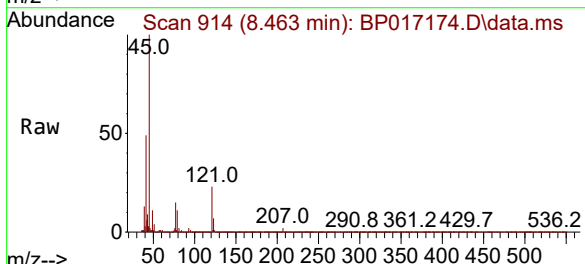




#16
Acetophenone
Concen: 18.726 ng/ul
RT: 8.804 min Scan# 91
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25




Instrument :
BNA_P
ClientSampleId :
SSTD020734


Tgt Ion:105 Resp: 449318
Ion Ratio Lower Upper
105 100
77 78.1 63.0 94.4
51 25.6 20.5 30.7



#17
N-Nitroso-di-n-propylamine
Concen: 18.281 ng/ul
RT: 8.769 min Scan# 966
Delta R.T. -0.012 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25

Tgt Ion: 70 Resp: 225412
Ion Ratio Lower Upper
70 100
42 57.9 43.9 65.9
101 9.5 7.0 10.4
130 20.9 15.8 23.6



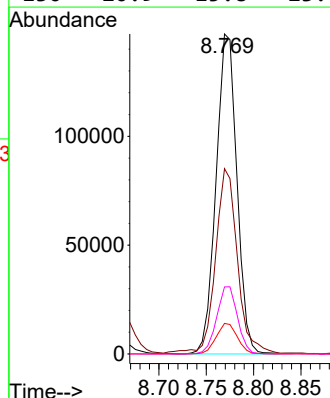





#18
4-Methylphenol
Concen: 18.128 ng/ul
RT: 8.728 min Scan# 91
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25




Instrument :
BNA_P
ClientSampleId :
SSTD020734


Tgt Ion:108 Resp: 291690
Ion Ratio Lower Upper
108 100
107 111.4 91.4 137.0



#19
Hexachloroethane
Concen: 20.002 ng/ul
RT: 9.016 min Scan# 1008
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25

Tgt Ion:117 Resp: 123215
Ion Ratio Lower Upper
117 100
201 103.5 79.9 119.9
199 65.6 49.4 74.2



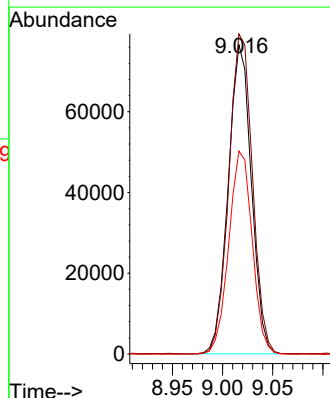





#22
Nitrobenzene
Concen: 20.753 ng/ul
RT: 9.193 min Scan# 1038
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25




Instrument :
BNA_P
ClientSampleId :
SSTD020734


Tgt Ion: 77 Resp: 345359
Ion Ratio Lower Upper
77 100
123 42.6 34.6 51.8
65 13.0 10.6 16.0



#23
Isophorone
Concen: 19.277 ng/ul
RT: 9.704 min Scan# 1125
Delta R.T. -0.012 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25

Tgt Ion: 82 Resp: 601168
Ion Ratio Lower Upper
82 100
95 7.0 5.6 8.4
138 16.9 14.0 21.0









#25
2-Nitrophenol
Concen: 21.059 ng/ul
RT: 9.899 min Scan# 1158
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25




Instrument :
BNA_P
ClientSampleId :
SSTD020734


Tgt Ion:139 Resp: 159676
Ion Ratio Lower Upper
139 100
65 51.5 41.9 62.9
109 31.4 23.5 35.3



#26
2,4-Dimethylphenol
Concen: 19.680 ng/ul
RT: 9.934 min Scan# 1164
Delta R.T. -0.012 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25

Tgt Ion:107 Resp: 304115
Ion Ratio Lower Upper
107 100
121 49.1 41.7 62.5
122 84.5 70.4 105.6









#27
 Bis(2-Chloroethoxy)methane
 Concen: 19.991 ng/ul
 RT: 10.193 min Scan# 1208
 Delta R.T. -0.012 min
 Lab File: BP017174.D
 Acq: 14 Sep 2023 13:25




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020734


Tgt Ion: 93 Resp: 390736
 Ion Ratio Lower Upper
 93 100
 95 32.5 26.2 39.4
 123 10.8 9.3 13.9

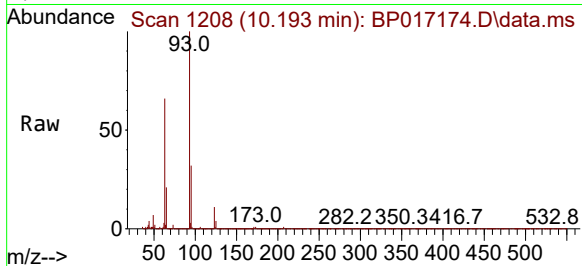

#29
 2,4-Dichlorophenol
 Concen: 20.448 ng/ul
 RT: 10.416 min Scan# 1246
 Delta R.T. -0.006 min
 Lab File: BP017174.D
 Acq: 14 Sep 2023 13:25

Tgt Ion: 162 Resp: 273083
 Ion Ratio Lower Upper
 162 100
 164 65.6 53.2 79.8
 98 35.1 30.0 45.0




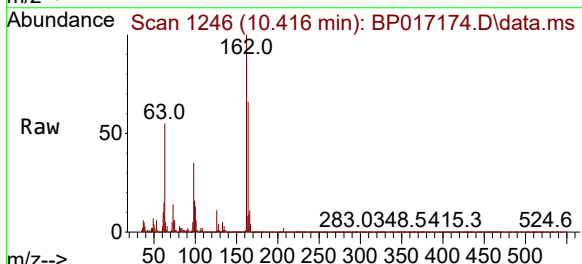




#30
Naphthalene
Concen: 20.305 ng/ul
RT: 10.828 min Scan# 1316
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25




Instrument :
BNA_P
ClientSampleId :
SSTD020734


Tgt Ion:128 Resp: 937708
Ion Ratio Lower Upper
128 100
129 10.8 8.6 13.0
127 13.1 10.4 15.6



#32
4-Chloroaniline
Concen: 19.194 ng/ul
RT: 10.963 min Scan# 1339
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25

Tgt Ion:127 Resp: 372481
Ion Ratio Lower Upper
127 100
129 32.5 24.8 37.2

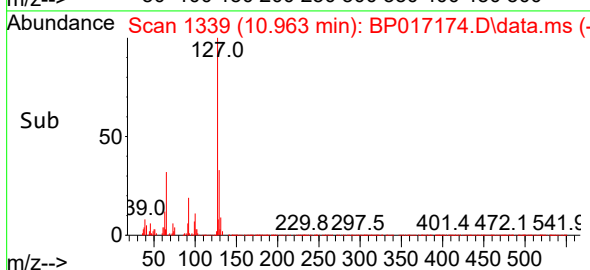



#33

Hexachlorobutadiene

Concen: 21.471 ng/ul

RT: 11.057 min Scan# 1355

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25

Instrument :

BNA_P

ClientSampleId :

SSTD020734





Tgt Ion:225 Resp: 194714

Ion Ratio Lower Upper

225 100

223 61.9 49.0 73.4

227 64.0 50.2 75.4



#34

Caprolactam

Concen: 16.367 ng/ul

RT: 11.787 min Scan# 1479

Delta R.T. -0.012 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25




Tgt Ion:113 Resp: 68710


Ion Ratio Lower Upper

113 100

55 164.9 130.7 196.1

56 126.2 96.8 145.2









#35
 4-Chloro-3-methylphenol
 Concen: 18.552 ng/ul
 RT: 12.063 min Scan# 1526
 Delta R.T. -0.006 min
 Lab File: BP017174.D
 Acq: 14 Sep 2023 13:25




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020734


Tgt Ion:107 Resp: 268073
 Ion Ratio Lower Upper
 107 100
 144 26.2 20.6 31.0
 142 77.9 63.4 95.0



#36
 2-Methylnaphthalene
 Concen: 19.851 ng/ul
 RT: 12.434 min Scan# 1589
 Delta R.T. -0.006 min
 Lab File: BP017174.D
 Acq: 14 Sep 2023 13:25

Tgt Ion:142 Resp: 618583
 Ion Ratio Lower Upper
 142 100
 141 89.9 70.1 105.1

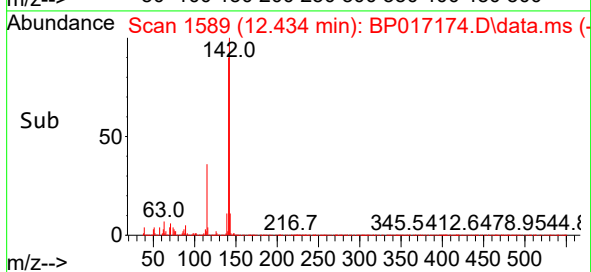



#37

1-Methylnaphthalene

Concen: 19.627 ng/ul

RT: 12.651 min Scan# 1626

Delta R.T. -0.012 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25

Instrument :

BNA_P

ClientSampleId :

SSTD020734





Tgt Ion:142 Resp: 619076

Ion Ratio Lower Upper

142 100

141 91.4 74.1 111.1

116 3.9 3.1 4.7



#39

1,2,4,5-Tetrachlorobenzene

Concen: 22.241 ng/ul

RT: 12.781 min Scan# 1648

Delta R.T. -0.012 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25

Tgt Ion:216 Resp: 351370




Ion Ratio Lower Upper


216 100

214 79.2 62.1 93.1

179 21.1 15.6 23.4

108 16.8 12.8 19.2

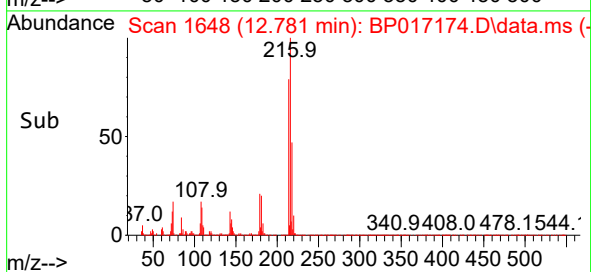



#40

Hexachlorocyclopentadiene

Concen: 21.728 ng/ul

RT: 12.734 min Scan# 1640

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25

Instrument :

BNA_P

ClientSampleId :

SSTD020734





Tgt Ion:237 Resp: 213880

Ion Ratio Lower Upper

237 100

235 61.2 50.4 75.6

272 13.0 10.2 15.4

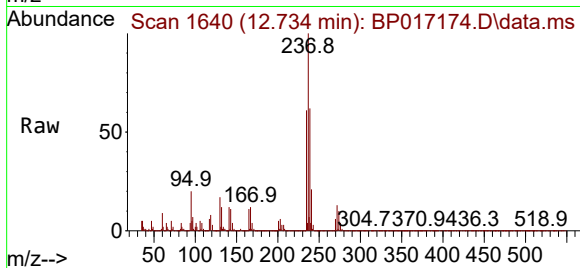

#41

2,4,6-Trichlorophenol

Concen: 21.126 ng/ul

RT: 13.040 min Scan# 1692

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25




Tgt Ion:196 Resp: 212022


Ion Ratio Lower Upper

196 100

198 94.2 76.0 114.0

200 32.4 25.0 37.4

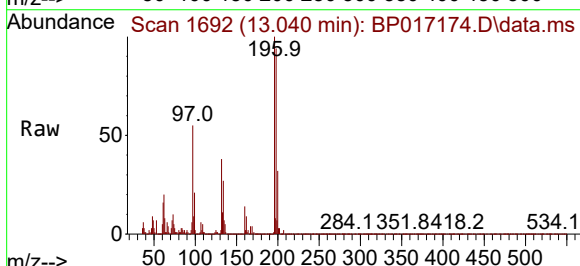



#42

2,4,5-Trichlorophenol

Concen: 20.924 ng/ul

RT: 13.110 min Scan# 1704

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25

Instrument :

BNA_P

ClientSampleId :

SSTD020734





Tgt Ion:196 Resp: 223261

Ion Ratio Lower Upper

196 100

198 96.4 76.9 115.3

200 32.7 25.0 37.6

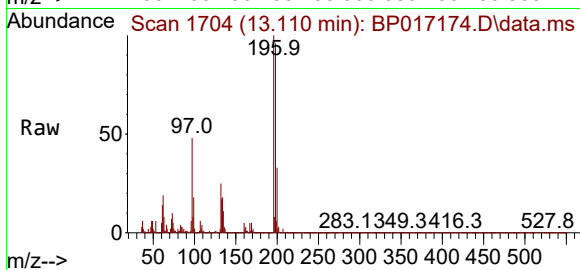

#43

1,1'-Biphenyl

Concen: 21.039 ng/ul

RT: 13.445 min Scan# 1761

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25




Tgt Ion:154 Resp: 800251


Ion Ratio Lower Upper

154 100

153 40.0 31.8 47.8

76 12.7 10.8 16.2

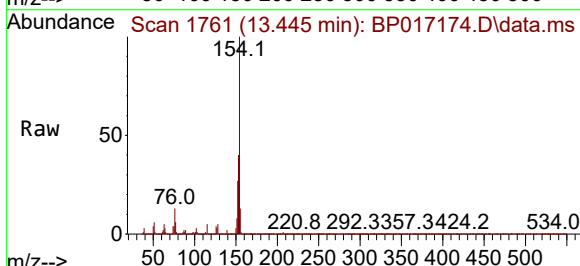



#44

2-Chloronaphthalene

Concen: 21.300 ng/ul

RT: 13.492 min Scan# 1769

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25

Instrument :

BNA_P

ClientSampleId :

SSTD020734





Tgt Ion:162 Resp: 643381

Ion Ratio Lower Upper

162 100

164 31.6 26.6 39.8

127 37.8 31.0 46.4



#45

2-Nitroaniline

Concen: 20.043 ng/ul

RT: 13.728 min Scan# 1809

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25




Tgt Ion: 65 Resp: 163987


Ion Ratio Lower Upper

65 100

92 69.8 55.6 83.4

138 103.5 82.2 123.2









#47
Dimethylphthalate
Concen: 20.087 ng/ul
RT: 14.075 min Scan# 1868
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25




Instrument :
BNA_P
ClientSampleId :
SSTD020734


Tgt Ion:163 Resp: 769702
Ion Ratio Lower Upper
163 100
194 4.1 3.3 4.9
164 9.8 7.9 11.9

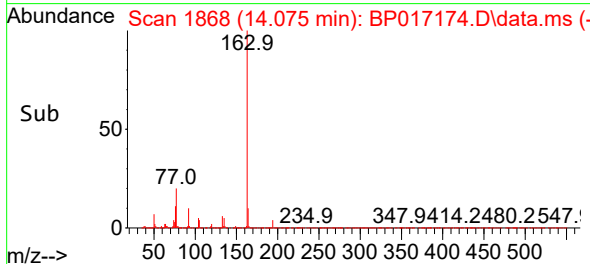

#48
2,6-Dinitrotoluene
Concen: 19.770 ng/ul
RT: 14.216 min Scan# 1892
Delta R.T. -0.012 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25

Tgt Ion:165 Resp: 138496
Ion Ratio Lower Upper
165 100
89 63.5 47.8 71.8
121 22.7 17.4 26.2

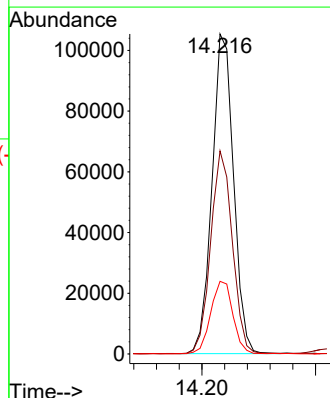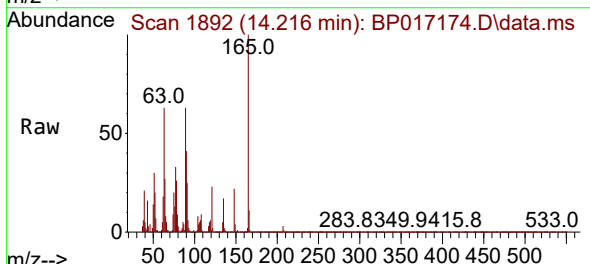



#50

Acenaphthylene

Concen: 20.652 ng/ul

RT: 14.339 min Scan# 1913

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25

Instrument :

BNA_P

ClientSampleId :

SSTD020734





Tgt Ion:152 Resp: 1021867

Ion Ratio Lower Upper

152 100

151 20.0 15.8 23.8

153 12.8 10.6 15.8



#51

3-Nitroaniline

Concen: 18.728 ng/ul

RT: 14.557 min Scan# 1950

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25




Tgt Ion:138 Resp: 140352


Ion Ratio Lower Upper

138 100

108 11.1 8.5 12.7

92 115.0 94.2 141.4









#52
Acenaphthene
Concen: 20.352 ng/ul
RT: 14.675 min Scan# 1970
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25




Instrument :
BNA_P
ClientSampleId :
SSTD020734


Tgt Ion:153 Resp: 666395
Ion Ratio Lower Upper
153 100
152 48.9 38.6 57.8
154 87.4 70.4 105.6

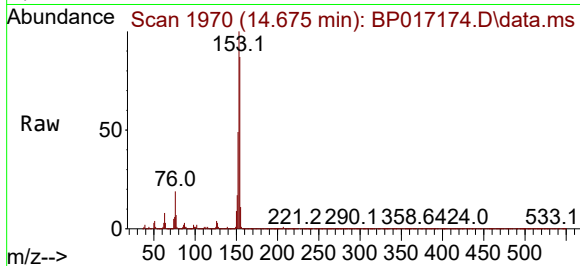

#53
2,4-Dinitrophenol
Concen: 15.724 ng/ul
RT: 14.757 min Scan# 1984
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25

Tgt Ion:184 Resp: 77155
Ion Ratio Lower Upper
184 100
63 68.7 55.2 82.8
154 66.1 53.0 79.4




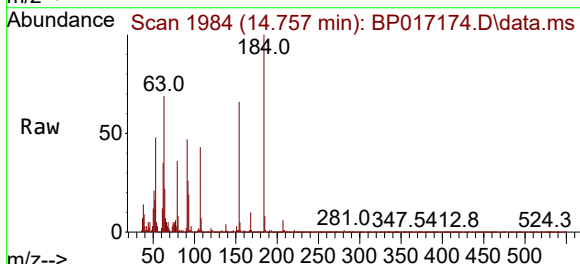




#55
4-Nitrophenol
Concen: 17.663 ng/ul
RT: 14.845 min Scan# 1999
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25




Instrument :
BNA_P
ClientSampleId :
SSTD020734


Tgt Ion:109 Resp: 103134
Ion Ratio Lower Upper
109 100
139 125.3 101.1 151.7
65 128.6 105.0 157.4

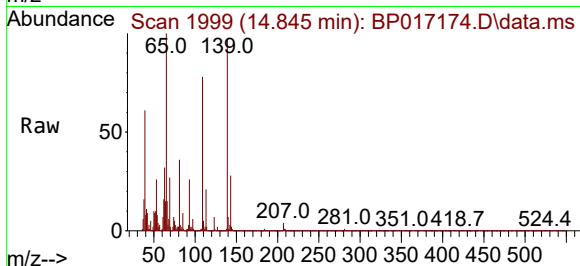

#56
Dibenzofuran
Concen: 20.423 ng/ul
RT: 15.010 min Scan# 2027
Delta R.T. -0.012 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25

Tgt Ion:168 Resp: 924078
Ion Ratio Lower Upper
168 100
139 37.7 29.9 44.9

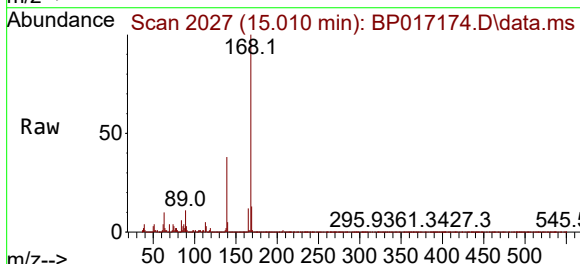



#57

2,4-Dinitrotoluene

Concen: 19.361 ng/ul

RT: 14.998 min Scan# 201963

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25

Instrument :

BNA_P

ClientSampleId :

SSTD020734





Tgt Ion:165 Resp: 201963

Ion Ratio Lower Upper

165 100

63 56.8 42.3 63.5

182 2.1 2.2 3.4#



#58

2,3,4,6-Tetrachlorophenol

Concen: 20.229 ng/ul

RT: 15.228 min Scan# 2064

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25

Tgt Ion:232 Resp: 189356




Ion Ratio Lower Upper


232 100

131 44.9 37.0 55.6

130 2.4 1.8 2.8

166 30.2 24.3 36.5


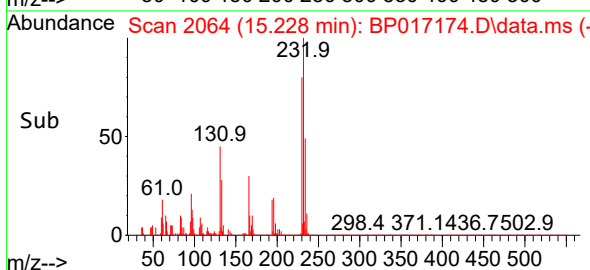






#59
Diethylphthalate
Concen: 19.746 ng/ul
RT: 15.428 min Scan# 2098
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25




Instrument :
BNA_P
ClientSampleId :
SSTD020734


Tgt Ion:149 Resp: 747048
Ion Ratio Lower Upper
149 100
177 22.2 17.5 26.3
150 12.4 10.0 15.0



#61
Fluorene
Concen: 20.165 ng/ul
RT: 15.663 min Scan# 2138
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25

Tgt Ion:166 Resp: 754347
Ion Ratio Lower Upper
166 100
165 98.7 78.2 117.2
167 13.6 11.0 16.4









#62
4-Chlorophenyl-phenylether
Concen: 20.999 ng/ul
RT: 15.657 min Scan# 2137
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25




Instrument :
BNA_P
ClientSampleId :
SSTD020734


Tgt Ion:204 Resp: 399390
Ion Ratio Lower Upper
204 100
206 32.2 27.3 40.9
141 54.4 45.0 67.6

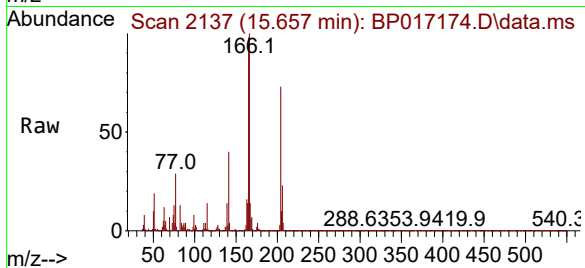

#63
4-Nitroaniline
Concen: 19.448 ng/ul
RT: 15.728 min Scan# 2149
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25

Tgt Ion:138 Resp: 135497
Ion Ratio Lower Upper
138 100
92 52.9 43.3 64.9
108 95.9 75.3 112.9


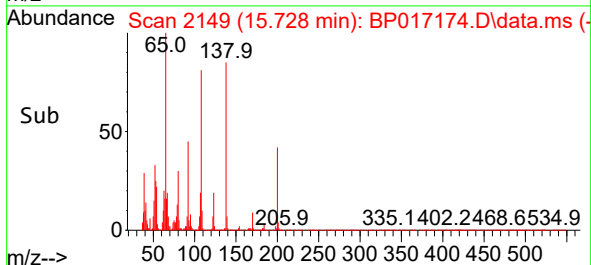

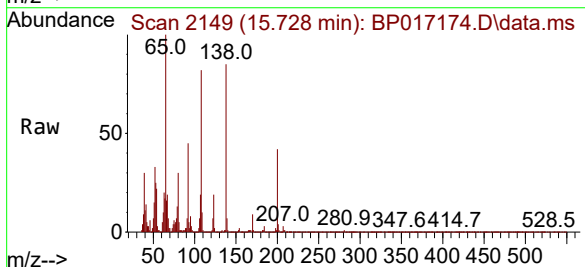




#66
4,6-Dinitro-2-methylphenol
Concen: 18.791 ng/ul
RT: 15.751 min Scan# 2153
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25




Instrument :
BNA_P
ClientSampleId :
SSTD020734


Tgt Ion:198 Resp: 126306
Ion Ratio Lower Upper
198 100
182 5.2 4.2 6.2
77 26.3 22.5 33.7

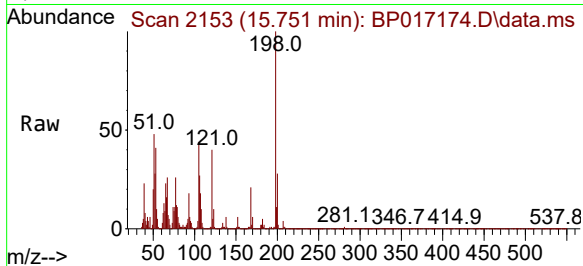

#67
N-Nitrosodiphenylamine
Concen: 20.859 ng/ul
RT: 15.881 min Scan# 2175
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25

Tgt Ion:169 Resp: 608005
Ion Ratio Lower Upper
169 100
168 68.2 52.7 79.1
167 38.0 29.0 43.4



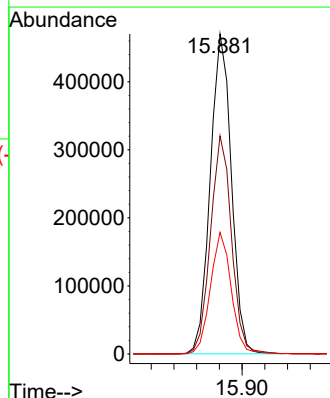
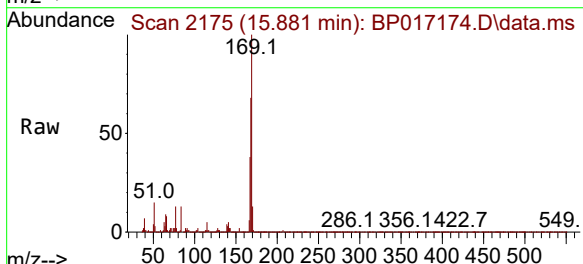




#68
4-Bromophenyl-phenylether
Concen: 21.424 ng/ul
RT: 16.557 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25




Instrument :
BNA_P
ClientSampleId :
SSTD020734


Tgt Ion:248 Resp: 228924
Ion Ratio Lower Upper
248 100
250 97.2 78.6 118.0
141 72.8 60.4 90.6

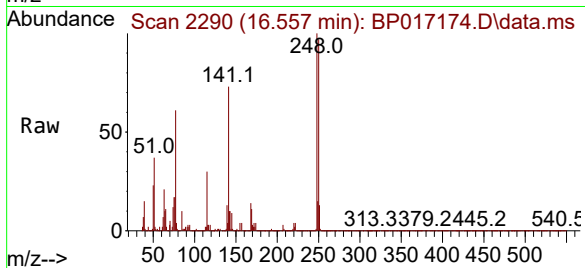

#69
Hexachlorobenzene
Concen: 20.990 ng/ul
RT: 16.639 min Scan# 2304
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25

Tgt Ion:284 Resp: 265478
Ion Ratio Lower Upper
284 100
142 36.1 28.6 42.8
249 31.8 25.0 37.6

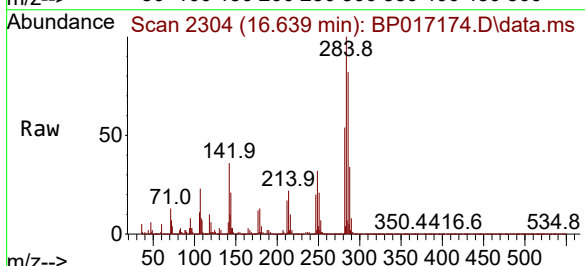



#70

Atrazine

Concen: 21.106 ng/ul

RT: 16.839 min Scan# 21

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25

Instrument :

BNA_P

ClientSampleId :

SSTD020734





Tgt Ion:200 Resp: 222685

Ion Ratio Lower Upper

200 100

173 24.8 20.7 31.1

215 48.2 38.8 58.2

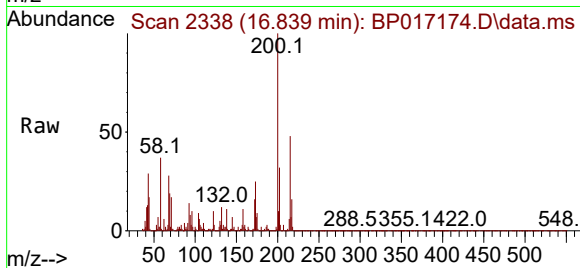

#71

Pentachlorophenol

Concen: 18.652 ng/ul

RT: 17.004 min Scan# 2366

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25




Tgt Ion:266 Resp: 153314


Ion Ratio Lower Upper

266 100

264 62.7 50.7 76.1

268 62.4 51.1 76.7

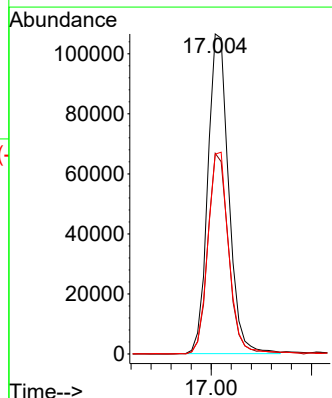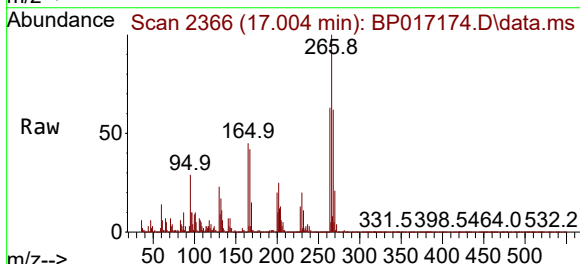



#72

Phenanthrene

Concen: 20.575 ng/ul

RT: 17.428 min Scan# 2438

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25

Instrument :

BNA_P

ClientSampleId :

SSTD020734





Tgt Ion:178 Resp: 1159057

Ion Ratio Lower Upper

178 100

179 15.3 12.2 18.2

176 19.0 15.6 23.4

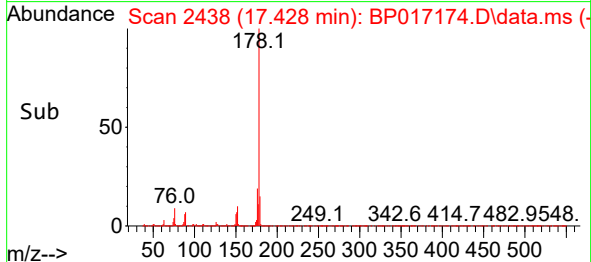

#74

Anthracene

Concen: 20.493 ng/ul

RT: 17.516 min Scan# 2453

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25




Tgt Ion:178 Resp: 1169288


Ion Ratio Lower Upper

178 100

179 15.4 12.4 18.6

176 19.5 14.9 22.3


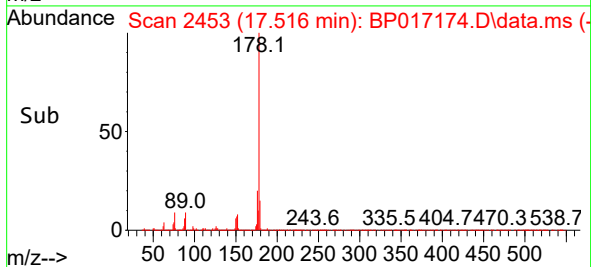

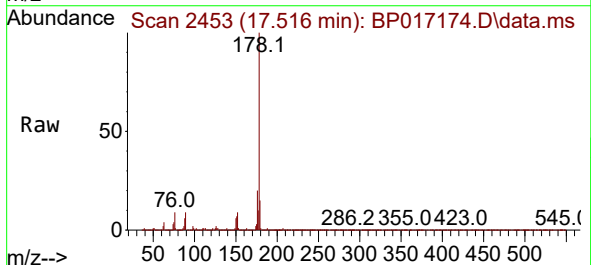




#75
1,2,3,4-Tetrachlorobenzene
Concen: 23.550 ng/uL
RT: 13.398 min Scan# 1753
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25




Instrument :
BNA_P
ClientSampleId :
SSTD020734


Tgt Ion:216 Resp: 365010
Ion Ratio Lower Upper
216 100
214 76.4 61.3 91.9
218 47.1 38.3 57.5



#76
Pentachlorobenzene
Concen: 22.538 ng/uL
RT: 14.904 min Scan# 2009
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25

Tgt Ion:250 Resp: 316975
Ion Ratio Lower Upper
250 100
248 60.9 51.1 76.7
252 63.6 50.7 76.1





#77

Carbazole

Concen: 20.202 ng/ul

RT: 17.804 min Scan# 2502

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25

Instrument :

BNA_P

ClientSampleId :

SSTD020734





Tgt Ion:167 Resp: 1012137

Ion Ratio Lower Upper

167 100

166 21.2 17.0 25.6

139 13.2 10.4 15.6



#78

Di-n-butylphthalate

Concen: 21.022 ng/ul

RT: 18.316 min Scan# 2589

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25




Tgt Ion:149 Resp: 1200134


Ion Ratio Lower Upper

149 100

150 9.1 7.2 10.8

104 5.4 4.2 6.4

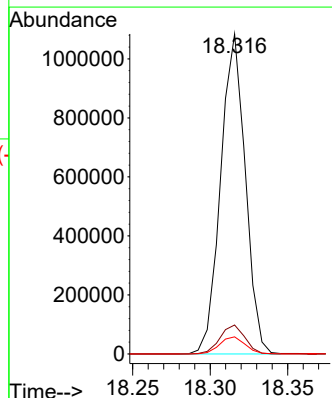



#80

Fluoranthene

Concen: 20.534 ng/ul

RT: 19.392 min Scan# 2772

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25

Instrument :

BNA_P

ClientSampleId :

SSTD020734





Tgt Ion:202 Resp: 1321184

Ion Ratio Lower Upper

202 100

101 10.7 8.3 12.5

100 8.3 6.4 9.6



#82

Pyrene

Concen: 20.552 ng/ul

RT: 19.751 min Scan# 2833

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25




Tgt Ion:202 Resp: 1397203


Ion Ratio Lower Upper

202 100

101 12.1 9.7 14.5

100 10.3 7.8 11.8





#83

Butylbenzylphthalate

Concen: 20.997 ng/ul

RT: 20.610 min Scan# 2979

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25

Instrument :

BNA_P

ClientSampleId :

SSTD020734





Tgt Ion:149 Resp: 509114

Ion Ratio Lower Upper

149 100

91 75.5 57.4 86.0

206 20.3 16.7 25.1

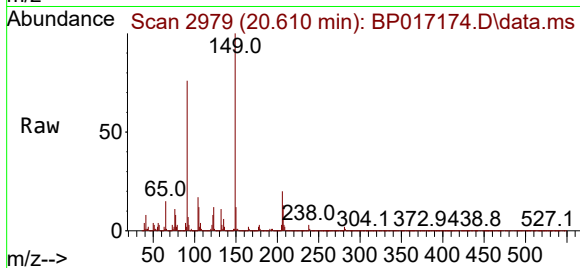

#84

3,3'-Dichlorobenzidine

Concen: 19.911 ng/ul

RT: 21.410 min Scan# 3115

Delta R.T. 0.000 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25




Tgt Ion:252 Resp: 428464


Ion Ratio Lower Upper

252 100

254 67.1 51.4 77.2

126 11.3 9.4 14.2

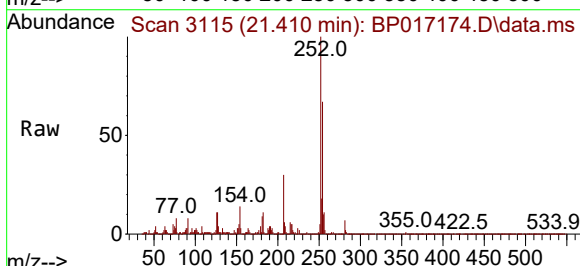



#85

Benzo(a)anthracene

Concen: 20.746 ng/ul

RT: 21.469 min Scan# 3125

Delta R.T. 0.000 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25

Instrument :

BNA_P

ClientSampleId :

SSTD020734





Tgt Ion:228 Resp: 1425742

Ion Ratio Lower Upper

228 100

229 19.4 16.1 24.1

226 27.2 22.2 33.4

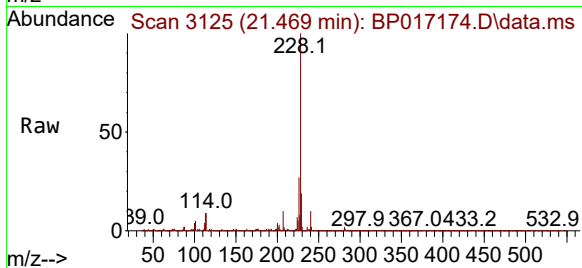

#86

Bis(2-ethylhexyl)phthalate

Concen: 21.812 ng/ul

RT: 21.345 min Scan# 3104

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25




Tgt Ion:149 Resp: 742410


Ion Ratio Lower Upper

149 100

167 27.6 21.3 31.9

279 3.9 3.4 5.2

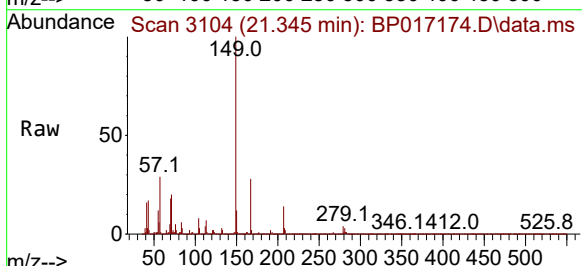



#87

Chrysene

Concen: 20.646 ng/ul

RT: 21.521 min Scan# 3134

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25

Instrument :

BNA_P

ClientSampleId :

SSTD020734





Tgt Ion:228 Resp: 1319864

Ion Ratio Lower Upper

228 100

226 30.7 23.9 35.9

229 19.8 15.3 22.9



#89

Di-n-octyl phthalate

Concen: 19.553 ng/ul




RT: 22.310 min Scan# 3268


Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25

Tgt Ion:149 Resp: 1271664





#90

Benzo(b)fluoranthene

Concen: 20.163 ng/ul

RT: 23.221 min Scan# 3423

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25

Instrument :

BNA_P

ClientSampleId :

SSTD020734





Tgt Ion:252 Resp: 1394017

Ion Ratio Lower Upper

252 100

253 22.1 18.2 27.2

125 9.7 7.5 11.3



#91

Benzo(k)fluoranthene

Concen: 20.363 ng/ul

RT: 23.274 min Scan# 3432

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25




Tgt Ion:252 Resp: 1399523


Ion Ratio Lower Upper

252 100

253 22.5 17.8 26.6

125 9.7 7.4 11.2


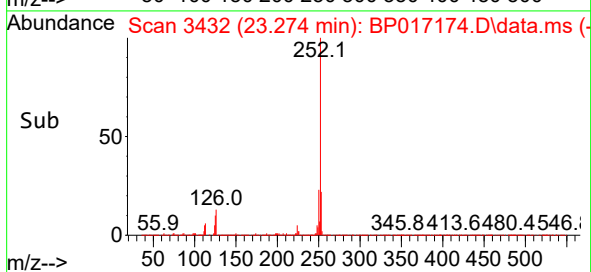






#93
Benzo(a)pyrene
Concen: 20.616 ng/ul
RT: 23.898 min Scan# 31
Delta R.T. -0.006 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25




Instrument :
BNA_P
ClientSampleId :
SSTD020734


Tgt Ion:252 Resp: 1322316
Ion Ratio Lower Upper
252 100
253 22.0 17.4 26.2
125 10.5 8.1 12.1

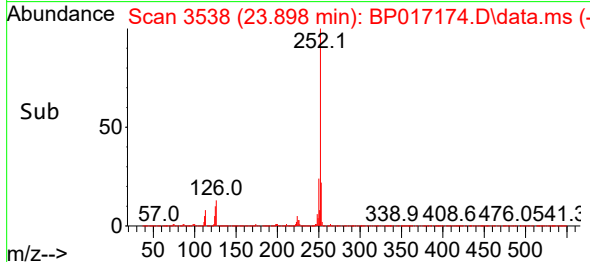

#94
Indeno(1,2,3-cd)pyrene
Concen: 23.142 ng/ul
RT: 26.686 min Scan# 4012
Delta R.T. -0.012 min
Lab File: BP017174.D
Acq: 14 Sep 2023 13:25

Tgt Ion:276 Resp: 1643719
Ion Ratio Lower Upper
276 100
138 21.5 17.5 26.3
277 24.4 19.6 29.4

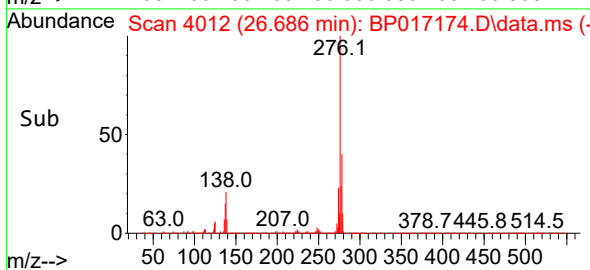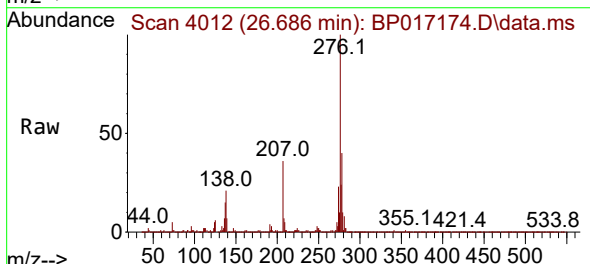



#95

Dibenzo(a,h)anthracene

Concen: 23.041 ng/ul

RT: 26.715 min Scan# 4016

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25

Instrument :

BNA_P

ClientSampleId :

SSTD020734





Tgt Ion:278 Resp: 1374735

Ion Ratio Lower Upper

278 100

139 14.7 11.9 17.9

279 24.3 19.0 28.6

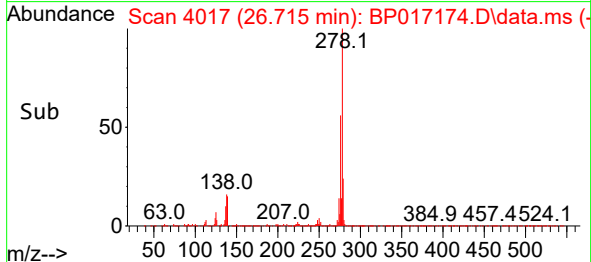

#96

Benzo(g,h,i)perylene

Concen: 23.635 ng/ul

RT: 27.527 min Scan# 4155

Delta R.T. -0.006 min

Lab File: BP017174.D

Acq: 14 Sep 2023 13:25

Tgt Ion:276 Resp: 1298067

Ion Ratio Lower Upper

276 100

138 20.2 16.2 24.4

277 24.6 19.6 29.4

