

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017180.D
 Acq On : 14 Sep 2023 16:56
 Operator : MA/JU
 Sample : 04324-07RE
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHF8

Quant Time: Sep 14 22:49:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 12 23:27:27 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	199441	20.000	ng/ul	0.00
20) Naphthalene-d8	10.775	136	791513	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.610	164	456701	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.381	188	971324	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	897248	20.000	ng/ul	0.00
88) Perylene-d12	24.004	264	1013915	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	22588	4.759	ng/uL	0.00
4) Pyridine-d5	3.752	84	96447	7.104	ng/ul	0.00
7) Phenol-d5	7.099	99	112340	6.927	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.293	67	331429	32.698	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132	324158	25.056	ng/ul	0.00
15) 4-Methylphenol-d8	8.658	113	202925	15.098	ng/ul	-0.01
21) Nitrobenzene-d5	9.146	128	190658	34.400	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.863	143	198468	33.542	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	340846	29.786	ng/ul	0.00
31) 4-Chloroaniline-d4	10.940	131	237916	13.794	ng/ul	0.00
46) Dimethylphthalate-d6	14.022	166	1135040	34.925	ng/ul	-0.01
49) Acenaphthylene-d8	14.310	160	1245465	33.773	ng/ul	0.00
54) 4-Nitrophenol-d4	14.834	143	25864	4.118	ng/ul	0.00
60) Fluorene-d10	15.604	176	982242	34.954	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.734	200	142877	26.328	ng/ul	-0.01
73) Anthracene-d10	17.481	188	1570298	38.050	ng/ul	0.00
81) Pyrene-d10	19.722	212	1878279	39.916	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.839	264	1923569	40.196	ng/ul	-0.01
Target Compounds						
34) Caprolactam	11.769	113	24384	6.697	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017180.D
Acq On : 14 Sep 2023 16:56
Operator : MA/JU
Sample : 04324-07RE
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHF8

Quant Time: Sep 14 22:49:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 12 23:27:27 2023
Response via : Initial Calibration

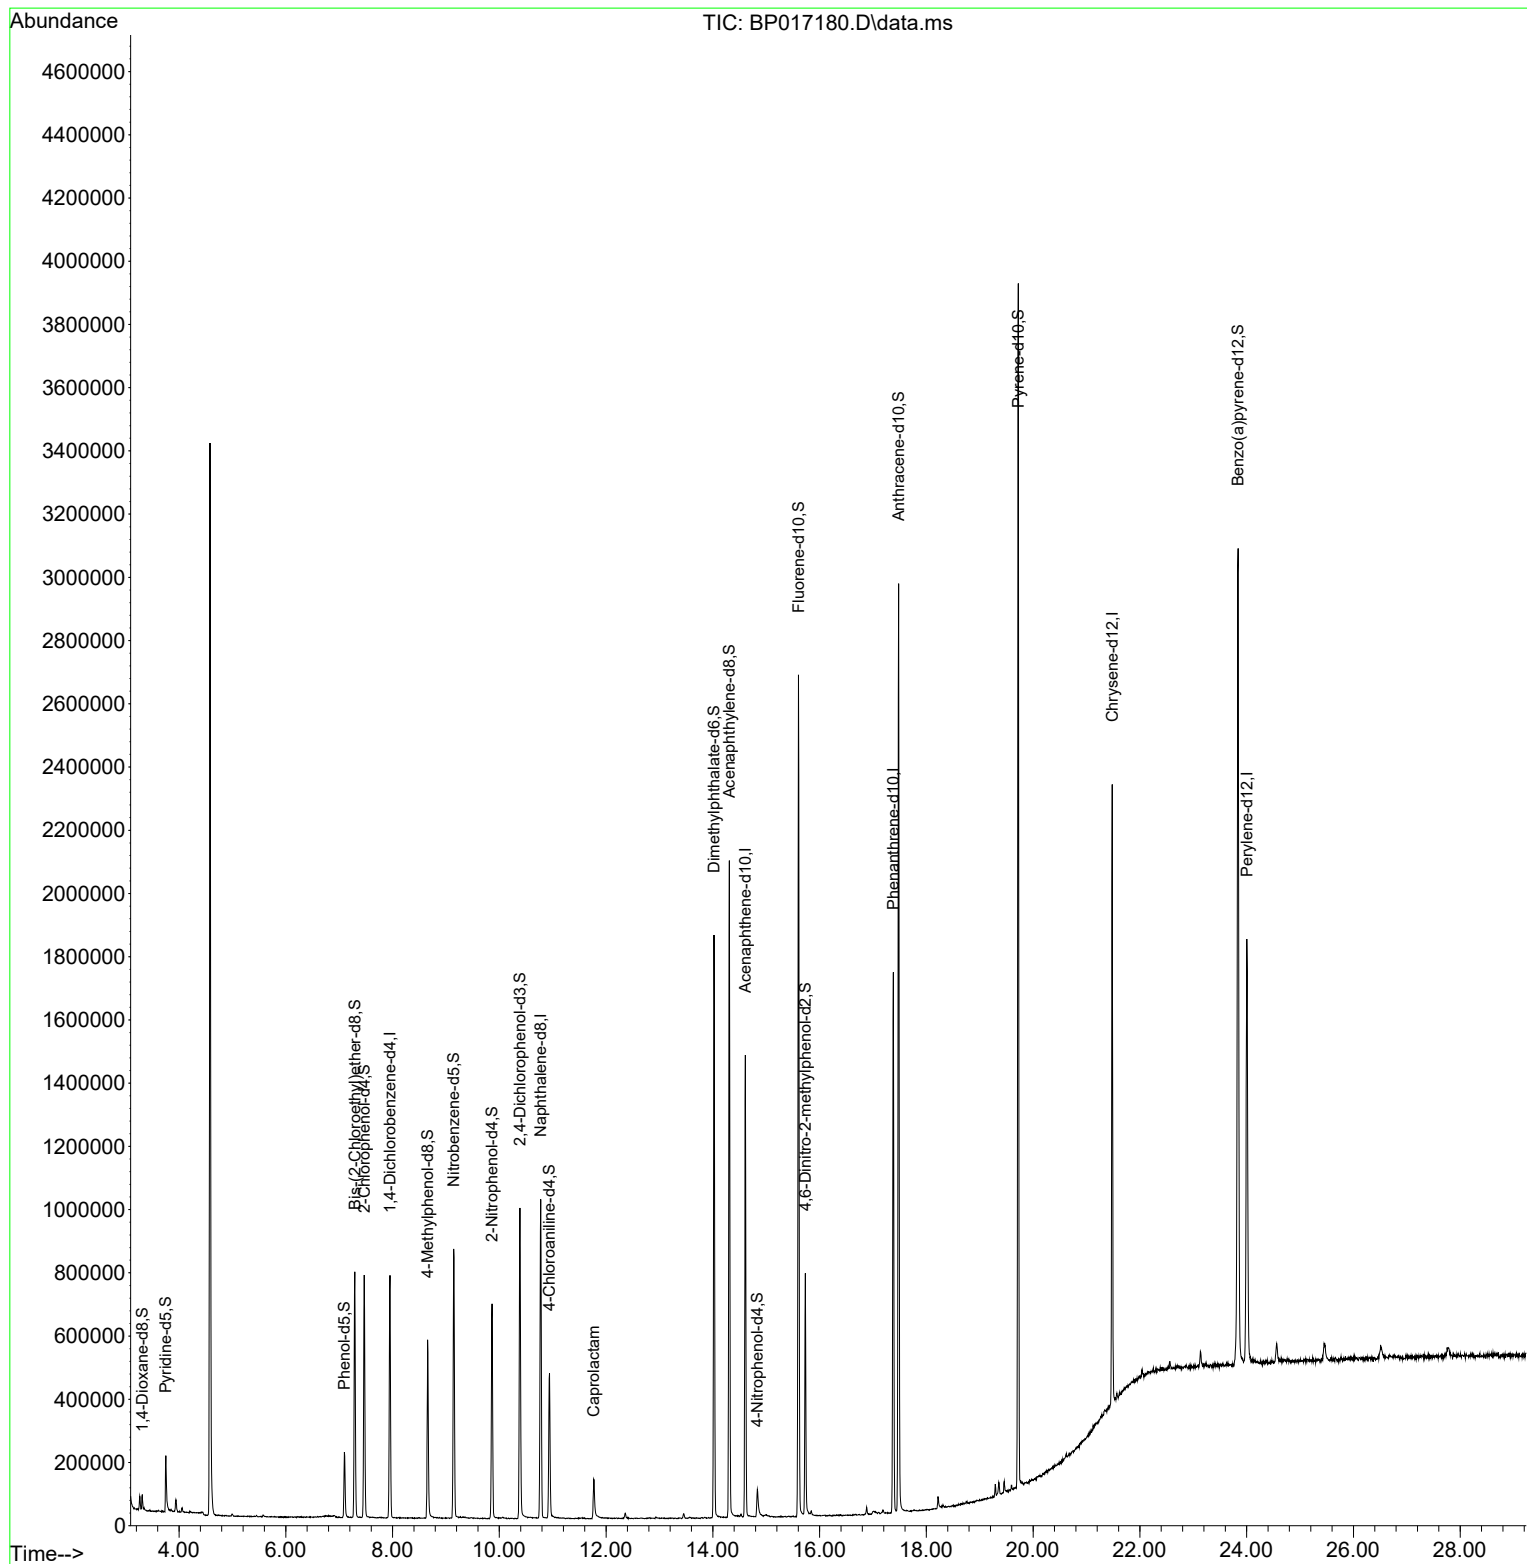

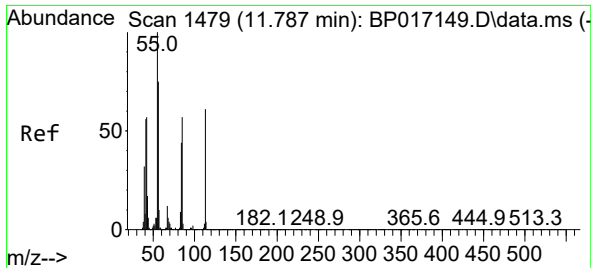

#34

Caprolactam

Concen: 6.697 ng/ul

RT: 11.769 min Scan# 14

Delta R.T. -0.029 min

Lab File: BP017180.D


Acq: 14 Sep 2023 16:56

Instrument :

BNA_P

ClientSampleId :

BBHF8

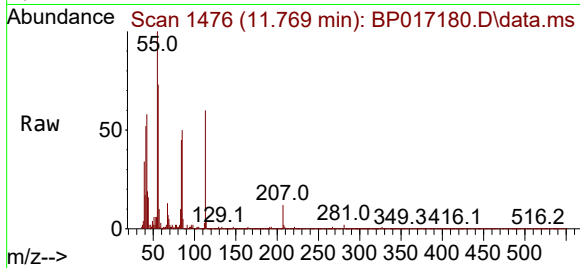

Tgt Ion:113 Resp: 24384

Ion Ratio Lower Upper

113 100

55 166.0 130.7 196.1

56 121.9 96.8 145.2

