

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017187.D
 Acq On : 14 Sep 2023 21:32
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020735

Quant Time: Sep 14 22:50:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 12 23:27:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	236745	20.000	ng/u1	0.00
20) Naphthalene-d8	10.775	136	970640	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.610	164	565858	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.381	188	1134829	20.000	ng/u1	0.00
79) Chrysene-d12	21.480	240	974012	20.000	ng/u1	0.00
88) Perylene-d12	24.004	264	1070799	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	46204	8.201	ng/uL	0.00
4) Pyridine-d5	3.746	84	336952	20.908	ng/u1	0.00
7) Phenol-d5	7.099	99	391502	20.337	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.293	67	256182	21.292	ng/u1	0.00
11) 2-Chlorophenol-d4	7.469	132	321564	20.939	ng/u1	0.00
15) 4-Methylphenol-d8	8.663	113	314201	19.694	ng/u1	0.00
21) Nitrobenzene-d5	9.146	128	152693	22.466	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.863	143	159114	21.929	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	307333	21.901	ng/u1	0.00
31) 4-Chloroaniline-d4	10.934	131	429949	20.328	ng/u1	-0.01
46) Dimethylphthalate-d6	14.022	166	860963	21.381	ng/u1	-0.01
49) Acenaphthylene-d8	14.310	160	1015784	22.232	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	133375	17.138	ng/u1	0.00
60) Fluorene-d10	15.604	176	743005	21.340	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.734	200	114321	18.031	ng/u1	-0.01
73) Anthracene-d10	17.481	188	1067651	22.143	ng/u1	0.00
81) Pyrene-d10	19.716	212	1177160	23.045	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.839	264	1105231	21.868	ng/u1	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.346	88	52528	8.671	ng/uL	95
5) Pyridine	3.764	79	351628	21.064	ng/u1	100
6) Benzaldehyde	7.105	77	264460	24.676	ng/u1	97
8) Phenol	7.128	94	415054	20.443	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.387	93	343633	21.221	ng/u1	98
12) 2-Chlorophenol	7.505	128	329761	21.155	ng/u1	99
13) 2-Methylphenol	8.393	108	302120	19.961	ng/u1	96
14) 2,2'-oxybis(1-Chloropr...	8.463	45	255184	11.628	ng/u1	99
16) Acetophenone	8.799	105	517928	20.741	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.769	70	264689	20.627	ng/u1	97
18) 4-Methylphenol	8.728	108	335012	20.006	ng/u1	95
19) Hexachloroethane	9.016	117	137065	21.380	ng/u1	96
22) Nitrobenzene	9.193	77	397713	22.470	ng/u1	98
23) Isophorone	9.705	82	698593	21.062	ng/u1	99
25) 2-Nitrophenol	9.893	139	179601	22.270	ng/u1	94
26) 2,4-Dimethylphenol	9.934	107	352402	21.441	ng/u1	97
27) Bis(2-Chloroethoxy)met...	10.193	93	449765	21.635	ng/u1	99
29) 2,4-Dichlorophenol	10.410	162	308541	21.721	ng/u1	98
30) Naphthalene	10.822	128	1065429	21.692	ng/u1	100
32) 4-Chloroaniline	10.963	127	430786	20.872	ng/u1	98
33) Hexachlorobutadiene	11.052	225	218647	22.669	ng/u1	99
34) Caprolactam	11.781	113	78567	17.596	ng/u1	93
35) 4-Chloro-3-methylphenol	12.063	107	310019	20.172	ng/u1	99
36) 2-Methylnaphthalene	12.428	142	707413	21.345	ng/u1	97


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017187.D
 Acq On : 14 Sep 2023 21:32
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020735

Quant Time: Sep 14 22:50:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 12 23:27:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.651	142	709900	21.161	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.781	216	404203	23.983	ng/ul	99
40) Hexachlorocyclopentadiene	12.728	237	210641	20.060	ng/ul	98
41) 2,4,6-Trichlorophenol	13.034	196	243361	22.730	ng/ul	99
42) 2,4,5-Trichlorophenol	13.104	196	258047	22.671	ng/ul	98
43) 1,1'-Biphenyl	13.440	154	916690	22.592	ng/ul	99
44) 2-Chloronaphthalene	13.487	162	732916	22.745	ng/ul	99
45) 2-Nitroaniline	13.728	65	193159	22.131	ng/ul	98
47) Dimethylphthalate	14.069	163	865926	21.183	ng/ul	99
48) 2,6-Dinitrotoluene	14.216	165	157236	21.040	ng/ul	98
50) Acenaphthylene	14.340	152	1163753	22.047	ng/ul	100
51) 3-Nitroaniline	14.557	138	157211	19.664	ng/ul	96
52) Acenaphthene	14.675	153	763578	21.861	ng/ul	100
53) 2,4-Dinitrophenol	14.757	184	56763	10.844	ng/ul	95
55) 4-Nitrophenol	14.845	109	113130	18.162	ng/ul	97
56) Dibenzofuran	15.010	168	1054537	21.847	ng/ul	100
57) 2,4-Dinitrotoluene	14.998	165	225282	20.244	ng/ul	92
58) 2,3,4,6-Tetrachlorophenol	15.228	232	212186	21.249	ng/ul	98
59) Diethylphthalate	15.428	149	832198	20.620	ng/ul	99
61) Fluorene	15.663	166	852848	21.371	ng/ul	98
62) 4-Chlorophenyl-phenyle...	15.651	204	448475	22.104	ng/ul	99
63) 4-Nitroaniline	15.722	138	143976	19.371	ng/ul	98
66) 4,6-Dinitro-2-methylph...	15.751	198	125928	18.507	ng/ul	97
67) N-Nitrosodiphenylamine	15.881	169	685228	23.222	ng/ul	99
68) 4-Bromophenyl-phenylether	16.557	248	258733	23.918	ng/ul	96
69) Hexachlorobenzene	16.634	284	298951	23.349	ng/ul	100
70) Atrazine	16.834	200	235043	22.005	ng/ul	99
71) Pentachlorophenol	17.004	266	164387	19.755	ng/ul	100
72) Phenanthrene	17.422	178	1253911	21.987	ng/ul	100
74) Anthracene	17.516	178	1294216	22.407	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.393	216	417415	26.603	ng/ul	99
76) Pentachlorobenzene	14.904	250	360381	25.312	ng/ul	99
77) Carbazole	17.798	167	1062061	20.940	ng/ul	99
78) Di-n-butylphthalate	18.310	149	1258500	21.775	ng/ul	99
80) Fluoranthene	19.386	202	1379068	23.098	ng/ul	99
82) Pyrene	19.745	202	1455483	23.071	ng/ul	98
83) Butylbenzylphthalate	20.610	149	494086	21.959	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.404	252	408910	20.477	ng/ul	99
85) Benzo(a)anthracene	21.463	228	1393212	21.846	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.345	149	701718	22.217	ng/ul	100
87) Chrysene	21.522	228	1317777	22.213	ng/ul	100
89) Di-n-octyl phthalate	22.304	149	1189088	20.027	ng/ul	100
90) Benzo(b)fluoranthene	23.221	252	1353743	21.448	ng/ul	98
91) Benzo(k)fluoranthene	23.269	252	1345551	21.444	ng/ul	100
93) Benzo(a)pyrene	23.892	252	1294005	22.098	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.680	276	1608012	24.798	ng/ul	99
95) Dibenzo(a,h)anthracene	26.698	278	1345224	24.696	ng/ul	99
96) Benzo(g,h,i)perylene	27.509	276	1270654	25.342	ng/ul	98





(#) = qualifier out of range (m) = manual integration (+) = signals summed

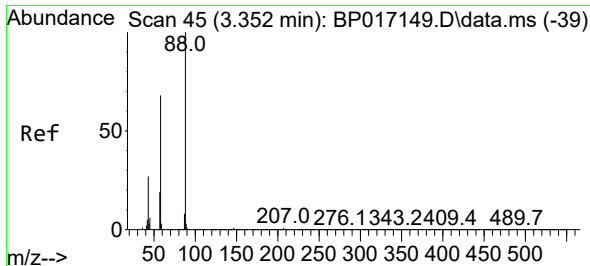

#2
1,4-Dioxane
Concen: 8.671 ng/uL
RT: 3.346 min Scan# 44
Delta R.T. -0.006 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32




Instrument :
BNA_P
ClientSampleId :
SSTD020735


Tgt Ion:	88	Resp:	52528
Ion	Ratio	Lower	Upper
88	100		
43	29.4	21.9	32.9
58	68.1	50.8	76.2

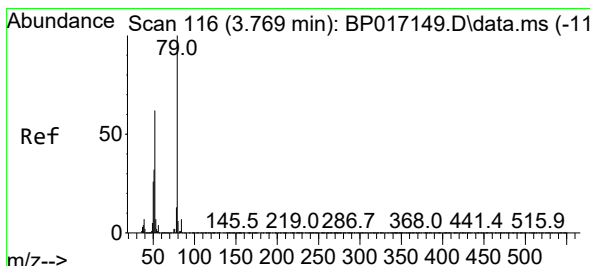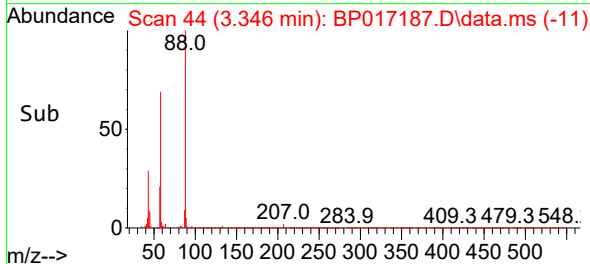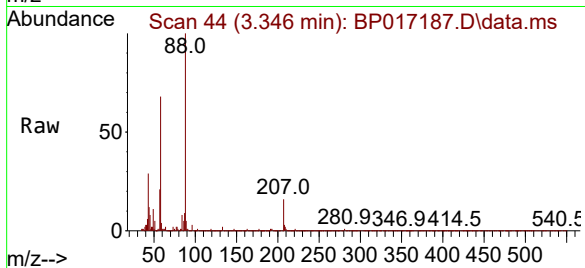

#5
Pyridine
Concen: 21.064 ng/uL
RT: 3.764 min Scan# 115
Delta R.T. -0.006 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32

Tgt Ion:	79	Resp:	351628
Ion	Ratio	Lower	Upper
79	100		
52	68.1	54.5	81.7
51	33.1	27.0	40.6


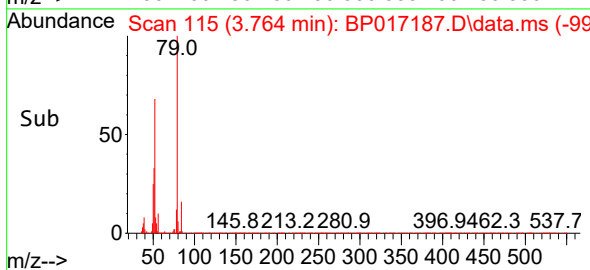

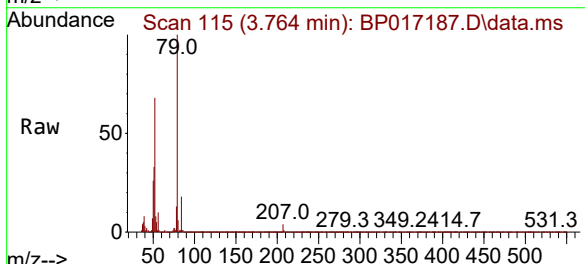




#6
Benzaldehyde
Concen: 24.676 ng/ul
RT: 7.105 min Scan# 684
Delta R.T. -0.012 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32




Instrument :
BNA_P
ClientSampleId :
SSTD020735


Tgt Ion: 77 Resp: 264460
Ion Ratio Lower Upper
77 100
105 93.3 75.3 112.9
106 89.0 74.6 111.8



#8
Phenol
Concen: 20.443 ng/ul
RT: 7.128 min Scan# 687
Delta R.T. -0.006 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32

Tgt Ion: 94 Resp: 415054
Ion Ratio Lower Upper
94 100
65 28.6 22.7 34.1
66 36.5 29.6 44.4









#10
Bis(2-Chloroethyl)ether
Concen: 21.221 ng/ul
RT: 7.387 min Scan# 731
Delta R.T. -0.006 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32




Instrument :
BNA_P
ClientSampleId :
SSTD020735


Tgt Ion: 93 Resp: 343633
Ion Ratio Lower Upper
93 100
63 75.7 59.5 89.3
95 33.6 25.8 38.6



#12
2-Chlorophenol
Concen: 21.155 ng/ul
RT: 7.505 min Scan# 751
Delta R.T. -0.006 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32

Tgt Ion:128 Resp: 329761
Ion Ratio Lower Upper
128 100
64 47.6 36.8 55.2
130 32.9 26.3 39.5





#13

2-Methylphenol

Concen: 19.961 ng/ul

RT: 8.393 min Scan# 902

Delta R.T. -0.006 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32

Instrument :

BNA_P

ClientSampleId :





SSTD020735

Tgt Ion:108 Resp: 302120

Ion Ratio Lower Upper

108 100

107 86.9 72.2 108.4

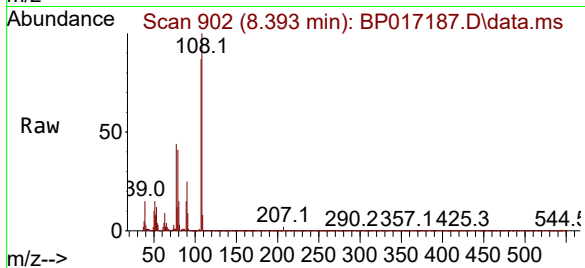

#14

2,2'-oxybis(1-Chloropropane)

Concen: 11.628 ng/ul

RT: 8.463 min Scan# 914

Delta R.T. -0.006 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32




Tgt Ion: 45 Resp: 255184


Ion Ratio Lower Upper

45 100

77 14.9 12.5 18.7

79 11.0 8.8 13.2


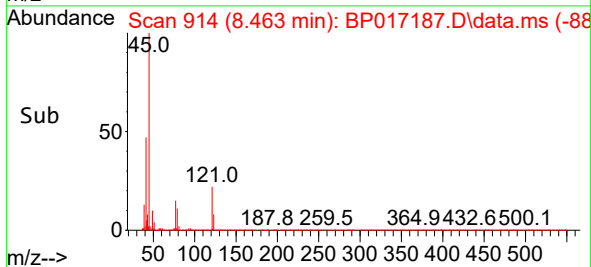

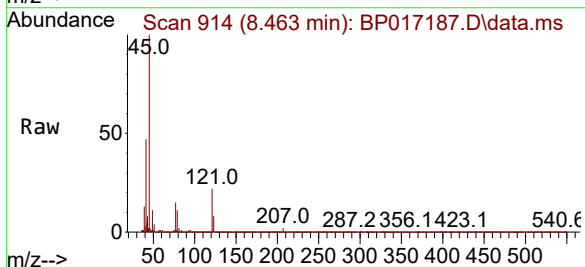




#16
Acetophenone
Concen: 20.741 ng/ul
RT: 8.799 min Scan# 91
Delta R.T. -0.012 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32




Instrument :
BNA_P
ClientSampleId :
SSTD020735


Tgt Ion:105 Resp: 517928
Ion Ratio Lower Upper
105 100
77 80.5 63.0 94.4
51 27.1 20.5 30.7



#17
N-Nitroso-di-n-propylamine
Concen: 20.627 ng/ul
RT: 8.769 min Scan# 966
Delta R.T. -0.012 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32

Tgt Ion: 70 Resp: 264689
Ion Ratio Lower Upper
70 100
42 57.6 43.9 65.9
101 9.6 7.0 10.4
130 20.1 15.8 23.6



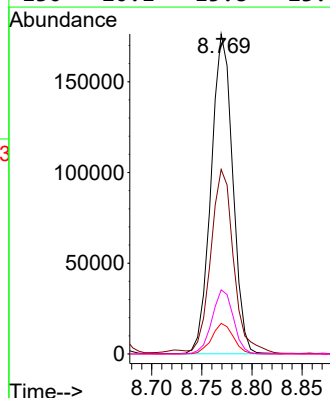





#18
4-Methylphenol
Concen: 20.006 ng/ul
RT: 8.728 min Scan# 91
Delta R.T. -0.006 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32




Instrument :
BNA_P
ClientSampleId :
SSTD020735


Tgt Ion:108 Resp: 335012
Ion Ratio Lower Upper
108 100
107 108.6 91.4 137.0



#19
Hexachloroethane
Concen: 21.380 ng/ul
RT: 9.016 min Scan# 1008
Delta R.T. -0.006 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32

Tgt Ion:117 Resp: 137065
Ion Ratio Lower Upper
117 100
201 104.7 79.9 119.9
199 63.7 49.4 74.2









#22
Nitrobenzene
Concen: 22.470 ng/ul
RT: 9.193 min Scan# 1038
Delta R.T. -0.006 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32




Instrument :
BNA_P
ClientSampleId :
SSTD020735


Tgt Ion: 77 Resp: 397713
Ion Ratio Lower Upper
77 100
123 41.8 34.6 51.8
65 12.9 10.6 16.0



#23
Isophorone
Concen: 21.062 ng/ul
RT: 9.705 min Scan# 1125
Delta R.T. -0.012 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32

Tgt Ion: 82 Resp: 698593
Ion Ratio Lower Upper
82 100
95 6.8 5.6 8.4
138 17.0 14.0 21.0









#25
2-Nitrophenol
Concen: 22.270 ng/ul
RT: 9.893 min Scan# 1157
Delta R.T. -0.012 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32




Instrument :
BNA_P
ClientSampleId :
SSTD020735


Tgt Ion:139 Resp: 179601
Ion Ratio Lower Upper
139 100
65 56.5 41.9 62.9
109 32.2 23.5 35.3



#26
2,4-Dimethylphenol
Concen: 21.441 ng/ul
RT: 9.934 min Scan# 1164
Delta R.T. -0.012 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32

Tgt Ion:107 Resp: 352402
Ion Ratio Lower Upper
107 100
121 50.2 41.7 62.5
122 84.9 70.4 105.6









#27
 Bis(2-Chloroethoxy)methane
 Concen: 21.635 ng/ul
 RT: 10.193 min Scan# 1208
 Delta R.T. -0.012 min
 Lab File: BP017187.D
 Acq: 14 Sep 2023 21:32




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020735


Tgt Ion: 93 Resp: 449765
 Ion Ratio Lower Upper
 93 100
 95 32.0 26.2 39.4
 123 11.1 9.3 13.9

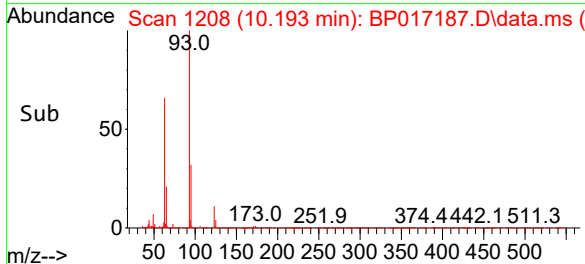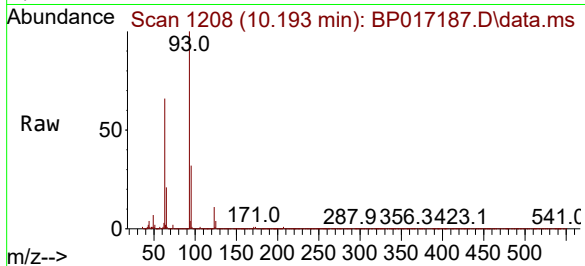

#29
 2,4-Dichlorophenol
 Concen: 21.721 ng/ul
 RT: 10.410 min Scan# 1245
 Delta R.T. -0.012 min
 Lab File: BP017187.D
 Acq: 14 Sep 2023 21:32

Tgt Ion: 162 Resp: 308541
 Ion Ratio Lower Upper
 162 100
 164 64.7 53.2 79.8
 98 36.4 30.0 45.0


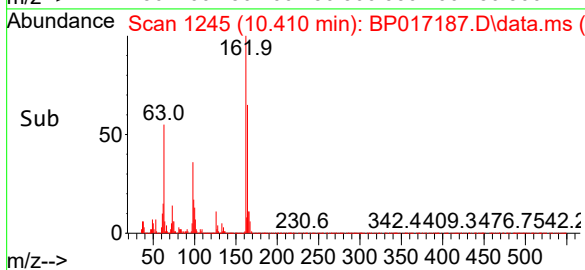

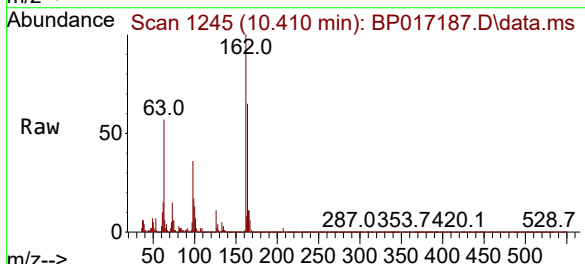




#30
Naphthalene
Concen: 21.692 ng/ul
RT: 10.822 min Scan# 11
Delta R.T. -0.012 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32




Instrument :
BNA_P
ClientSampleId :
SSTD020735


Tgt Ion:128 Resp: 1065429
Ion Ratio Lower Upper
128 100
129 10.9 8.6 13.0
127 13.1 10.4 15.6



#32
4-Chloroaniline
Concen: 20.872 ng/ul
RT: 10.963 min Scan# 1339
Delta R.T. -0.006 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32


Tgt Ion:127 Resp: 430786
Ion Ratio Lower Upper
127 100
129 32.1 24.8 37.2








#33
Hexachlorobutadiene
Concen: 22.669 ng/ul
RT: 11.052 min Scan# 11
Delta R.T. -0.012 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32

Instrument :
BNA_P
ClientSampleId :
SSTD020735







Tgt Ion:225 Resp: 218647
Ion Ratio Lower Upper
225 100
223 62.1 49.0 73.4
227 63.3 50.2 75.4



#34
Caprolactam
Concen: 17.596 ng/ul
RT: 11.781 min Scan# 1478
Delta R.T. -0.018 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32

Tgt Ion:113 Resp: 78567
Ion Ratio Lower Upper
113 100
55 169.3 130.7 196.1
56 132.9 96.8 145.2









#35
4-Chloro-3-methylphenol
Concen: 20.172 ng/ul
RT: 12.063 min Scan# 1526
Delta R.T. -0.006 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32




Instrument :
BNA_P
ClientSampleId :
SSTD020735


Tgt Ion:107 Resp: 310019
Ion Ratio Lower Upper
107 100
144 26.1 20.6 31.0
142 80.1 63.4 95.0

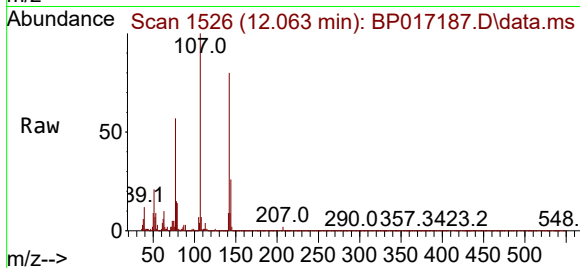

#36
2-Methylnaphthalene
Concen: 21.345 ng/ul
RT: 12.428 min Scan# 1588
Delta R.T. -0.012 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32

Tgt Ion:142 Resp: 707413
Ion Ratio Lower Upper
142 100
141 90.0 70.1 105.1




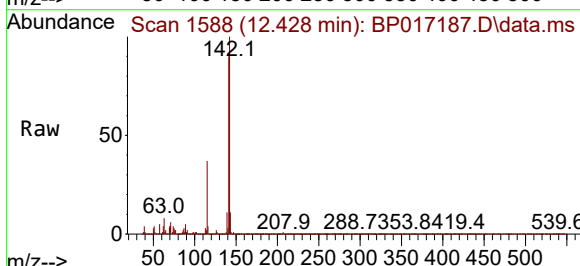




#37
1-Methylnaphthalene
Concen: 21.161 ng/ul
RT: 12.651 min Scan# 1626
Delta R.T. -0.012 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32




Instrument :
BNA_P
ClientSampleId :
SSTD020735


Tgt Ion:142 Resp: 709900
Ion Ratio Lower Upper
142 100
141 93.6 74.1 111.1
116 4.2 3.1 4.7



#39
1,2,4,5-Tetrachlorobenzene
Concen: 23.983 ng/ul
RT: 12.781 min Scan# 1648
Delta R.T. -0.012 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32

Tgt Ion:216 Resp: 404203
Ion Ratio Lower Upper
216 100
214 78.7 62.1 93.1
179 20.5 15.6 23.4
108 16.7 12.8 19.2





#40

Hexachlorocyclopentadiene

Concen: 20.060 ng/ul

RT: 12.728 min Scan# 1639

Delta R.T. -0.012 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32

Instrument :

BNA_P

ClientSampleId :

SSTD020735





Tgt Ion:237 Resp: 210641

Ion Ratio Lower Upper

237 100

235 61.5 50.4 75.6

272 12.5 10.2 15.4



#41

2,4,6-Trichlorophenol

Concen: 22.730 ng/ul

RT: 13.034 min Scan# 1691

Delta R.T. -0.012 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32




Tgt Ion:196 Resp: 243361


Ion Ratio Lower Upper

196 100

198 93.6 76.0 114.0

200 30.4 25.0 37.4





#42

2,4,5-Trichlorophenol

Concen: 22.671 ng/ul

RT: 13.104 min Scan# 1

Delta R.T. -0.012 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32

Instrument :

BNA_P

ClientSampleId :

SSTD020735





Tgt Ion:196 Resp: 258047

Ion Ratio Lower Upper

196 100

198 97.8 76.9 115.3

200 30.5 25.0 37.6

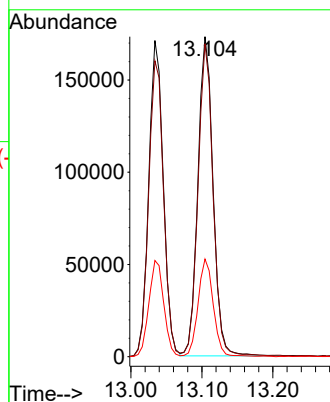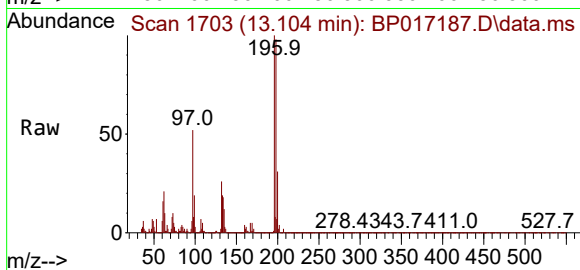

#43

1,1'-Biphenyl

Concen: 22.592 ng/ul

RT: 13.440 min Scan# 1760

Delta R.T. -0.012 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32




Tgt Ion:154 Resp: 916690


Ion Ratio Lower Upper

154 100

153 40.2 31.8 47.8

76 13.8 10.8 16.2

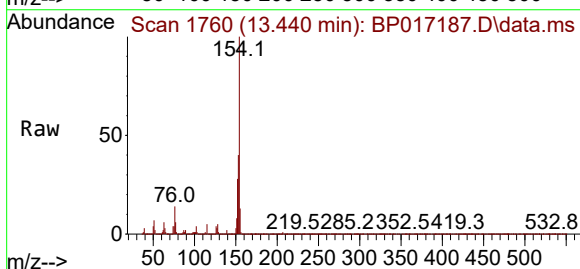



#44

2-Chloronaphthalene

Concen: 22.745 ng/ul

RT: 13.487 min Scan# 1769

Delta R.T. -0.012 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32

Instrument :

BNA_P

ClientSampleId :

SSTD020735





Tgt Ion:162 Resp: 732916

Ion Ratio Lower Upper

162 100

164 33.2 26.6 39.8

127 39.2 31.0 46.4



#45

2-Nitroaniline

Concen: 22.131 ng/ul

RT: 13.728 min Scan# 1809

Delta R.T. -0.006 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32




Tgt Ion: 65 Resp: 193159


Ion Ratio Lower Upper

65 100

92 65.3 55.6 83.4

138 102.6 82.2 123.2









#47
Dimethylphthalate
Concen: 21.183 ng/ul
RT: 14.069 min Scan# 1867
Delta R.T. -0.012 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32




Instrument :
BNA_P
ClientSampleId :
SSTD020735


Tgt Ion:163 Resp: 865926
Ion Ratio Lower Upper
163 100
194 3.9 3.3 4.9
164 10.4 7.9 11.9



#48
2,6-Dinitrotoluene
Concen: 21.040 ng/ul
RT: 14.216 min Scan# 1892
Delta R.T. -0.012 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32

Tgt Ion:165 Resp: 157236
Ion Ratio Lower Upper
165 100
89 62.1 47.8 71.8
121 21.8 17.4 26.2





#50

Acenaphthylene

Concen: 22.047 ng/ul

RT: 14.340 min Scan# 1913

Delta R.T. -0.006 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32

Instrument :

BNA_P

ClientSampleId :

SSTD020735





Tgt Ion:152 Resp: 1163753

Ion Ratio Lower Upper

152 100

151 20.0 15.8 23.8

153 13.1 10.6 15.8



#51

3-Nitroaniline

Concen: 19.664 ng/ul

RT: 14.557 min Scan# 1950

Delta R.T. -0.006 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32




Tgt Ion:138 Resp: 157211


Ion Ratio Lower Upper

138 100

108 10.5 8.5 12.7

92 113.4 94.2 141.4





#52

Acenaphthene

Concen: 21.861 ng/ul

RT: 14.675 min Scan# 1970

Delta R.T. -0.006 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32

Instrument :

BNA_P

ClientSampleId :

SSTD020735





Tgt Ion:153 Resp: 763578

Ion Ratio Lower Upper

153 100

152 48.8 38.6 57.8

154 87.8 70.4 105.6

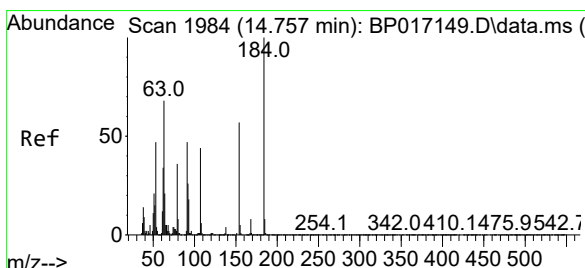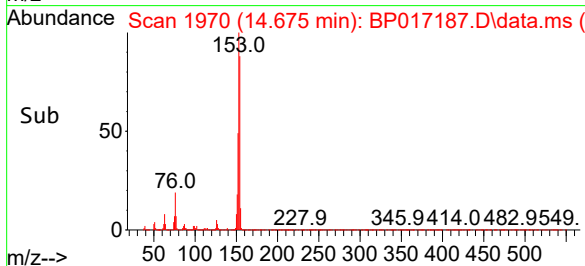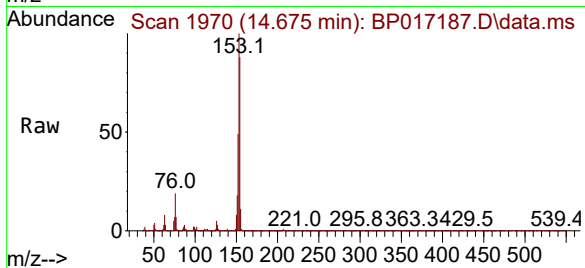

#53

2,4-Dinitrophenol

Concen: 10.844 ng/ul

RT: 14.757 min Scan# 1984

Delta R.T. -0.006 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32




Tgt Ion:184 Resp: 56763


Ion Ratio Lower Upper

184 100

63 72.3 55.2 82.8

154 71.1 53.0 79.4


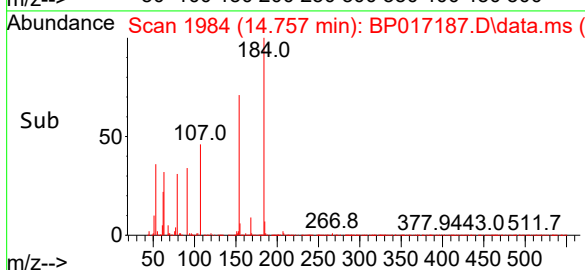

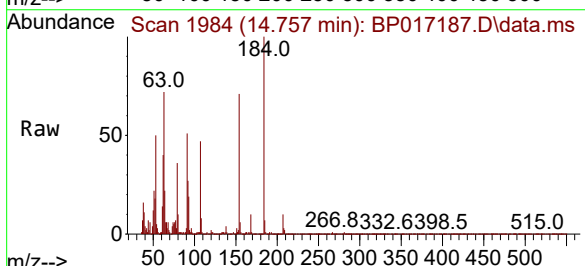




#55
4-Nitrophenol
Concen: 18.162 ng/ul
RT: 14.845 min Scan# 1999
Delta R.T. -0.006 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32




Instrument :
BNA_P
ClientSampleId :
SSTD020735


Tgt Ion:109 Resp: 113130
Ion Ratio Lower Upper
109 100
139 123.9 101.1 151.7
65 127.2 105.0 157.4

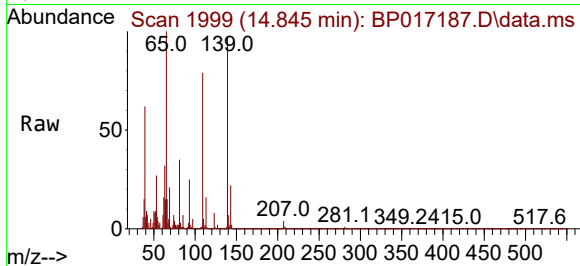

#56
Dibenzofuran
Concen: 21.847 ng/ul
RT: 15.010 min Scan# 2027
Delta R.T. -0.012 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32

Tgt Ion:168 Resp: 1054537
Ion Ratio Lower Upper
168 100
139 37.6 29.9 44.9

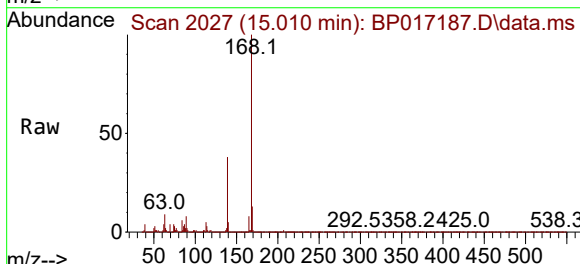



#57

2,4-Dinitrotoluene

Concen: 20.244 ng/ul

RT: 14.998 min Scan# 20

Delta R.T. -0.006 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32

Instrument :

BNA_P

ClientSampleId :

SSTD020735





Tgt Ion:165 Resp: 225282

Ion Ratio Lower Upper

165 100

63 58.9 42.3 63.5

182 2.5 2.2 3.4



#58

2,3,4,6-Tetrachlorophenol

Concen: 21.249 ng/ul

RT: 15.228 min Scan# 2064

Delta R.T. -0.006 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32

Tgt Ion:232 Resp: 212186




Ion Ratio Lower Upper


232 100

131 44.4 37.0 55.6

130 2.5 1.8 2.8

166 29.7 24.3 36.5





#59

Diethylphthalate

Concen: 20.620 ng/ul

RT: 15.428 min Scan# 2098

Delta R.T. -0.006 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32

Instrument :

BNA_P

ClientSampleId :

SSTD020735





Tgt Ion:149 Resp: 832198

Ion Ratio Lower Upper

149 100

177 22.1 17.5 26.3

150 12.1 10.0 15.0

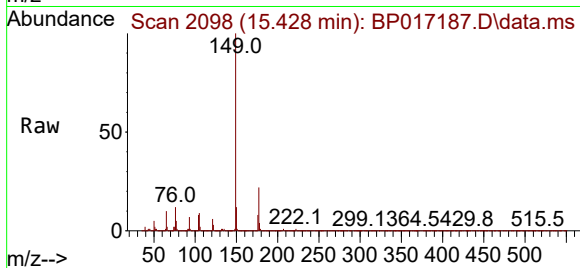

#61

Fluorene

Concen: 21.371 ng/ul

RT: 15.663 min Scan# 2138

Delta R.T. -0.006 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32




Tgt Ion:166 Resp: 852848


Ion Ratio Lower Upper

166 100

165 99.2 78.2 117.2

167 13.2 11.0 16.4


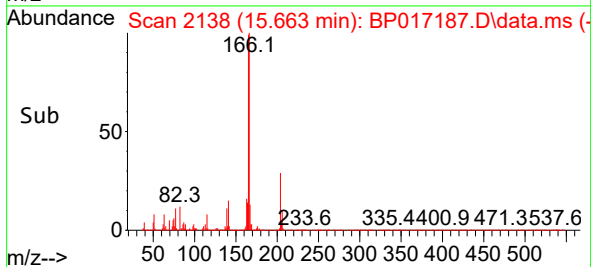

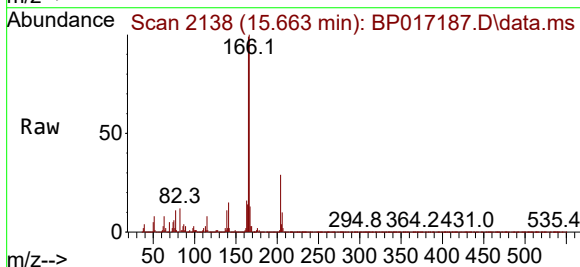




#62
4-Chlorophenyl-phenylether
Concen: 22.104 ng/ul
RT: 15.651 min Scan# 2137
Delta R.T. -0.012 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32




Instrument :
BNA_P
ClientSampleId :
SSTD020735


Tgt Ion:204 Resp: 448475
Ion Ratio Lower Upper
204 100
206 33.5 27.3 40.9
141 57.0 45.0 67.6

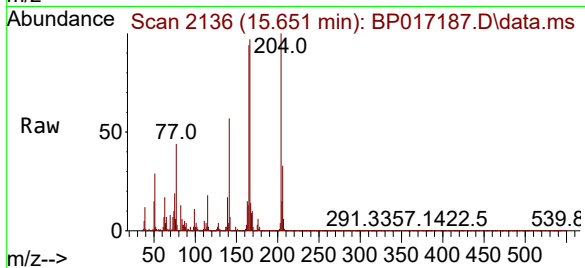

#63
4-Nitroaniline
Concen: 19.371 ng/ul
RT: 15.722 min Scan# 2148
Delta R.T. -0.012 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32

Tgt Ion:138 Resp: 143976
Ion Ratio Lower Upper
138 100
92 54.6 43.3 64.9
108 96.6 75.3 112.9




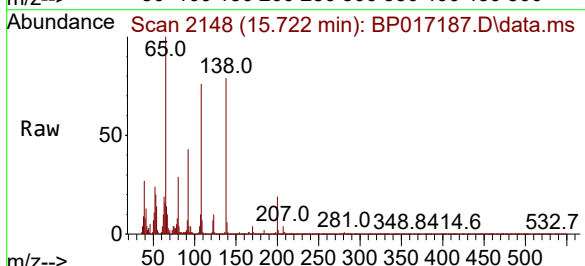




#66
4,6-Dinitro-2-methylphenol
Concen: 18.507 ng/ul
RT: 15.751 min Scan# 2153
Delta R.T. -0.006 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32




Instrument :
BNA_P
ClientSampleId :
SSTD020735


Tgt Ion:198 Resp: 125928
Ion Ratio Lower Upper
198 100
182 4.8 4.2 6.2
77 26.2 22.5 33.7

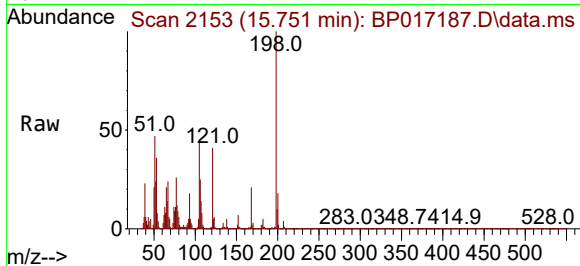

#67
N-Nitrosodiphenylamine
Concen: 23.222 ng/ul
RT: 15.881 min Scan# 2175
Delta R.T. -0.006 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32

Tgt Ion:169 Resp: 685228
Ion Ratio Lower Upper
169 100
168 66.8 52.7 79.1
167 37.3 29.0 43.4




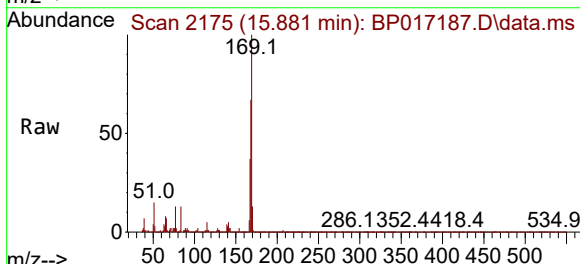




#68
4-Bromophenyl-phenylether
Concen: 23.918 ng/ul
RT: 16.557 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32




Instrument :
BNA_P
ClientSampleId :
SSTD020735


Tgt Ion:248 Resp: 258733
Ion Ratio Lower Upper
248 100
250 95.9 78.6 118.0
141 69.6 60.4 90.6

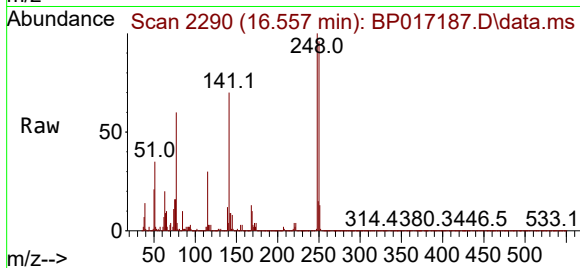

#69
Hexachlorobenzene
Concen: 23.349 ng/ul
RT: 16.634 min Scan# 2303
Delta R.T. -0.012 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32

Tgt Ion:284 Resp: 298951
Ion Ratio Lower Upper
284 100
142 36.0 28.6 42.8
249 31.3 25.0 37.6

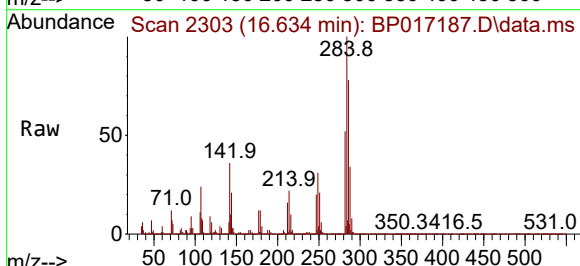



#70

Atrazine

Concen: 22.005 ng/ul

RT: 16.834 min Scan# 21

Delta R.T. -0.012 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32

Instrument :

BNA_P

ClientSampleId :

SSTD020735





Tgt Ion:200 Resp: 235043

Ion Ratio Lower Upper

200 100

173 25.3 20.7 31.1

215 49.3 38.8 58.2

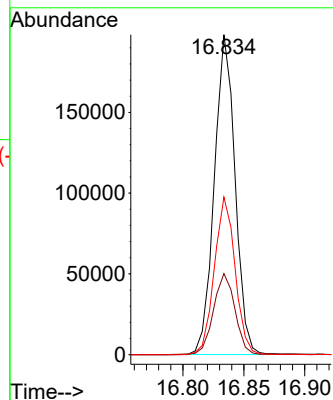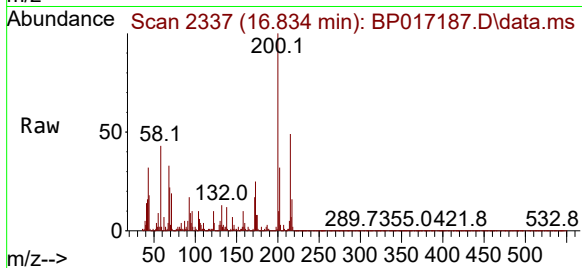

#71

Pentachlorophenol

Concen: 19.755 ng/ul

RT: 17.004 min Scan# 2366

Delta R.T. -0.006 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32




Tgt Ion:266 Resp: 164387


Ion Ratio Lower Upper

266 100

264 63.7 50.7 76.1

268 64.3 51.1 76.7

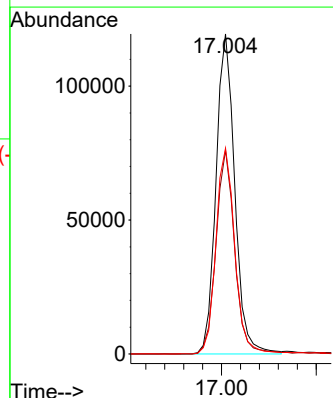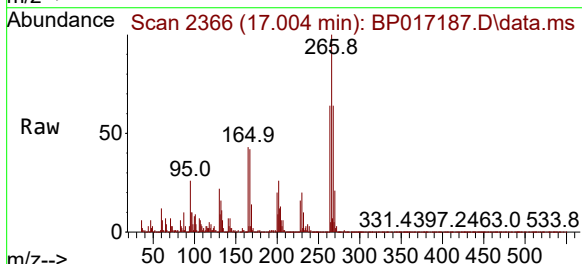



#72

Phenanthrene

Concen: 21.987 ng/ul

RT: 17.422 min Scan# 2438

Delta R.T. -0.012 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32

Instrument :

BNA_P

ClientSampleId :

SSTD020735





Tgt Ion:178 Resp: 1253911

Ion Ratio Lower Upper

178 100

179 15.3 12.2 18.2

176 19.7 15.6 23.4



#74

Anthracene

Concen: 22.407 ng/ul

RT: 17.516 min Scan# 2453

Delta R.T. -0.006 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32




Tgt Ion:178 Resp: 1294216


Ion Ratio Lower Upper

178 100

179 15.4 12.4 18.6

176 19.2 14.9 22.3





#75

1,2,3,4-Tetrachlorobenzene

Concen: 26.603 ng/uL

RT: 13.393 min Scan# 1

Delta R.T. -0.012 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32

Instrument :

BNA_P

ClientSampleId :

SSTD020735





Tgt Ion:216 Resp: 417415

Ion Ratio Lower Upper

216 100

214 78.1 61.3 91.9

218 48.4 38.3 57.5



#76

Pentachlorobenzene

Concen: 25.312 ng/uL

RT: 14.904 min Scan# 2009

Delta R.T. -0.006 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32




Tgt Ion:250 Resp: 360381


Ion Ratio Lower Upper

250 100

248 62.5 51.1 76.7

252 62.6 50.7 76.1


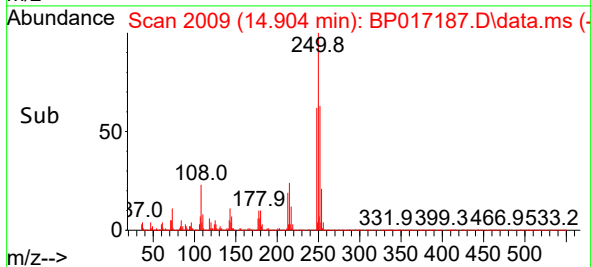

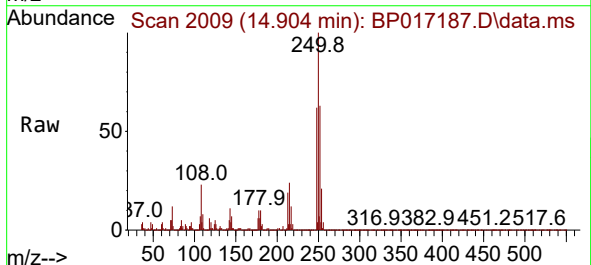




#77
 Carbazole
 Concen: 20.940 ng/ul
 RT: 17.798 min Scan# 2501
 Delta R.T. -0.012 min
 Lab File: BP017187.D
 Acq: 14 Sep 2023 21:32




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020735


Tgt Ion:167 Resp: 1062061
 Ion Ratio Lower Upper
 167 100
 166 21.6 17.0 25.6
 139 13.6 10.4 15.6



#78
 Di-n-butylphthalate
 Concen: 21.775 ng/ul
 RT: 18.310 min Scan# 2588
 Delta R.T. -0.012 min
 Lab File: BP017187.D
 Acq: 14 Sep 2023 21:32

Tgt Ion:149 Resp: 1258500
 Ion Ratio Lower Upper
 149 100
 150 9.2 7.2 10.8
 104 5.9 4.2 6.4

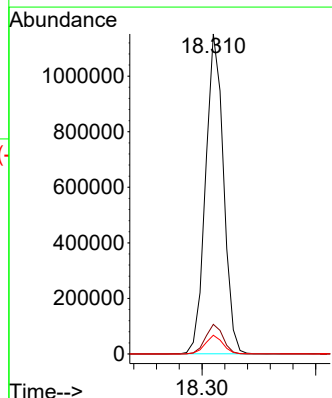



#80

Fluoranthene

Concen: 23.098 ng/ul

RT: 19.386 min Scan# 21

Delta R.T. -0.012 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32

Instrument :

BNA_P

ClientSampleId :

SSTD020735





Tgt Ion:202 Resp: 1379068

Ion Ratio Lower Upper

202 100

101 11.0 8.3 12.5

100 8.4 6.4 9.6



#82

Pyrene

Concen: 23.071 ng/ul

RT: 19.745 min Scan# 2832

Delta R.T. -0.012 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32




Tgt Ion:202 Resp: 1455483


Ion Ratio Lower Upper

202 100

101 13.1 9.7 14.5

100 10.7 7.8 11.8

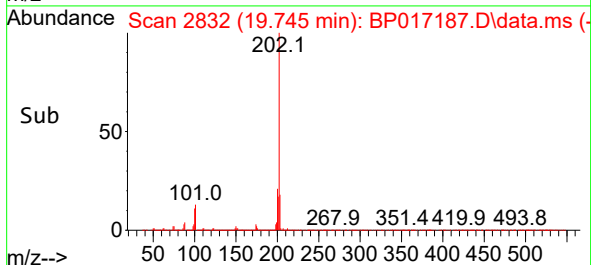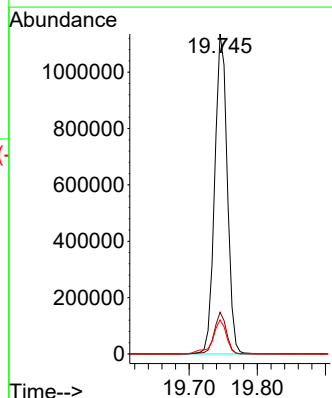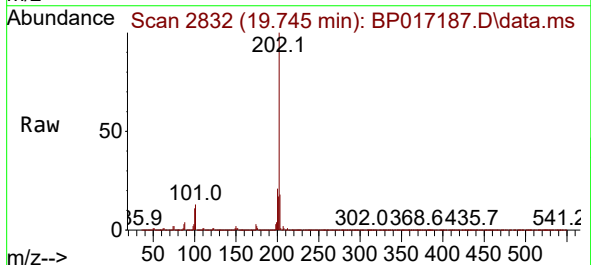



#83

Butylbenzylphthalate

Concen: 21.959 ng/ul

RT: 20.610 min Scan# 2979

Delta R.T. -0.006 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32

Instrument :

BNA_P

ClientSampleId :

SSTD020735





Tgt Ion:149 Resp: 494086

Ion Ratio Lower Upper

149 100

91 74.4 57.4 86.0

206 21.9 16.7 25.1



#84

3,3'-Dichlorobenzidine

Concen: 20.477 ng/ul

RT: 21.404 min Scan# 3114

Delta R.T. -0.006 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32




Tgt Ion:252 Resp: 408910


Ion Ratio Lower Upper

252 100

254 63.3 51.4 77.2

126 10.8 9.4 14.2





#85

Benzo(a)anthracene

Concen: 21.846 ng/ul

RT: 21.463 min Scan# 3125

Delta R.T. -0.006 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32

Instrument :

BNA_P

ClientSampleId :

SSTD020735





Tgt Ion:228 Resp: 1393212

Ion Ratio Lower Upper

228 100

229 19.6 16.1 24.1

226 27.5 22.2 33.4

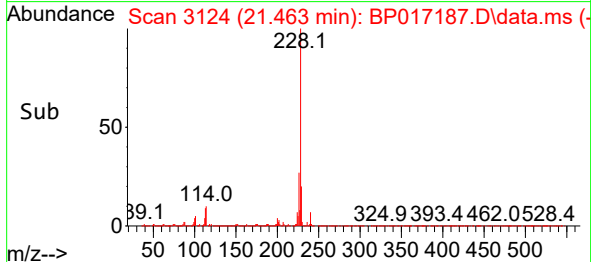

#86

Bis(2-ethylhexyl)phthalate

Concen: 22.217 ng/ul

RT: 21.345 min Scan# 3104

Delta R.T. -0.006 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32




Tgt Ion:149 Resp: 701718


Ion Ratio Lower Upper

149 100

167 26.5 21.3 31.9

279 4.8 3.4 5.2





#87

Chrysene

Concen: 22.213 ng/ul

RT: 21.522 min Scan# 3134

Delta R.T. -0.006 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32

Instrument :

BNA_P

ClientSampleId :

SSTD020735





Tgt Ion:228 Resp: 1317777

Ion Ratio Lower Upper

228 100

226 29.9 23.9 35.9

229 19.4 15.3 22.9

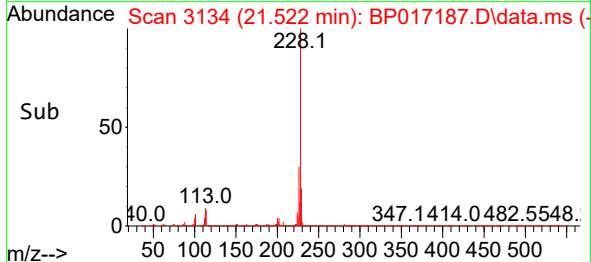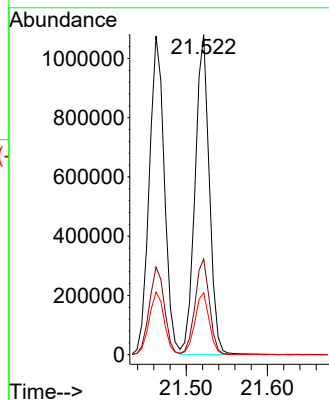

#89

Di-n-octyl phthalate

Concen: 20.027 ng/ul




RT: 22.304 min Scan# 3267


Delta R.T. -0.012 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32

Tgt Ion:149 Resp: 1189088

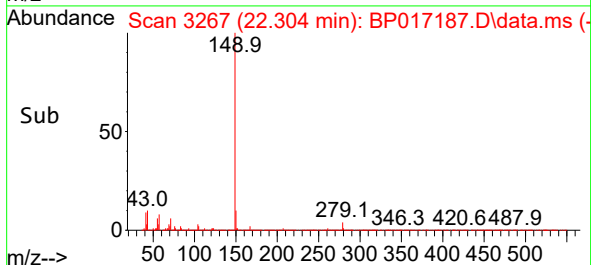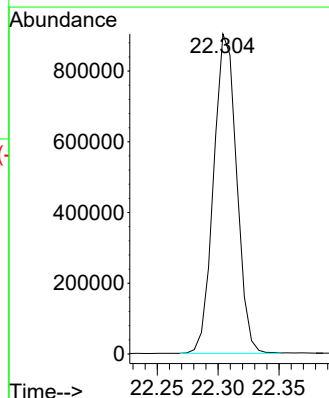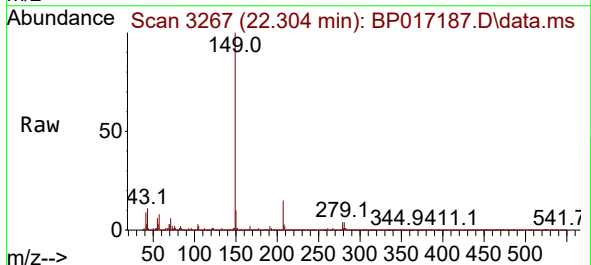



#90

Benzo(b)fluoranthene

Concen: 21.448 ng/ul

RT: 23.221 min Scan# 3423

Delta R.T. -0.006 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32

Instrument :

BNA_P

ClientSampleId :

SSTD020735





Tgt Ion:252 Resp: 1353743

Ion Ratio Lower Upper

252 100

253 21.6 18.2 27.2

125 8.6 7.5 11.3



#91

Benzo(k)fluoranthene

Concen: 21.444 ng/ul

RT: 23.269 min Scan# 3431

Delta R.T. -0.012 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32




Tgt Ion:252 Resp: 1345551


Ion Ratio Lower Upper

252 100

253 22.3 17.8 26.6

125 9.5 7.4 11.2





#93

Benzo(a)pyrene

Concen: 22.098 ng/ul

RT: 23.892 min Scan# 3537

Delta R.T. -0.012 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32

Instrument :

BNA_P

ClientSampleId :

SSTD020735





Tgt Ion:252 Resp: 1294005

Ion Ratio Lower Upper

252 100

253 21.3 17.4 26.2

125 10.0 8.1 12.1



#94

Indeno(1,2,3-cd)pyrene

Concen: 24.798 ng/ul

RT: 26.680 min Scan# 4011

Delta R.T. -0.018 min

Lab File: BP017187.D

Acq: 14 Sep 2023 21:32




Tgt Ion:276 Resp: 1608012


Ion Ratio Lower Upper

276 100

138 21.6 17.5 26.3

277 24.8 19.6 29.4









#95
Dibenzo(a,h)anthracene
Concen: 24.696 ng/ul
RT: 26.698 min Scan# 4016
Delta R.T. -0.023 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32

Instrument :
BNA_P
ClientSampleId :
SSTD020735

Tgt Ion:278 Resp: 1345224
Ion Ratio Lower Upper
278 100
139 15.5 11.9 17.9
279 23.9 19.0 28.6



#96
Benzo(g,h,i)perylene
Concen: 25.342 ng/ul
RT: 27.509 min Scan# 4152
Delta R.T. -0.023 min
Lab File: BP017187.D
Acq: 14 Sep 2023 21:32

Tgt Ion:276 Resp: 1270654
Ion Ratio Lower Upper
276 100
138 20.9 16.2 24.4
277 23.5 19.6 29.4

