

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
 Data File : BP017123.D
 Acq On : 12 Sep 2023 18:59
 Operator : MA/JU
 Sample : 04247-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJ83

Quant Time: Sep 13 01:02:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 12 23:27:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	211375	20.000	ng/u1	0.00
20) Naphthalene-d8	10.781	136	1008348	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.616	164	730969	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.386	188	1703185	20.000	ng/u1	0.00
79) Chrysene-d12	21.480	240	1655988	20.000	ng/u1	0.00
88) Perylene-d12	24.010	264	1804256	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	34202	6.800	ng/uL	0.00
4) Pyridine-d5	3.752	84	206077	14.322	ng/u1	0.00
7) Phenol-d5	7.105	99	203054	11.814	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.299	67	463172	43.115	ng/u1	0.00
11) 2-Chlorophenol-d4	7.475	132	487635	35.564	ng/u1	0.00
15) 4-Methylphenol-d8	8.663	113	342087	24.015	ng/u1	0.00
21) Nitrobenzene-d5	9.157	128	288197	40.817	ng/u1	0.00
24) 2-Nitrophenol-d4	9.869	143	305850	40.575	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.393	165	525373	36.039	ng/u1	0.00
31) 4-Chloroaniline-d4	10.946	131	646948	29.443	ng/u1	0.00
46) Dimethylphthalate-d6	14.028	166	1955807	37.599	ng/u1	0.00
49) Acenaphthylene-d8	14.316	160	2081395	35.264	ng/u1	0.00
54) 4-Nitrophenol-d4	14.834	143	79371	7.895	ng/u1	0.00
60) Fluorene-d10	15.610	176	1698119	37.755	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.739	200	314831	33.085	ng/u1	0.00
73) Anthracene-d10	17.486	188	2973585	41.092	ng/u1	0.00
81) Pyrene-d10	19.722	212	3671765	42.278	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.845	264	3577666	42.012	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.352	88	10885	2.012	ng/uL	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091223\
Data File : BP017123.D
Acq On : 12 Sep 2023 18:59
Operator : MA/JU
Sample : 04247-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ83


Quant Time: Sep 13 01:02:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 12 23:27:27 2023
Response via : Initial Calibration

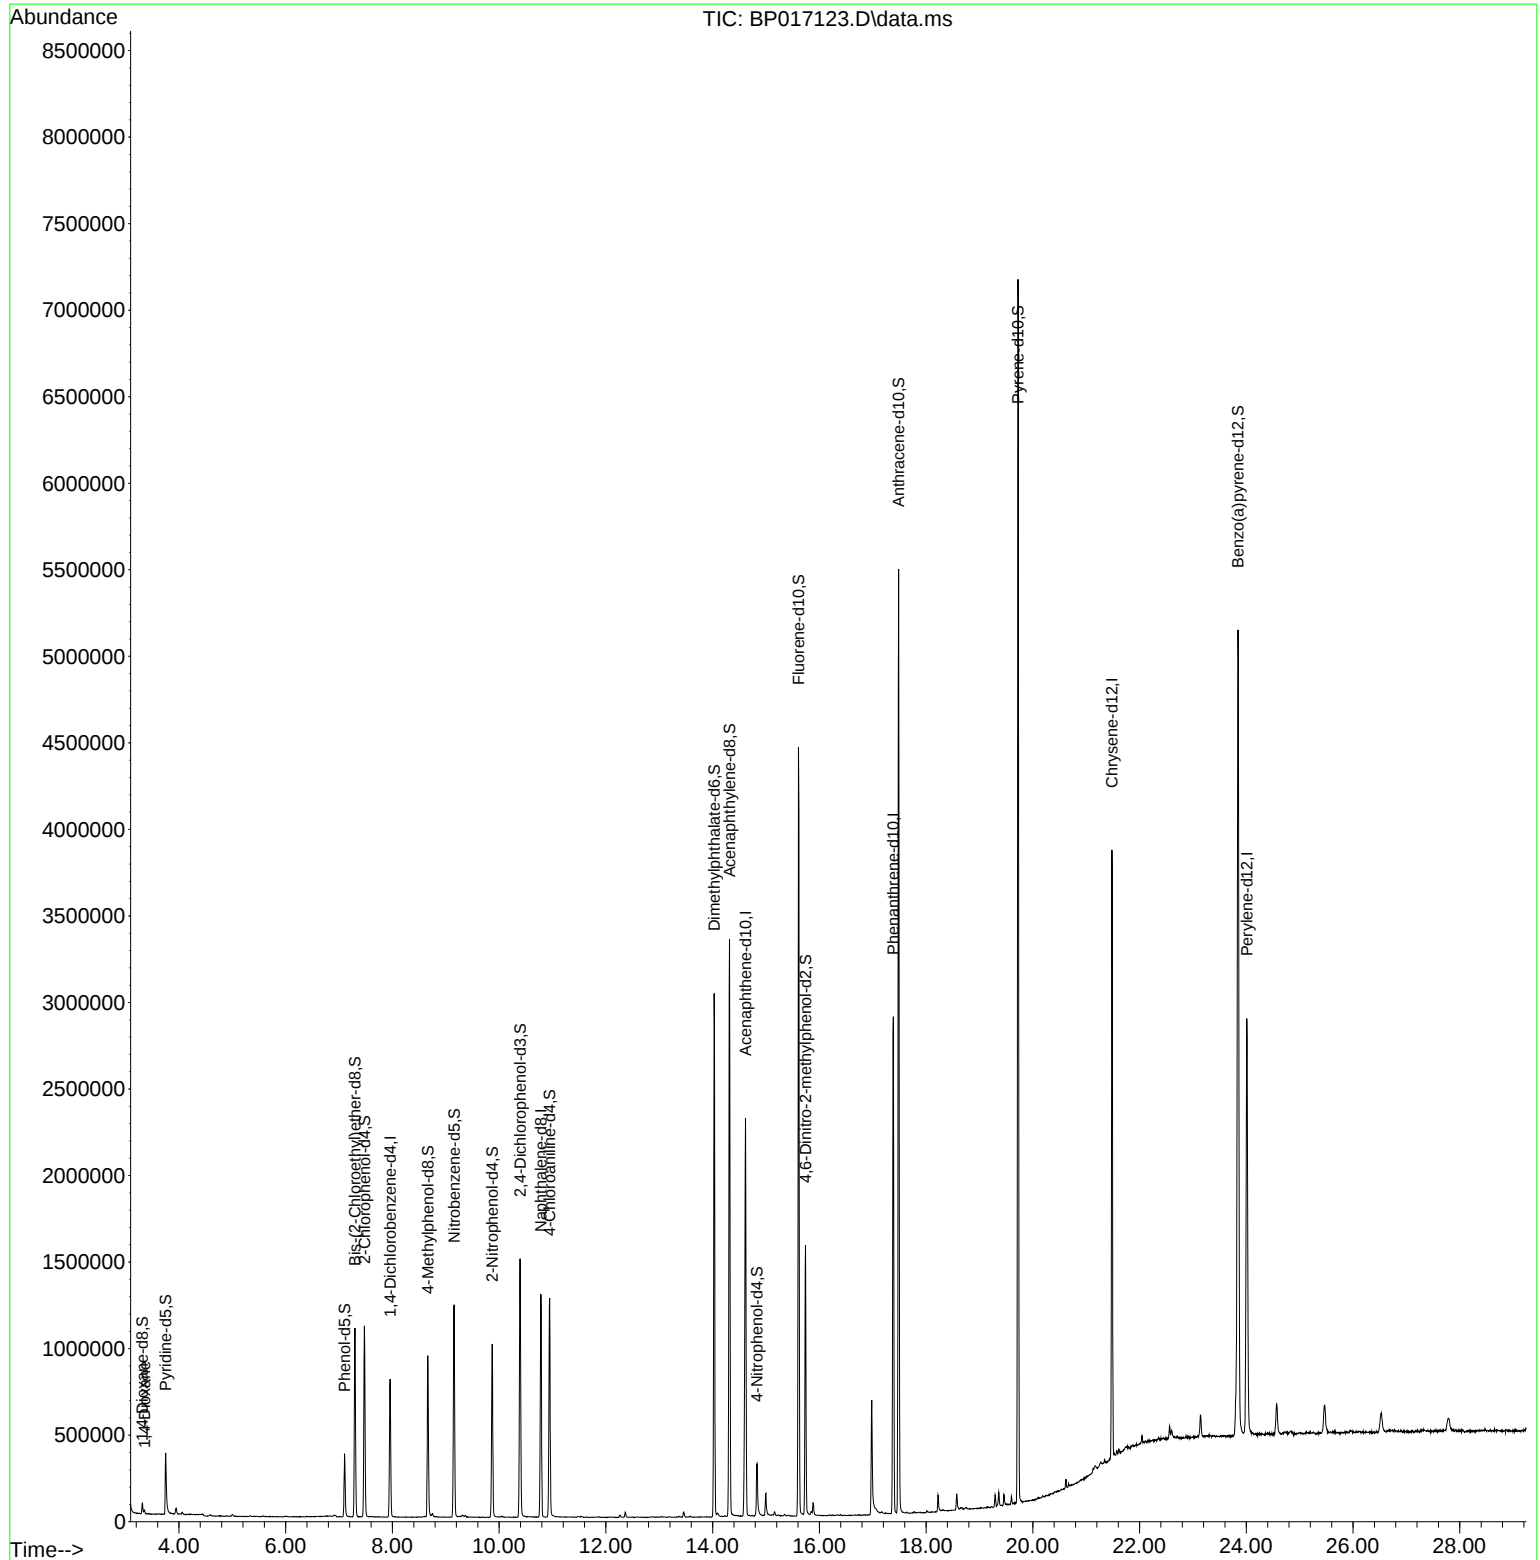

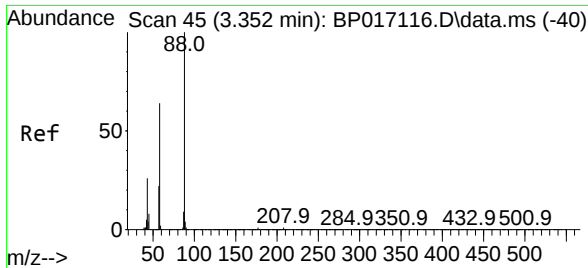

#2
 1,4-Dioxane
 Concen: 2.012 ng/uL
 RT: 3.352 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BP017123.D
 Acq: 12 Sep 2023 18:59

Instrument :
 BNA_P
 ClientSampleId :
 BBJ83

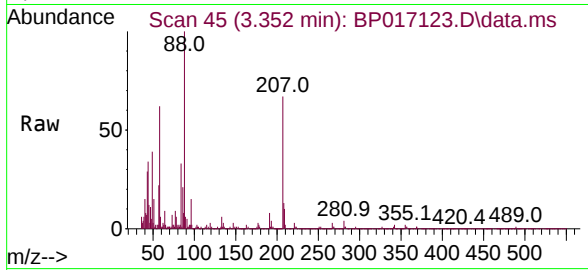

Tgt Ion:	88	Resp:	10885
Ion	Ratio	Lower	Upper
88	100		
43	28.9	21.9	32.9
58	61.7	50.8	76.2

